

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061219\
 Data File : PL049449.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2019 13:33
 Operator : SM\AJ
 Sample : K3303-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BAT-B02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 01:35:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.935	225.3E6	60986657	20.443	21.110
28)	SA Decachlor...	7.989	8.968	193.8E6	54280068	15.242	16.253
Target Compounds							
2)	A alpha-BHC	3.760	0.000	12527667	0	0.695	N.D. #
3)	MA gamma-BHC...	4.037	4.589f	7175503	7405252	0.423	1.978 #
6)	B beta-BHC	0.000	4.804f	0	737023	N.D.	0.428 #
9)	A Endosulfan I	5.347f	6.163	93908327	7284480	6.417	2.262 #
10)	B gamma-Chl...	0.000	6.022	0	3782191	N.D.	1.093 #
11)	B alpha-Chl...	5.276	6.101	38758426	5096900	2.481	1.469 #
13)	MA Dieldrin	5.566	0.000	37081167	0	2.425	N.D. #
14)	MA Endrin	5.810	0.000	91009104	0	6.310	N.D. #
15)	B Endosulfa...	6.094	6.851	45719058	13342596	3.462	4.399 #
16)	A 4,4'-DDD	5.936	6.749	23265904	25257815	1.955	9.603 #
17)	MA 4,4'-DDT	6.176	0.000	10008004	0	0.813	N.D. #
18)	B Endrin al...	6.225f	0.000	14253195	0	1.302	N.D. #
19)	B Endosulfa...	6.481f	0.000	6952625	0	0.535	N.D. #
20)	A Methoxychlor	0.000	7.488f	0	5128659	N.D.	3.094 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061219\
Data File : PL049449.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2019 13:33
Operator : SM\AJ
Sample : K3303-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BAT-B02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 01:35:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

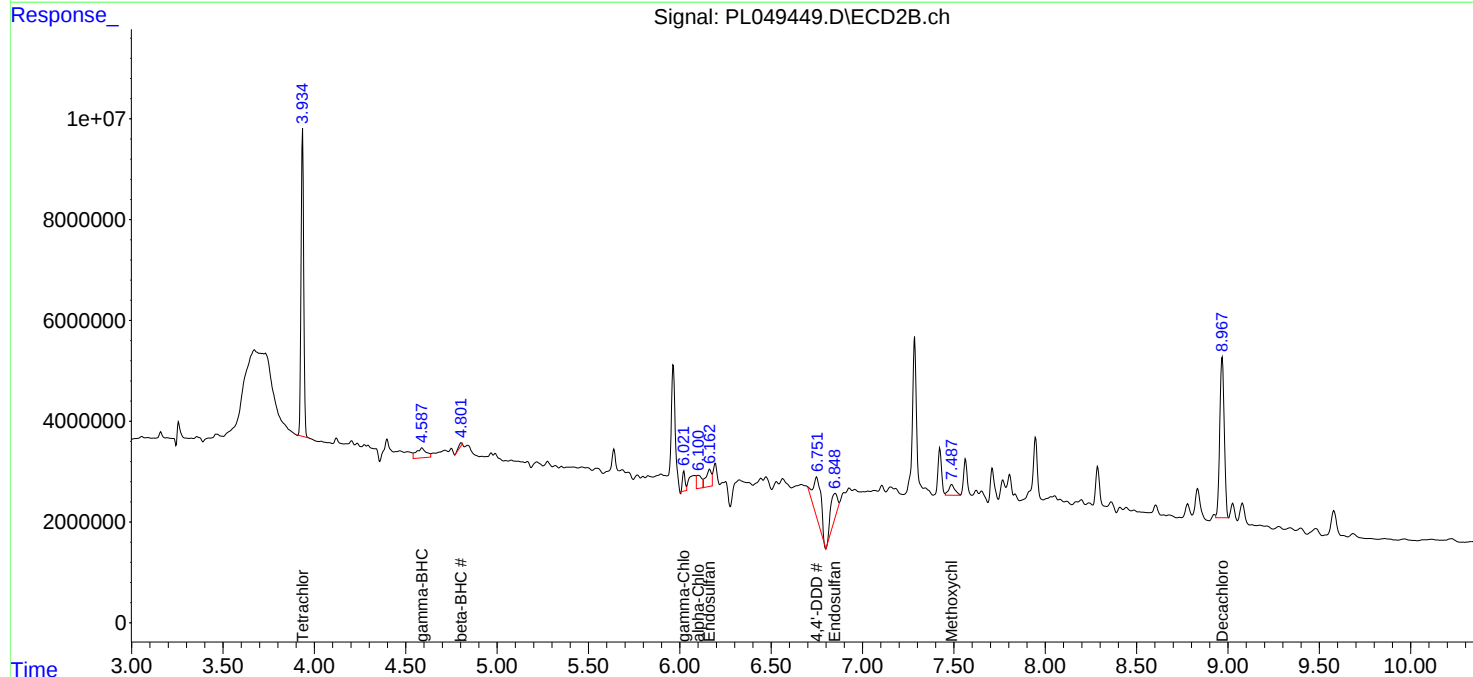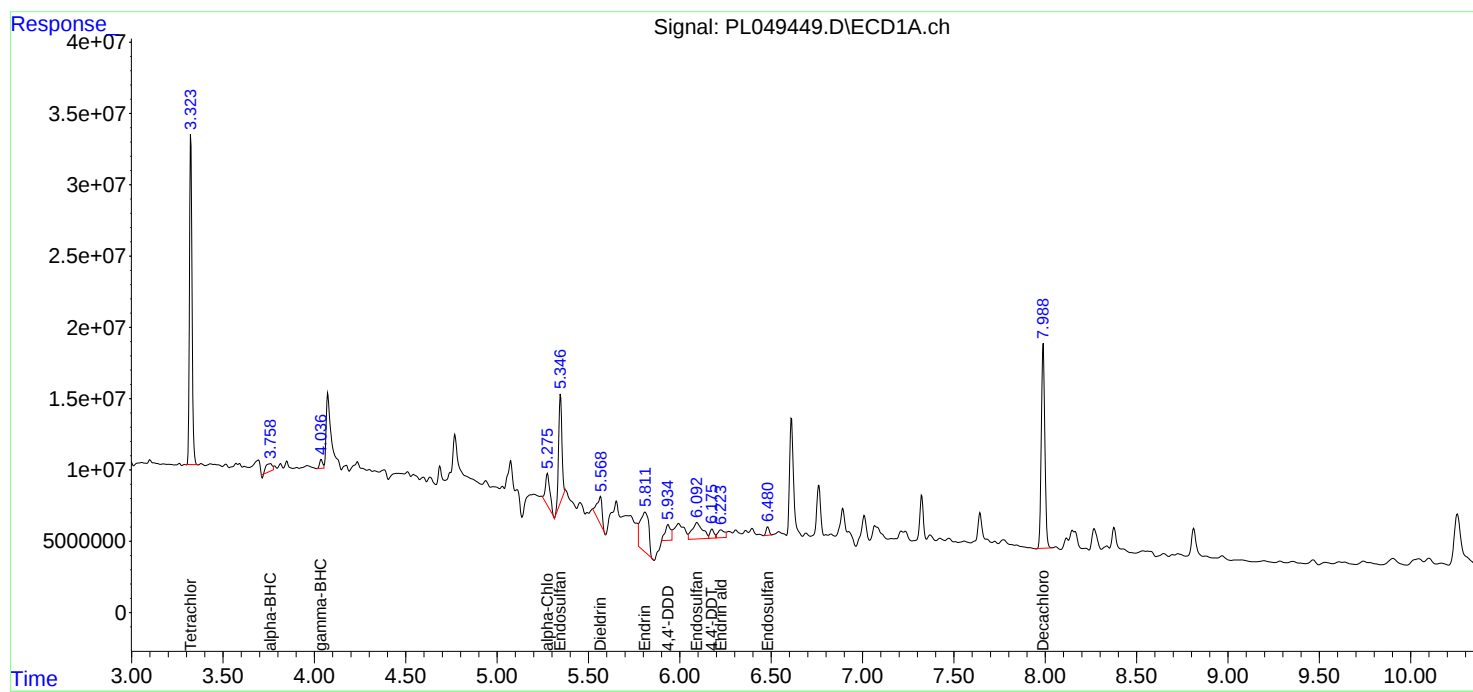


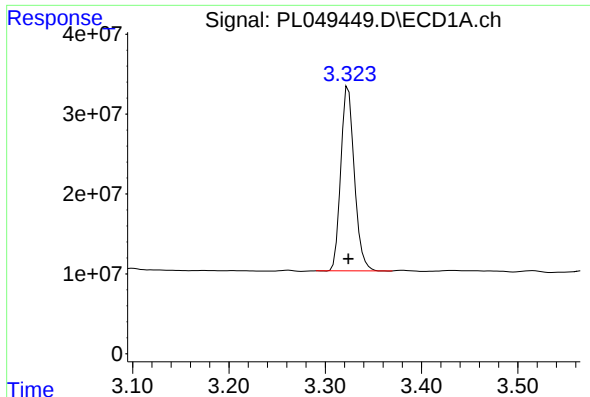

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: 0.000 min
Response: 225261360
Conc: 20.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
BAT-B02

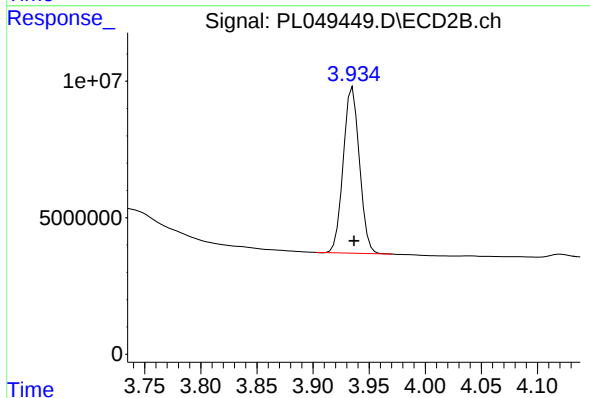


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.001 min
Response: 60986657
Conc: 21.11 ng/ml

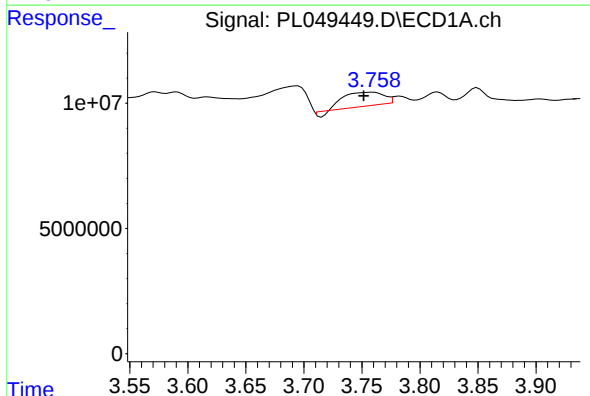


#2 alpha-BHC

R.T.: 3.760 min
Delta R.T.: 0.008 min
Response: 12527667
Conc: 0.70 ng/ml

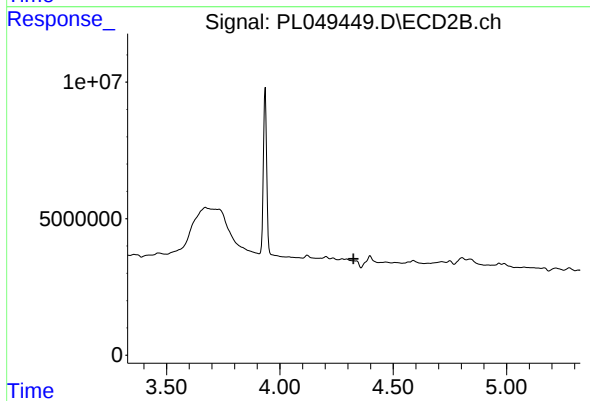

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.325 min
Response: 0
Conc: N.D.

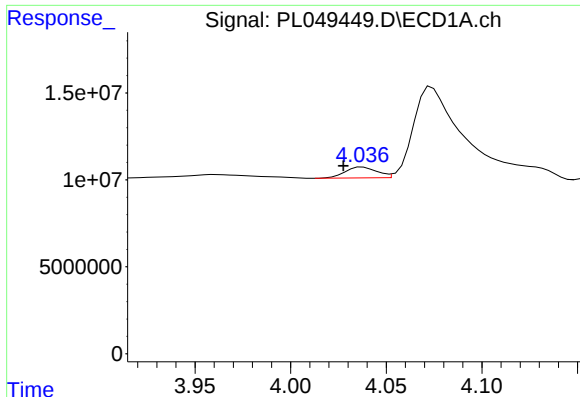

#3 gamma-BHC (Lindane)


R.T.: 4.037 min
Delta R.T.: 0.010 min
Response: 7175503
Conc: 0.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
BAT-B02

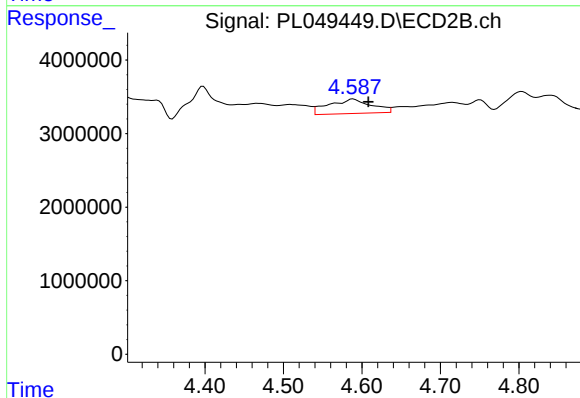


#3 gamma-BHC (Lindane)

R.T.: 4.589 min
Delta R.T.: -0.019 min
Response: 7405252
Conc: 1.98 ng/ml

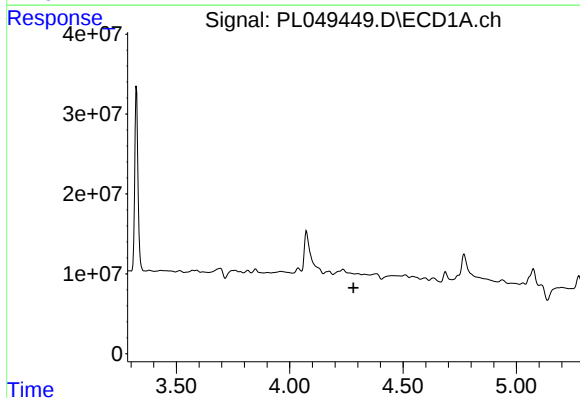


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.282 min
Response: 0
Conc: N.D.

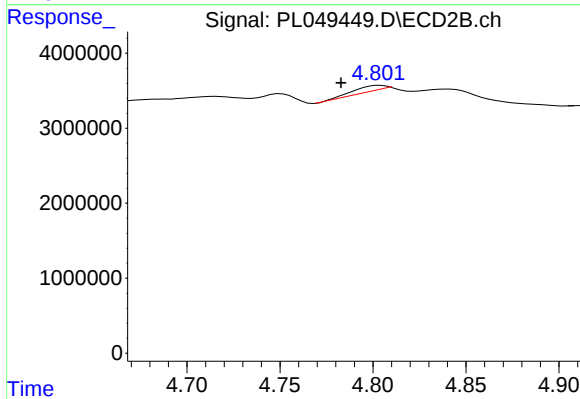

#6 beta-BHC


R.T.: 4.804 min
Delta R.T.: 0.021 min
Response: 737023
Conc: 0.43 ng/ml

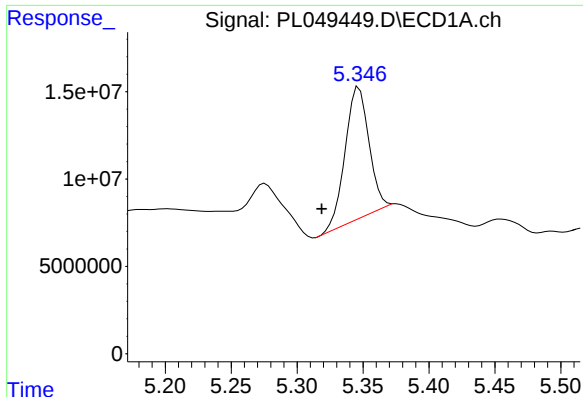

#9 Endosulfan I


R.T.: 5.347 min
Delta R.T.: 0.028 min
Response: 93908327
Conc: 6.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
BAT-B02

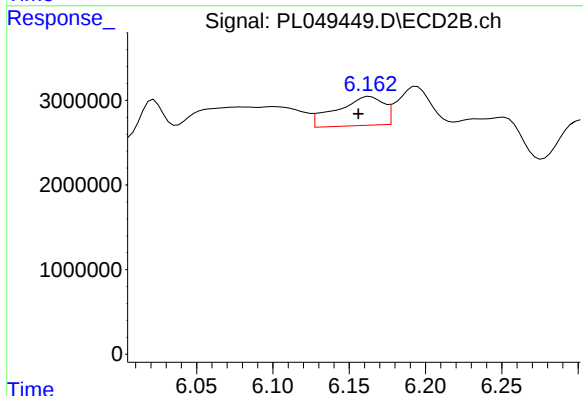


#9 Endosulfan I

R.T.: 6.163 min
Delta R.T.: 0.007 min
Response: 7284480
Conc: 2.26 ng/ml

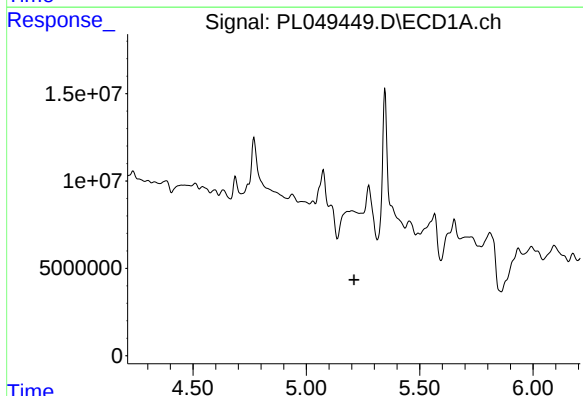


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.211 min
Response: 0
Conc: N.D.

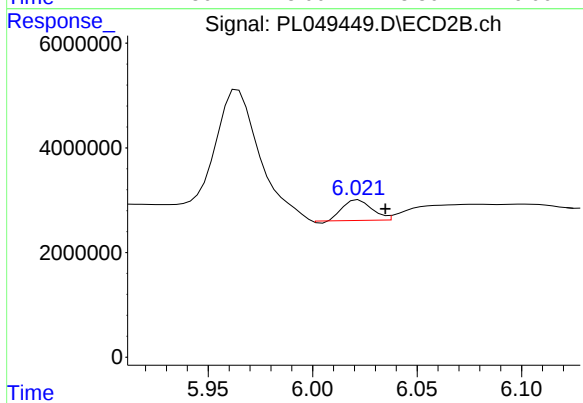

#10 gamma-Chlordane


R.T.: 6.022 min
Delta R.T.: -0.013 min
Response: 3782191
Conc: 1.09 ng/ml

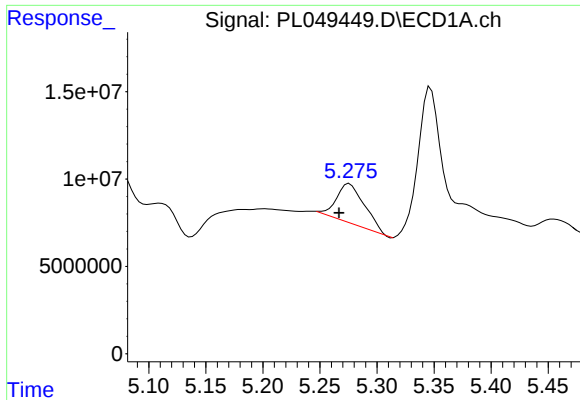

#11 alpha-Chlordane


R.T.: 5.276 min
Delta R.T.: 0.009 min
Response: 38758426
Conc: 2.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
BAT-B02

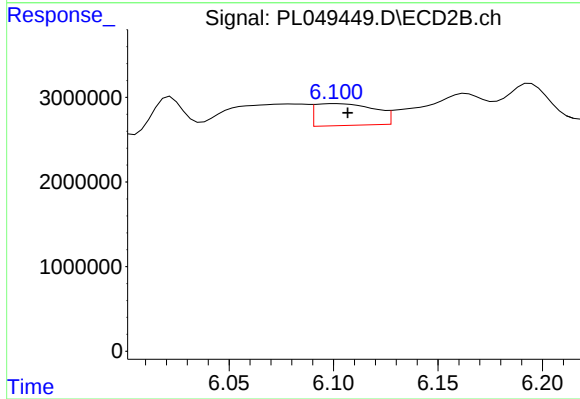


#11 alpha-Chlordane

R.T.: 6.101 min
Delta R.T.: -0.005 min
Response: 5096900
Conc: 1.47 ng/ml

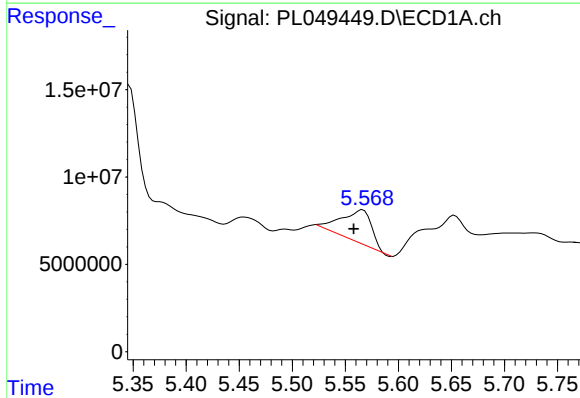


#13 Dieldrin

R.T.: 5.566 min
Delta R.T.: 0.008 min
Response: 37081167
Conc: 2.43 ng/ml

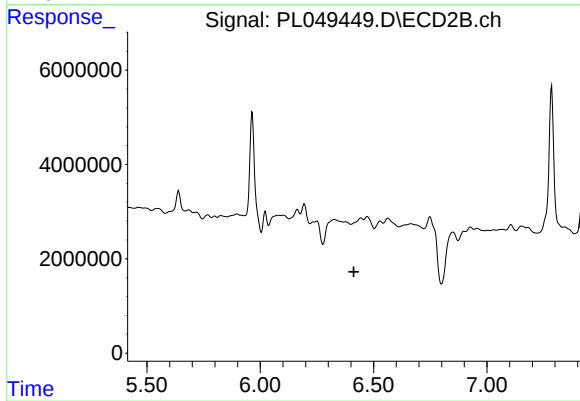

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.413 min
Response: 0
Conc: N.D.

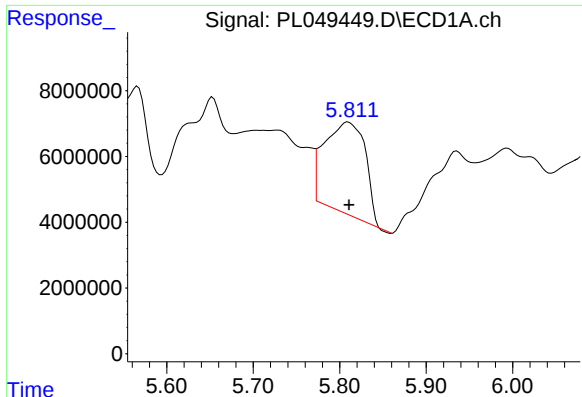

#14 Endrin


R.T.: 5.810 min
Delta R.T.: -0.001 min
Response: 91009104
Conc: 6.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
BAT-B02

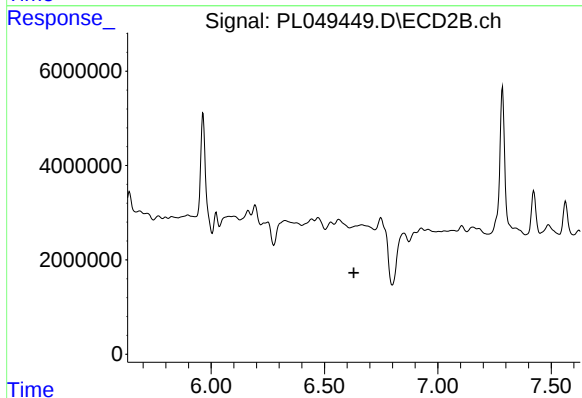


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.630 min
Response: 0
Conc: N.D.

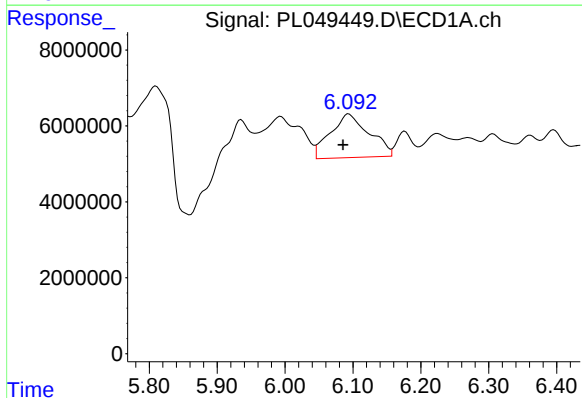


#15 Endosulfan II

R.T.: 6.094 min
Delta R.T.: 0.008 min
Response: 45719058
Conc: 3.46 ng/ml

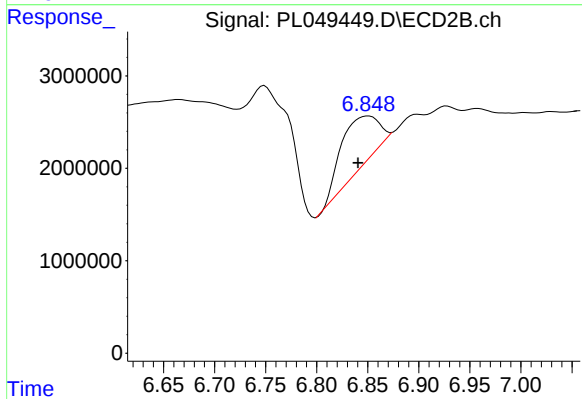

#15 Endosulfan II


R.T.: 6.851 min
Delta R.T.: 0.010 min
Response: 13342596
Conc: 4.40 ng/ml

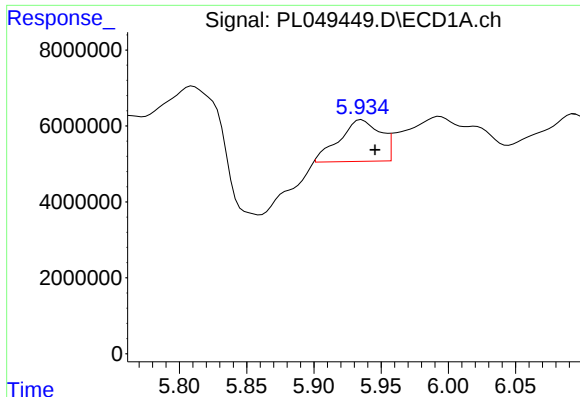

#16 4,4'-DDD


R.T.: 5.936 min
Delta R.T.: -0.010 min
Response: 23265904
Conc: 1.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
BAT-B02

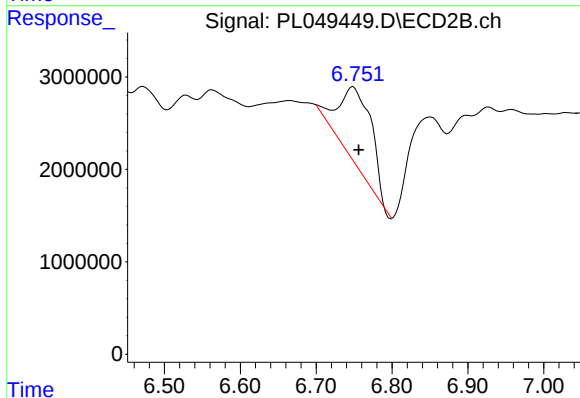


#16 4,4'-DDD

R.T.: 6.749 min
Delta R.T.: -0.007 min
Response: 25257815
Conc: 9.60 ng/ml

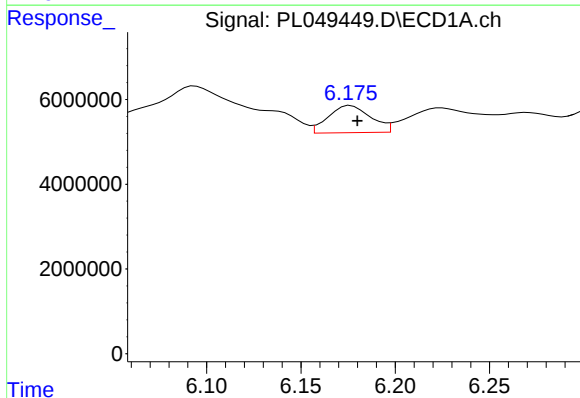


#17 4,4'-DDT

R.T.: 6.176 min
Delta R.T.: -0.003 min
Response: 10008004
Conc: 0.81 ng/ml

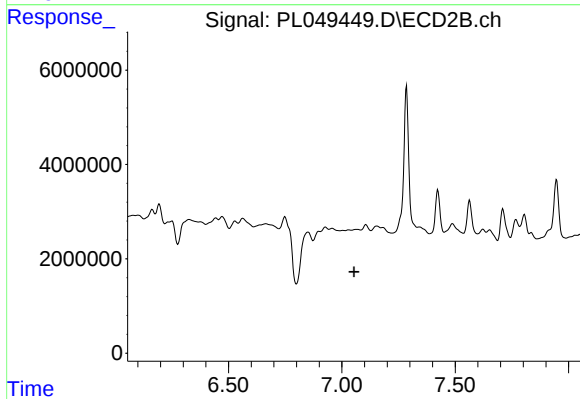

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.054 min
Response: 0
Conc: N.D.

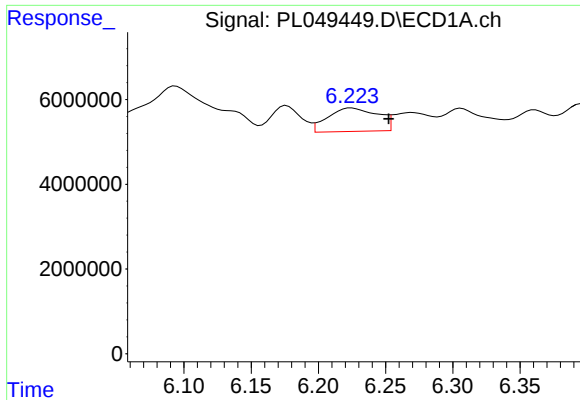

#18 Endrin aldehyde


R.T.: 6.225 min
Delta R.T.: -0.028 min
Response: 14253195
Conc: 1.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
BAT-B02

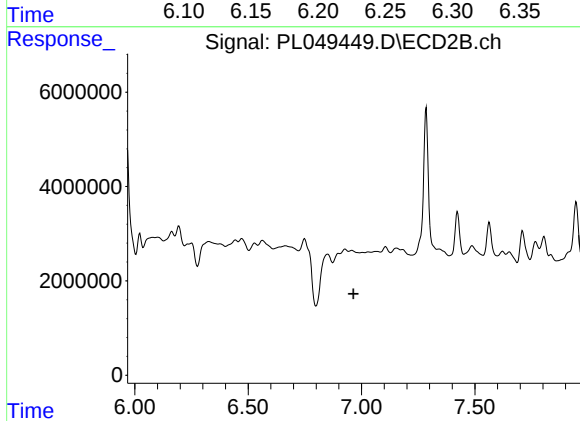


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.965 min
Response: 0
Conc: N.D.

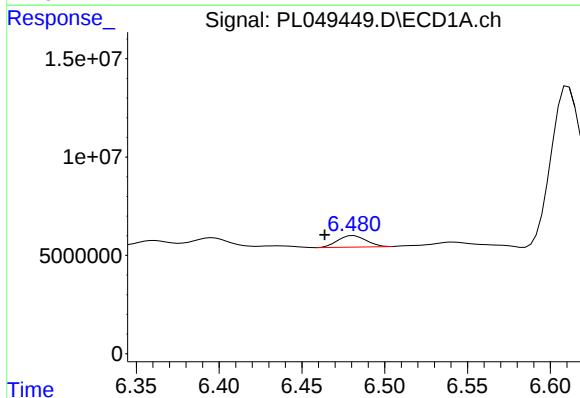


#19 Endosulfan Sulfate

R.T.: 6.481 min
Delta R.T.: 0.018 min
Response: 6952625
Conc: 0.54 ng/ml

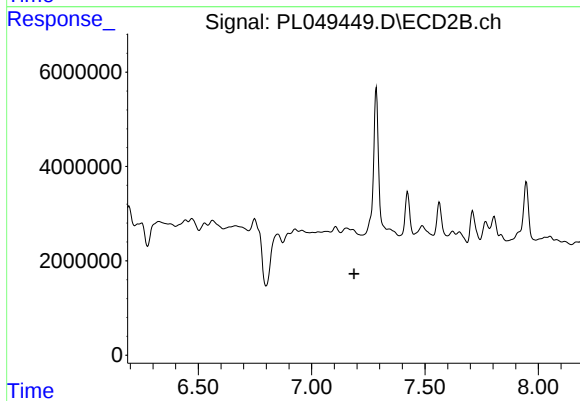

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

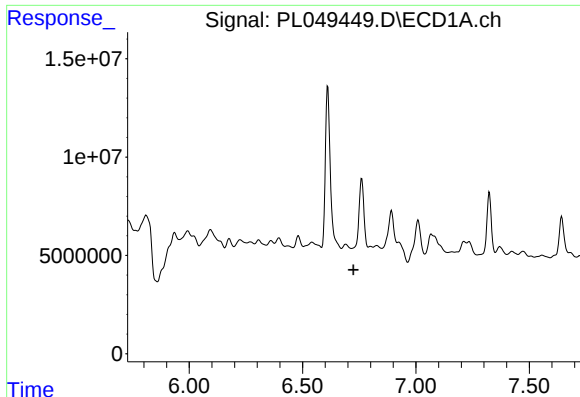

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.725 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BAT-B02

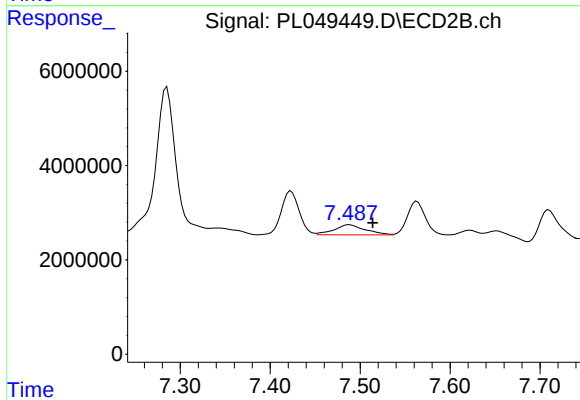


#20 Methoxychlor

R.T.: 7.488 min
Delta R.T.: -0.026 min
Response: 5128659
Conc: 3.09 ng/ml

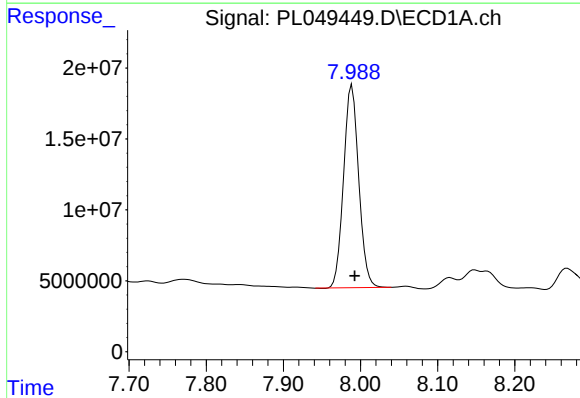

#28 Decachlorobiphenyl

R.T.: 7.989 min
Delta R.T.: -0.003 min
Response: 193811460
Conc: 15.24 ng/ml

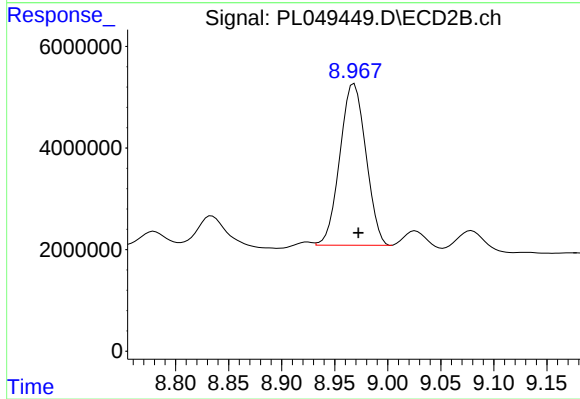

#28 Decachlorobiphenyl

R.T.: 8.968 min
Delta R.T.: -0.004 min
Response: 54280068
Conc: 16.25 ng/ml