

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061219\
 Data File : PL049455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2019 15:04
 Operator : SM\AJ
 Sample : K3285-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 M-1-OW(0-10)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 01:36:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.935	179.6E6	49644108	16.300	17.184
28)	SA Decachlor...	7.989	8.970	174.0E6	50529535	13.687	15.130
Target Compounds							
10)	B gamma-Chl...	5.230f	6.032	51966595	3615440	3.255	1.045 #
11)	B alpha-Chl...	5.264	6.106	16461945	15797940	1.054	4.554 #
12)	B 4,4'-DDE	5.433	6.263	68007804	16215416	4.348	4.940
14)	MA Endrin	5.813	0.000	7602302	0	0.527	N.D. #
16)	A 4,4'-DDD	0.000	6.755	0	5582691	N.D.	2.122 #
17)	MA 4,4'-DDT	6.176	7.051	40270954	7218103	3.271	2.575
18)	B Endrin al...	6.275f	0.000	9620474	0	0.879	N.D. #
20)	A Methoxychlor	6.702f	0.000	10907744	0	1.701	N.D. #
22)	Mirex	0.000	8.110	0	1881227	N.D.	0.724 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061219\
Data File : PL049455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2019 15:04
Operator : SM\AJ
Sample : K3285-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
M-1-OW(0-10)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 01:36:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

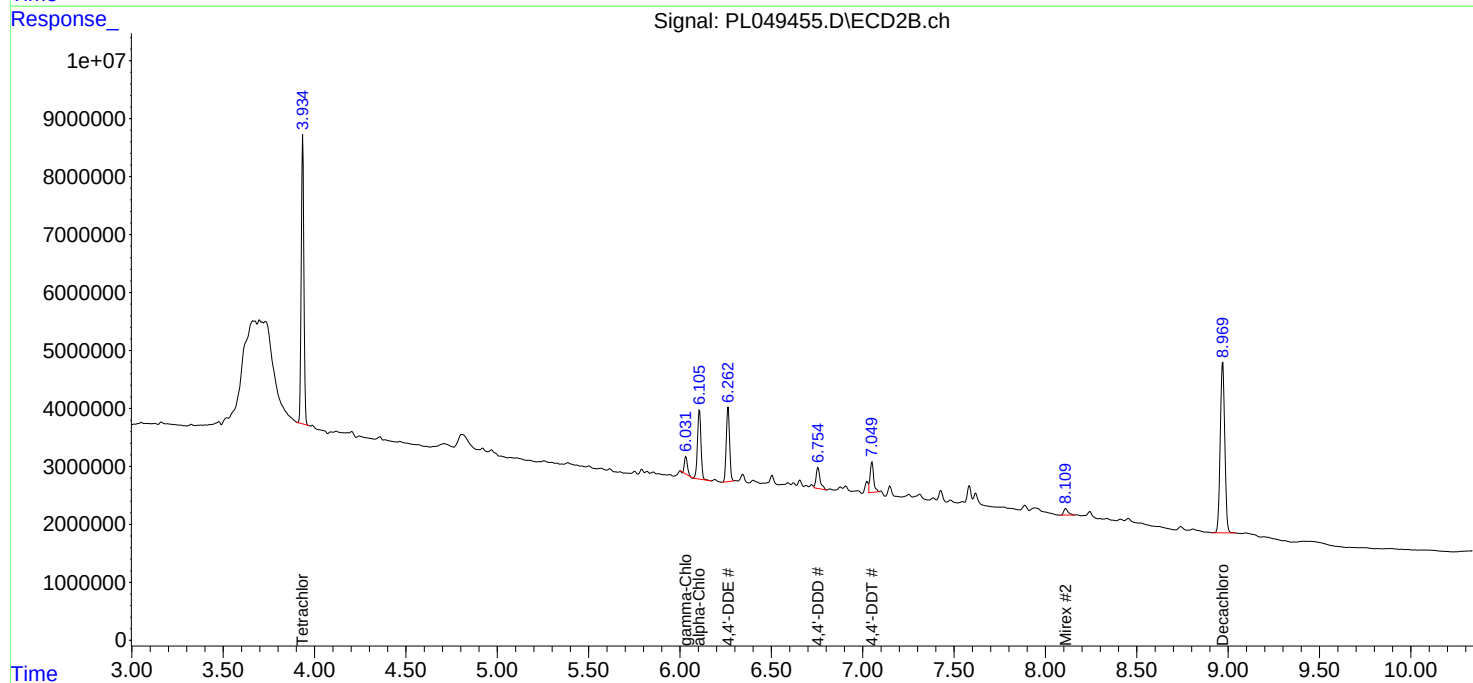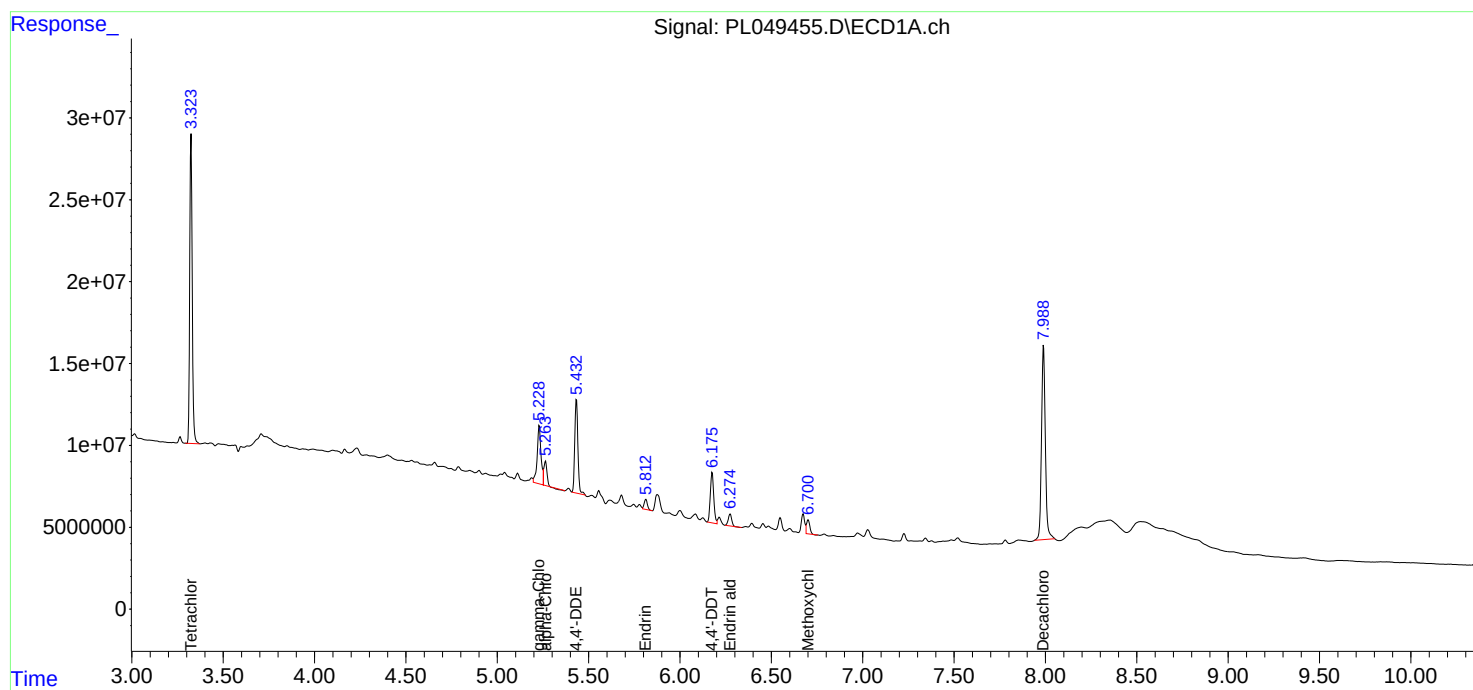


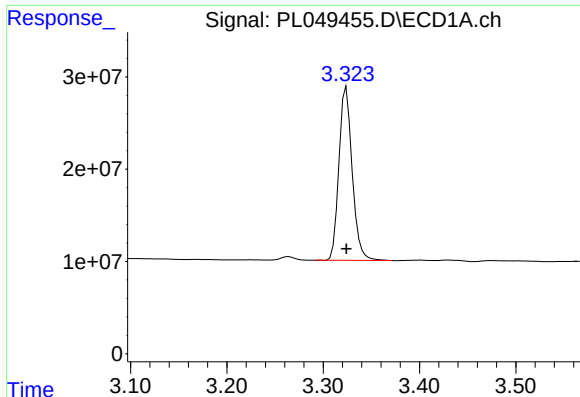

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: 0.000 min
Response: 179608610
Conc: 16.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
M-1-OW(0-10)

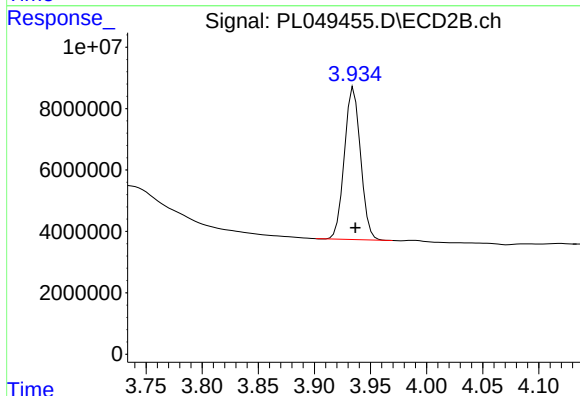


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.001 min
Response: 49644108
Conc: 17.18 ng/ml

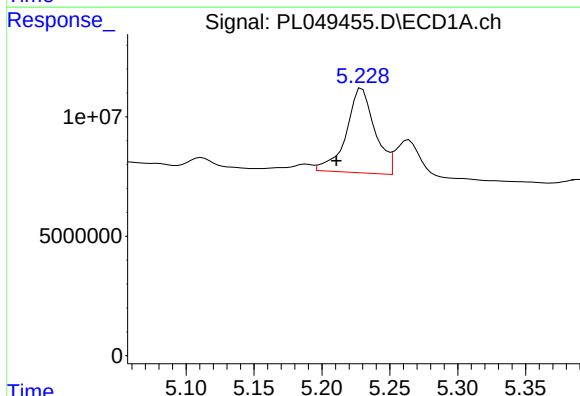


#10 gamma-Chlordane

R.T.: 5.230 min
Delta R.T.: 0.019 min
Response: 51966595
Conc: 3.26 ng/ml

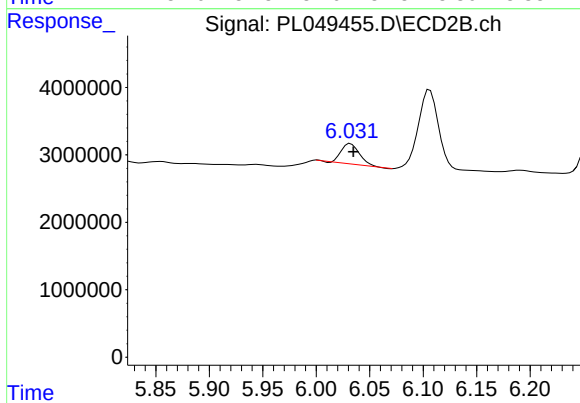

#10 gamma-Chlordane


R.T.: 6.032 min
Delta R.T.: -0.003 min
Response: 3615440
Conc: 1.05 ng/ml

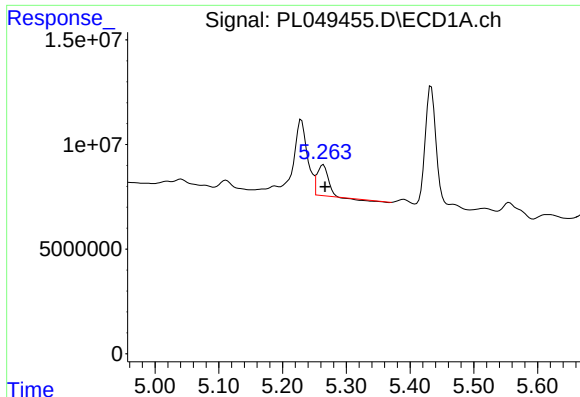

#11 alpha-Chlordane


R.T.: 5.264 min
Delta R.T.: -0.003 min
Response: 16461945
Conc: 1.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
M-1-OW(0-10)

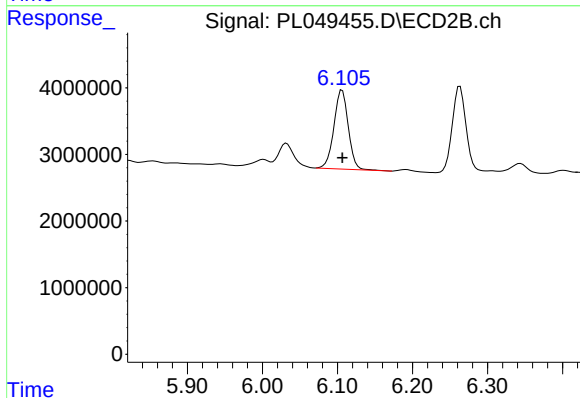


#11 alpha-Chlordane

R.T.: 6.106 min
Delta R.T.: 0.000 min
Response: 15797940
Conc: 4.55 ng/ml

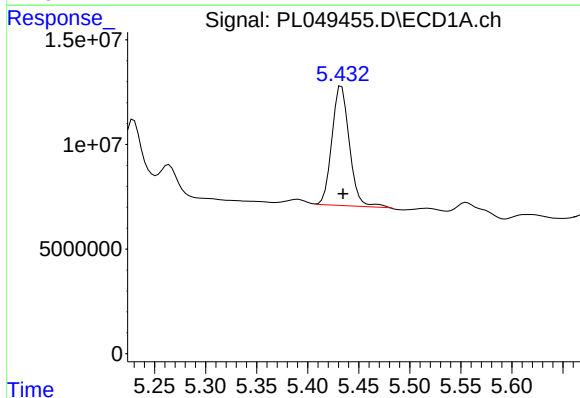


#12 4,4'-DDE

R.T.: 5.433 min
Delta R.T.: -0.002 min
Response: 68007804
Conc: 4.35 ng/ml

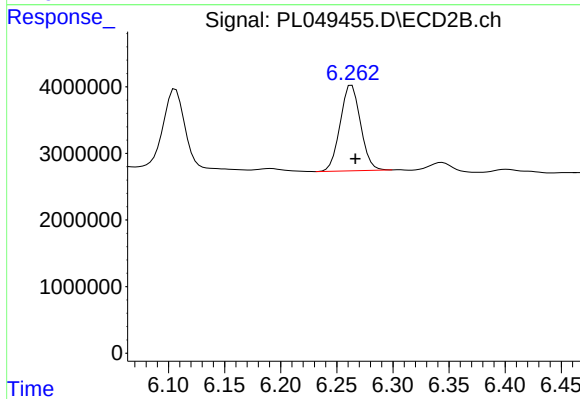

#12 4,4'-DDE


R.T.: 6.263 min
Delta R.T.: -0.003 min
Response: 16215416
Conc: 4.94 ng/ml

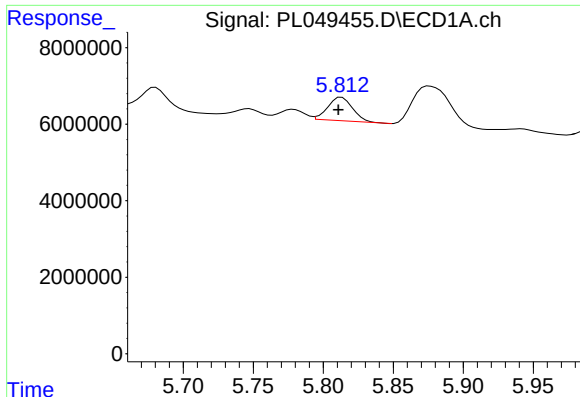

#14 Endrin


R.T.: 5.813 min
Delta R.T.: 0.002 min
Response: 7602302
Conc: 0.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
M-1-OW(0-10)

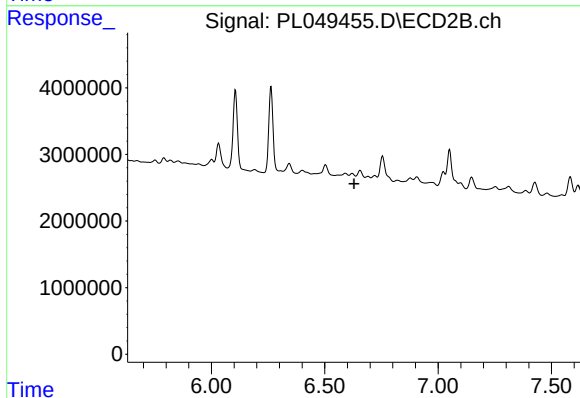


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.630 min
Response: 0
Conc: N.D.

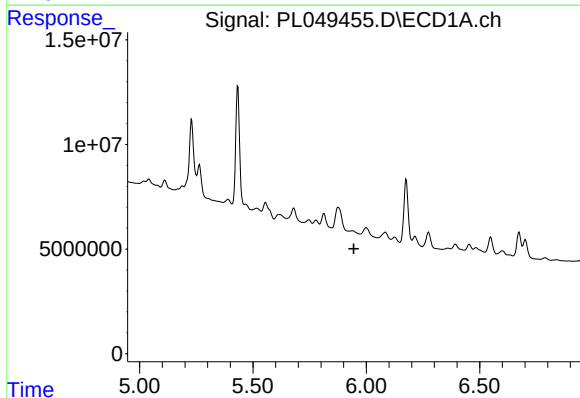


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.945 min
Response: 0
Conc: N.D.

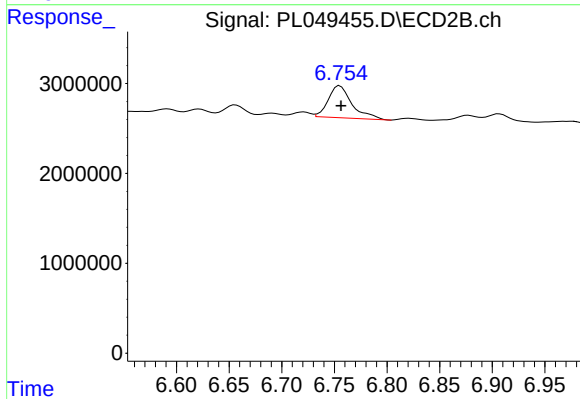

#16 4,4'-DDD


R.T.: 6.755 min
Delta R.T.: -0.001 min
Response: 5582691
Conc: 2.12 ng/ml

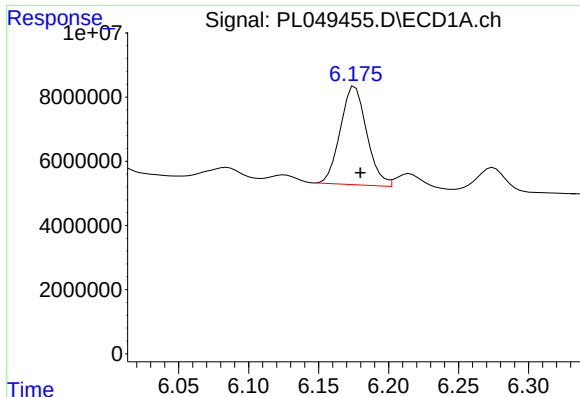

#17 4,4'-DDT


R.T.: 6.176 min
Delta R.T.: -0.004 min
Response: 40270954
Conc: 3.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
M-1-OW(0-10)

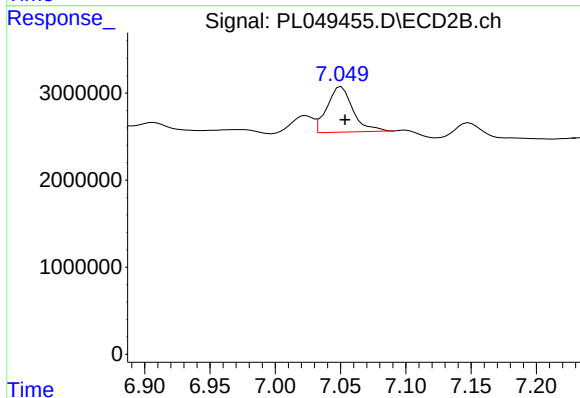


#17 4,4'-DDT

R.T.: 7.051 min
Delta R.T.: -0.003 min
Response: 7218103
Conc: 2.57 ng/ml

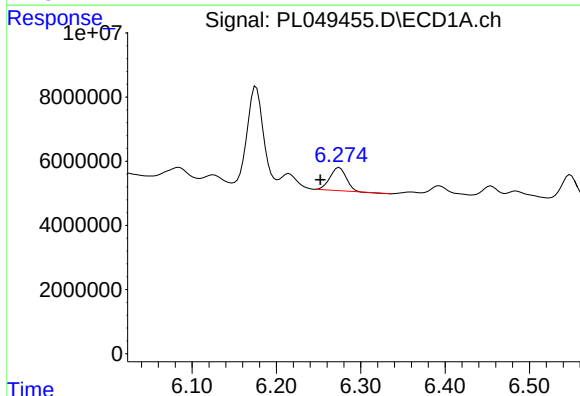


#18 Endrin aldehyde

R.T.: 6.275 min
Delta R.T.: 0.023 min
Response: 9620474
Conc: 0.88 ng/ml

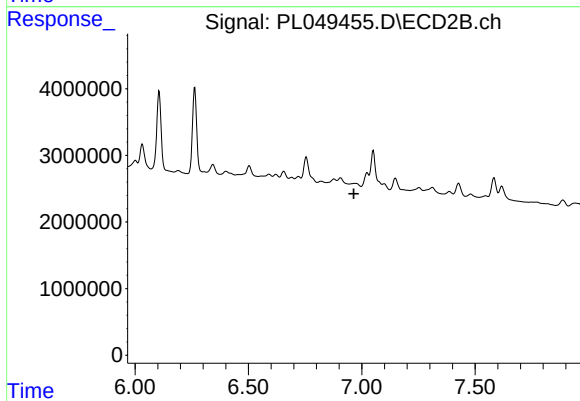

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.965 min
Response: 0
Conc: N.D.

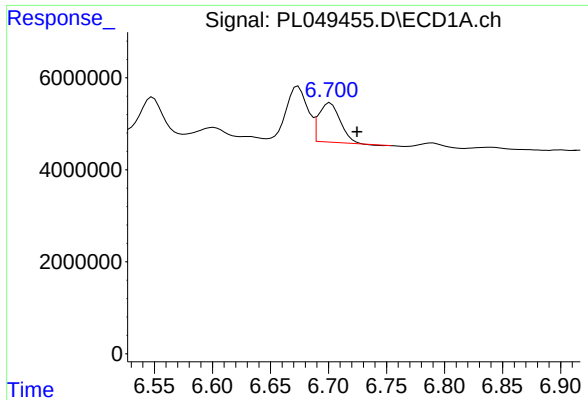

#20 Methoxychlor


R.T.: 6.702 min
Delta R.T.: -0.023 min
Response: 10907744
Conc: 1.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
M-1-OW(0-10)

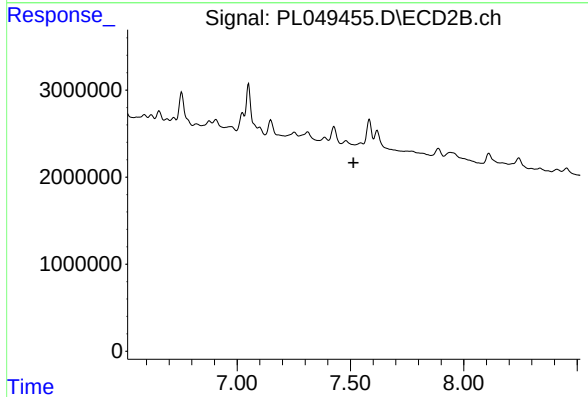


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.514 min
Response: 0
Conc: N.D.

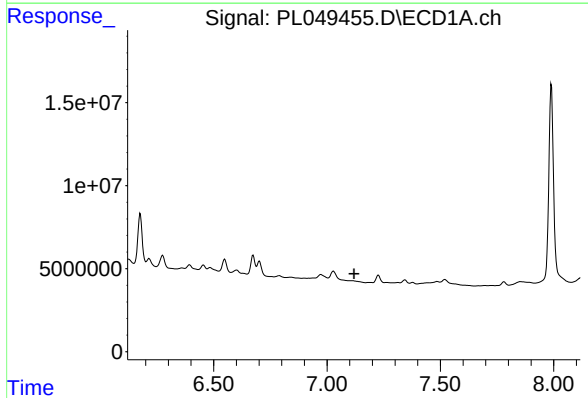


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.120 min
Response: 0
Conc: N.D.

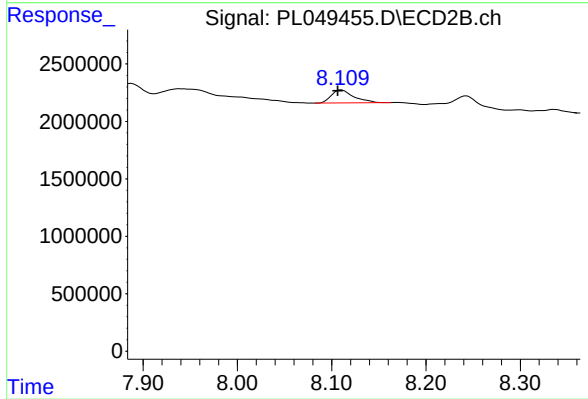

#22 Mirex


R.T.: 8.110 min
Delta R.T.: 0.004 min
Response: 1881227
Conc: 0.72 ng/ml

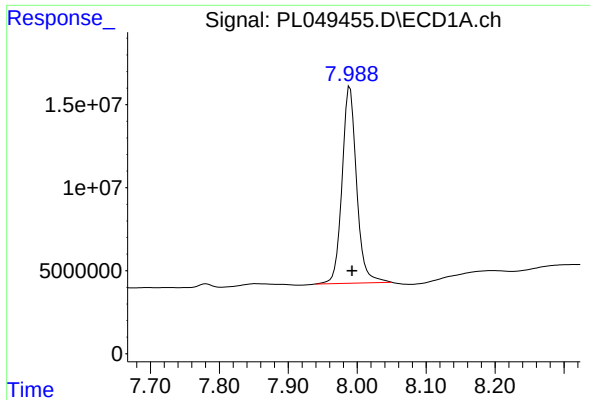

#28 Decachlorobiphenyl

R.T.: 7.989 min
Delta R.T.: -0.003 min
Response: 174038551
Conc: 13.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
M-1-OW(0-10)

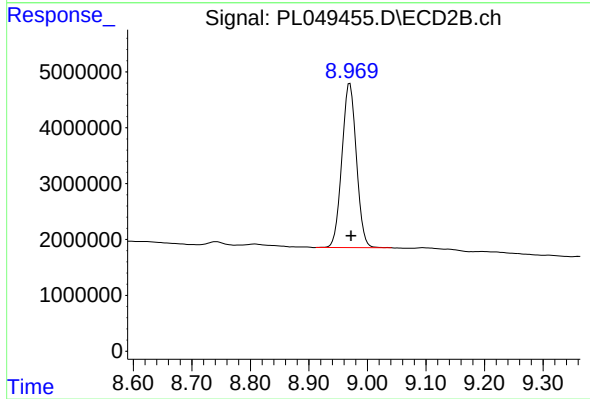

#28 Decachlorobiphenyl

R.T.: 8.970 min
Delta R.T.: -0.002 min
Response: 50529535
Conc: 15.13 ng/ml