

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061219\
 Data File : PL049456.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2019 15:19
 Operator : SM\AJ
 Sample : K3303-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BAT-B03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 01:37:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.935	183.1E6	49993031	16.620	17.304
28)	SA Decachlor...	7.989	8.968	153.0E6	47670714	12.030	14.274
Target Compounds							
6)	B beta-BHC	0.000	4.807f	0	2536308	N.D.	1.472 #
20)	A Methoxychlor	6.702f	0.000	10105820	0	1.576	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061219\
Data File : PL049456.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2019 15:19
Operator : SM\AJ
Sample : K3303-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
BAT-B03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 01:37:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

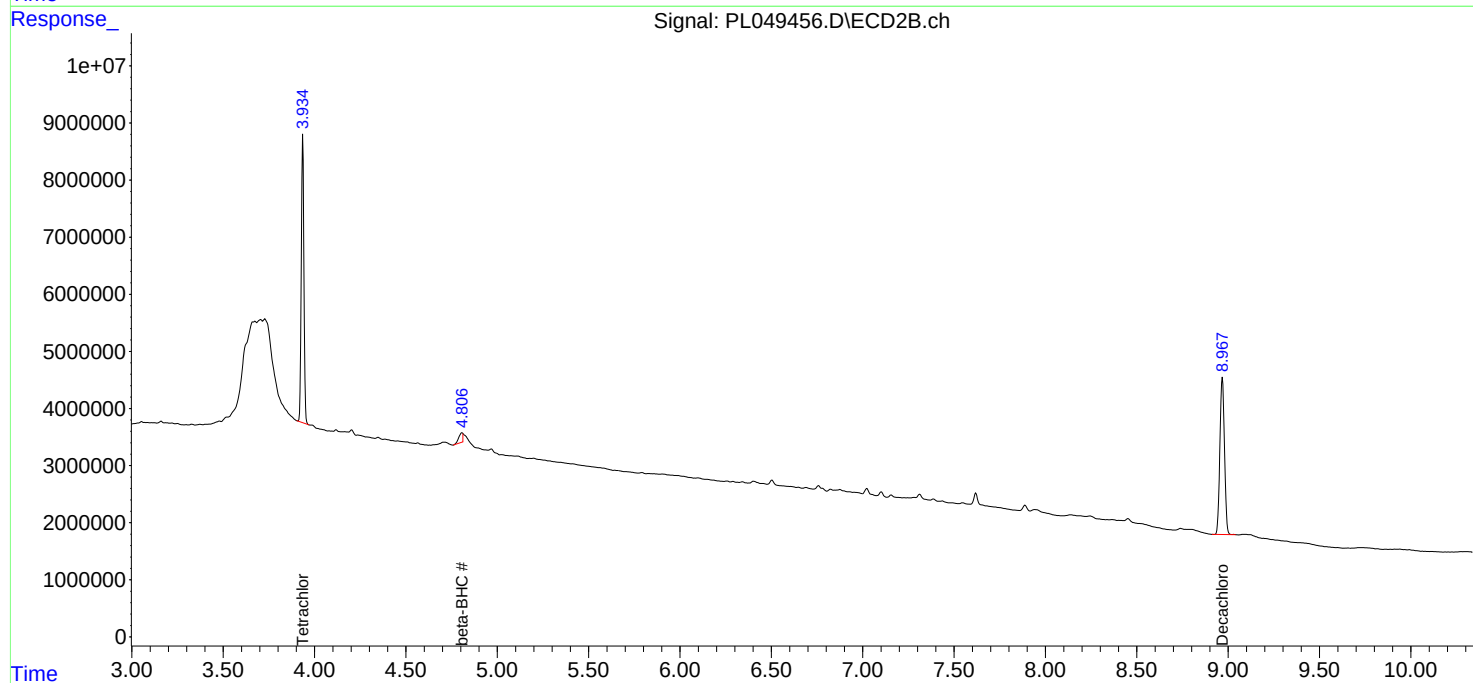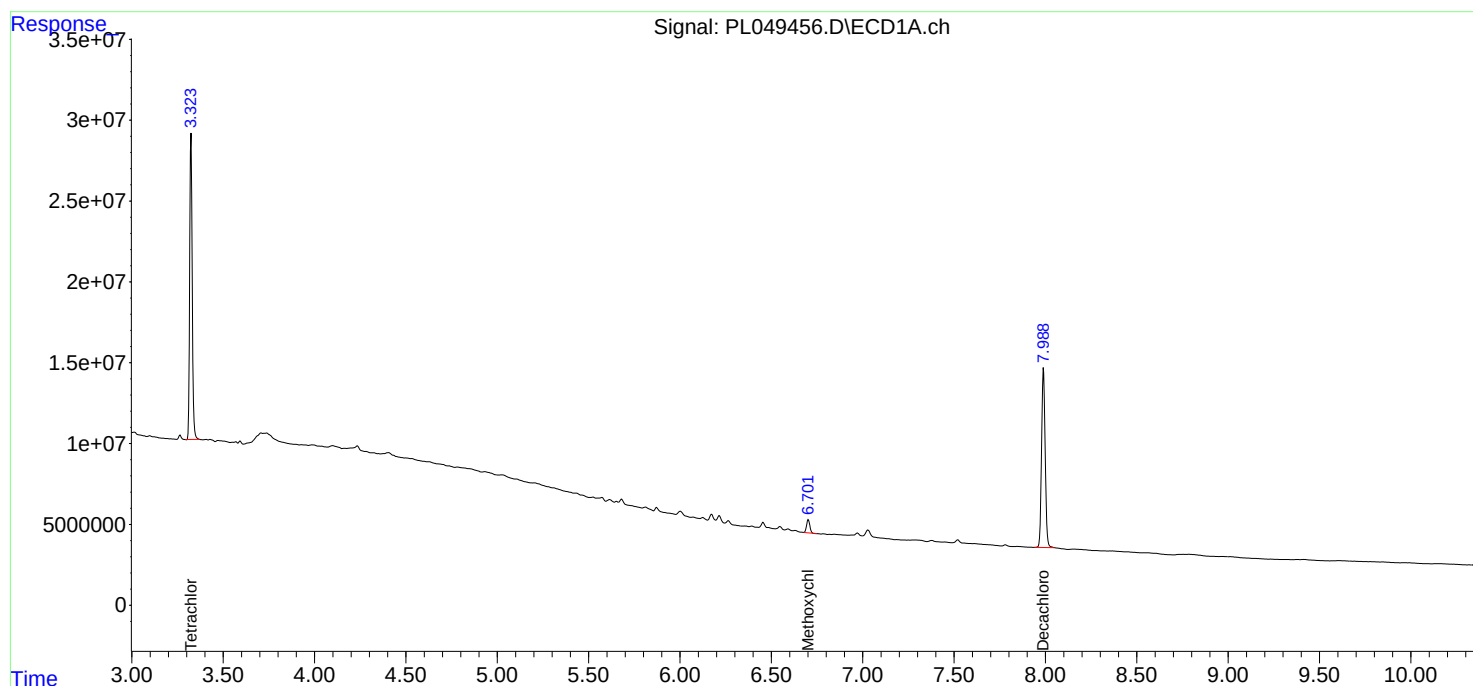


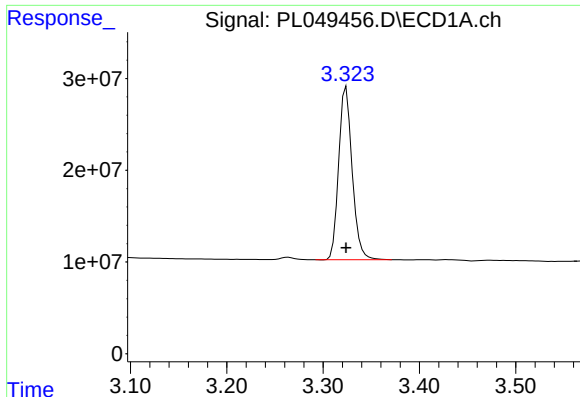

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: 0.000 min
Response: 183137051
Conc: 16.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
BAT-B03

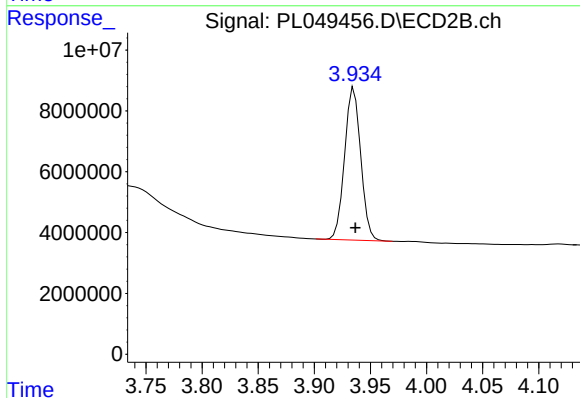


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.001 min
Response: 49993031
Conc: 17.30 ng/ml

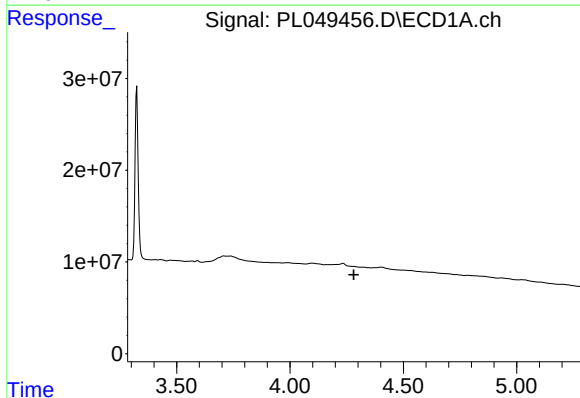


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.282 min
Response: 0
Conc: N.D.

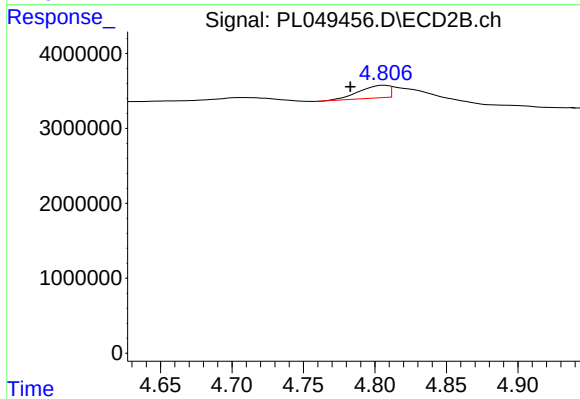

#6 beta-BHC


R.T.: 4.807 min
Delta R.T.: 0.024 min
Response: 2536308
Conc: 1.47 ng/ml

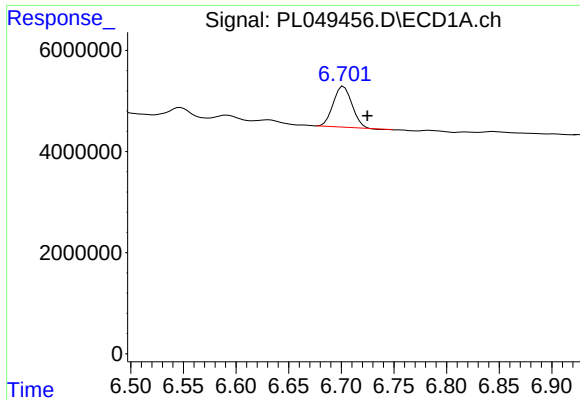

#20 Methoxychlor


R.T.: 6.702 min
Delta R.T.: -0.023 min
Response: 10105820
Conc: 1.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
BAT-B03

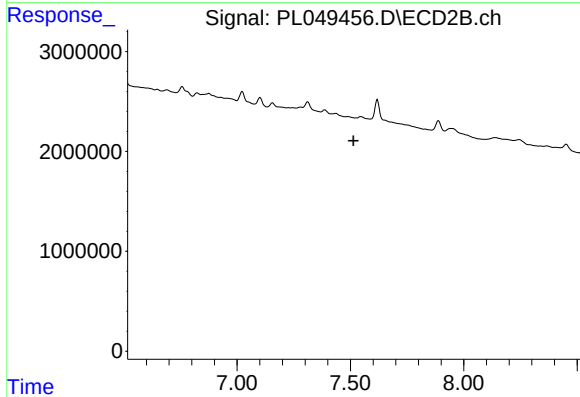


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.514 min
Response: 0
Conc: N.D.

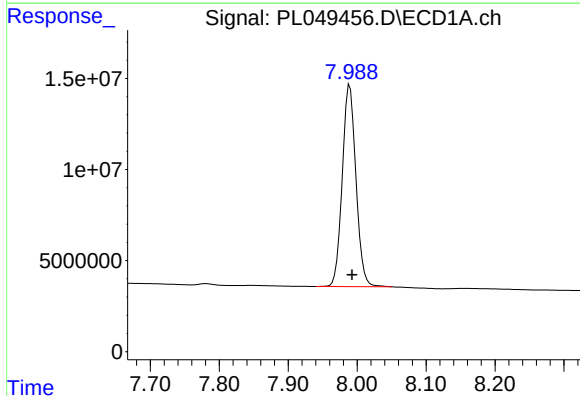

#28 Decachlorobiphenyl

R.T.: 7.989 min
Delta R.T.: -0.003 min
Response: 152964237
Conc: 12.03 ng/ml

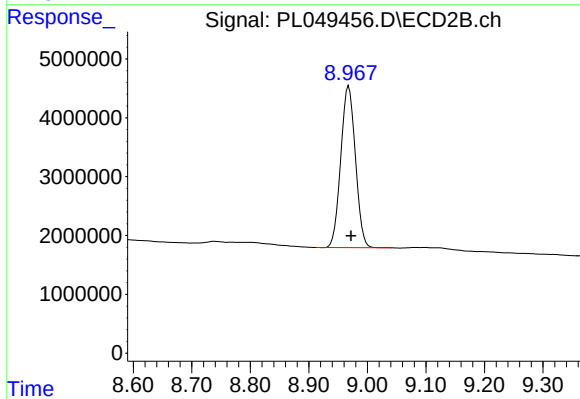

#28 Decachlorobiphenyl

R.T.: 8.968 min
Delta R.T.: -0.004 min
Response: 47670714
Conc: 14.27 ng/ml