

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
 Data File : PL067318.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2021 11:06
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 08:52:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.481	5.531	10735741	17488053	19.527	18.550
28)	SA Decachlor...	10.226	11.434	14428096	20490512	20.359	20.572
Target Compounds							
4)	MA Heptachlor	5.991f	0.000	499122	0	0.662	N.D. #
5)	MB Aldrin	0.000	7.518	0	3133586	N.D.	2.895 #
6)	B beta-BHC	5.991	0.000	499122	0	1.395	N.D. #
7)	B delta-BHC	0.000	7.000f	0	1467640	N.D.	1.249 #
9)	A Endosulfan I	7.306	0.000	58294	0	0.087	N.D. #
15)	B Endosulfa...	8.178	9.131f	1255822	917792	2.039	1.151 #
21)	B Endrin ke...	9.131	0.000	119575	0	0.157	N.D. #
24)	Chlordane-2	6.489	7.518f	219309	3133586	8.190	85.978 #
27)	Chlordane-5	8.178	0.000	1255822	0	57.398	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
Data File : PL067318.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2021 11:06
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 08:52:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

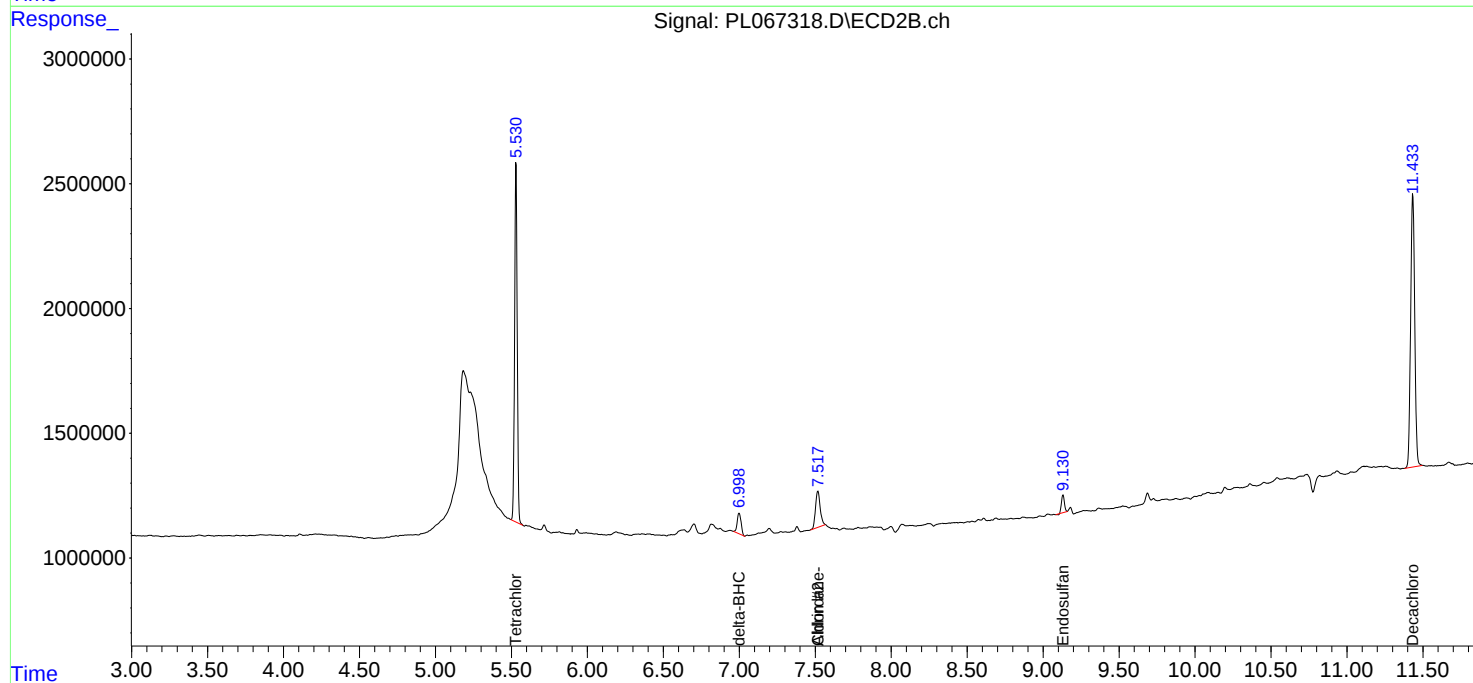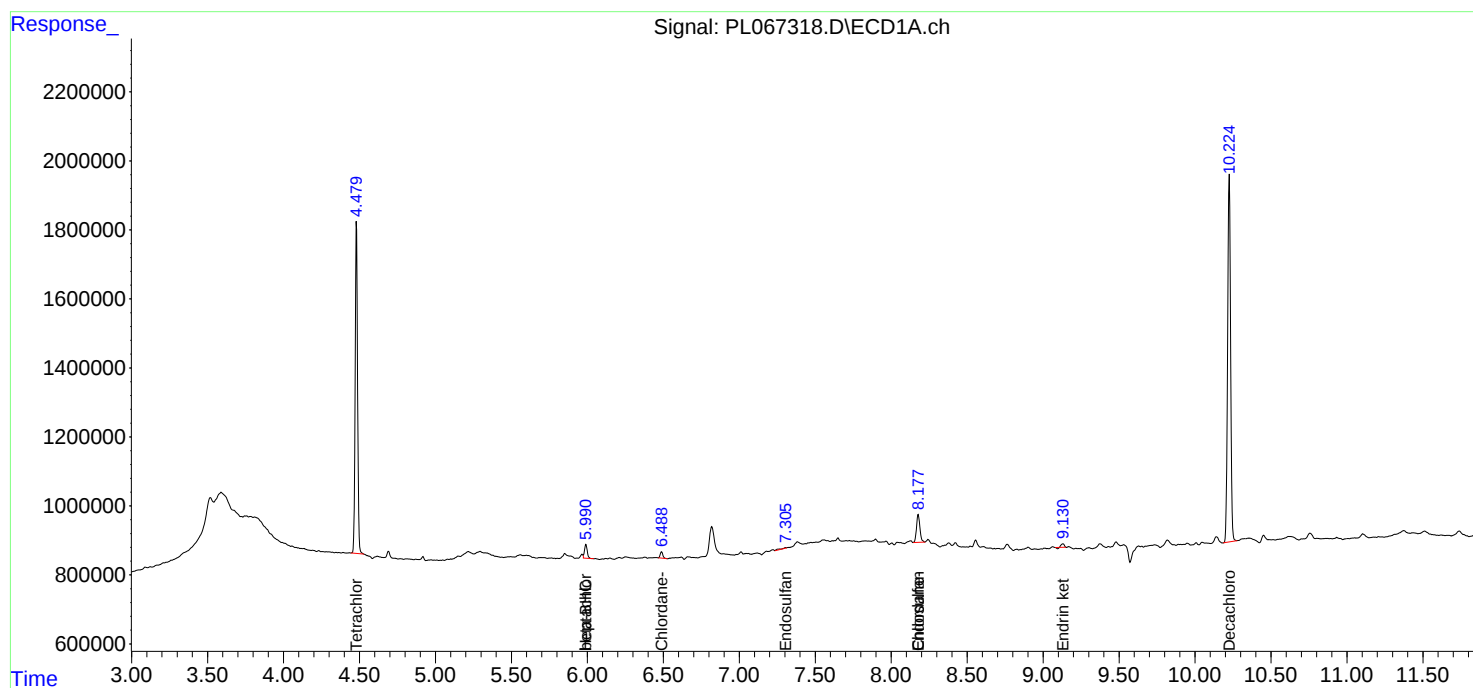


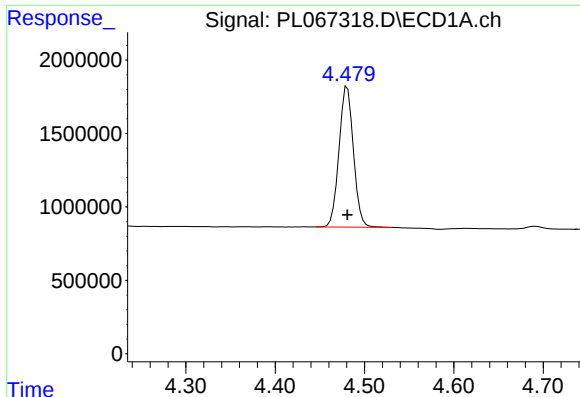

#1 Tetrachloro-m-xylene


R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 10735741
Conc: 19.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

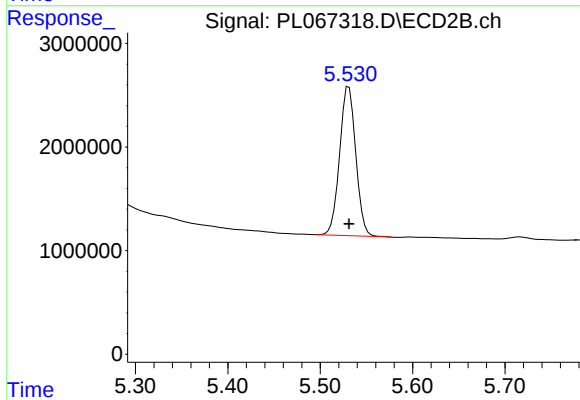


#1 Tetrachloro-m-xylene

R.T.: 5.531 min
Delta R.T.: 0.000 min
Response: 17488053
Conc: 18.55 ng/ml

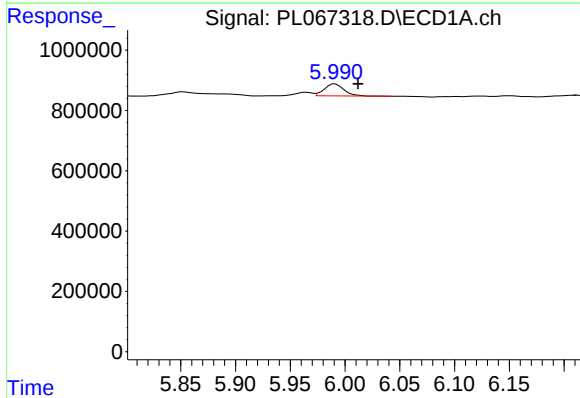


#4 Heptachlor

R.T.: 5.991 min
Delta R.T.: -0.021 min
Response: 499122
Conc: 0.66 ng/ml

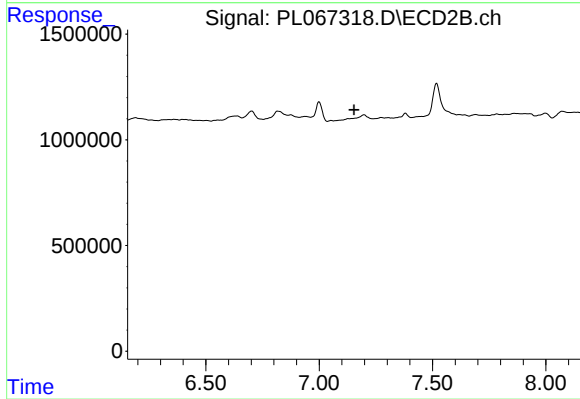

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.155 min
Response: 0
Conc: N.D.

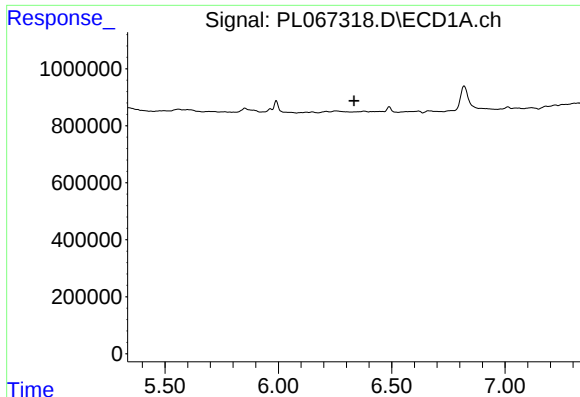

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 6.334 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

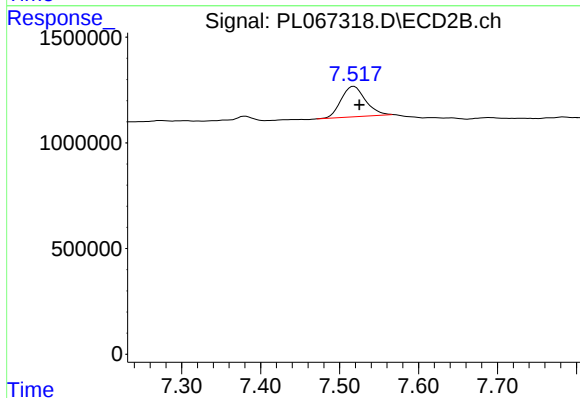


#5 Aldrin

R.T.: 7.518 min
Delta R.T.: -0.007 min
Response: 3133586
Conc: 2.90 ng/ml

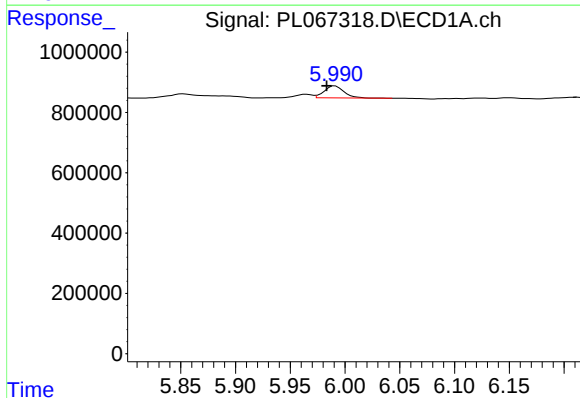


#6 beta-BHC

R.T.: 5.991 min
Delta R.T.: 0.008 min
Response: 499122
Conc: 1.39 ng/ml

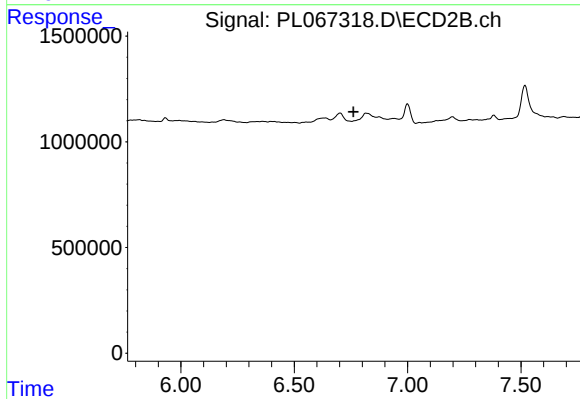

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.762 min
Response: 0
Conc: N.D.

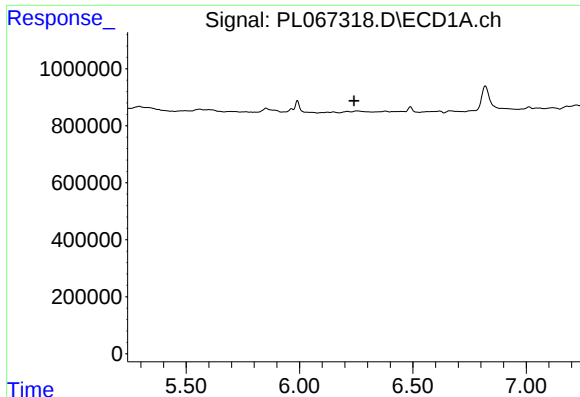

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

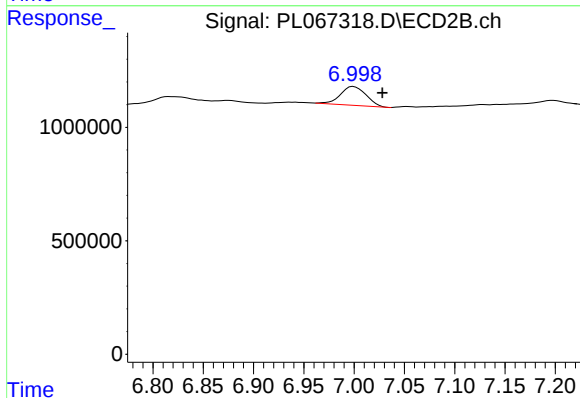


#7 delta-BHC

R.T.: 7.000 min
Delta R.T.: -0.029 min
Response: 1467640
Conc: 1.25 ng/ml

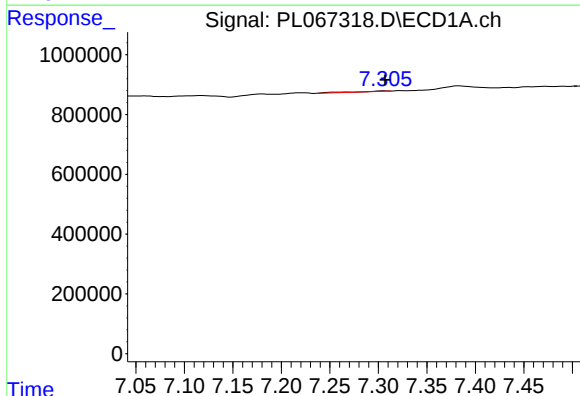


#9 Endosulfan I

R.T.: 7.306 min
Delta R.T.: 0.000 min
Response: 58294
Conc: 0.09 ng/ml

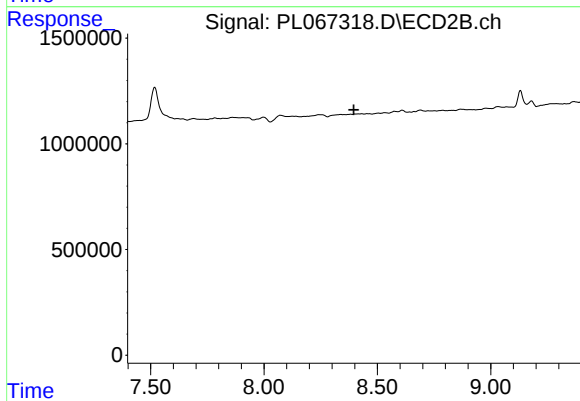

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 8.397 min
Response: 0
Conc: N.D.

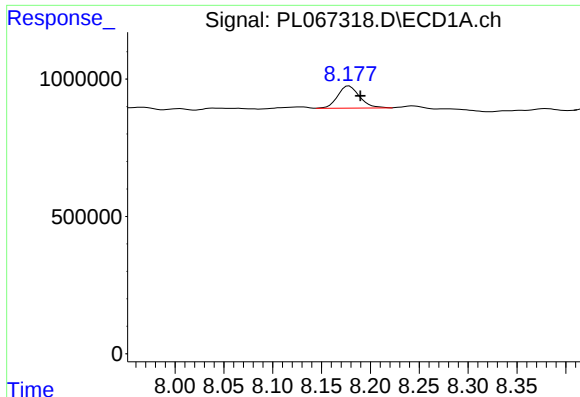

#15 Endosulfan II


R.T.: 8.178 min
Delta R.T.: -0.012 min
Response: 1255822
Conc: 2.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

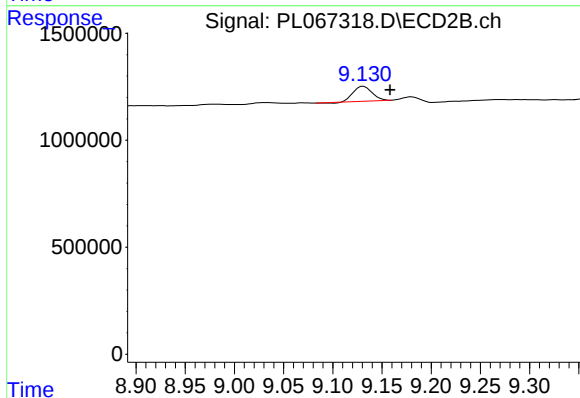


#15 Endosulfan II

R.T.: 9.131 min
Delta R.T.: -0.027 min
Response: 917792
Conc: 1.15 ng/ml

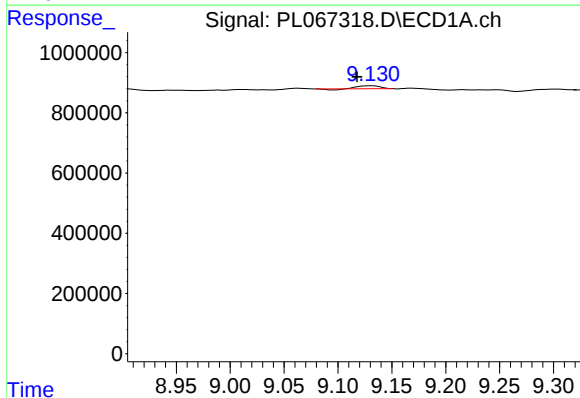


#21 Endrin ketone

R.T.: 9.131 min
Delta R.T.: 0.014 min
Response: 119575
Conc: 0.16 ng/ml

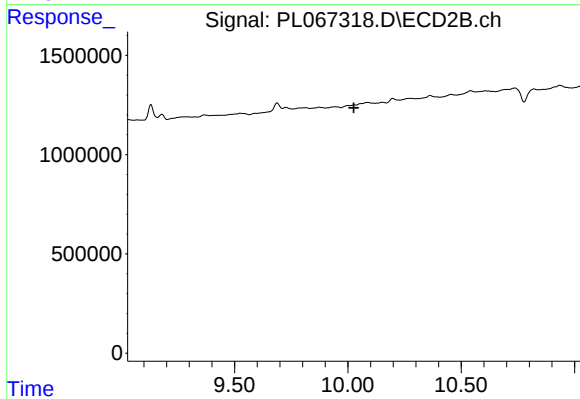

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 10.027 min
Response: 0
Conc: N.D.

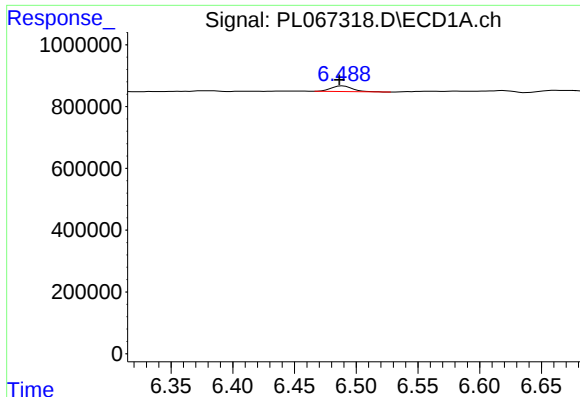

#24 Chlordane-2


R.T.: 6.489 min
Delta R.T.: 0.003 min
Response: 219309
Conc: 8.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

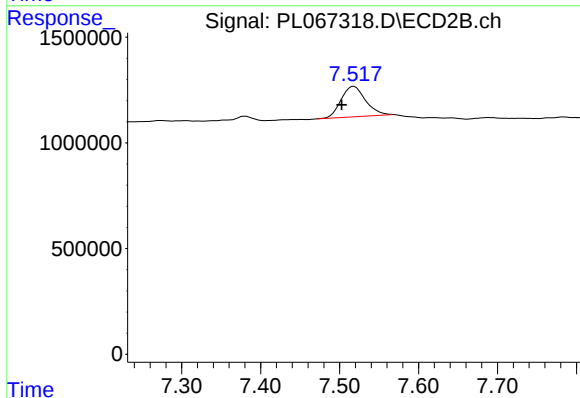


#24 Chlordane-2

R.T.: 7.518 min
Delta R.T.: 0.015 min
Response: 3133586
Conc: 85.98 ng/ml

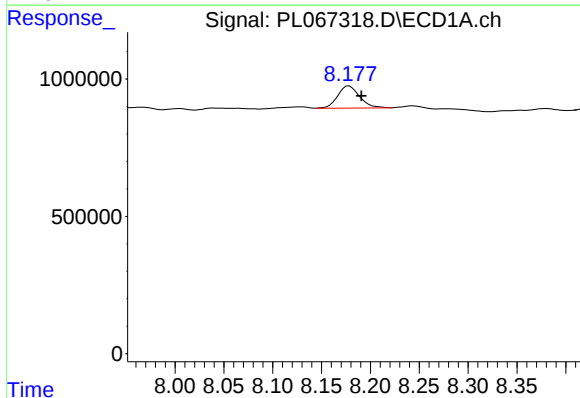


#27 Chlordane-5

R.T.: 8.178 min
Delta R.T.: -0.013 min
Response: 1255822
Conc: 57.40 ng/ml

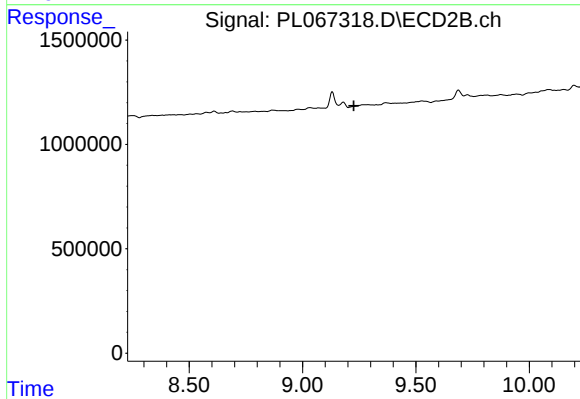

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

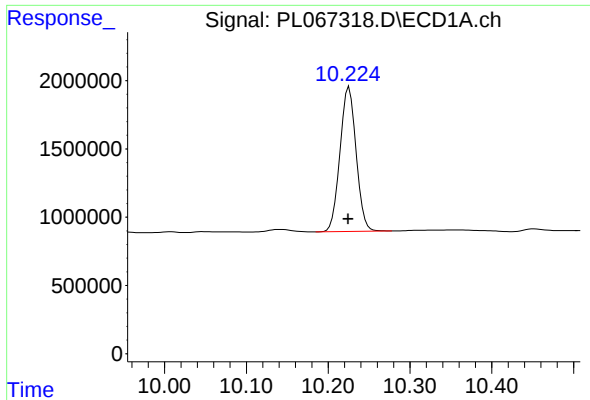

#28 Decachlorobiphenyl

R.T.: 10.226 min
Delta R.T.: 0.001 min
Response: 14428096
Conc: 20.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

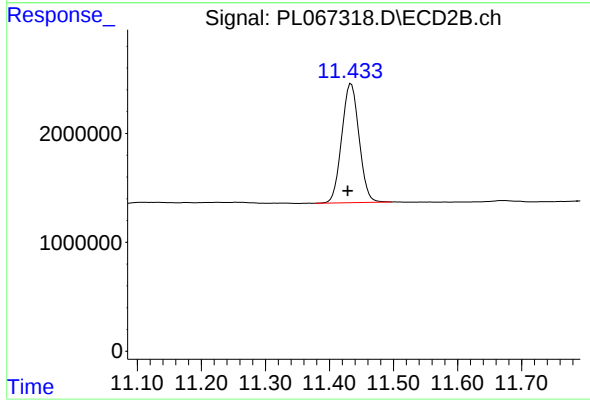

#28 Decachlorobiphenyl

R.T.: 11.434 min
Delta R.T.: 0.005 min
Response: 20490512
Conc: 20.57 ng/ml