

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
 Data File : PL067323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2021 12:29
 Operator : AR\AJ
 Sample : M2625-18
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 08:53:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	5.528	12646995	21776491	23.004	23.099
28)	SA Decachlor...	10.221	11.425	16612148	24305508	23.441	24.402
Target Compounds							
5)	MB Aldrin	0.000	7.515	0	1818518	N.D.	1.680 #
7)	B delta-BHC	0.000	7.001f	0	1059597	N.D.	0.901 #
8)	B Heptachlo...	0.000	7.995	0	809010	N.D.	0.808 #
14)	MA Endrin	7.895f	0.000	521025	0	0.795	N.D. #
15)	B Endosulfa...	8.175	9.175f	542378	932884	0.881	1.170 #
18)	B Endrin al...	8.377	0.000	713918	0	1.410	N.D. #
21)	B Endrin ke...	9.127	10.003f	657407	317445	0.863	0.350 #
24)	Chlordane-2	0.000	7.515	0	1818518	N.D.	49.896 #
27)	Chlordane-5	8.175f	0.000	542378	0	24.790	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
Data File : PL067323.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2021 12:29
Operator : AR\AJ
Sample : M2625-18
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 08:53:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

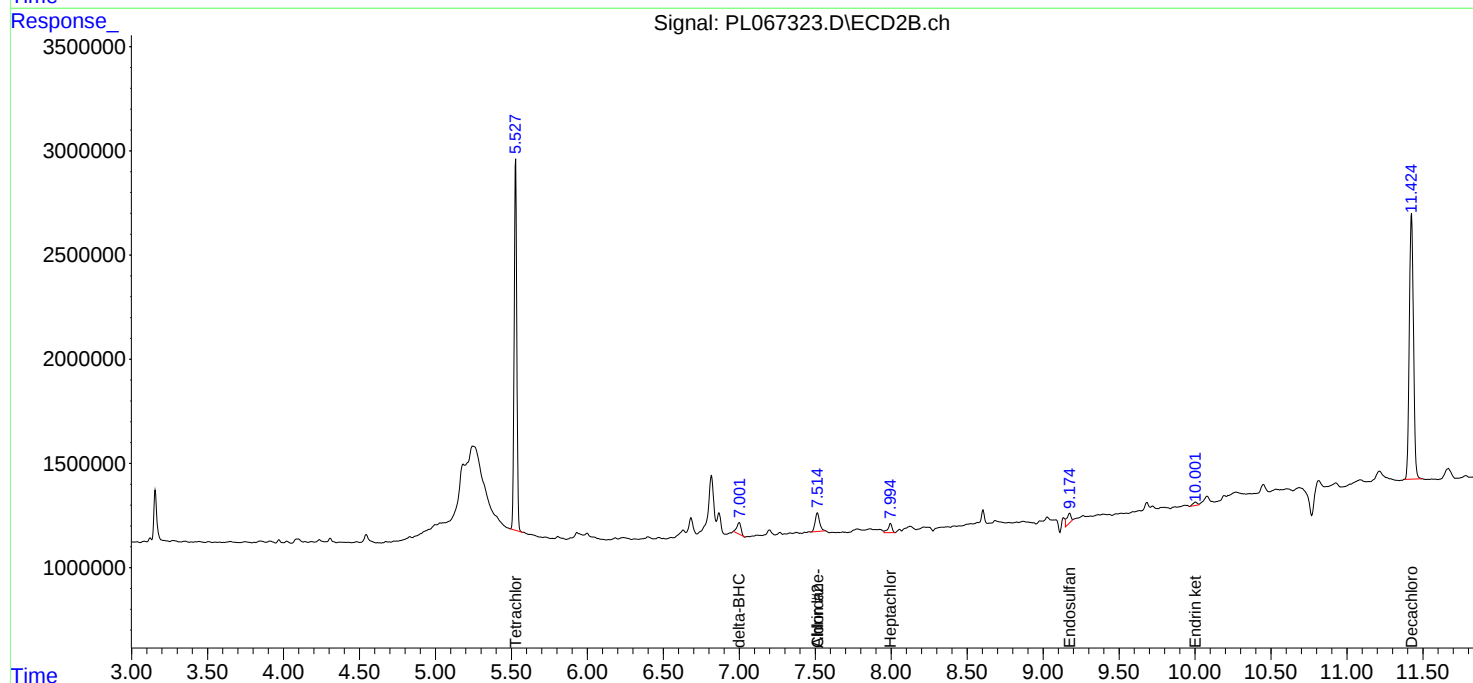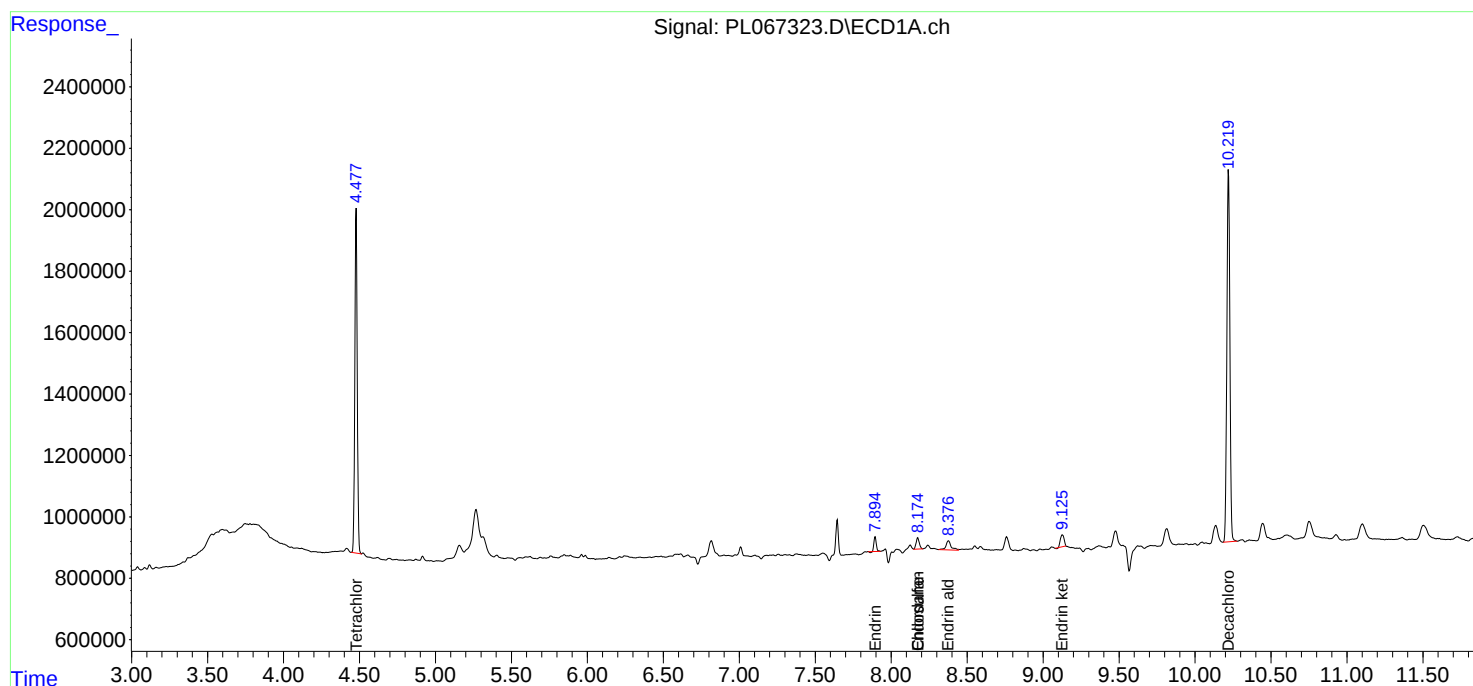


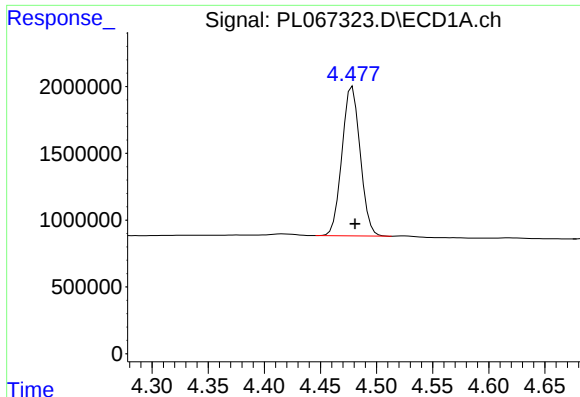

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: -0.002 min
Response: 12646995
Conc: 23.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

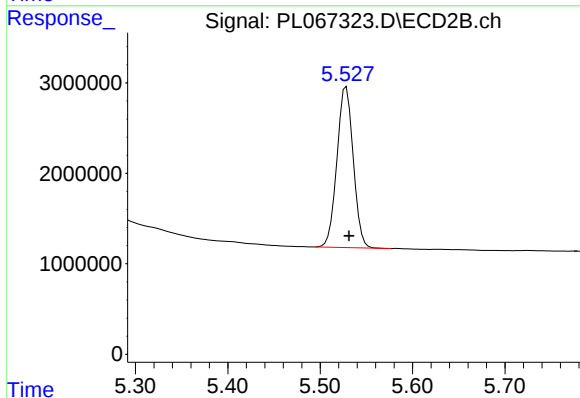


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 21776491
Conc: 23.10 ng/ml

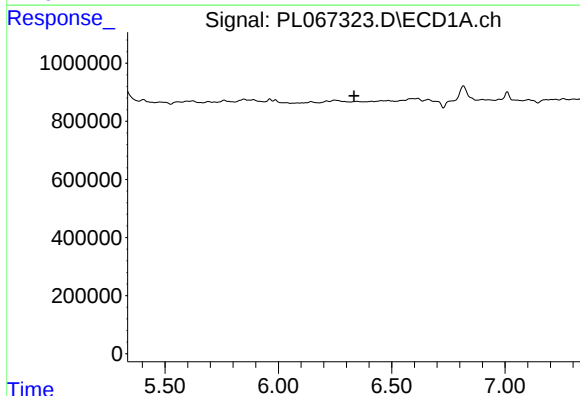


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.334 min
Response: 0
Conc: N.D.

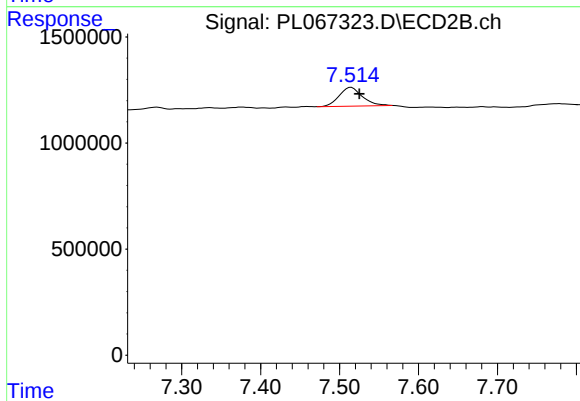

#5 Aldrin


R.T.: 7.515 min
Delta R.T.: -0.010 min
Response: 1818518
Conc: 1.68 ng/ml

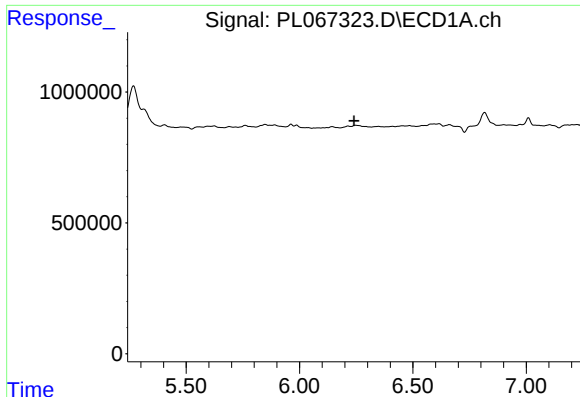

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

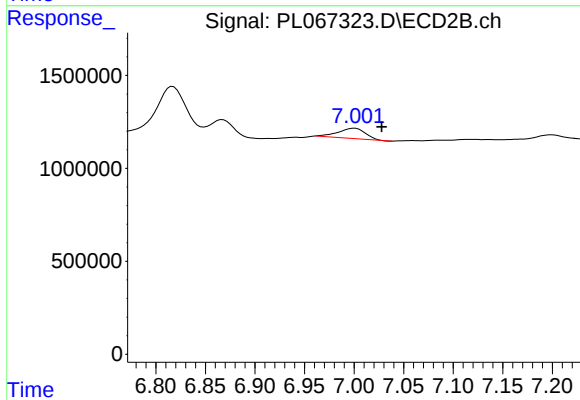


#7 delta-BHC

R.T.: 7.001 min
Delta R.T.: -0.027 min
Response: 1059597
Conc: 0.90 ng/ml

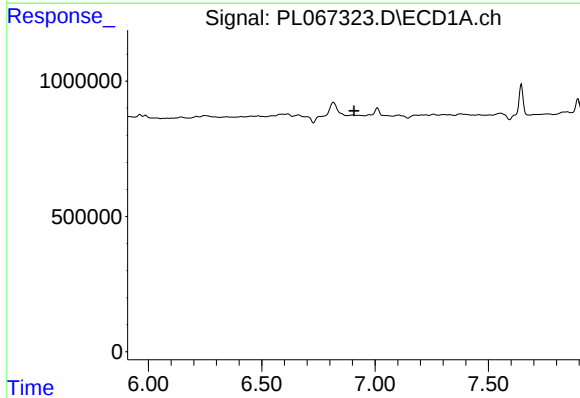


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.907 min
Response: 0
Conc: N.D.

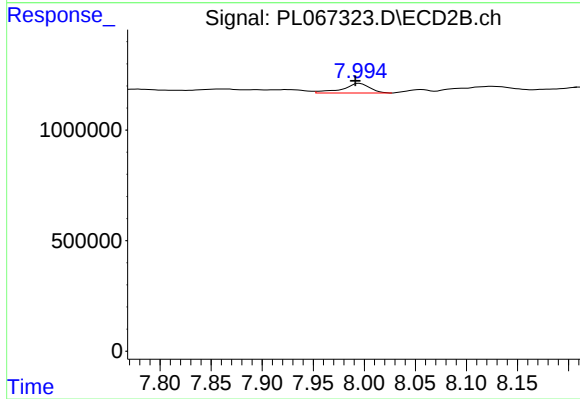

#8 Heptachlor epoxide


R.T.: 7.995 min
Delta R.T.: 0.004 min
Response: 809010
Conc: 0.81 ng/ml

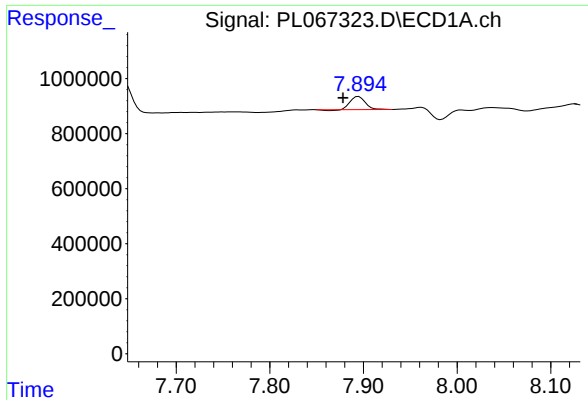

#14 Endrin


R.T.: 7.895 min
Delta R.T.: 0.017 min
Response: 521025
Conc: 0.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

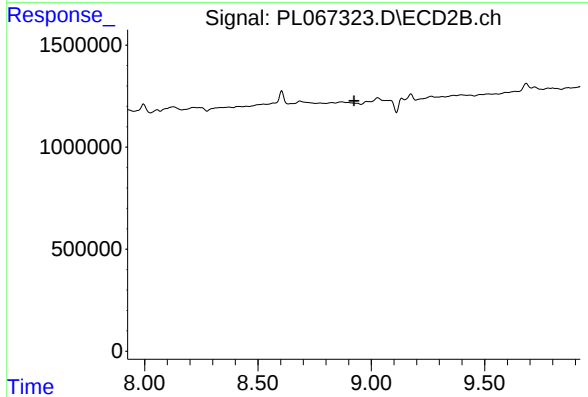


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.924 min
Response: 0
Conc: N.D.

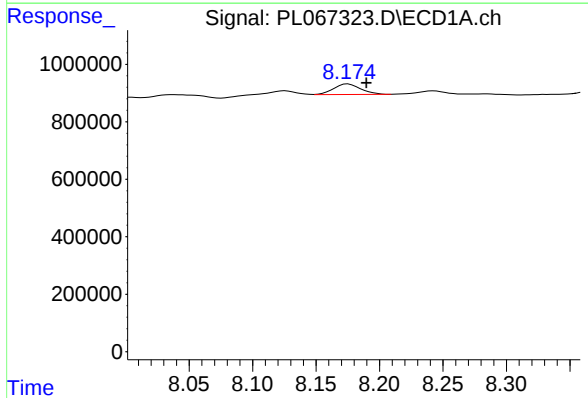


#15 Endosulfan II

R.T.: 8.175 min
Delta R.T.: -0.015 min
Response: 542378
Conc: 0.88 ng/ml

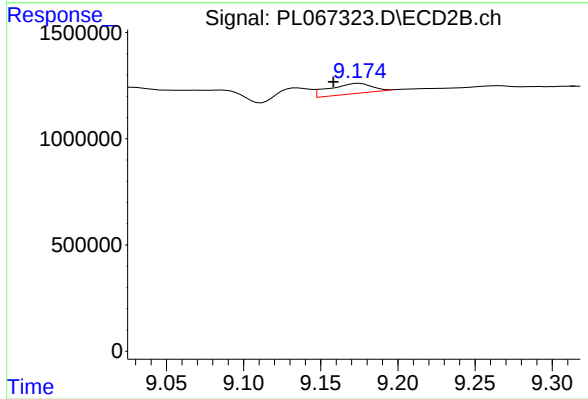

#15 Endosulfan II


R.T.: 9.175 min
Delta R.T.: 0.017 min
Response: 932884
Conc: 1.17 ng/ml

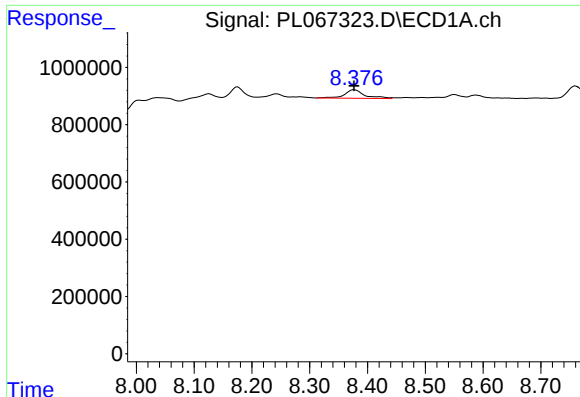

#18 Endrin aldehyde


R.T.: 8.377 min
Delta R.T.: 0.000 min
Response: 713918
Conc: 1.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

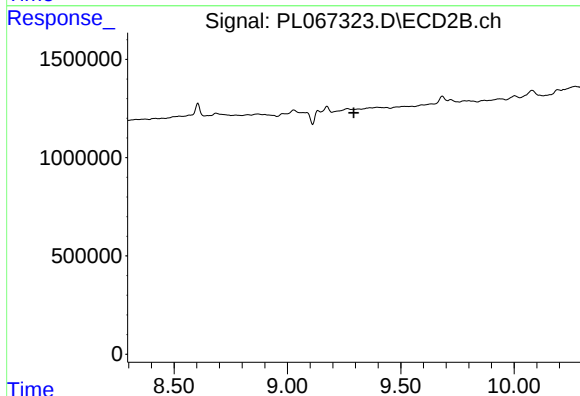


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 9.292 min
Response: 0
Conc: N.D.

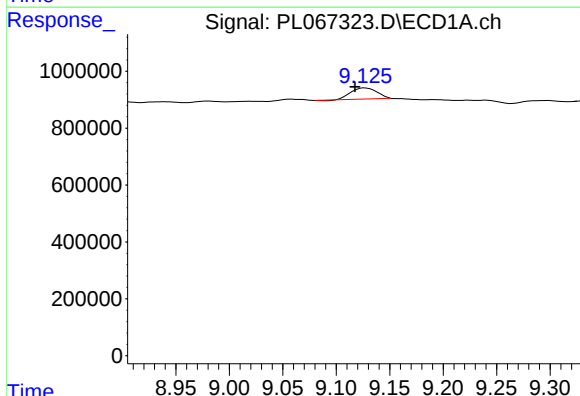


#21 Endrin ketone

R.T.: 9.127 min
Delta R.T.: 0.009 min
Response: 657407
Conc: 0.86 ng/ml

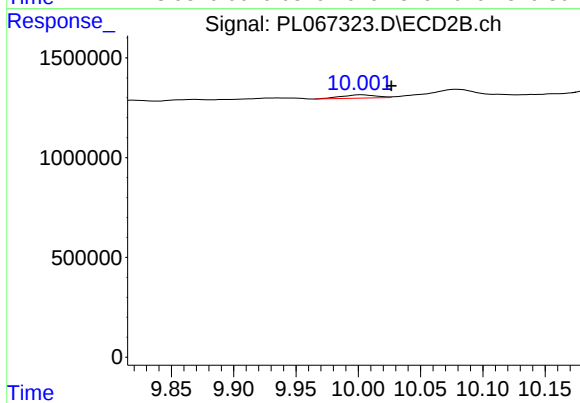

#21 Endrin ketone


R.T.: 10.003 min
Delta R.T.: -0.024 min
Response: 317445
Conc: 0.35 ng/ml

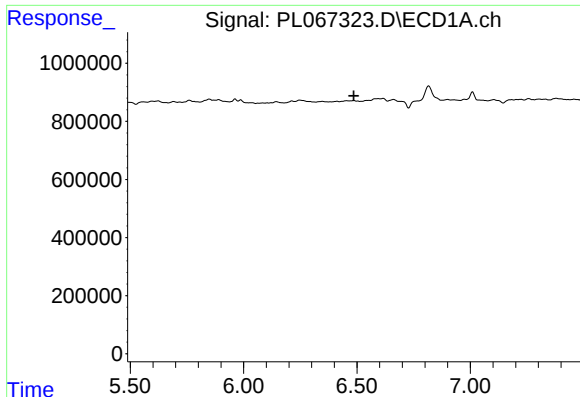

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 6.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

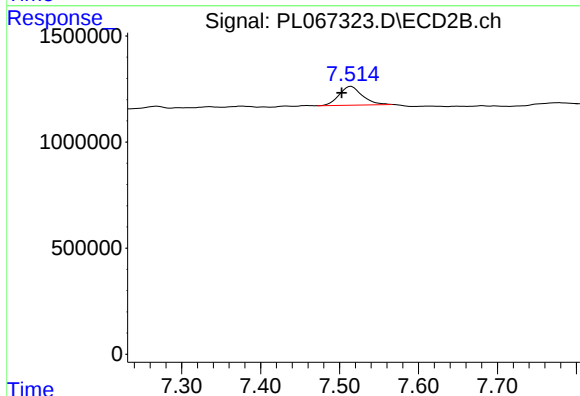


#24 Chlordane-2

R.T.: 7.515 min
Delta R.T.: 0.012 min
Response: 1818518
Conc: 49.90 ng/ml

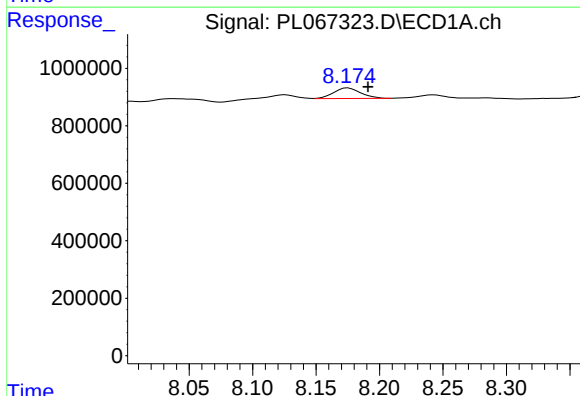


#27 Chlordane-5

R.T.: 8.175 min
Delta R.T.: -0.016 min
Response: 542378
Conc: 24.79 ng/ml

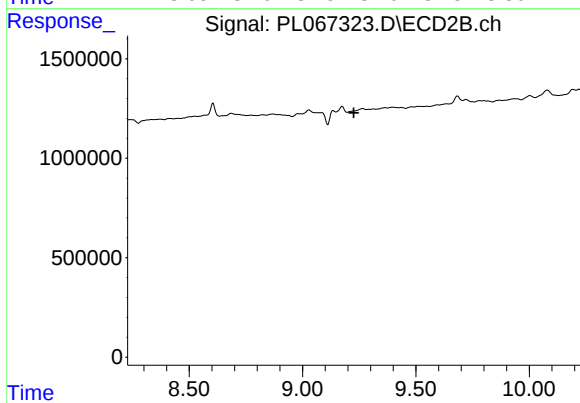

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

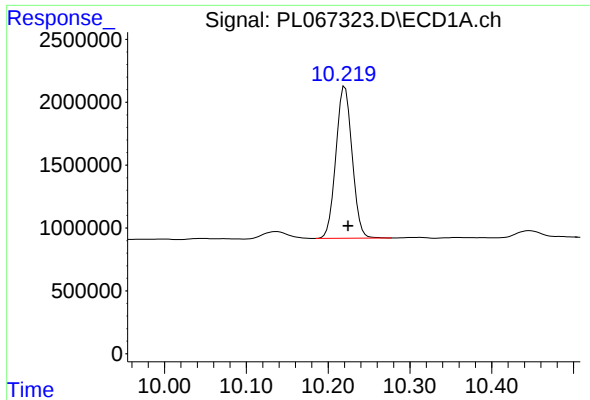

#28 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: -0.004 min
Response: 16612148
Conc: 23.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

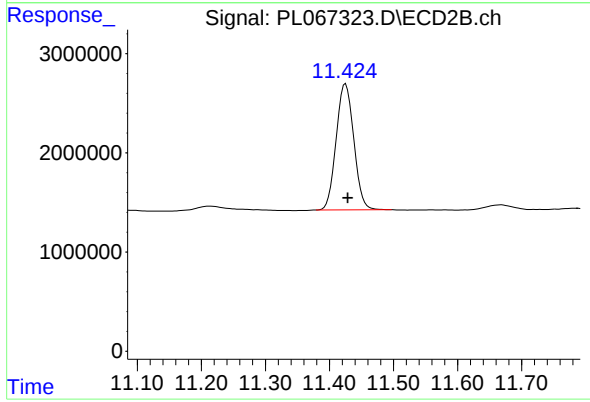

#28 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: -0.003 min
Response: 24305508
Conc: 24.40 ng/ml