

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
 Data File : PL067324.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2021 12:46
 Operator : AR\AJ
 Sample : M2625-19
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 08:54:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	5.528	11872977	20328851	21.596	21.564
28)	SA Decachlor...	10.221	11.426	15299475	22304186	21.589	22.392
Target Compounds							
2)	A alpha-BHC	5.165f	0.000	310672	0	0.422	N.D. #
5)	MB Aldrin	0.000	7.513	0	1763086	N.D.	1.629 #
14)	MA Endrin	7.894f	0.000	466004	0	0.711	N.D. #
15)	B Endosulfa...	8.175	9.175f	478968	572428	0.778	0.718
21)	B Endrin ke...	0.000	10.001f	0	264399	N.D.	0.292 #
22)	Mirex	9.292	0.000	199335	0	0.317	N.D. #
24)	Chlordane-2	0.000	7.513	0	1763086	N.D.	48.375 #
27)	Chlordane-5	8.175f	0.000	478968	0	21.892	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
Data File : PL067324.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2021 12:46
Operator : AR\AJ
Sample : M2625-19
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 08:54:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

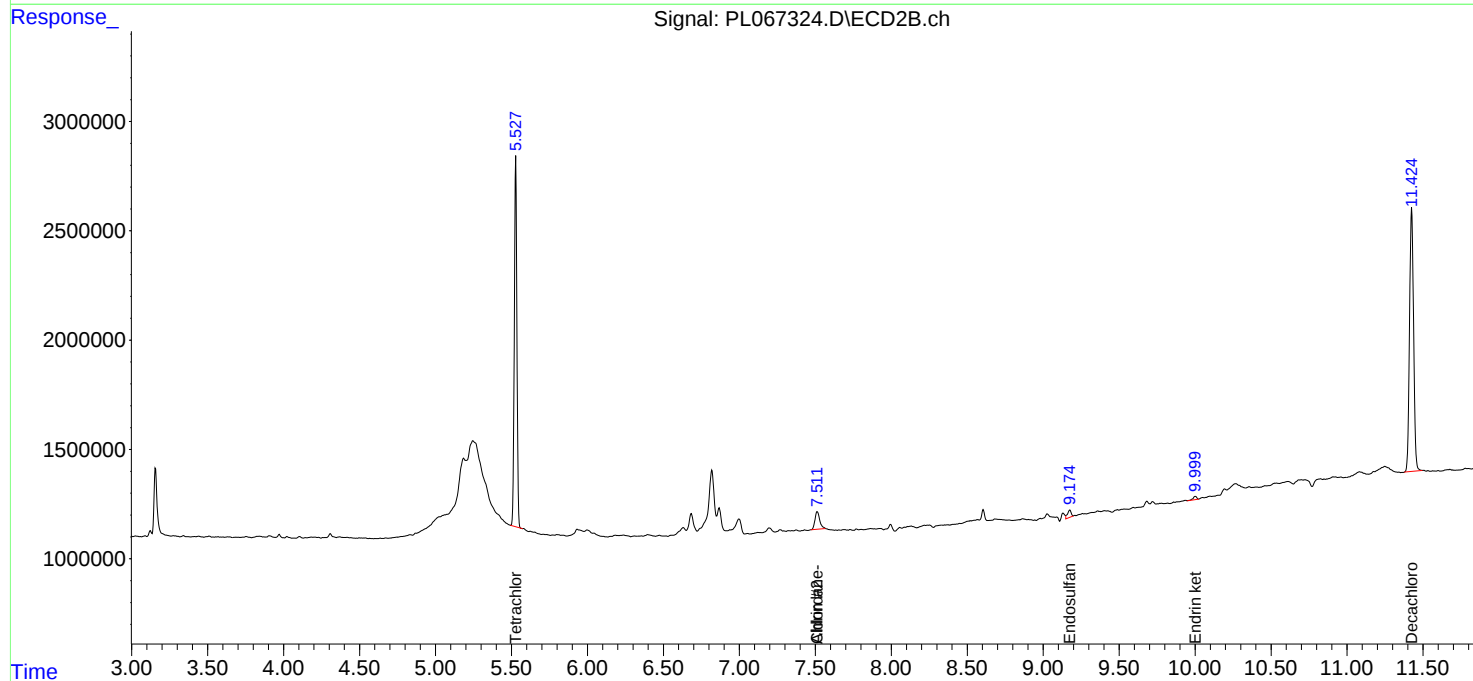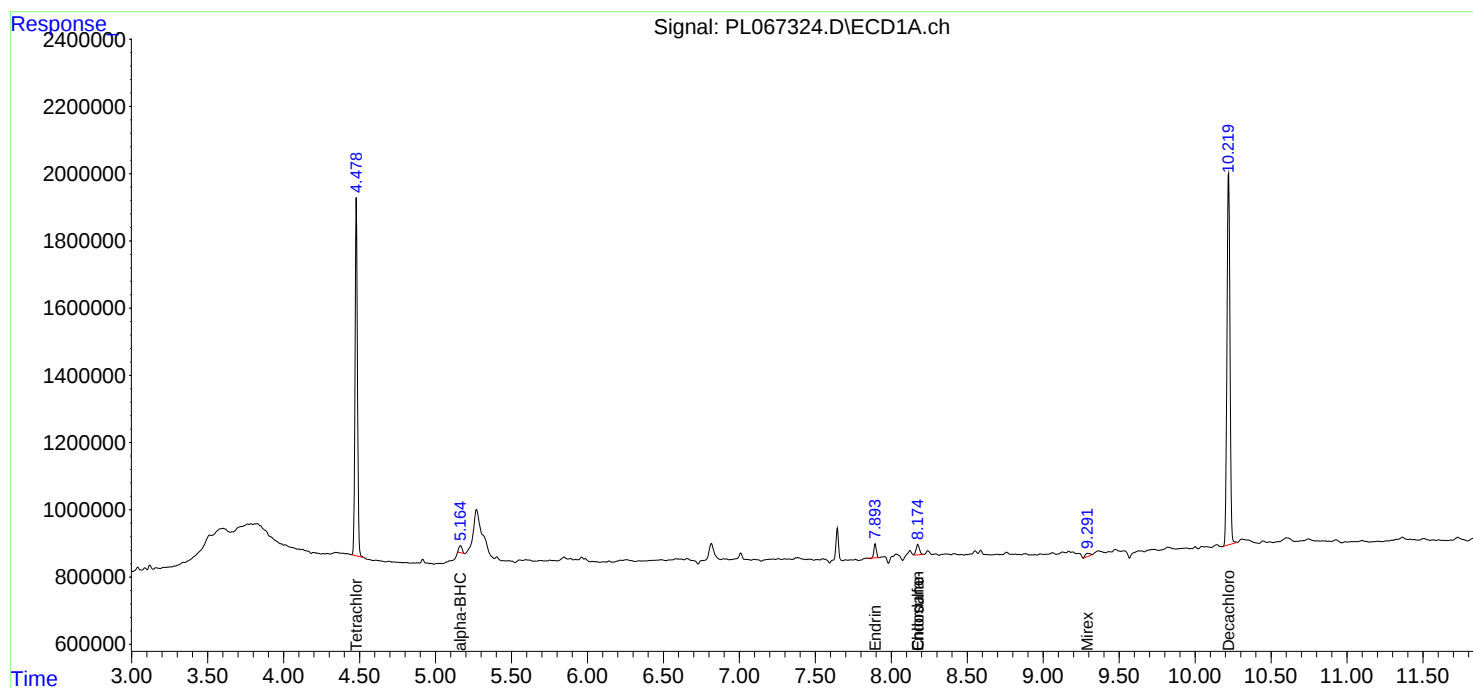


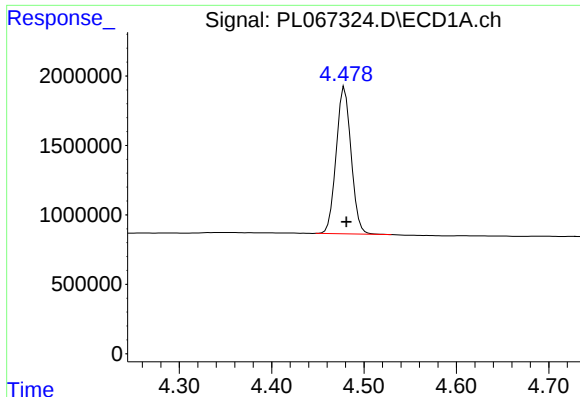

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: -0.002 min
Response: 11872977
Conc: 21.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

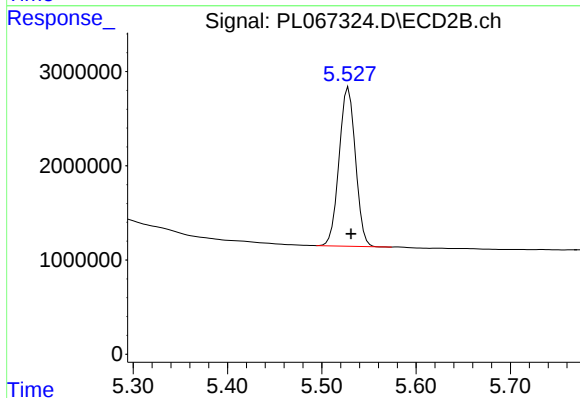


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 20328851
Conc: 21.56 ng/ml

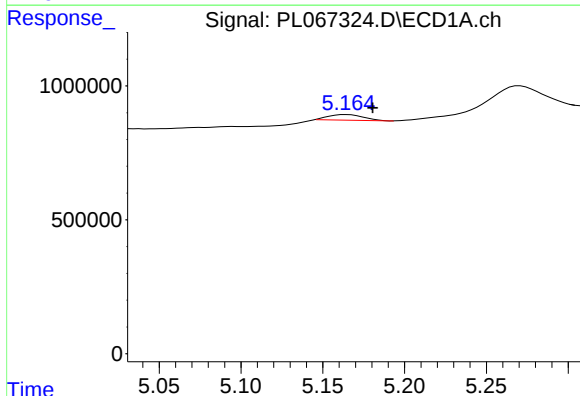


#2 alpha-BHC

R.T.: 5.165 min
Delta R.T.: -0.016 min
Response: 310672
Conc: 0.42 ng/ml

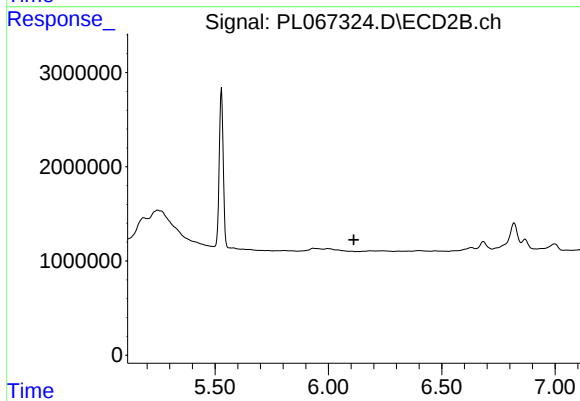

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

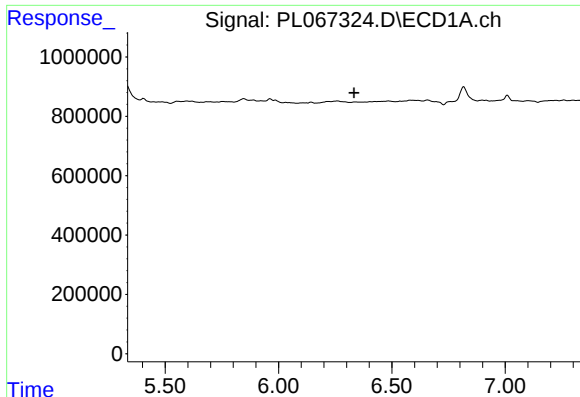

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 6.334 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

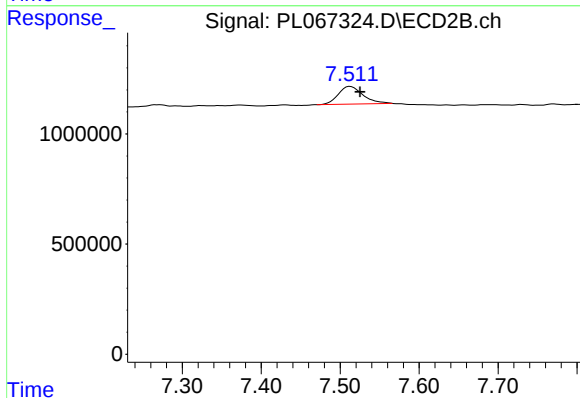


#5 Aldrin

R.T.: 7.513 min
Delta R.T.: -0.013 min
Response: 1763086
Conc: 1.63 ng/ml

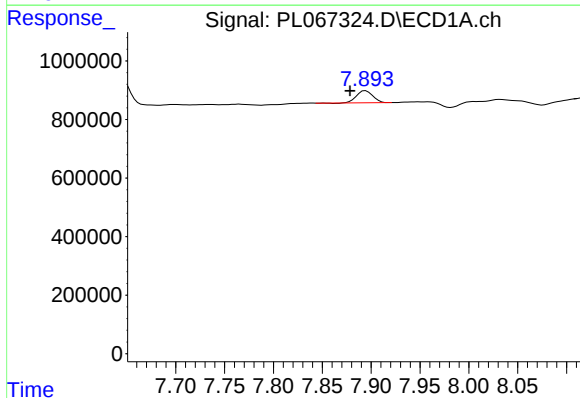


#14 Endrin

R.T.: 7.894 min
Delta R.T.: 0.016 min
Response: 466004
Conc: 0.71 ng/ml

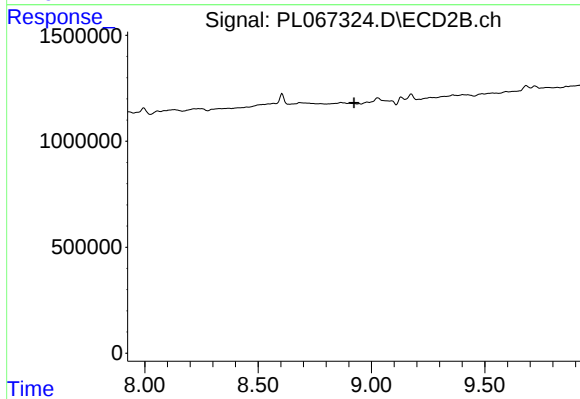

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.924 min
Response: 0
Conc: N.D.

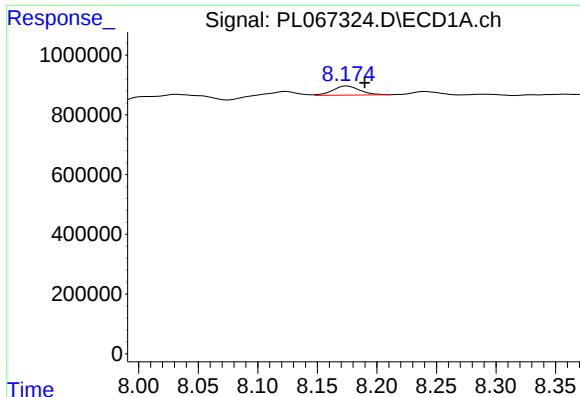

#15 Endosulfan II


R.T.: 8.175 min
Delta R.T.: -0.015 min
Response: 478968
Conc: 0.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

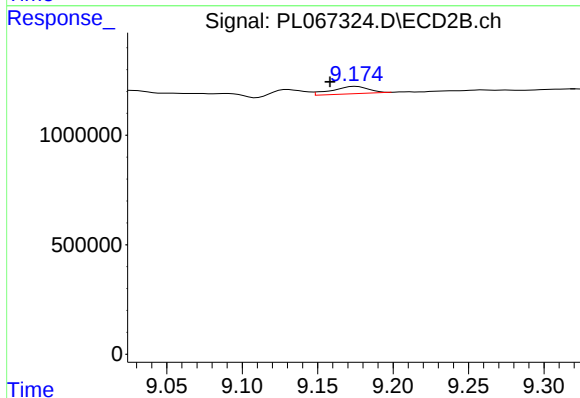


#15 Endosulfan II

R.T.: 9.175 min
Delta R.T.: 0.017 min
Response: 572428
Conc: 0.72 ng/ml

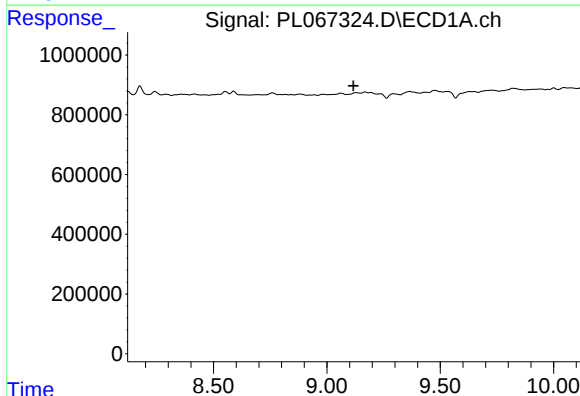


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.118 min
Response: 0
Conc: N.D.

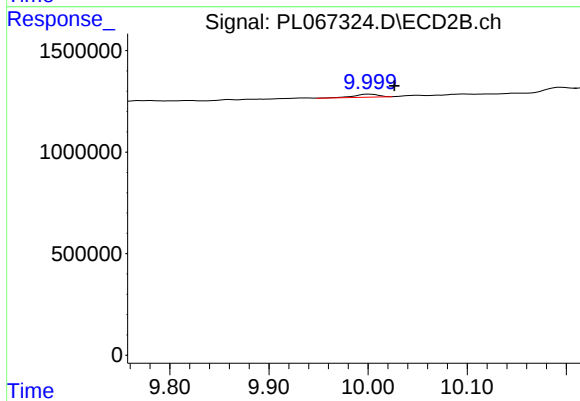

#21 Endrin ketone


R.T.: 10.001 min
Delta R.T.: -0.026 min
Response: 264399
Conc: 0.29 ng/ml

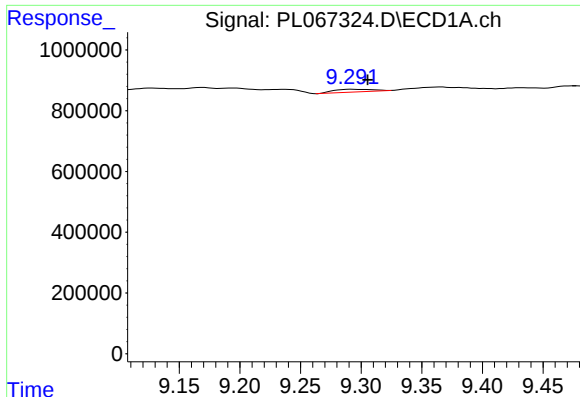

#22 Mirex


R.T.: 9.292 min
Delta R.T.: -0.013 min
Response: 199335
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

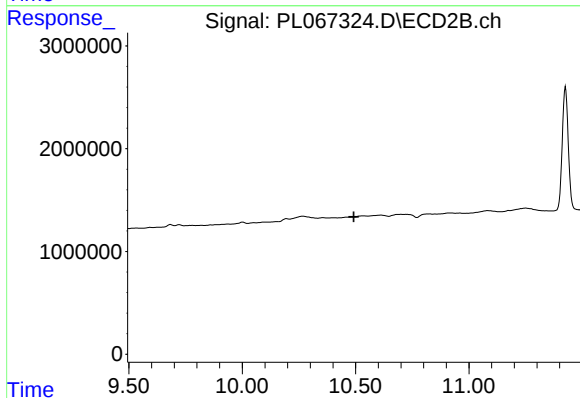


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 10.492 min
Response: 0
Conc: N.D.

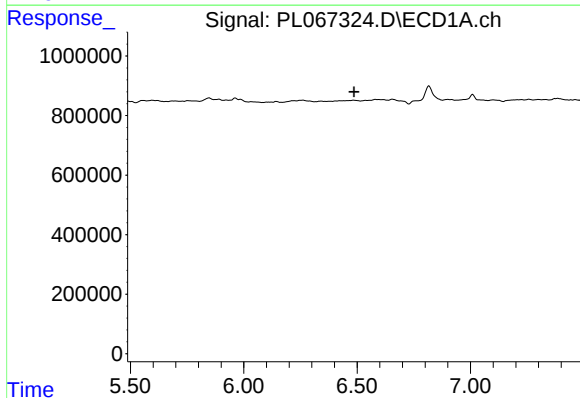


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 6.486 min
Response: 0
Conc: N.D.

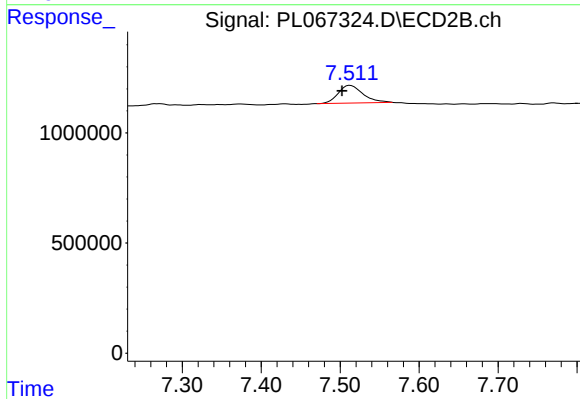

#24 Chlordane-2


R.T.: 7.513 min
Delta R.T.: 0.010 min
Response: 1763086
Conc: 48.38 ng/ml

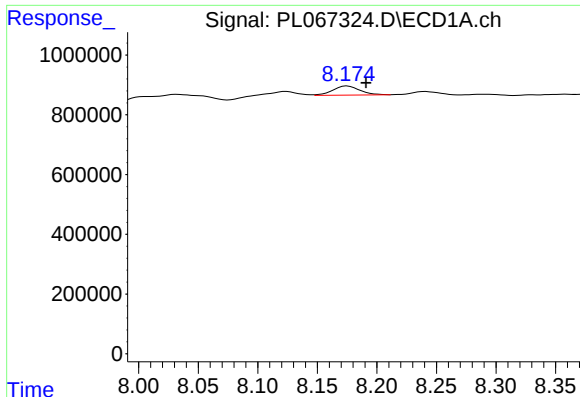

#27 Chlordane-5


R.T.: 8.175 min
Delta R.T.: -0.016 min
Response: 478968
Conc: 21.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

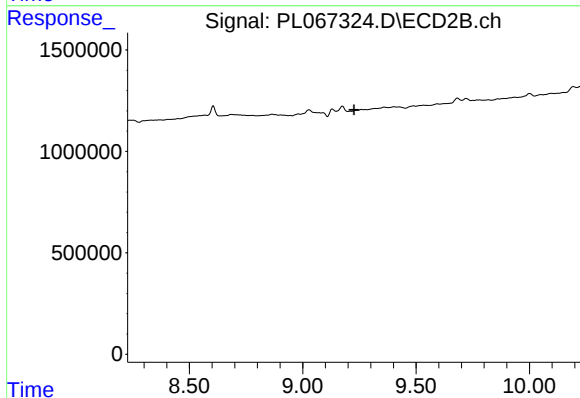


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

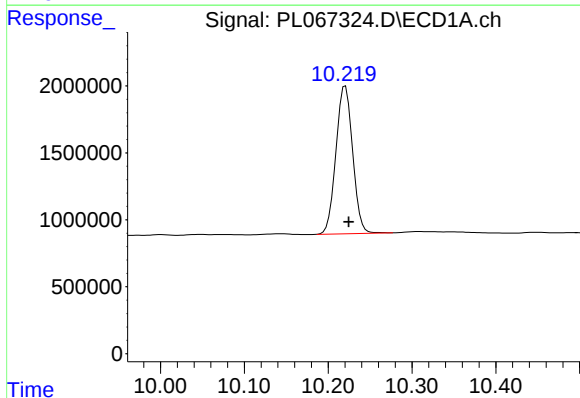

#28 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: -0.004 min
Response: 15299475
Conc: 21.59 ng/ml

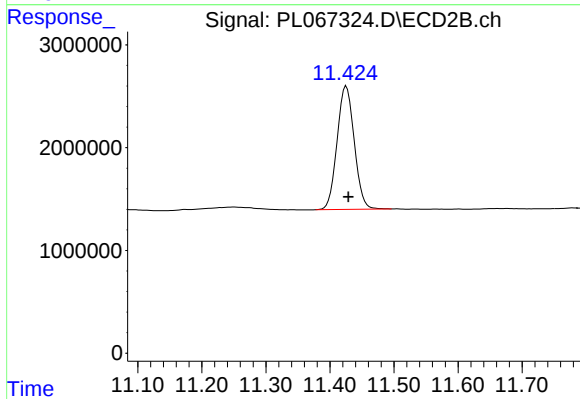

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.003 min
Response: 22304186
Conc: 22.39 ng/ml