

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
 Data File : PL067325.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2021 13:02
 Operator : AR\AJ
 Sample : M2625-20
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 08:54:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.528	11457736	19747918	20.840	20.948
28)	SA Decachlor...	10.221	11.427	14241622	20959358	20.096	21.042
Target Compounds							
2)	A alpha-BHC	5.167	0.000	296481	0	0.403	N.D. #
5)	MB Aldrin	0.000	7.514	0	1599339	N.D.	1.478 #
7)	B delta-BHC	0.000	6.999f	0	1168129	N.D.	0.994 #
14)	MA Endrin	7.894f	0.000	460210	0	0.702	N.D. #
15)	B Endosulfa...	8.177	9.176f	547318	439130	0.889	0.551 #
19)	B Endosulfa...	8.589f	0.000	850204	0	1.339	N.D. #
21)	B Endrin ke...	0.000	10.003f	0	954213	N.D.	1.053 #
24)	Chlordane-2	0.000	7.514	0	1599339	N.D.	43.882 #
27)	Chlordane-5	8.177	0.000	547318	0	25.016	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
Data File : PL067325.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2021 13:02
Operator : AR\AJ
Sample : M2625-20
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 08:54:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

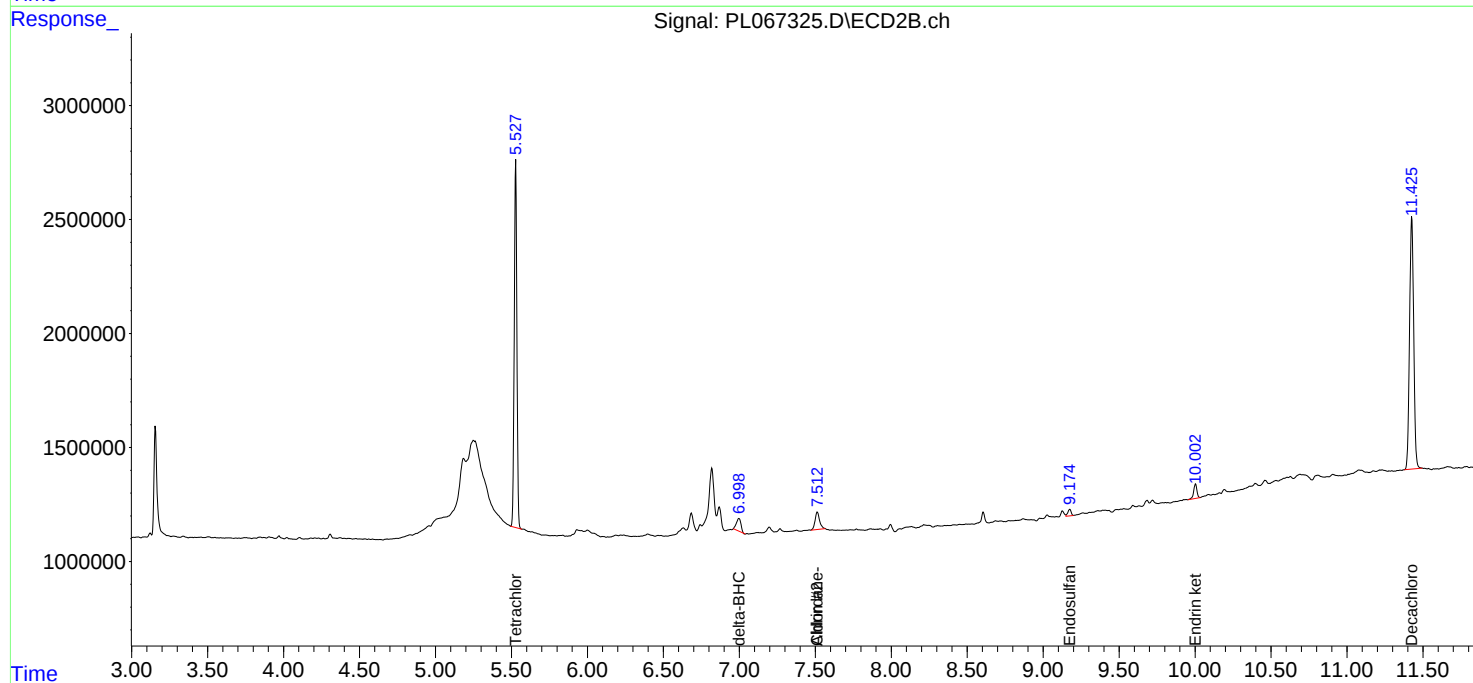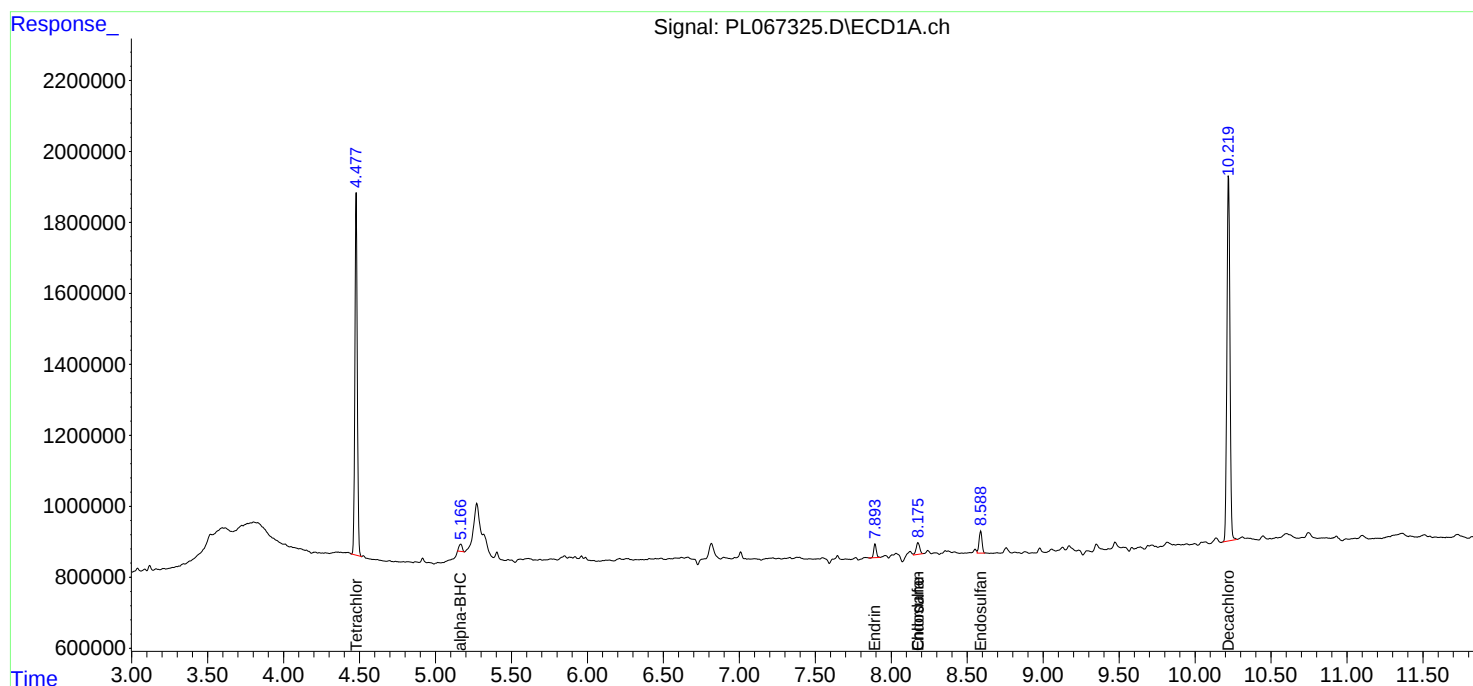


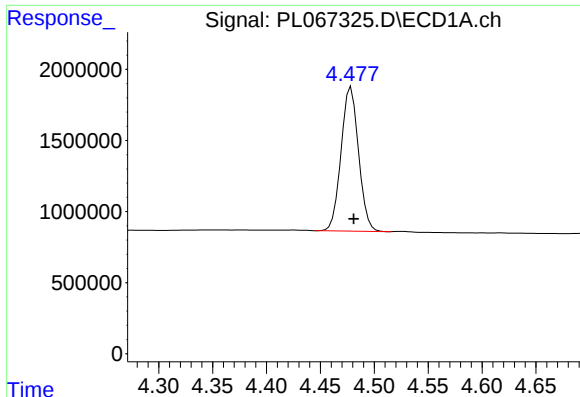

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 11457736
Conc: 20.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

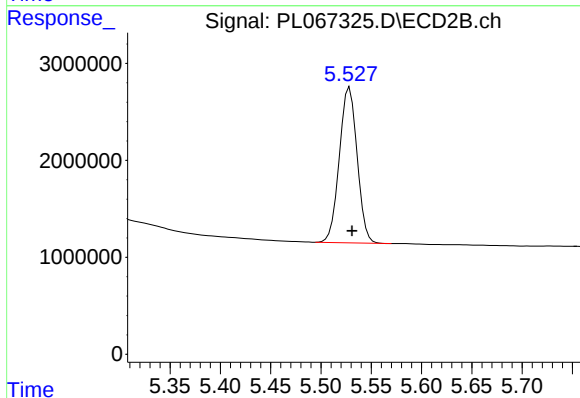


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 19747918
Conc: 20.95 ng/ml

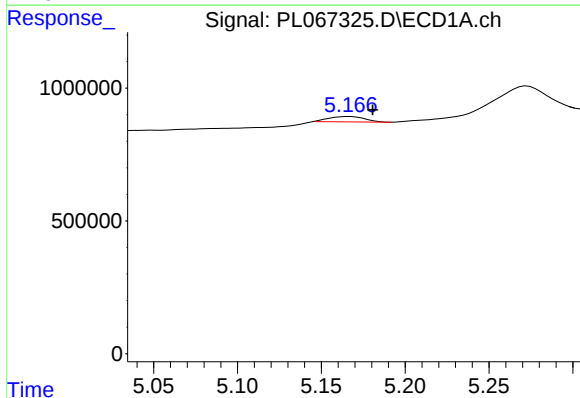


#2 alpha-BHC

R.T.: 5.167 min
Delta R.T.: -0.013 min
Response: 296481
Conc: 0.40 ng/ml

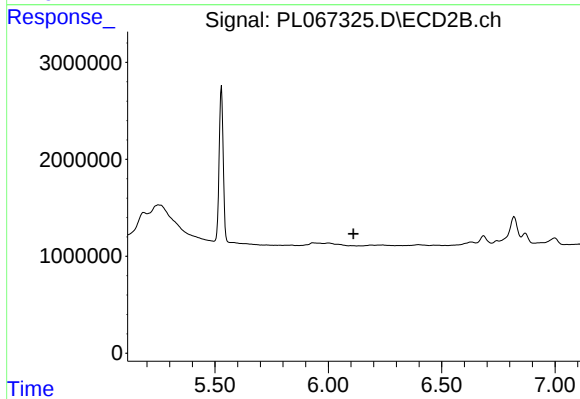

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

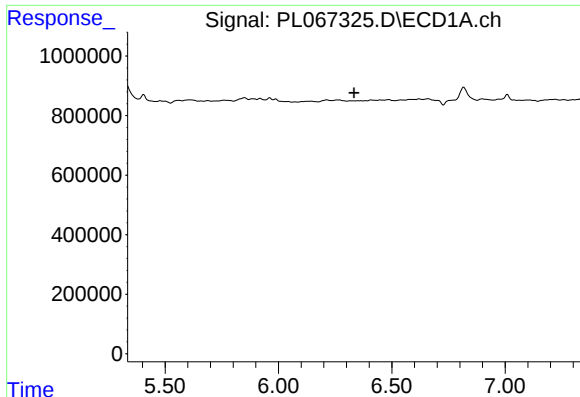

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 6.334 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

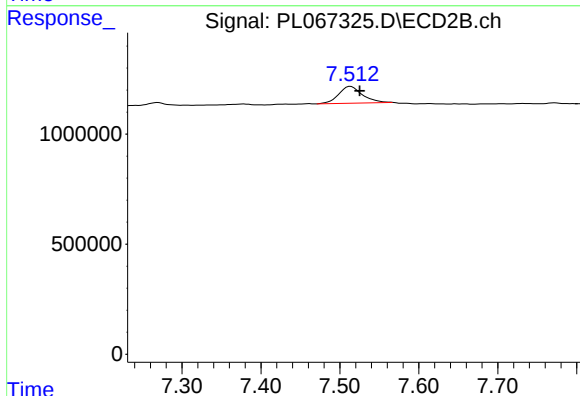


#5 Aldrin

R.T.: 7.514 min
Delta R.T.: -0.011 min
Response: 1599339
Conc: 1.48 ng/ml

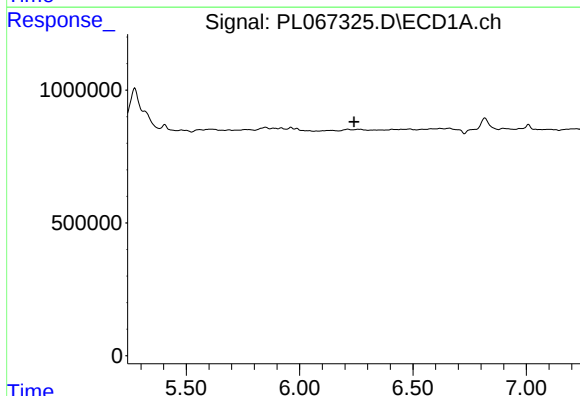


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.241 min
Response: 0
Conc: N.D.

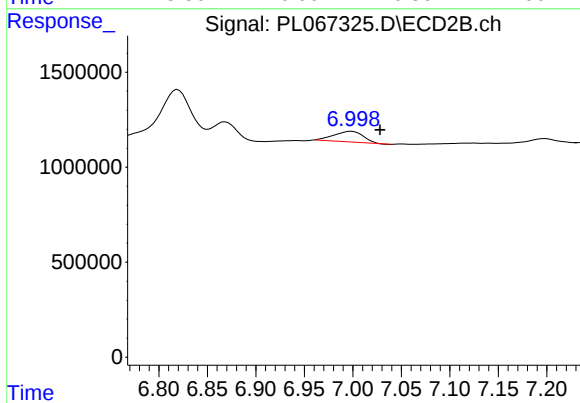

#7 delta-BHC


R.T.: 6.999 min
Delta R.T.: -0.029 min
Response: 1168129
Conc: 0.99 ng/ml

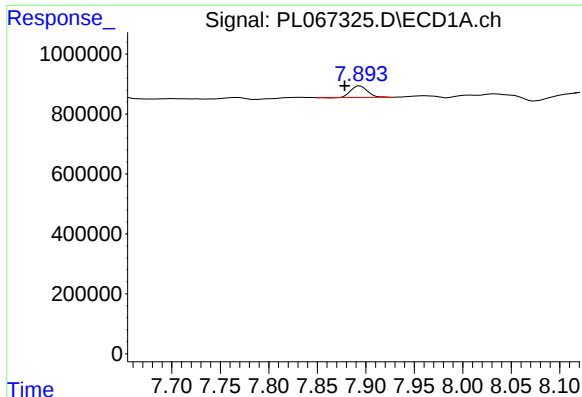

#14 Endrin


R.T.: 7.894 min
Delta R.T.: 0.016 min
Response: 460210
Conc: 0.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

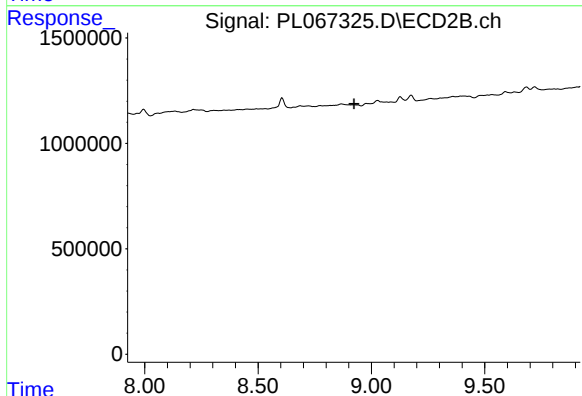


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.924 min
Response: 0
Conc: N.D.

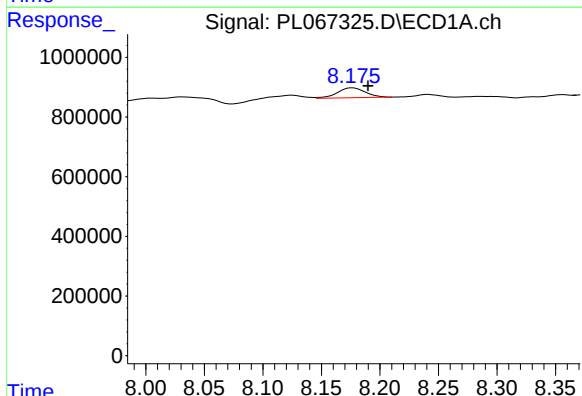


#15 Endosulfan II

R.T.: 8.177 min
Delta R.T.: -0.013 min
Response: 547318
Conc: 0.89 ng/ml

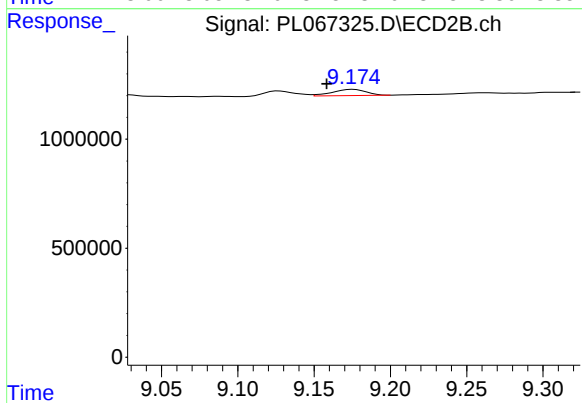

#15 Endosulfan II

R.T.: 9.176 min
Delta R.T.: 0.017 min
Response: 439130
Conc: 0.55 ng/ml

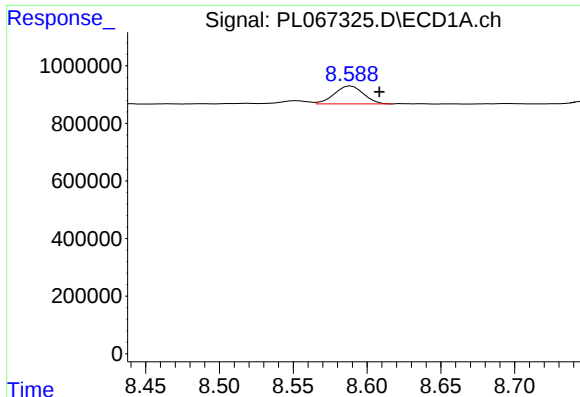

#19 Endosulfan Sulfate


R.T.: 8.589 min

Delta R.T.: -0.019 min

Response: 850204

Conc: 1.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

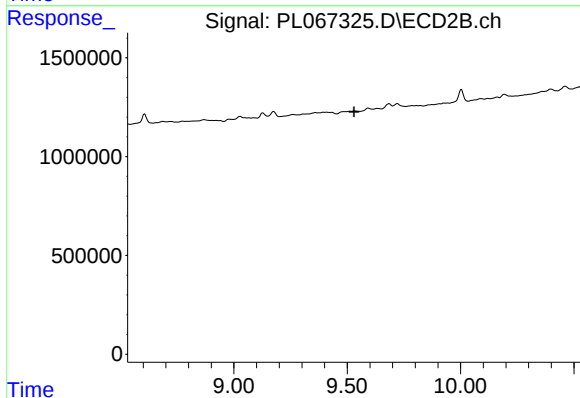


#19 Endosulfan Sulfate

R.T.: 0.000 min

Exp R.T. : 9.530 min

Response: 0

Conc: N.D.

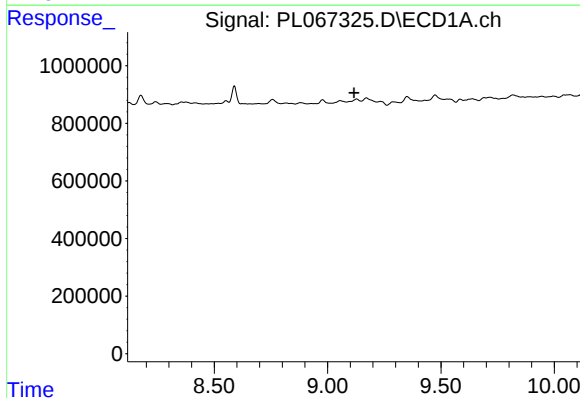


#21 Endrin ketone

R.T.: 0.000 min

Exp R.T. : 9.118 min

Response: 0

Conc: N.D.

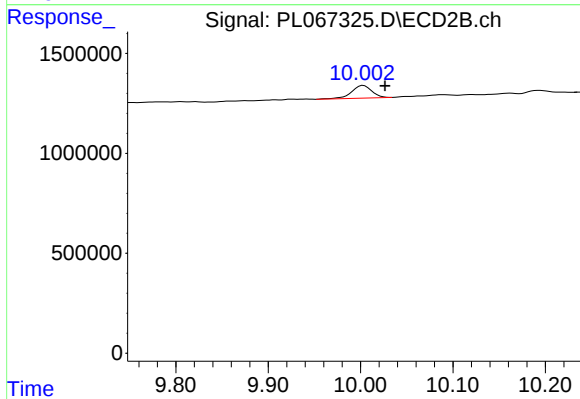


#21 Endrin ketone

R.T.: 10.003 min

Delta R.T.: -0.023 min

Response: 954213


Conc: 1.05 ng/ml

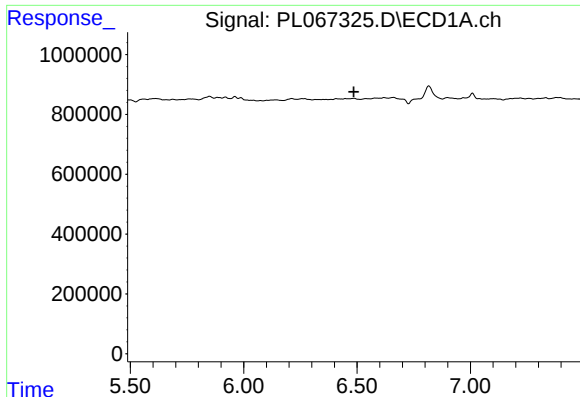

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 6.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

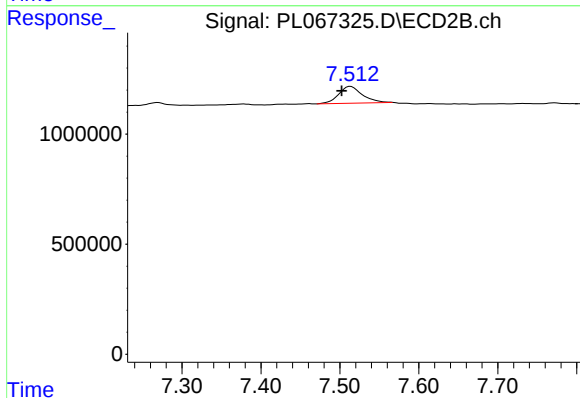


#24 Chlordane-2

R.T.: 7.514 min
Delta R.T.: 0.011 min
Response: 1599339
Conc: 43.88 ng/ml

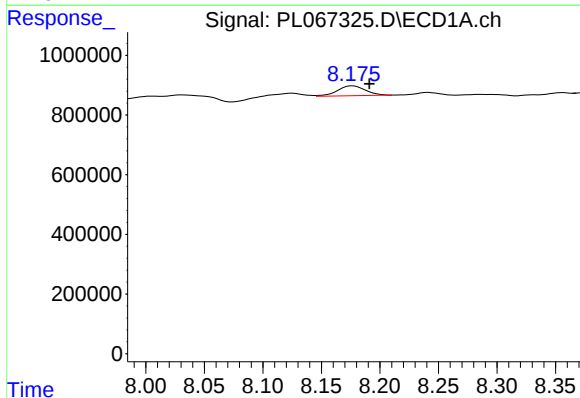


#27 Chlordane-5

R.T.: 8.177 min
Delta R.T.: -0.014 min
Response: 547318
Conc: 25.02 ng/ml

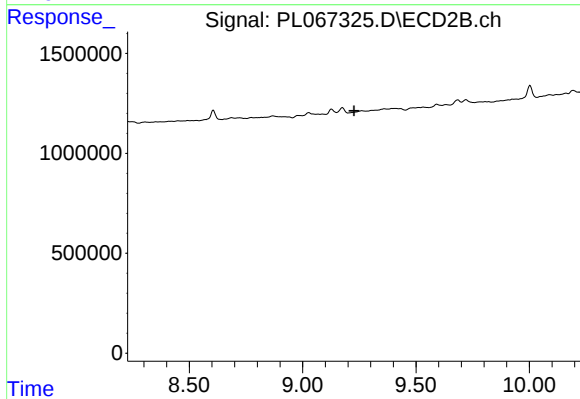

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

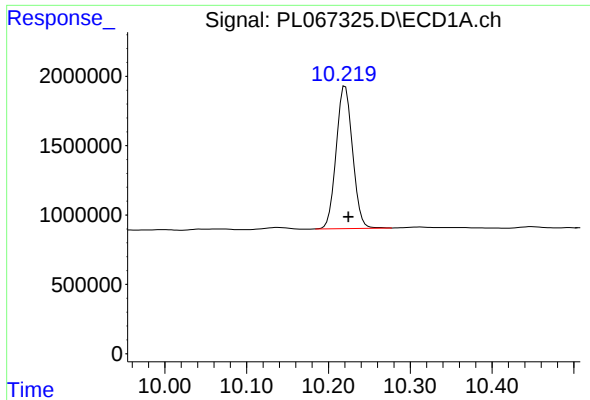

#28 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: -0.004 min
Response: 14241622
Conc: 20.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

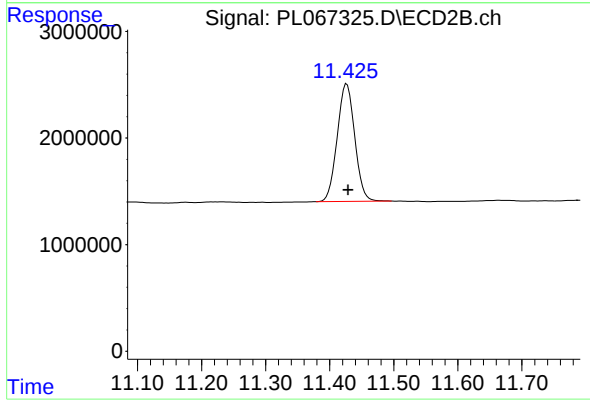

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.002 min
Response: 20959358
Conc: 21.04 ng/ml