

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
 Data File : PL067337.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2021 18:48
 Operator : AR\AJ
 Sample : M2625-23
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 08:57:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.482	5.524	12807003	21970056	23.295	23.305
28)	SA Decachlor...	10.224	11.426	16603029	24984706	23.428	25.084
Target Compounds							
4)	MA Heptachlor	0.000	7.165	0	591151	N.D.	0.530 #
6)	B beta-BHC	5.966f	6.751	777880	2988631	2.174	5.504 #
7)	B delta-BHC	0.000	7.003f	0	1989082	N.D.	1.692 #
15)	B Endosulfa...	0.000	9.174f	0	464762	N.D.	0.583 #
16)	A 4,4'-DDD	8.031f	0.000	208218	0	0.358	N.D. #
18)	B Endrin al...	8.381	0.000	291444	0	0.576	N.D. #
21)	B Endrin ke...	9.132	0.000	244298	0	0.321	N.D. #
23)	Chlordane-1	0.000	6.895f	0	279499	N.D.	9.898 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
Data File : PL067337.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2021 18:48
Operator : AR\AJ
Sample : M2625-23
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 08:57:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

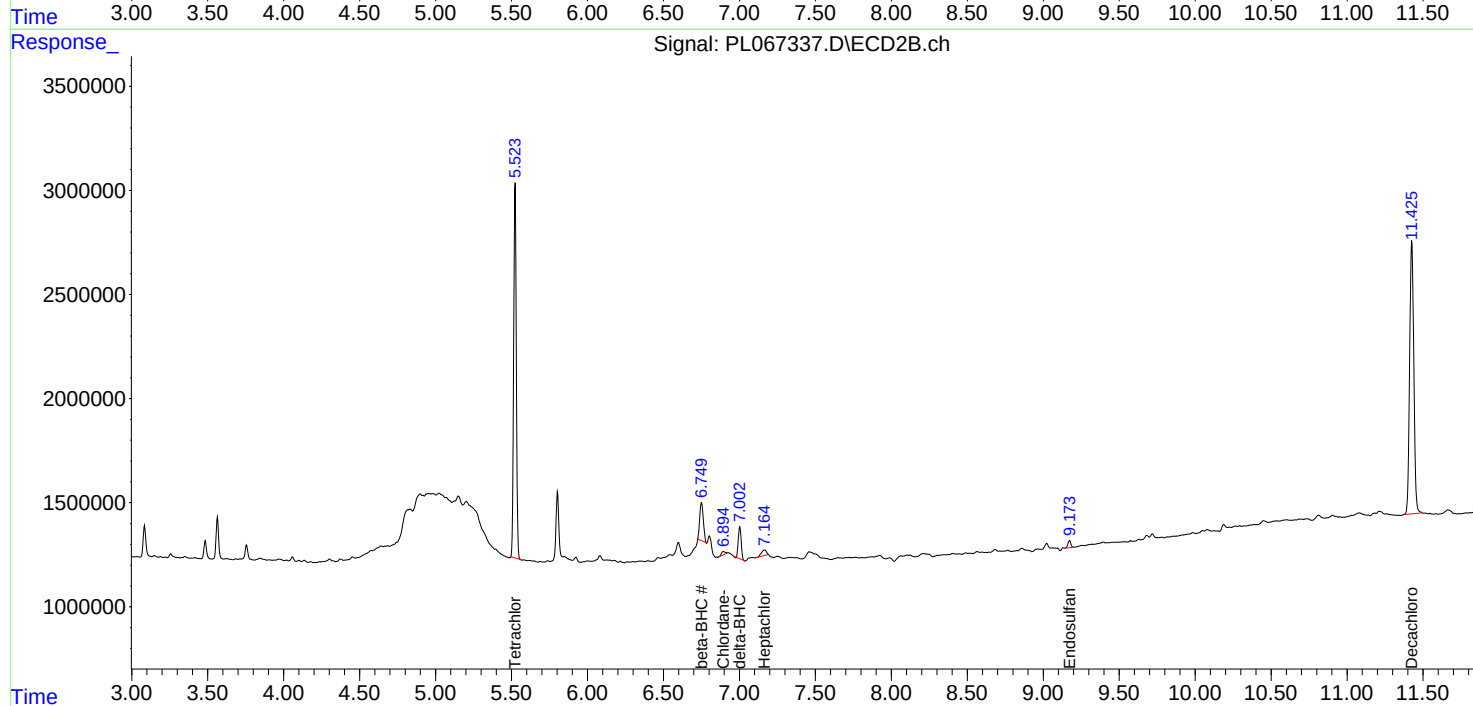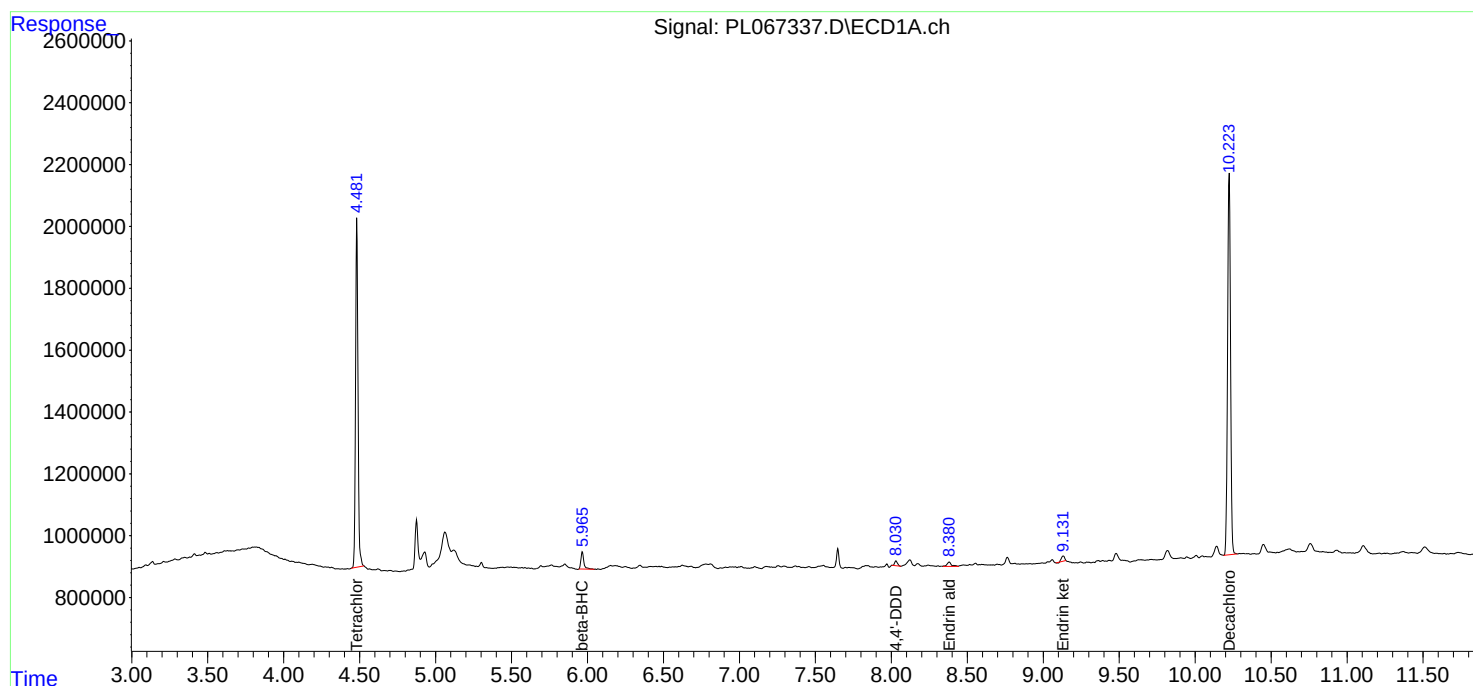


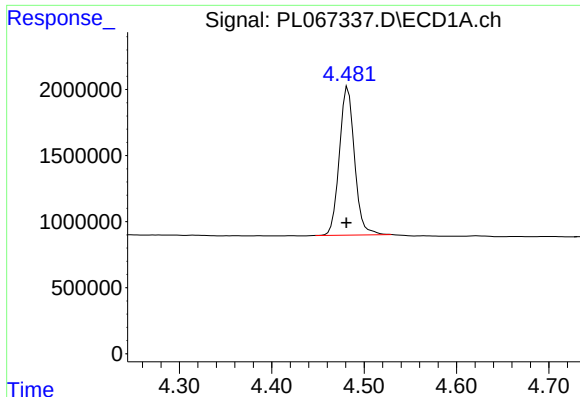

#1 Tetrachloro-m-xylene


R.T.: 4.482 min
Delta R.T.: 0.001 min
Response: 12807003
Conc: 23.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

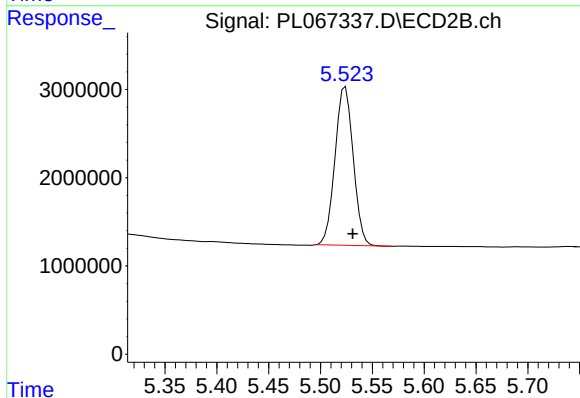


#1 Tetrachloro-m-xylene

R.T.: 5.524 min
Delta R.T.: -0.007 min
Response: 21970056
Conc: 23.30 ng/ml

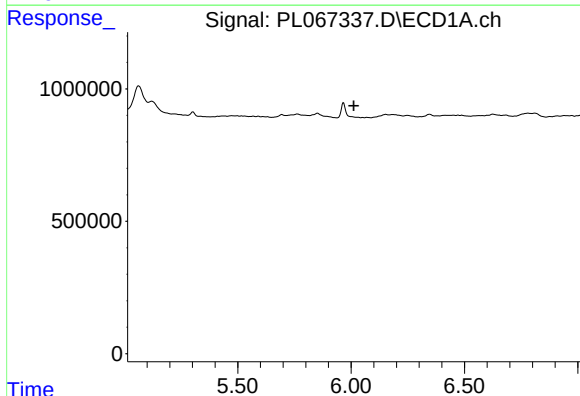


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 6.012 min
Response: 0
Conc: N.D.

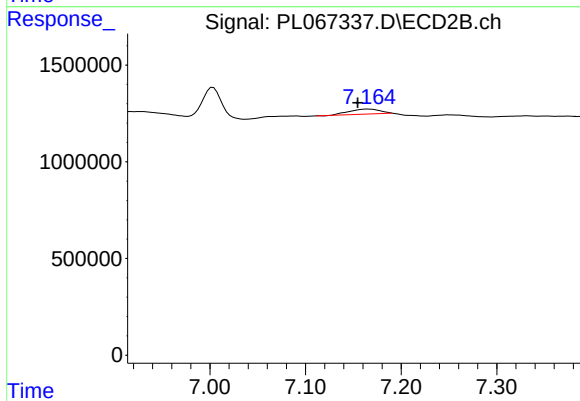

#4 Heptachlor


R.T.: 7.165 min
Delta R.T.: 0.011 min
Response: 591151
Conc: 0.53 ng/ml

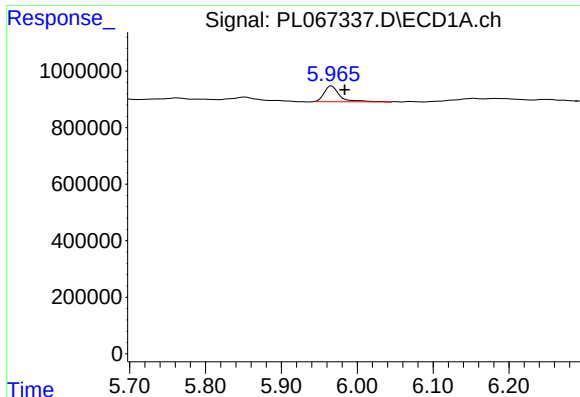

#6 beta-BHC


R.T.: 5.966 min
Delta R.T.: -0.017 min
Response: 777880
Conc: 2.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

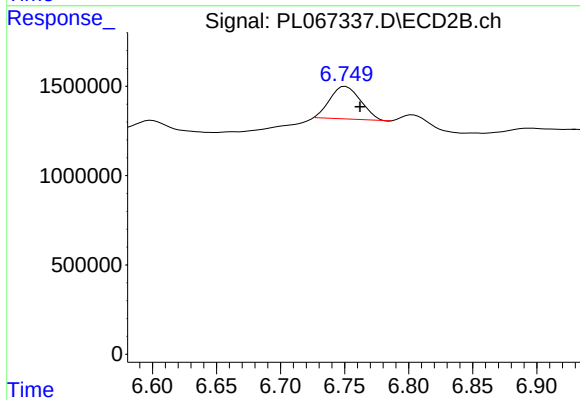


#6 beta-BHC

R.T.: 6.751 min
Delta R.T.: -0.011 min
Response: 2988631
Conc: 5.50 ng/ml

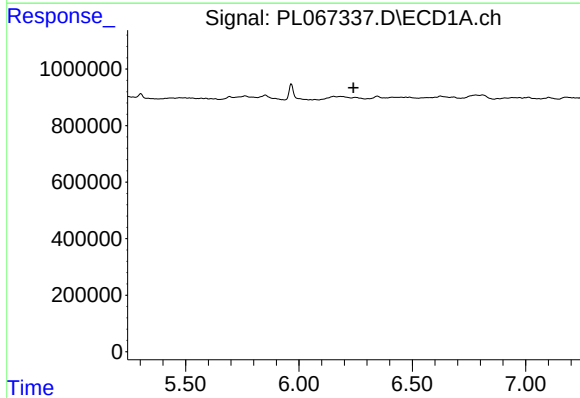


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

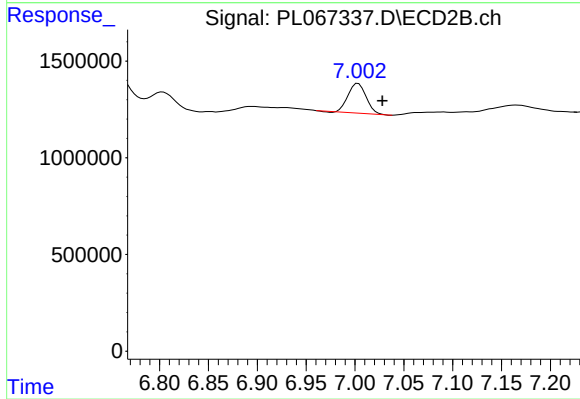

#7 delta-BHC


R.T.: 7.003 min
Delta R.T.: -0.025 min
Response: 1989082
Conc: 1.69 ng/ml

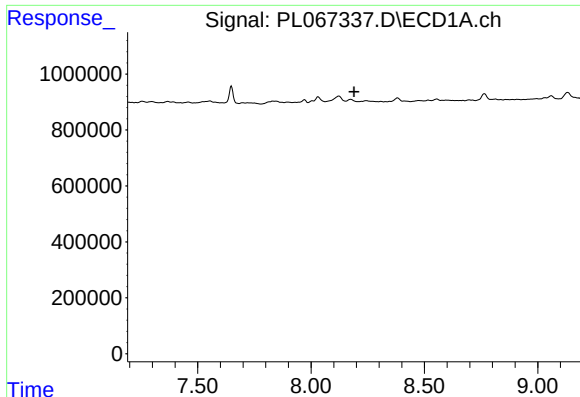

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

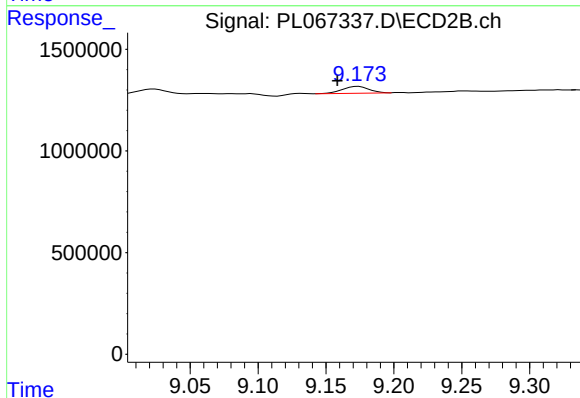


#15 Endosulfan II

R.T.: 9.174 min
Delta R.T.: 0.016 min
Response: 464762
Conc: 0.58 ng/ml

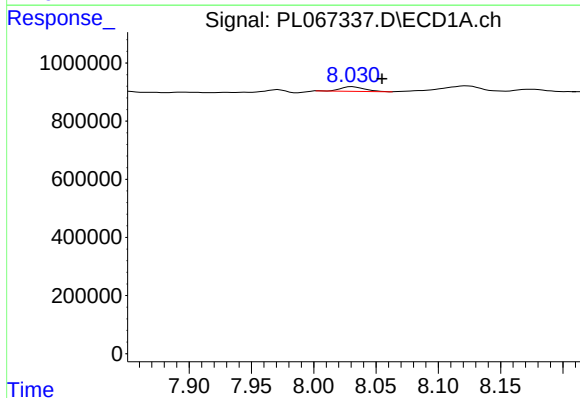


#16 4,4'-DDD

R.T.: 8.031 min
Delta R.T.: -0.024 min
Response: 208218
Conc: 0.36 ng/ml

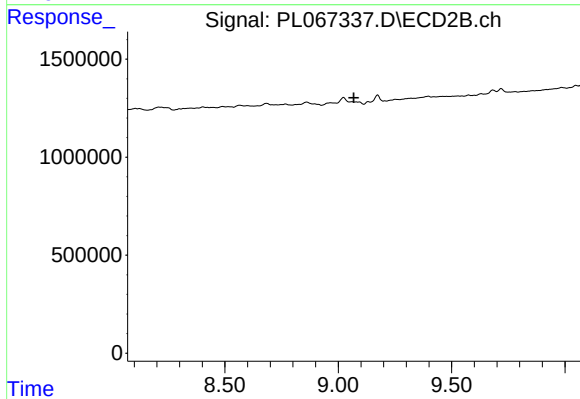

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 9.069 min
Response: 0
Conc: N.D.

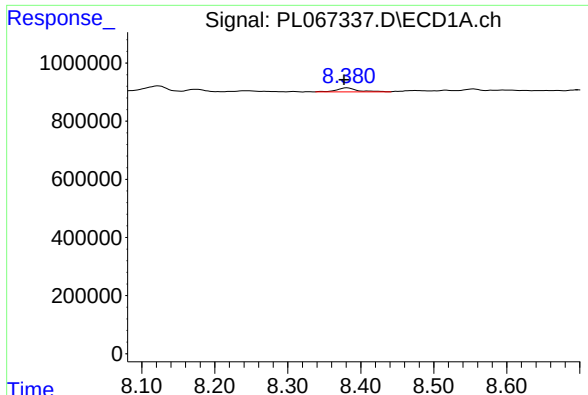

#18 Endrin aldehyde


R.T.: 8.381 min
Delta R.T.: 0.004 min
Response: 291444
Conc: 0.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

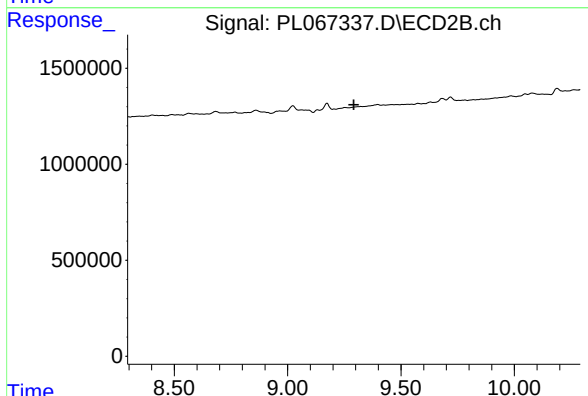


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 9.292 min
Response: 0
Conc: N.D.

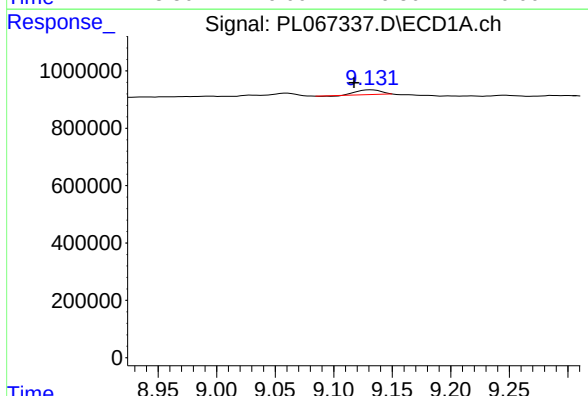


#21 Endrin ketone

R.T.: 9.132 min
Delta R.T.: 0.015 min
Response: 244298
Conc: 0.32 ng/ml

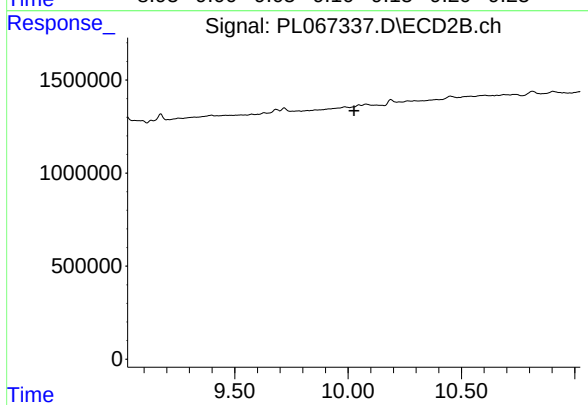

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 10.027 min
Response: 0
Conc: N.D.

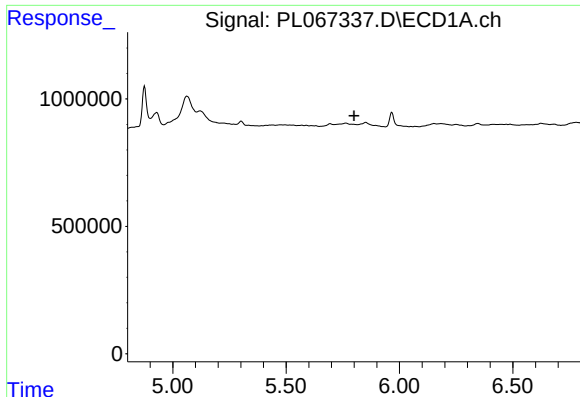

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.800 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

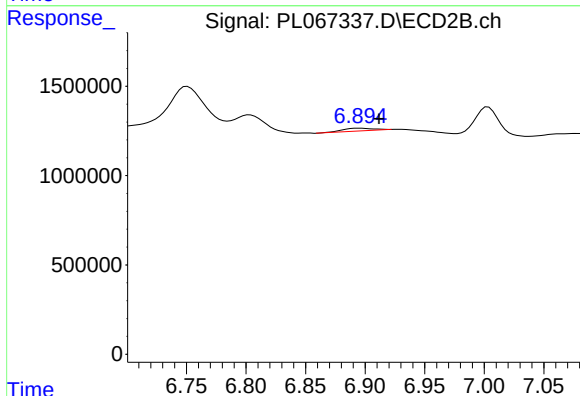


#23 Chlordane-1

R.T.: 6.895 min
Delta R.T.: -0.016 min
Response: 279499
Conc: 9.90 ng/ml

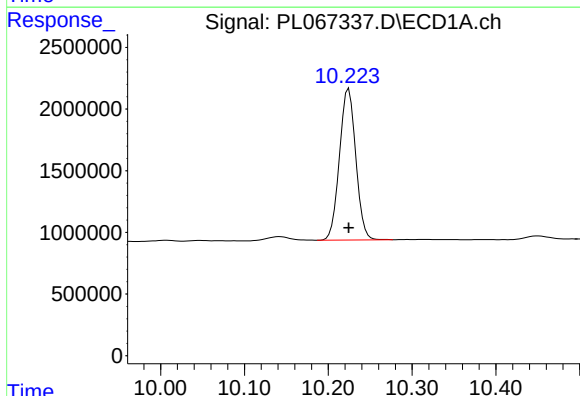

#28 Decachlorobiphenyl

R.T.: 10.224 min
Delta R.T.: 0.000 min
Response: 16603029
Conc: 23.43 ng/ml

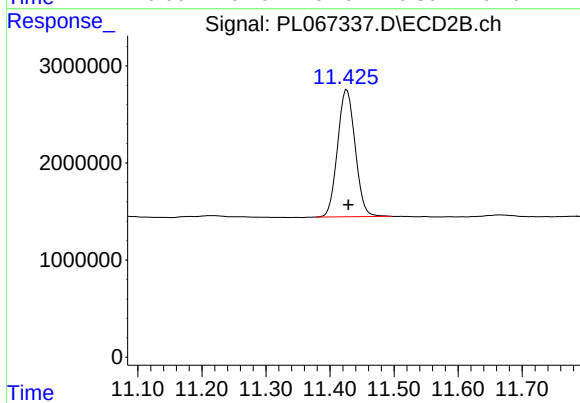

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.002 min
Response: 24984706
Conc: 25.08 ng/ml