

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
 Data File : PL067342.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2021 20:11
 Operator : AR\AJ
 Sample : M2625-28
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 08:58:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	5.528	12466817	20755258	22.676	22.016
28)	SA Decachlor...	10.222	11.425	14871821	22570890	20.985	22.660
Target Compounds							
2)	A alpha-BHC	5.170	0.000	325011	0	0.442	N.D. #
7)	B delta-BHC	0.000	7.005f	0	2420044	N.D.	2.059 #
8)	B Heptachlo...	0.000	7.962f	0	2917304	N.D.	2.912 #
15)	B Endosulfa...	0.000	9.178f	0	642868	N.D.	0.806 #
24)	Chlordane-2	6.470f	0.000	409274	0	15.284	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
Data File : PL067342.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2021 20:11
Operator : AR\AJ
Sample : M2625-28
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 08:58:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

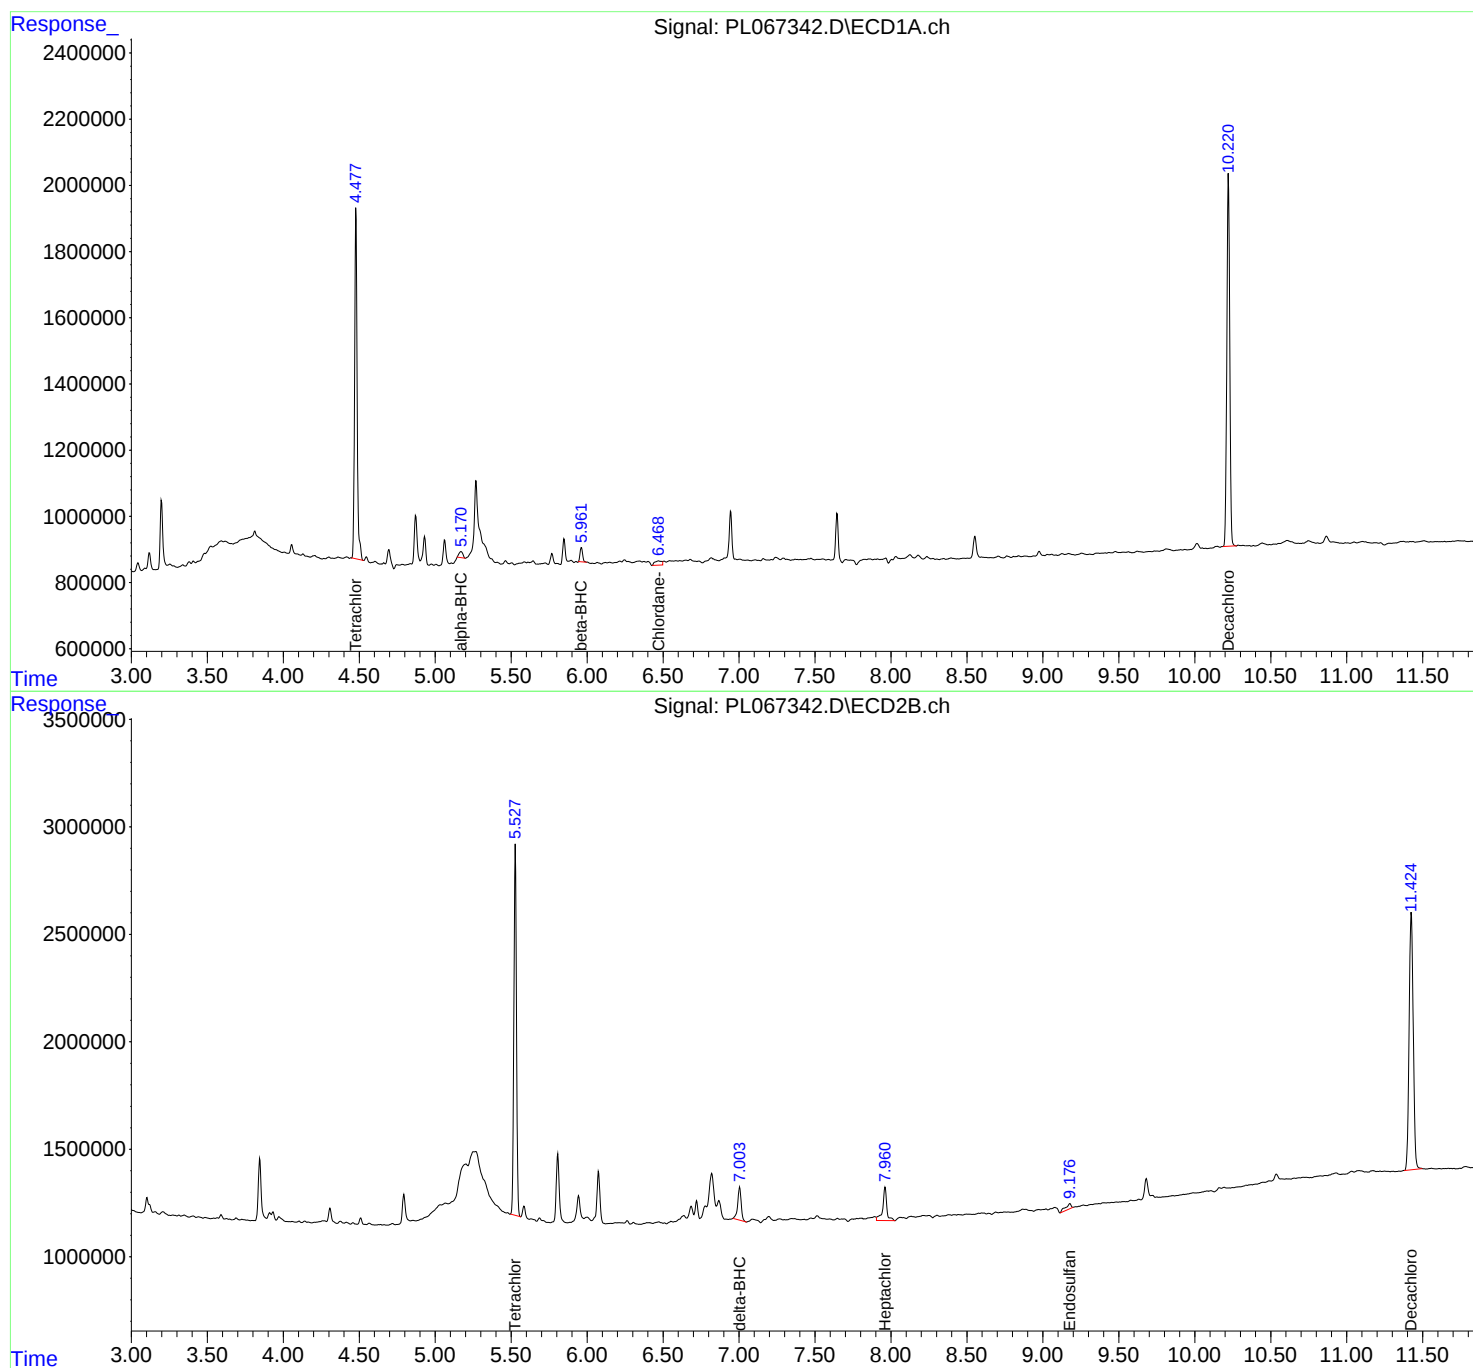


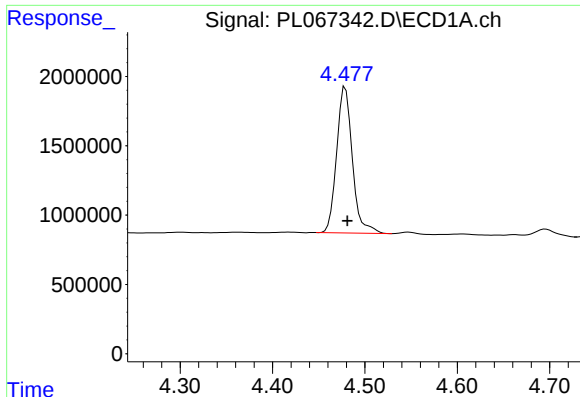

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: -0.002 min
Response: 12466817
Conc: 22.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

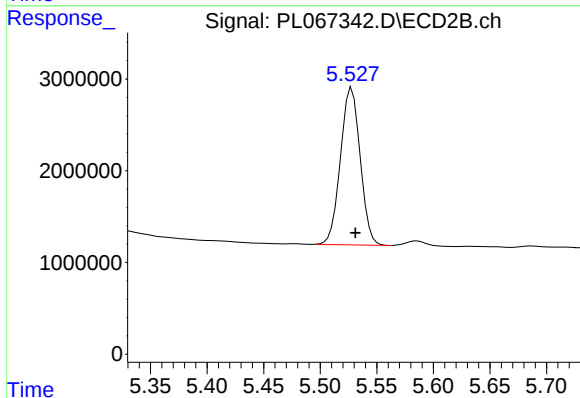


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 20755258
Conc: 22.02 ng/ml

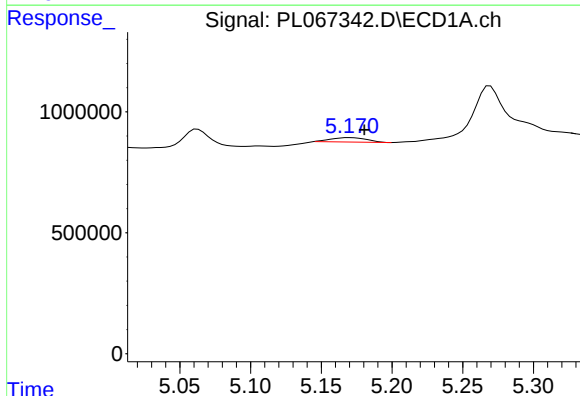


#2 alpha-BHC

R.T.: 5.170 min
Delta R.T.: -0.010 min
Response: 325011
Conc: 0.44 ng/ml

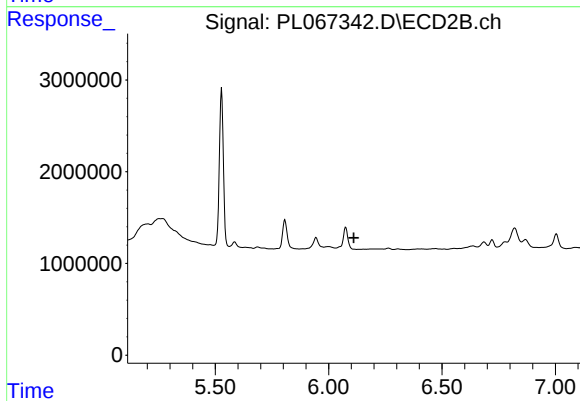

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 6.112 min
Response: 0
Conc: N.D.

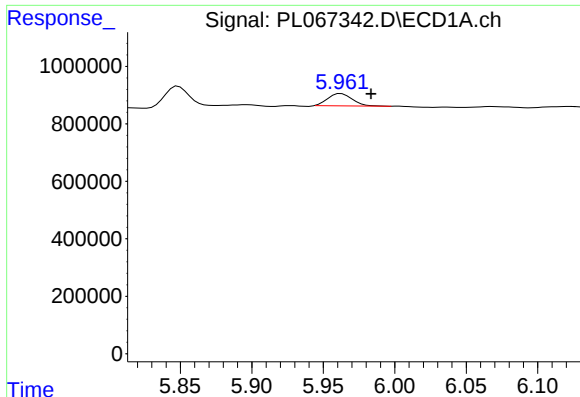

#6 beta-BHC


R.T.: 5.963 min
Delta R.T.: -0.021 min
Response: 507678
Conc: 1.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

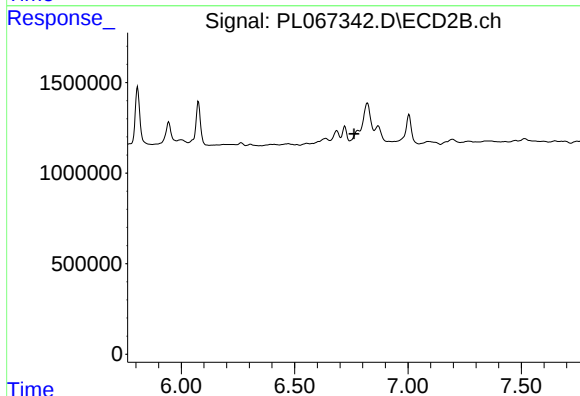


#6 beta-BHC

R.T.: 6.779 min
Delta R.T.: 0.017 min
Response: -940036
Conc: N.D.

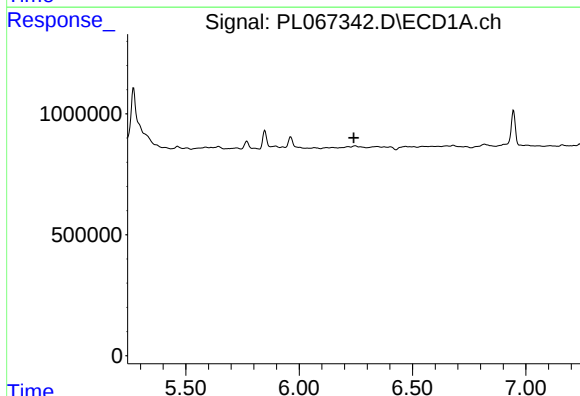


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

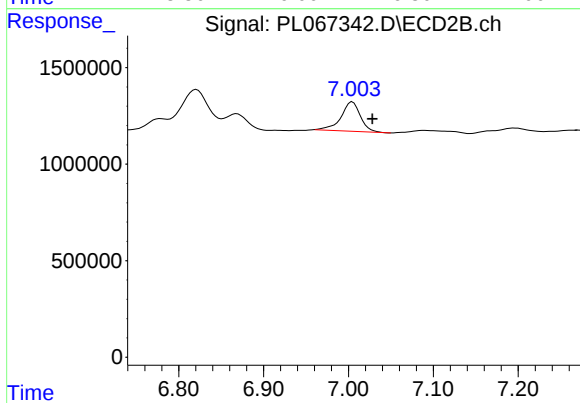

#7 delta-BHC


R.T.: 7.005 min
Delta R.T.: -0.023 min
Response: 2420044
Conc: 2.06 ng/ml

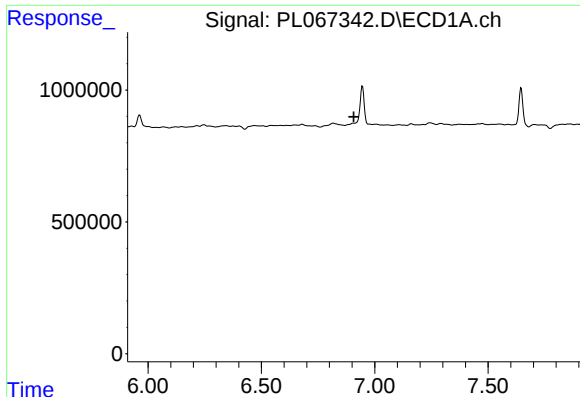

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 6.907 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

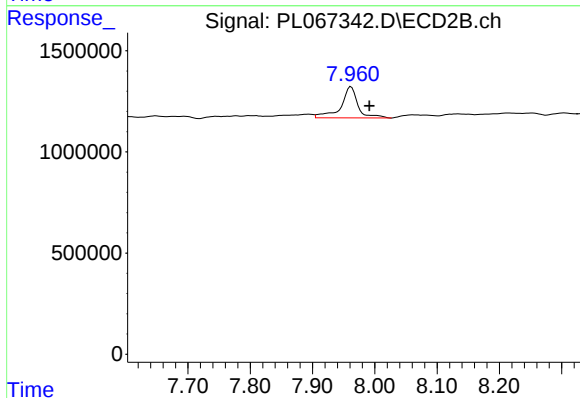


#8 Heptachlor epoxide

R.T.: 7.962 min
Delta R.T.: -0.029 min
Response: 2917304
Conc: 2.91 ng/ml

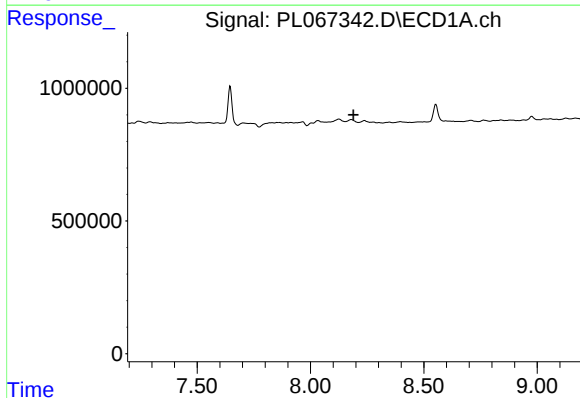


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.190 min
Response: 0
Conc: N.D.

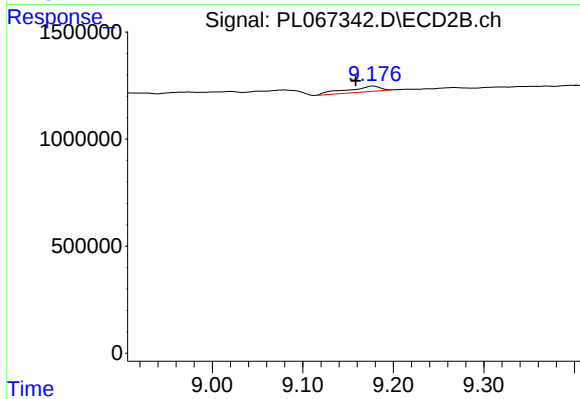

#15 Endosulfan II


R.T.: 9.178 min
Delta R.T.: 0.020 min
Response: 642868
Conc: 0.81 ng/ml

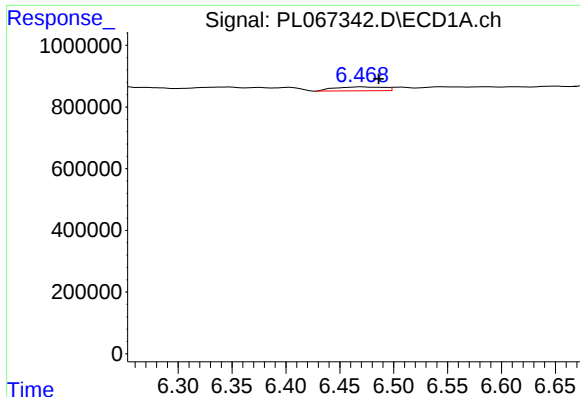

#24 Chlordane-2


R.T.: 6.470 min
Delta R.T.: -0.016 min
Response: 409274
Conc: 15.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

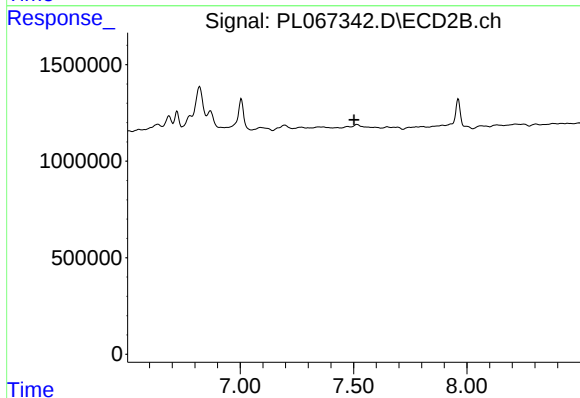


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

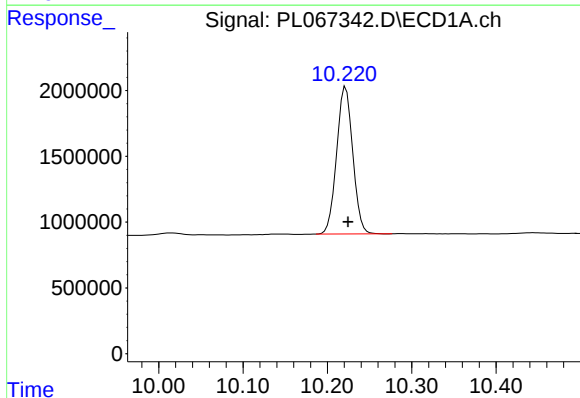

#28 Decachlorobiphenyl

R.T.: 10.222 min
Delta R.T.: -0.003 min
Response: 14871821
Conc: 20.99 ng/ml

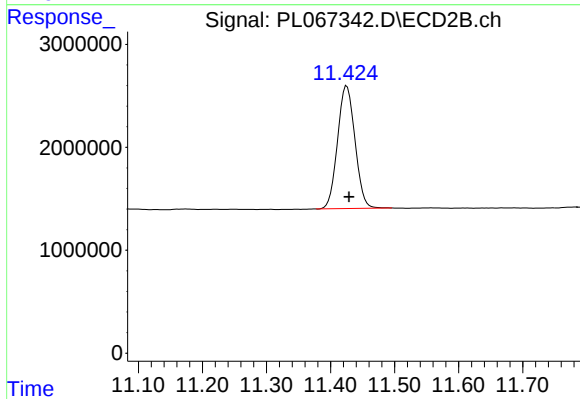

#28 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: -0.003 min
Response: 22570890
Conc: 22.66 ng/ml