

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
 Data File : PL067350.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2021 22:23
 Operator : AR\AJ
 Sample : M2625-33
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 08:59:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.528	12414439	19946891	22.581	21.159
28)	SA Decachlor...	10.220	11.425	15866949	23794202	22.389	23.888
Target Compounds							
2)	A alpha-BHC	5.169	0.000	359909	0	0.489	N.D. #
3)	MA gamma-BHC...	5.624f	0.000	210009	0	0.280	N.D. #
6)	B beta-BHC	5.962f	6.778f	722604	-316829	2.020	N.D. #
7)	B delta-BHC	6.245	7.005f	158421	2983983	0.214	2.538 #
8)	B Heptachlo...	0.000	7.962f	0	2874851	N.D.	2.870 #
15)	B Endosulfa...	0.000	9.176f	0	257604	N.D.	0.323 #
18)	B Endrin al...	8.378	0.000	324793	0	0.642	N.D. #
21)	B Endrin ke...	9.126	0.000	285045	0	0.374	N.D. #
24)	Chlordane-2	6.481	0.000	485197	0	18.119	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
Data File : PL067350.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2021 22:23
Operator : AR\AJ
Sample : M2625-33
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 08:59:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

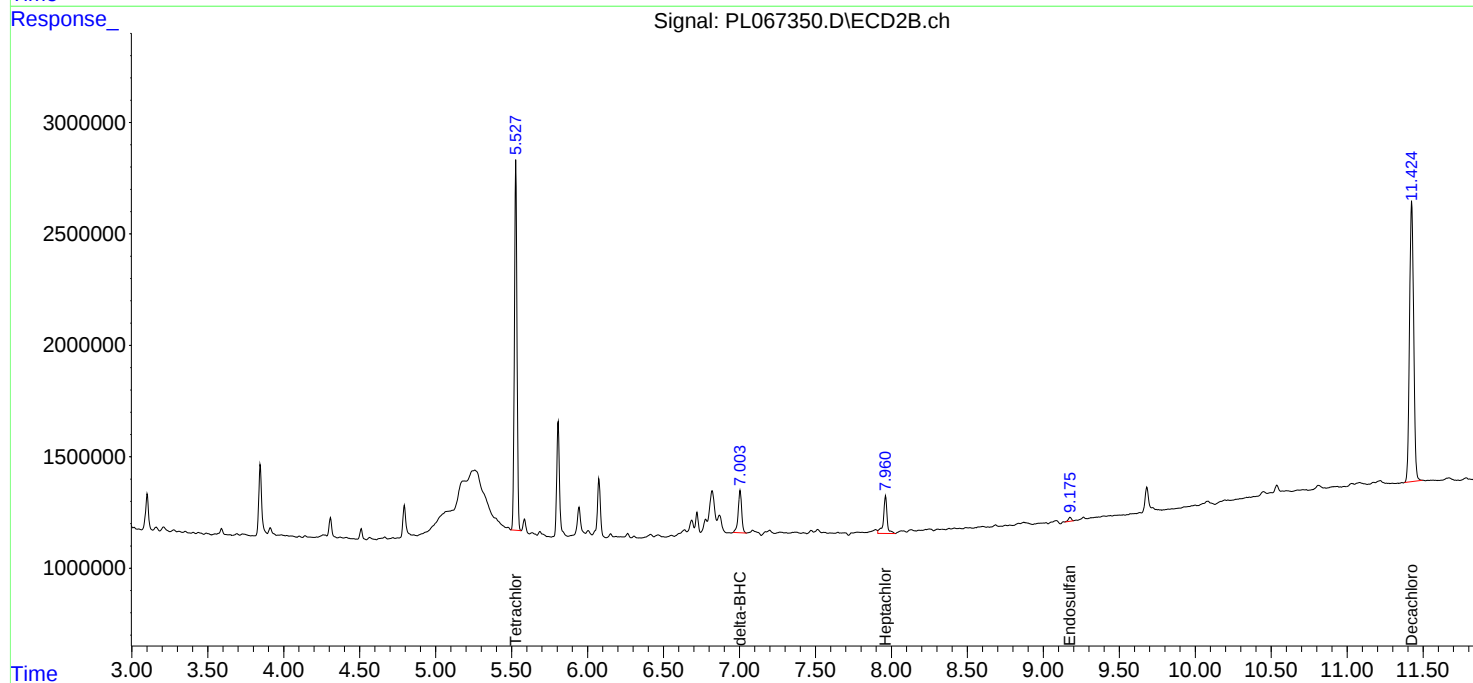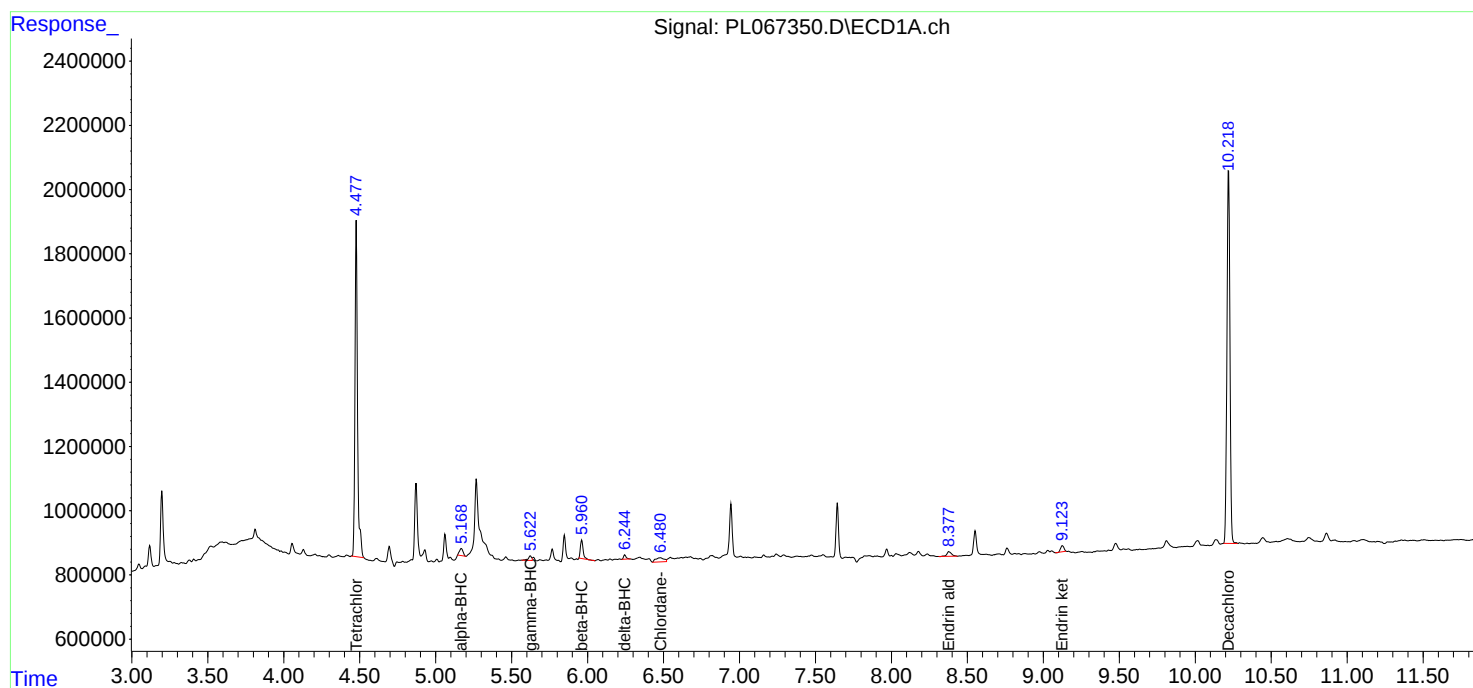


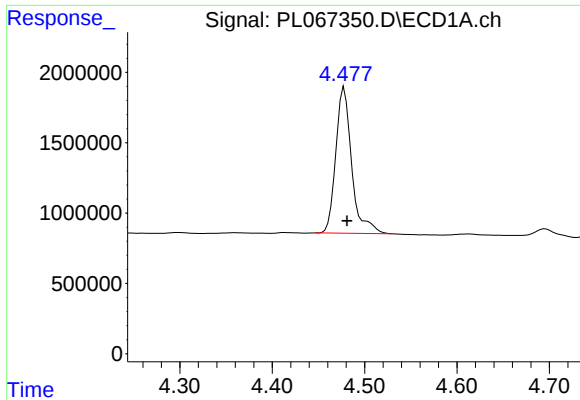

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 12414439
Conc: 22.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

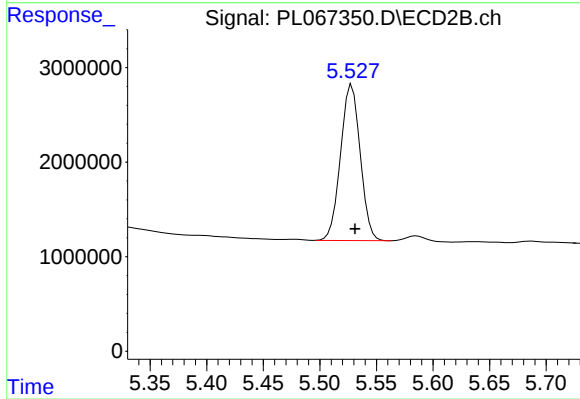


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 19946891
Conc: 21.16 ng/ml

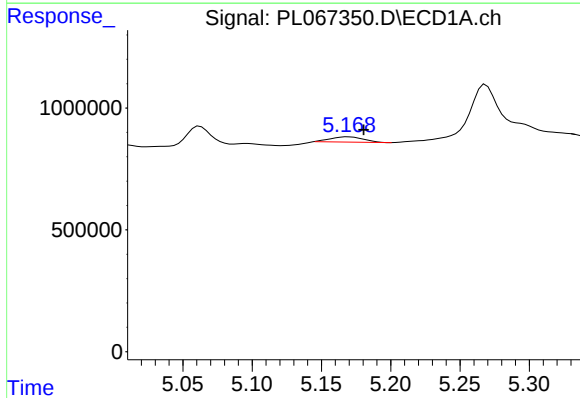


#2 alpha-BHC

R.T.: 5.169 min
Delta R.T.: -0.011 min
Response: 359909
Conc: 0.49 ng/ml

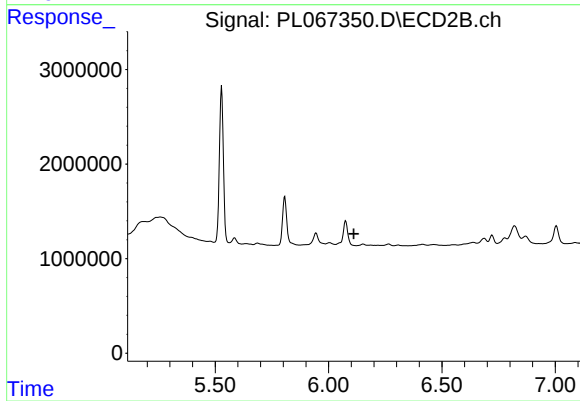

#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

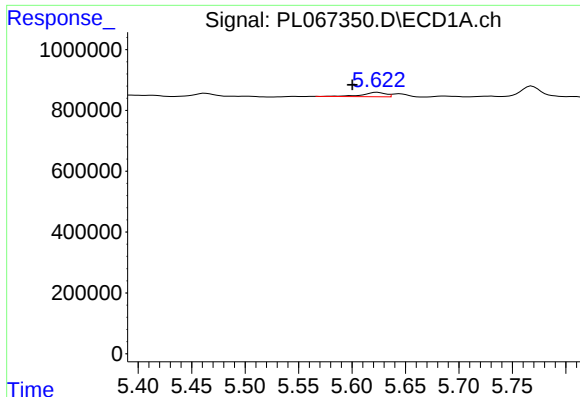

#3 gamma-BHC (Lindane)


R.T.: 5.624 min

Delta R.T.: 0.024 min

Response: 210009

Conc: 0.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

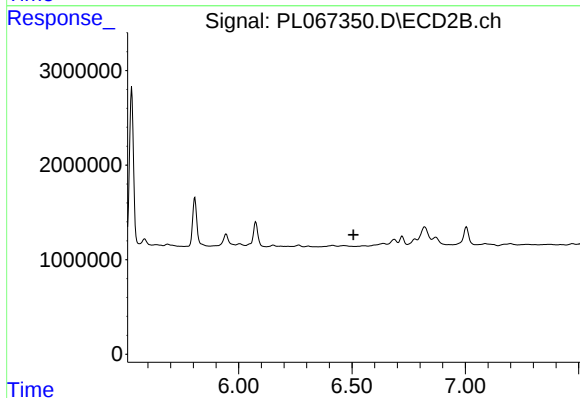


#3 gamma-BHC (Lindane)

R.T.: 0.000 min

Exp R.T. : 6.507 min

Response: 0

Conc: N.D.

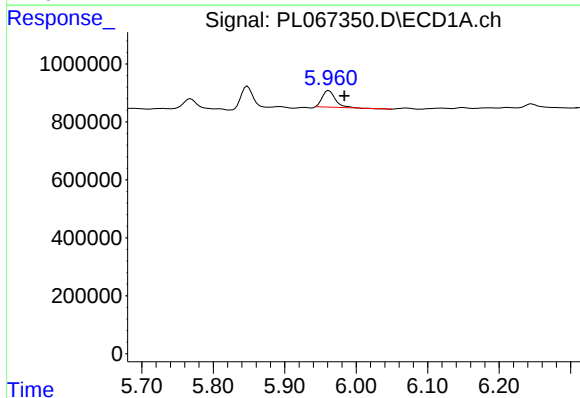


#6 beta-BHC

R.T.: 5.962 min

Delta R.T.: -0.022 min

Response: 722604

Conc: 2.02 ng/ml

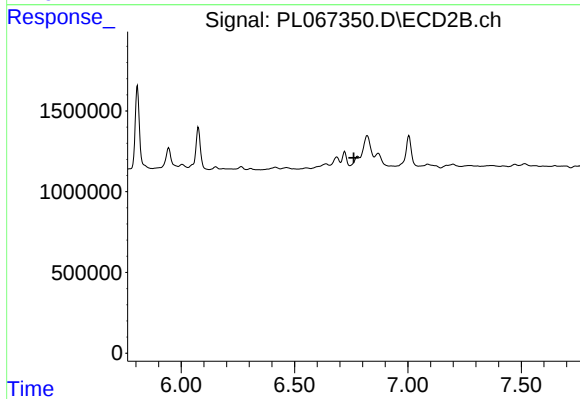


#6 beta-BHC

R.T.: 6.778 min

Delta R.T.: 0.016 min

Response: -316829


Conc: N.D.

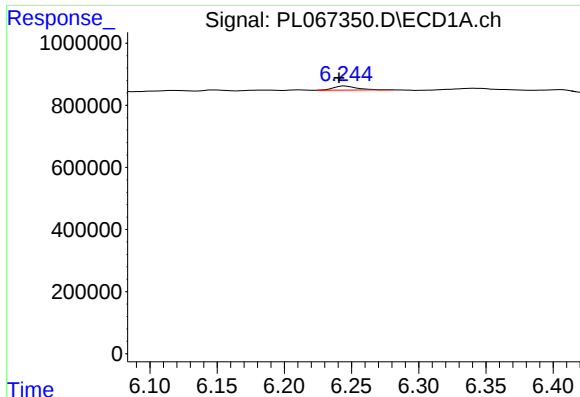

#7 delta-BHC


R.T.: 6.245 min
Delta R.T.: 0.005 min
Response: 158421
Conc: 0.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

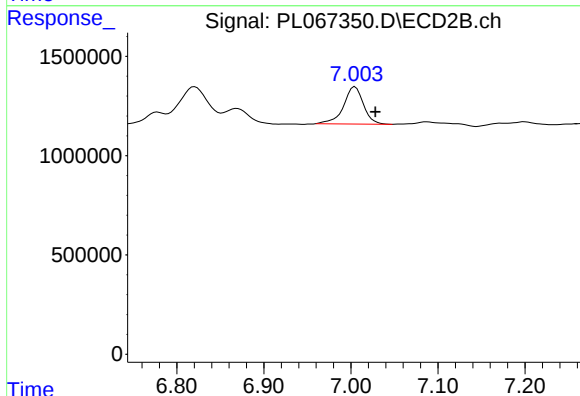


#7 delta-BHC

R.T.: 7.005 min
Delta R.T.: -0.023 min
Response: 2983983
Conc: 2.54 ng/ml

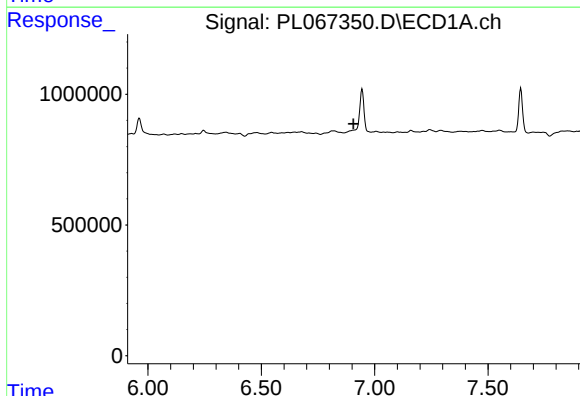


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.907 min
Response: 0
Conc: N.D.

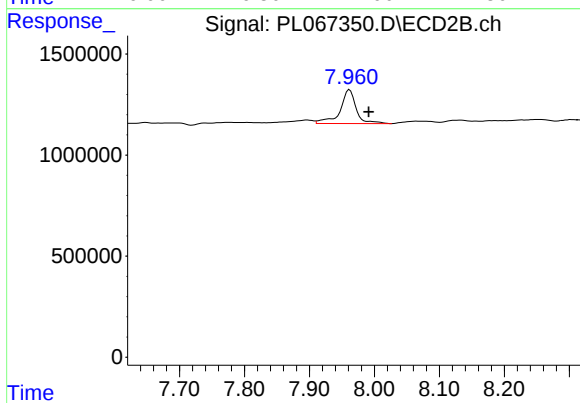

#8 Heptachlor epoxide


R.T.: 7.962 min
Delta R.T.: -0.029 min
Response: 2874851
Conc: 2.87 ng/ml

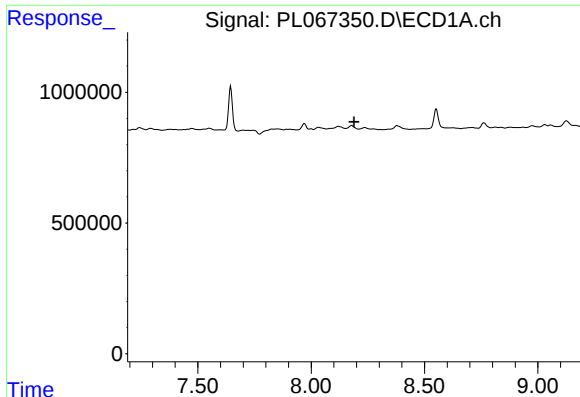

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

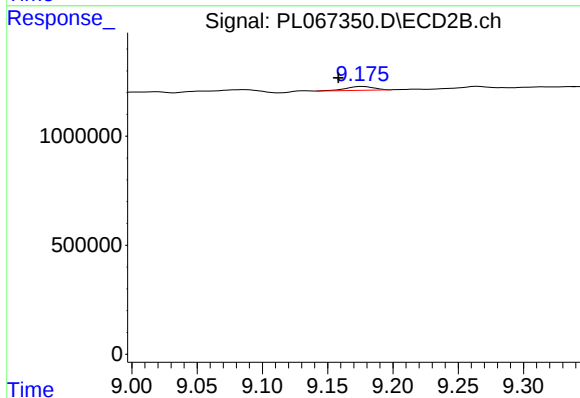


#15 Endosulfan II

R.T.: 9.176 min
Delta R.T.: 0.018 min
Response: 257604
Conc: 0.32 ng/ml

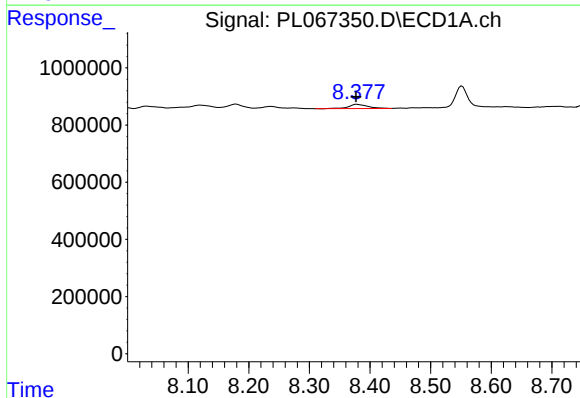


#18 Endrin aldehyde

R.T.: 8.378 min
Delta R.T.: 0.001 min
Response: 324793
Conc: 0.64 ng/ml

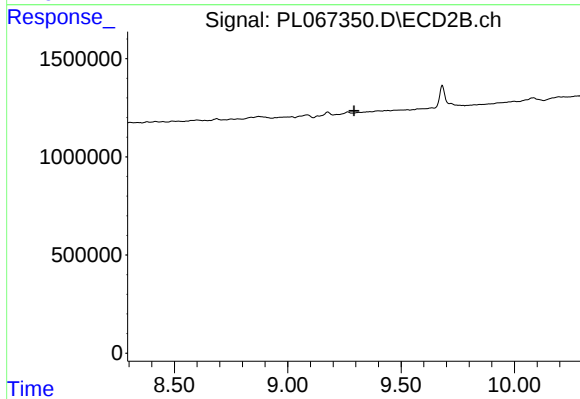

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 9.292 min
Response: 0
Conc: N.D.

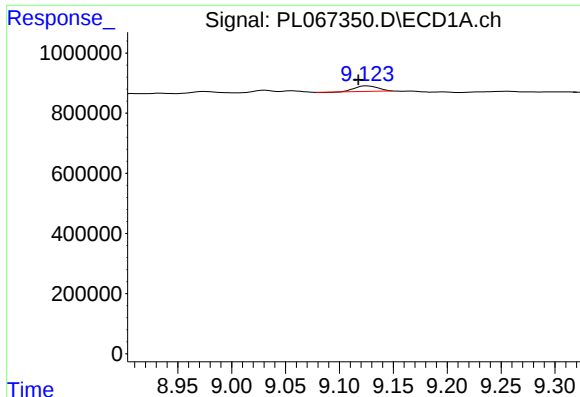

#21 Endrin ketone


R.T.: 9.126 min
Delta R.T.: 0.008 min
Response: 285045
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

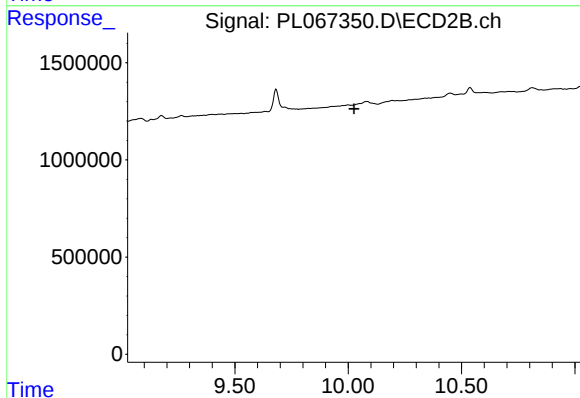


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 10.027 min
Response: 0
Conc: N.D.

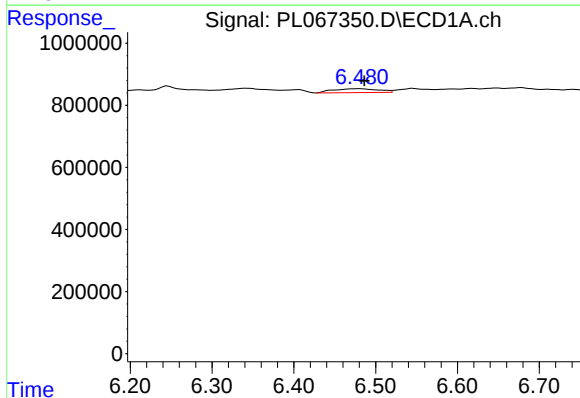


#24 Chlordane-2

R.T.: 6.481 min
Delta R.T.: -0.005 min
Response: 485197
Conc: 18.12 ng/ml

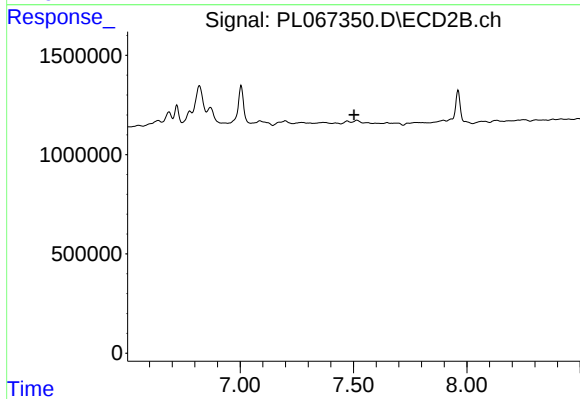

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

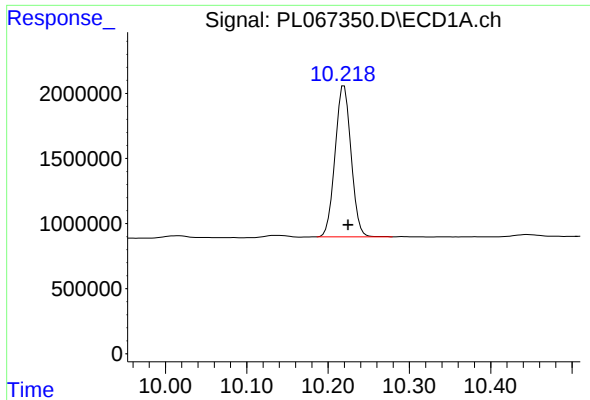

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.005 min
Response: 15866949
Conc: 22.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

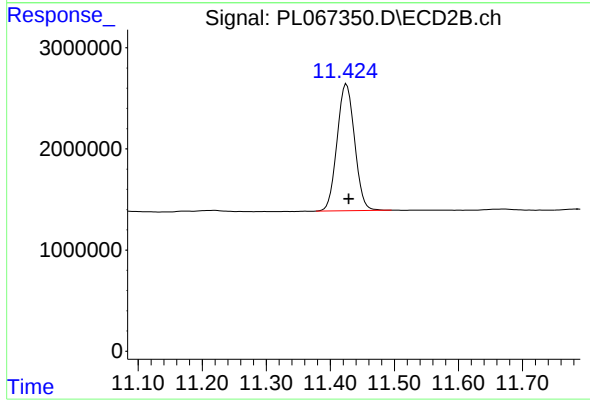

#28 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: -0.003 min
Response: 23794202
Conc: 23.89 ng/ml