

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
 Data File : PL067351.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2021 22:40
 Operator : AR\AJ
 Sample : M2625-34
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 08:59:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.528	12332227	20819711	22.431	22.084
28)	SA Decachlor...	10.220	11.426	16805271	25353163	23.713	25.454
Target Compounds							
2)	A alpha-BHC	5.165f	0.000	247697	0	0.337	N.D. #
7)	B delta-BHC	0.000	7.005f	0	2678532	N.D.	2.279 #
8)	B Heptachlo...	0.000	7.961f	0	2904380	N.D.	2.899 #
15)	B Endosulfa...	0.000	9.177f	0	596833	N.D.	0.749 #
24)	Chlordane-2	6.471f	0.000	582027	0	21.735	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
Data File : PL067351.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2021 22:40
Operator : AR\AJ
Sample : M2625-34
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 08:59:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

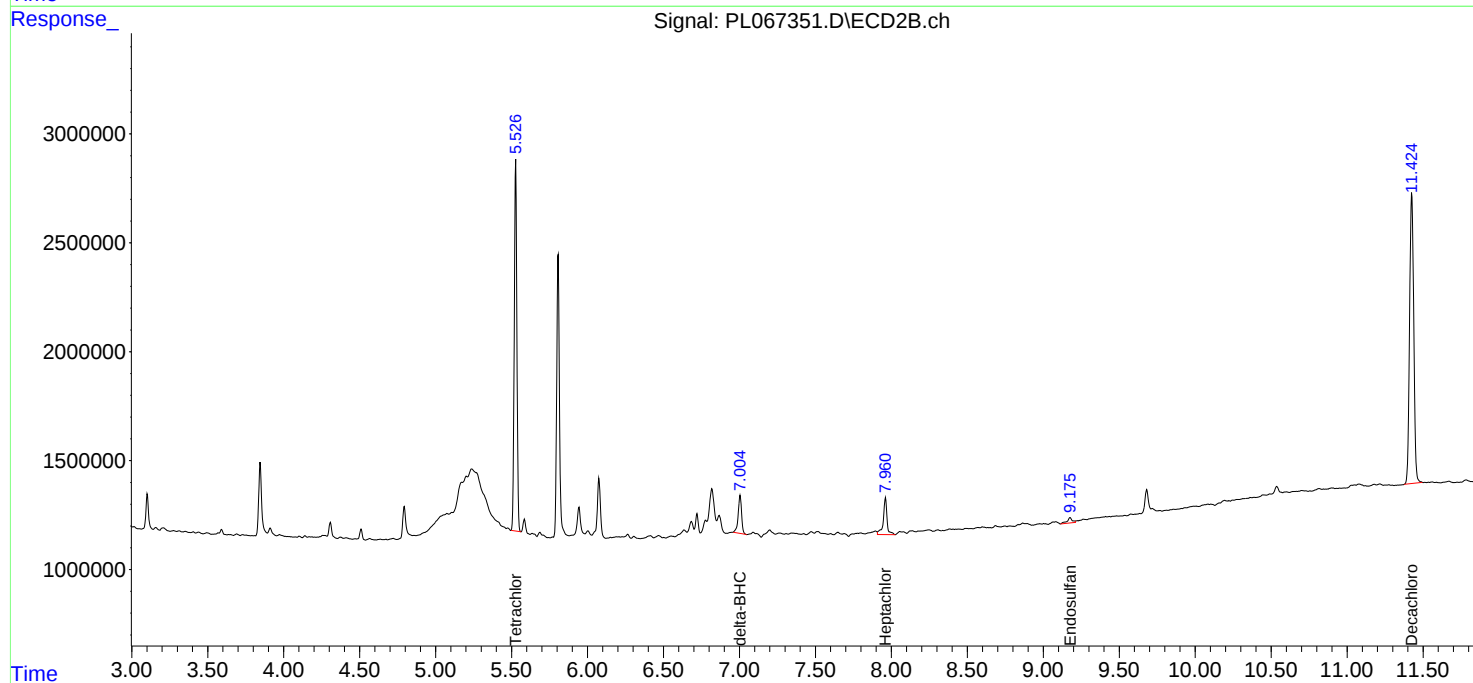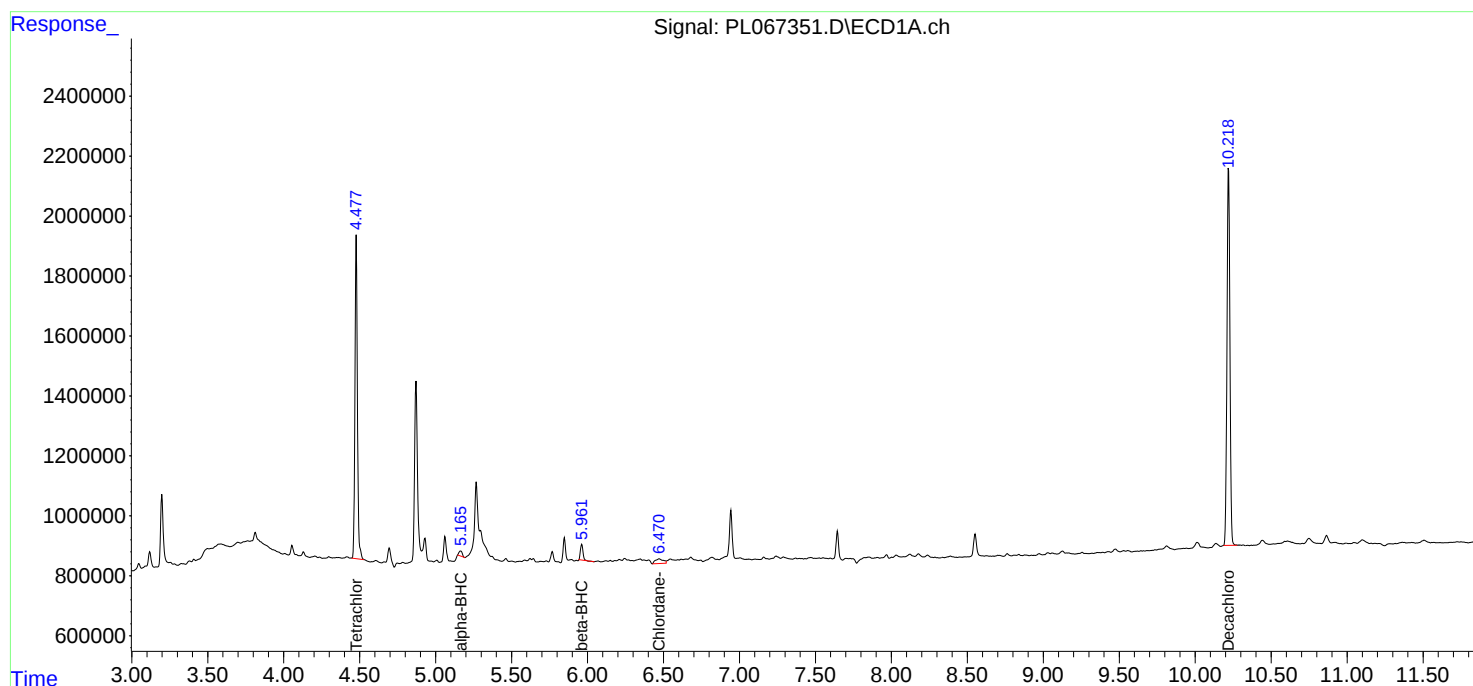


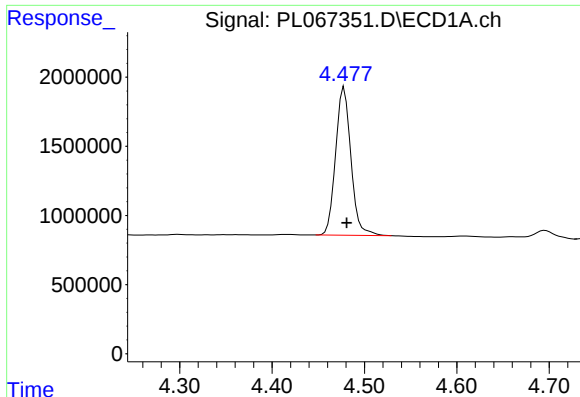

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 12332227
Conc: 22.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

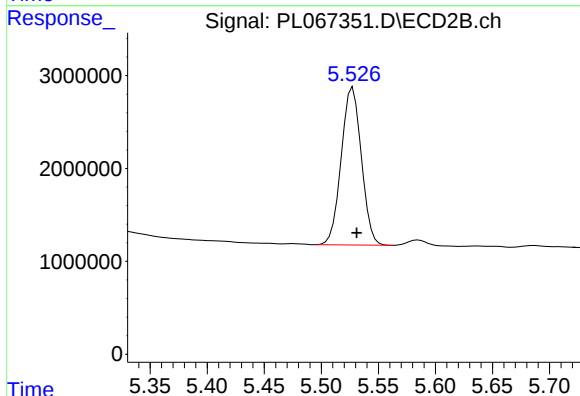


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 20819711
Conc: 22.08 ng/ml

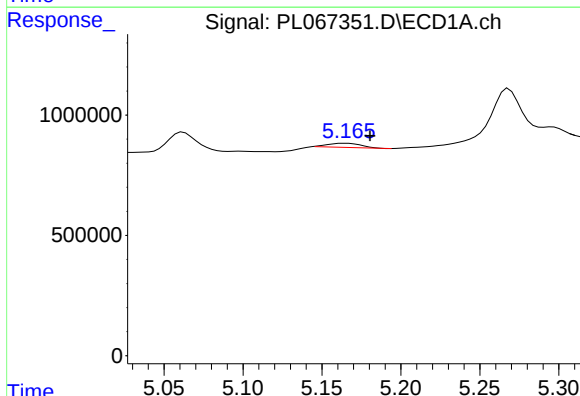


#2 alpha-BHC

R.T.: 5.165 min
Delta R.T.: -0.015 min
Response: 247697
Conc: 0.34 ng/ml

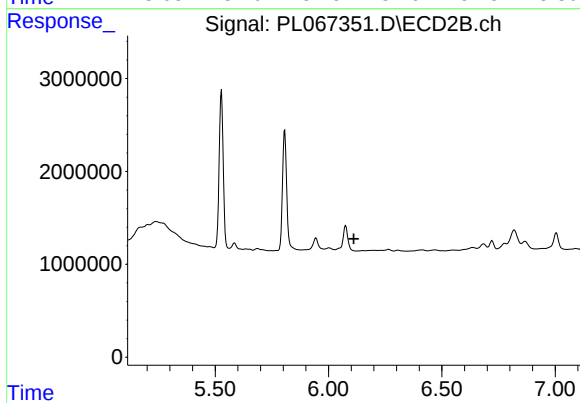

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

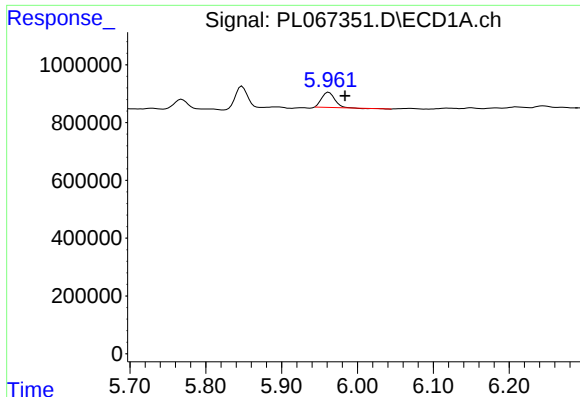

#6 beta-BHC


R.T.: 5.962 min
Delta R.T.: -0.021 min
Response: 630462
Conc: 1.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

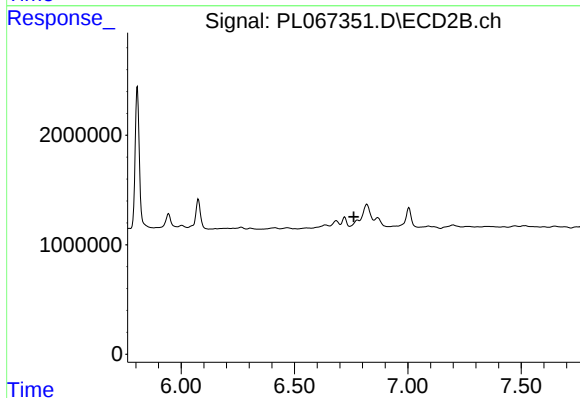


#6 beta-BHC

R.T.: 6.777 min
Delta R.T.: 0.015 min
Response: -991637
Conc: N.D.

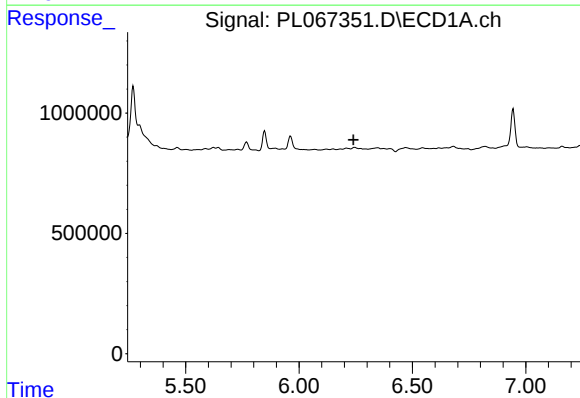


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

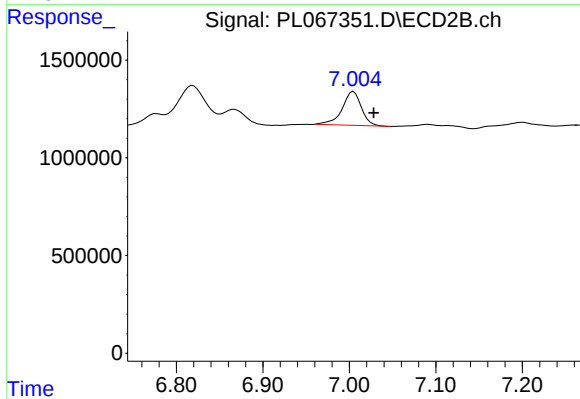

#7 delta-BHC


R.T.: 7.005 min
Delta R.T.: -0.023 min
Response: 2678532
Conc: 2.28 ng/ml

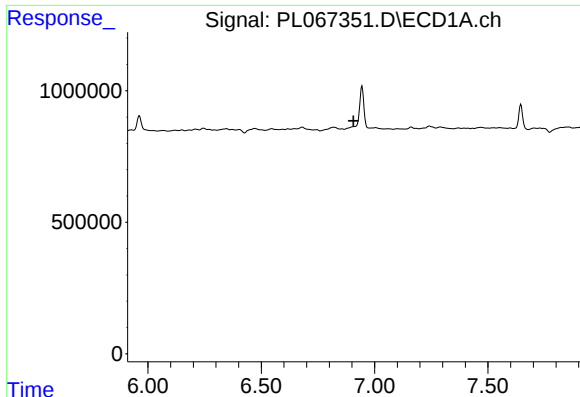

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 6.907 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

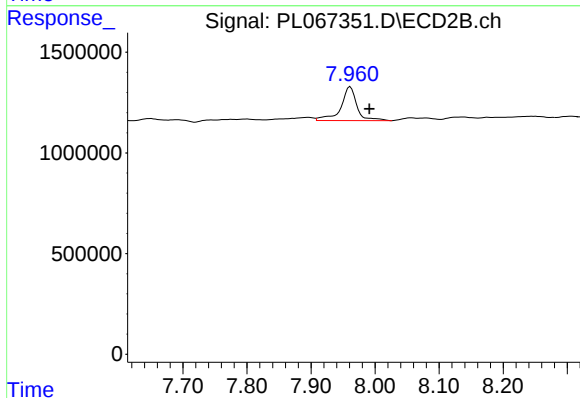


#8 Heptachlor epoxide

R.T.: 7.961 min
Delta R.T.: -0.030 min
Response: 2904380
Conc: 2.90 ng/ml

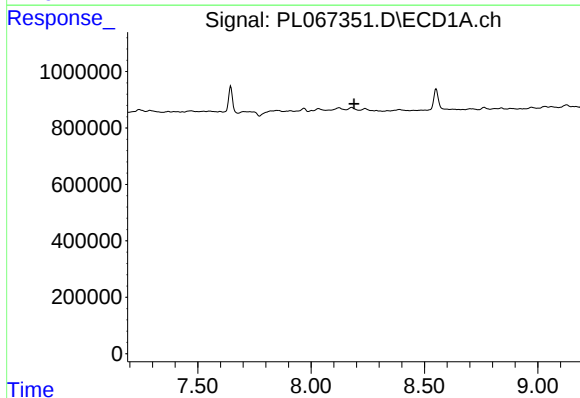


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.190 min
Response: 0
Conc: N.D.

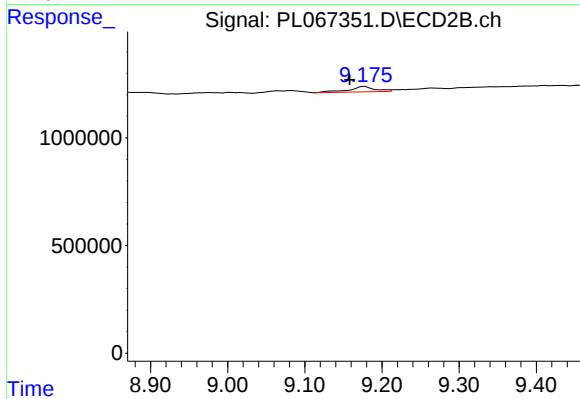

#15 Endosulfan II


R.T.: 9.177 min
Delta R.T.: 0.018 min
Response: 596833
Conc: 0.75 ng/ml

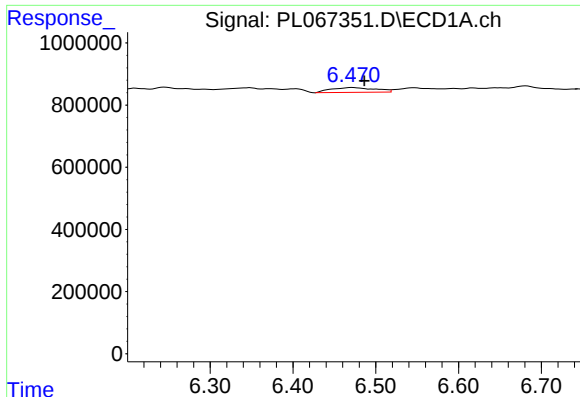

#24 Chlordane-2


R.T.: 6.471 min
Delta R.T.: -0.015 min
Response: 582027
Conc: 21.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

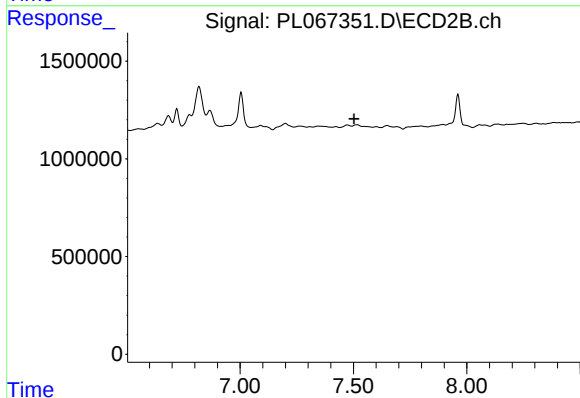


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

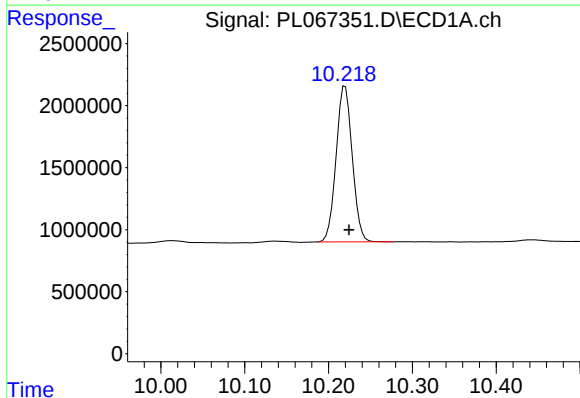

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.005 min
Response: 16805271
Conc: 23.71 ng/ml

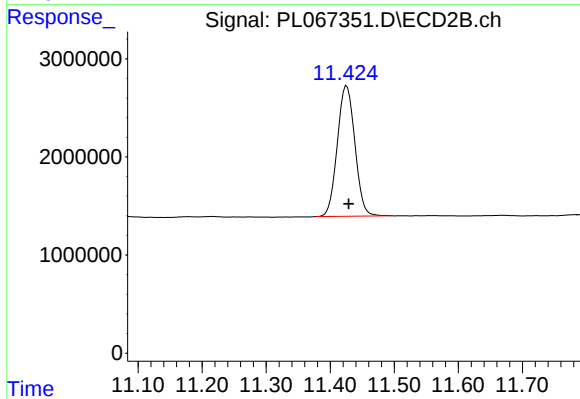

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.003 min
Response: 25353163
Conc: 25.45 ng/ml