

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
 Data File : PL067361.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2021 01:26
 Operator : AR\AJ
 Sample : M2673-01
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 09:01:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.528	10978310	18766553	19.968	19.907
28)	SA Decachlor...	10.219	11.425	11387328	16799700	16.068	16.866
Target Compounds							
2)	A alpha-BHC	5.165f	0.000	250994	0	0.341	N.D. #
7)	B delta-BHC	0.000	7.000f	0	1242254	N.D.	1.057 #
15)	B Endosulfa...	0.000	9.178f	0	2300428	N.D.	2.885 #
22)	Mirex	9.296	0.000	143052	0	0.227	N.D. #
24)	Chlordane-2	6.474	0.000	610179	0	22.786	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
Data File : PL067361.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2021 01:26
Operator : AR\AJ
Sample : M2673-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 09:01:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

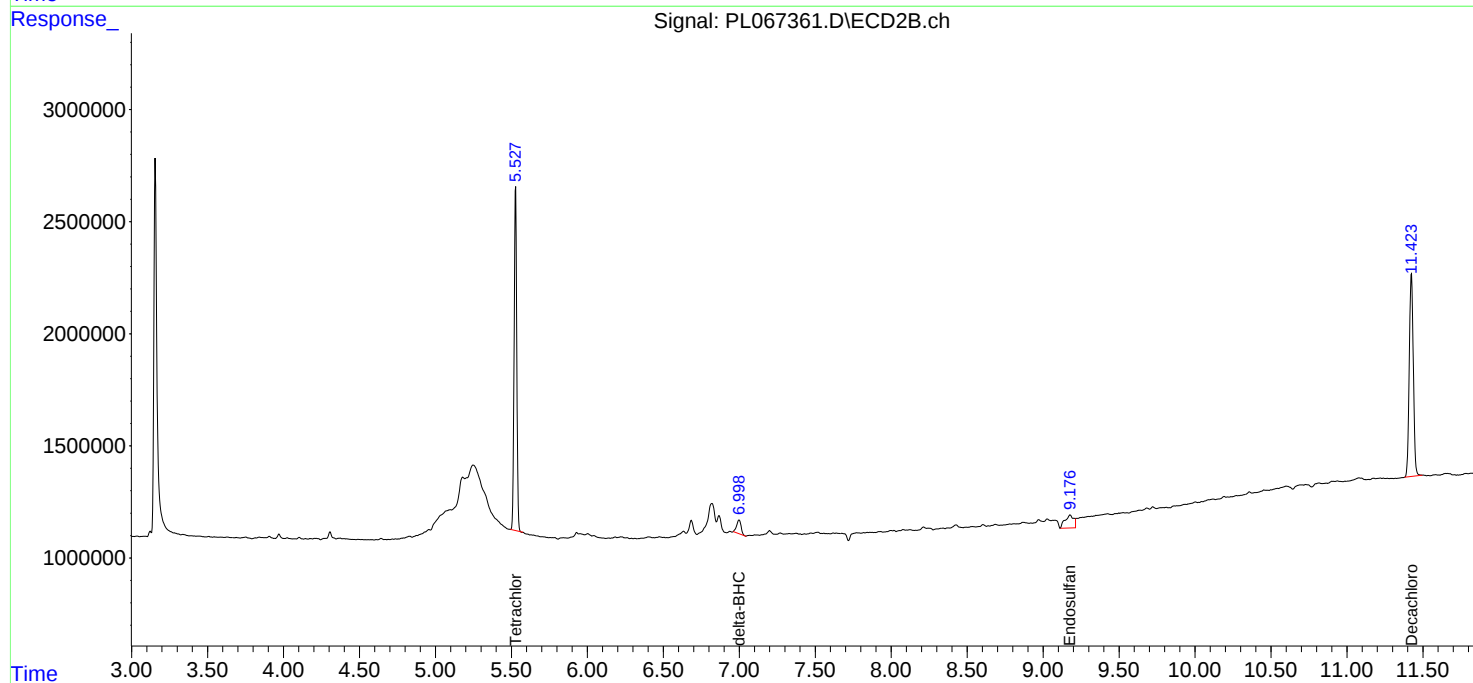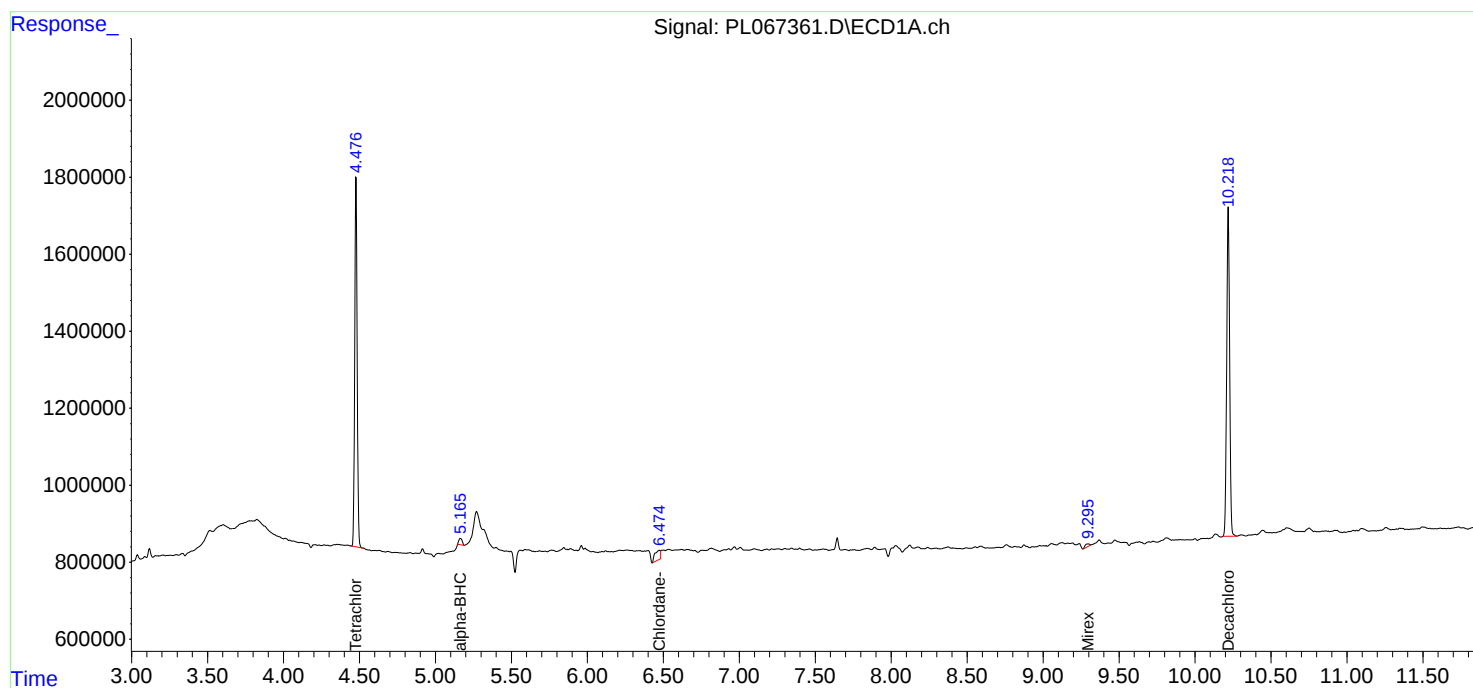


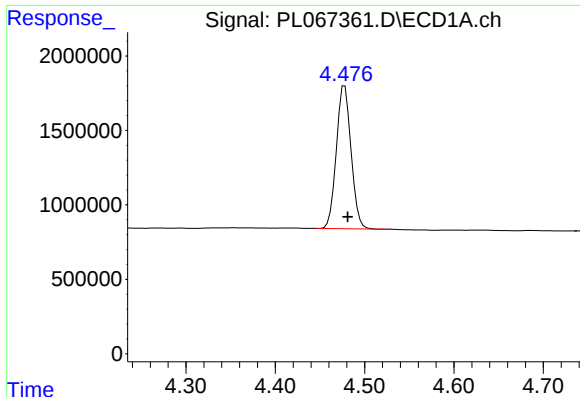

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 10978310
Conc: 19.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

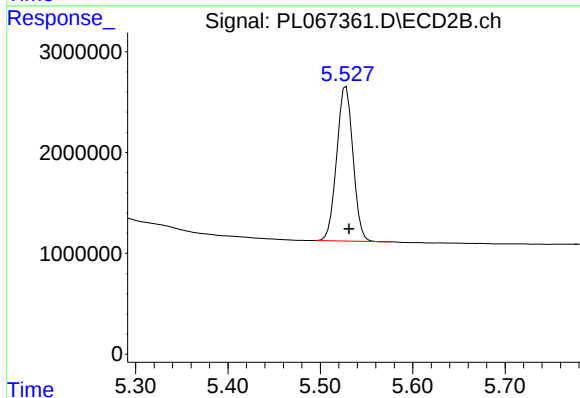


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 18766553
Conc: 19.91 ng/ml

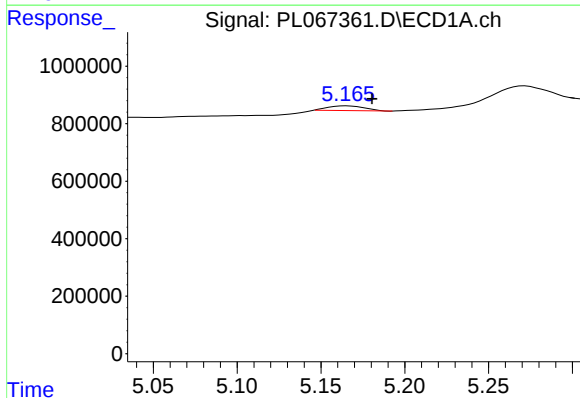


#2 alpha-BHC

R.T.: 5.165 min
Delta R.T.: -0.016 min
Response: 250994
Conc: 0.34 ng/ml

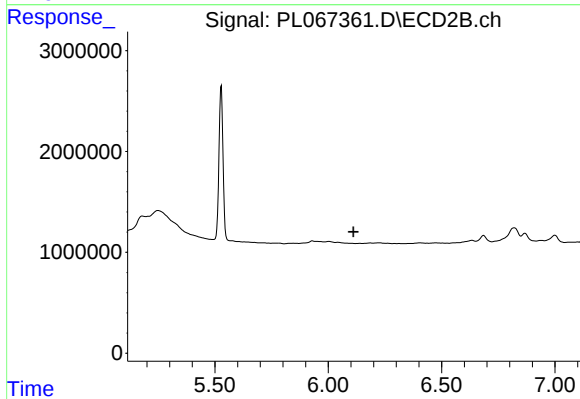

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

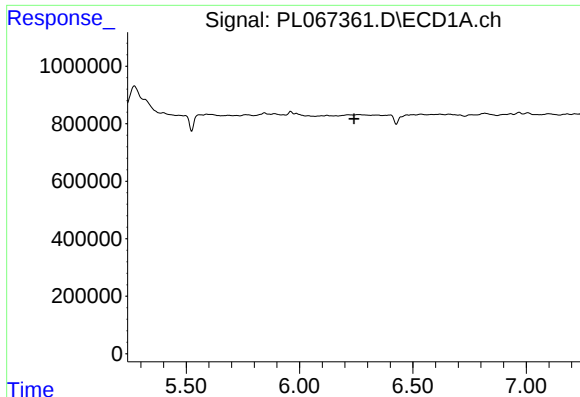

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

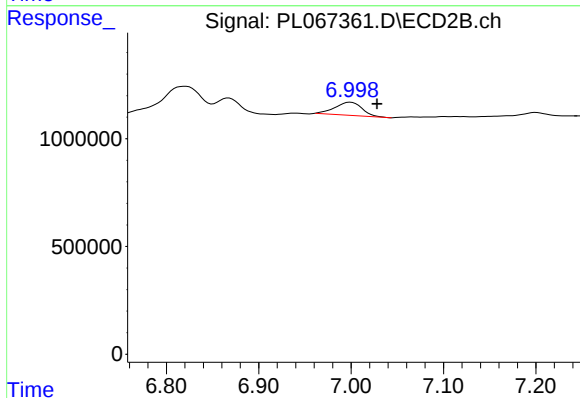


#7 delta-BHC

R.T.: 7.000 min
Delta R.T.: -0.029 min
Response: 1242254
Conc: 1.06 ng/ml

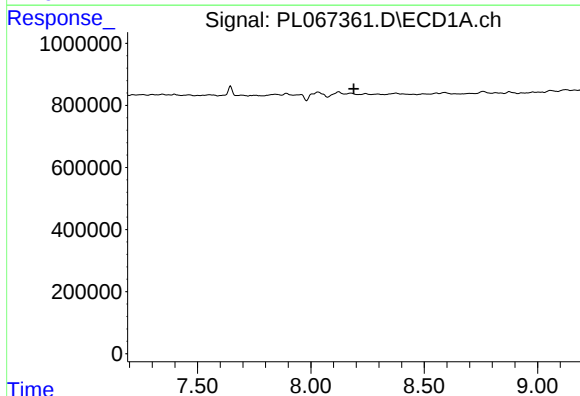


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.190 min
Response: 0
Conc: N.D.

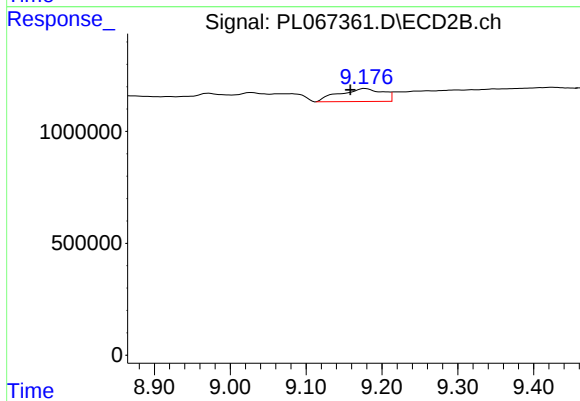

#15 Endosulfan II

R.T.: 9.178 min
Delta R.T.: 0.019 min
Response: 2300428
Conc: 2.89 ng/ml

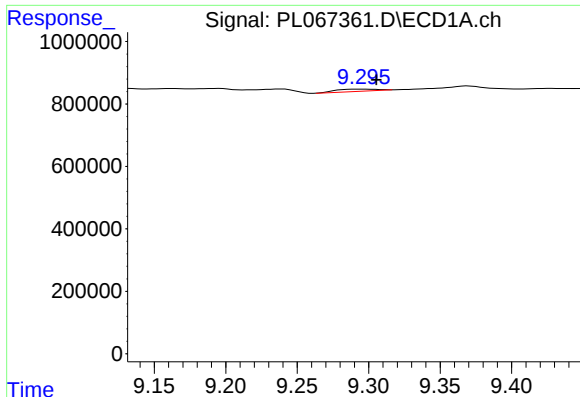

#22 Mirex


R.T.: 9.296 min

Delta R.T.: -0.009 min

Response: 143052

Conc: 0.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

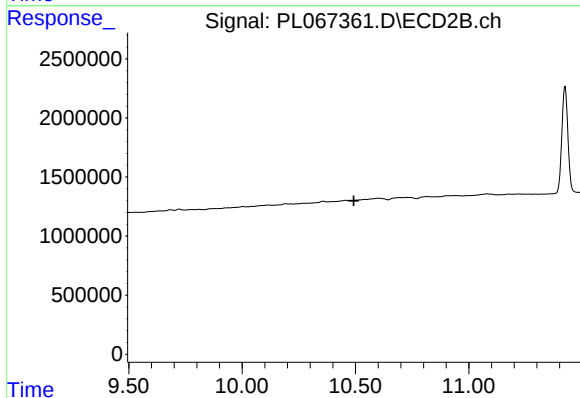


#22 Mirex

R.T.: 0.000 min

Exp R.T. : 10.492 min

Response: 0

Conc: N.D.

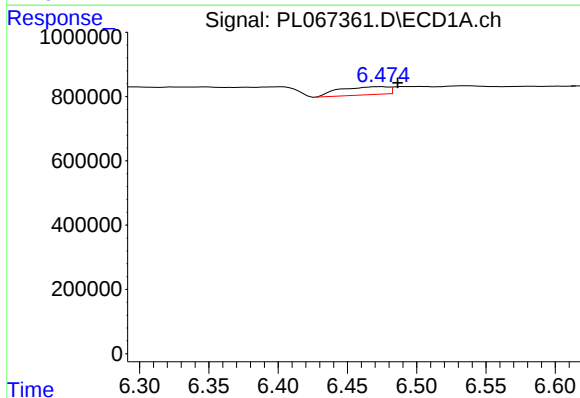


#24 Chlordane-2

R.T.: 6.474 min

Delta R.T.: -0.012 min

Response: 610179

Conc: 22.79 ng/ml

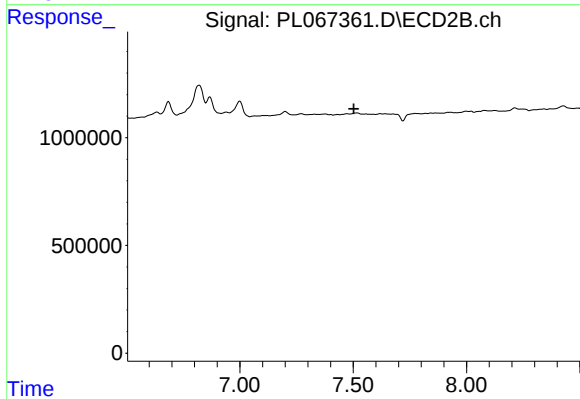


#24 Chlordane-2

R.T.: 0.000 min

Exp R.T. : 7.503 min

Response: 0


Conc: N.D.

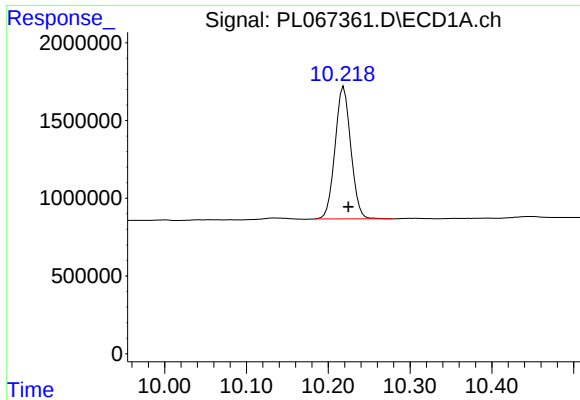

#28 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.005 min
Response: 11387328
Conc: 16.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

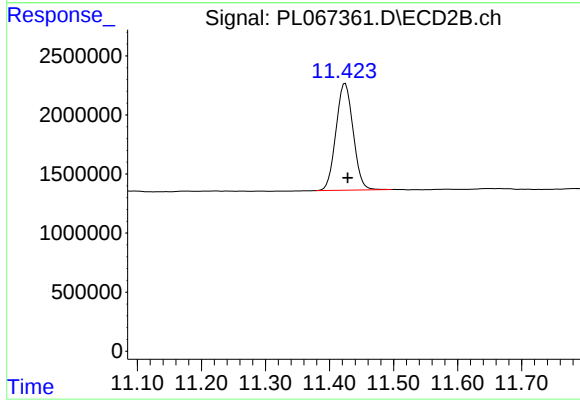

#28 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: -0.004 min
Response: 16799700
Conc: 16.87 ng/ml