

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
 Data File : PL067365.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2021 02:32
 Operator : AR\AJ
 Sample : M2673-03
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 09:02:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	5.528	11700132	19978587	21.281	21.192
28)	SA Decachlor...	10.219	11.426	14583615	21268692	20.578	21.353
Target Compounds							
6)	B beta-BHC	5.961f	0.000	246321	0	0.688	N.D. #
7)	B delta-BHC	0.000	7.002f	0	1325322	N.D.	1.127 #
8)	B Heptachlo...	0.000	8.021f	0	2204882	N.D.	2.201 #
14)	MA Endrin	7.893	0.000	193512	0	0.295	N.D. #
15)	B Endosulfa...	0.000	9.179f	0	581847	N.D.	0.730 #
18)	B Endrin al...	8.355f	0.000	6063	0	0.012	N.D. #
19)	B Endosulfa...	8.588f	0.000	364148	0	0.574	N.D. #
20)	A Methoxychlor	8.882f	9.859	749127	760667	2.107	1.956
21)	B Endrin ke...	9.101f	10.040	321556	504366	0.422	0.556 #
24)	Chlordane-2	6.468f	0.000	2037940	0	76.104	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
Data File : PL067365.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2021 02:32
Operator : AR\AJ
Sample : M2673-03
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 09:02:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

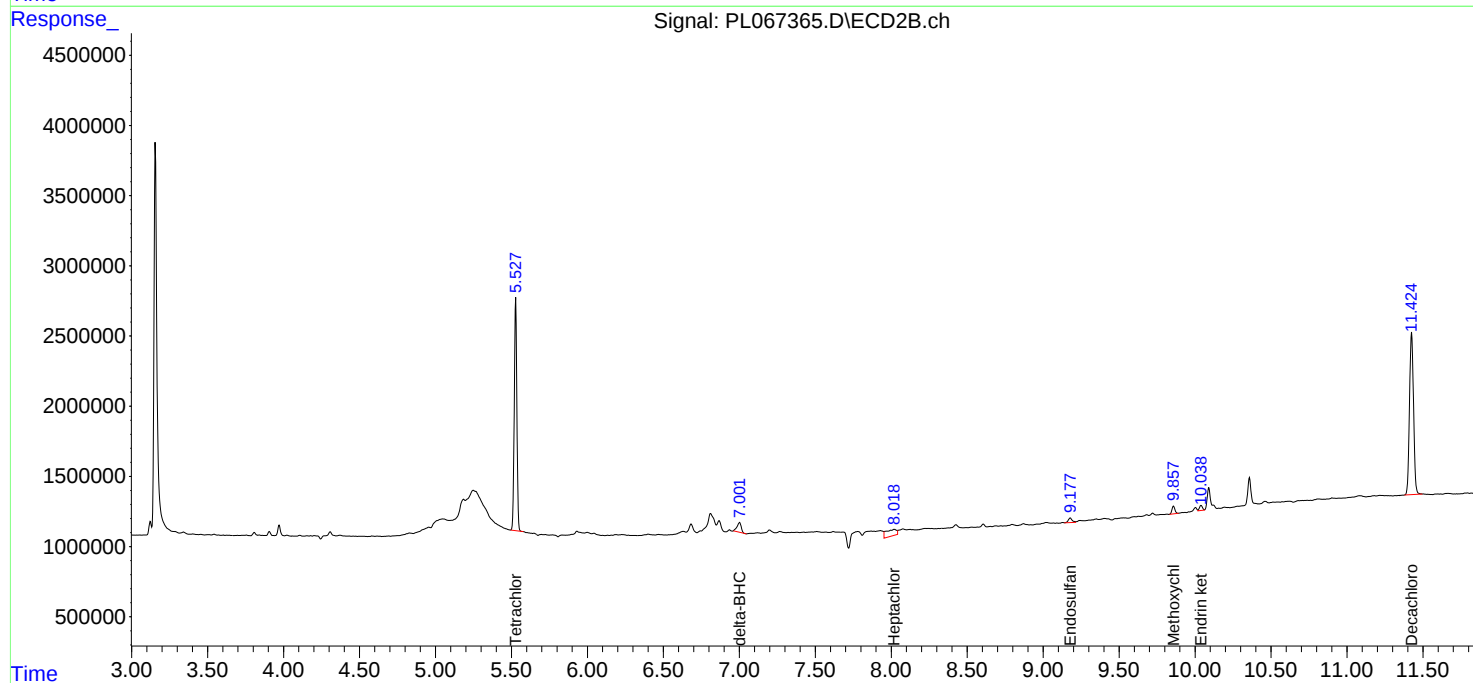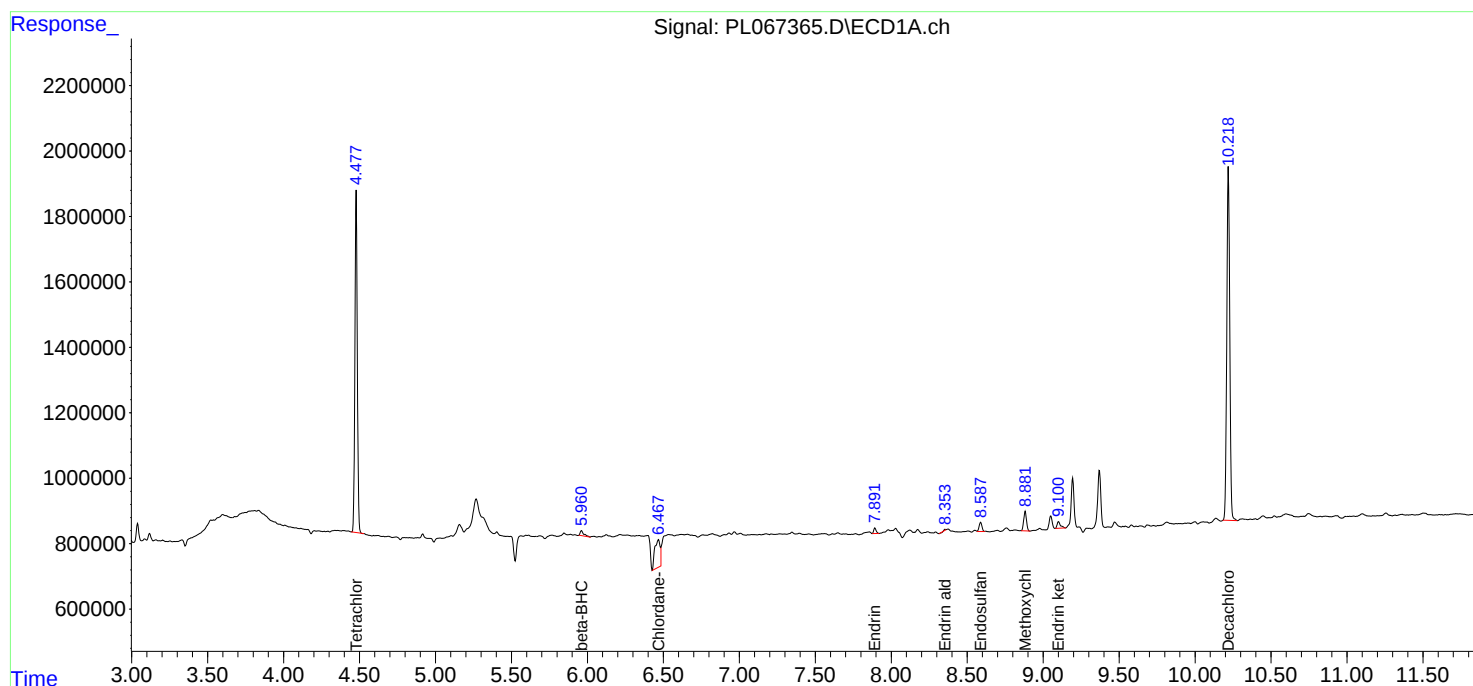


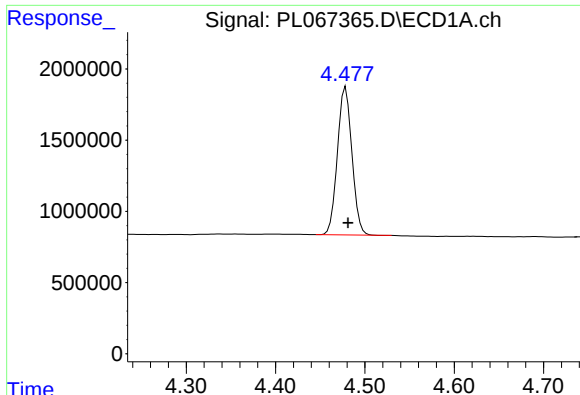

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: -0.002 min
Response: 11700132
Conc: 21.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

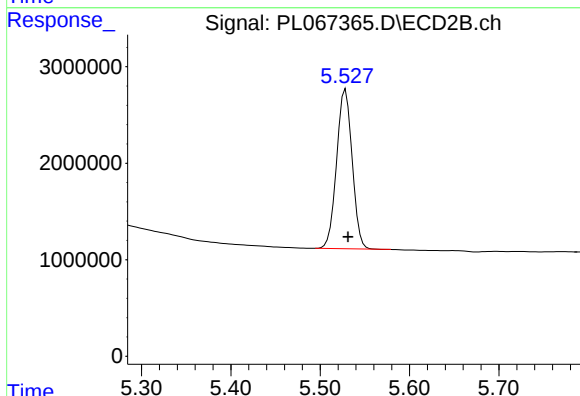


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 19978587
Conc: 21.19 ng/ml

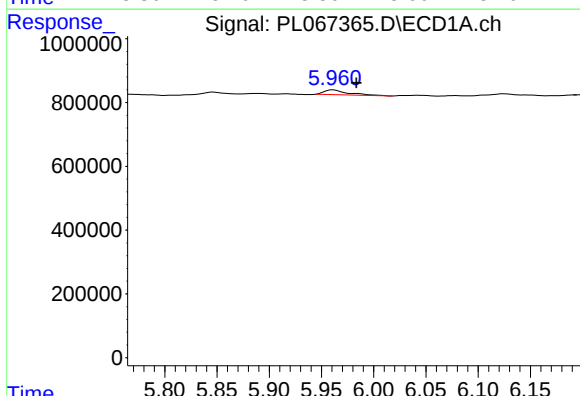


#6 beta-BHC

R.T.: 5.961 min
Delta R.T.: -0.022 min
Response: 246321
Conc: 0.69 ng/ml

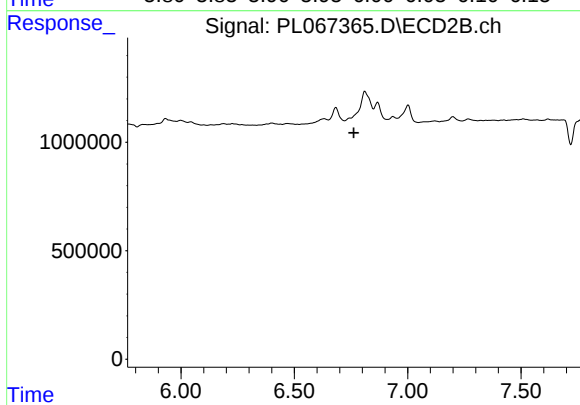

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.762 min
Response: 0
Conc: N.D.

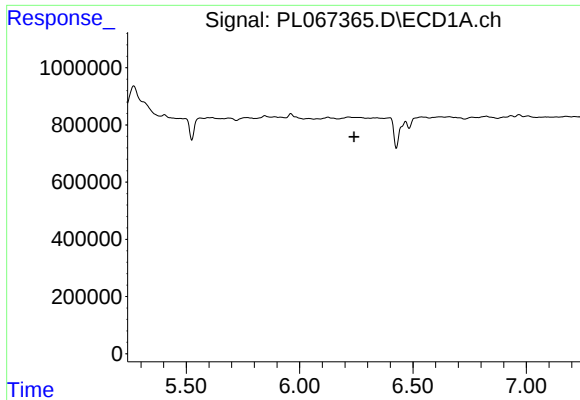

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

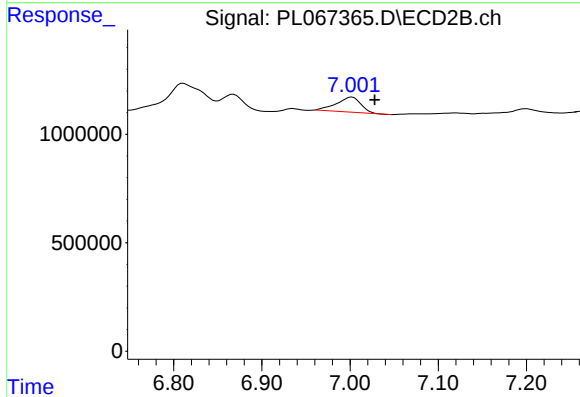


#7 delta-BHC

R.T.: 7.002 min
Delta R.T.: -0.026 min
Response: 1325322
Conc: 1.13 ng/ml

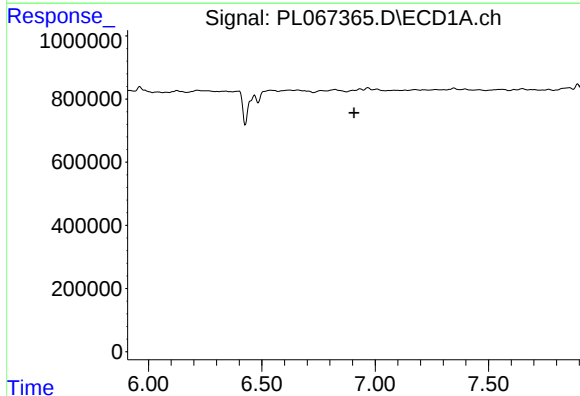


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.907 min
Response: 0
Conc: N.D.

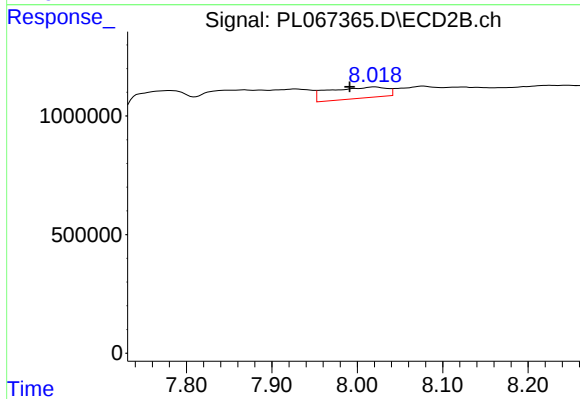

#8 Heptachlor epoxide


R.T.: 8.021 min
Delta R.T.: 0.029 min
Response: 2204882
Conc: 2.20 ng/ml

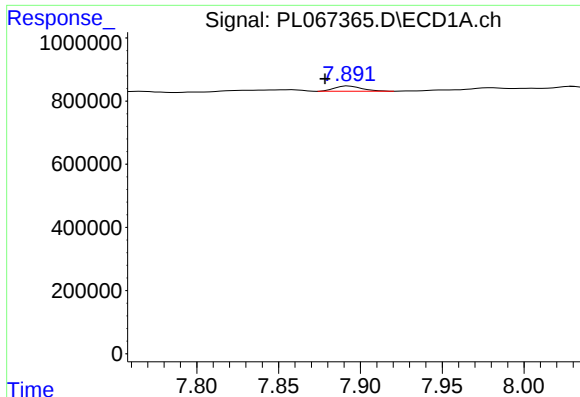

#14 Endrin


R.T.: 7.893 min
Delta R.T.: 0.015 min
Response: 193512
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

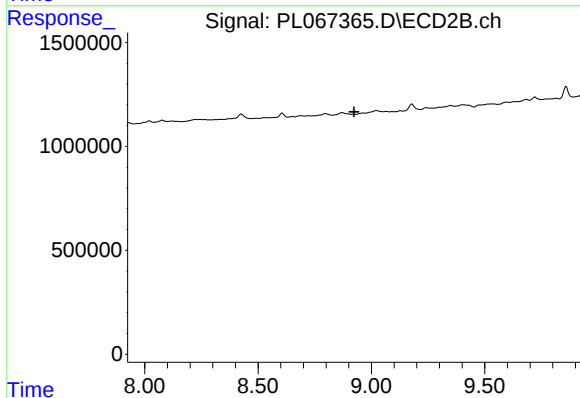


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.924 min
Response: 0
Conc: N.D.

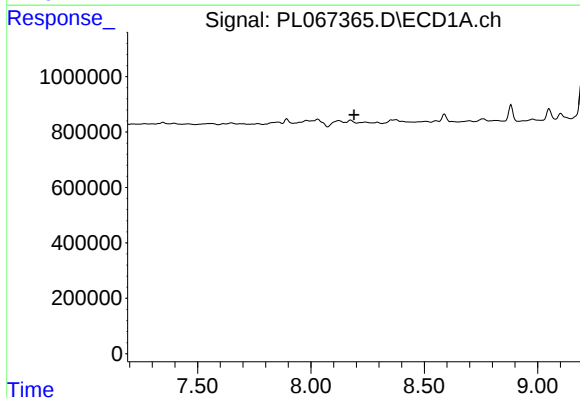


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.190 min
Response: 0
Conc: N.D.

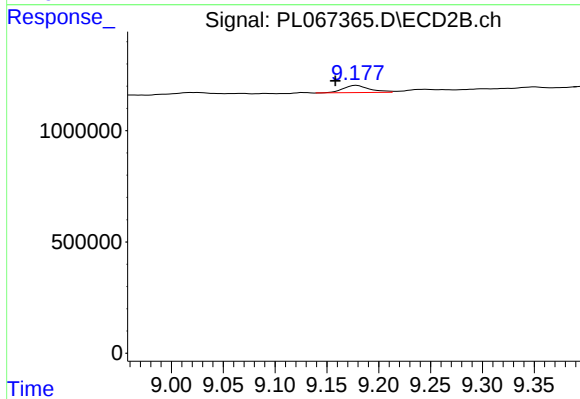

#15 Endosulfan II


R.T.: 9.179 min
Delta R.T.: 0.020 min
Response: 581847
Conc: 0.73 ng/ml

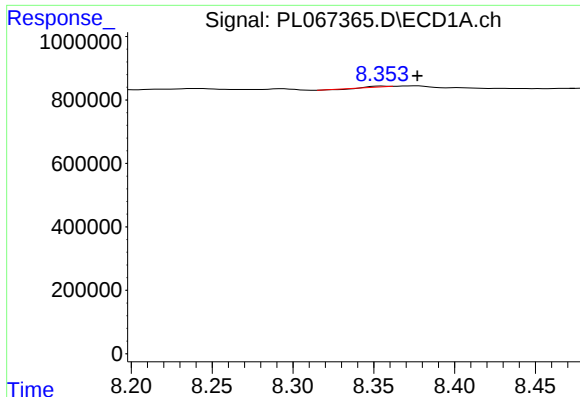

#18 Endrin aldehyde


R.T.: 8.355 min
Delta R.T.: -0.022 min
Response: 6063
Conc: 0.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

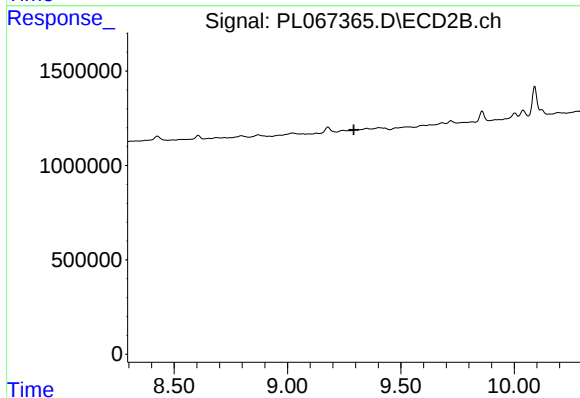


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 9.292 min
Response: 0
Conc: N.D.

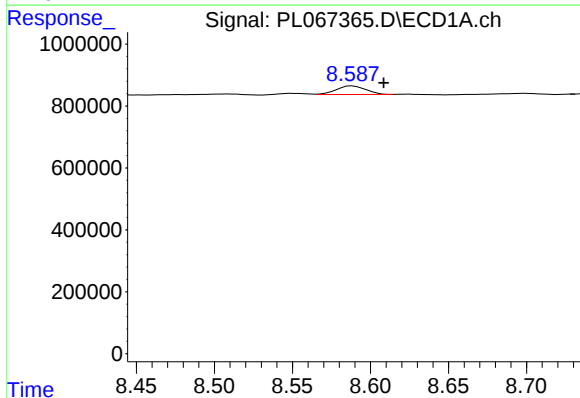


#19 Endosulfan Sulfate

R.T.: 8.588 min
Delta R.T.: -0.020 min
Response: 364148
Conc: 0.57 ng/ml

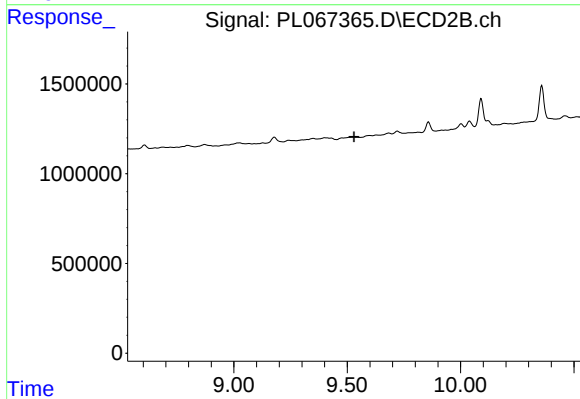

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 9.530 min
Response: 0
Conc: N.D.

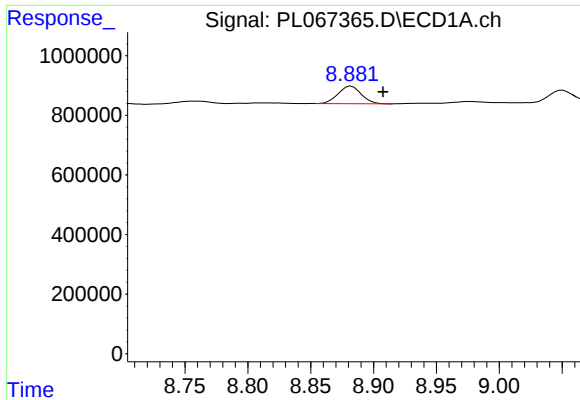

#20 Methoxychlor


R.T.: 8.882 min
Delta R.T.: -0.025 min
Response: 749127
Conc: 2.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

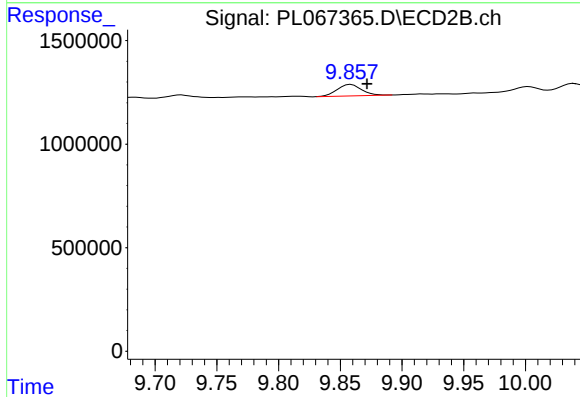


#20 Methoxychlor

R.T.: 9.859 min
Delta R.T.: -0.013 min
Response: 760667
Conc: 1.96 ng/ml

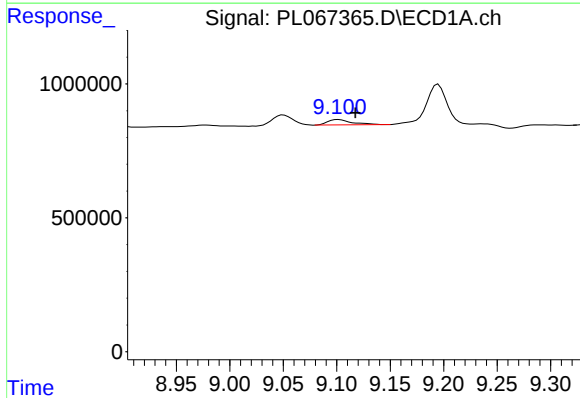


#21 Endrin ketone

R.T.: 9.101 min
Delta R.T.: -0.016 min
Response: 321556
Conc: 0.42 ng/ml

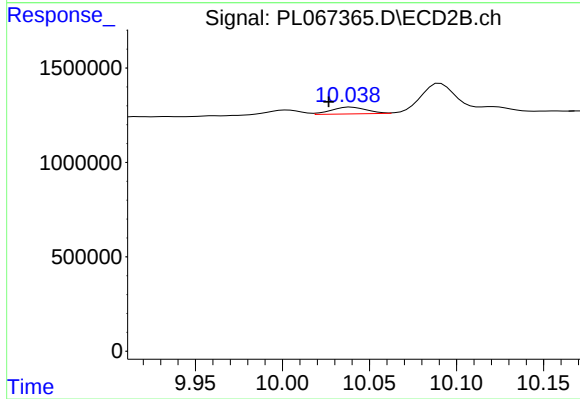

#21 Endrin ketone


R.T.: 10.040 min
Delta R.T.: 0.013 min
Response: 504366
Conc: 0.56 ng/ml

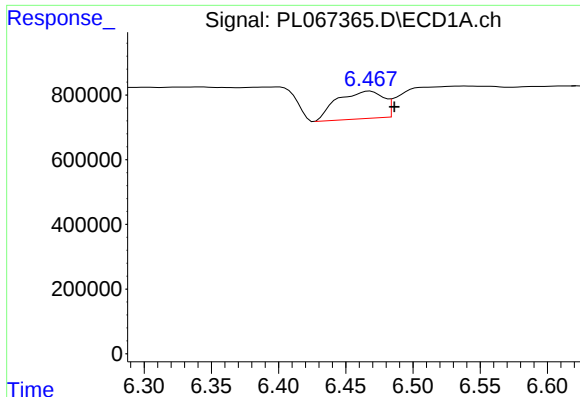

#24 Chlordane-2


R.T.: 6.468 min
Delta R.T.: -0.018 min
Response: 2037940
Conc: 76.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

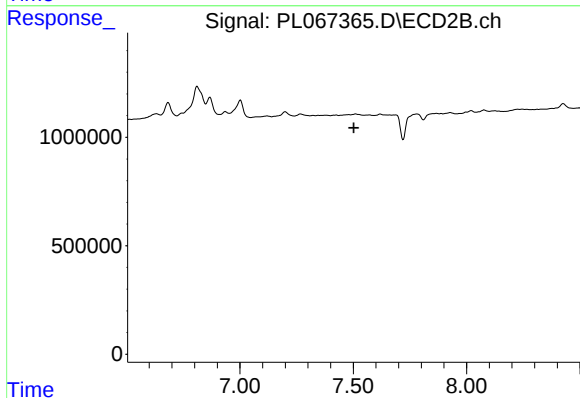


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

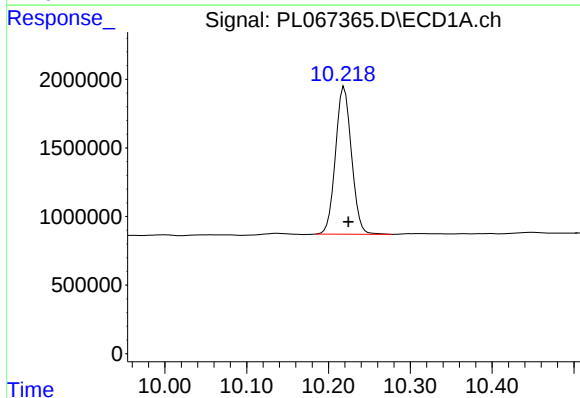

#28 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.005 min
Response: 14583615
Conc: 20.58 ng/ml

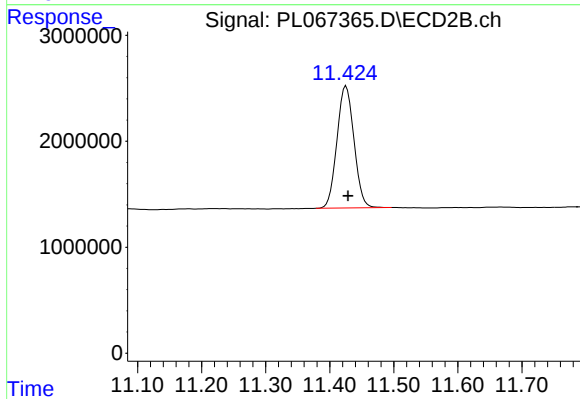

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.003 min
Response: 21268692
Conc: 21.35 ng/ml