

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
 Data File : PL067366.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2021 02:49
 Operator : AR\AJ
 Sample : M2674-01
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 09:03:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.528	11824604	19284545	21.508	20.456
28)	SA Decachlor...	10.220	11.426	18896592	27910434	26.664	28.021
Target Compounds							
2)	A alpha-BHC	5.159f	6.111	381772	376727	0.519	0.305 #
6)	B beta-BHC	5.966f	6.764	823117	157976	2.300	0.291 #
7)	B delta-BHC	0.000	7.003f	0	930857	N.D.	0.792 #
12)	B 4,4'-DDE	7.460	0.000	253715	0	0.381	N.D. #
14)	MA Endrin	7.895f	0.000	555702	0	0.848	N.D. #
17)	MA 4,4'-DDT	8.341f	0.000	347724	0	0.598	N.D. #
18)	B Endrin al...	8.384	0.000	56743	0	0.112	N.D. #
23)	Chlordane-1	5.785f	0.000	692151	0	37.410	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
Data File : PL067366.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2021 02:49
Operator : AR\AJ
Sample : M2674-01
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 09:03:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

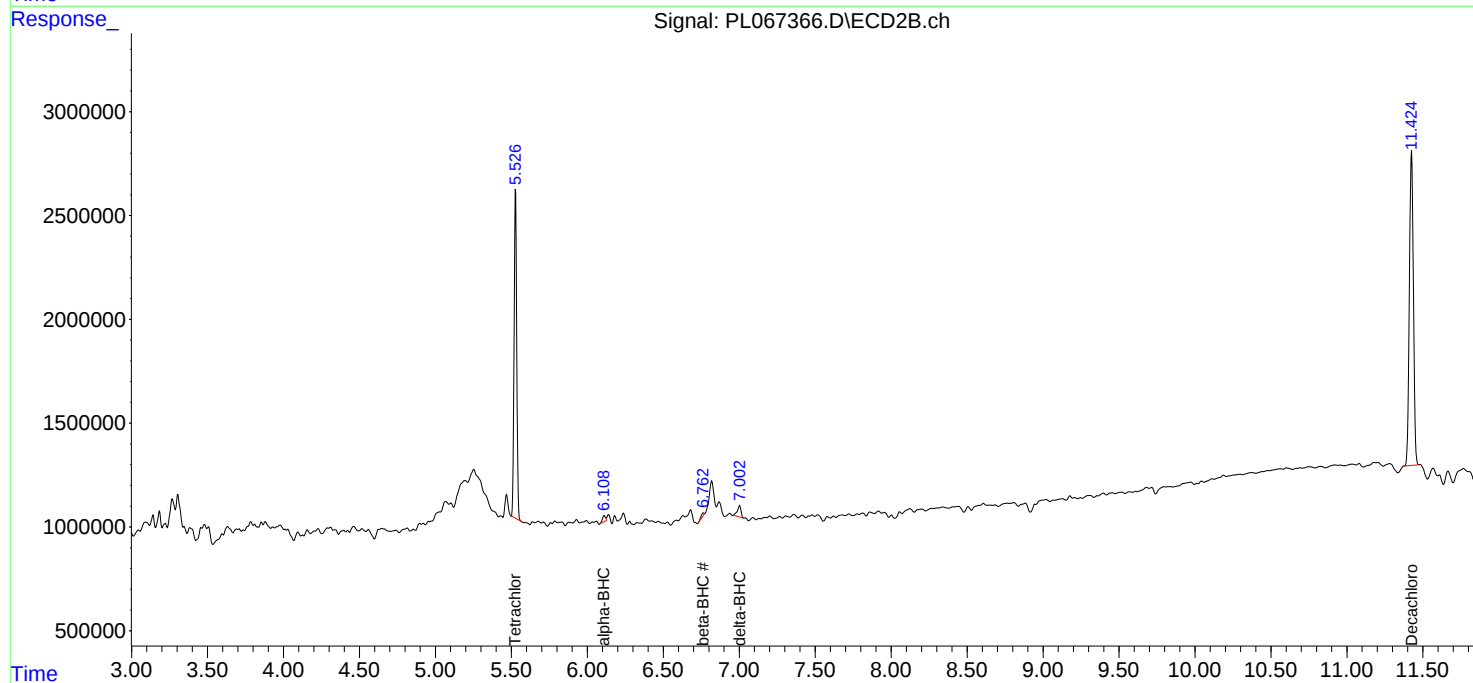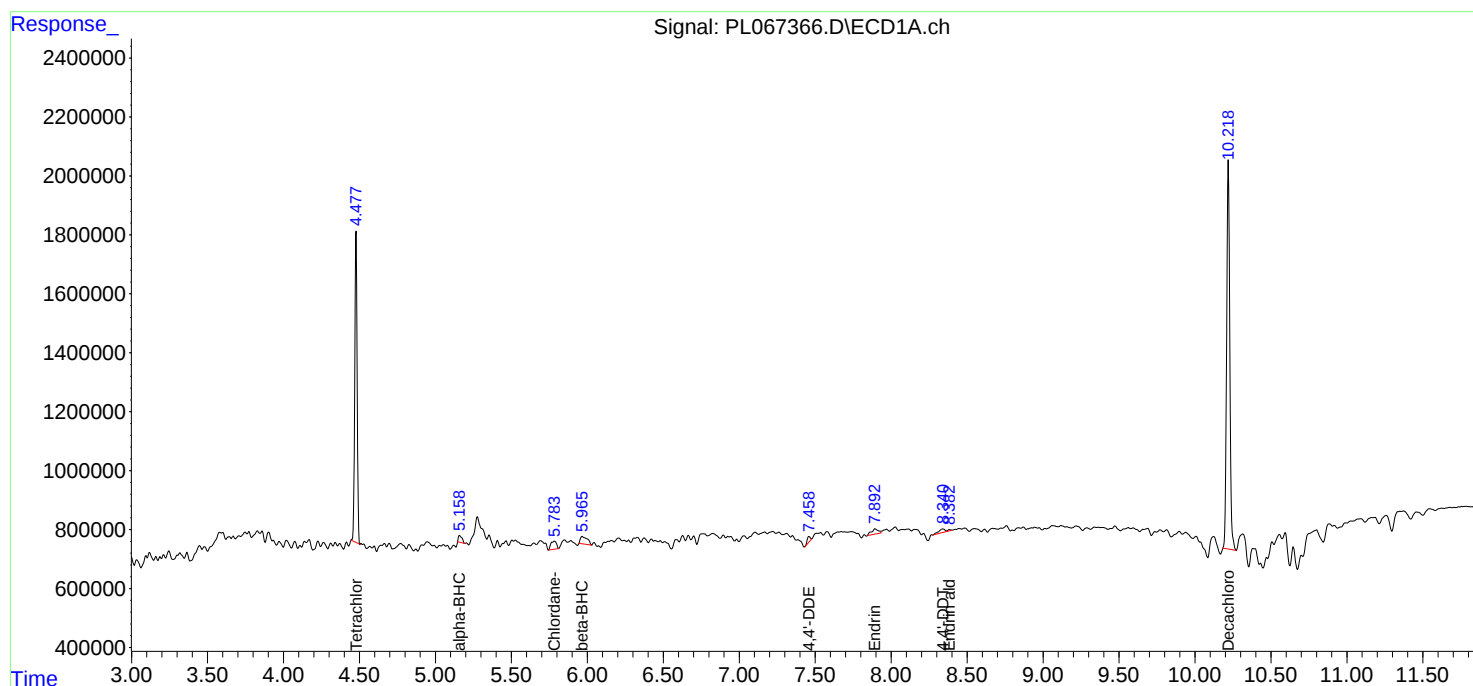


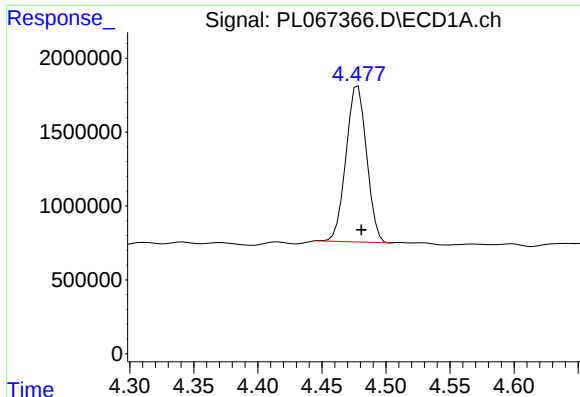

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 11824604
Conc: 21.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

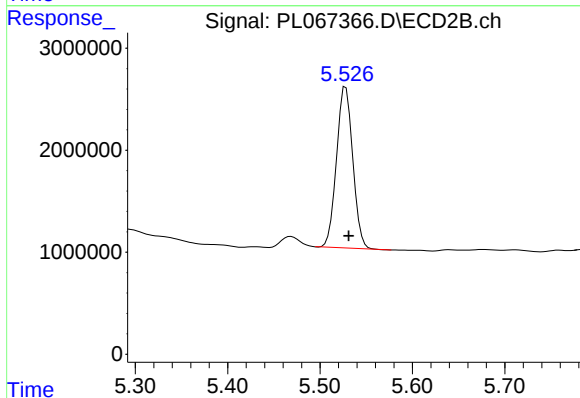


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 19284545
Conc: 20.46 ng/ml

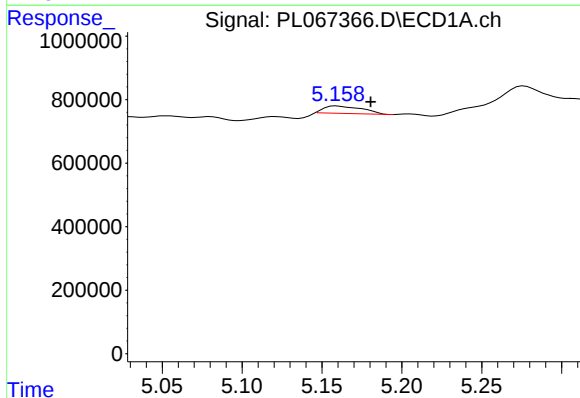


#2 alpha-BHC

R.T.: 5.159 min
Delta R.T.: -0.021 min
Response: 381772
Conc: 0.52 ng/ml

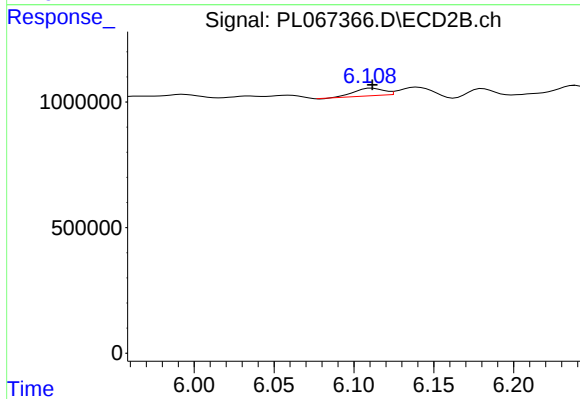

#2 alpha-BHC


R.T.: 6.111 min
Delta R.T.: 0.000 min
Response: 376727
Conc: 0.30 ng/ml

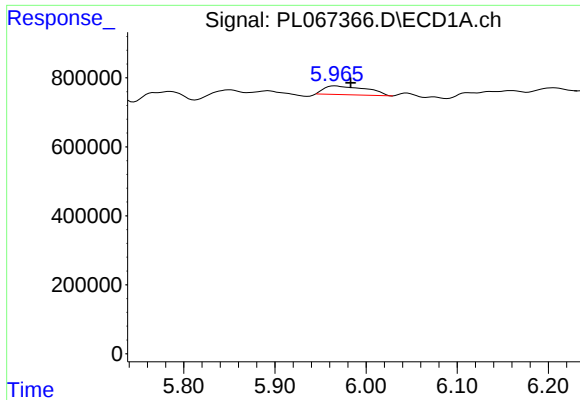

#6 beta-BHC


R.T.: 5.966 min
Delta R.T.: -0.017 min
Response: 823117
Conc: 2.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

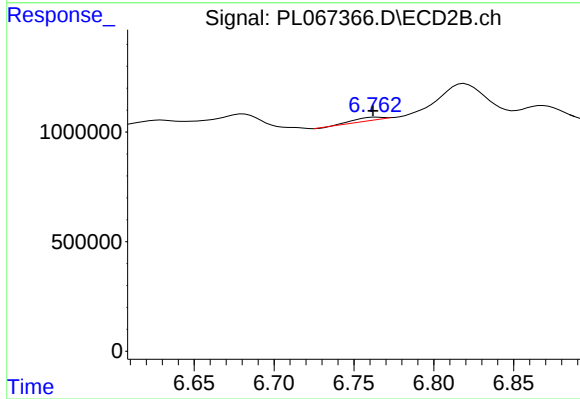


#6 beta-BHC

R.T.: 6.764 min
Delta R.T.: 0.002 min
Response: 157976
Conc: 0.29 ng/ml

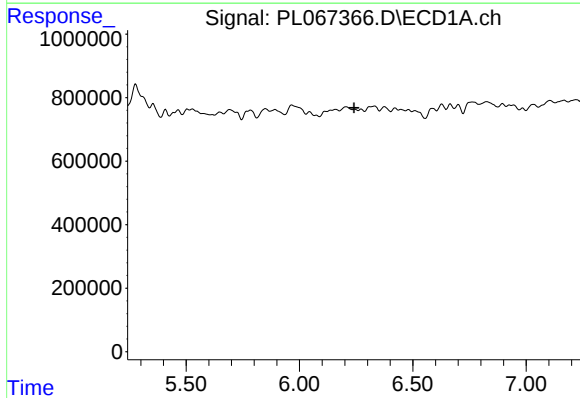


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

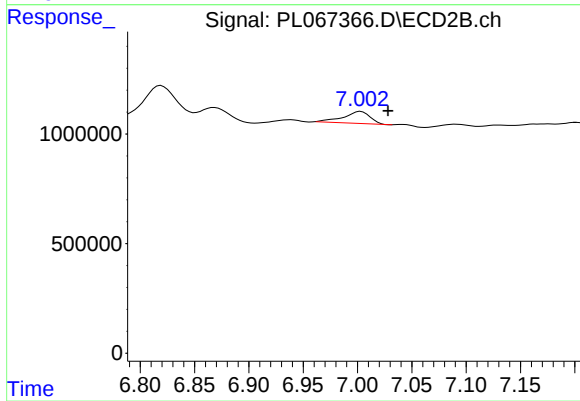

#7 delta-BHC


R.T.: 7.003 min
Delta R.T.: -0.025 min
Response: 930857
Conc: 0.79 ng/ml

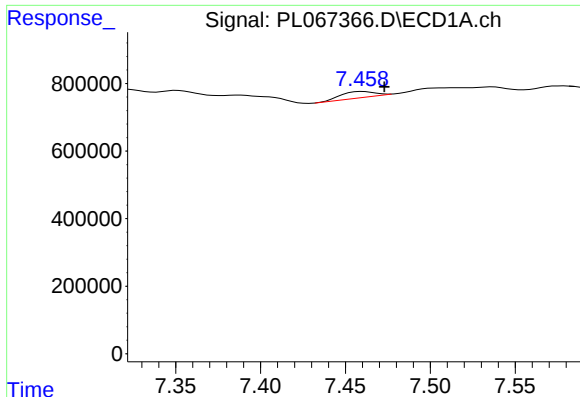

#12 4,4'-DDE


R.T.: 7.460 min
Delta R.T.: -0.013 min
Response: 253715
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

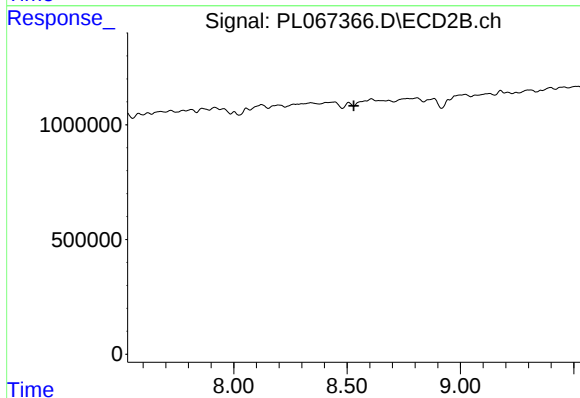


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 8.530 min
Response: 0
Conc: N.D.

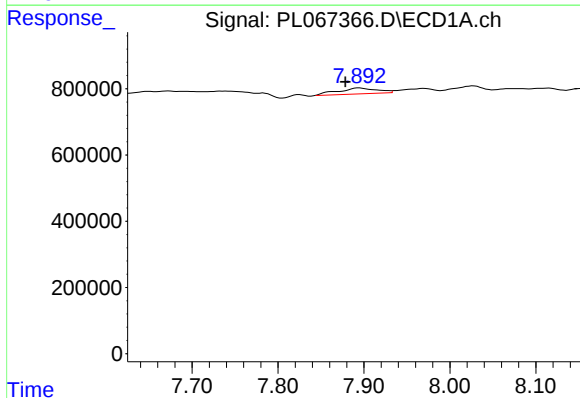


#14 Endrin

R.T.: 7.895 min
Delta R.T.: 0.016 min
Response: 555702
Conc: 0.85 ng/ml

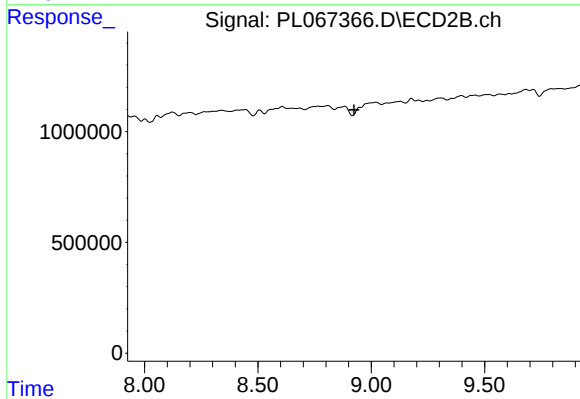

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.924 min
Response: 0
Conc: N.D.

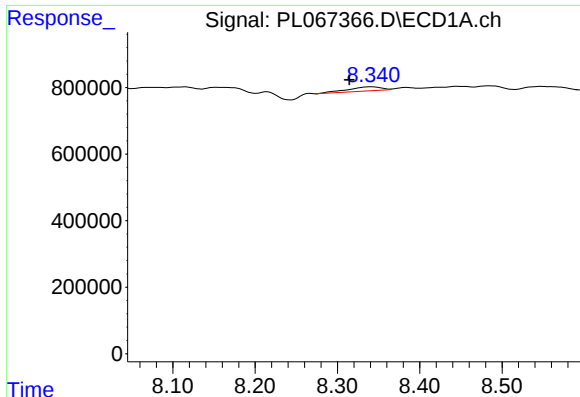

#17 4,4'-DDT


R.T.: 8.341 min
Delta R.T.: 0.027 min
Response: 347724
Conc: 0.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

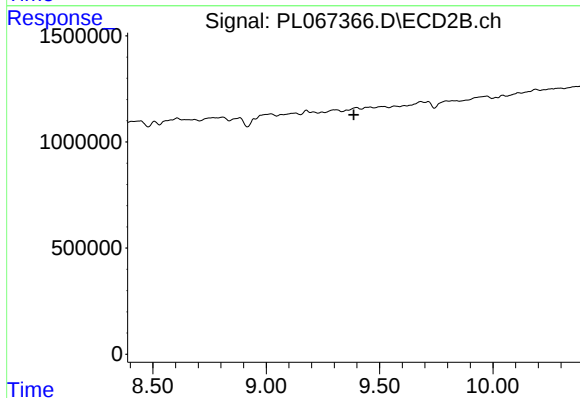


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.386 min
Response: 0
Conc: N.D.

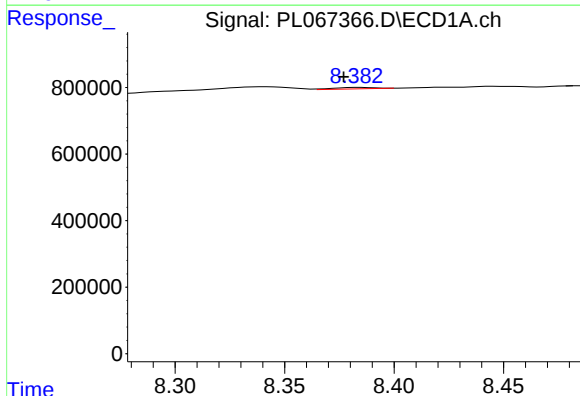


#18 Endrin aldehyde

R.T.: 8.384 min
Delta R.T.: 0.007 min
Response: 56743
Conc: 0.11 ng/ml

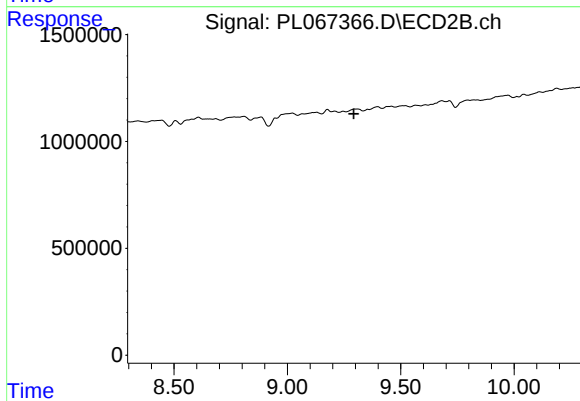

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 9.292 min
Response: 0
Conc: N.D.

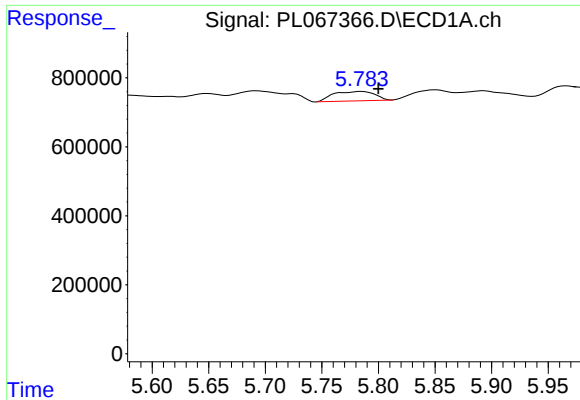

#23 Chlordane-1


R.T.: 5.785 min
Delta R.T.: -0.015 min
Response: 692151
Conc: 37.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

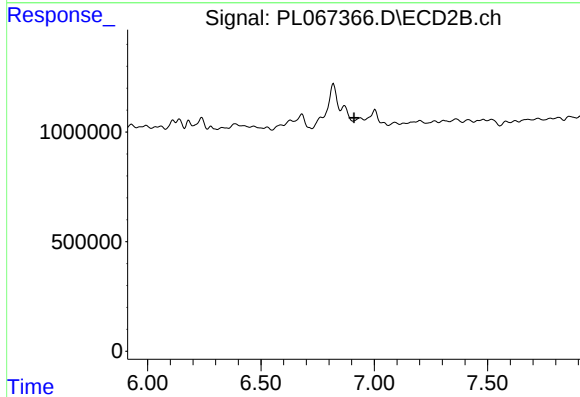


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 6.912 min
Response: 0
Conc: N.D.

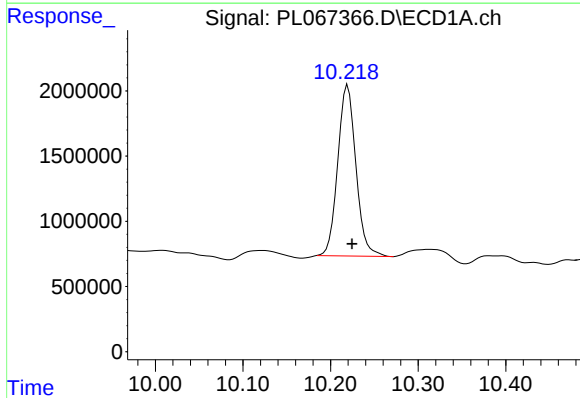

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.005 min
Response: 18896592
Conc: 26.66 ng/ml

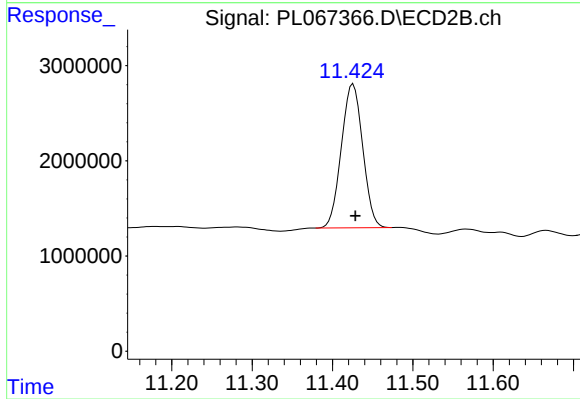

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.003 min
Response: 27910434
Conc: 28.02 ng/ml