

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
 Data File : PL067373.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2021 04:45
 Operator : AR\AJ
 Sample : M2674-05
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 09:04:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.528	3516487	5837795	6.396	6.192
28)	SA Decachlor...	10.220	11.425	5903825	7312042	8.331	7.341
Target Compounds							
2)	A alpha-BHC	5.175	6.111	350522	413939	0.477	0.335 #
6)	B beta-BHC	5.967f	6.766	876789	243037	2.450	0.448 #
7)	B delta-BHC	0.000	7.003f	0	1015256	N.D.	0.864 #
12)	B 4,4'-DDE	7.460	0.000	211738	0	0.318	N.D. #
13)	MA Dieldrin	7.582	0.000	237199	0	0.338	N.D. #
14)	MA Endrin	7.897f	0.000	615908	0	0.939	N.D. #
15)	B Endosulfa...	0.000	9.178f	0	178606	N.D.	0.224 #
17)	MA 4,4'-DDT	8.341f	0.000	127986	0	0.220	N.D. #
18)	B Endrin al...	8.390	0.000	109406	0	0.216	N.D. #
22)	Mirex	9.290f	0.000	178549	0	0.284	N.D. #
23)	Chlordane-1	5.786	0.000	328521	0	17.756	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
Data File : PL067373.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2021 04:45
Operator : AR\AJ
Sample : M2674-05
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 09:04:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

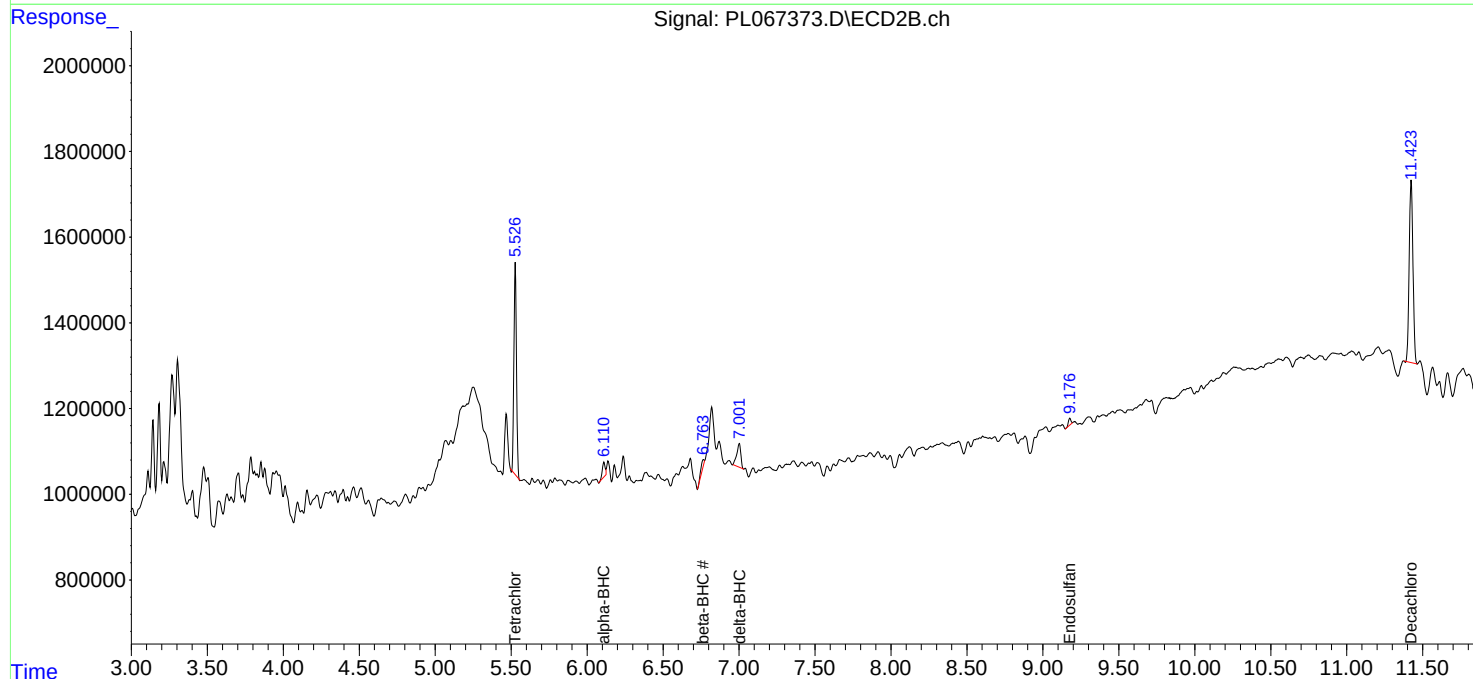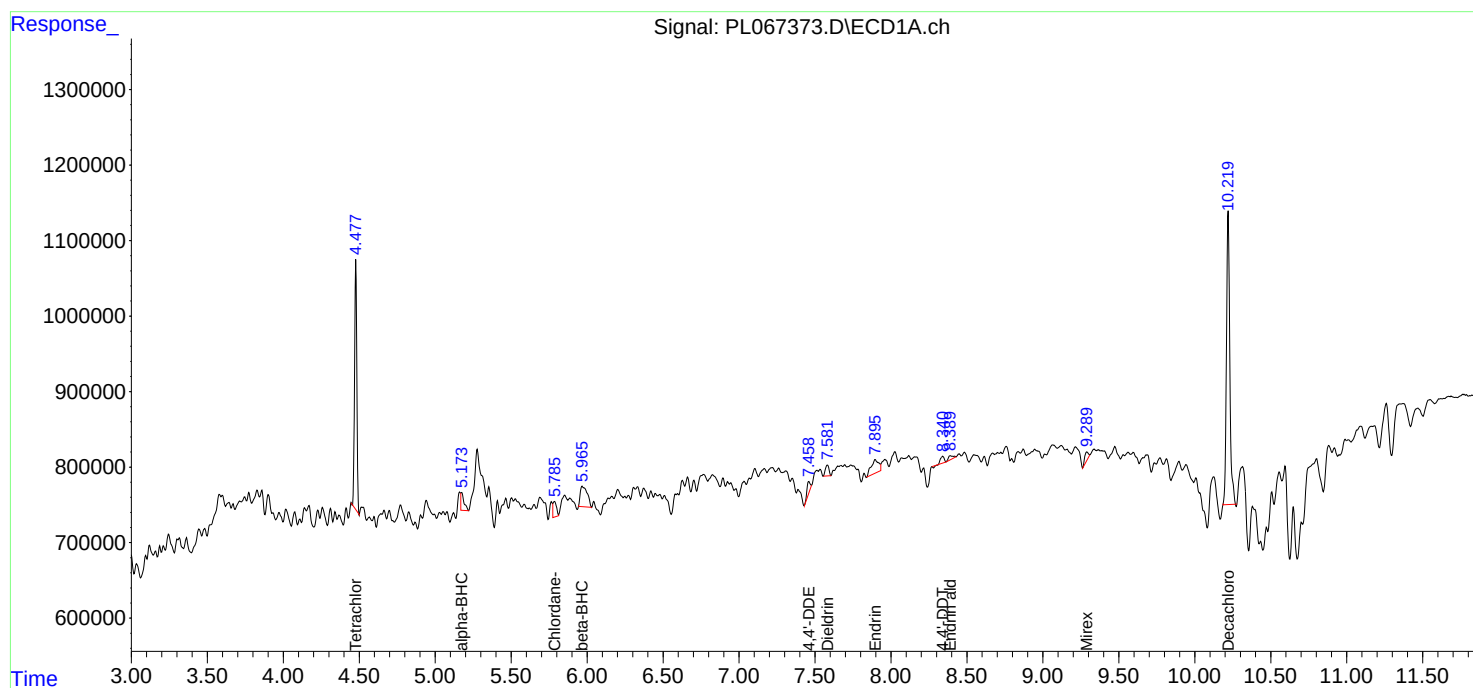


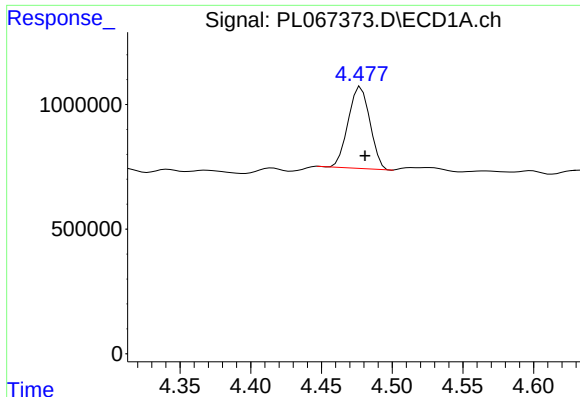

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 3516487
Conc: 6.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

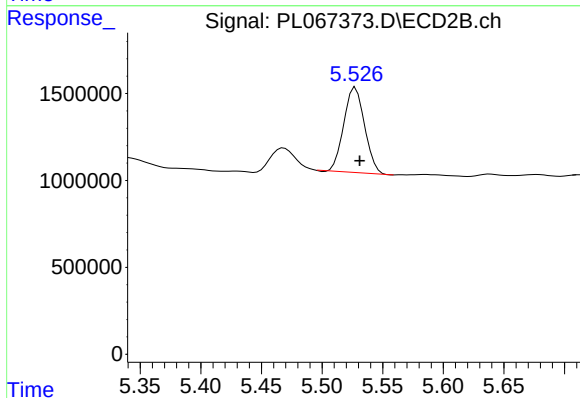


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 5837795
Conc: 6.19 ng/ml

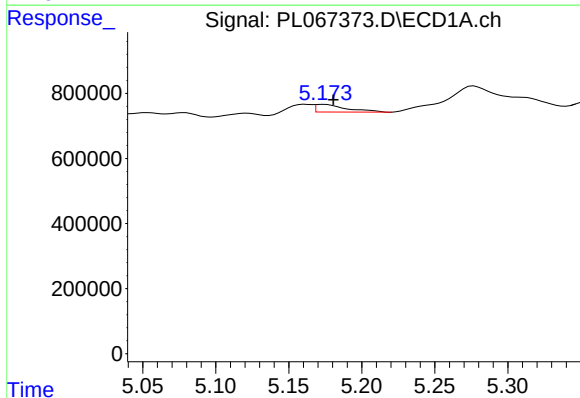


#2 alpha-BHC

R.T.: 5.175 min
Delta R.T.: -0.006 min
Response: 350522
Conc: 0.48 ng/ml

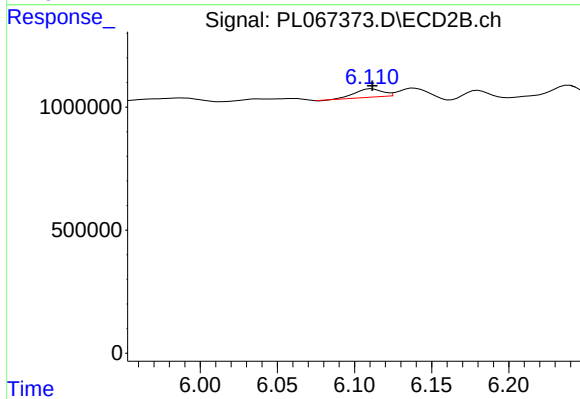

#2 alpha-BHC


R.T.: 6.111 min
Delta R.T.: 0.000 min
Response: 413939
Conc: 0.33 ng/ml

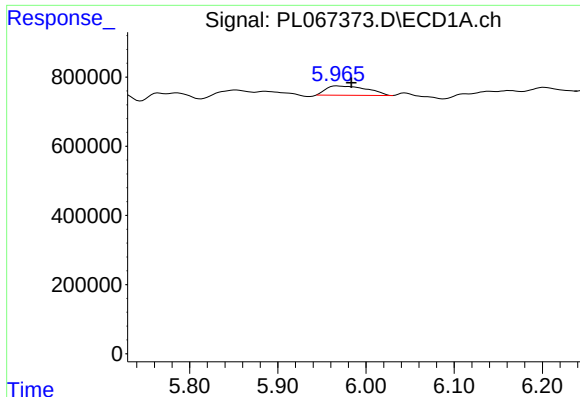

#6 beta-BHC


R.T.: 5.967 min
Delta R.T.: -0.017 min
Response: 876789
Conc: 2.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

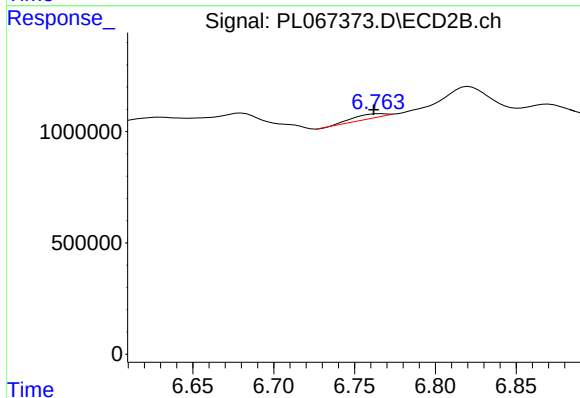


#6 beta-BHC

R.T.: 6.766 min
Delta R.T.: 0.004 min
Response: 243037
Conc: 0.45 ng/ml

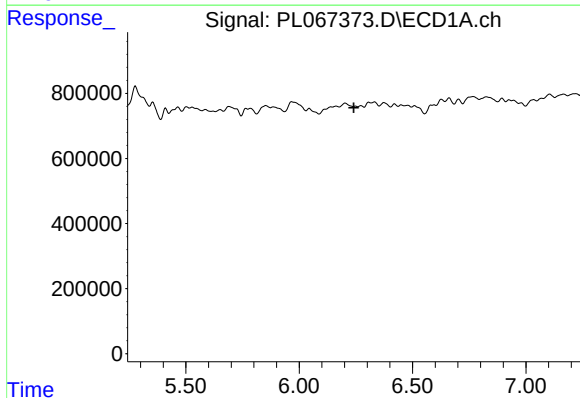


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

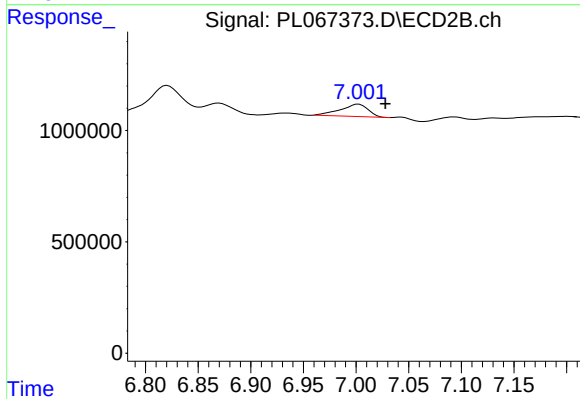

#7 delta-BHC


R.T.: 7.003 min
Delta R.T.: -0.026 min
Response: 1015256
Conc: 0.86 ng/ml

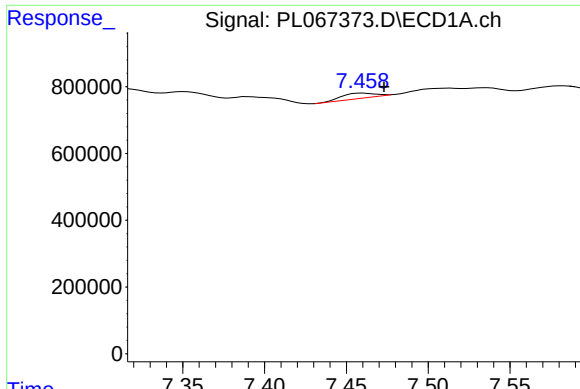

#12 4,4'-DDE


R.T.: 7.460 min
Delta R.T.: -0.013 min
Response: 211738
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

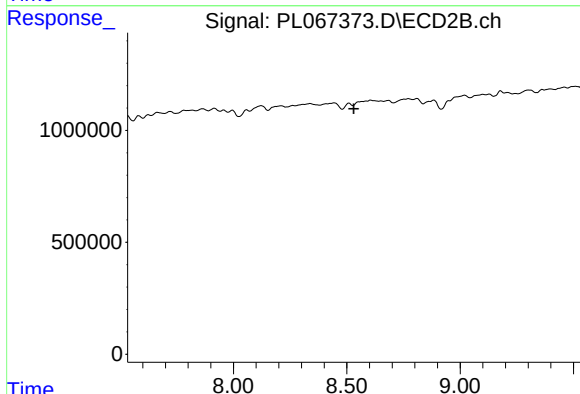


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 8.530 min
Response: 0
Conc: N.D.

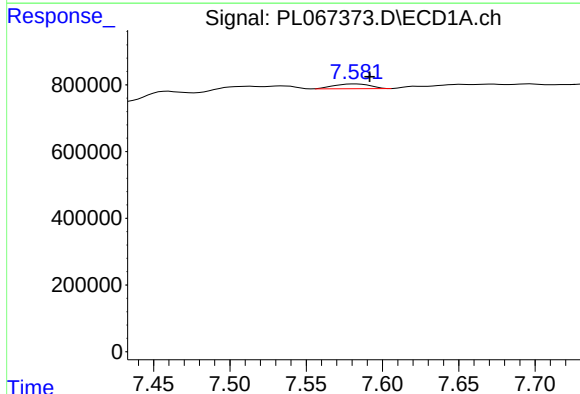


#13 Dieldrin

R.T.: 7.582 min
Delta R.T.: -0.009 min
Response: 237199
Conc: 0.34 ng/ml

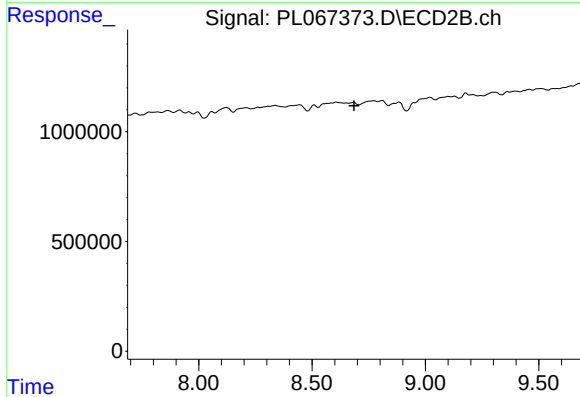

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 8.685 min
Response: 0
Conc: N.D.

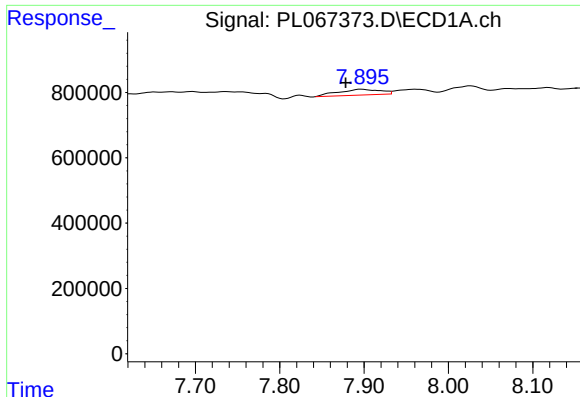

#14 Endrin


R.T.: 7.897 min
Delta R.T.: 0.018 min
Response: 615908
Conc: 0.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

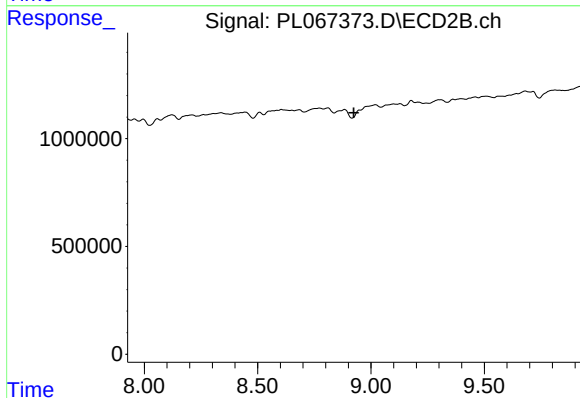


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.924 min
Response: 0
Conc: N.D.

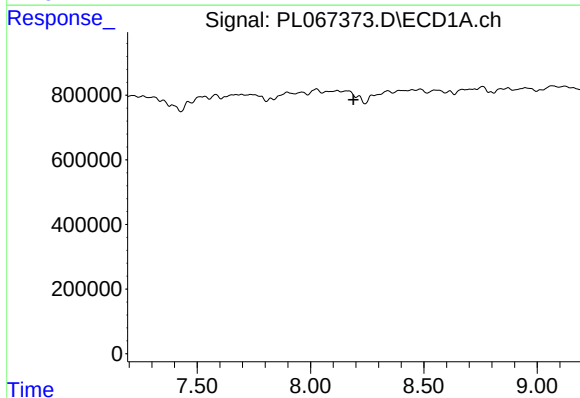


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.190 min
Response: 0
Conc: N.D.

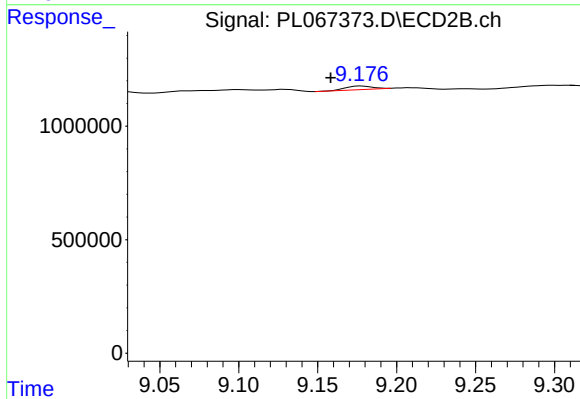

#15 Endosulfan II


R.T.: 9.178 min
Delta R.T.: 0.020 min
Response: 178606
Conc: 0.22 ng/ml

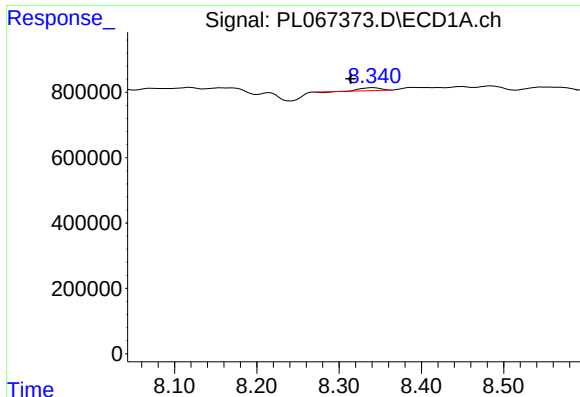

#17 4,4'-DDT


R.T.: 8.341 min
Delta R.T.: 0.027 min
Response: 127986
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

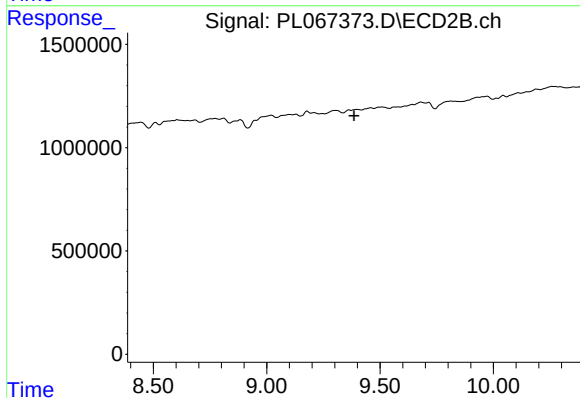


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.386 min
Response: 0
Conc: N.D.

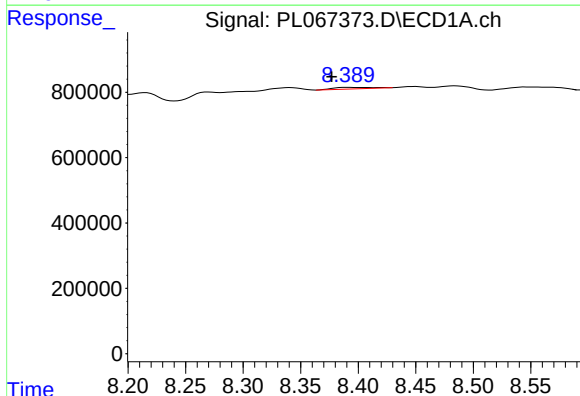


#18 Endrin aldehyde

R.T.: 8.390 min
Delta R.T.: 0.013 min
Response: 109406
Conc: 0.22 ng/ml

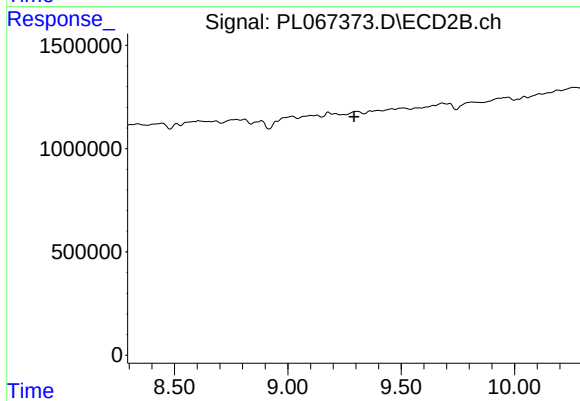

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 9.292 min
Response: 0
Conc: N.D.

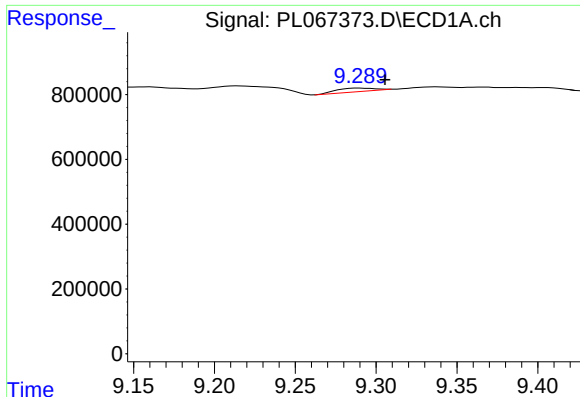

#22 Mirex


R.T.: 9.290 min
Delta R.T.: -0.016 min
Response: 178549
Conc: 0.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

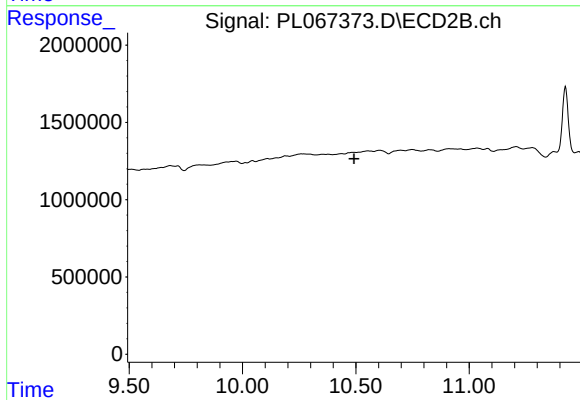


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 10.492 min
Response: 0
Conc: N.D.

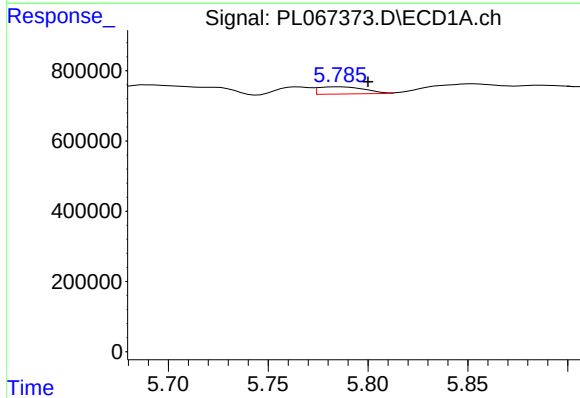


#23 Chlordane-1

R.T.: 5.786 min
Delta R.T.: -0.014 min
Response: 328521
Conc: 17.76 ng/ml

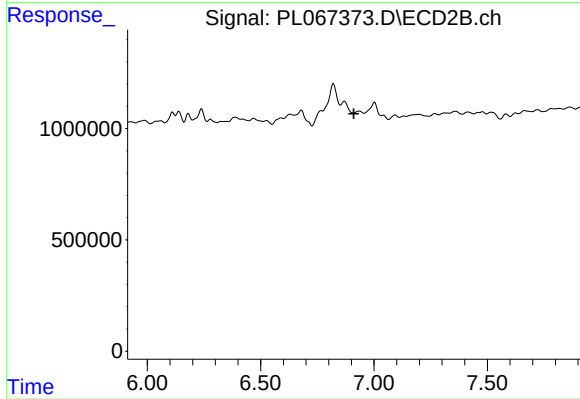

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 6.912 min
Response: 0
Conc: N.D.

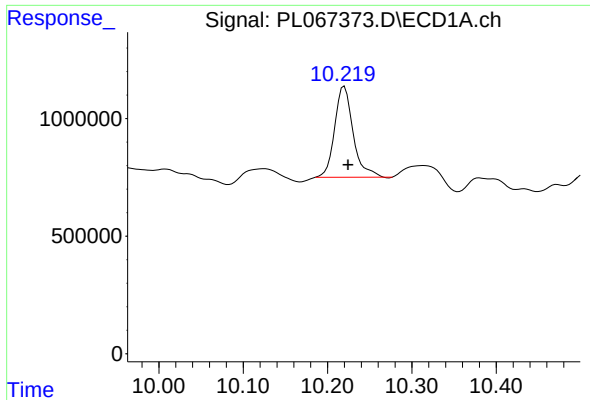

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.004 min
Response: 5903825
Conc: 8.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

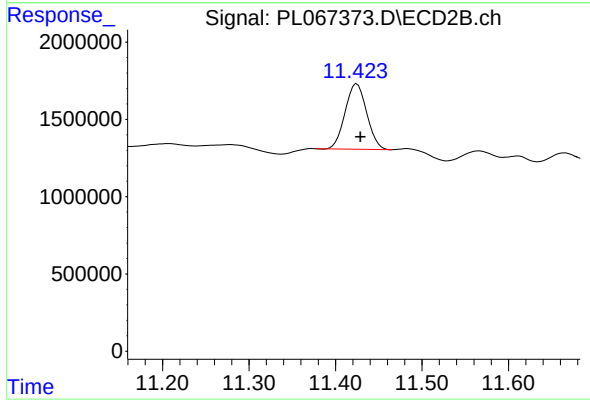

#28 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: -0.004 min
Response: 7312042
Conc: 7.34 ng/ml