

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
 Data File : PL067374.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2021 05:02
 Operator : AR\AJ
 Sample : M2674-06
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 09:04:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.528	4808230	7488768	8.746	7.944
28)	SA Decachlor...	10.220	11.426	8317693	10860016	11.737	10.903
Target Compounds							
2)	A alpha-BHC	5.159f	0.000	311148	0	0.423	N.D. #
6)	B beta-BHC	5.964f	0.000	693179	0	1.937	N.D. #
7)	B delta-BHC	0.000	7.004f	0	1324665	N.D.	1.127 #
12)	B 4,4'-DDE	7.459	0.000	289109	0	0.435	N.D. #
14)	MA Endrin	7.896f	0.000	511192	0	0.780	N.D. #
15)	B Endosulfa...	0.000	9.179f	0	292946	N.D.	0.367 #
21)	B Endrin ke...	0.000	10.046f	0	243865	N.D.	0.269 #
23)	Chlordane-1	5.789	0.000	697021	0	37.673	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
Data File : PL067374.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2021 05:02
Operator : AR\AJ
Sample : M2674-06
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 09:04:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

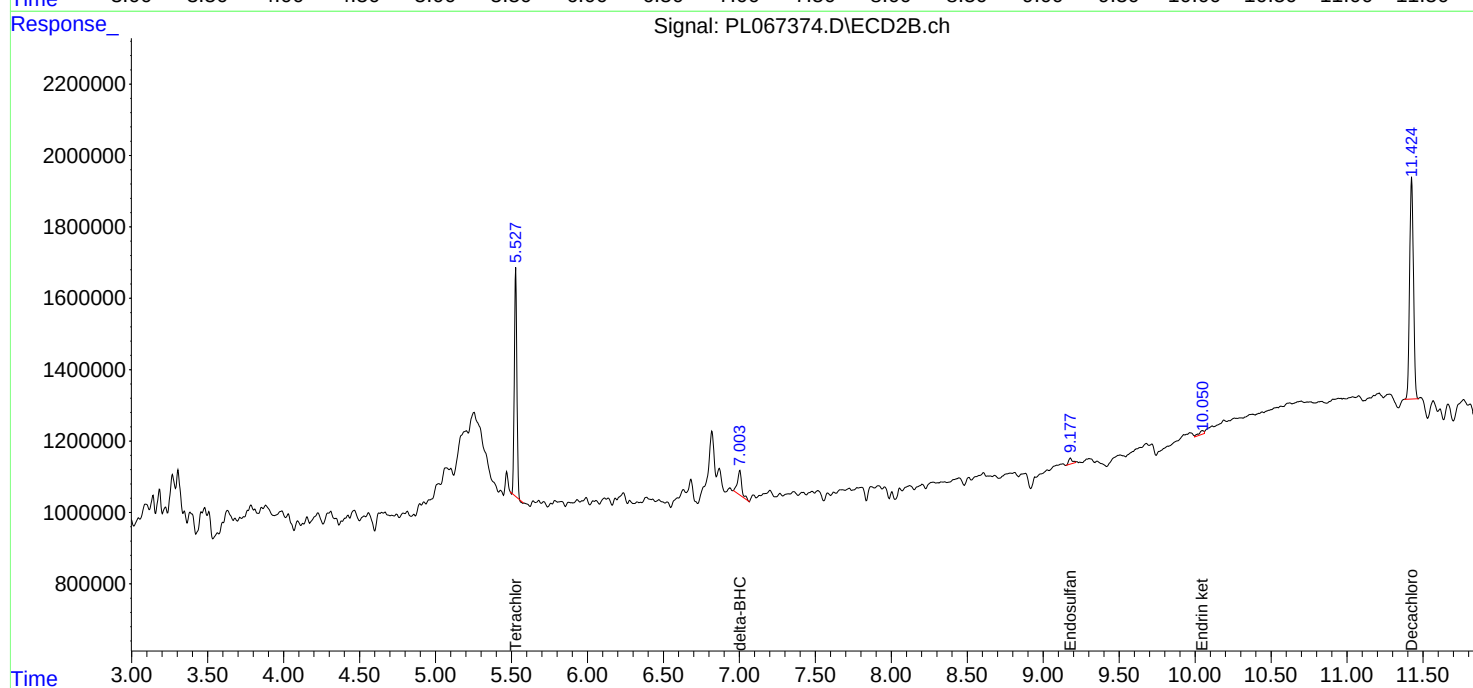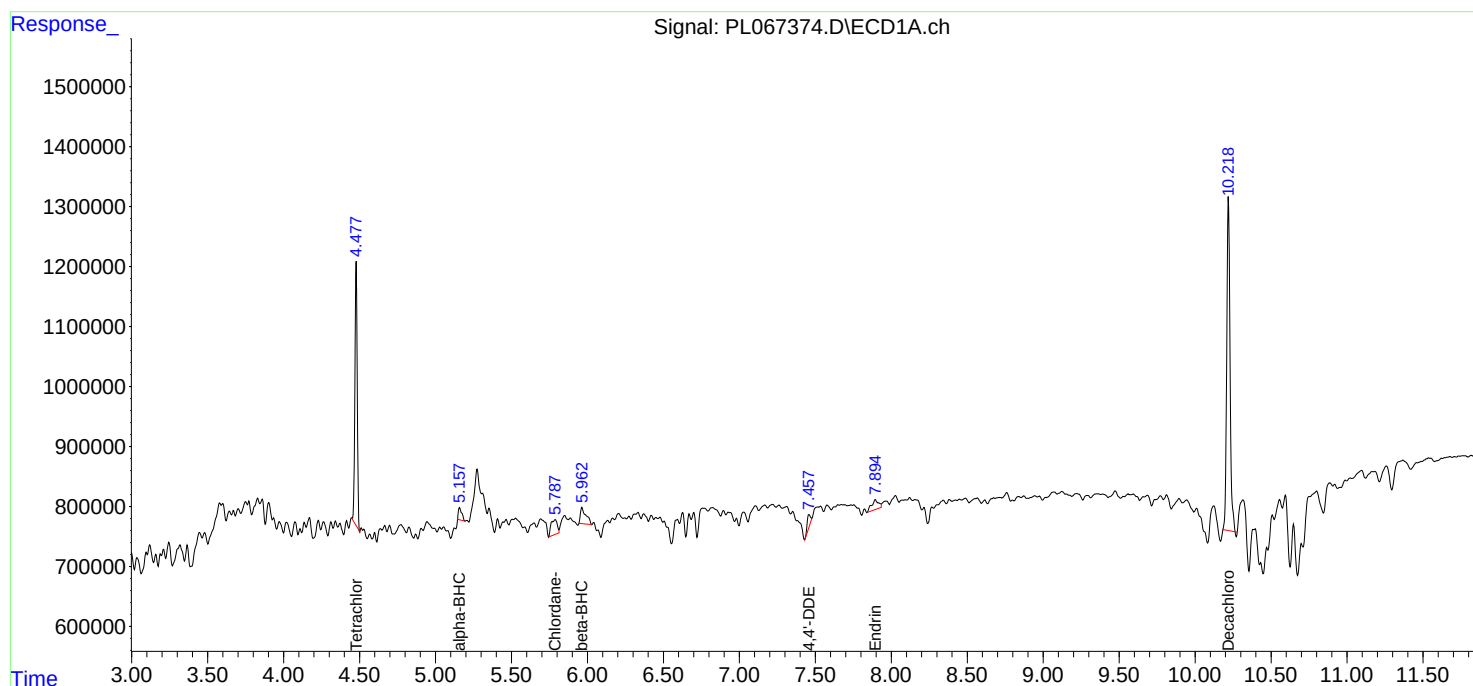


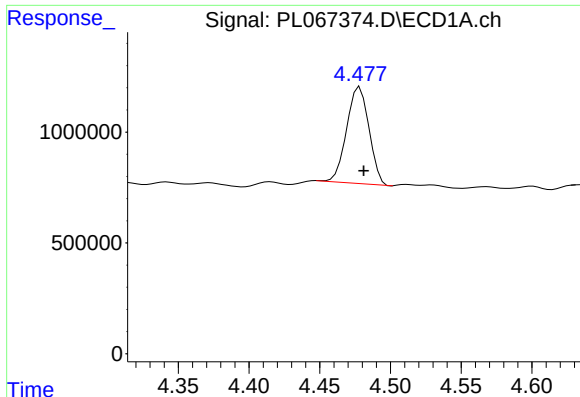

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 4808230
Conc: 8.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

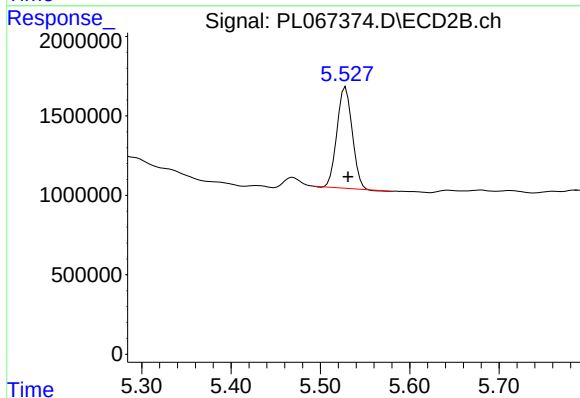


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 7488768
Conc: 7.94 ng/ml

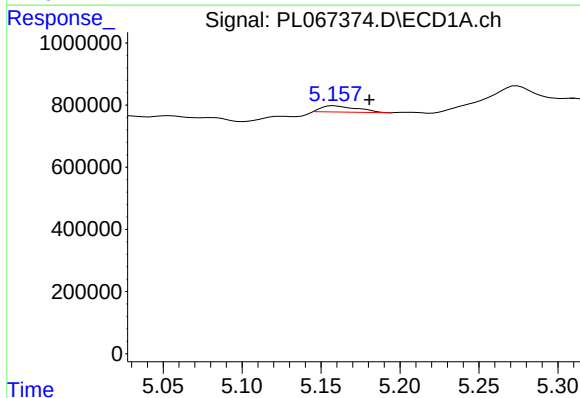


#2 alpha-BHC

R.T.: 5.159 min
Delta R.T.: -0.022 min
Response: 311148
Conc: 0.42 ng/ml

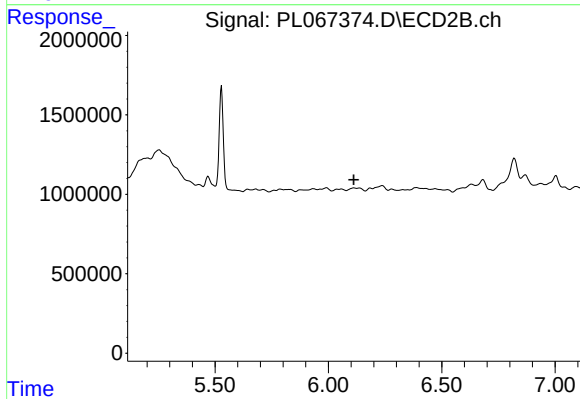

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 6.112 min
Response: 0
Conc: N.D.

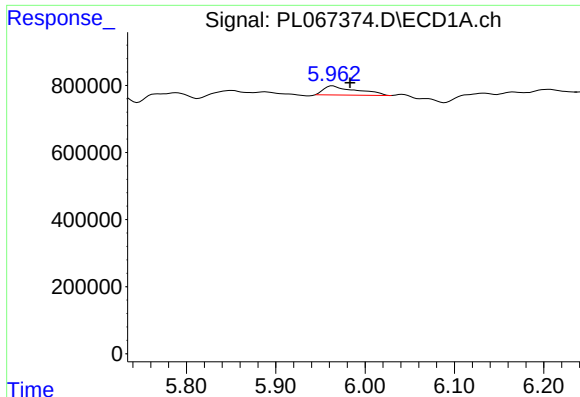

#6 beta-BHC


R.T.: 5.964 min
Delta R.T.: -0.020 min
Response: 693179
Conc: 1.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

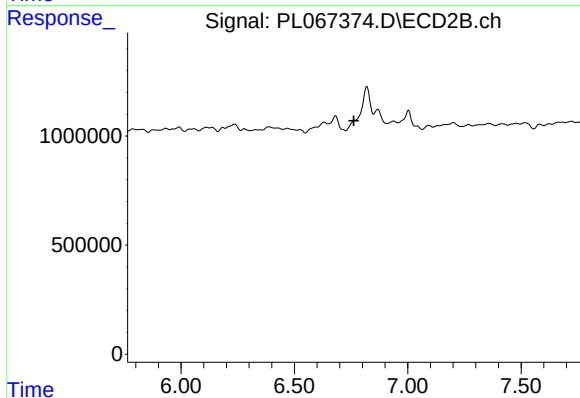


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

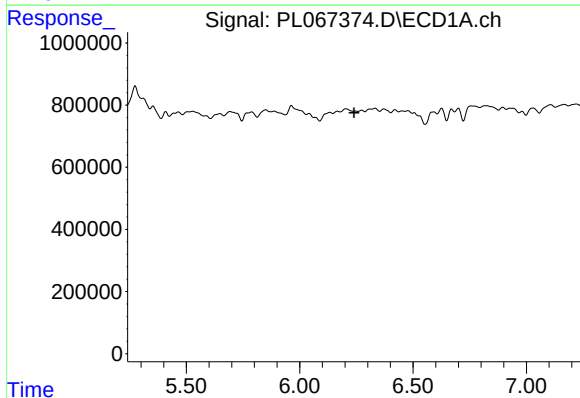


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

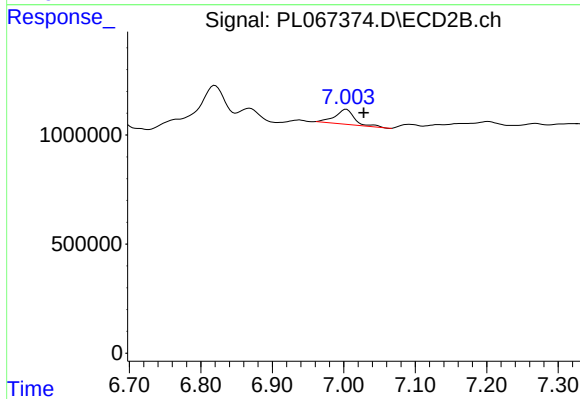

#7 delta-BHC


R.T.: 7.004 min
Delta R.T.: -0.024 min
Response: 1324665
Conc: 1.13 ng/ml

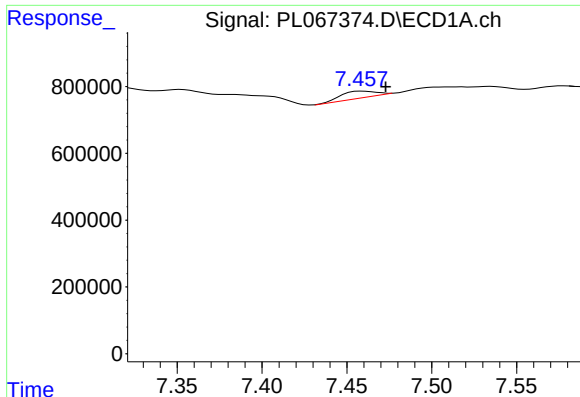

#12 4,4'-DDE


R.T.: 7.459 min
Delta R.T.: -0.014 min
Response: 289109
Conc: 0.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

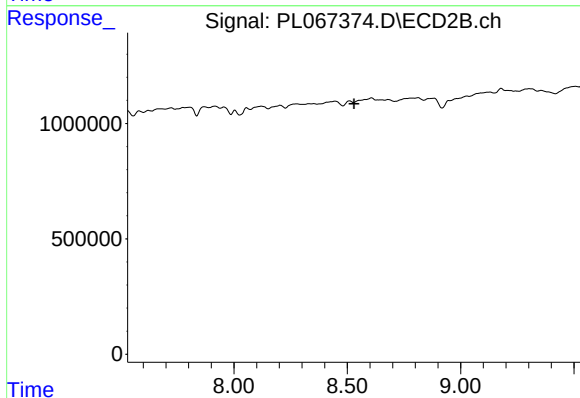


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 8.530 min
Response: 0
Conc: N.D.

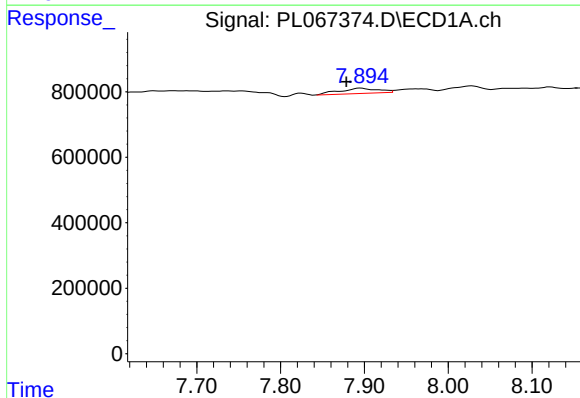


#14 Endrin

R.T.: 7.896 min
Delta R.T.: 0.017 min
Response: 511192
Conc: 0.78 ng/ml

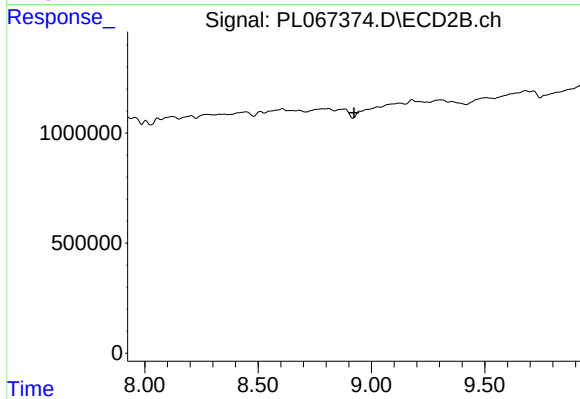

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.924 min
Response: 0
Conc: N.D.

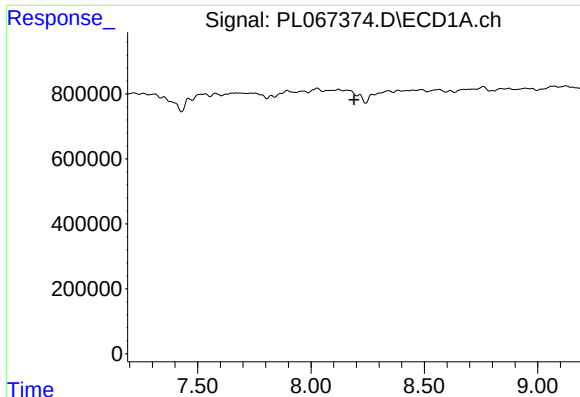

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

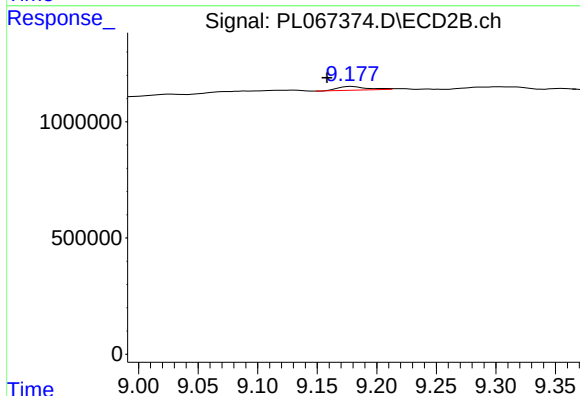


#15 Endosulfan II

R.T.: 9.179 min
Delta R.T.: 0.021 min
Response: 292946
Conc: 0.37 ng/ml

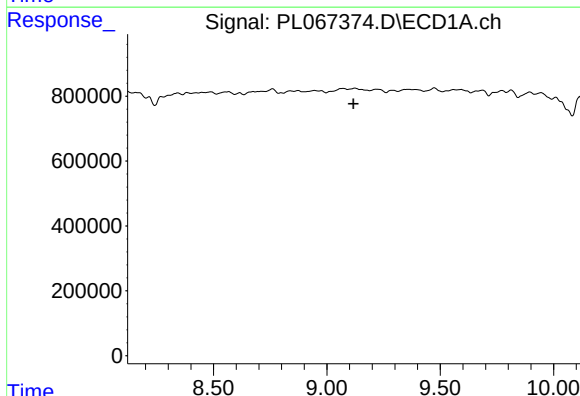


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.118 min
Response: 0
Conc: N.D.

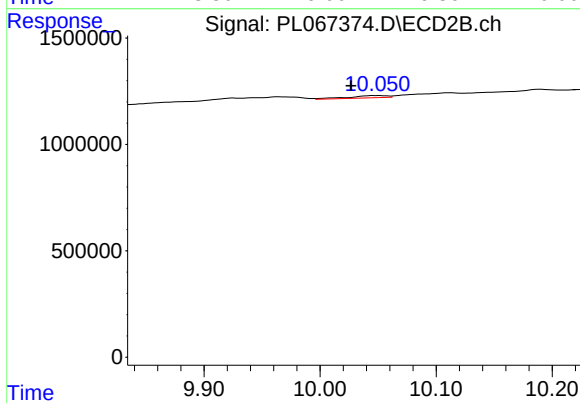

#21 Endrin ketone


R.T.: 10.046 min
Delta R.T.: 0.020 min
Response: 243865
Conc: 0.27 ng/ml

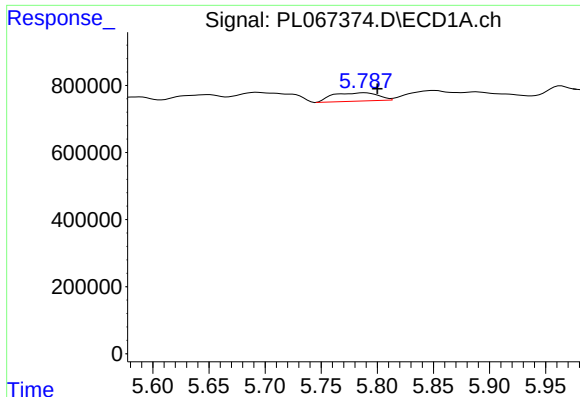

#23 Chlordane-1


R.T.: 5.789 min
Delta R.T.: -0.011 min
Response: 697021
Conc: 37.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

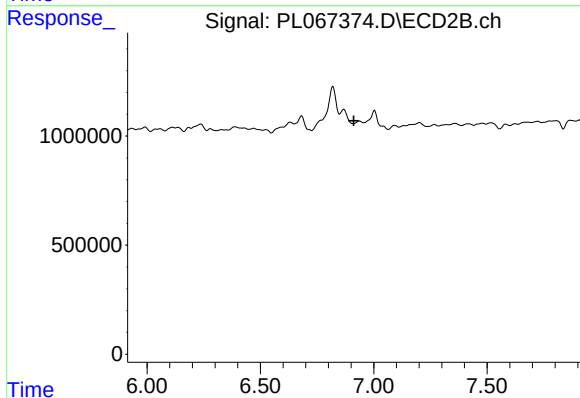


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 6.912 min
Response: 0
Conc: N.D.

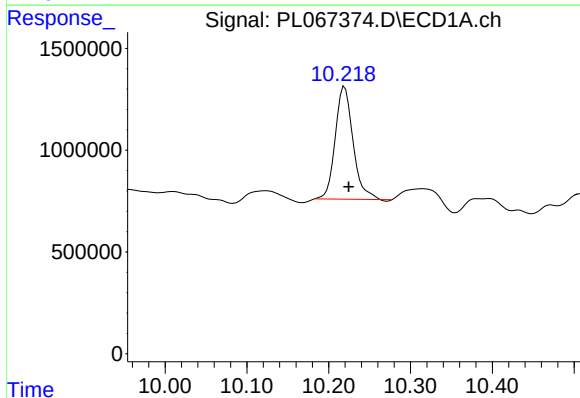

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.005 min
Response: 8317693
Conc: 11.74 ng/ml

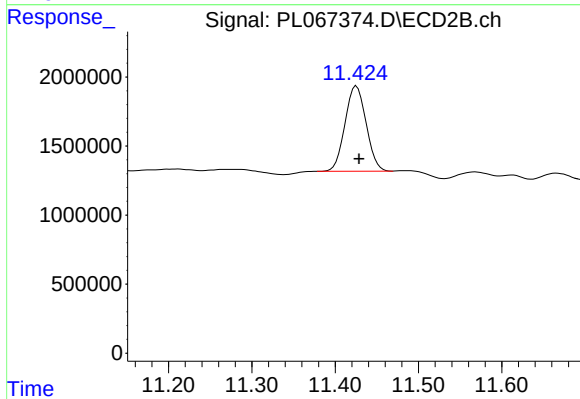

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.003 min
Response: 10860016
Conc: 10.90 ng/ml