

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
 Data File : PL067368.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2021 03:22
 Operator : AR\AJ
 Sample : M2678-02
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 0205-COMP-F(DISCRETE-CL-05)

Manual Integrations
 APPROVED

Ankita
 6/14/2021 1:09:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 09:03:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.528	10806020	18460659	19.655	19.582
28)	SA Decachlor...	10.220	11.425	11226785	16899282	15.842	16.966
Target Compounds							
12)	B 4,4'-DDE	7.468	8.525	3395774	4478303	5.104	4.943
16)	A 4,4'-DDD	8.048	9.064	937187	1362367	1.612	1.916m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
Data File : PL067368.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2021 03:22
Operator : AR\AJ
Sample : M2678-02
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
0205-COMP-F(DISCRETE-CL-05)


Manual Integrations
APPROVED

Ankita
6/14/2021 1:09:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 09:03:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

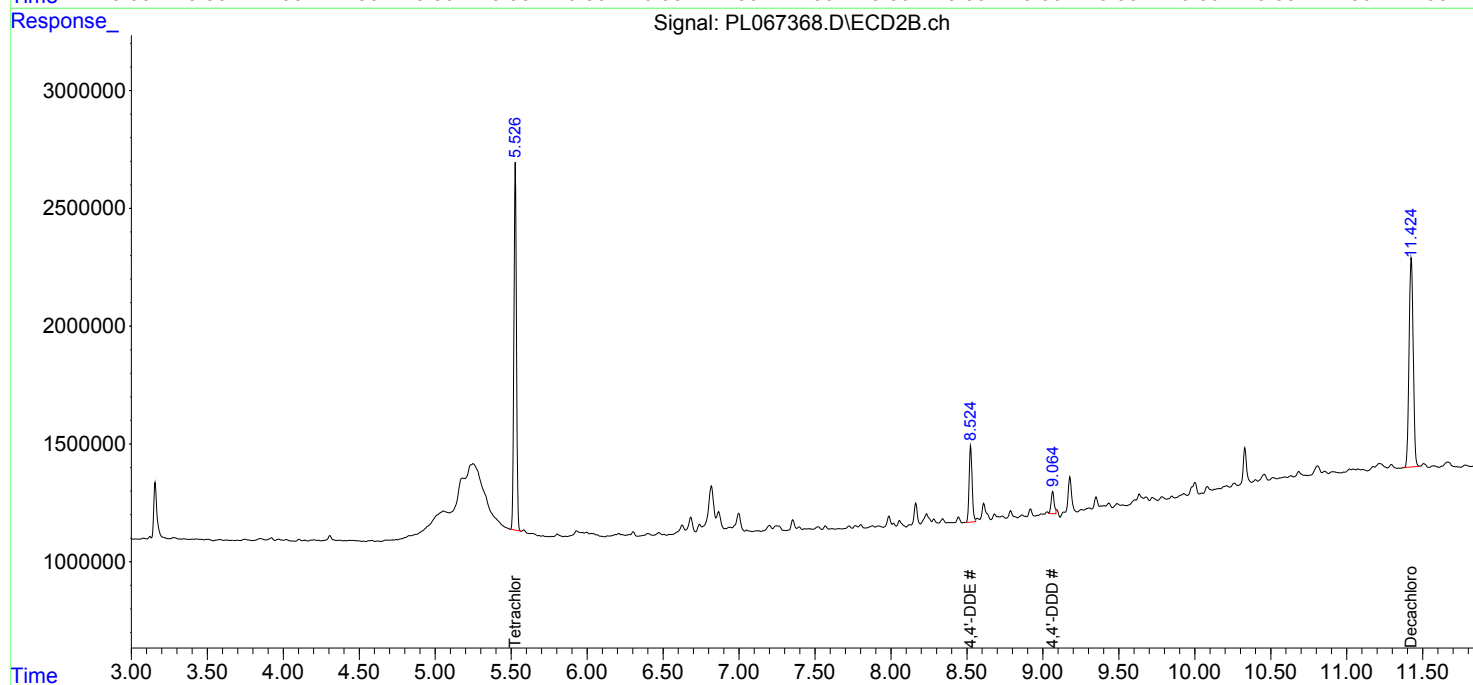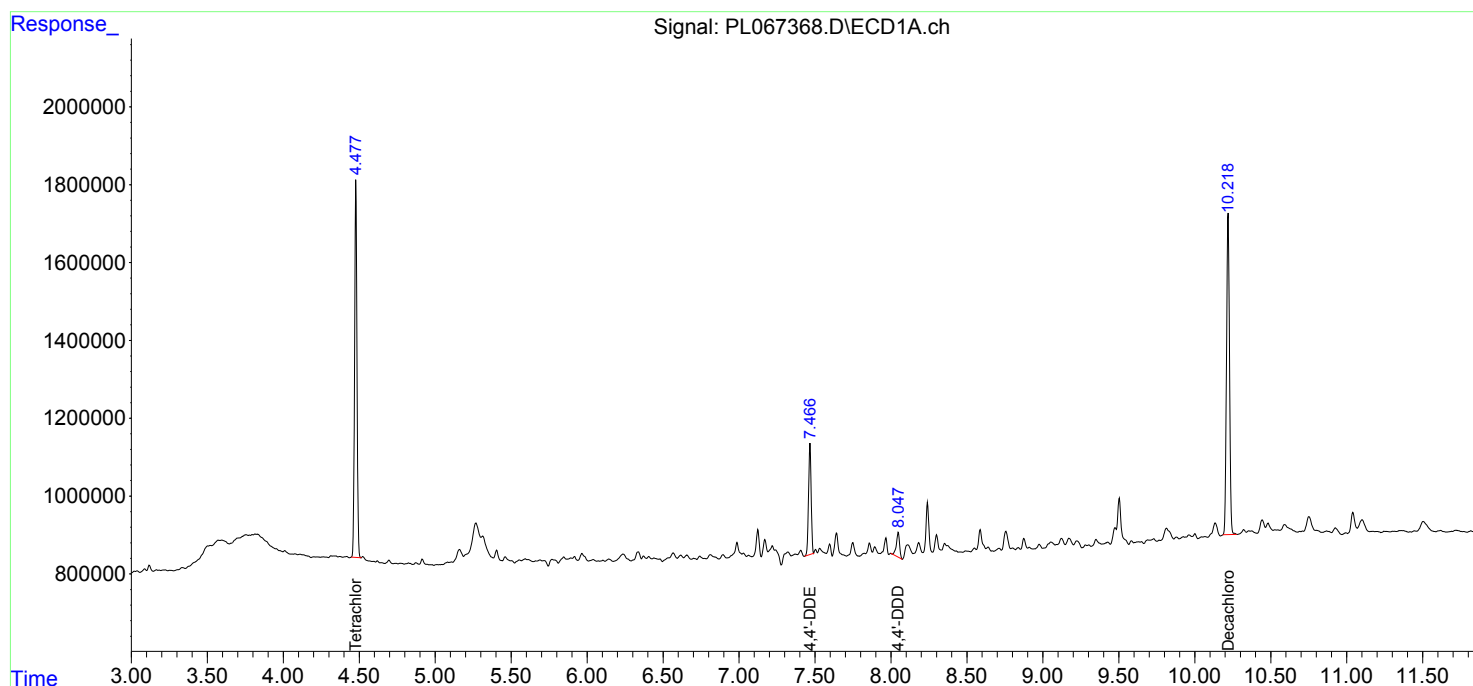

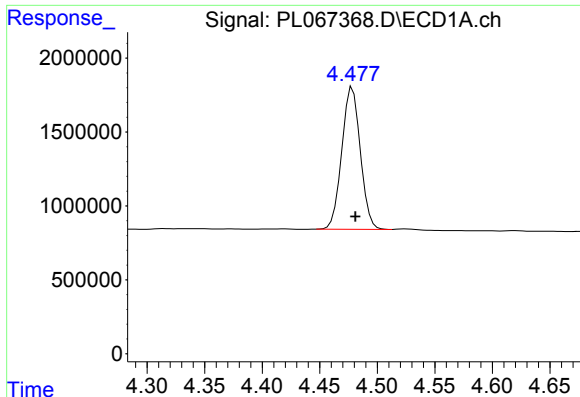


#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 10806020
Conc: 19.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
0205-COMP-F(DISCRETE-CL-05)


Manual Integrations
APPROVED

Ankita
6/14/2021 1:09:47 PM

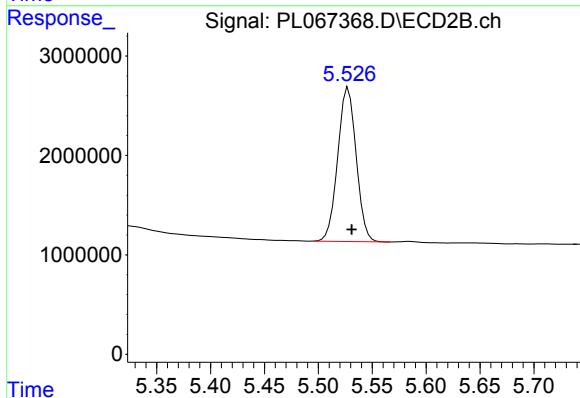


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 18460659
Conc: 19.58 ng/ml

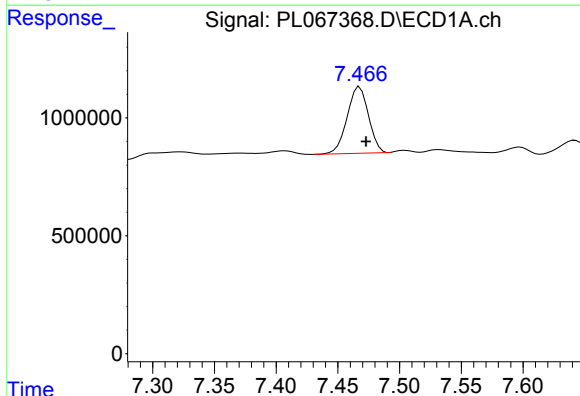


#12 4,4'-DDE

R.T.: 7.468 min
Delta R.T.: -0.005 min
Response: 3395774
Conc: 5.10 ng/ml

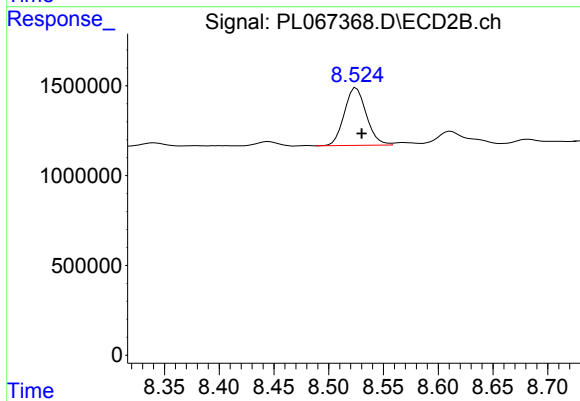

#12 4,4'-DDE

R.T.: 8.525 min
Delta R.T.: -0.005 min
Response: 4478303
Conc: 4.94 ng/ml

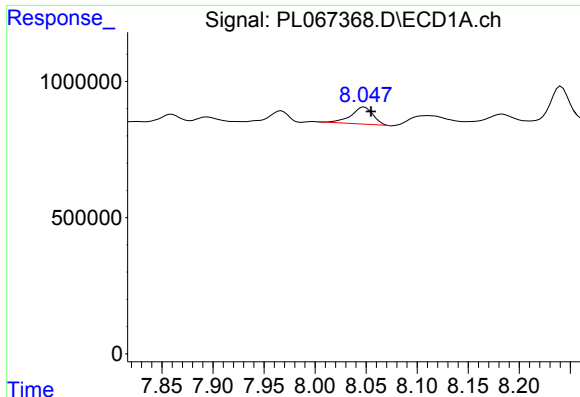


#16 4,4'-DDD

R.T.: 8.048 min
Delta R.T.: -0.006 min
Response: 937187
Conc: 1.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
0205-COMP-F(DISCRETE-CL-05)


Manual Integrations
APPROVED

Ankita
6/14/2021 1:09:47 PM

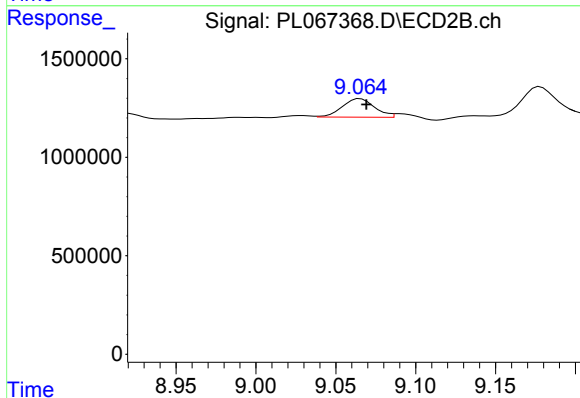


#16 4,4'-DDD

R.T.: 9.064 min
Delta R.T.: -0.005 min
Response: 1362367
Conc: 1.92 ng/ml m

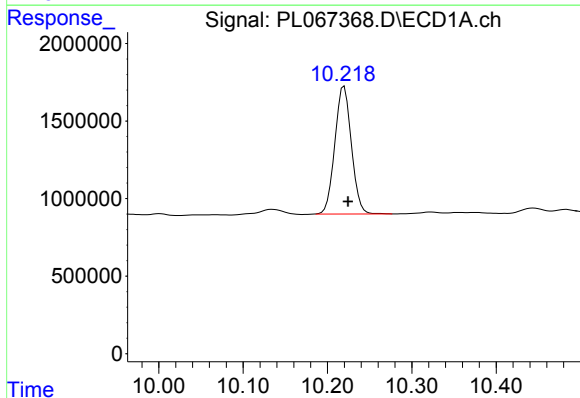

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.005 min
Response: 11226785
Conc: 15.84 ng/ml

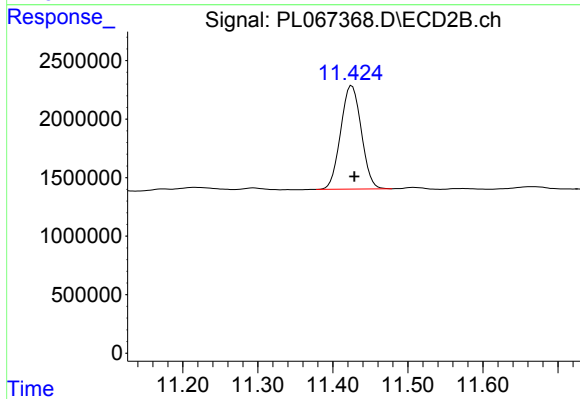

#28 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: -0.003 min
Response: 16899282
Conc: 16.97 ng/ml