

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
 Data File : PL067378.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2021 06:08
 Operator : AR\AJ
 Sample : M2678-07
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 0241-AMND-COMP-F(CL-05)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 09:05:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.528	3852263	6222089	7.007	6.600
28)	SA Decachlor...	10.220	11.424	7990439	11782119	11.275	11.829
Target Compounds							
12)	B 4,4'-DDE	7.467	8.526	3529325	5200584	5.305	5.741



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
Data File : PL067378.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2021 06:08
Operator : AR\AJ
Sample : M2678-07
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
0241-AMND-COMP-F(CL-05)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 09:05:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

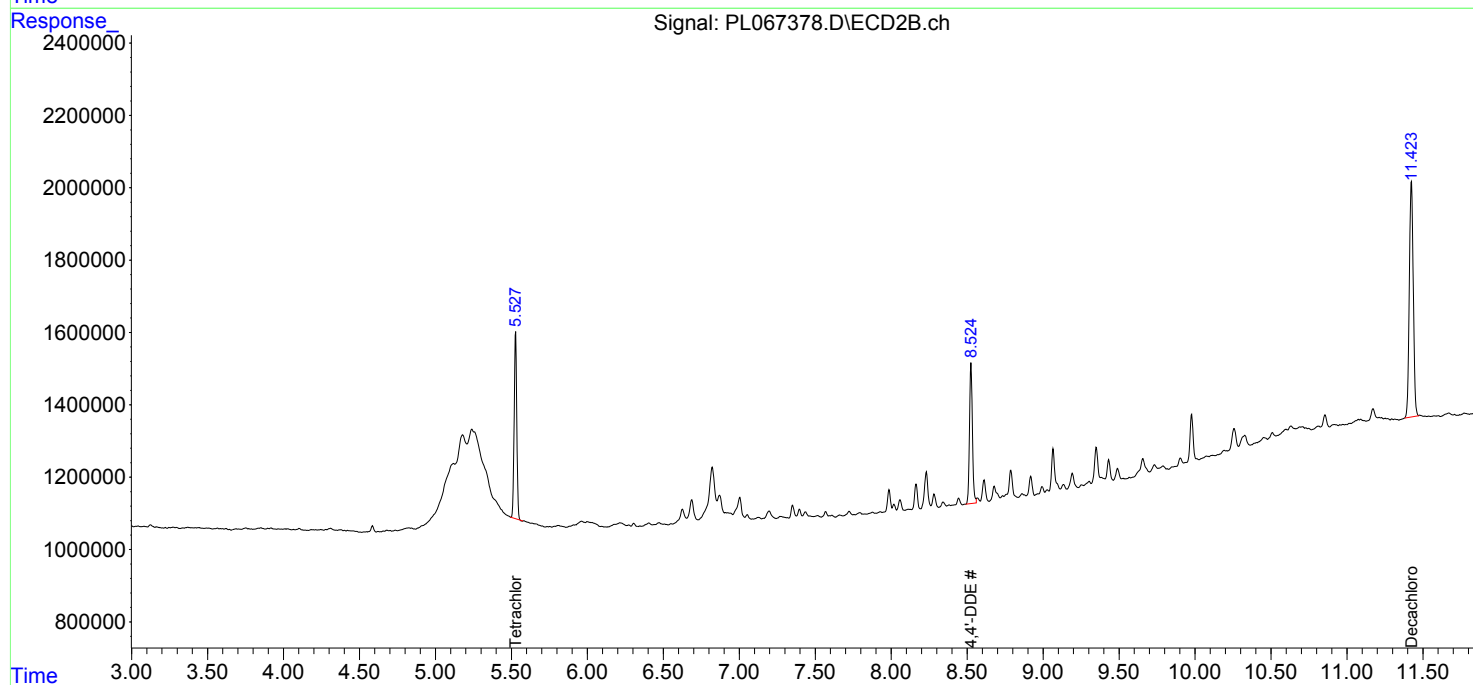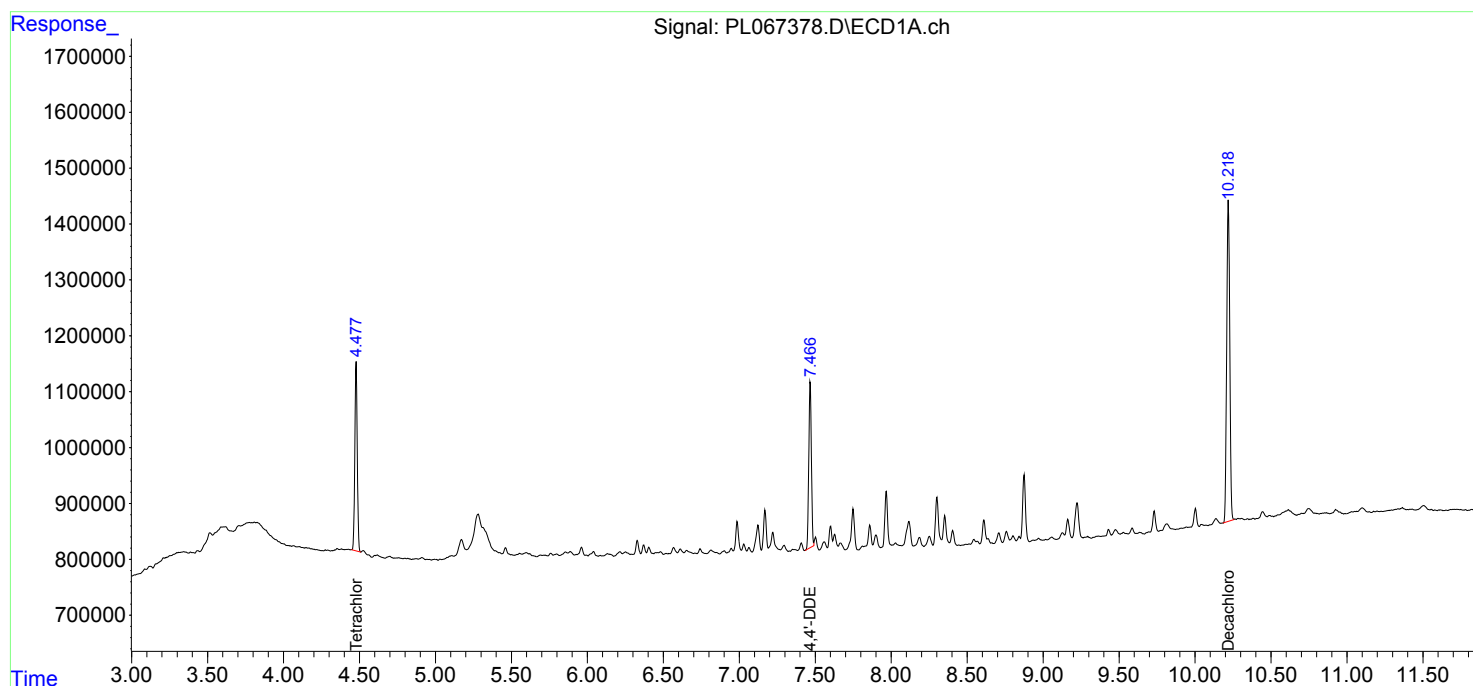


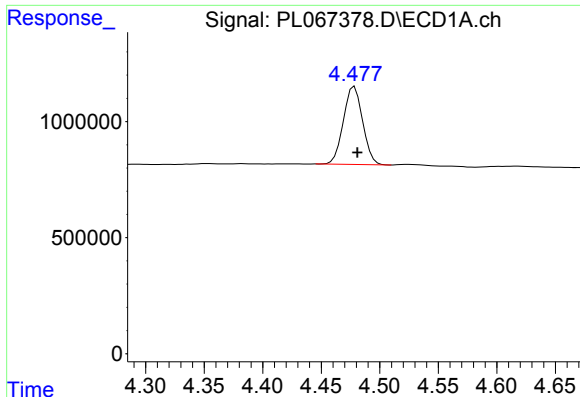

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 3852263
Conc: 7.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
0241-AMND-COMP-F(CL-05)

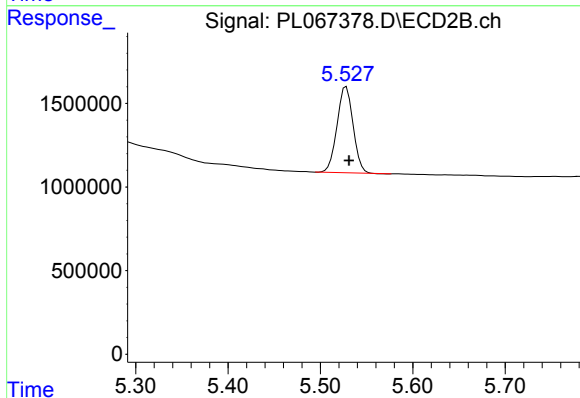


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 6222089
Conc: 6.60 ng/ml

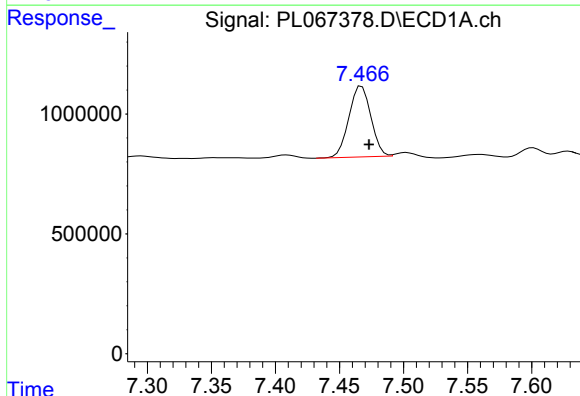


#12 4,4'-DDE

R.T.: 7.467 min
Delta R.T.: -0.006 min
Response: 3529325
Conc: 5.30 ng/ml

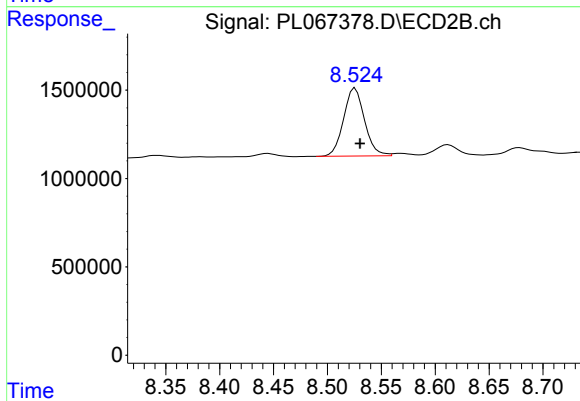

#12 4,4'-DDE


R.T.: 8.526 min
Delta R.T.: -0.005 min
Response: 5200584
Conc: 5.74 ng/ml

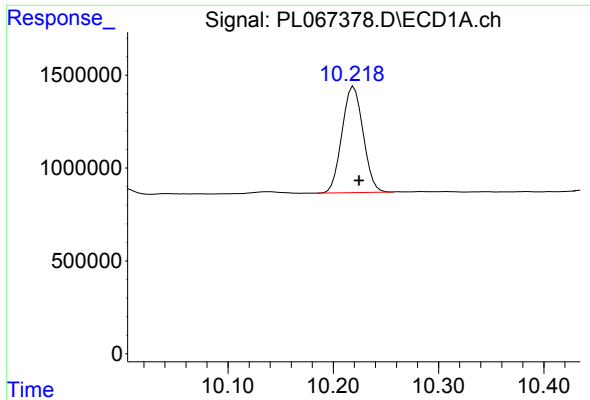

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.005 min
Response: 7990439
Conc: 11.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
0241-AMND-COMP-F(CL-05)

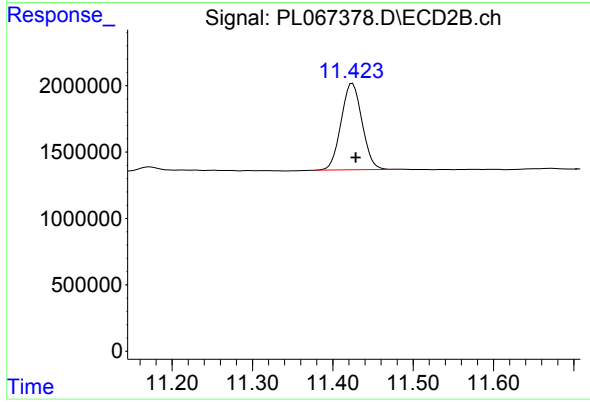

#28 Decachlorobiphenyl

R.T.: 11.424 min
Delta R.T.: -0.004 min
Response: 11782119
Conc: 11.83 ng/ml