

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
 Data File : PL067384.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2021 07:48
 Operator : AR\AJ
 Sample : M2678-10
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 0243-AMND-COMPOSITE-H

Manual Integrations
 APPROVED

Ankita
 6/14/2021 1:09:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 09:06:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.528	12040681	20608732	21.901	21.861
28)	SA Decachlor...	10.220	11.424	14904737	21854021	21.032	21.941
Target Compounds							
12)	B 4,4'-DDE	7.466	8.525	599388	815995	0.901m	0.901
16)	A 4,4'-DDD	8.048	9.063	605012	680321	1.041m	0.957m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061221\
Data File : PL067384.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2021 07:48
Operator : AR\AJ
Sample : M2678-10
Misc :
ALS Vial : 58 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
0243-AMND-COMPOSITE-H


Manual Integrations
APPROVED

Ankita
6/14/2021 1:09:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 09:06:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

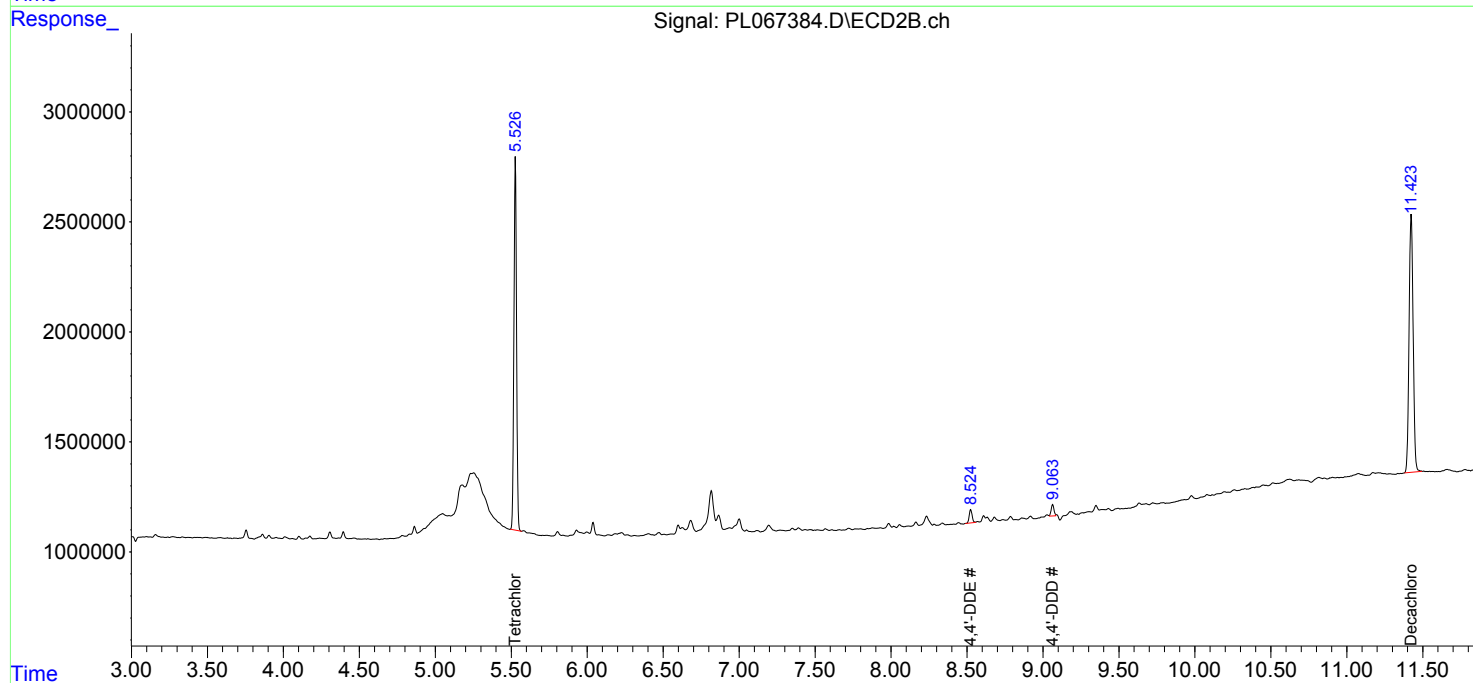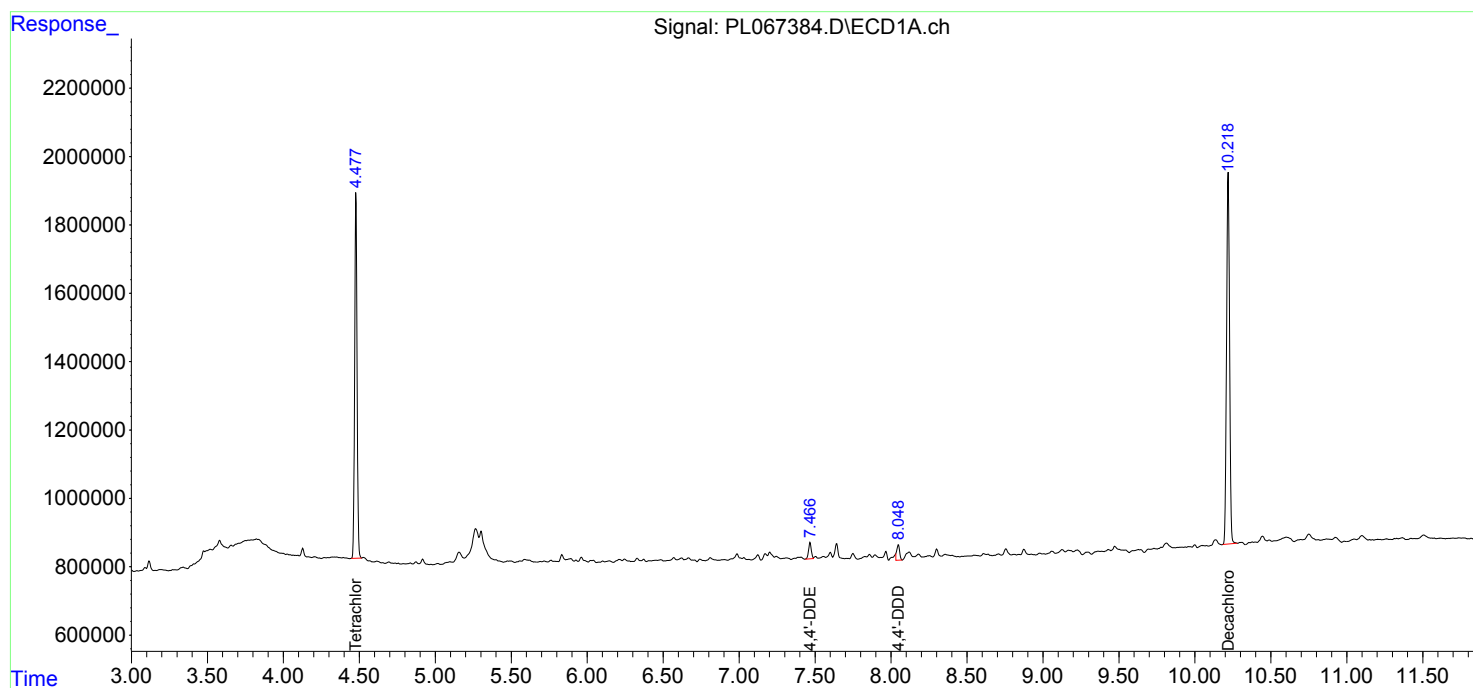

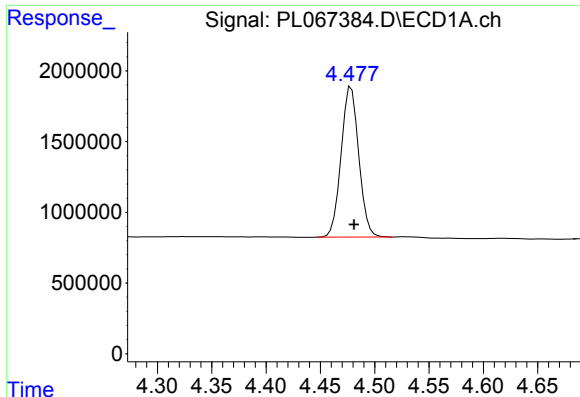


#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 12040681
Conc: 21.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
0243-AMND-COMPOSITE-H


Manual Integrations
APPROVED

Ankita
6/14/2021 1:09:52 PM

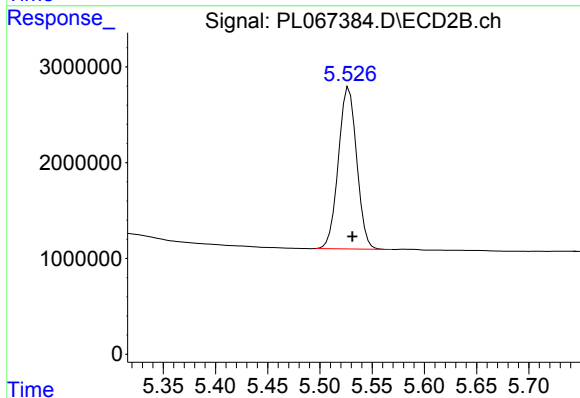


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 20608732
Conc: 21.86 ng/ml

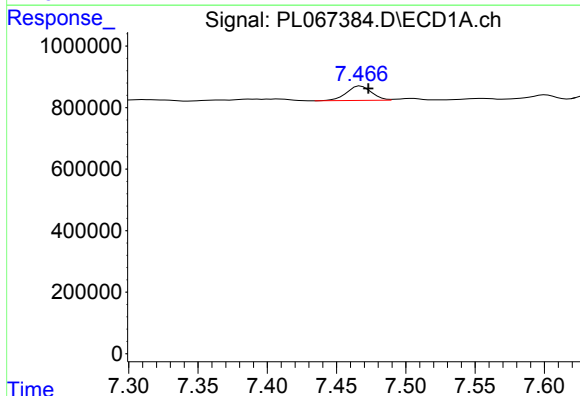


#12 4,4'-DDE

R.T.: 7.466 min
Delta R.T.: -0.007 min
Response: 599388
Conc: 0.90 ng/ml m

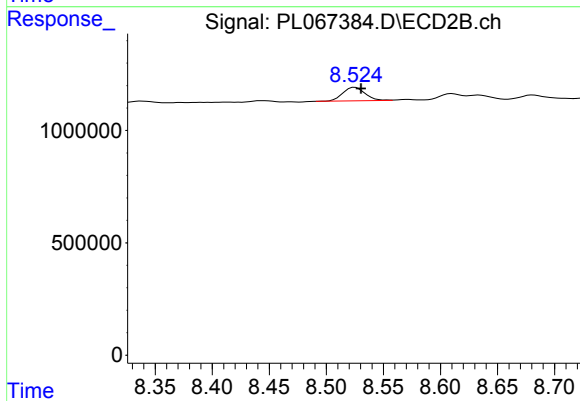

#12 4,4'-DDE

R.T.: 8.525 min
Delta R.T.: -0.005 min
Response: 815995
Conc: 0.90 ng/ml

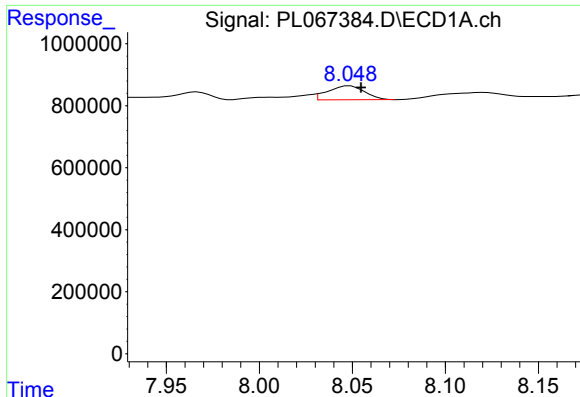


#16 4,4'-DDD

R.T.: 8.048 min
Delta R.T.: -0.007 min
Response: 605012
Conc: 1.04 ng/ml m

Instrument :
ECD_L
ClientSampleId :
0243-AMND-COMPOSITE-H


Manual Integrations
APPROVED

Ankita
6/14/2021 1:09:52 PM

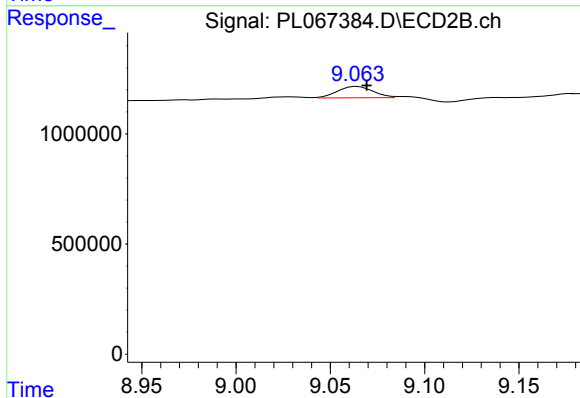


#16 4,4'-DDD

R.T.: 9.063 min
Delta R.T.: -0.006 min
Response: 680321
Conc: 0.96 ng/ml m

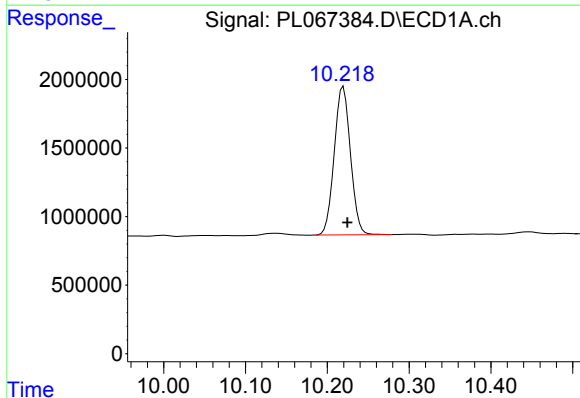

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.005 min
Response: 14904737
Conc: 21.03 ng/ml

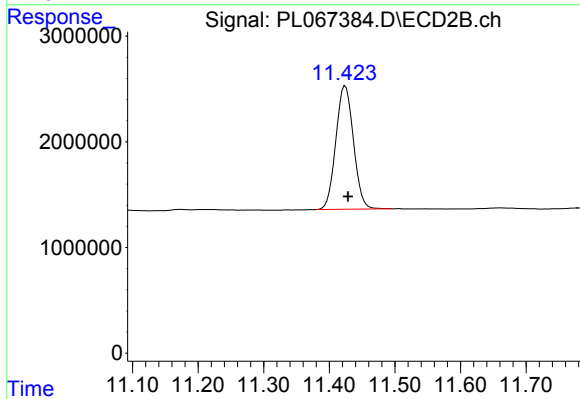

#28 Decachlorobiphenyl

R.T.: 11.424 min
Delta R.T.: -0.004 min
Response: 21854021
Conc: 21.94 ng/ml