

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061225\
 Data File : PL096018.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2025 09:04
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 22:52:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061125.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 11 14:04:36 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
8) B	Heptachlo...	5.716	0.000	9339053	0	2.368	N.D. #
10) B	gamma-Chl...	5.952f	0.000	2483273	0	0.614	N.D. #
25)	Chlordane-3	5.952f	0.000	2483273	0	3.403	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061225\
Data File : PL096018.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2025 09:04
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 22:52:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061125.M
Quant Title : GC Extractables
QLast Update : Wed Jun 11 14:04:36 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

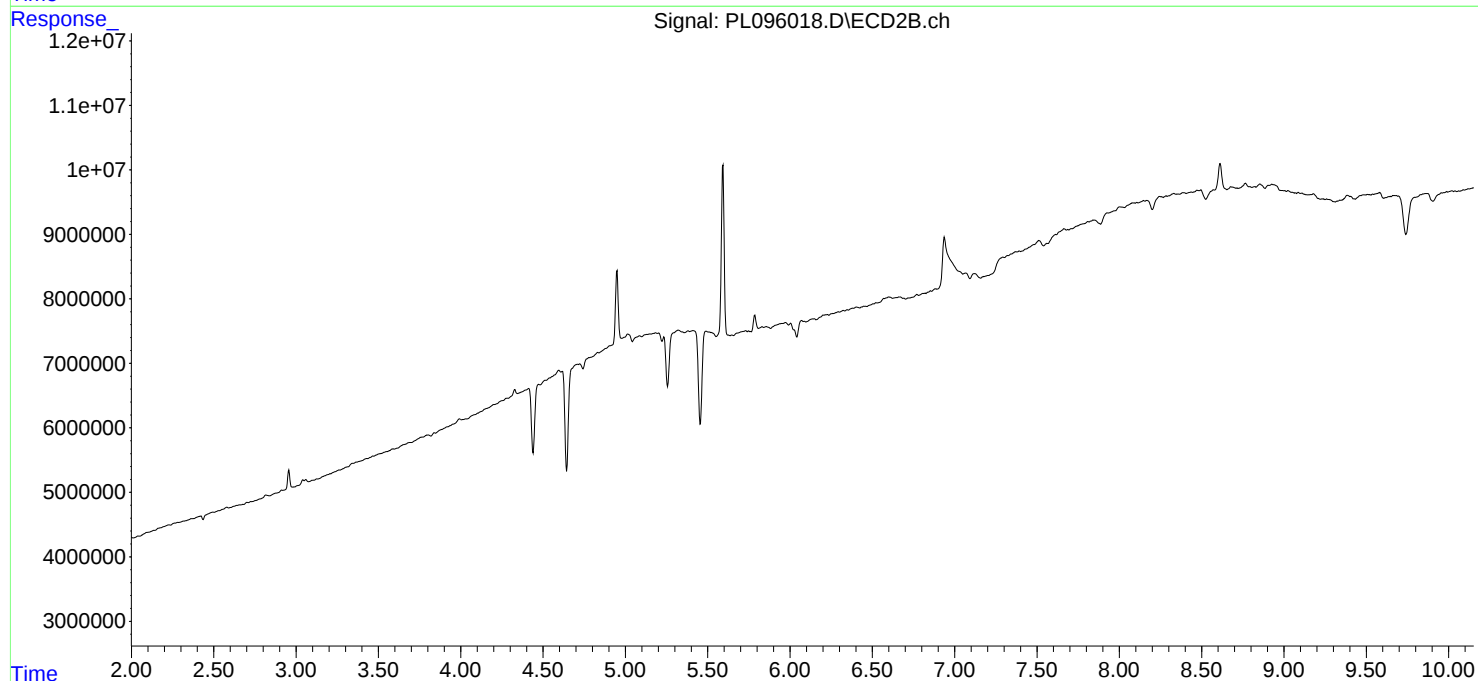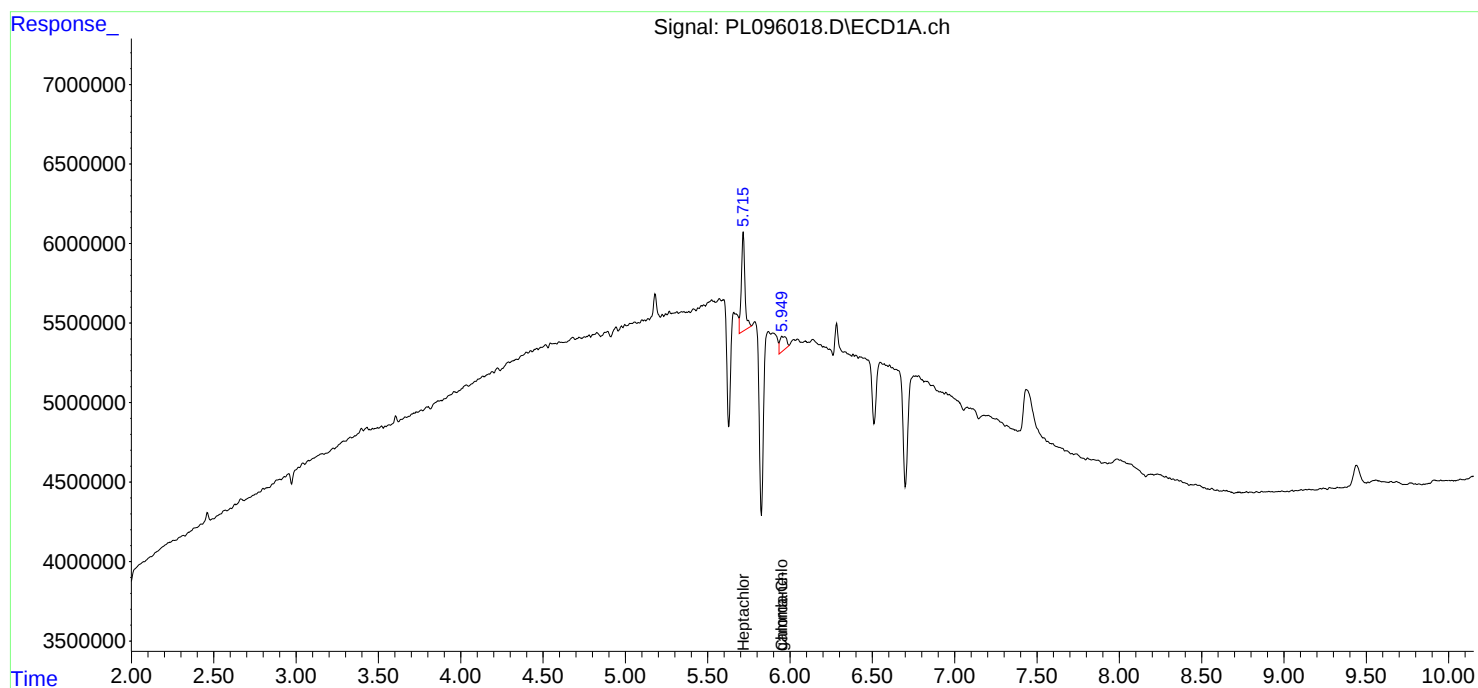


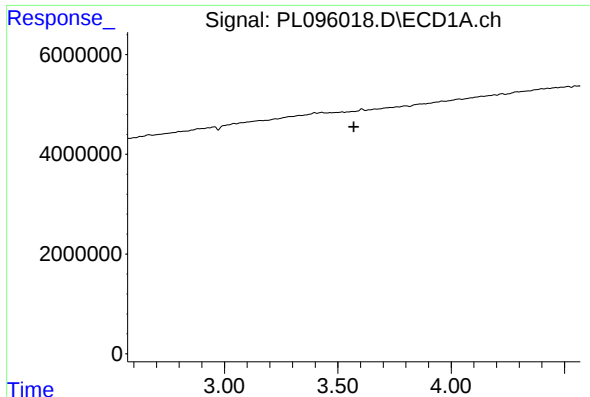

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.571 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

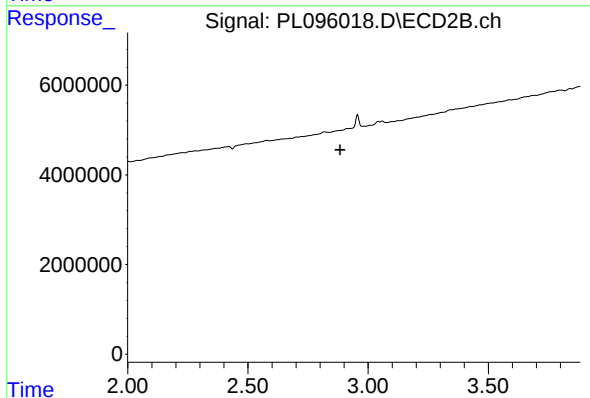


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.883 min
Response: 0
Conc: N.D.

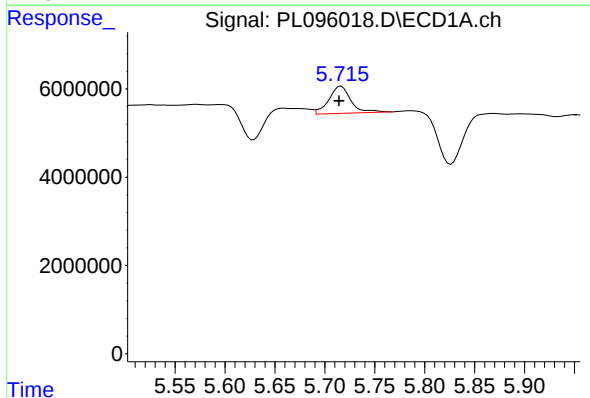


#8 Heptachlor epoxide

R.T.: 5.716 min
Delta R.T.: 0.002 min
Response: 9339053
Conc: 2.37 ng/ml

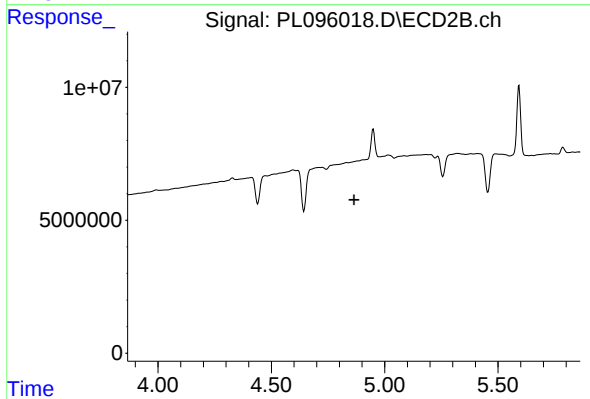

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.865 min
Response: 0
Conc: N.D.

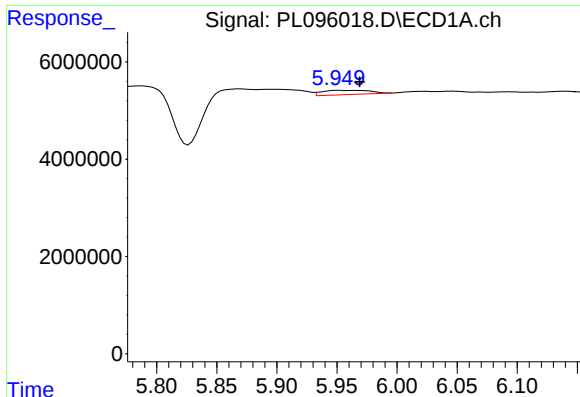

#10 gamma-Chlordane


R.T.: 5.952 min
Delta R.T.: -0.017 min
Response: 2483273
Conc: 0.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

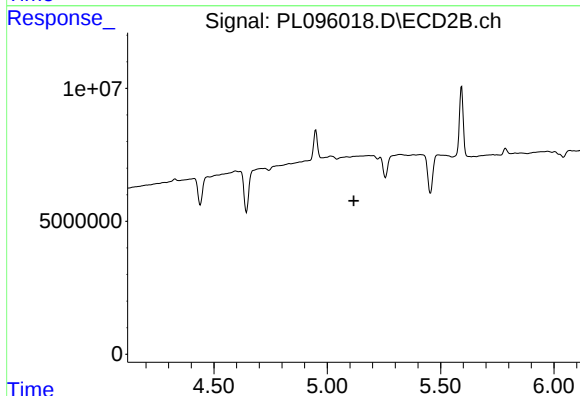


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.117 min
Response: 0
Conc: N.D.

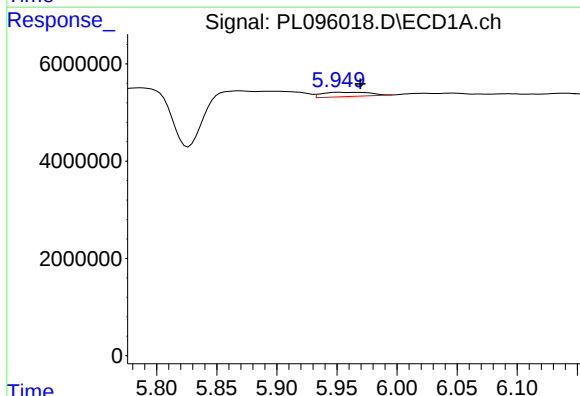


#25 Chlordane-3

R.T.: 5.952 min
Delta R.T.: -0.018 min
Response: 2483273
Conc: 3.40 ng/ml

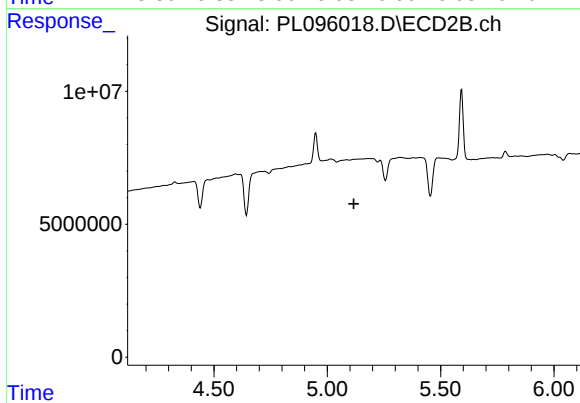

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.117 min
Response: 0
Conc: N.D.

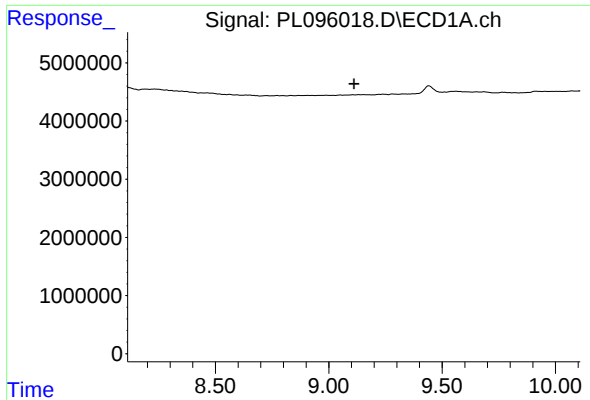

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.112 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

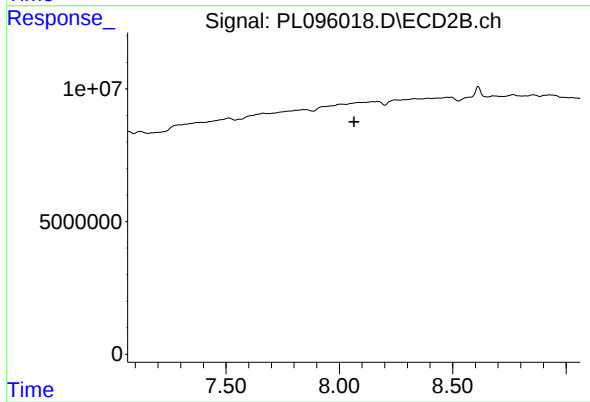

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.065 min
Response: 0
Conc: N.D.