

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061225\
 Data File : PL096028.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2025 17:24
 Operator : AR\AJ
 Sample : Q2296-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 22:53:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061125.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 11 14:04:36 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.571	2.883	87127683	75559796	26.813	18.617 #
28)	SA Decachlor...	9.114	8.065	39890947	87873110	16.319	18.482
Target Compounds							
3)	MA gamma-BHC...	0.000	3.728	0	8375737	N.D.	1.441 #
9)	A Endosulfan I	6.122f	5.256f	8698028	39186973	2.327	7.083 #
10)	B gamma-Chl...	5.948f	0.000	9601319	0	2.375	N.D. #
13)	MA Dieldrin	0.000	5.502	0	20656271	N.D.	3.807 #
15)	B Endosulfa...	0.000	6.073	0	8013932	N.D.	1.627 #
20)	A Methoxychlor	0.000	6.778f	0	12107776	N.D.	4.704 #
23)	Chlordane-1	0.000	3.897	0	12075117	N.D.	61.091 #
25)	Chlordane-3	5.948f	0.000	9601319	0	13.159	N.D. #
27)	Chlordane-5	0.000	6.073	0	8013932	N.D.	31.155 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061225\
Data File : PL096028.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2025 17:24
Operator : AR\AJ
Sample : Q2296-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
WC-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 22:53:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061125.M
Quant Title : GC Extractables
QLast Update : Wed Jun 11 14:04:36 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

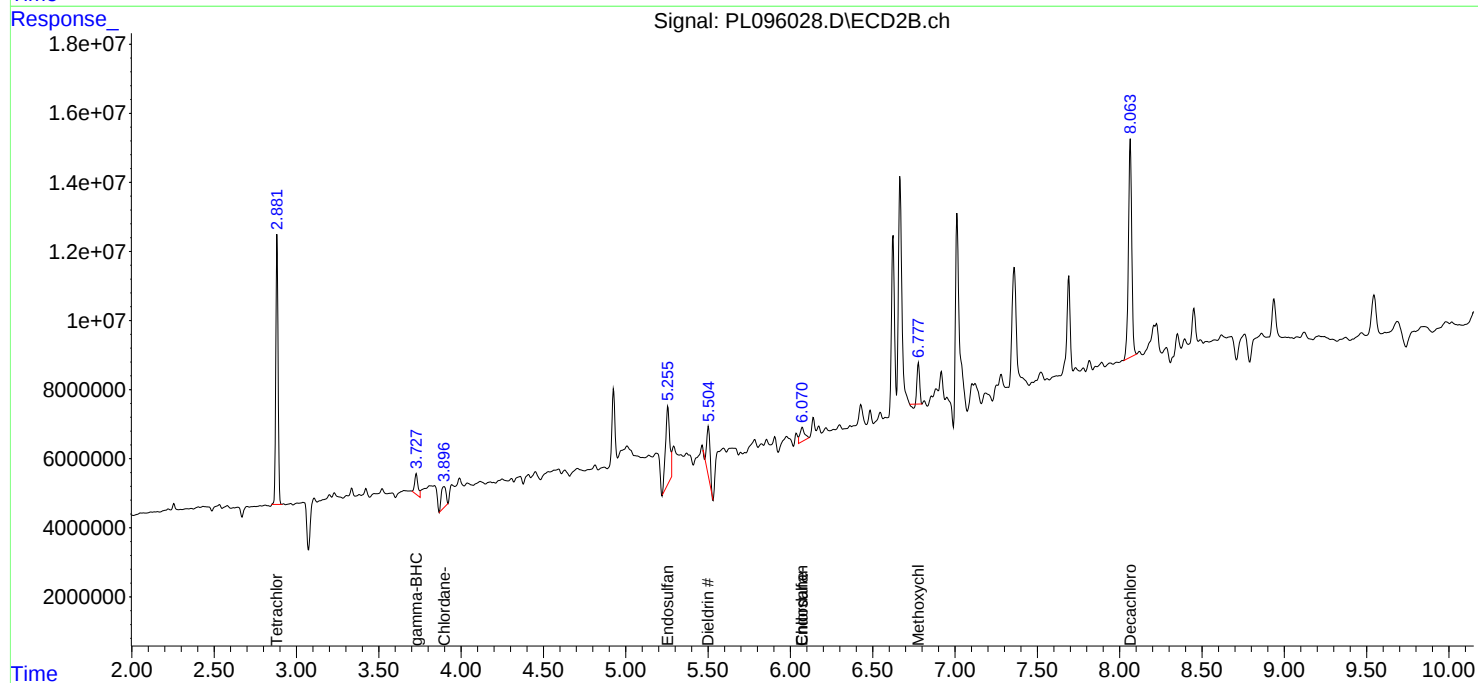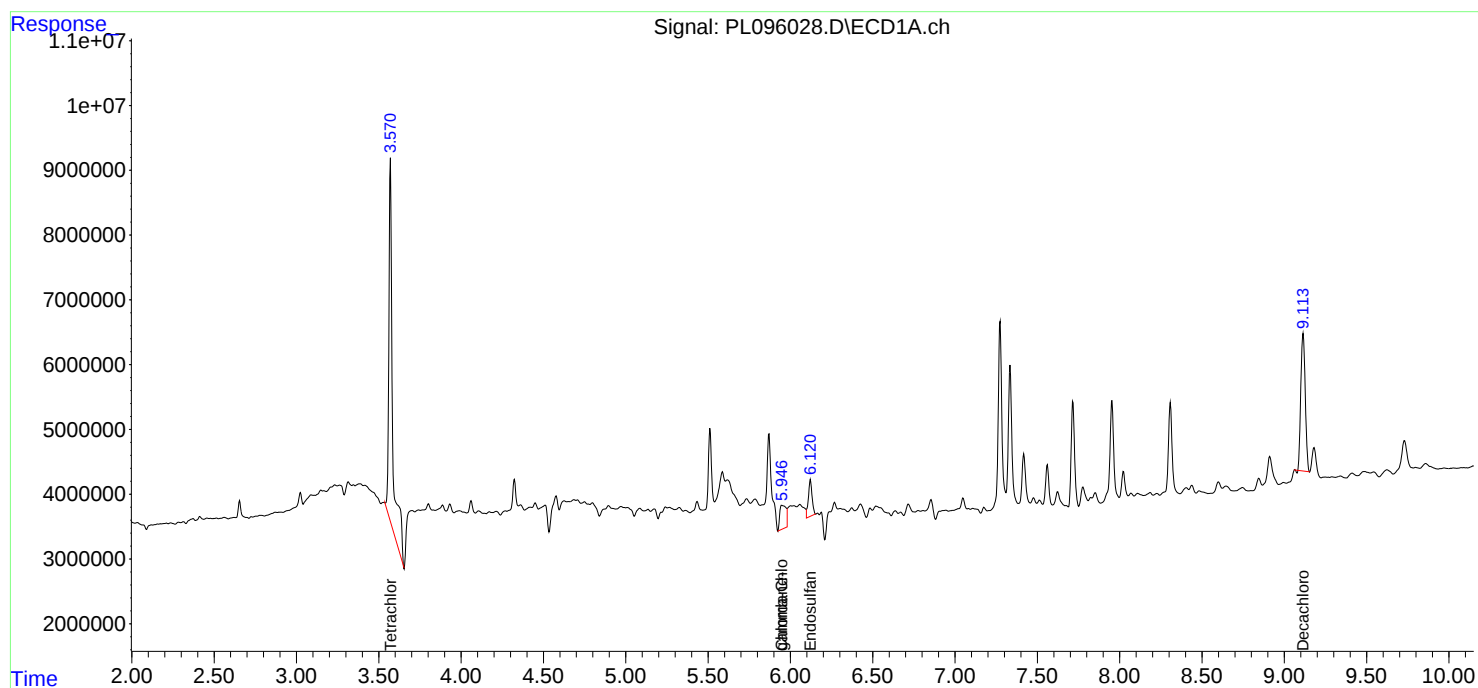


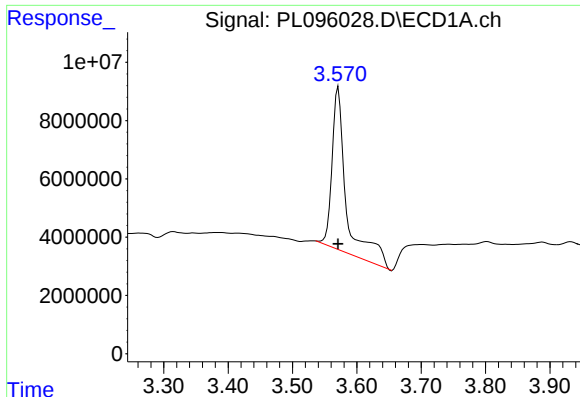

#1 Tetrachloro-m-xylene


R.T.: 3.571 min
Delta R.T.: 0.000 min
Response: 87127683
Conc: 26.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-2

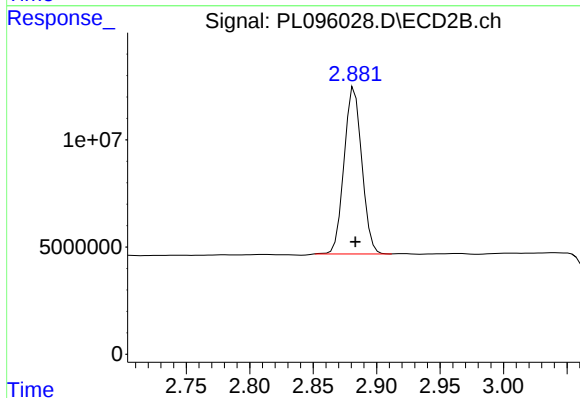


#1 Tetrachloro-m-xylene

R.T.: 2.883 min
Delta R.T.: 0.000 min
Response: 75559796
Conc: 18.62 ng/ml

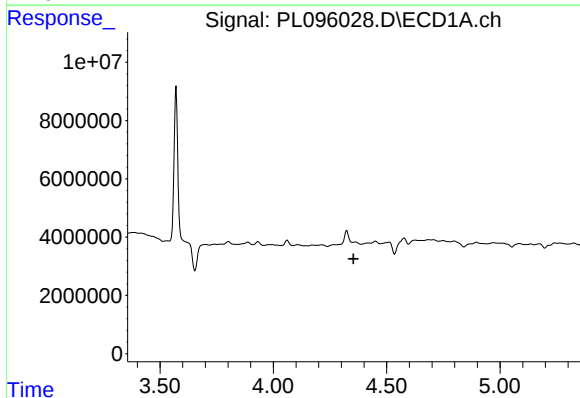


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.354 min
Response: 0
Conc: N.D.

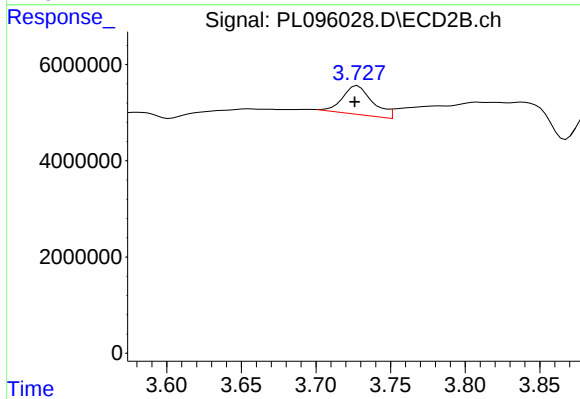

#3 gamma-BHC (Lindane)


R.T.: 3.728 min
Delta R.T.: 0.002 min
Response: 8375737
Conc: 1.44 ng/ml

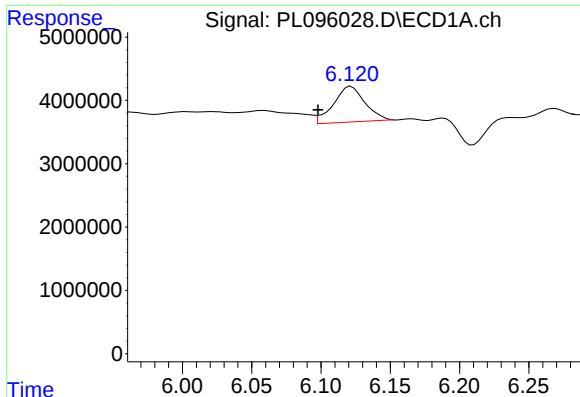

#9 Endosulfan I


R.T.: 6.122 min
Delta R.T.: 0.024 min
Response: 8698028
Conc: 2.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-2

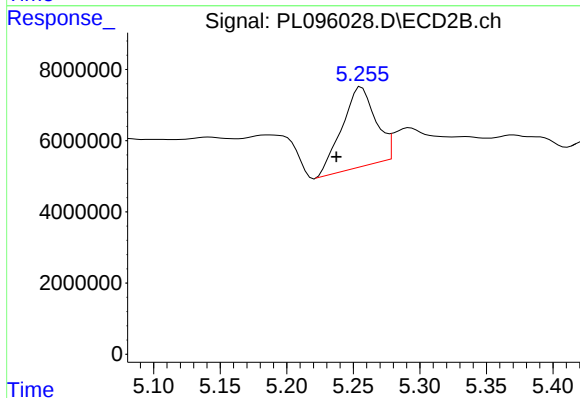


#9 Endosulfan I

R.T.: 5.256 min
Delta R.T.: 0.019 min
Response: 39186973
Conc: 7.08 ng/ml

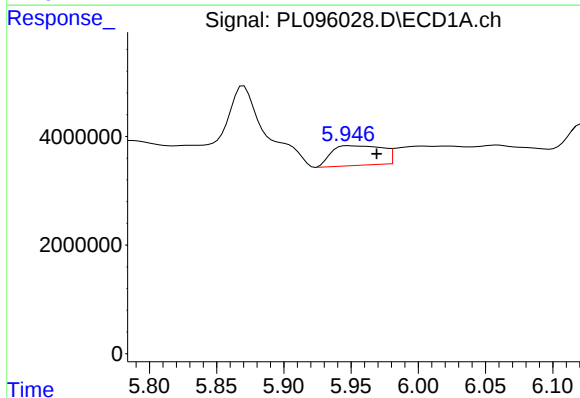


#10 gamma-Chlordane

R.T.: 5.948 min
Delta R.T.: -0.021 min
Response: 9601319
Conc: 2.38 ng/ml

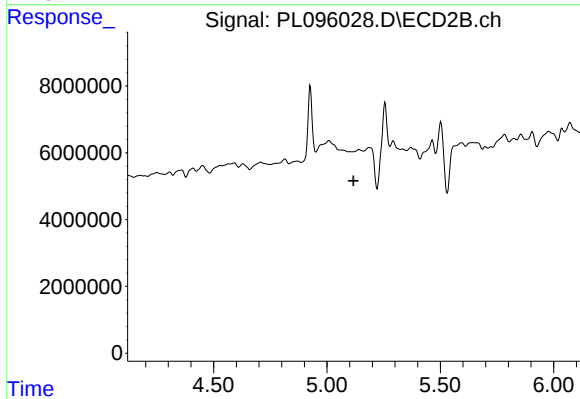

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.117 min
Response: 0
Conc: N.D.

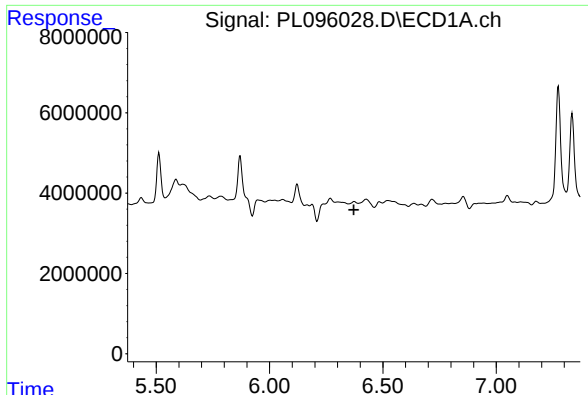

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-2

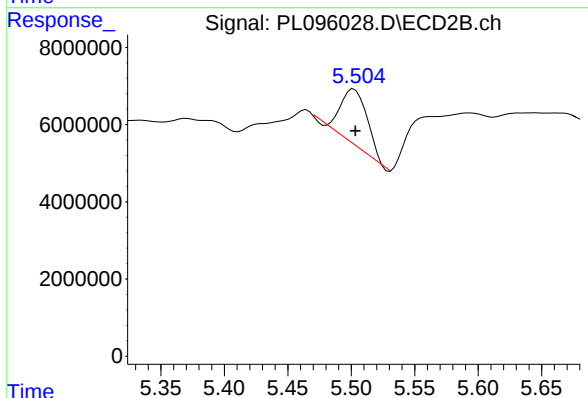


#13 Dieldrin

R.T.: 5.502 min
Delta R.T.: -0.001 min
Response: 20656271
Conc: 3.81 ng/ml

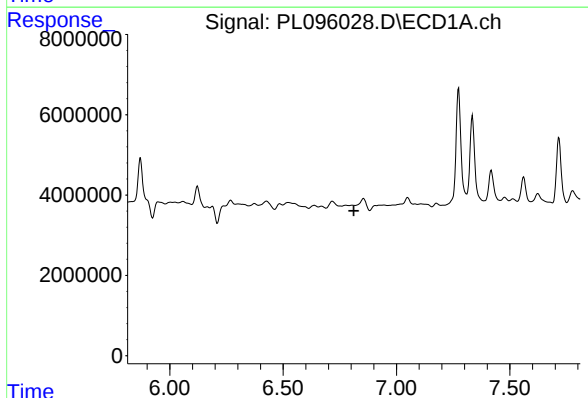


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.812 min
Response: 0
Conc: N.D.

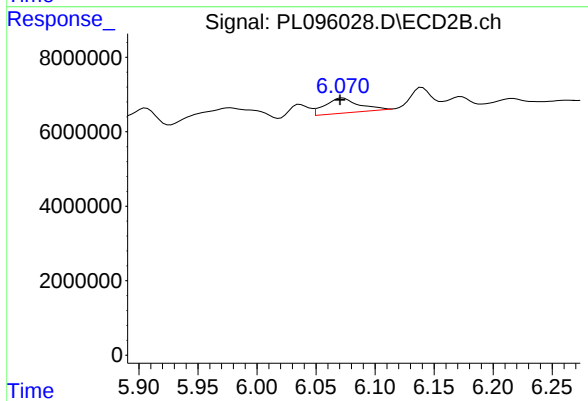

#15 Endosulfan II


R.T.: 6.073 min
Delta R.T.: 0.002 min
Response: 8013932
Conc: 1.63 ng/ml

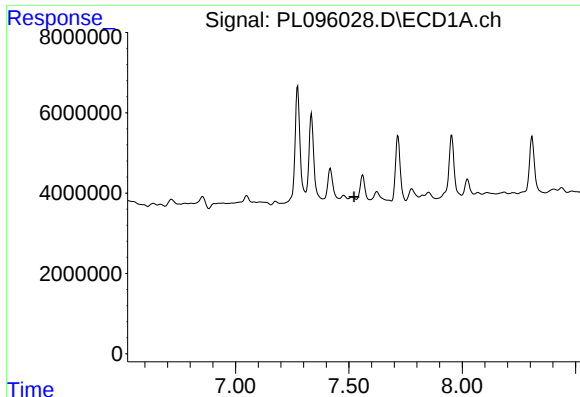

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-2

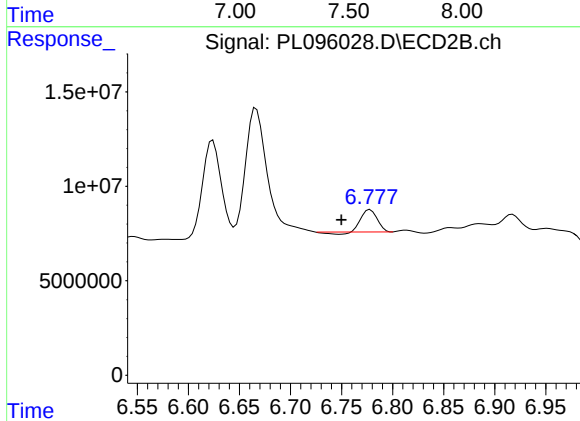


#20 Methoxychlor

R.T.: 6.778 min
Delta R.T.: 0.028 min
Response: 12107776
Conc: 4.70 ng/ml

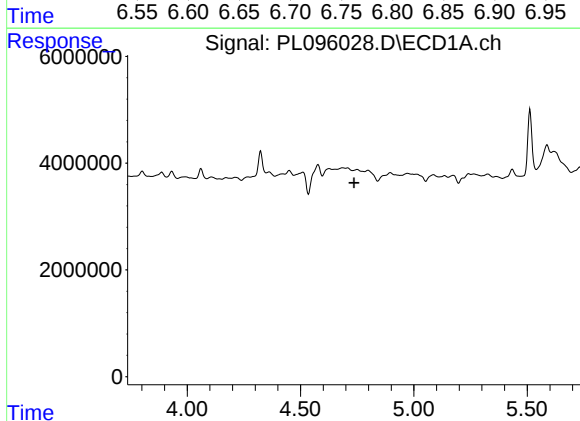


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.737 min
Response: 0
Conc: N.D.

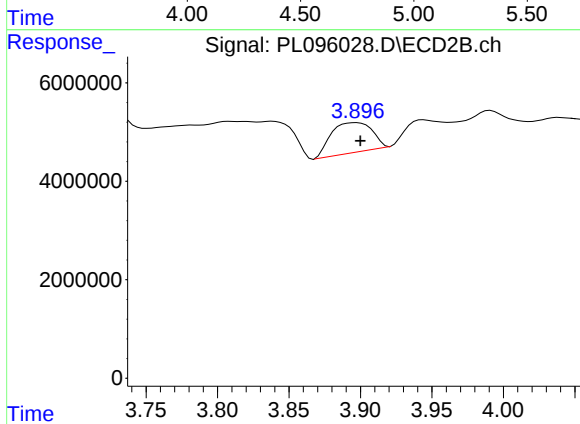

#23 Chlordane-1


R.T.: 3.897 min
Delta R.T.: -0.003 min
Response: 12075117
Conc: 61.09 ng/ml

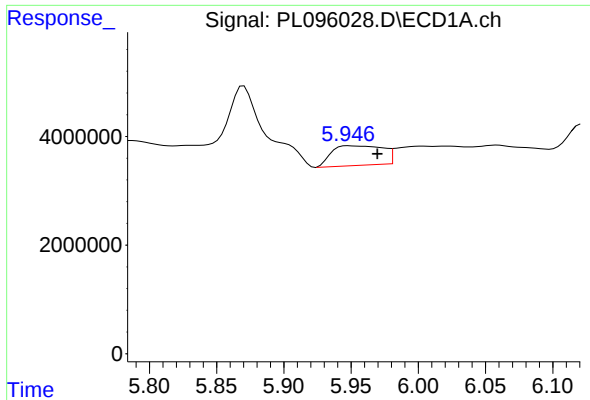

#25 Chlordane-3


R.T.: 5.948 min
Delta R.T.: -0.022 min
Response: 9601319
Conc: 13.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-2

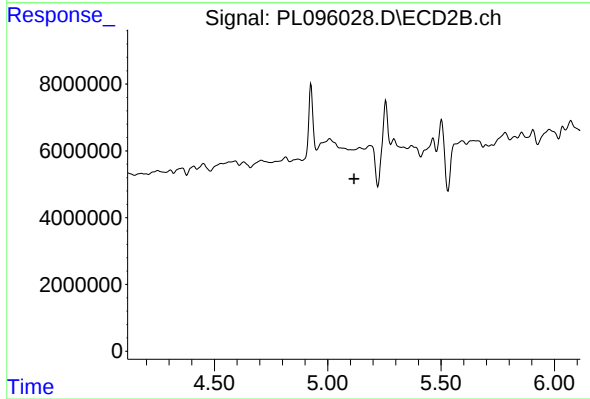


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.117 min
Response: 0
Conc: N.D.

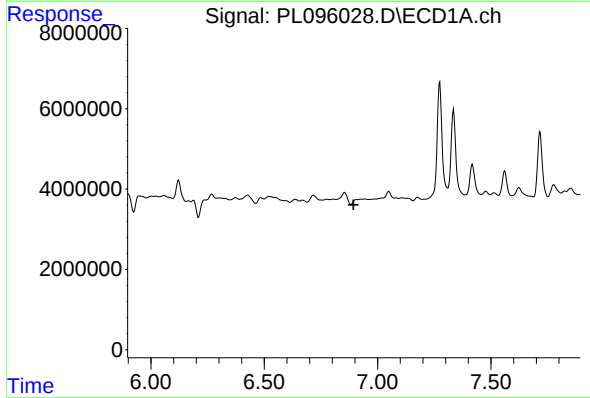


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.894 min
Response: 0
Conc: N.D.

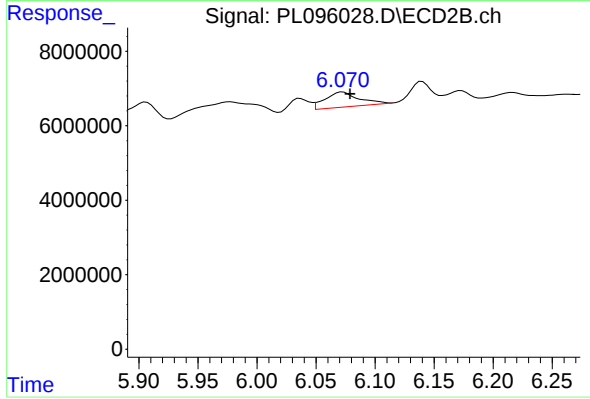

#27 Chlordane-5

R.T.: 6.073 min
Delta R.T.: -0.006 min
Response: 8013932
Conc: 31.15 ng/ml

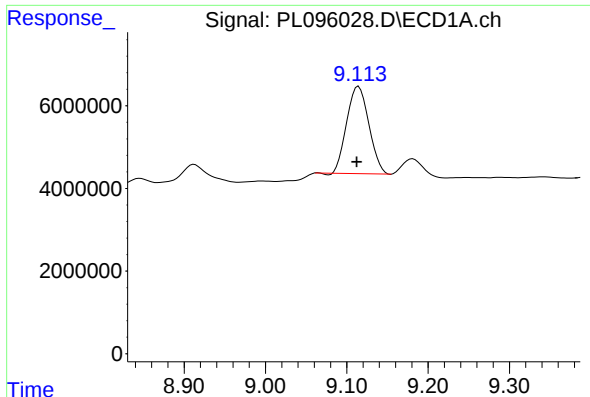

#28 Decachlorobiphenyl


R.T.: 9.114 min

Delta R.T.: 0.002 min

Response: 39890947

Conc: 16.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-2

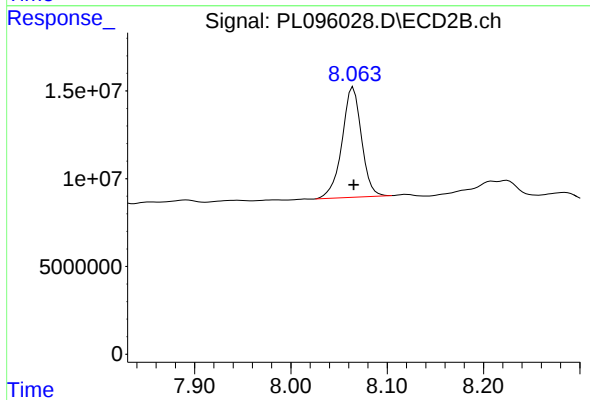

#28 Decachlorobiphenyl

R.T.: 8.065 min

Delta R.T.: 0.000 min

Response: 87873110

Conc: 18.48 ng/ml