

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061225\
 Data File : PL096026.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2025 16:56
 Operator : AR\AJ
 Sample : Q2295-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP02-MH5-WC

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/13/2025
 Supervised By :mohammad ahmed 06/16/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 22:53:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061125.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 11 14:04:36 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.570	2.883	63300824	79098466	19.481m	19.489
28) SA Decachlor...	9.113	8.065	40486891	75159509	16.563	15.808

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061225\
Data File : PL096026.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2025 16:56
Operator : AR\AJ
Sample : Q2295-05
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP02-MH5-WC


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/13/2025
Supervised By : mohammad ahmed 06/16/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 22:53:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061125.M
Quant Title : GC Extractables
QLast Update : Wed Jun 11 14:04:36 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

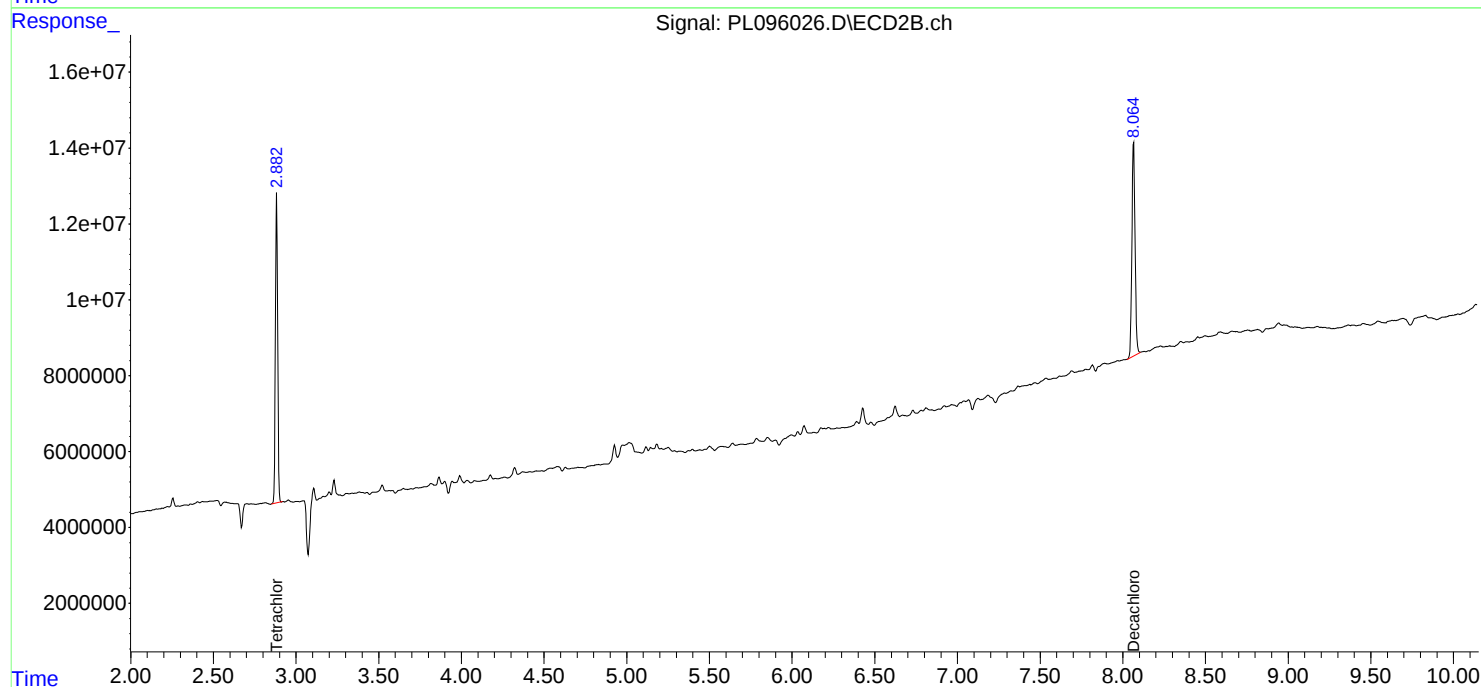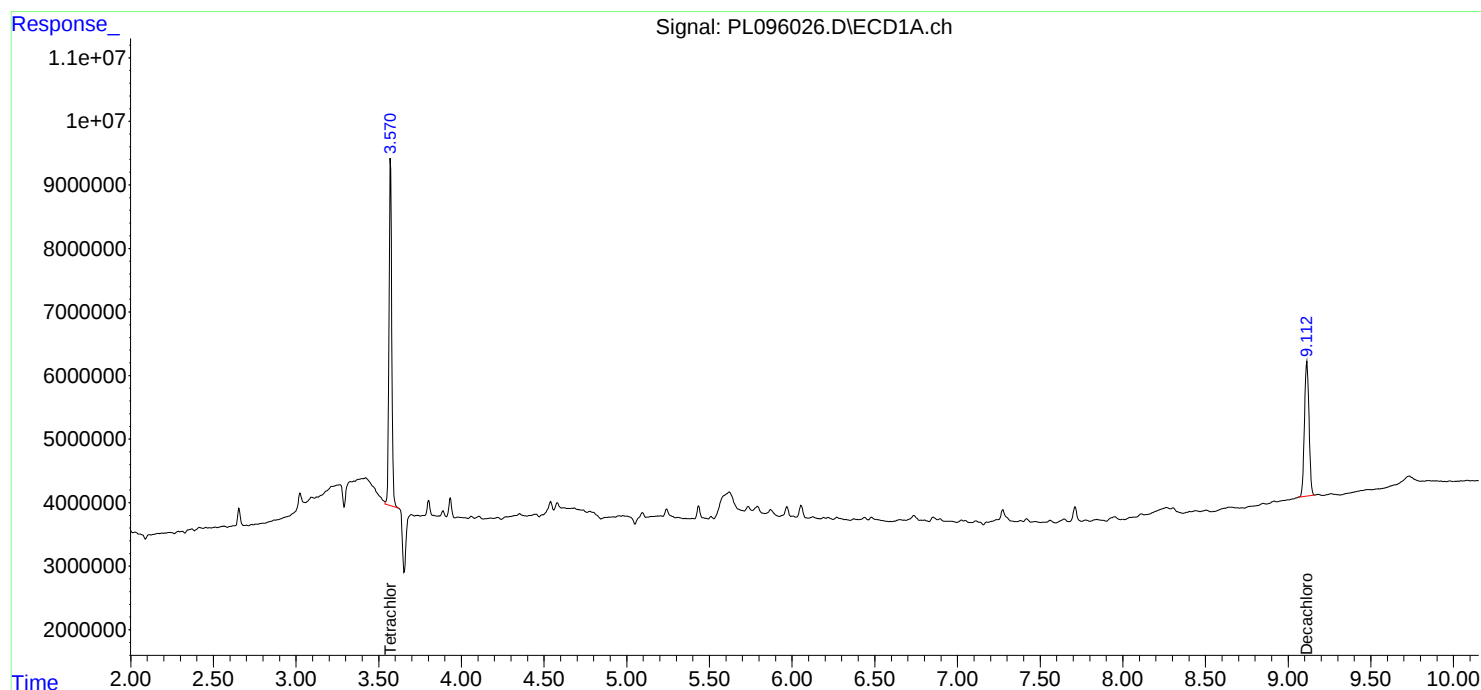

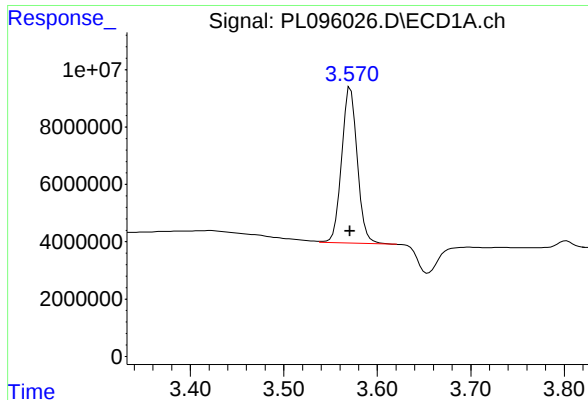


#1 Tetrachloro-m-xylene

R.T.: 3.570 min
Delta R.T.: -0.001 min
Response: 63300824
Conc: 19.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP02-MH5-WC


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/13/2025
Supervised By :mohammad ahmed 06/16/2025

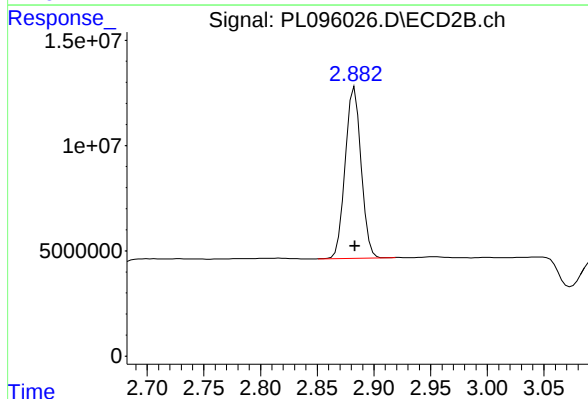


#1 Tetrachloro-m-xylene

R.T.: 2.883 min
Delta R.T.: 0.000 min
Response: 79098466
Conc: 19.49 ng/ml

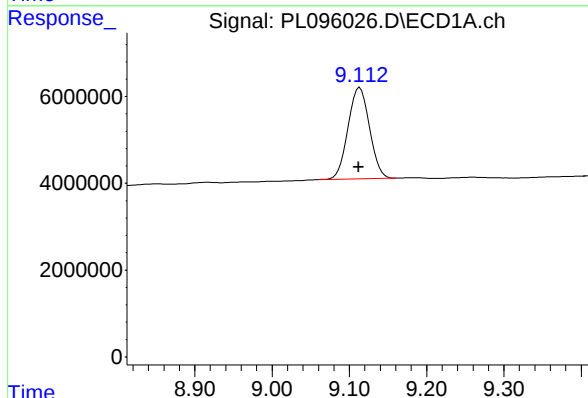

#28 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: 0.001 min
Response: 40486891
Conc: 16.56 ng/ml

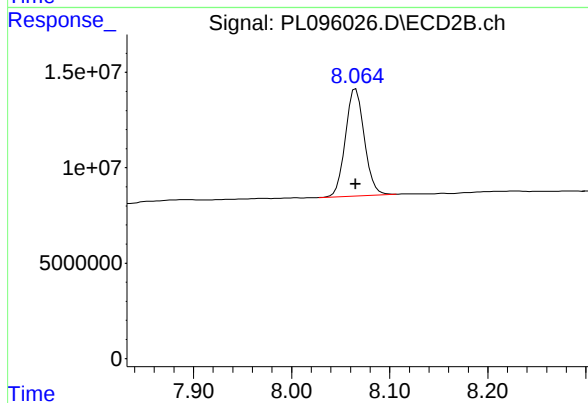

#28 Decachlorobiphenyl

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 75159509
Conc: 15.81 ng/ml