

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061319\
 Data File : PL049459.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2019 08:45
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 00:59:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

8) B	Heptachlo...	0.000	5.799	0	8444387	N.D.	2.583 #
12) B	4,4'-DDE	5.460f	0.000	8140869	0	0.520	N.D. #
13) MA	Dieldrin	5.560	0.000	11954821	0	0.782	N.D. #
14) MA	Endrin	5.829f	0.000	21819612	0	1.513	N.D. #
16) A	4,4'-DDD	5.954	0.000	70891294	0	5.957	N.D. #
17) MA	4,4'-DDT	6.181	0.000	257.5E6	0	20.913	N.D. #
18) B	Endrin al...	6.270f	0.000	250.7E6	0	22.903	N.D. #
20) A	Methoxychlor	6.741f	0.000	257.8E6	0	40.194	N.D. #
21) B	Endrin ke...	6.946	0.000	65957555	0	4.635	N.D. #
22)	Mirex	7.112	0.000	14537152	0	1.380	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061319\
Data File : PL049459.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2019 08:45
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 00:59:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

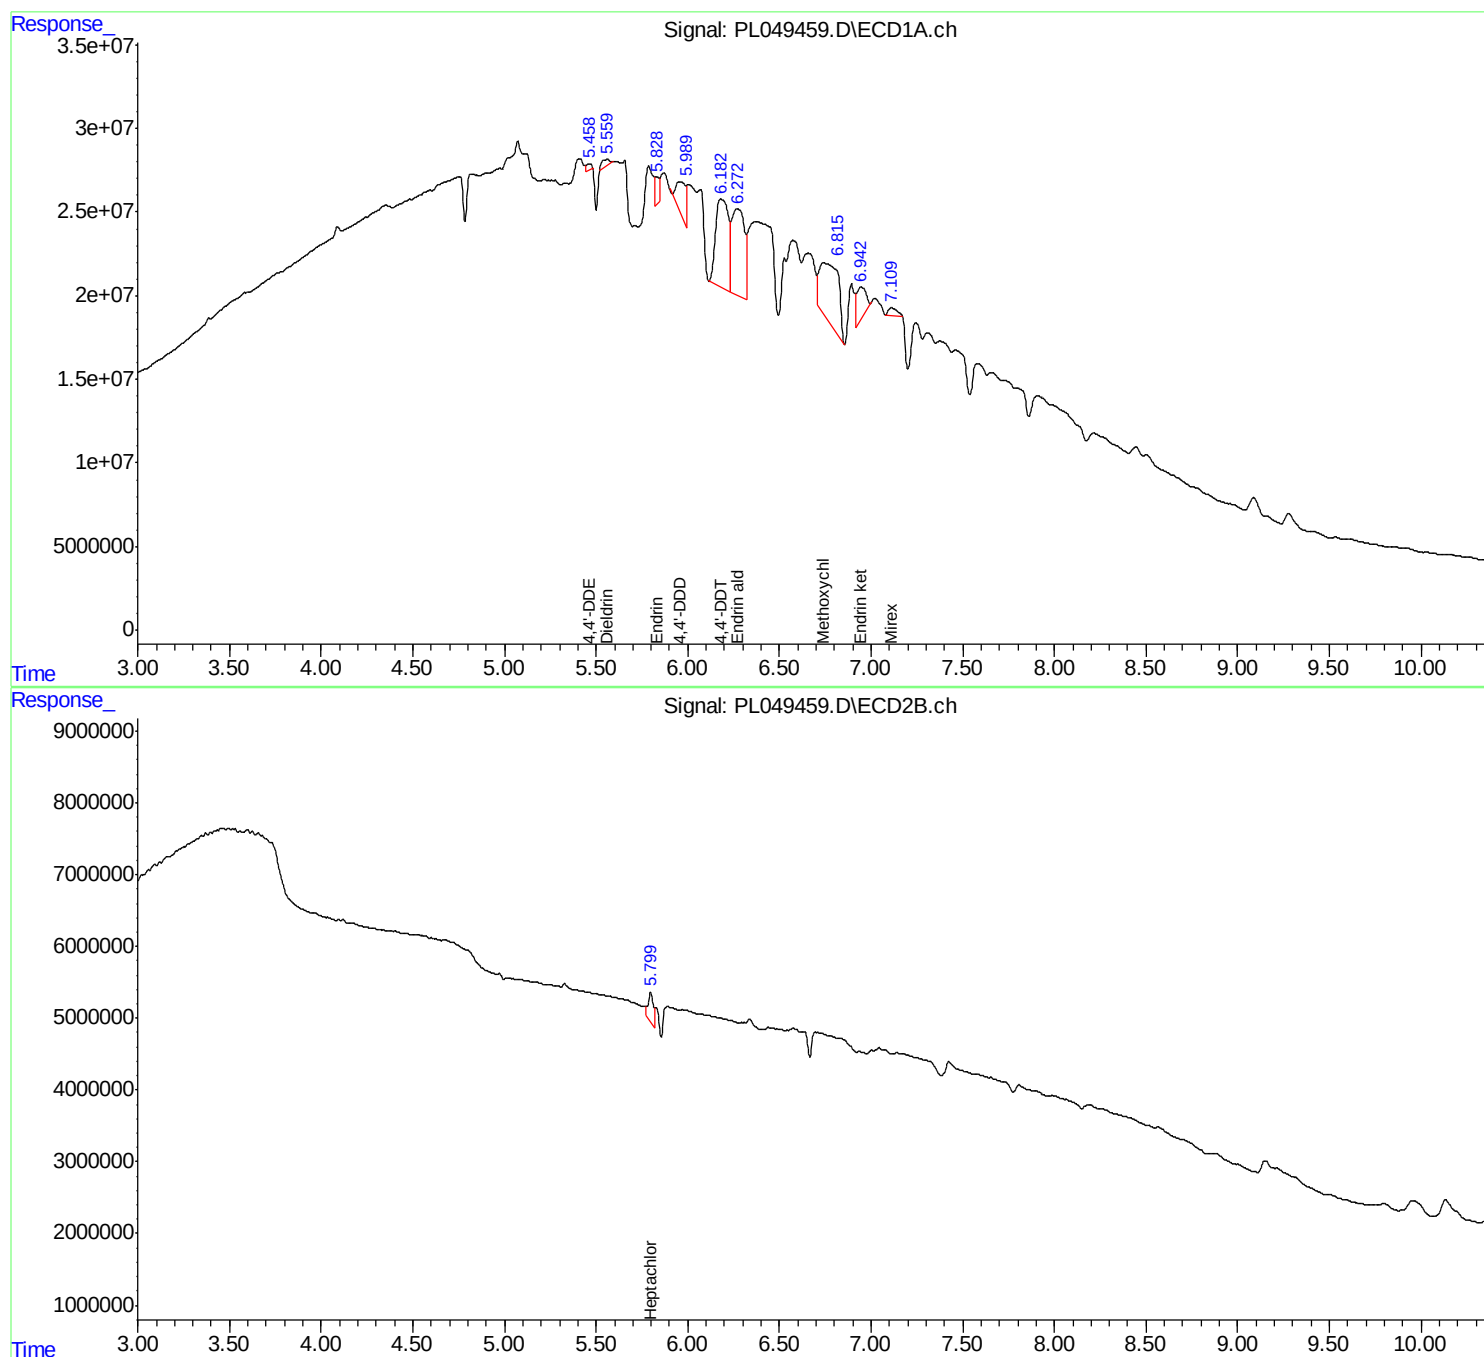


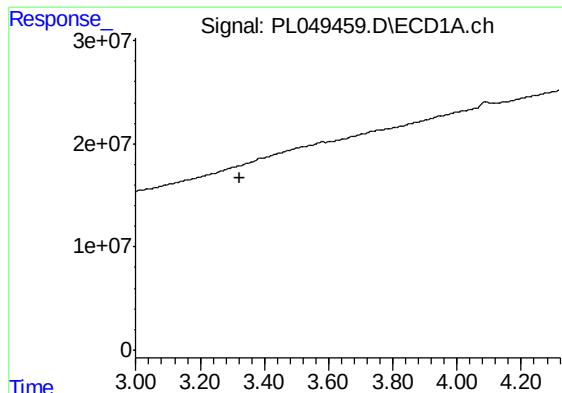

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.324 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

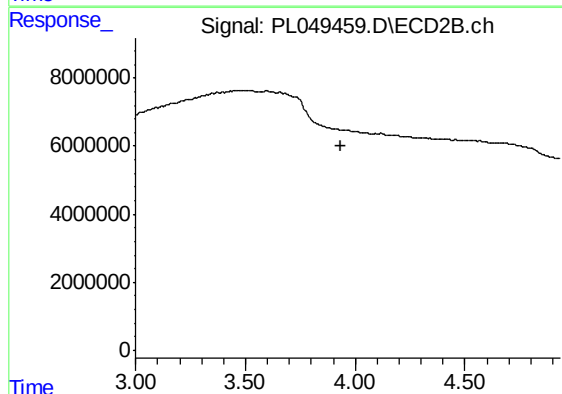


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.936 min
Response: 0
Conc: N.D.

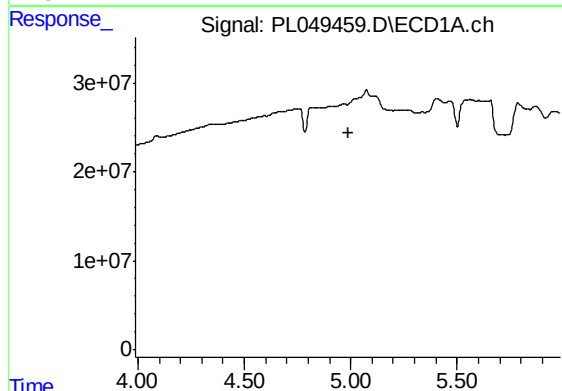


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.988 min
Response: 0
Conc: N.D.

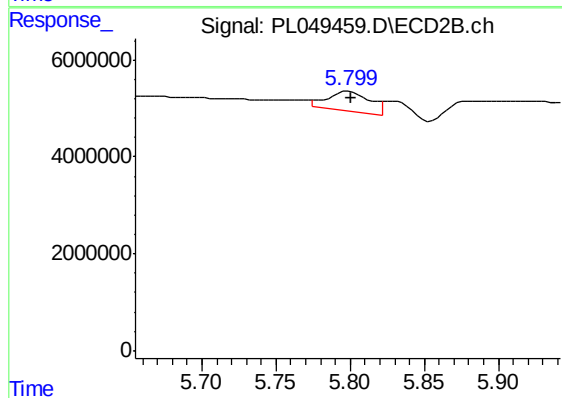

#8 Heptachlor epoxide


R.T.: 5.799 min
Delta R.T.: -0.001 min
Response: 8444387
Conc: 2.58 ng/ml

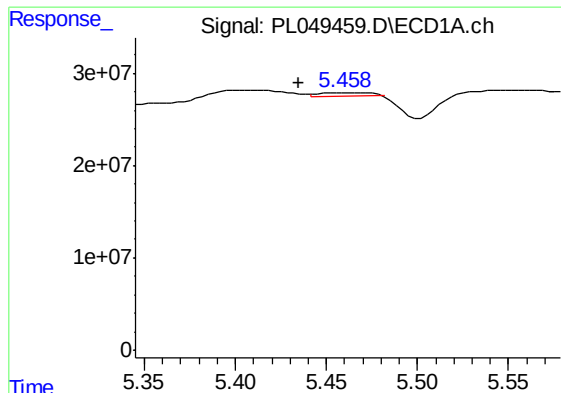

#12 4,4'-DDE


R.T.: 5.460 min
Delta R.T.: 0.026 min
Response: 8140869
Conc: 0.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

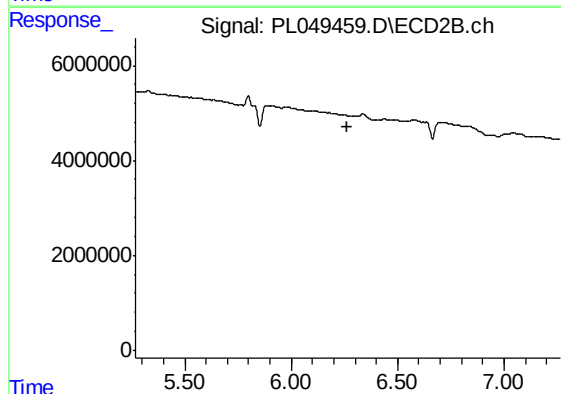


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.267 min
Response: 0
Conc: N.D.

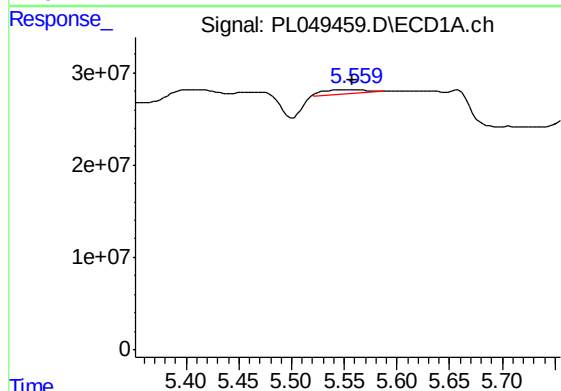


#13 Dieldrin

R.T.: 5.560 min
Delta R.T.: 0.002 min
Response: 11954821
Conc: 0.78 ng/ml

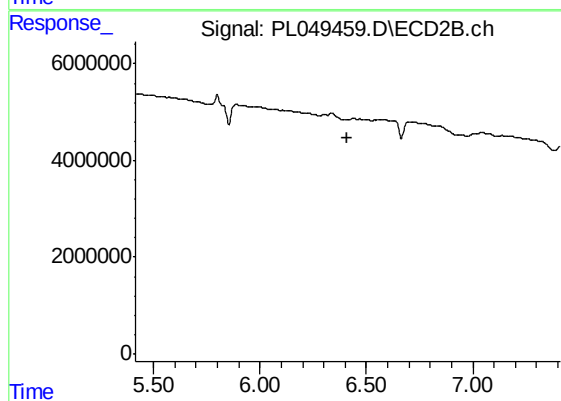

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.413 min
Response: 0
Conc: N.D.

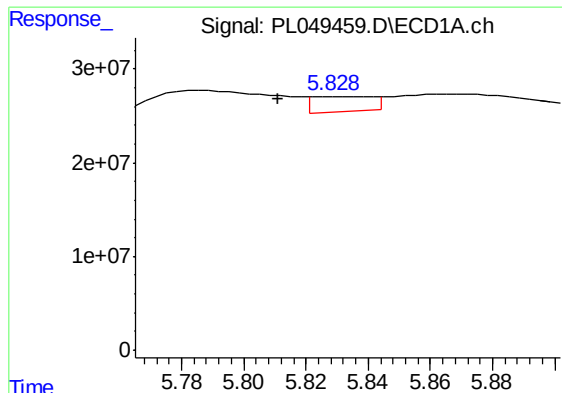

#14 Endrin


R.T.: 5.829 min
Delta R.T.: 0.019 min
Response: 21819612
Conc: 1.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

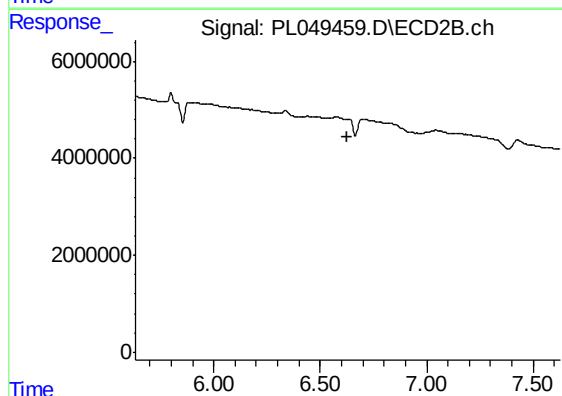


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.630 min
Response: 0
Conc: N.D.

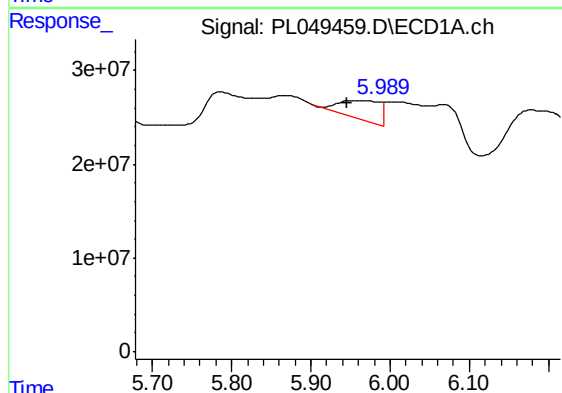


#16 4,4'-DDD

R.T.: 5.954 min
Delta R.T.: 0.009 min
Response: 70891294
Conc: 5.96 ng/ml

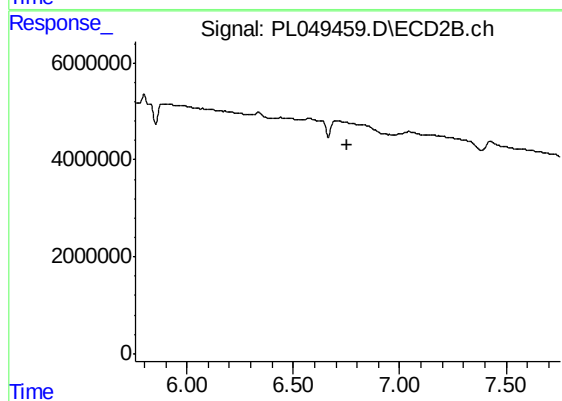

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.756 min
Response: 0
Conc: N.D.

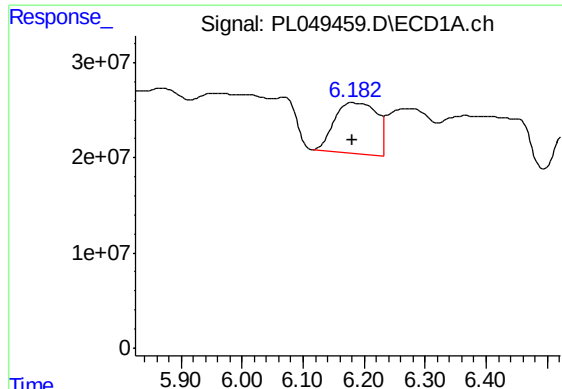

#17 4,4'-DDT


R.T.: 6.181 min
Delta R.T.: 0.000 min
Response: 257494828
Conc: 20.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

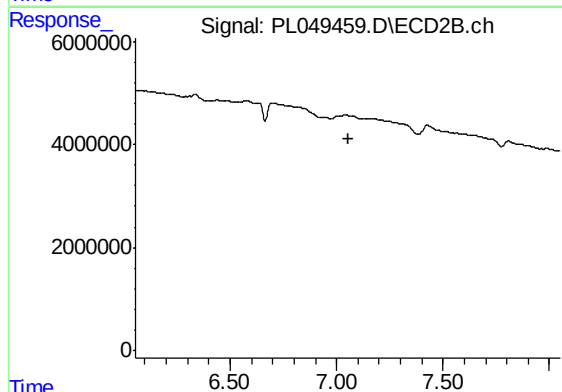


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.054 min
Response: 0
Conc: N.D.

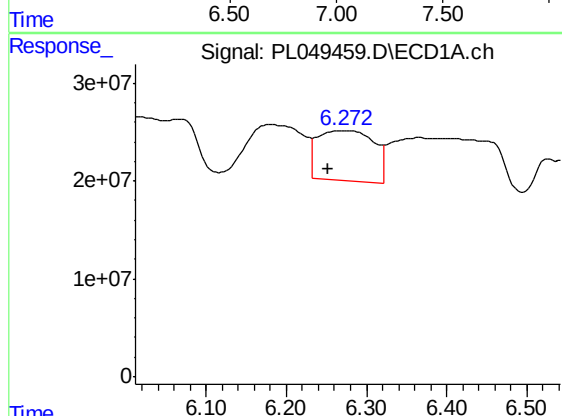


#18 Endrin aldehyde

R.T.: 6.270 min
Delta R.T.: 0.018 min
Response: 250650753
Conc: 22.90 ng/ml

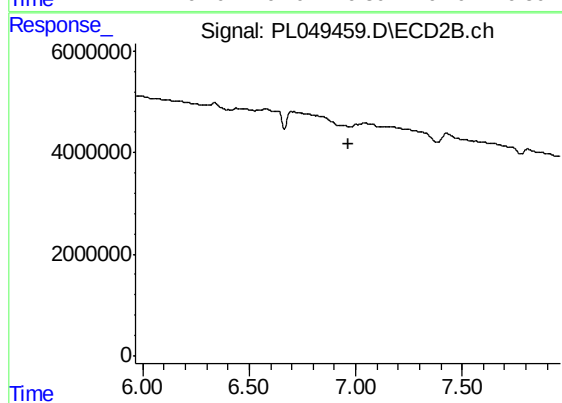

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.965 min
Response: 0
Conc: N.D.

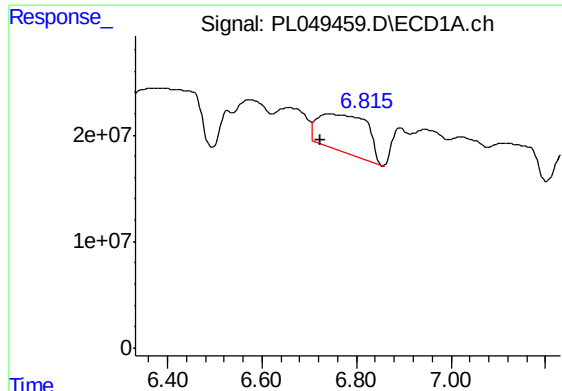

#20 Methoxychlor


R.T.: 6.741 min
Delta R.T.: 0.016 min
Response: 257791236
Conc: 40.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

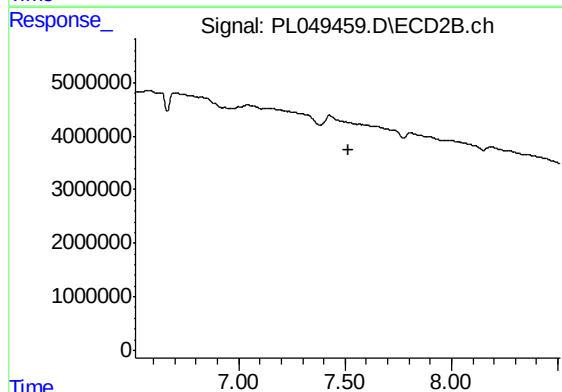


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.514 min
Response: 0
Conc: N.D.

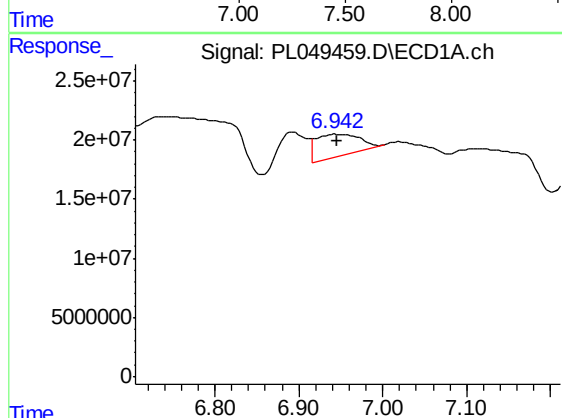


#21 Endrin ketone

R.T.: 6.946 min
Delta R.T.: 0.000 min
Response: 65957555
Conc: 4.63 ng/ml

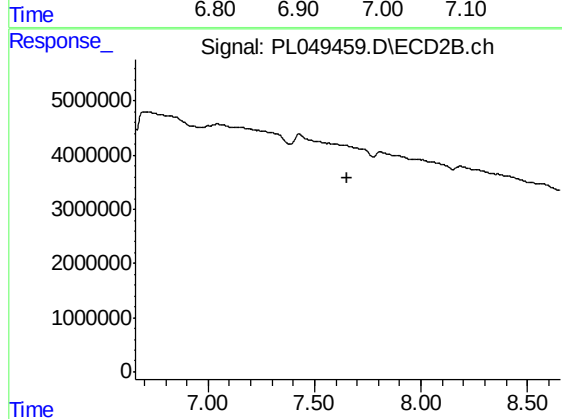

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.657 min
Response: 0
Conc: N.D.

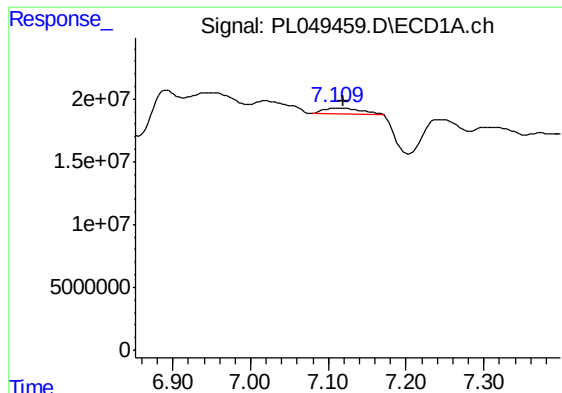

#22 Mirex


R.T.: 7.112 min
Delta R.T.: -0.008 min
Response: 14537152
Conc: 1.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

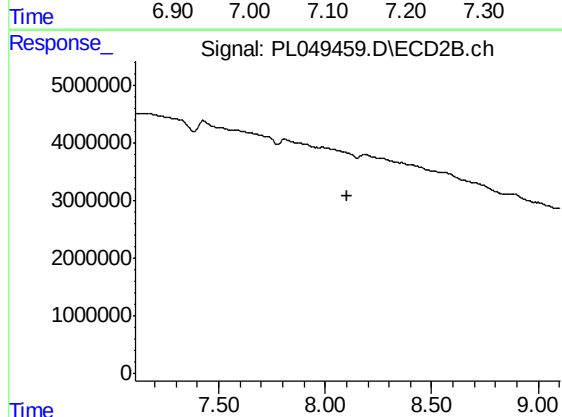


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.107 min
Response: 0
Conc: N.D.

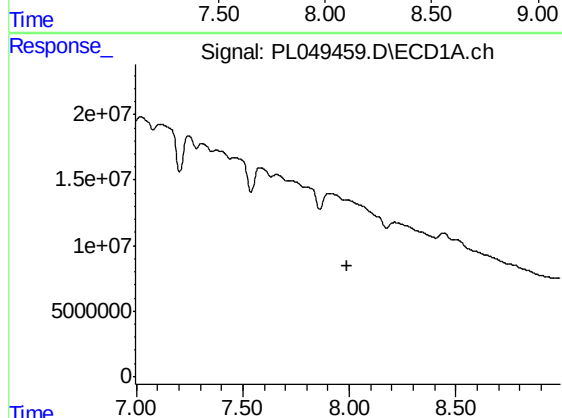

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.992 min
Response: 0
Conc: N.D.

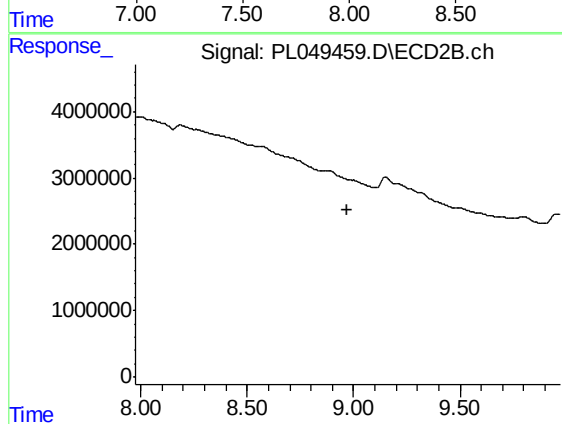

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.972 min
Response: 0
Conc: N.D.