

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061319\
 Data File : PL049478.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2019 17:06
 Operator : SM\AJ
 Sample : K3294-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S2(0-5)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 01:04:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.325	3.936	227.8E6	60778567	20.673	21.038
28)	SA Decachlor...	7.992	8.974	191.5E6	57705873	15.061	17.279
Target Compounds							
3)	MA gamma-BHC...	4.041	0.000	9924582	0	0.586	N.D. #
5)	MB Aldrin	4.567f	5.403	315.8E6	31502497	18.497	8.562 #
6)	B beta-BHC	0.000	4.807f	0	2824691	N.D.	1.640 #
10)	B gamma-Chl...	5.225	0.000	14737561	0	0.923	N.D. #
12)	B 4,4'-DDE	5.434	6.265	13285603	3225546	0.849	0.983
14)	MA Endrin	0.000	6.625	0	1222464	N.D.	0.410 #
15)	B Endosulfa...	0.000	6.816f	0	1082470	N.D.	0.357 #
20)	A Methoxychlor	6.704f	0.000	8225527	0	1.282	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061319\
Data File : PL049478.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2019 17:06
Operator : SM\AJ
Sample : K3294-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
S2(0-5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 01:04:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

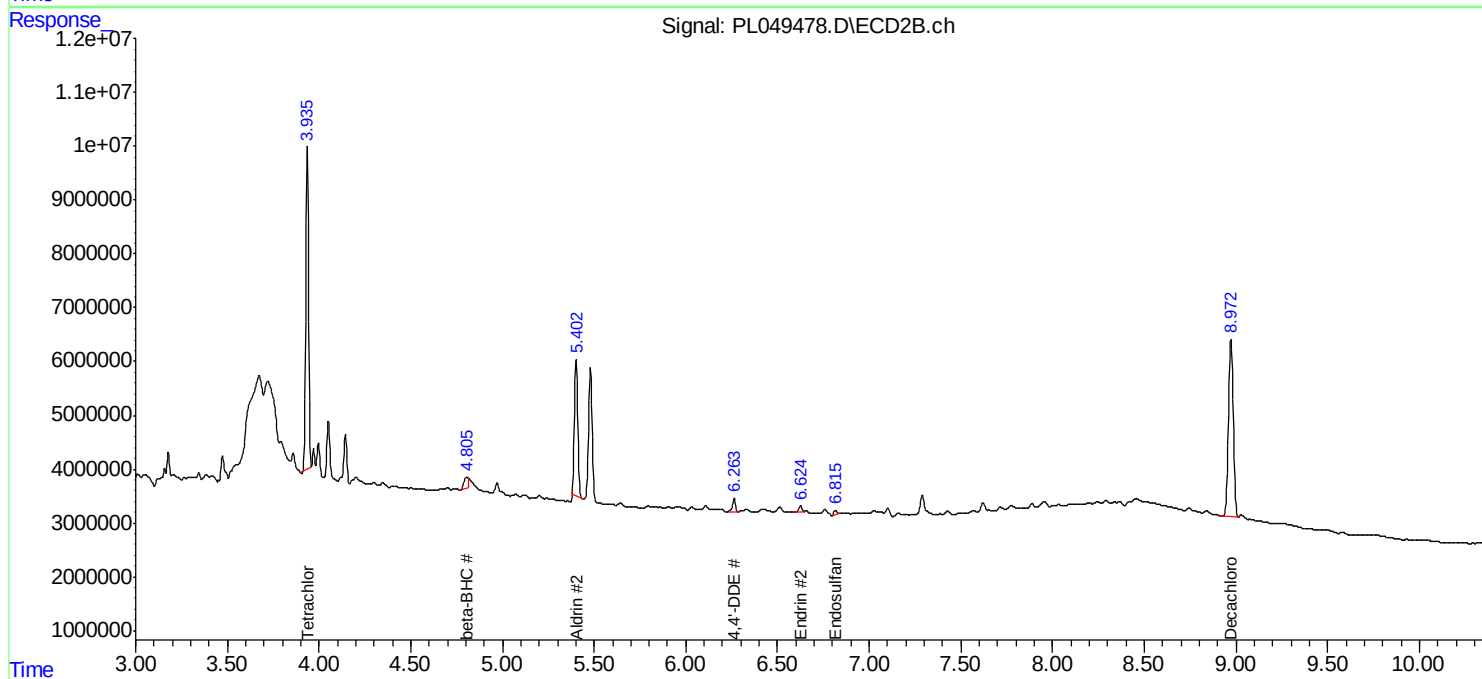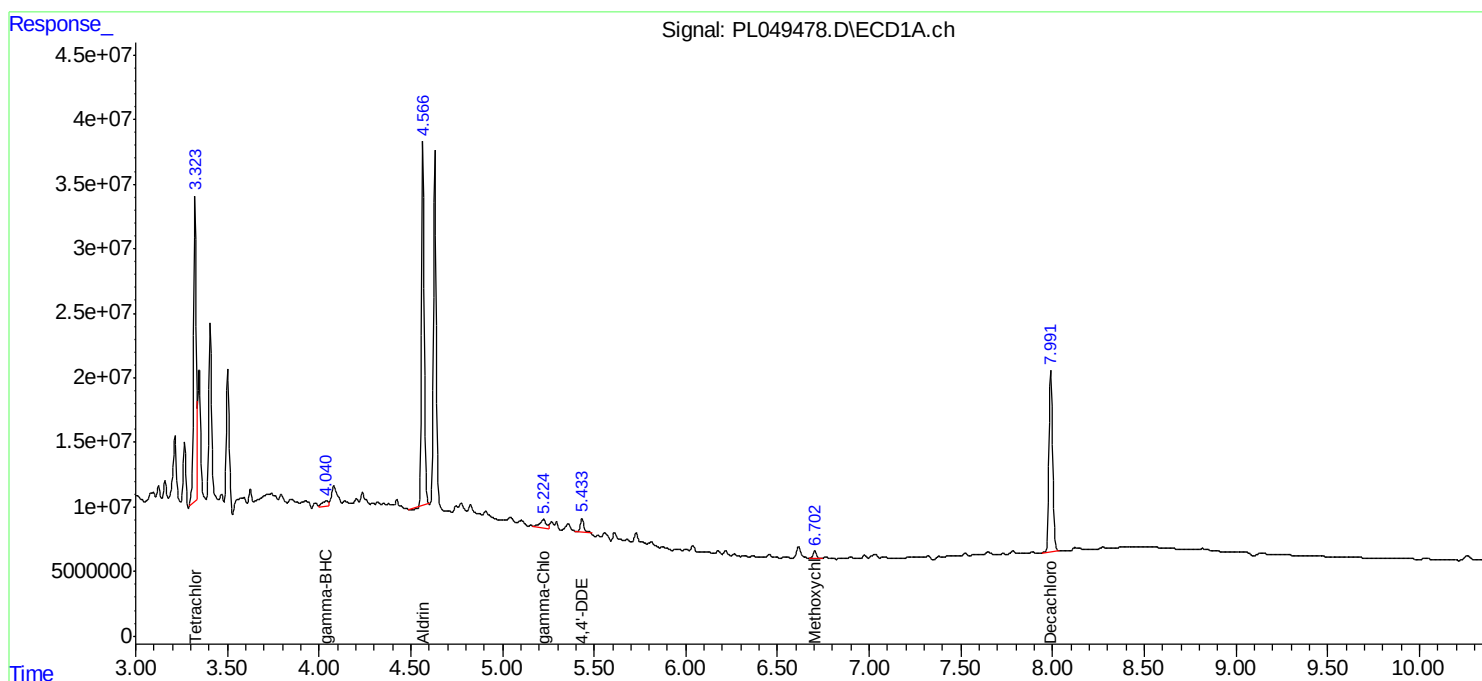


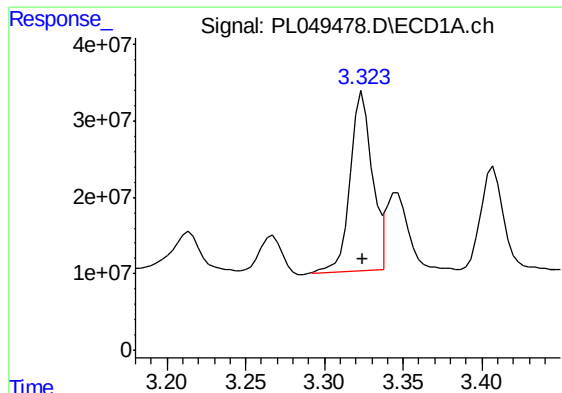

#1 Tetrachloro-m-xylene


R.T.: 3.325 min
Delta R.T.: 0.000 min
Response: 227794772
Conc: 20.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
S2(0-5)

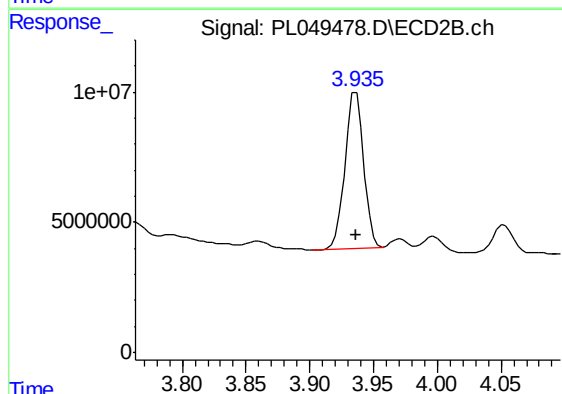


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 60778567
Conc: 21.04 ng/ml

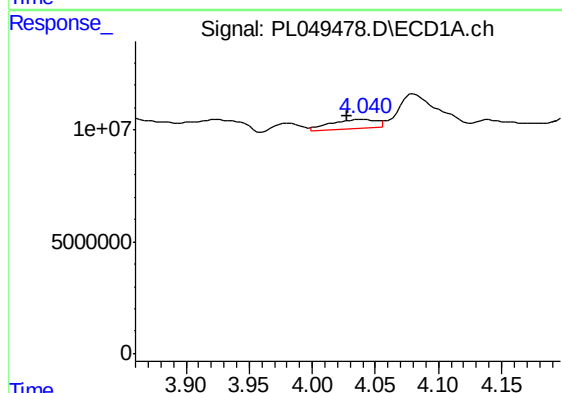


#3 gamma-BHC (Lindane)

R.T.: 4.041 min
Delta R.T.: 0.013 min
Response: 9924582
Conc: 0.59 ng/ml

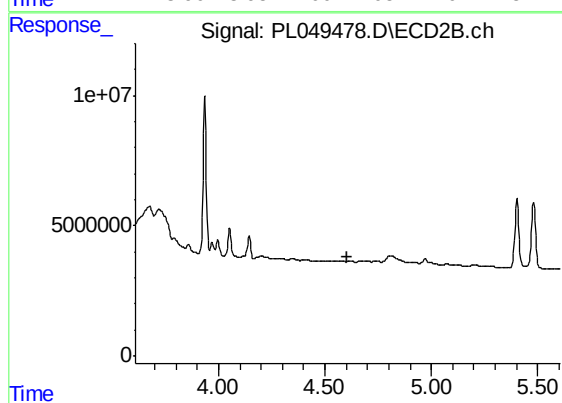

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.608 min
Response: 0
Conc: N.D.

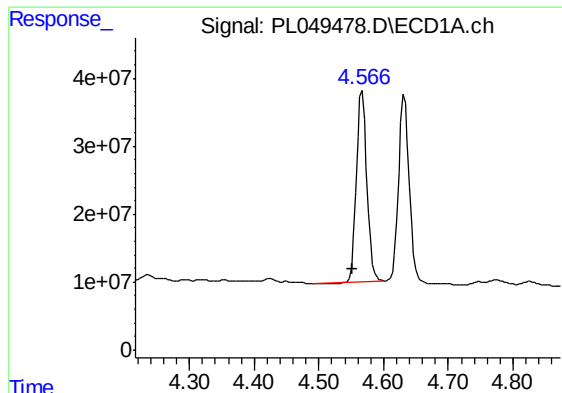

#5 Aldrin


R.T.: 4.567 min
Delta R.T.: 0.016 min
Response: 315827731
Conc: 18.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
S2(0-5)

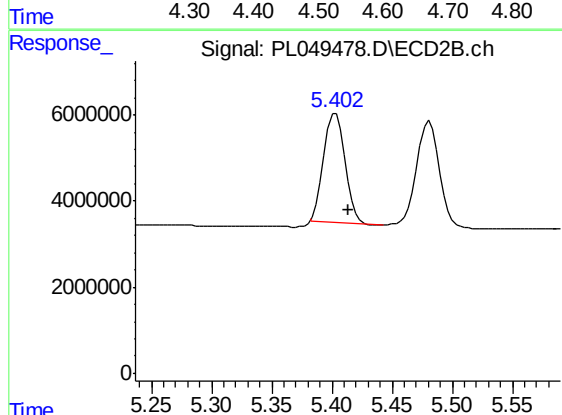


#5 Aldrin

R.T.: 5.403 min
Delta R.T.: -0.011 min
Response: 31502497
Conc: 8.56 ng/ml

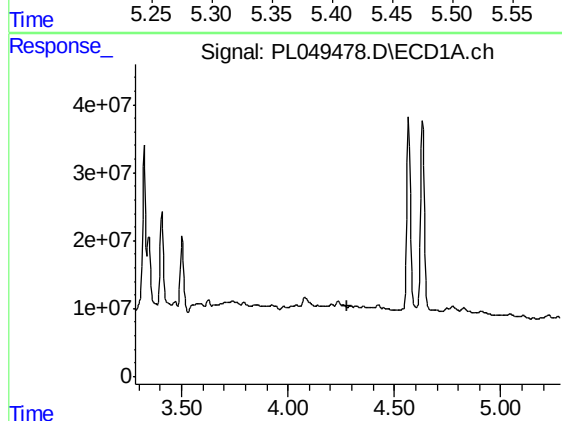


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.282 min
Response: 0
Conc: N.D.

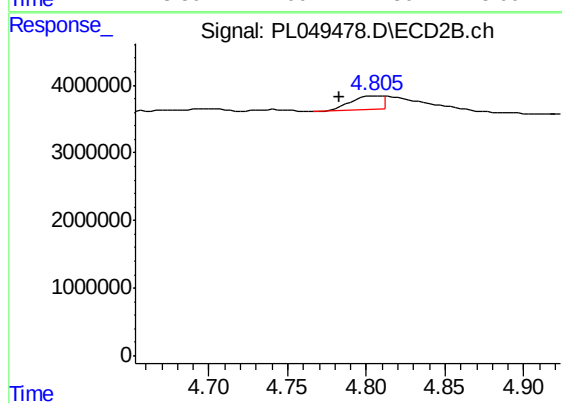

#6 beta-BHC


R.T.: 4.807 min
Delta R.T.: 0.024 min
Response: 2824691
Conc: 1.64 ng/ml

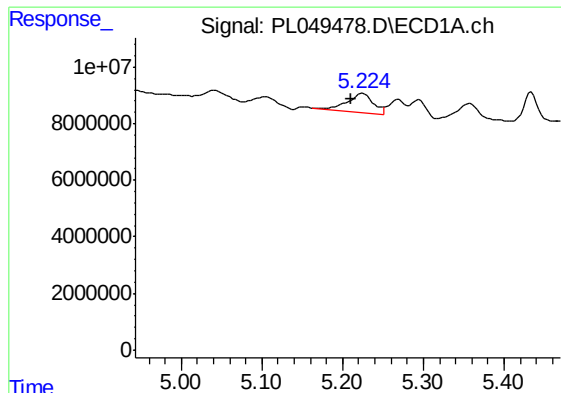

#10 gamma-Chlordane


R.T.: 5.225 min
Delta R.T.: 0.015 min
Response: 14737561
Conc: 0.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
S2(0-5)

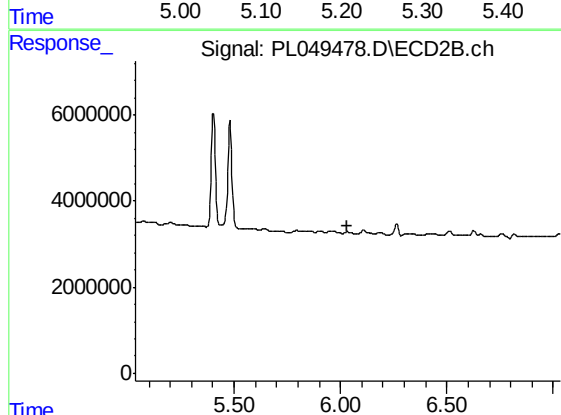


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.035 min
Response: 0
Conc: N.D.

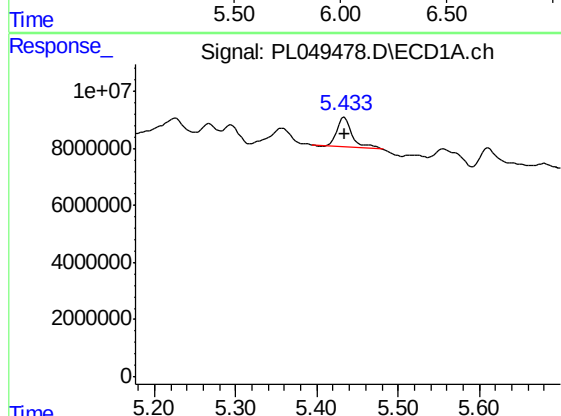


#12 4,4'-DDE

R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 13285603
Conc: 0.85 ng/ml

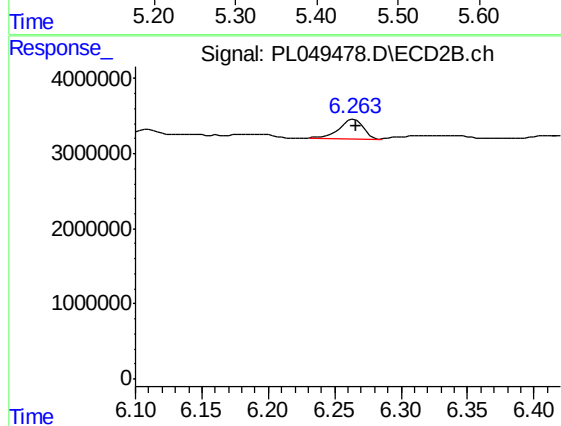

#12 4,4'-DDE


R.T.: 6.265 min
Delta R.T.: -0.002 min
Response: 3225546
Conc: 0.98 ng/ml

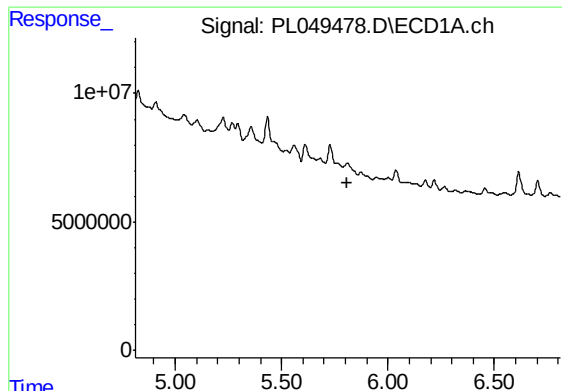

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 5.811 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S2(0-5)

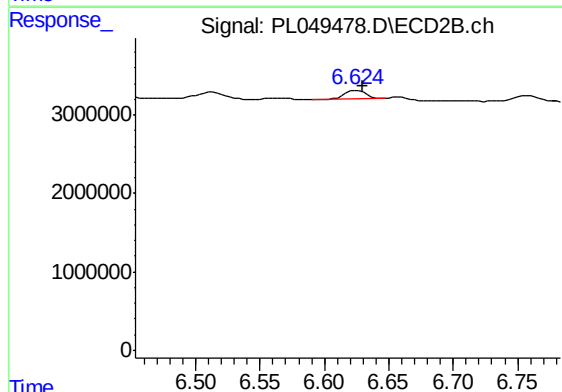


#14 Endrin

R.T.: 6.625 min
Delta R.T.: -0.004 min
Response: 1222464
Conc: 0.41 ng/ml

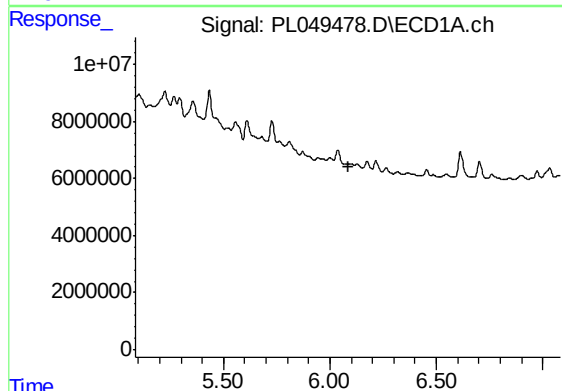


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.085 min
Response: 0
Conc: N.D.

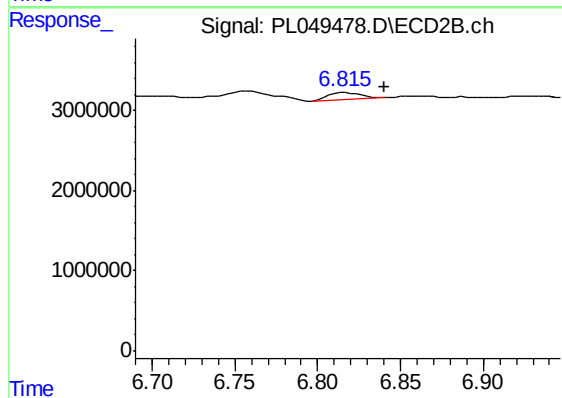

#15 Endosulfan II


R.T.: 6.816 min
Delta R.T.: -0.024 min
Response: 1082470
Conc: 0.36 ng/ml

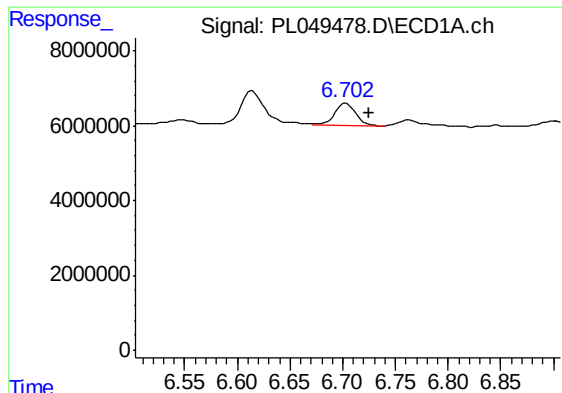

#20 Methoxychlor


R.T.: 6.704 min
Delta R.T.: -0.021 min
Response: 8225527
Conc: 1.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
S2(0-5)

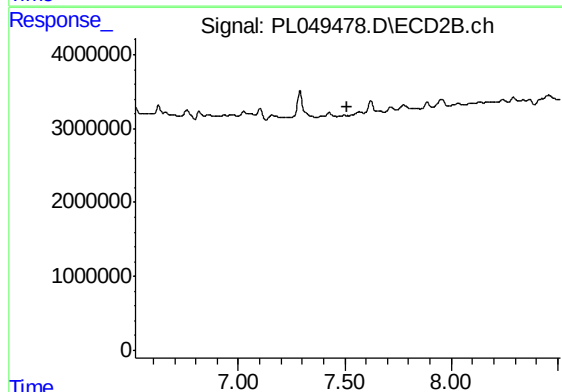


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.514 min
Response: 0
Conc: N.D.

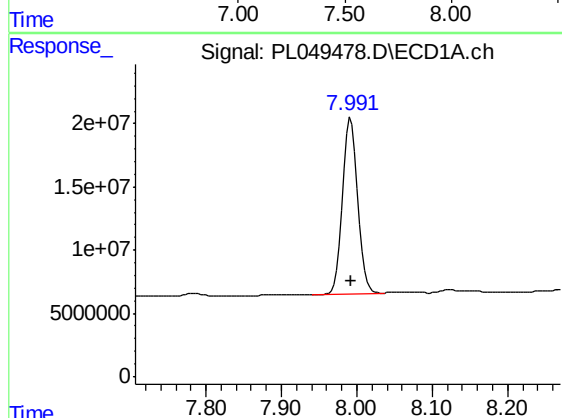

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: 0.000 min
Response: 191509649
Conc: 15.06 ng/ml

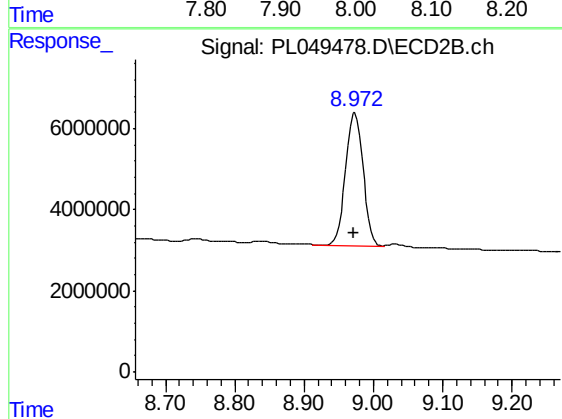

#28 Decachlorobiphenyl

R.T.: 8.974 min
Delta R.T.: 0.001 min
Response: 57705873
Conc: 17.28 ng/ml