

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061319\
 Data File : PL049466.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2019 11:39
 Operator : SM\AJ
 Sample : K3300-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TI-633-X

Manual Integrations
 APPROVED

Ankita
 6/14/2019 10:23:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 01:01:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.332	3.930	599.9E6	31386028	54.446m	10.864m#
28)	SA Decachlor...	7.991	8.972	75981178	16145555	5.975m	4.834m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061319\
Data File : PL049466.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2019 11:39
Operator : SM\AJ
Sample : K3300-02
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TI-633-X


Manual Integrations
APPROVED

Ankita
6/14/2019 10:23:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 01:01:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

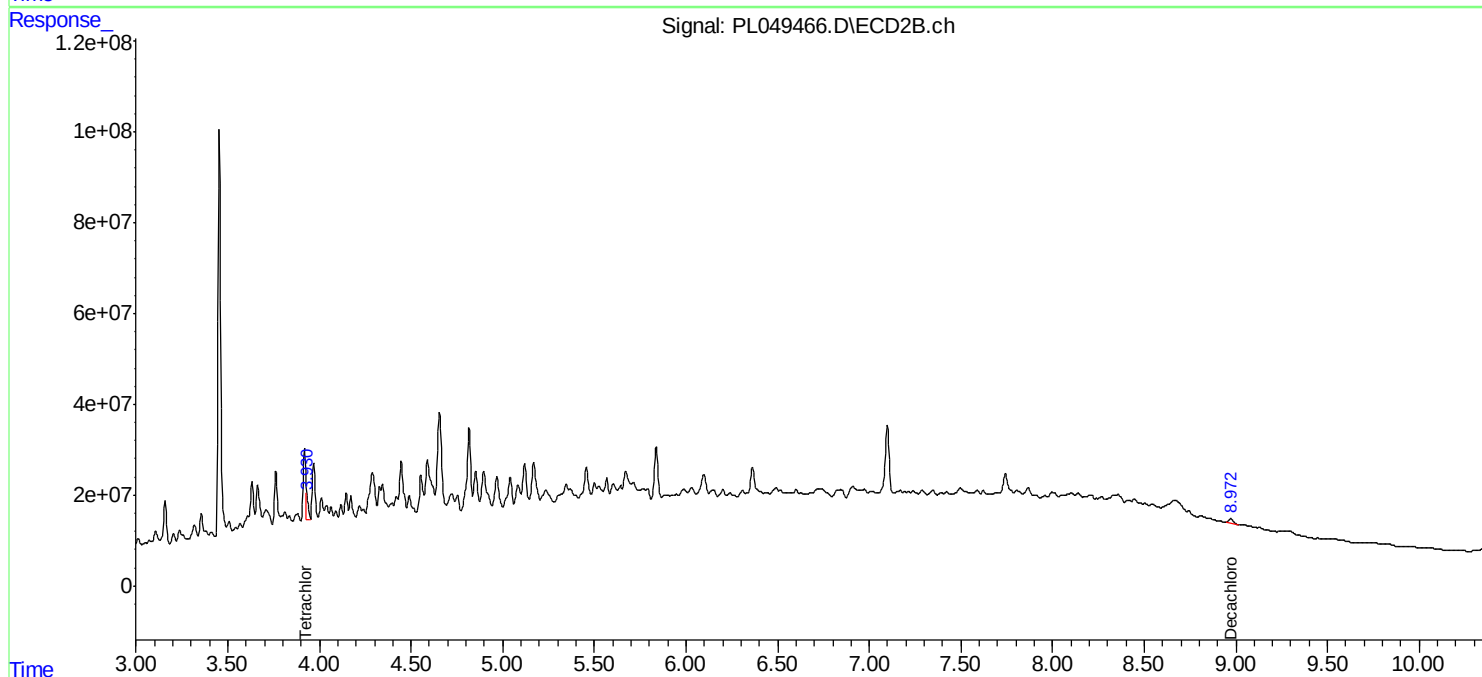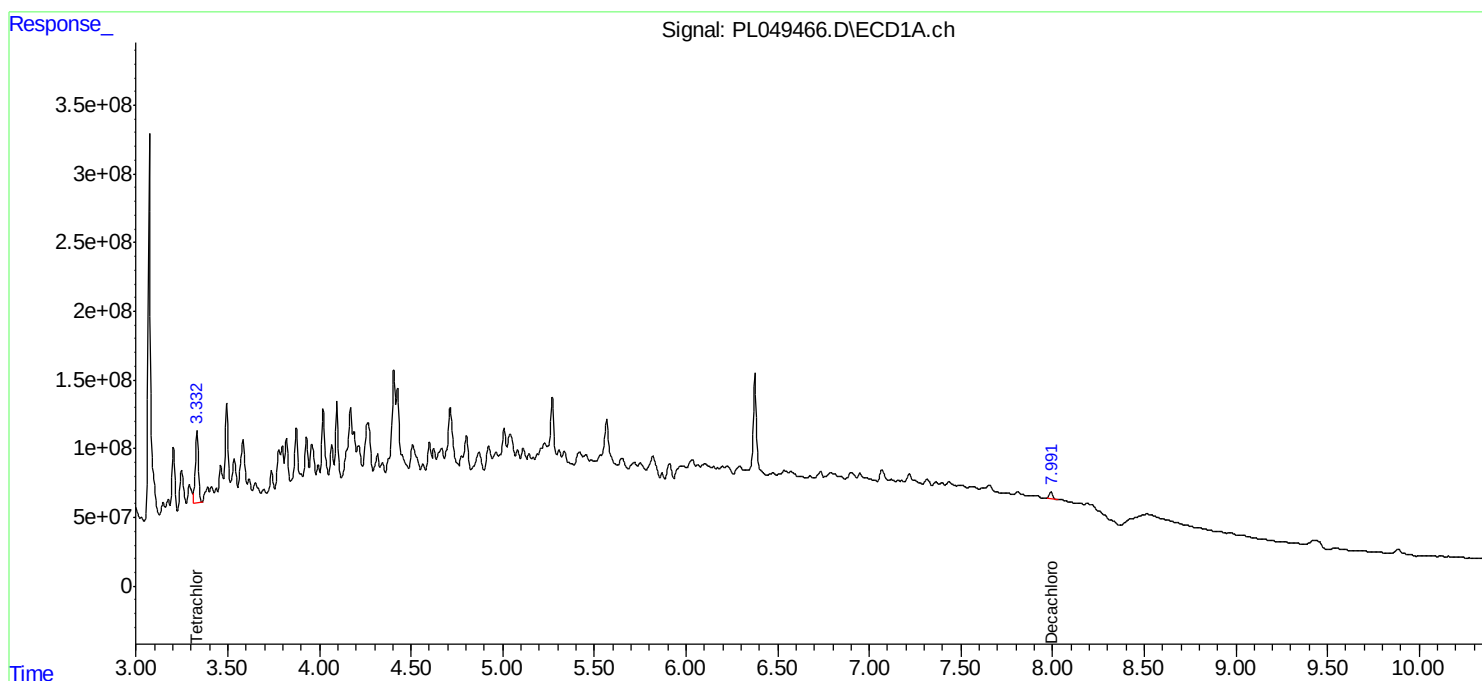

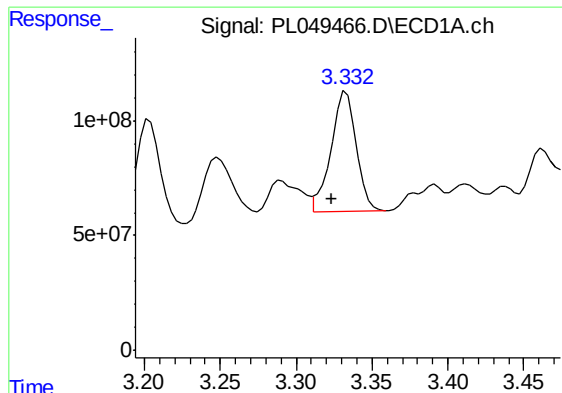


#1 Tetrachloro-m-xylene

R.T.: 3.332 min
Delta R.T.: 0.008 min
Response: 599928896
Conc: 54.45 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TI-633-X


Manual Integrations
APPROVED

Ankita
6/14/2019 10:23:46 AM

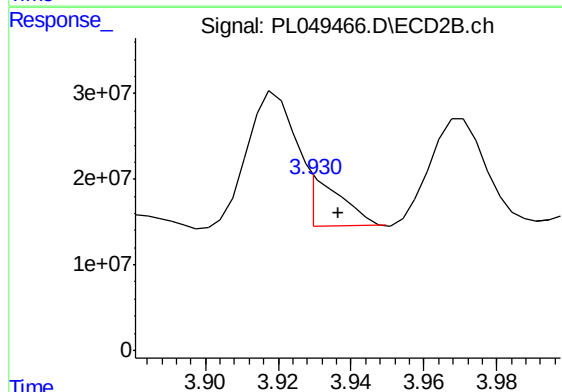


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: -0.007 min
Response: 31386028
Conc: 10.86 ng/ml m

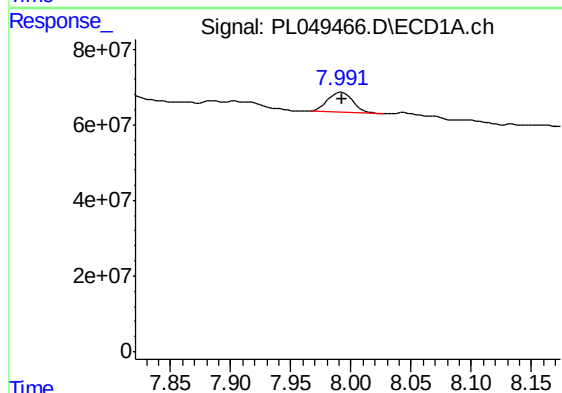

#28 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: -0.002 min
Response: 75981178
Conc: 5.98 ng/ml m

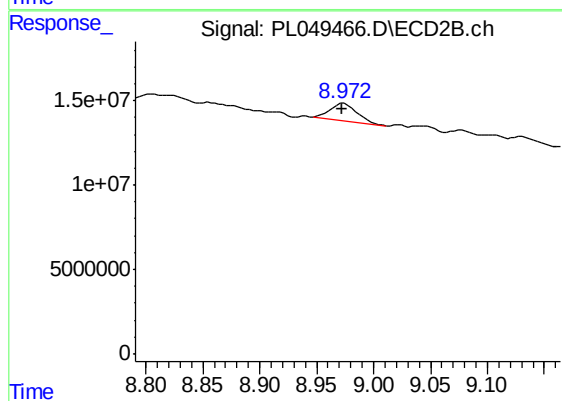

#28 Decachlorobiphenyl

R.T.: 8.972 min
Delta R.T.: 0.000 min
Response: 16145555
Conc: 4.83 ng/ml m