

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061322\
 Data File : PL075746.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2022 21:46
 Operator : AR\AJ
 Sample : N3304-05 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 23:23:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.642	4.638	614489	1729481	0.911	1.031
28)	SA Decachlor...	11.636	10.381	1070465	1752116	1.748	1.244 #
Target Compounds							
7)	B delta-BHC	0.000	6.404	0	678891	N.D.	0.317 #
12)	B 4,4'-DDE	0.000	7.623	0	261327	N.D.	0.163 #
14)	MA Endrin	0.000	8.039	0	983528	N.D.	0.719 #
15)	B Endosulfa...	9.307	0.000	278046	0	0.447	N.D. #
16)	A 4,4'-DDD	9.201	0.000	162336	0	0.297	N.D. #
17)	MA 4,4'-DDT	9.491f	8.461	139968	486486	0.219	0.346 #
19)	B Endosulfa...	0.000	8.768	0	259000	N.D.	0.176 #
21)	B Endrin ke...	10.186f	0.000	954646	0	1.358	N.D. #
27)	Chlordane-5	0.000	8.121	0	411727	N.D.	8.672 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061322\
Data File : PL075746.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2022 21:46
Operator : AR\AJ
Sample : N3304-05 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 23:23:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

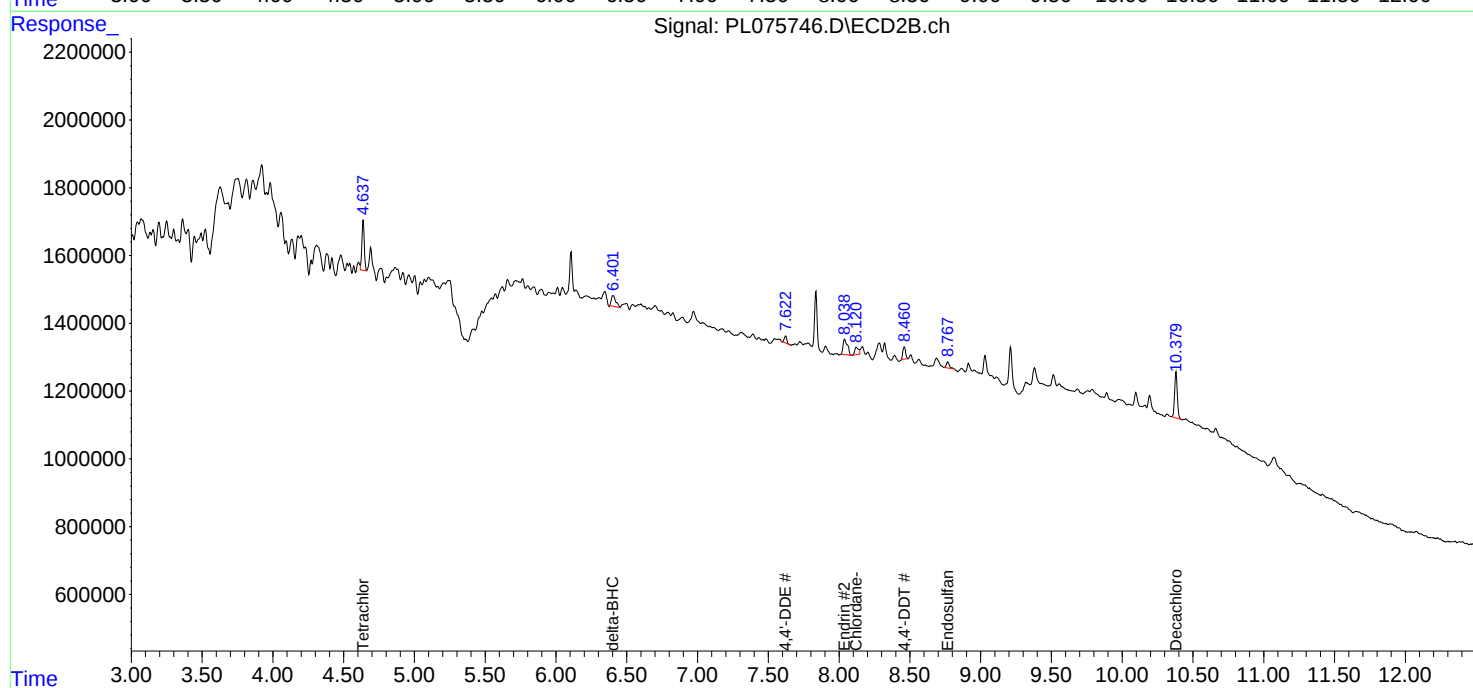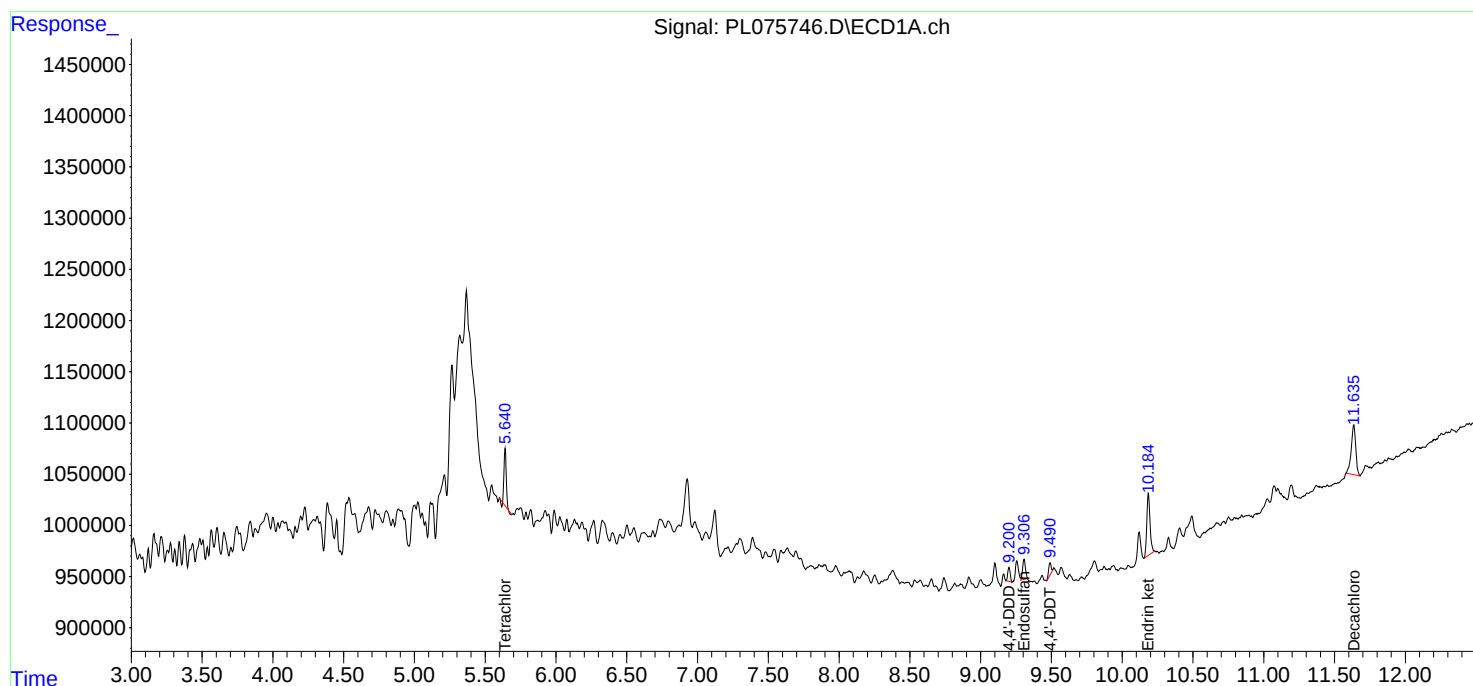


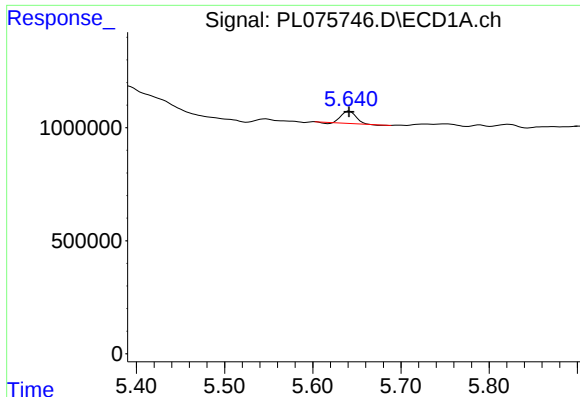

#1 Tetrachloro-m-xylene


R.T.: 5.642 min
Delta R.T.: 0.000 min
Response: 614489
Conc: 0.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

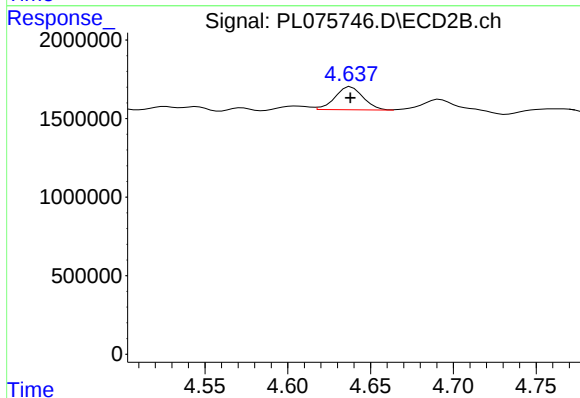


#1 Tetrachloro-m-xylene

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 1729481
Conc: 1.03 ng/ml

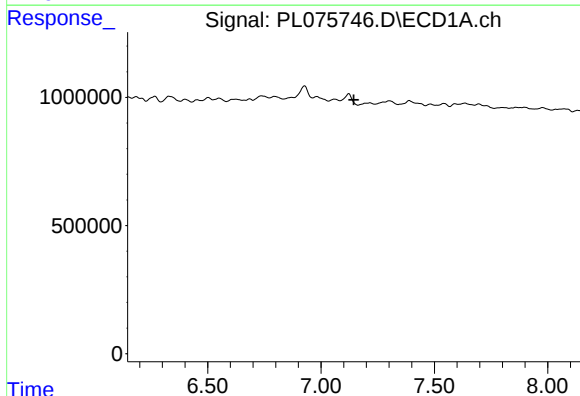


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

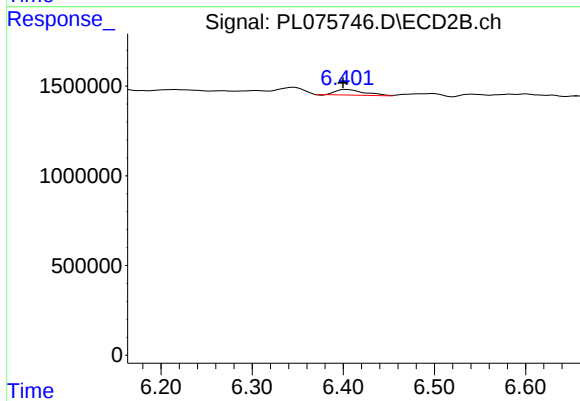

#7 delta-BHC


R.T.: 6.404 min
Delta R.T.: 0.004 min
Response: 678891
Conc: 0.32 ng/ml

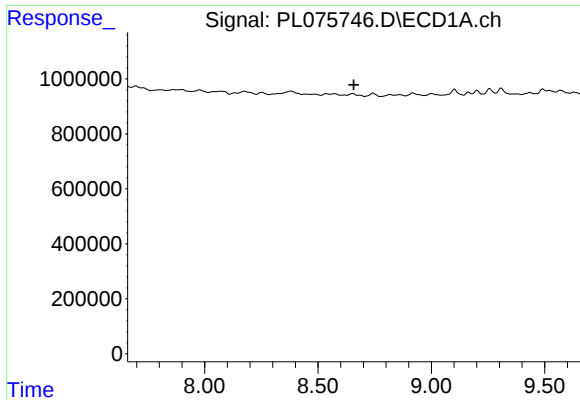

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 8.658 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

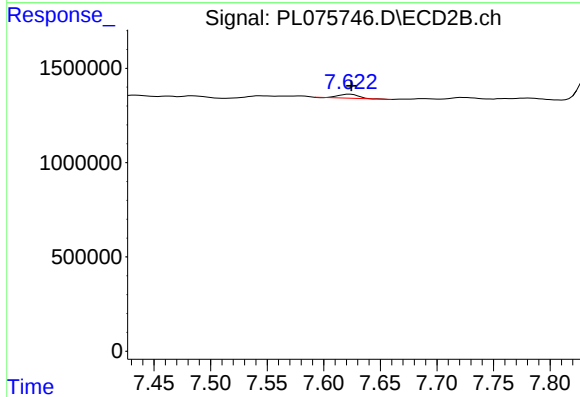


#12 4,4'-DDE

R.T.: 7.623 min
Delta R.T.: -0.001 min
Response: 261327
Conc: 0.16 ng/ml

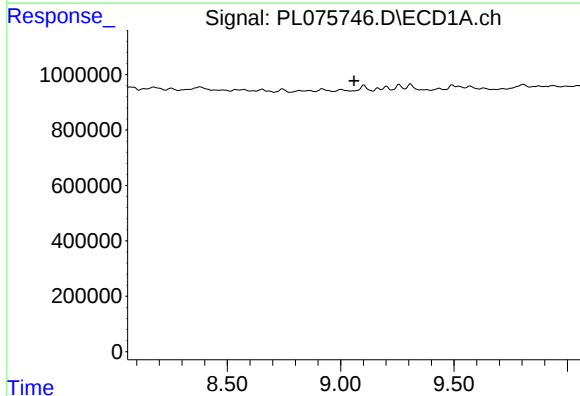


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.059 min
Response: 0
Conc: N.D.

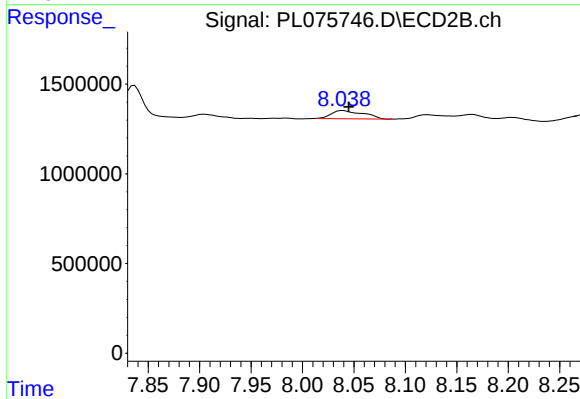

#14 Endrin


R.T.: 8.039 min
Delta R.T.: -0.006 min
Response: 983528
Conc: 0.72 ng/ml

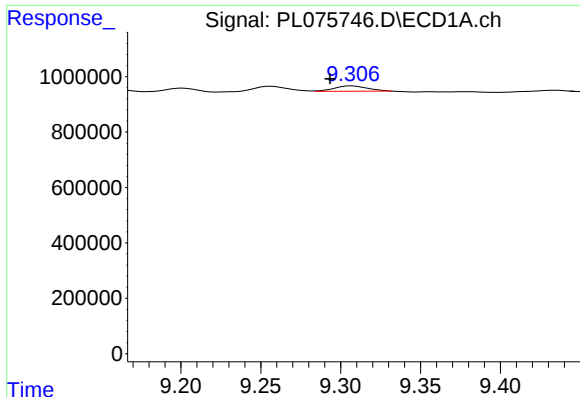

#15 Endosulfan II


R.T.: 9.307 min
Delta R.T.: 0.014 min
Response: 278046
Conc: 0.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

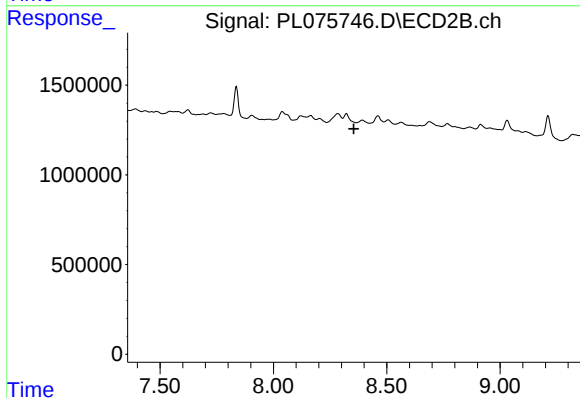


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

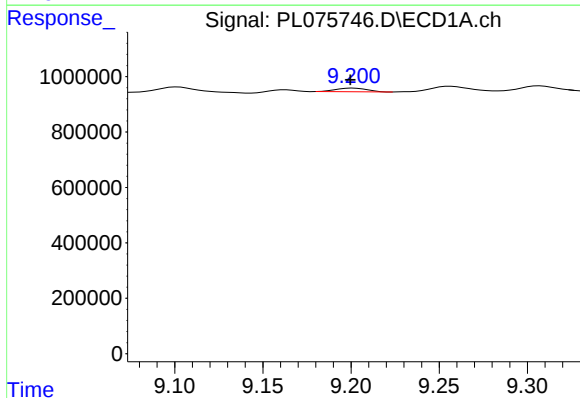


#16 4,4'-DDD

R.T.: 9.201 min
Delta R.T.: 0.002 min
Response: 162336
Conc: 0.30 ng/ml

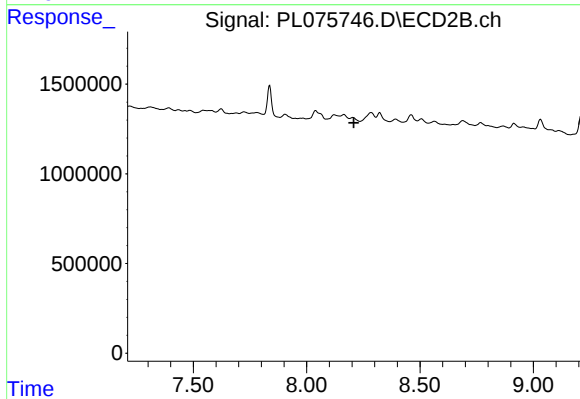

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 8.208 min
Response: 0
Conc: N.D.

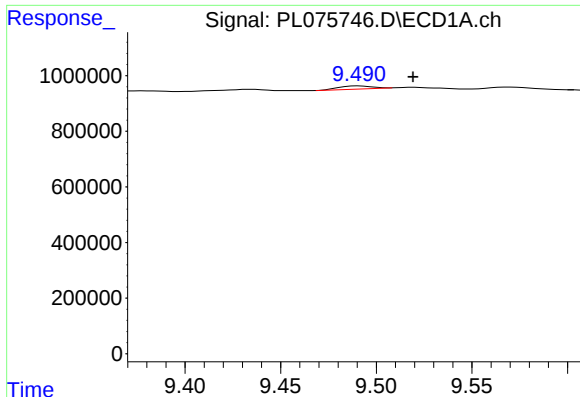

#17 4,4'-DDT


R.T.: 9.491 min
Delta R.T.: -0.028 min
Response: 139968
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

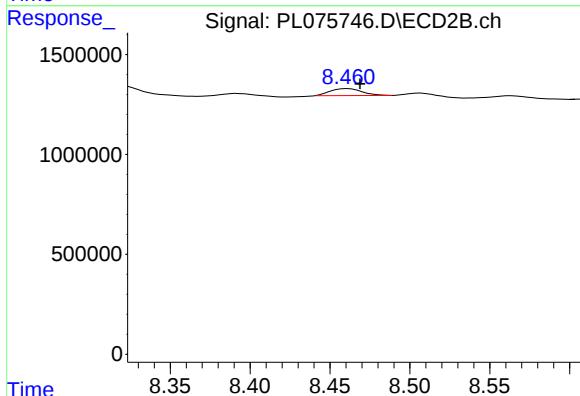


#17 4,4'-DDT

R.T.: 8.461 min
Delta R.T.: -0.008 min
Response: 486486
Conc: 0.35 ng/ml

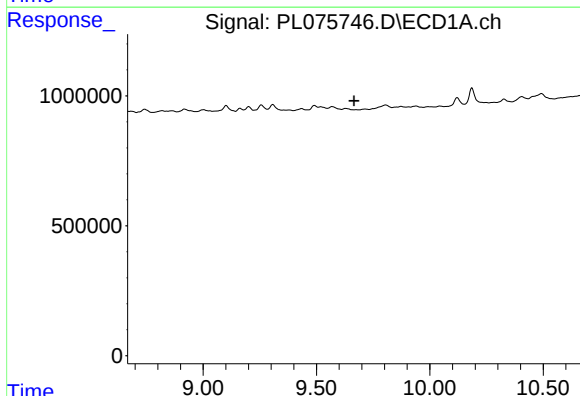


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 9.666 min
Response: 0
Conc: N.D.

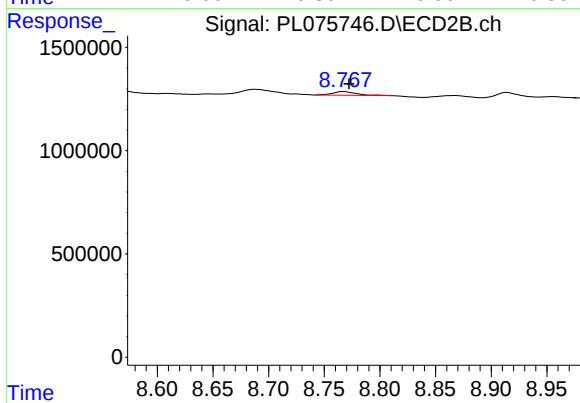

#19 Endosulfan Sulfate


R.T.: 8.768 min
Delta R.T.: -0.004 min
Response: 259000
Conc: 0.18 ng/ml

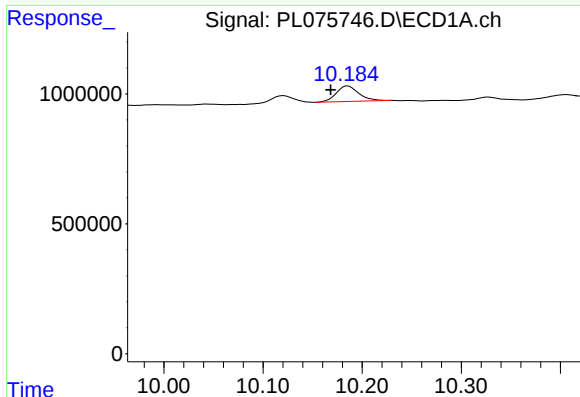

#21 Endrin ketone


R.T.: 10.186 min
Delta R.T.: 0.017 min
Response: 954646
Conc: 1.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

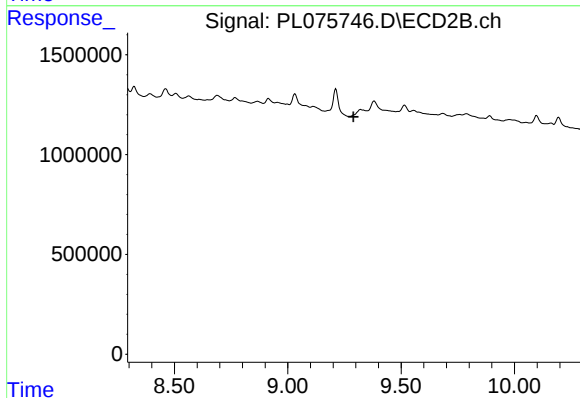


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

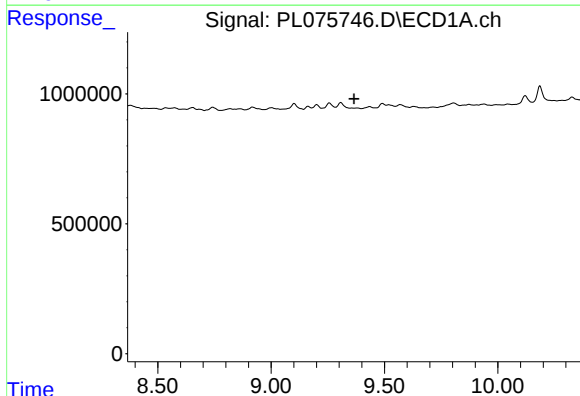


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.366 min
Response: 0
Conc: N.D.

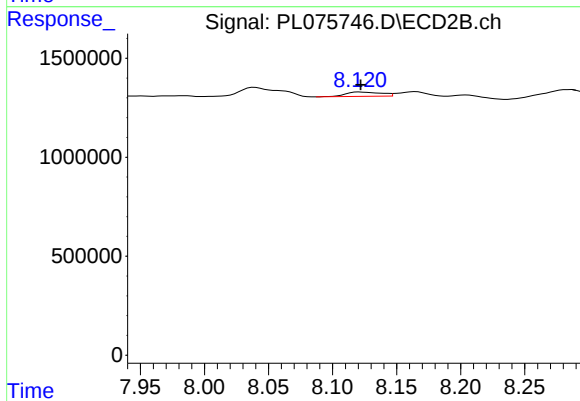

#27 Chlordane-5


R.T.: 8.121 min
Delta R.T.: 0.000 min
Response: 411727
Conc: 8.67 ng/ml

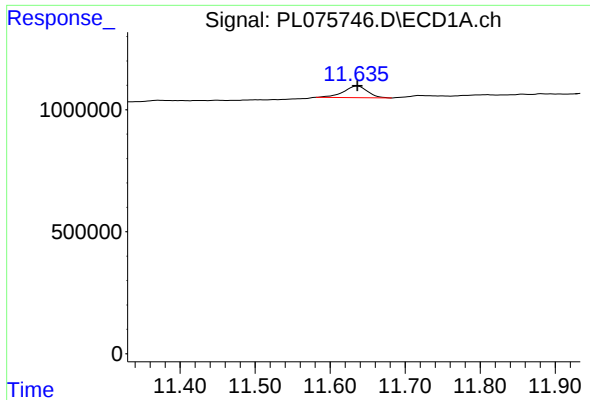

#28 Decachlorobiphenyl

R.T.: 11.636 min
Delta R.T.: 0.000 min
Response: 1070465
Conc: 1.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

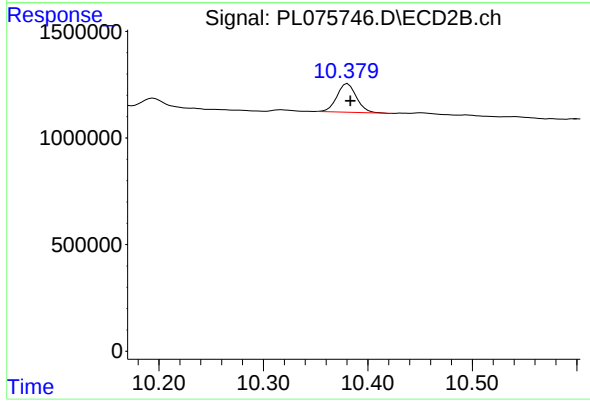

#28 Decachlorobiphenyl

R.T.: 10.381 min
Delta R.T.: -0.002 min
Response: 1752116
Conc: 1.24 ng/ml