

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061323\
 Data File : PL083398.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2023 15:48
 Operator : AR\AJ
 Sample : 03154-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CHRT-24051

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/14/2023
 Supervised By : Ankita Jodhani 06/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 21:28:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.324	2.630	9143180	7561052	3.111	2.912m
28) SA Decachlor...	8.743	7.739	9275854	11095813	4.423	4.462

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061323\
Data File : PL083398.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2023 15:48
Operator : AR\AJ
Sample : 03154-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CHRT-24051


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/14/2023
Supervised By : Ankita Jodhani 06/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 21:28:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

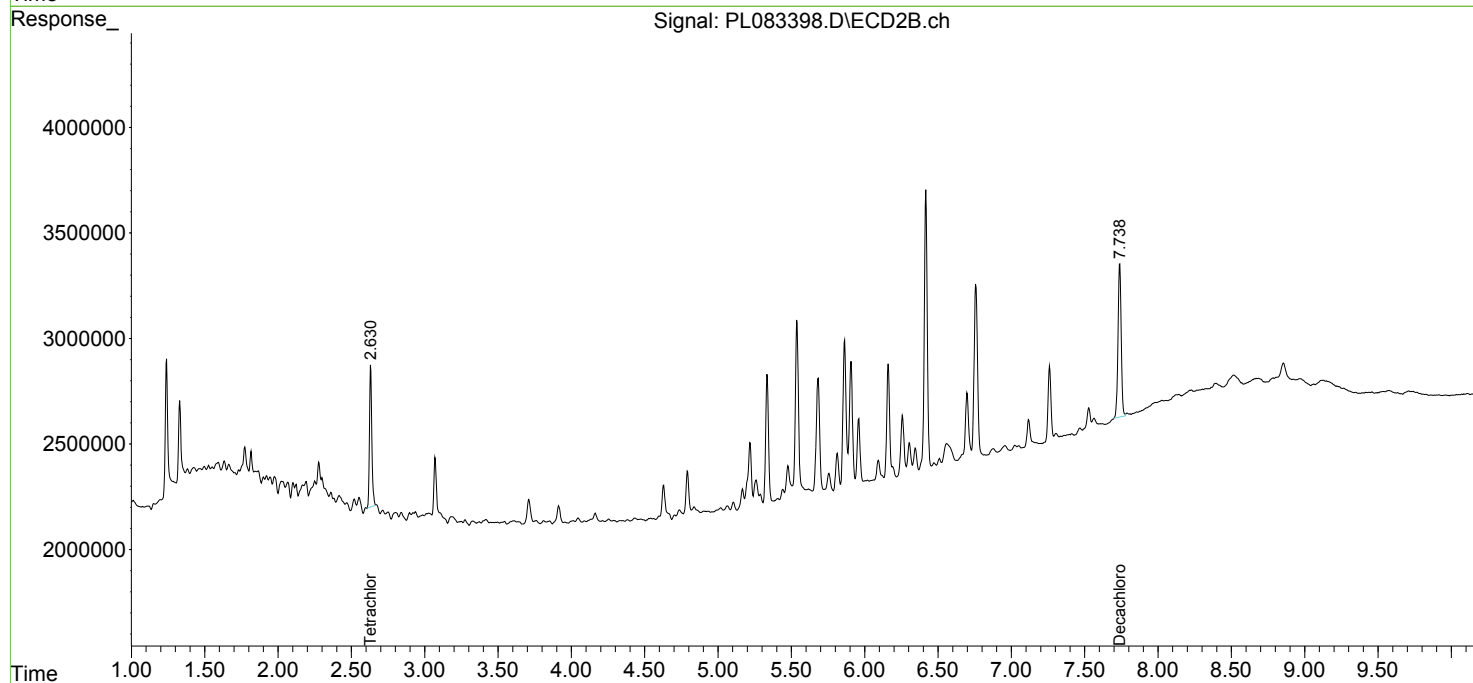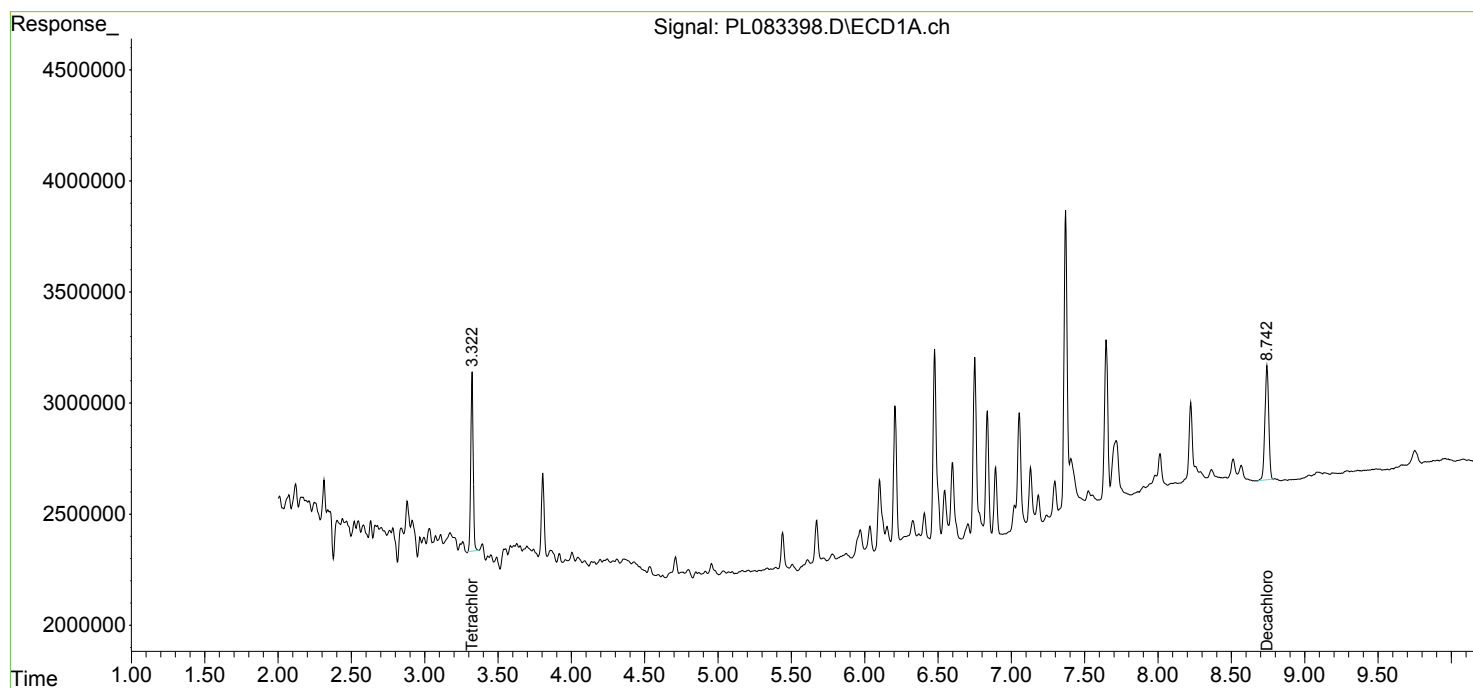

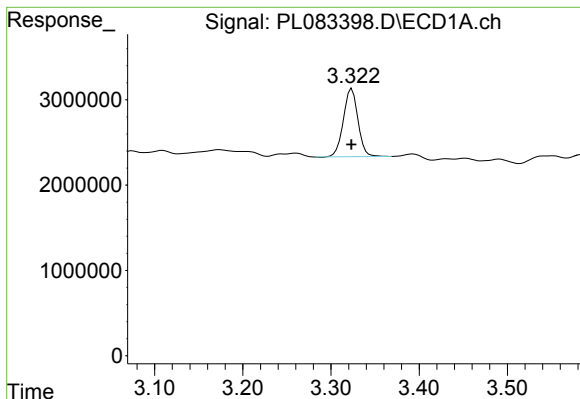


#1 Tetrachloro-m-xylene

R.T.: 3.324 min
Delta R.T.: 0.000 min
Response: 9143180
Conc: 3.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-24051


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/14/2023
Supervised By :Ankita Jodhani 06/14/2023

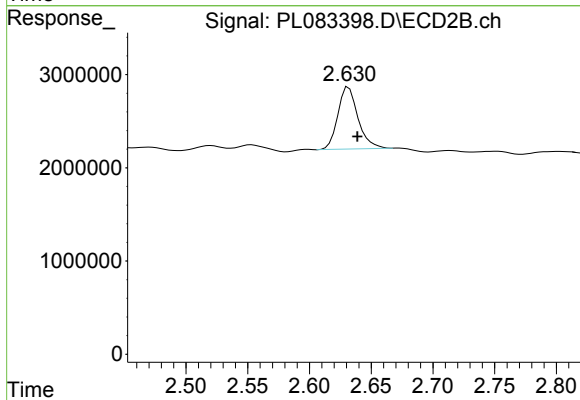


#1 Tetrachloro-m-xylene

R.T.: 2.630 min
Delta R.T.: -0.009 min
Response: 7561052
Conc: 2.91 ng/ml m

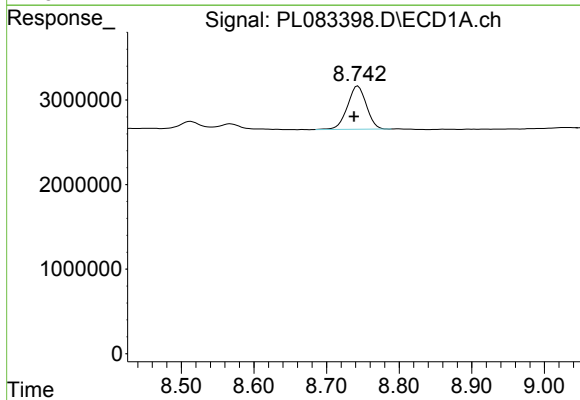

#28 Decachlorobiphenyl

R.T.: 8.743 min
Delta R.T.: 0.005 min
Response: 9275854
Conc: 4.42 ng/ml

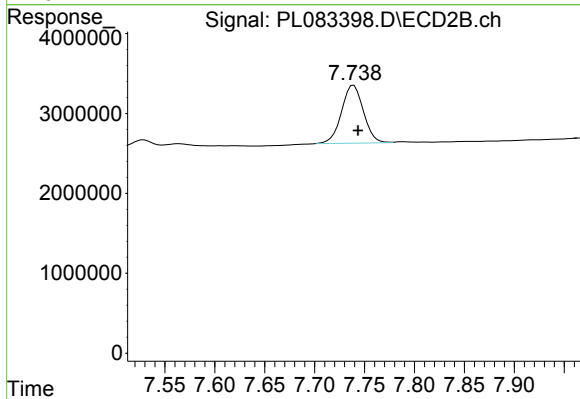

#28 Decachlorobiphenyl

R.T.: 7.739 min
Delta R.T.: -0.004 min
Response: 11095813
Conc: 4.46 ng/ml