

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061325\
 Data File : PL096048.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2025 14:02
 Operator : AR\AJ
 Sample : Q2308-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 22:32:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061125.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 11 14:04:36 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.571	2.883	35426312	48877939	10.902	12.043
28)	SA Decachlor...	9.114	8.065	31527336	39145180	12.897	8.233 #
Target Compounds							
9)	A Endosulfan I	0.000	5.249	0	6284924	N.D.	1.136 #
16)	A 4,4'-DDD	0.000	5.908f	0	9960049	N.D.	2.176 #
23)	Chlordane-1	0.000	3.894	0	11489180	N.D.	58.127 #
24)	Chlordane-2	0.000	4.510f	0	11063311	N.D.	50.551 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061325\
Data File : PL096048.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2025 14:02
Operator : AR\AJ
Sample : Q2308-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 22:32:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061125.M
Quant Title : GC Extractables
QLast Update : Wed Jun 11 14:04:36 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

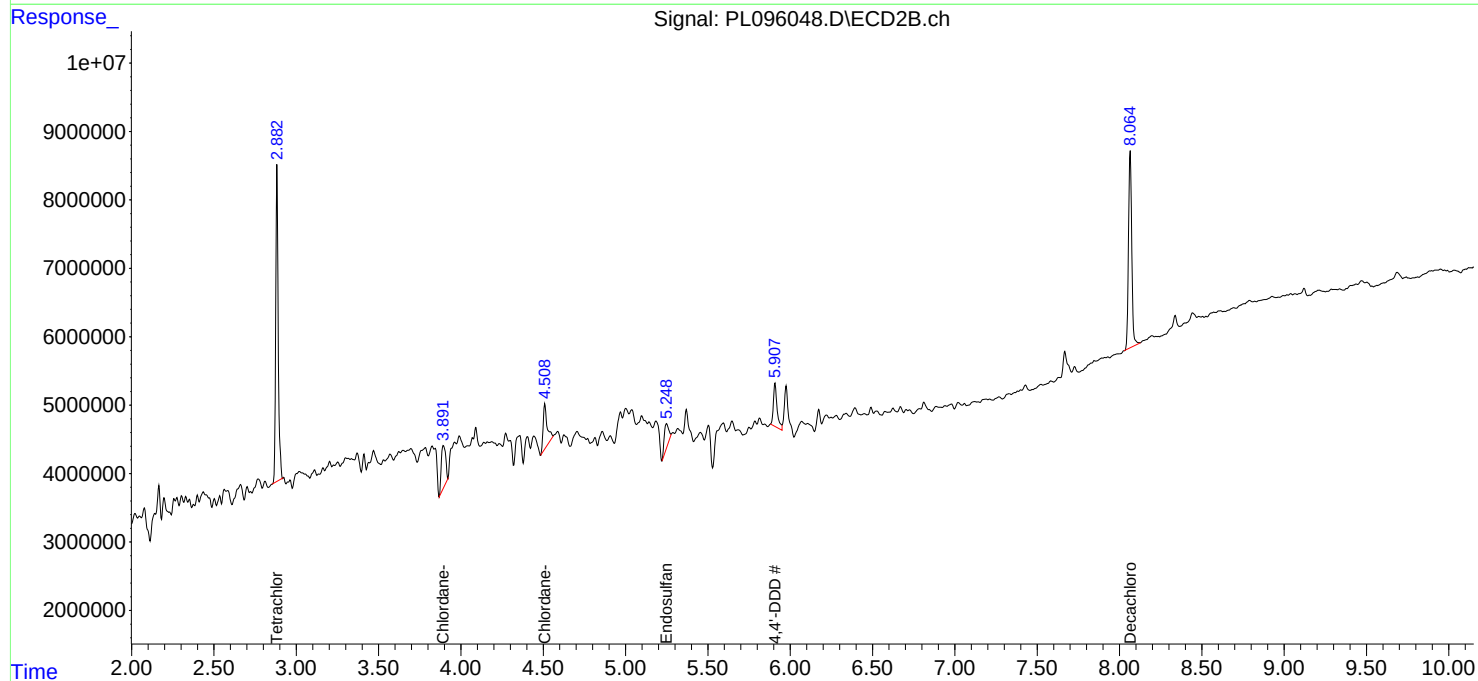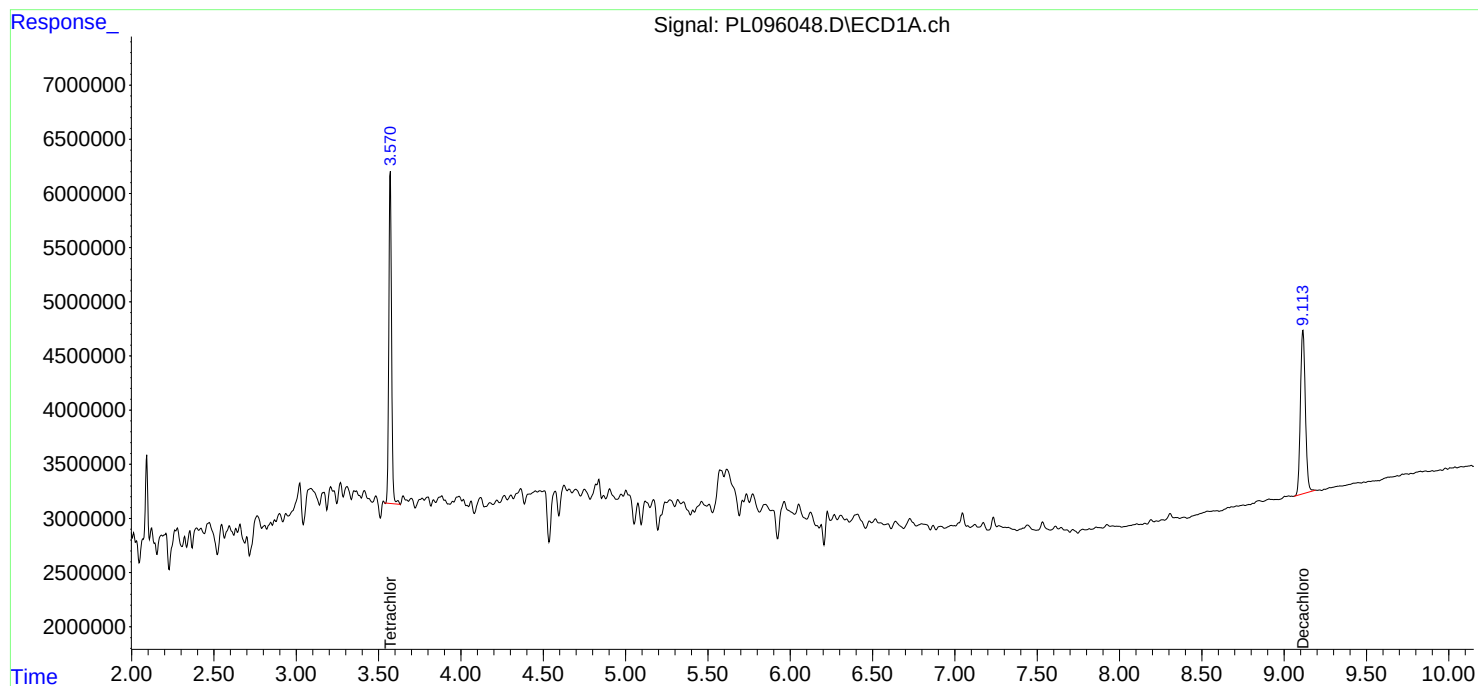


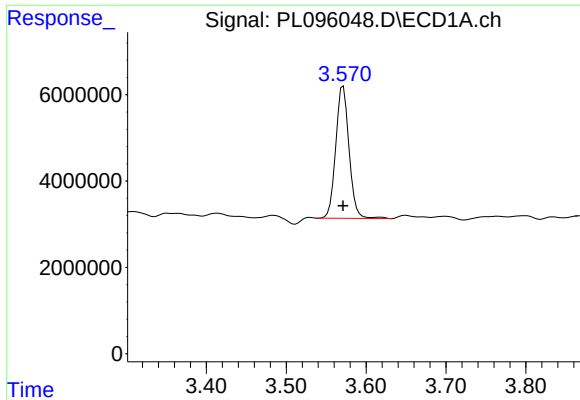

#1 Tetrachloro-m-xylene


R.T.: 3.571 min
Delta R.T.: 0.000 min
Response: 35426312
Conc: 10.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

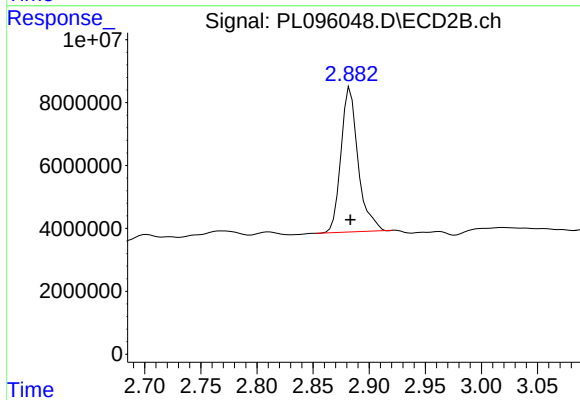


#1 Tetrachloro-m-xylene

R.T.: 2.883 min
Delta R.T.: 0.000 min
Response: 48877939
Conc: 12.04 ng/ml

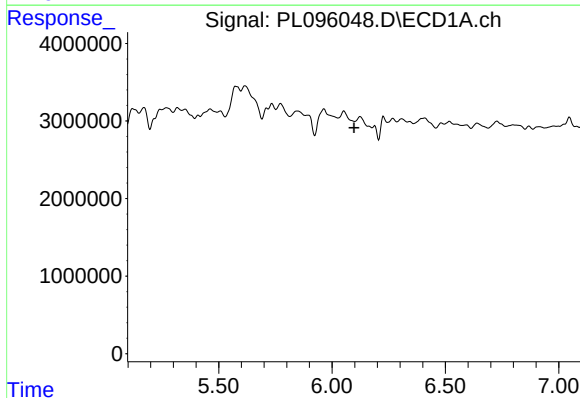


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

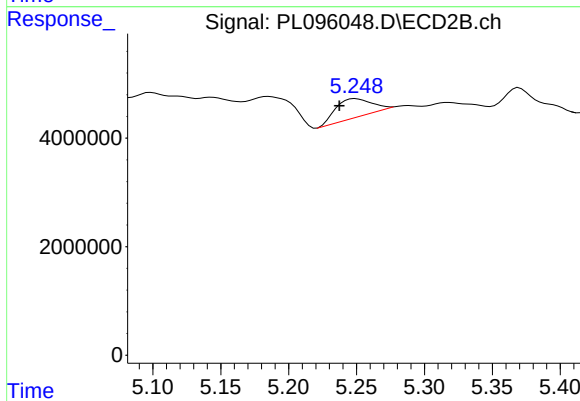

#9 Endosulfan I


R.T.: 5.249 min
Delta R.T.: 0.012 min
Response: 6284924
Conc: 1.14 ng/ml

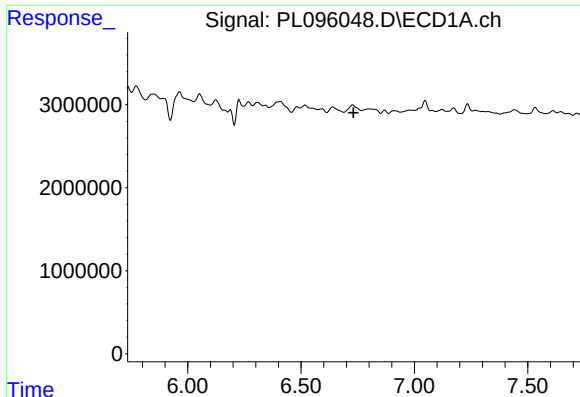

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.732 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

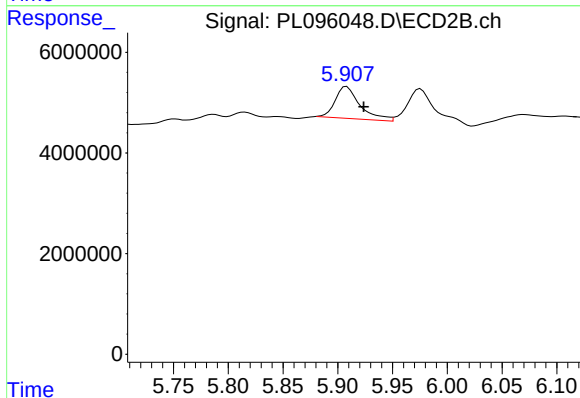


#16 4,4'-DDD

R.T.: 5.908 min
Delta R.T.: -0.016 min
Response: 9960049
Conc: 2.18 ng/ml

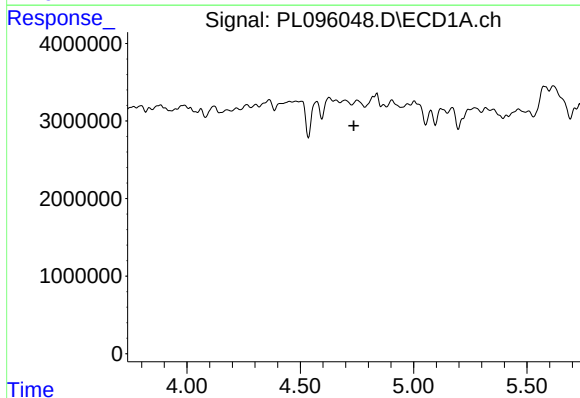


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.737 min
Response: 0
Conc: N.D.

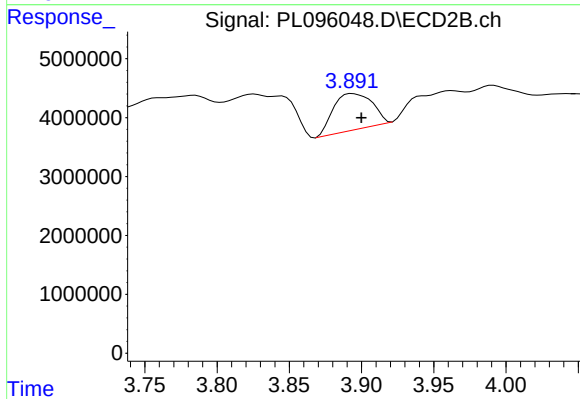

#23 Chlordane-1


R.T.: 3.894 min
Delta R.T.: -0.006 min
Response: 11489180
Conc: 58.13 ng/ml

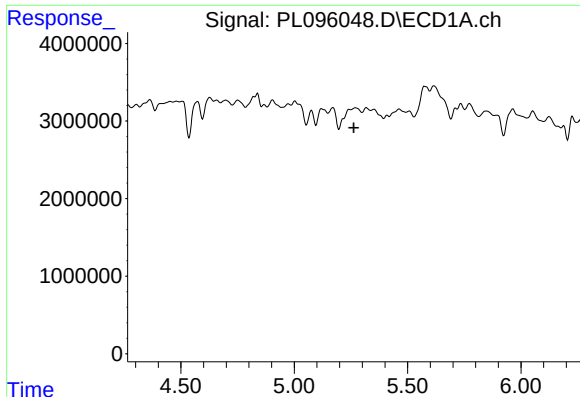

#24 Chloroform-2


R.T.: 0.000 min
Exp R.T.: 5.263 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

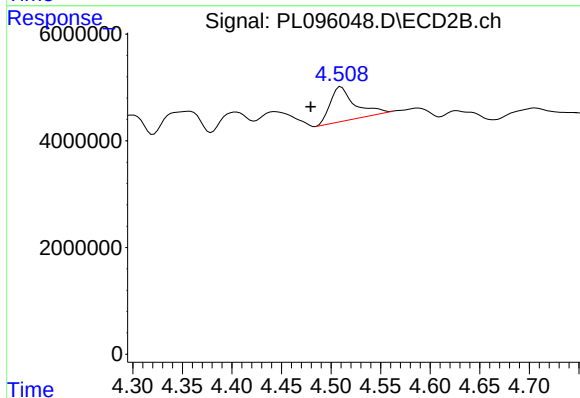


#24 Chloroform-2

R.T.: 4.510 min
Delta R.T.: 0.030 min
Response: 11063311
Conc: 50.55 ng/ml

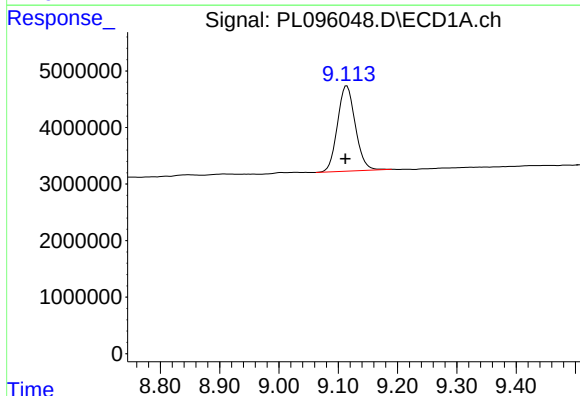

#28 Decachlorobiphenyl

R.T.: 9.114 min
Delta R.T.: 0.002 min
Response: 31527336
Conc: 12.90 ng/ml

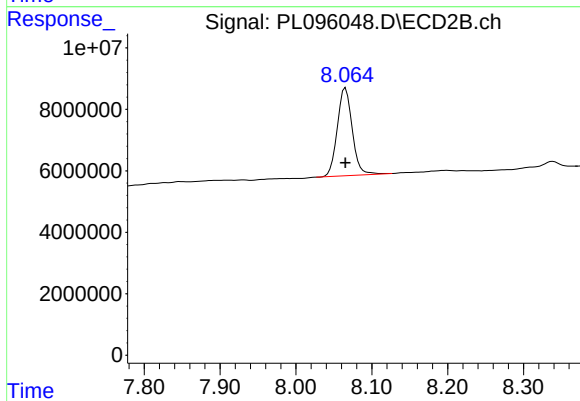

#28 Decachlorobiphenyl

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 39145180
Conc: 8.23 ng/ml