

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
 Data File : PL036918.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2018 15:06
 Operator : UA\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 15:37:14 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 14 15:36:33 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.341	3.938	374.1E6	130.2E6	50.000	50.000
28)	SA Decachlor...	8.026	8.950	319.3E6	123.5E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.187	4.922	145.3E6	57176831	500.000	500.000
24)	Chlordane-2	4.681	5.385	157.9E6	59668906	500.000	500.000
25)	Chlordane-3	5.237	6.024	492.2E6	192.5E6	500.000	500.000
26)	Chlordane-4	5.294	6.100	440.0E6	229.6E6	500.000	500.000
27)	Chlordane-5	5.902	6.892	64639101	44165484	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
Data File : PL036918.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2018 15:06
Operator : UA\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 15:37:14 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
Quant Title : GC Extractables
QLast Update : Thu Jun 14 15:36:33 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

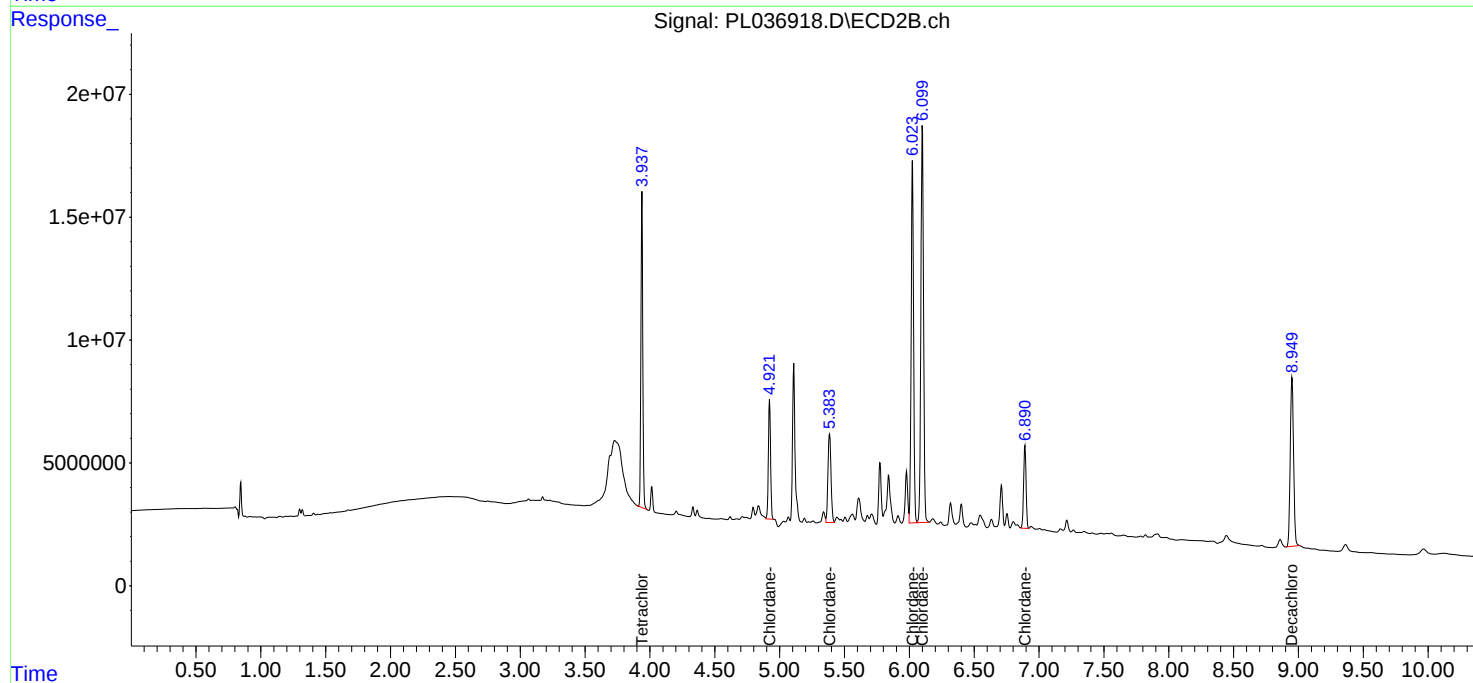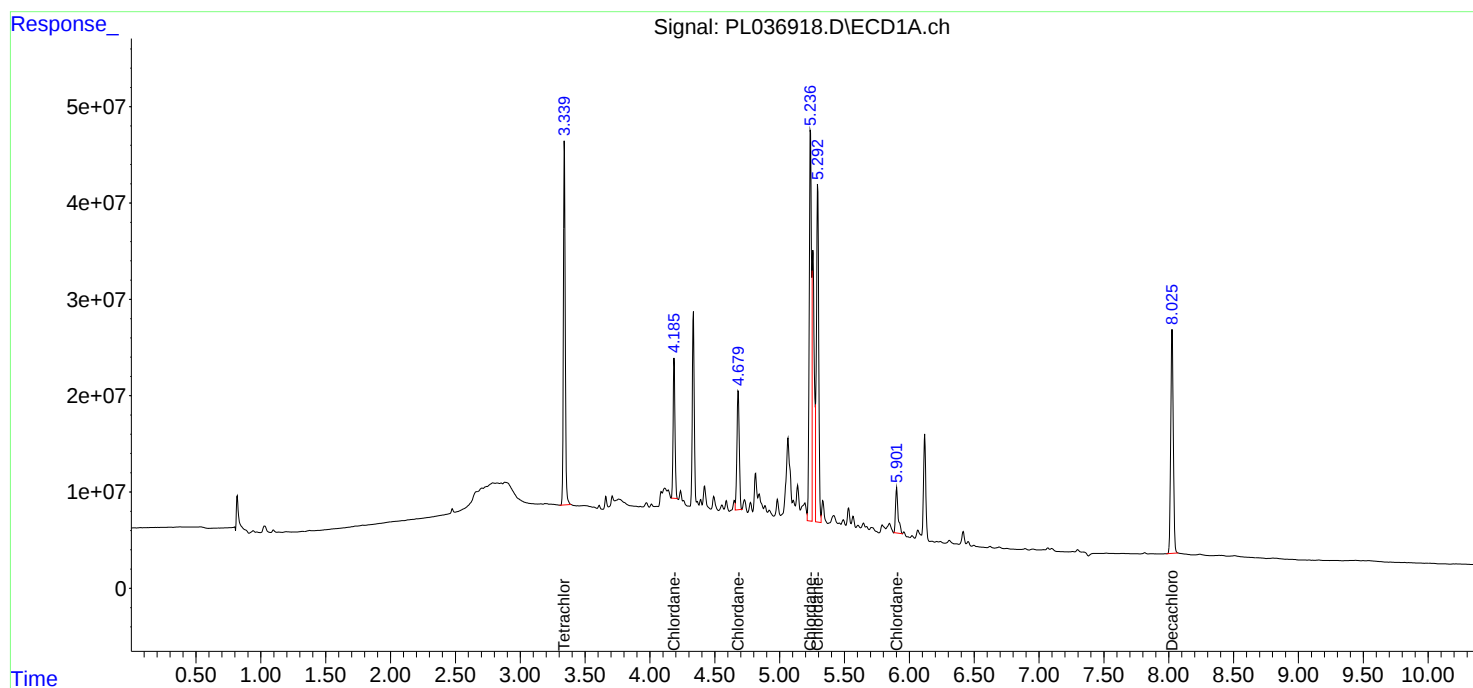


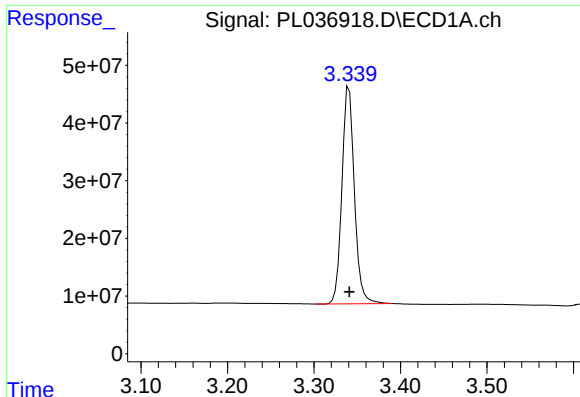

#1 Tetrachloro-m-xylene


R.T.: 3.341 min
Delta R.T.: 0.000 min
Response: 374066424
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

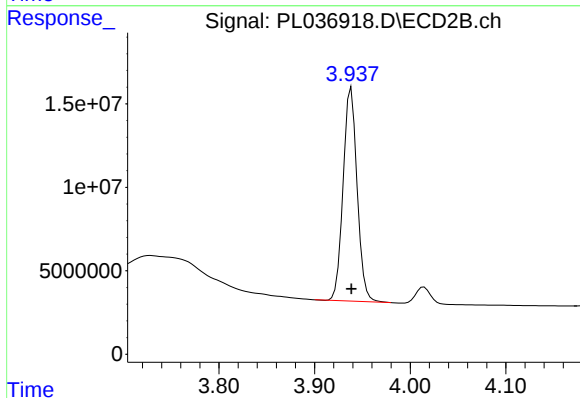


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: 0.000 min
Response: 130221701
Conc: 50.00 ng/ml

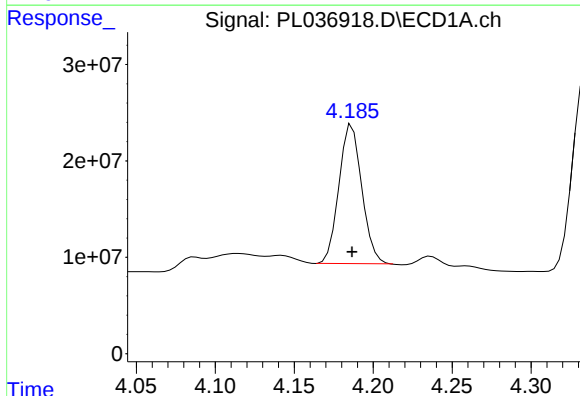


#23 Chlordane-1

R.T.: 4.187 min
Delta R.T.: 0.000 min
Response: 145279409
Conc: 500.00 ng/ml

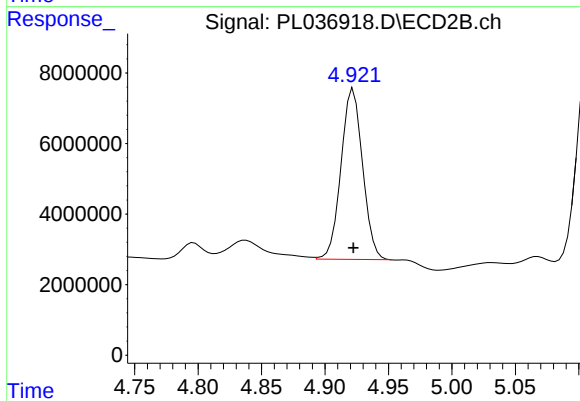

#23 Chlordane-1


R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 57176831
Conc: 500.00 ng/ml

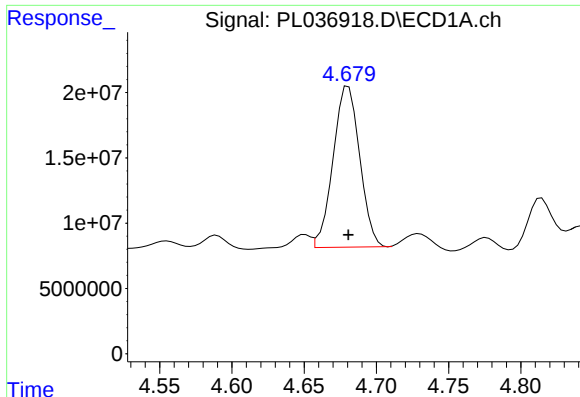

#24 Chlordane-2


R.T.: 4.681 min
Delta R.T.: 0.000 min
Response: 157895806
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

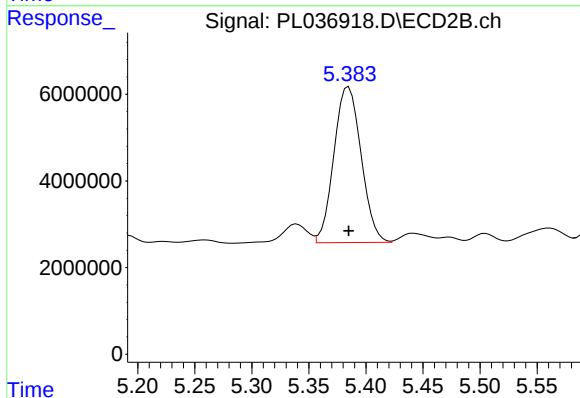


#24 Chlordane-2

R.T.: 5.385 min
Delta R.T.: 0.000 min
Response: 59668906
Conc: 500.00 ng/ml

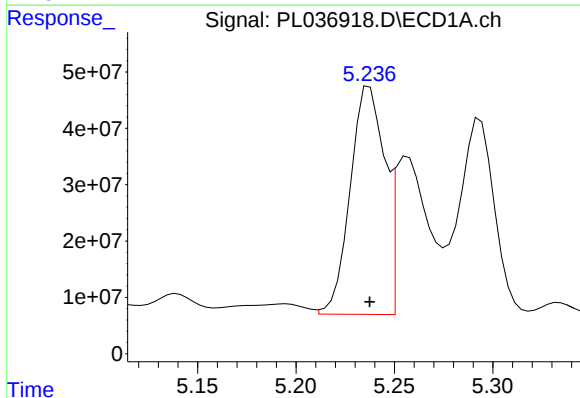


#25 Chlordane-3

R.T.: 5.237 min
Delta R.T.: 0.000 min
Response: 492242960
Conc: 500.00 ng/ml

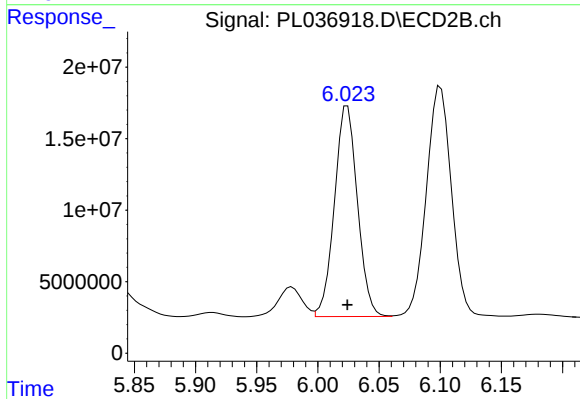

#25 Chlordane-3


R.T.: 6.024 min
Delta R.T.: 0.000 min
Response: 192513960
Conc: 500.00 ng/ml

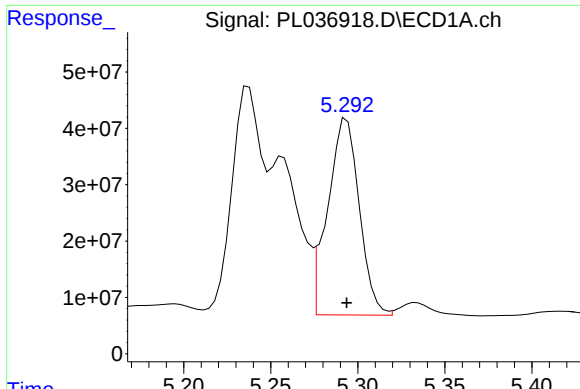

#26 Chlordane-4


R.T.: 5.294 min
Delta R.T.: 0.000 min
Response: 440001433
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

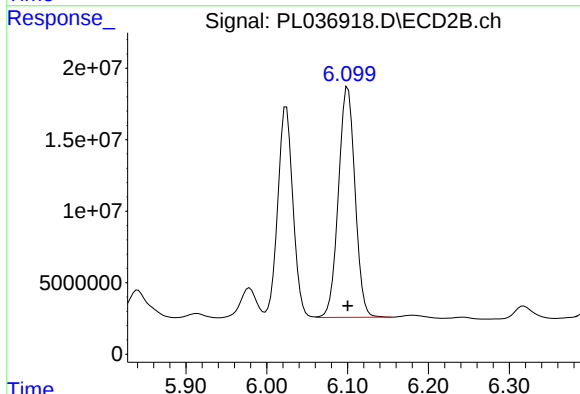


#26 Chlordane-4

R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 229635263
Conc: 500.00 ng/ml

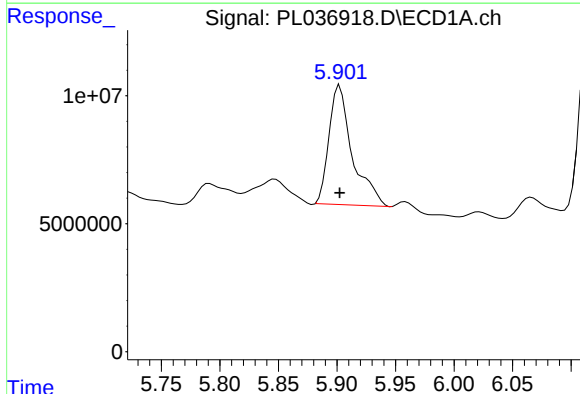


#27 Chlordane-5

R.T.: 5.902 min
Delta R.T.: 0.000 min
Response: 64639101
Conc: 500.00 ng/ml

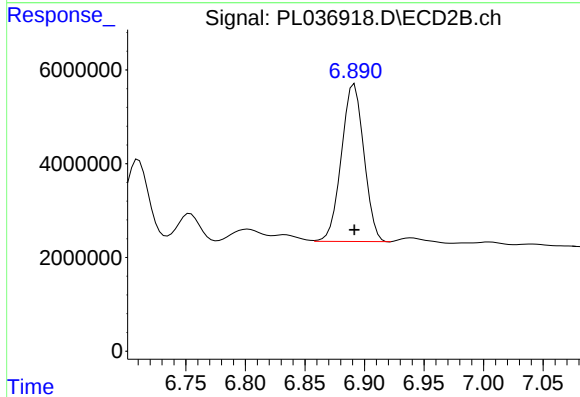

#27 Chlordane-5


R.T.: 6.892 min
Delta R.T.: 0.000 min
Response: 44165484
Conc: 500.00 ng/ml

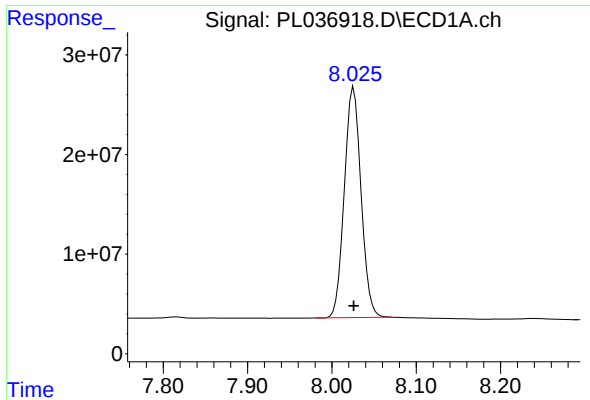

#28 Decachlorobiphenyl

R.T.: 8.026 min
Delta R.T.: 0.000 min
Response: 319251653
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

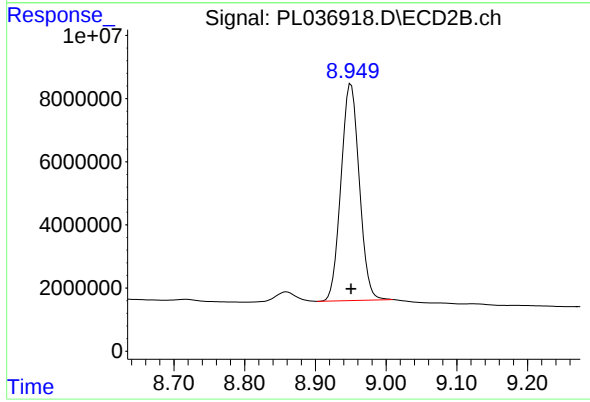

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: 0.000 min
Response: 123514011
Conc: 50.00 ng/ml