

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
 Data File : PL036952.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2018 23:20
 Operator : UA\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 02:36:38 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 14 16:13:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.340	3.938	119.1E6	42568456	16.749	16.651
28)	SA Decachlor...	8.024	8.948	126.0E6	47903820	19.360	18.779
Target Compounds							
6)	B beta-BHC	4.260f	0.000	4162644	0	0.975	N.D. #
8)	B Heptachlo...	0.000	5.781	0	11357629	N.D.	4.116 #
10)	B gamma-Chl...	5.169f	0.000	27892379	0	3.317	N.D. #
14)	MA Endrin	5.857	0.000	10805158	0	1.551	N.D. #
23)	Chlordane-1	4.124	0.000	14626538	0	50.762	N.D. #
24)	Chlordane-2	0.000	5.318	0	10901924	N.D.	93.921 #
25)	Chlordane-3	5.169	0.000	27892379	0	29.672	N.D. #
27)	Chlordane-5	5.857	0.000	10805158	0	86.626	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
Data File : PL036952.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2018 23:20
Operator : UA\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 02:36:38 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
Quant Title : GC Extractables
QLast Update : Thu Jun 14 16:13:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

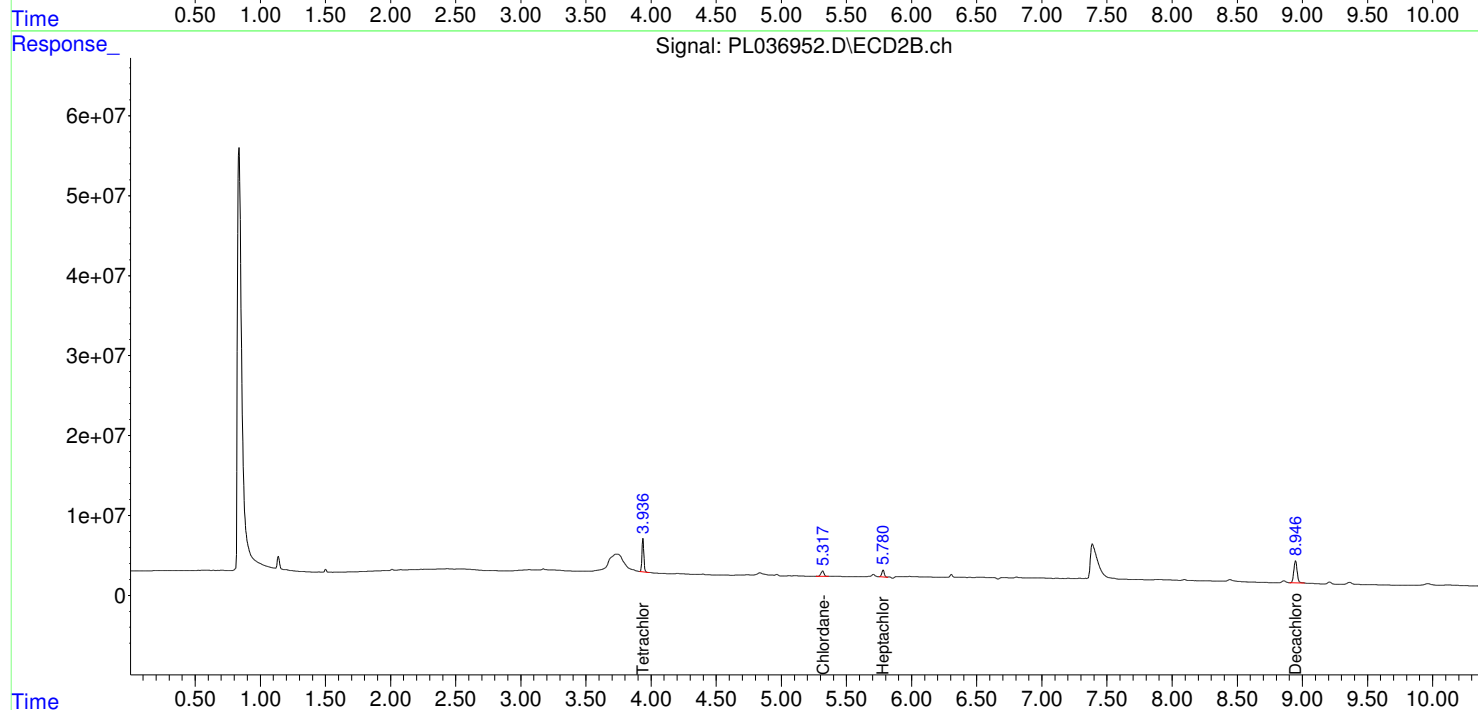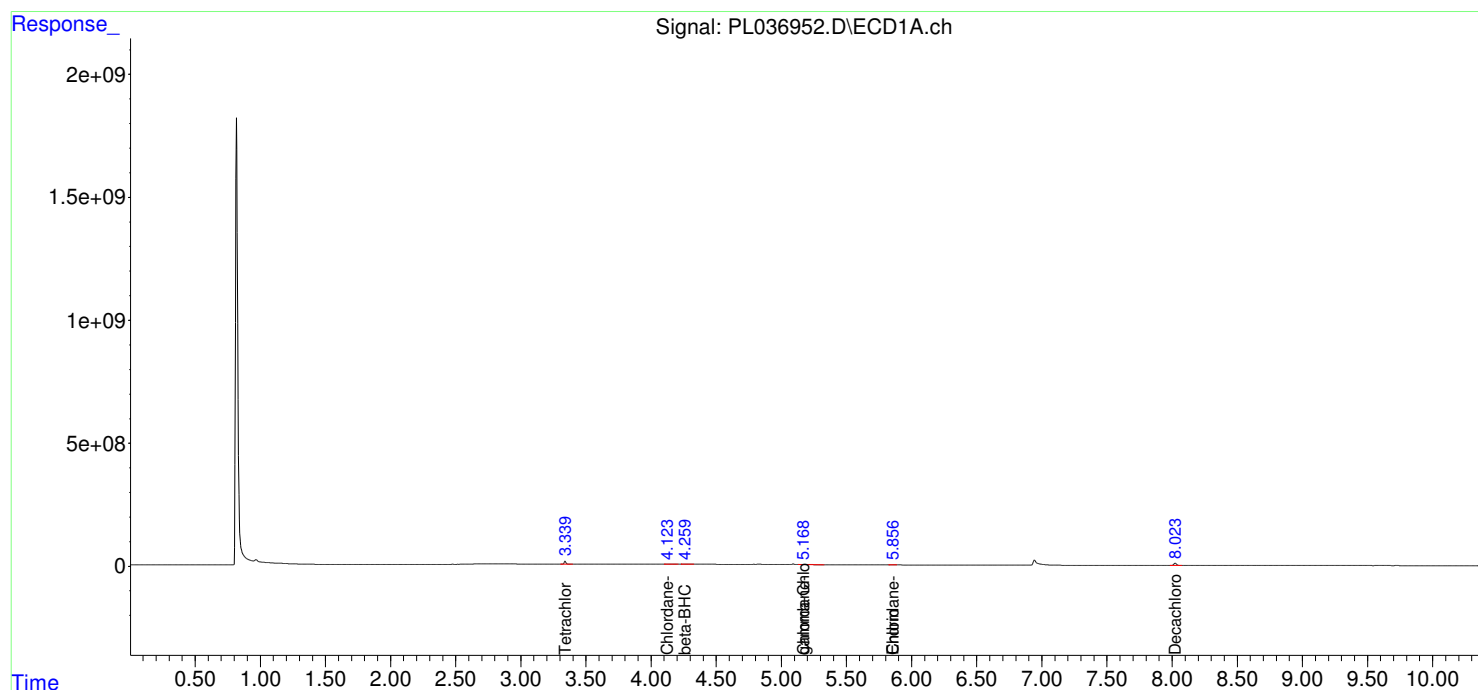


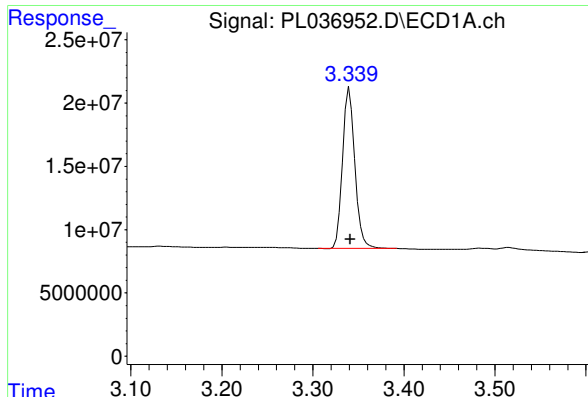

#1 Tetrachloro-m-xylene


R.T.: 3.340 min
Delta R.T.: 0.000 min
Response: 119102851
Conc: 16.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

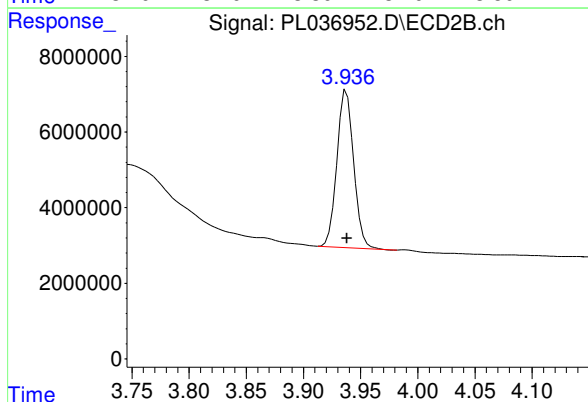


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: 0.000 min
Response: 42568456
Conc: 16.65 ng/ml

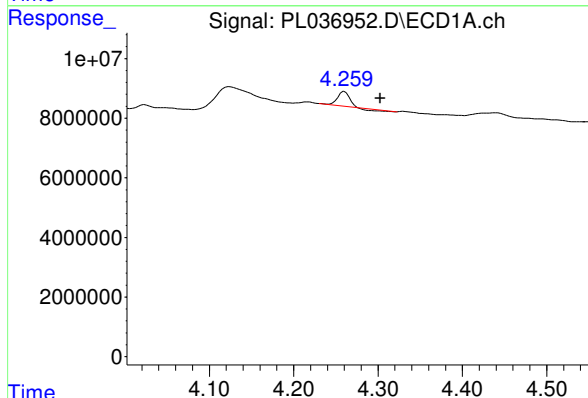


#6 beta-BHC

R.T.: 4.260 min
Delta R.T.: -0.042 min
Response: 4162644
Conc: 0.97 ng/ml

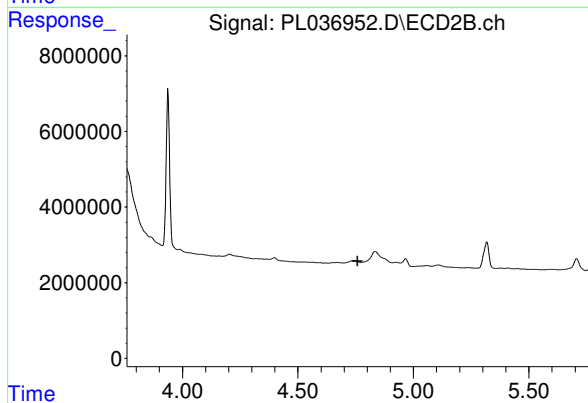

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.758 min
Response: 0
Conc: N.D.

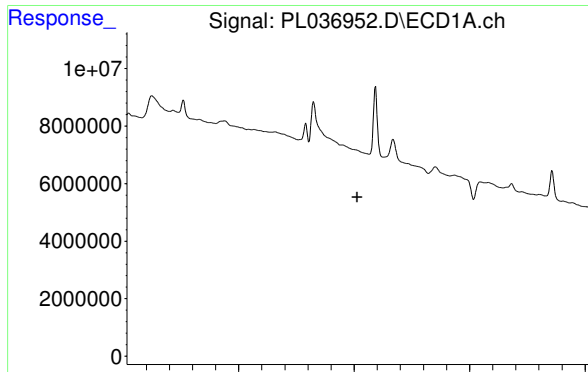

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.014 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

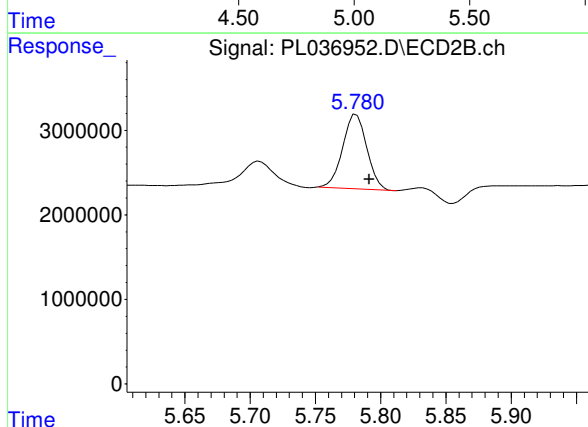


#8 Heptachlor epoxide

R.T.: 5.781 min
Delta R.T.: -0.010 min
Response: 11357629
Conc: 4.12 ng/ml

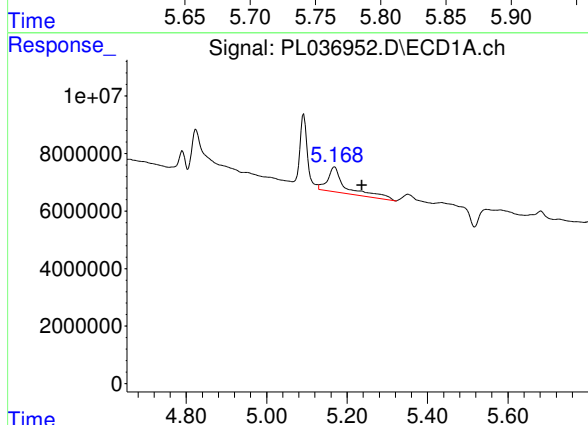


#10 gamma-Chlordane

R.T.: 5.169 min
Delta R.T.: -0.068 min
Response: 27892379
Conc: 3.32 ng/ml

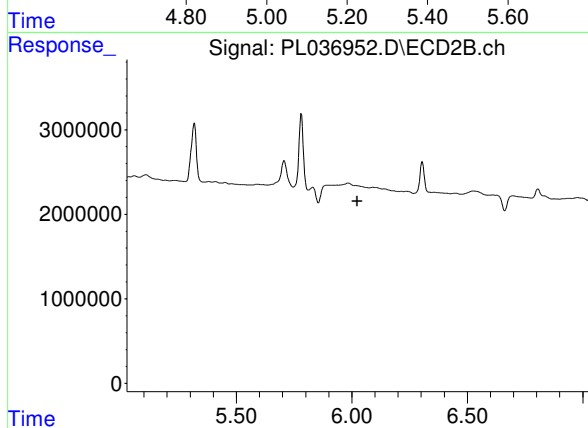

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.024 min
Response: 0
Conc: N.D.

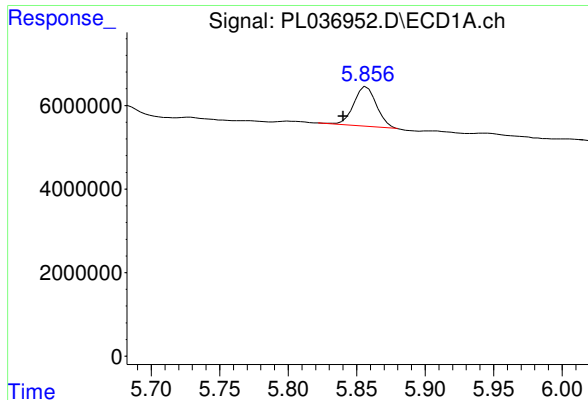

#14 Endrin


R.T.: 5.857 min
Delta R.T.: 0.017 min
Response: 10805158
Conc: 1.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

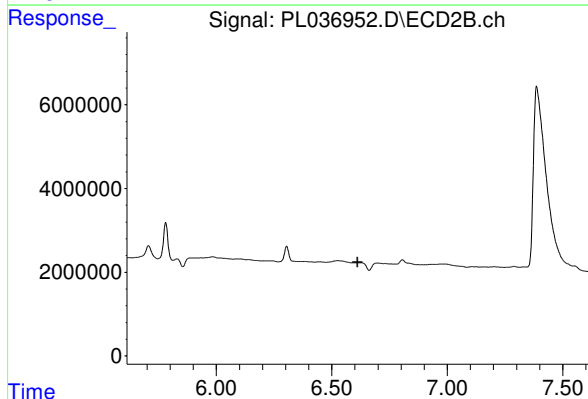


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.612 min
Response: 0
Conc: N.D.

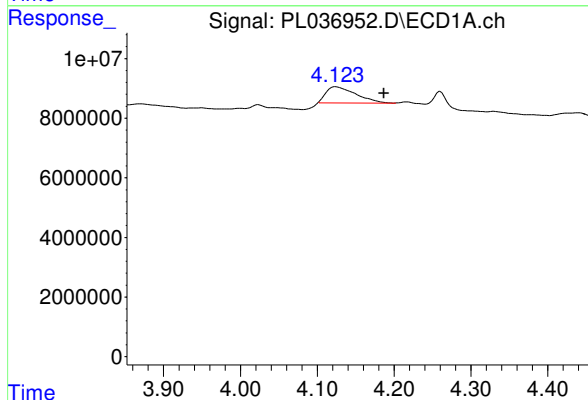


#23 Chlordane-1

R.T.: 4.124 min
Delta R.T.: -0.062 min
Response: 14626538
Conc: 50.76 ng/ml

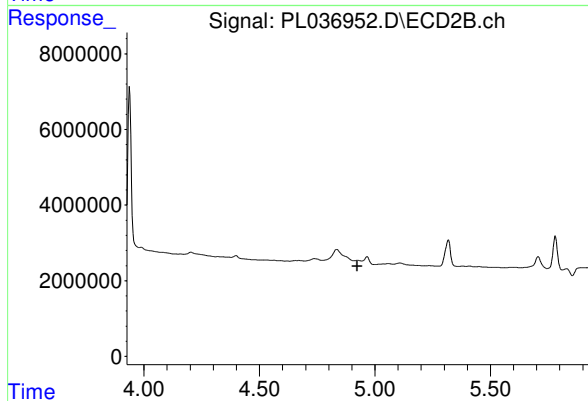

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.922 min
Response: 0
Conc: N.D.

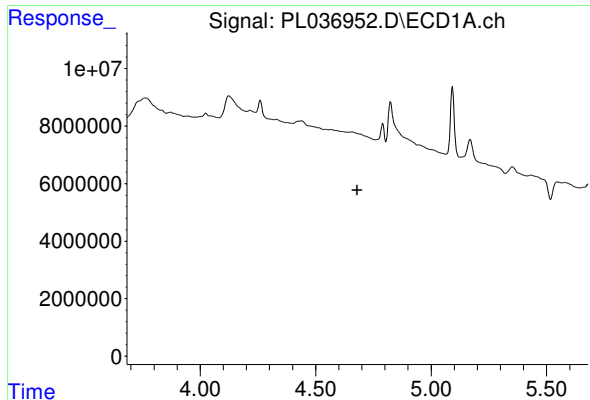

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.681 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

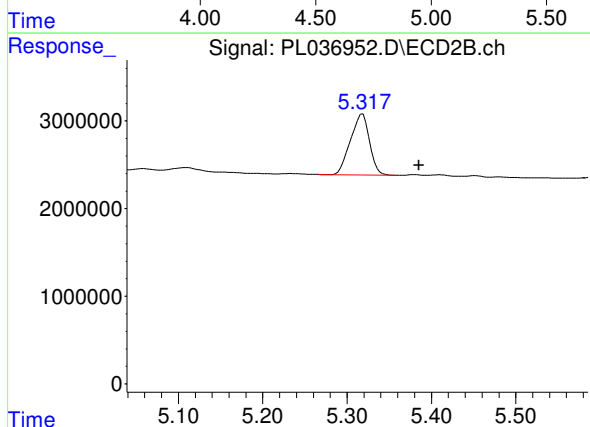


#24 Chlordane-2

R.T.: 5.318 min
Delta R.T.: -0.066 min
Response: 10901924
Conc: 93.92 ng/ml

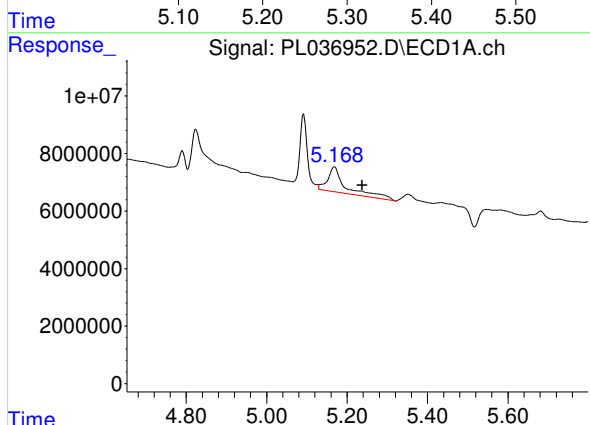


#25 Chlordane-3

R.T.: 5.169 min
Delta R.T.: -0.068 min
Response: 27892379
Conc: 29.67 ng/ml

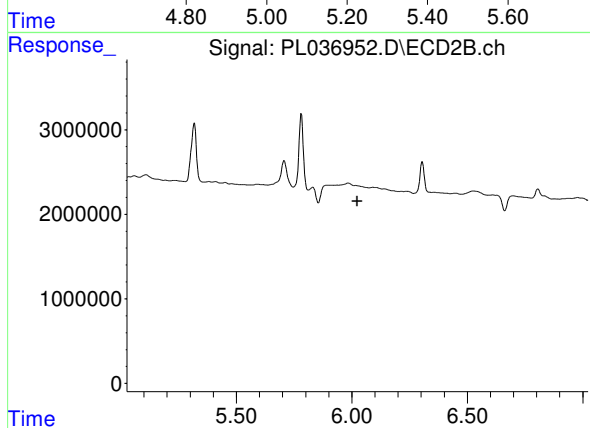

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.024 min
Response: 0
Conc: N.D.

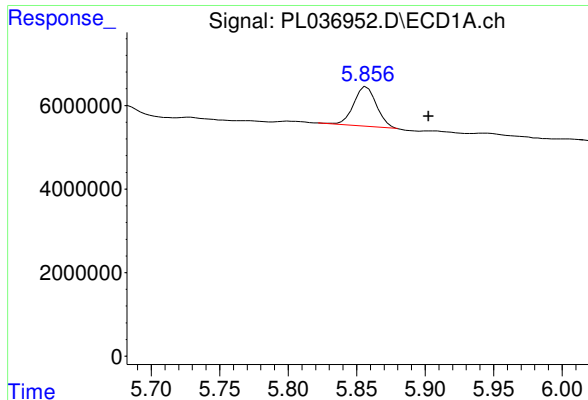

#27 Chlordane-5


R.T.: 5.857 min
Delta R.T.: -0.045 min
Response: 10805158
Conc: 86.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

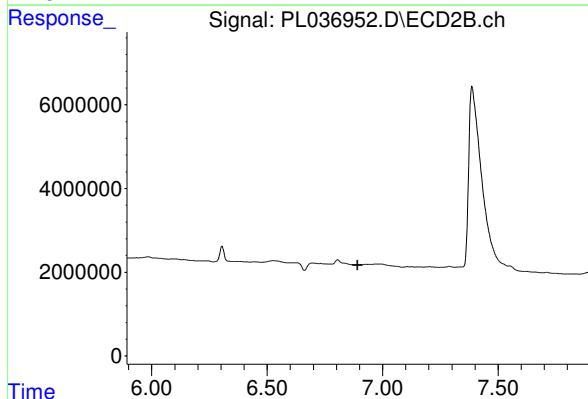


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.892 min
Response: 0
Conc: N.D.

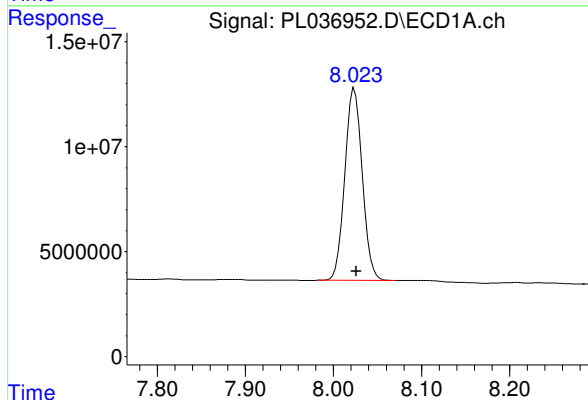

#28 Decachlorobiphenyl

R.T.: 8.024 min
Delta R.T.: -0.002 min
Response: 125957951
Conc: 19.36 ng/ml

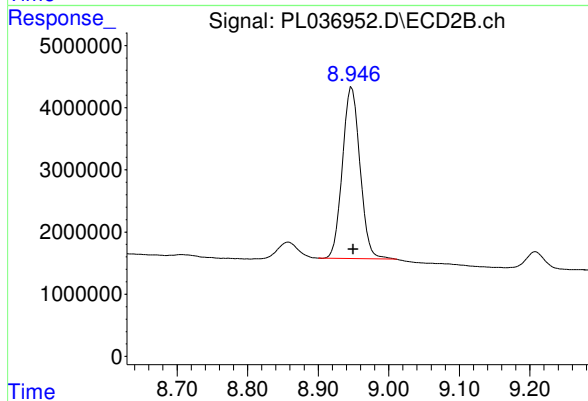

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.002 min
Response: 47903820
Conc: 18.78 ng/ml