

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
 Data File : PL036960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2018 01:12
 Operator : UA\AJ
 Sample : J3490-04
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 02:37:11 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 14 16:13:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.340	3.938	146.6E6	49569416	20.611	19.389
28) SA	Decachlor...	8.023	8.949	102.1E6	39861103	15.690	15.626
Target Compounds							
3) MA	gamma-BHC...	4.017f	0.000	5030649	0	0.520	N.D. #
6) B	beta-BHC	4.263f	0.000	15379442	0	3.601	N.D. #
10) B	gamma-Chl...	5.168f	0.000	11523402	0	1.370	N.D. #
25)	Chlordane-3	5.168	0.000	11523402	0	12.259	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
Data File : PL036960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2018 01:12
Operator : UA\AJ
Sample : J3490-04
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 02:37:11 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
Quant Title : GC Extractables
QLast Update : Thu Jun 14 16:13:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

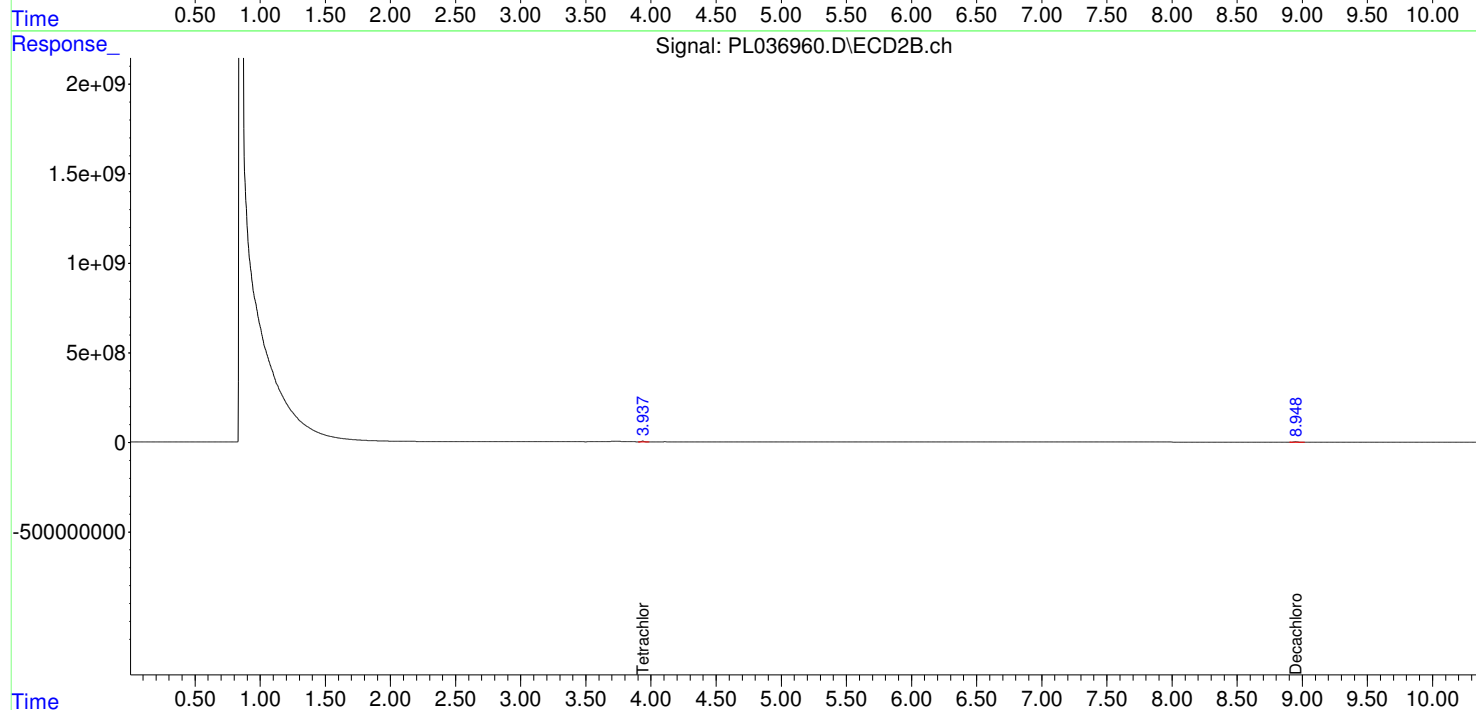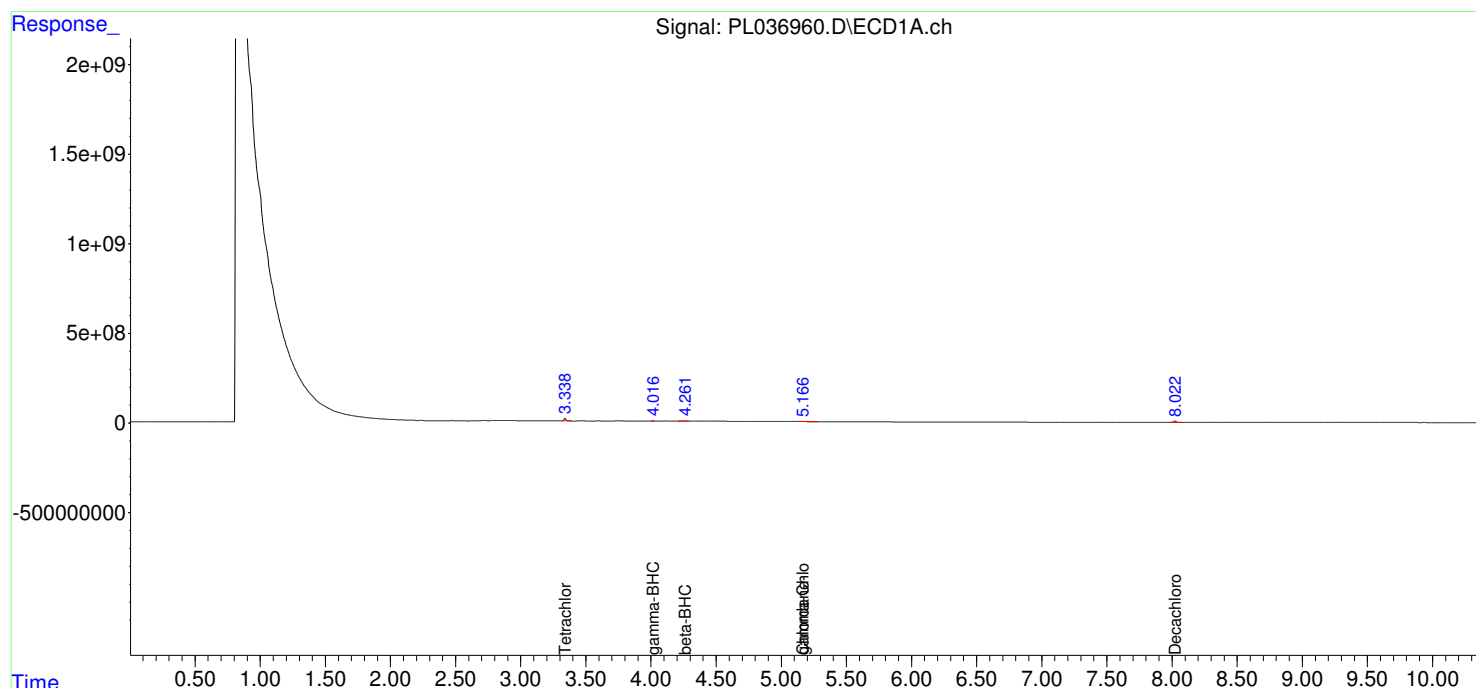


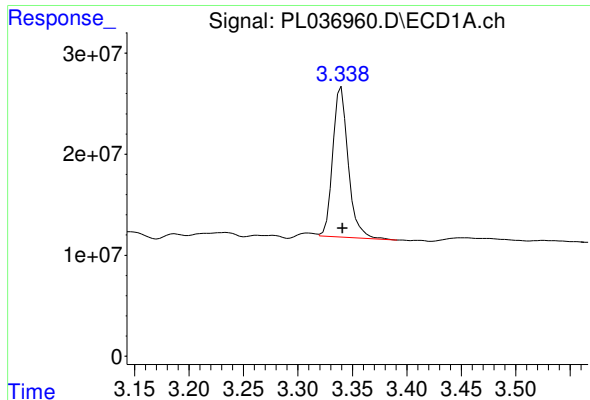

#1 Tetrachloro-m-xylene


R.T.: 3.340 min
Delta R.T.: -0.001 min
Response: 146572528
Conc: 20.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

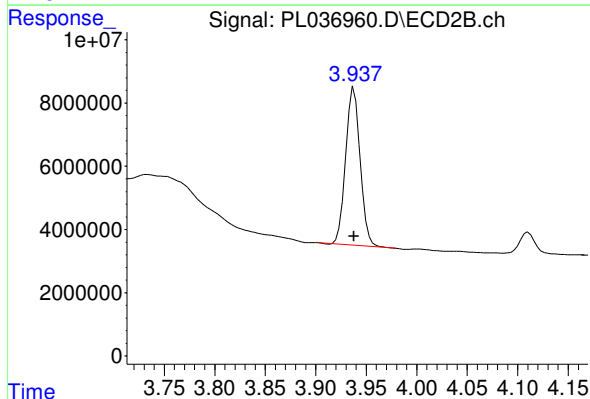


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: 0.000 min
Response: 49569416
Conc: 19.39 ng/ml

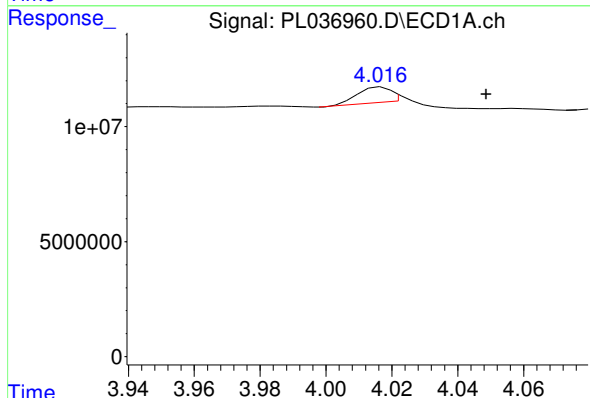


#3 gamma-BHC (Lindane)

R.T.: 4.017 min
Delta R.T.: -0.032 min
Response: 5030649
Conc: 0.52 ng/ml

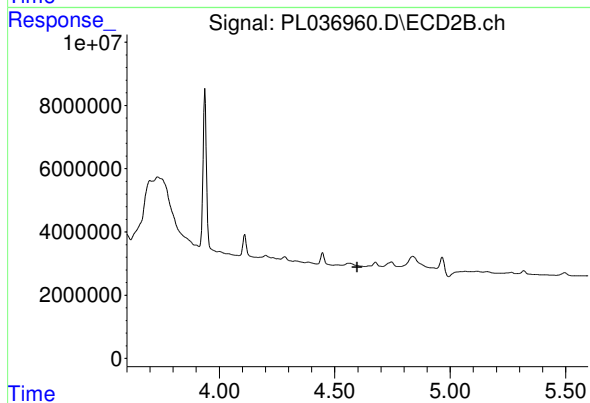

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.597 min
Response: 0
Conc: N.D.

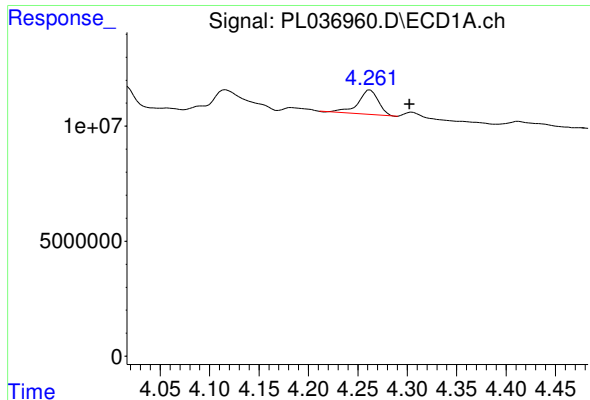

#6 beta-BHC


R.T.: 4.263 min
Delta R.T.: -0.040 min
Response: 15379442
Conc: 3.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

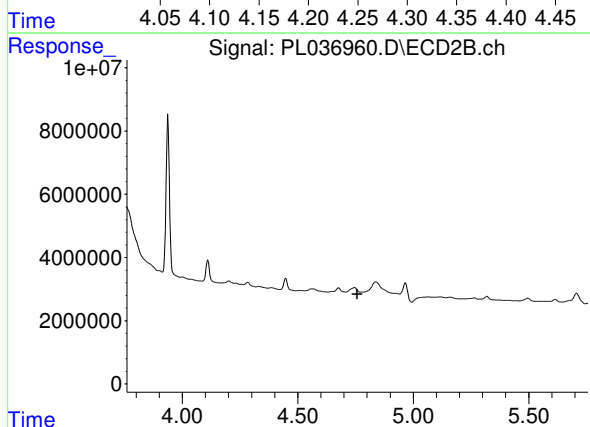


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

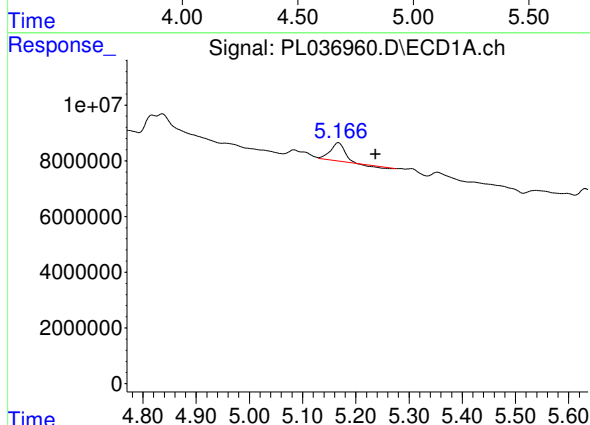


#10 gamma-Chlordane

R.T.: 5.168 min
Delta R.T.: -0.069 min
Response: 11523402
Conc: 1.37 ng/ml

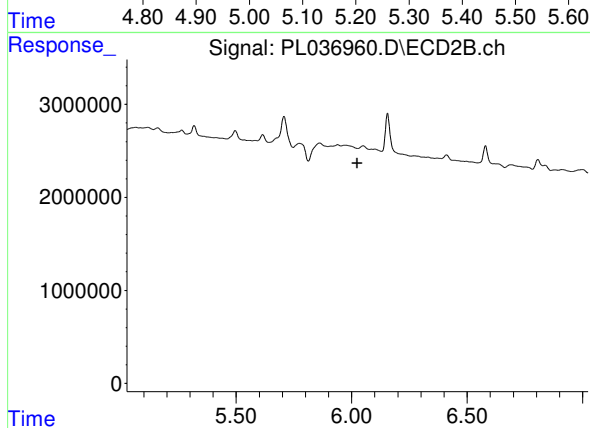

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.024 min
Response: 0
Conc: N.D.

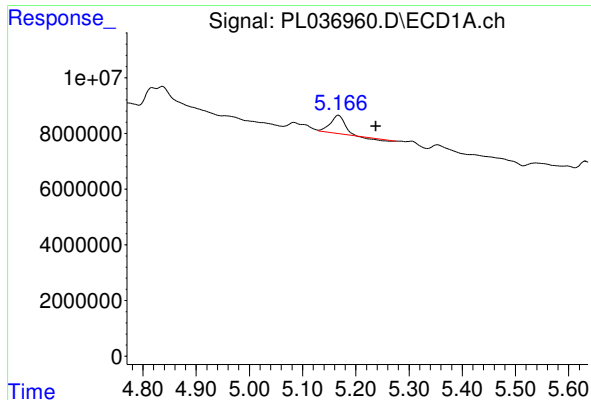

#25 Chlordane-3


R.T.: 5.168 min
Delta R.T.: -0.070 min
Response: 11523402
Conc: 12.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

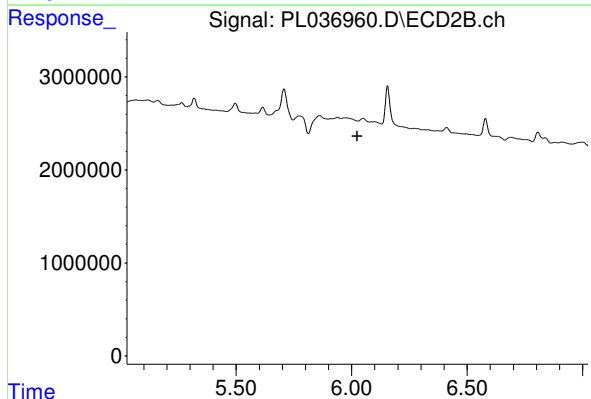


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 6.024 min
Response: 0
Conc: N.D.

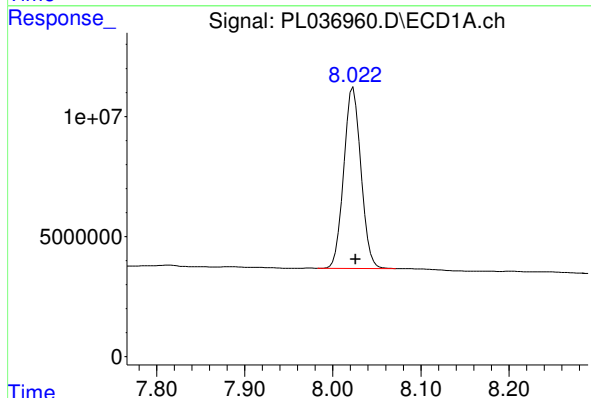

#28 Decachlorobiphenyl

R.T.: 8.023 min
Delta R.T.: -0.002 min
Response: 102079663
Conc: 15.69 ng/ml

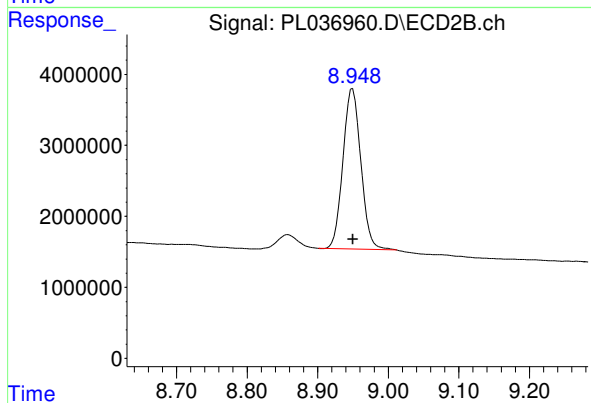

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: 0.000 min
Response: 39861103
Conc: 15.63 ng/ml