

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
 Data File : PL036965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2018 02:22
 Operator : UA\AJ
 Sample : PB110232BL
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 03:34:41 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 14 16:13:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.340	3.938	137.2E6	50161095	19.292	19.621
28)	SA Decachlor...	8.023	8.950	118.7E6	46382710	18.243	18.182
Target Compounds							
6)	B beta-BHC	4.260f	0.000	4618623	0	1.082	N.D. #
10)	B gamma-Chl...	5.168f	0.000	15938838	0	1.895	N.D. #
23)	Chlordane-1	4.133	0.000	13491362	0	46.823	N.D. #
25)	Chlordane-3	5.168	0.000	15938838	0	16.956	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
Data File : PL036965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2018 02:22
Operator : UA\AJ
Sample : PB110232BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 03:34:41 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
Quant Title : GC Extractables
QLast Update : Thu Jun 14 16:13:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

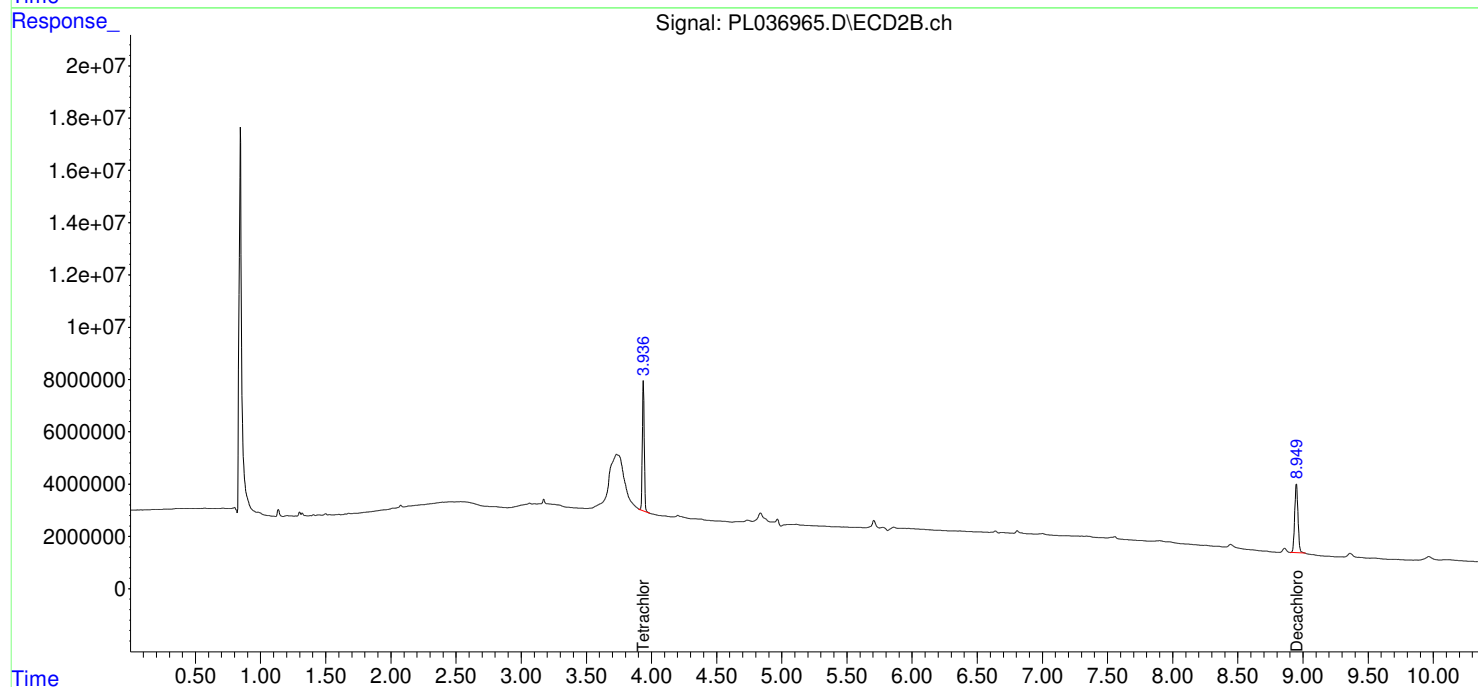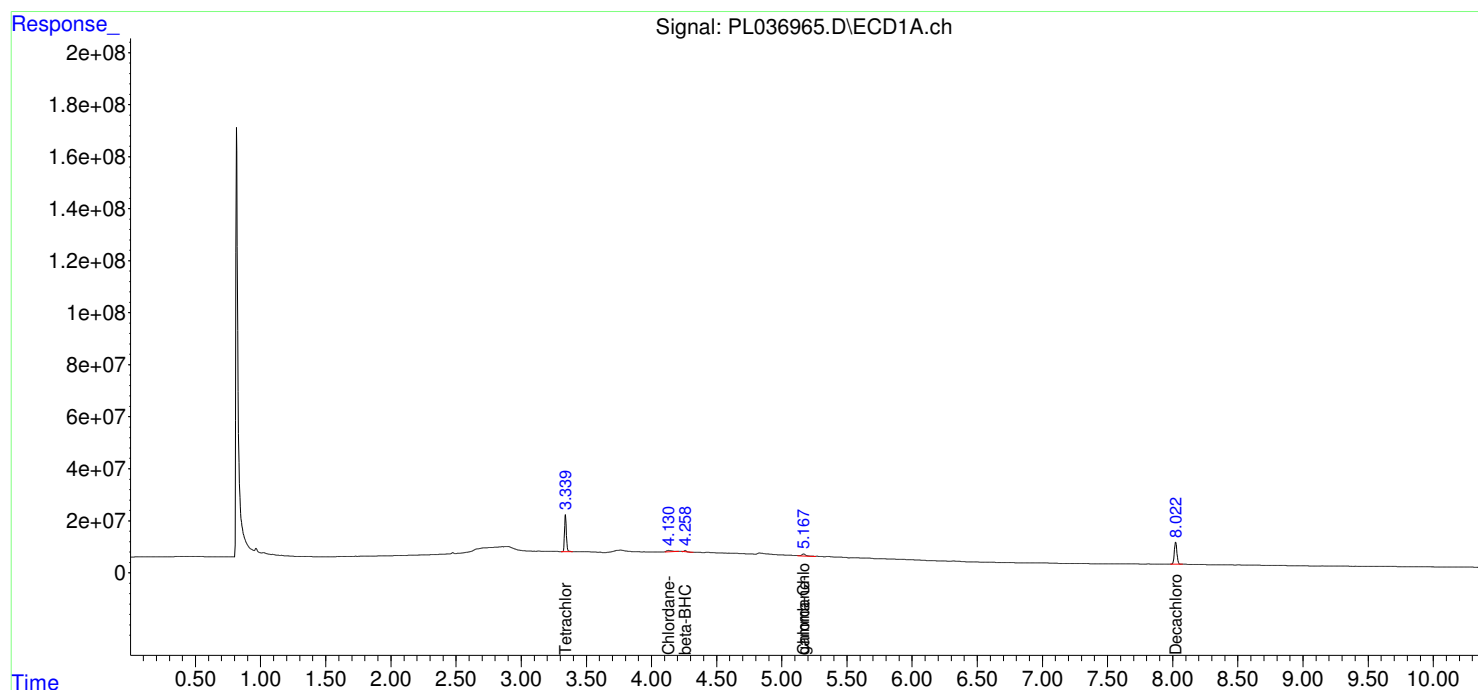


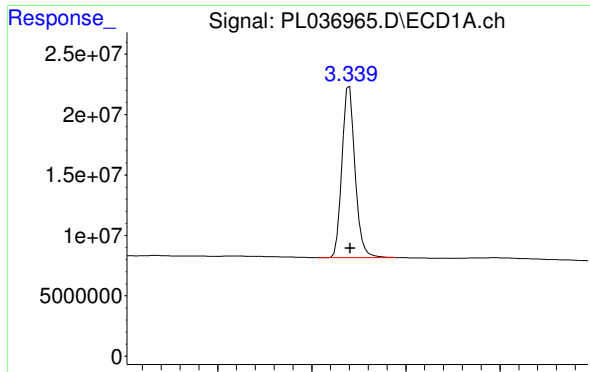

#1 Tetrachloro-m-xylene


R.T.: 3.340 min
Delta R.T.: -0.001 min
Response: 137187779
Conc: 19.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

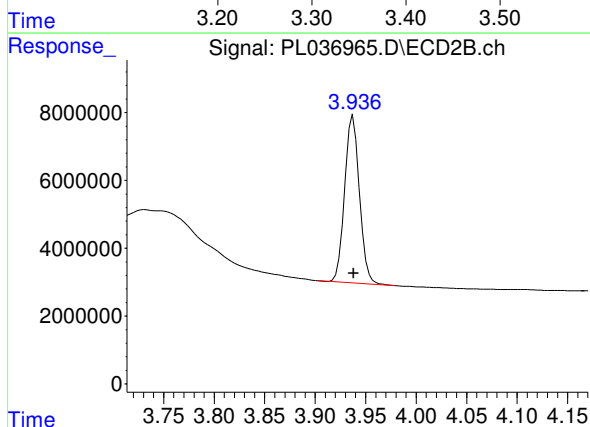


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: 0.000 min
Response: 50161095
Conc: 19.62 ng/ml

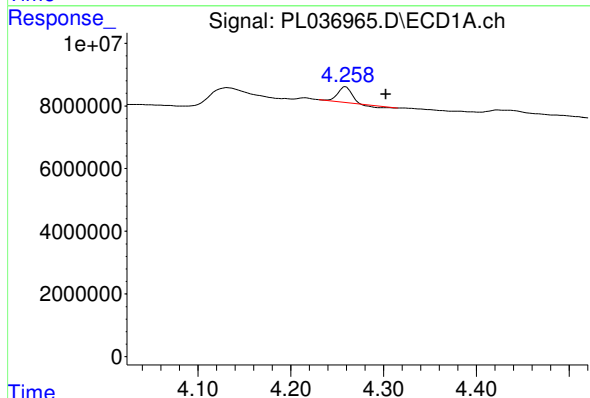


#6 beta-BHC

R.T.: 4.260 min
Delta R.T.: -0.043 min
Response: 4618623
Conc: 1.08 ng/ml

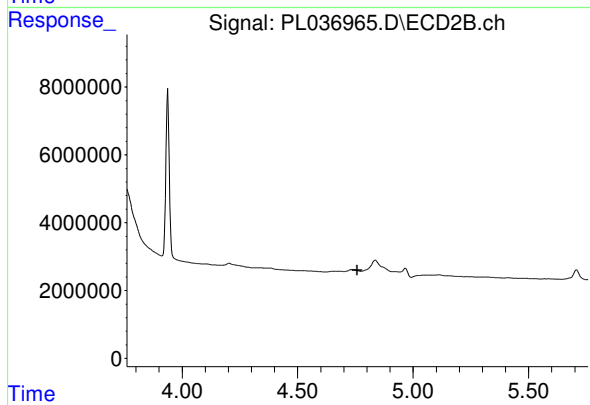

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.758 min
Response: 0
Conc: N.D.

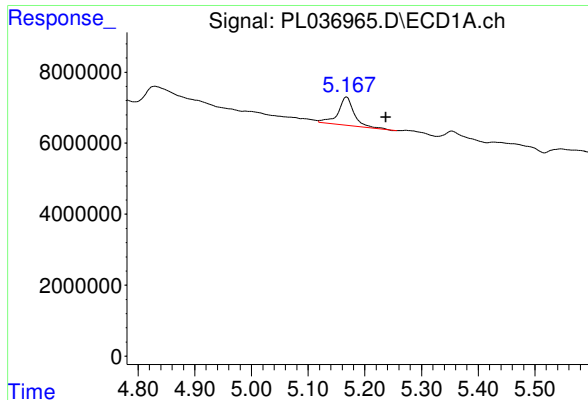

#10 gamma-Chlordane


R.T.: 5.168 min
Delta R.T.: -0.069 min
Response: 15938838
Conc: 1.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

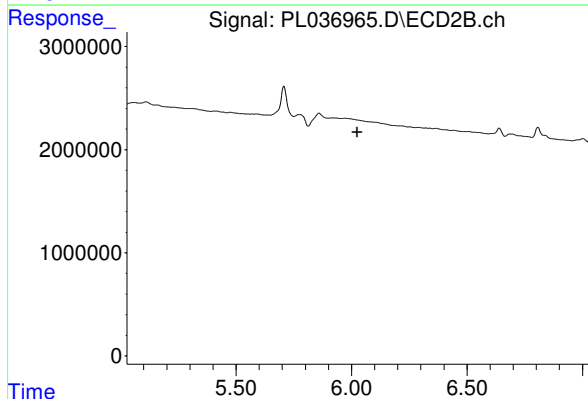


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.024 min
Response: 0
Conc: N.D.

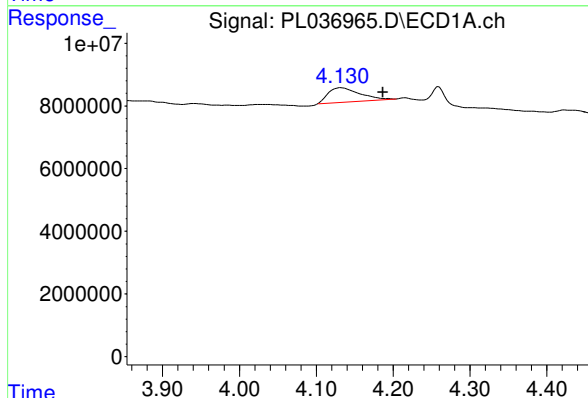


#23 Chlordane-1

R.T.: 4.133 min
Delta R.T.: -0.054 min
Response: 13491362
Conc: 46.82 ng/ml

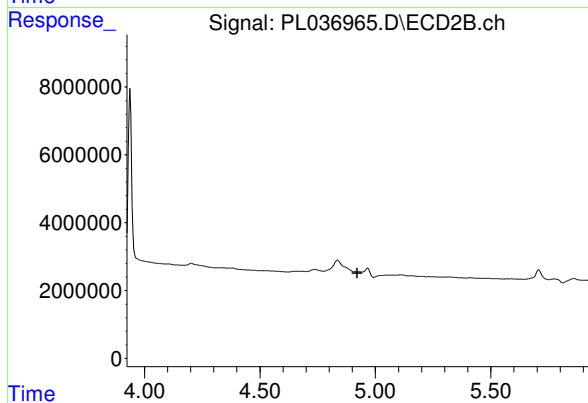

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.922 min
Response: 0
Conc: N.D.

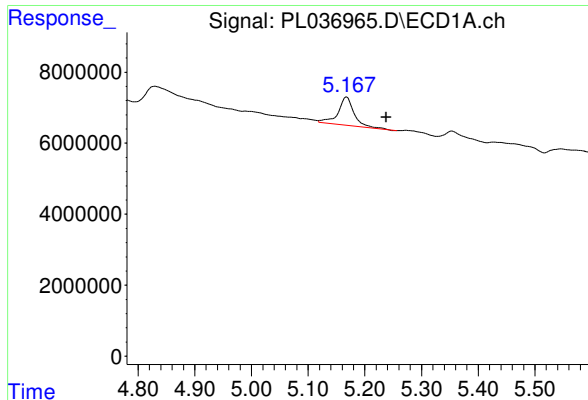

#25 Chlordane-3


R.T.: 5.168 min
Delta R.T.: -0.069 min
Response: 15938838
Conc: 16.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

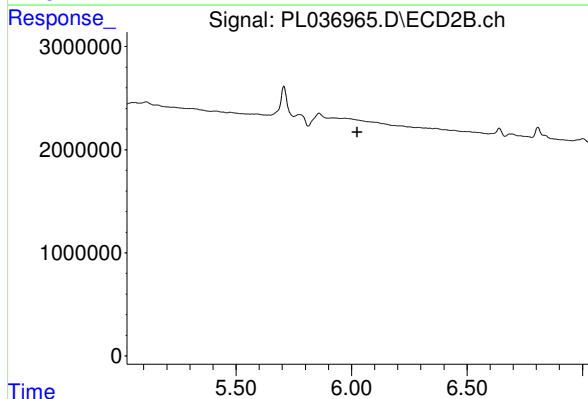


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 6.024 min
Response: 0
Conc: N.D.

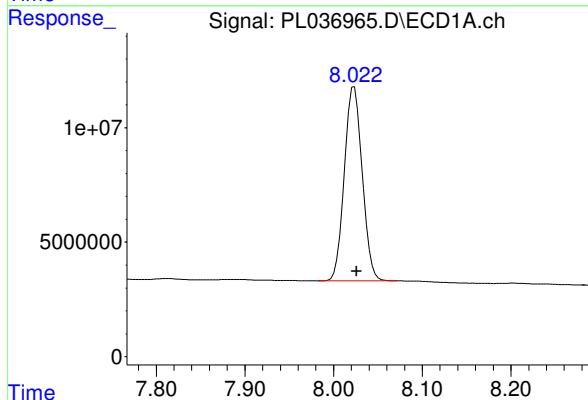

#28 Decachlorobiphenyl

R.T.: 8.023 min
Delta R.T.: -0.003 min
Response: 118688347
Conc: 18.24 ng/ml

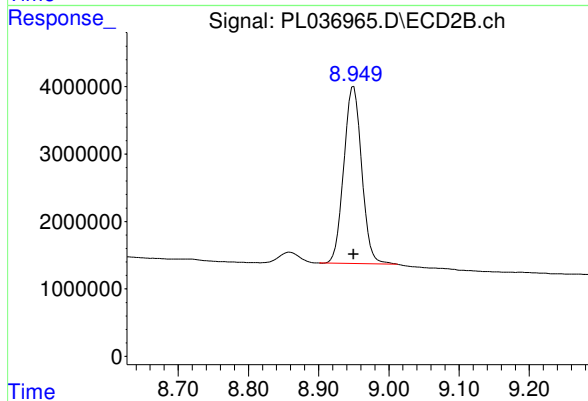

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: 0.000 min
Response: 46382710
Conc: 18.18 ng/ml