

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
 Data File : PL036968.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2018 03:04
 Operator : UA\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 03:34:58 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 14 16:13:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.340	3.938	122.1E6	43493830	17.165	17.013
28)	SA Decachlor...	8.025	8.950	128.9E6	48971927	19.816	19.197
Target Compounds							
6)	B beta-BHC	4.261f	0.000	4741625	0	1.110	N.D. #
8)	B Heptachlo...	0.000	5.782	0	21306504	N.D.	7.722 #
10)	B gamma-Chl...	5.169f	0.000	12207059	0	1.451	N.D. #
14)	MA Endrin	5.858	0.000	19358647	0	2.779	N.D. #
23)	Chlordane-1	4.130	0.000	15131942	0	52.516	N.D. #
24)	Chlordane-2	0.000	5.320	0	22907712	N.D.	197.352 #
25)	Chlordane-3	5.169	0.000	12207059	0	12.986	N.D. #
27)	Chlordane-5	5.858	0.000	19358647	0	155.200	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
Data File : PL036968.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2018 03:04
Operator : UA\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 03:34:58 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
Quant Title : GC Extractables
QLast Update : Thu Jun 14 16:13:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

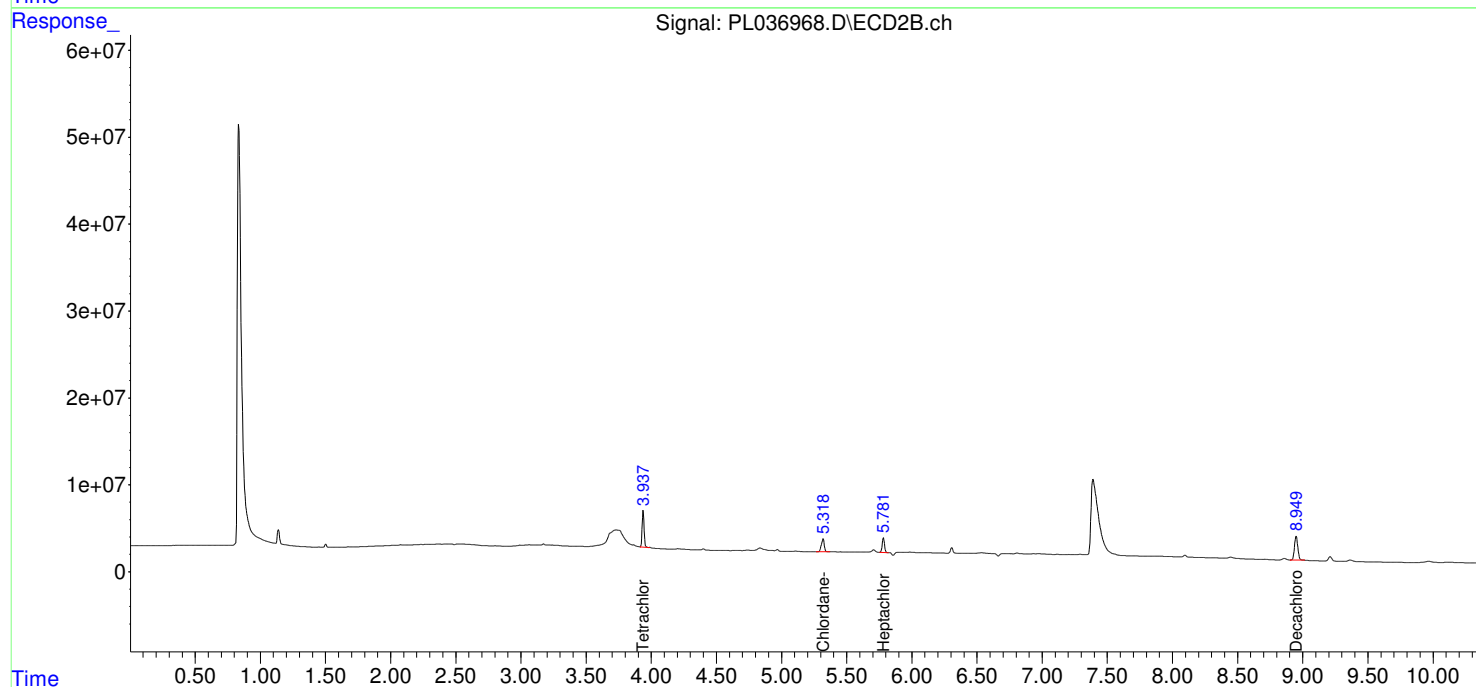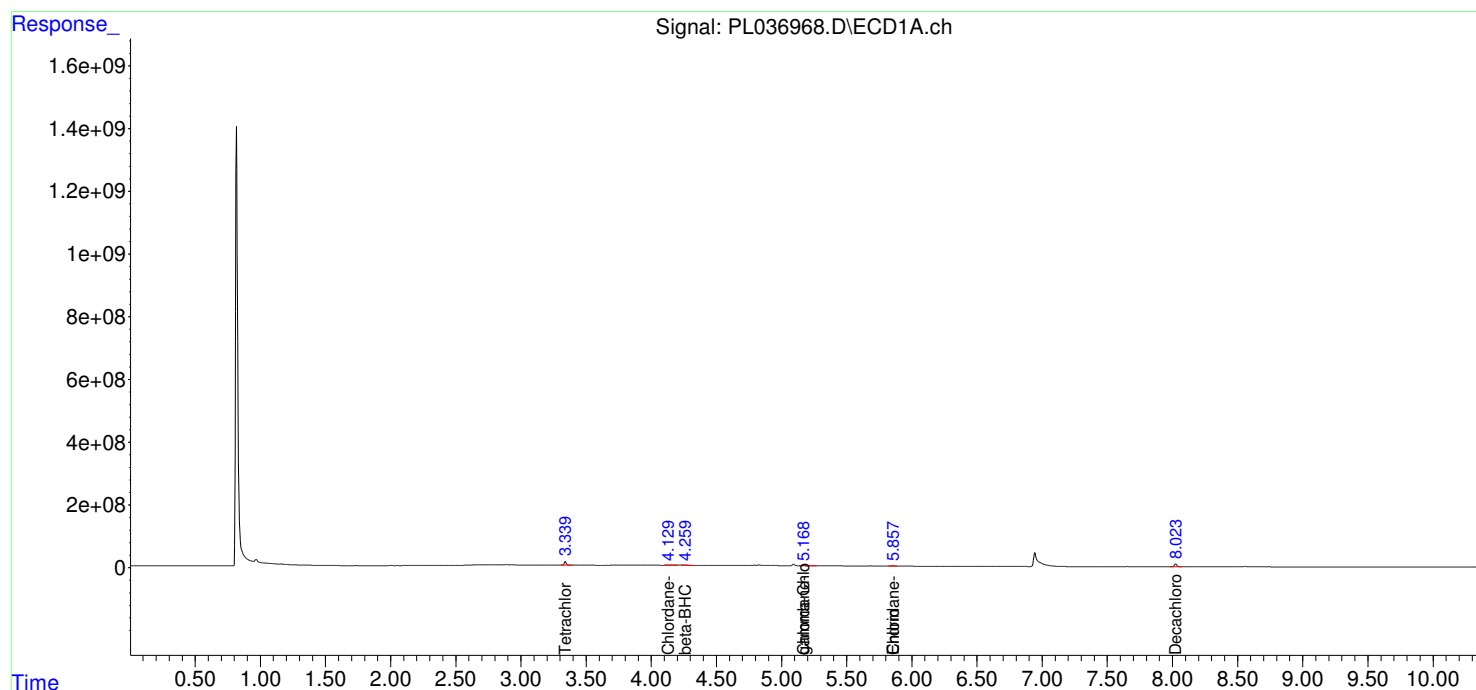


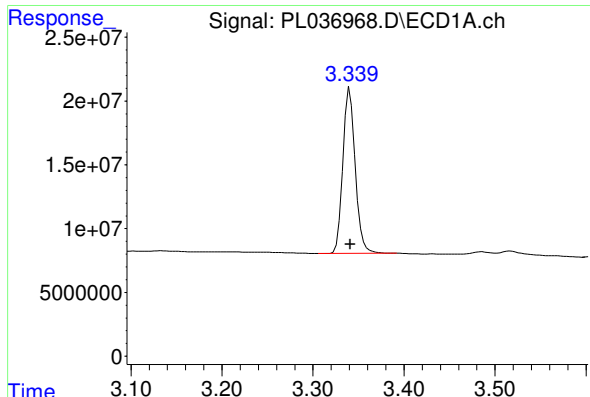

#1 Tetrachloro-m-xylene


R.T.: 3.340 min
Delta R.T.: 0.000 min
Response: 122064424
Conc: 17.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

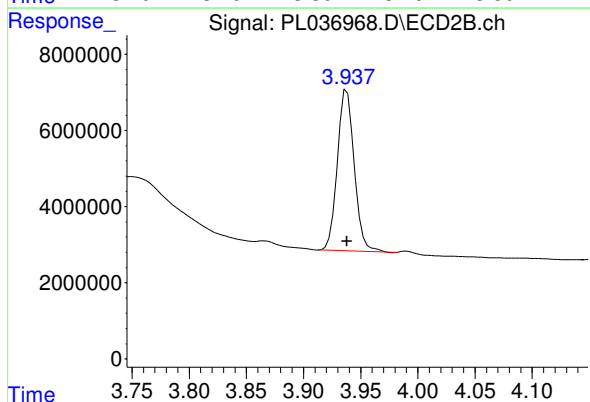


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: 0.000 min
Response: 43493830
Conc: 17.01 ng/ml

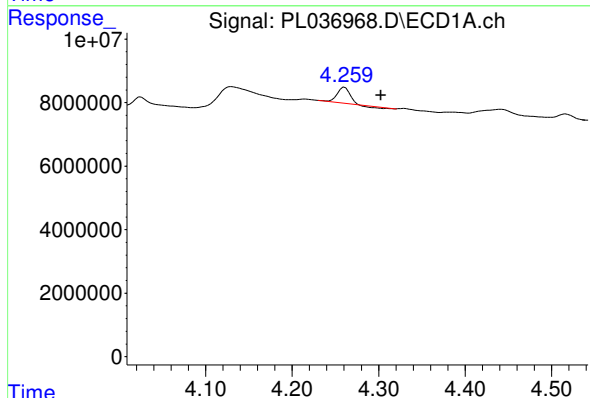


#6 beta-BHC

R.T.: 4.261 min
Delta R.T.: -0.042 min
Response: 4741625
Conc: 1.11 ng/ml

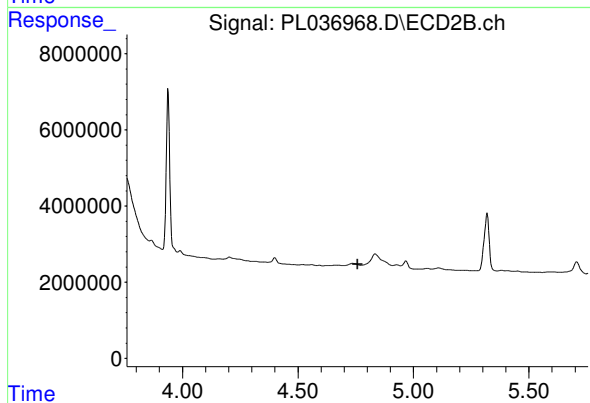

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.758 min
Response: 0
Conc: N.D.

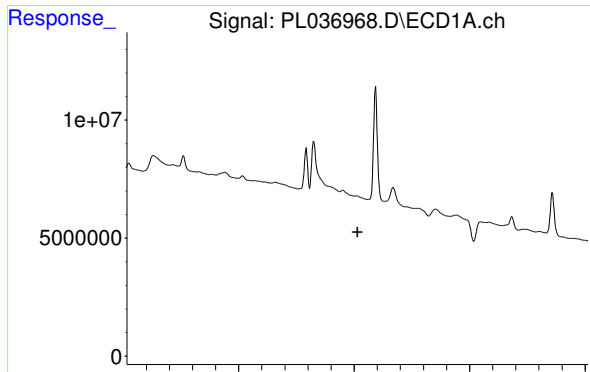

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.014 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

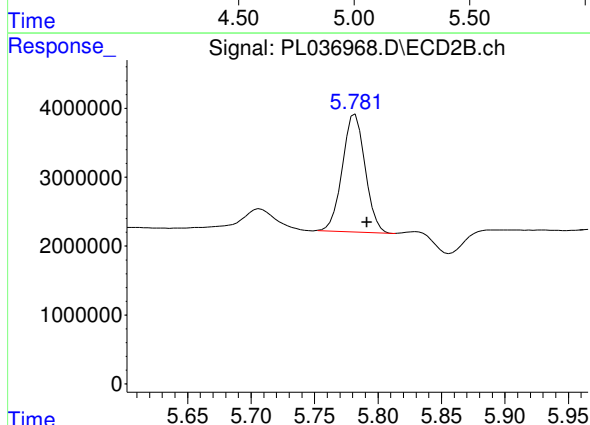


#8 Heptachlor epoxide

R.T.: 5.782 min
Delta R.T.: -0.009 min
Response: 21306504
Conc: 7.72 ng/ml

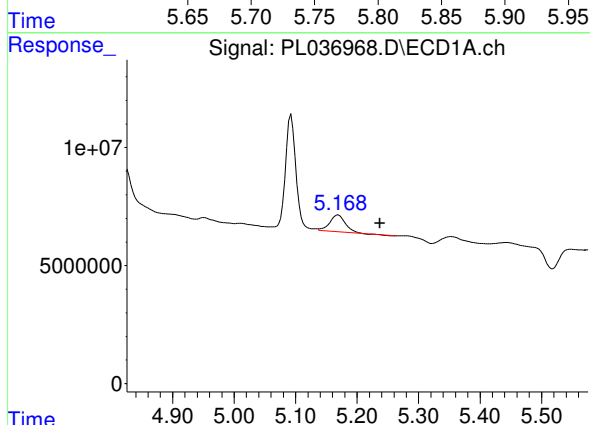


#10 gamma-Chlordane

R.T.: 5.169 min
Delta R.T.: -0.068 min
Response: 12207059
Conc: 1.45 ng/ml

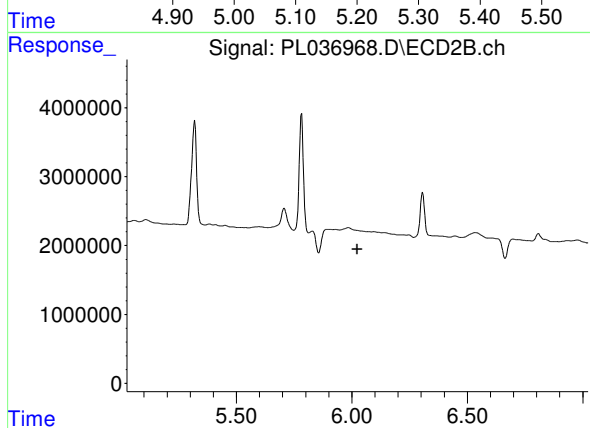

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.024 min
Response: 0
Conc: N.D.

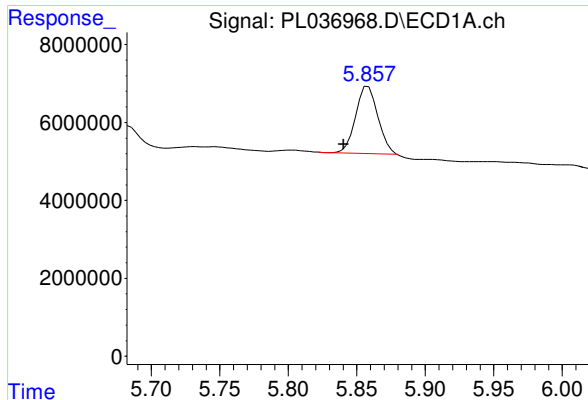

#14 Endrin


R.T.: 5.858 min
Delta R.T.: 0.018 min
Response: 19358647
Conc: 2.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

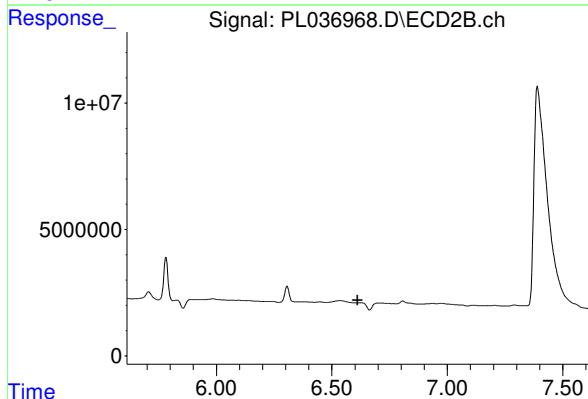


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.612 min
Response: 0
Conc: N.D.

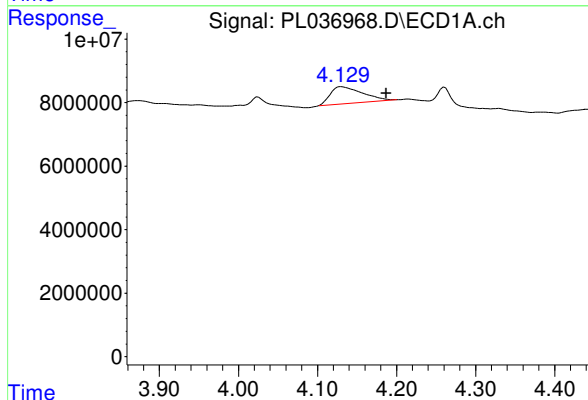


#23 Chlordane-1

R.T.: 4.130 min
Delta R.T.: -0.056 min
Response: 15131942
Conc: 52.52 ng/ml

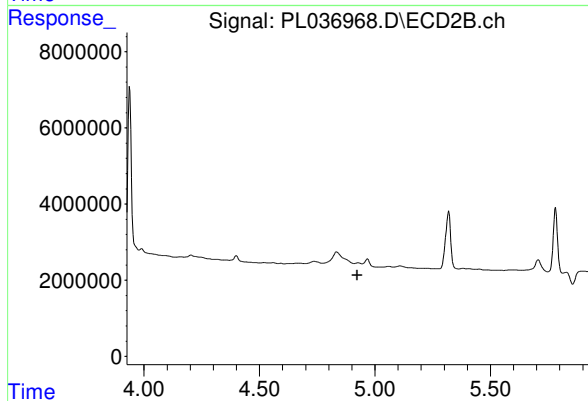

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.922 min
Response: 0
Conc: N.D.

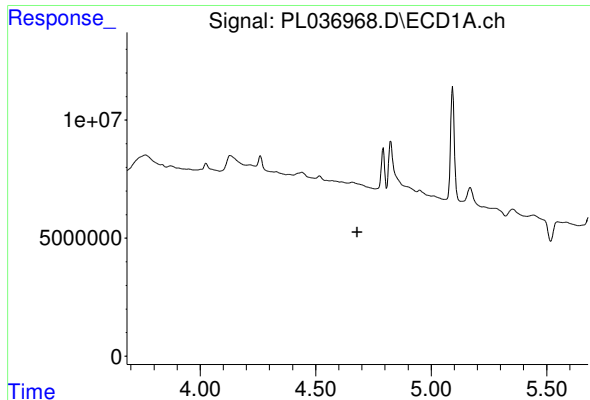

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.681 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

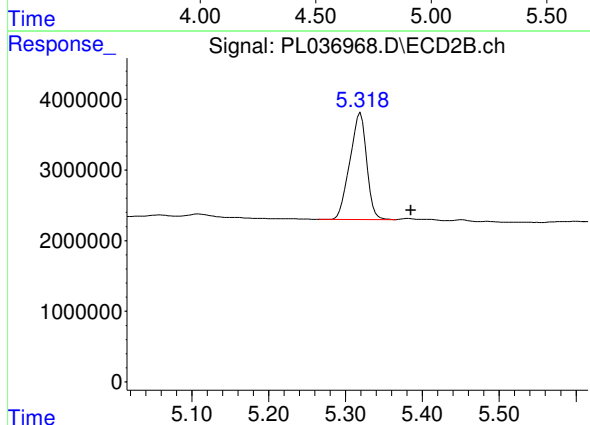


#24 Chlordane-2

R.T.: 5.320 min
Delta R.T.: -0.065 min
Response: 22907712
Conc: 197.35 ng/ml

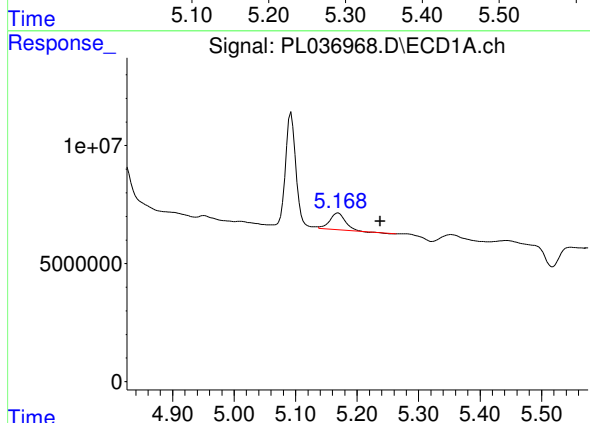


#25 Chlordane-3

R.T.: 5.169 min
Delta R.T.: -0.068 min
Response: 12207059
Conc: 12.99 ng/ml

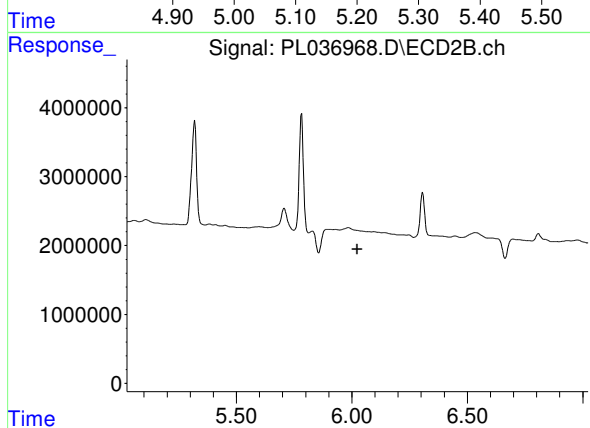

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.024 min
Response: 0
Conc: N.D.

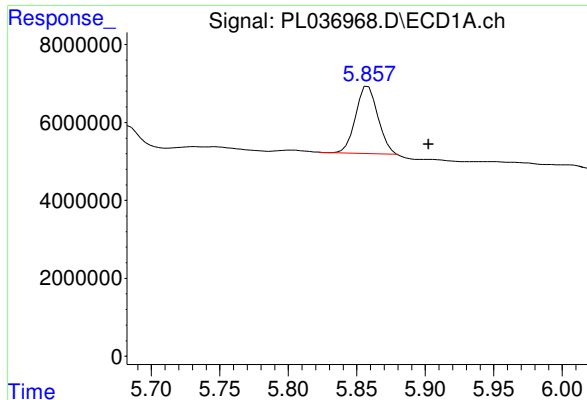

#27 Chlordane-5


R.T.: 5.858 min
Delta R.T.: -0.044 min
Response: 19358647
Conc: 155.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

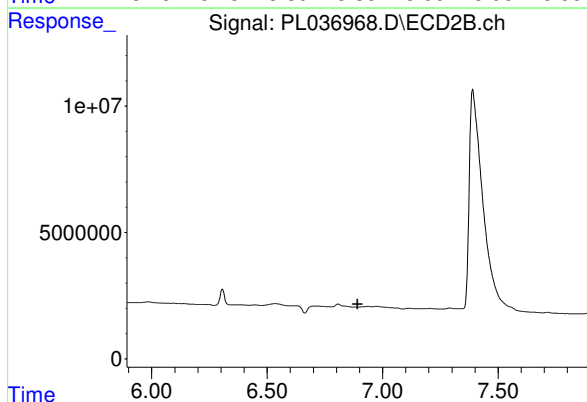


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.892 min
Response: 0
Conc: N.D.

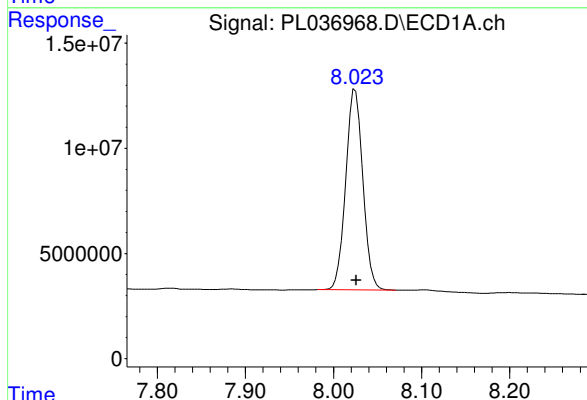

#28 Decachlorobiphenyl

R.T.: 8.025 min
Delta R.T.: 0.000 min
Response: 128924293
Conc: 19.82 ng/ml

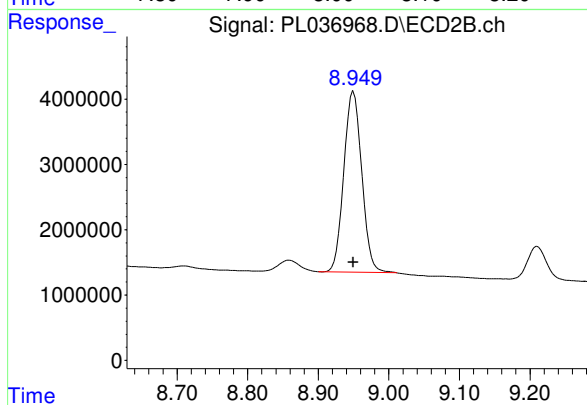

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: 0.000 min
Response: 48971927
Conc: 19.20 ng/ml