

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
 Data File : PL036910.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2018 13:13
 Operator : UA\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Manual Integrations
 APPROVED

UGO
 6/15/2018 11:54:15 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 00:53:38 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 14 16:13:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.341	3.938	143.5E6	52004607	20.182	20.342
28)	SA Decachlor...	8.026	8.950	137.8E6	54254847	21.185	21.268
Target Compounds							
10)	B gamma-Chl...	5.236	6.022	81607959	27504404	9.704m	9.888m
12)	B 4,4'-DDE	5.463	6.252	165.1E6	49313163	20.998m	20.099
13)	MA Dieldrin	5.587	6.398	164.5E6	53358753	20.481	20.733
19)	B Endosulfa...	6.495	7.159	123.6E6	44383810	20.444	20.460
20)	A Methoxychlor	6.760	7.488	329.9E6	122.5E6	103.935	101.126
21)	B Endrin ke...	6.978	7.623	134.5E6	40267506	20.516m	17.674

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
Data File : PL036910.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2018 13:13
Operator : UA\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
RESCHK


Manual Integrations
APPROVED

UGO
6/15/2018 11:54:15 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 00:53:38 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
Quant Title : GC Extractables
QLast Update : Thu Jun 14 16:13:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

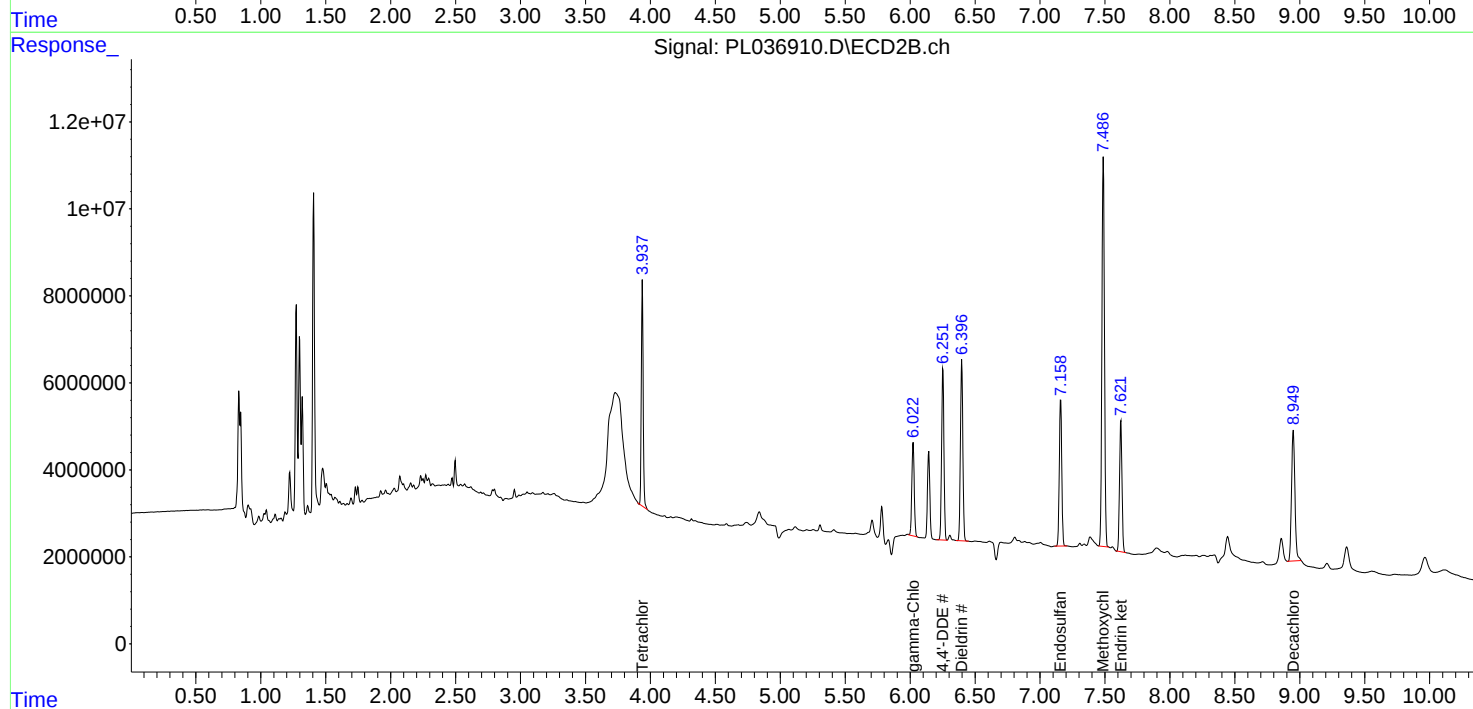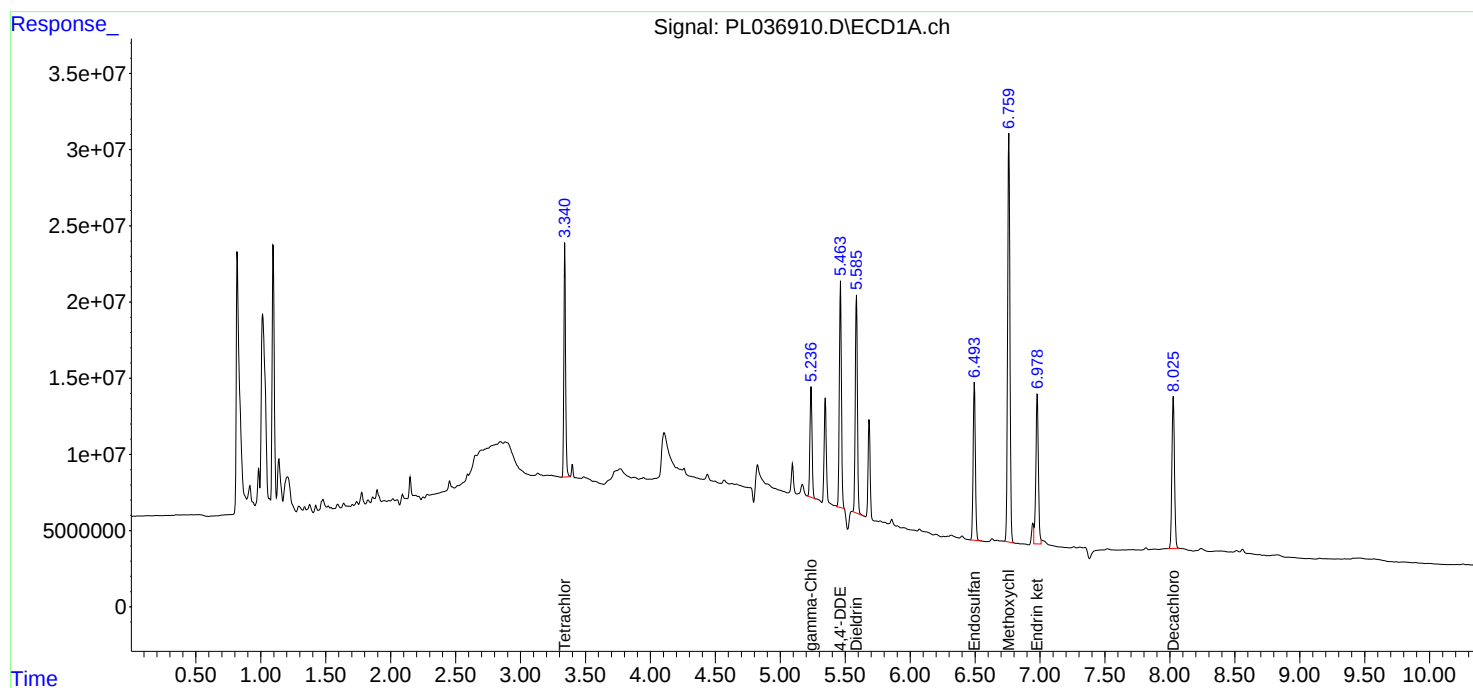

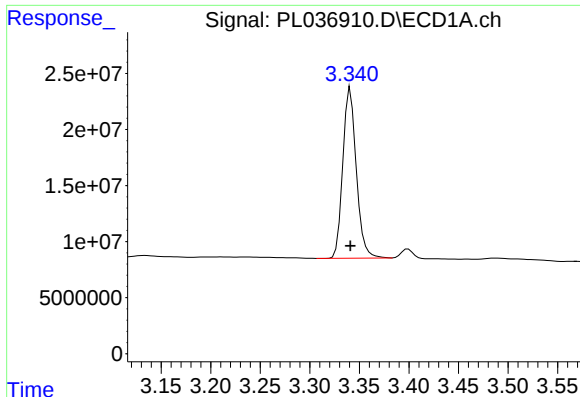


#1 Tetrachloro-m-xylene

R.T.: 3.341 min
Delta R.T.: 0.000 min
Response: 143517263
Conc: 20.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK


Manual Integrations
APPROVED

UGO
6/15/2018 11:54:15 AM

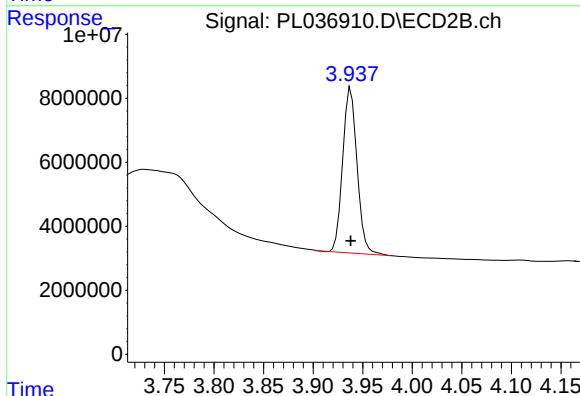


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: 0.000 min
Response: 52004607
Conc: 20.34 ng/ml

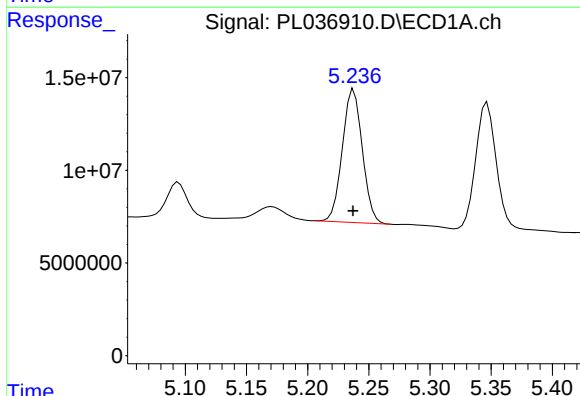


#10 gamma-Chlordane

R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 81607959
Conc: 9.70 ng/ml m

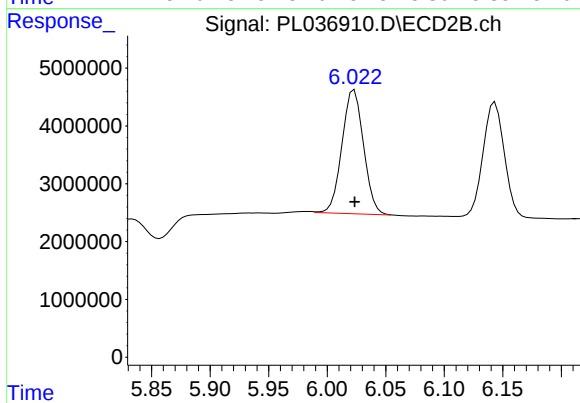

#10 gamma-Chlordane

R.T.: 6.022 min
Delta R.T.: -0.002 min
Response: 27504404
Conc: 9.89 ng/ml m

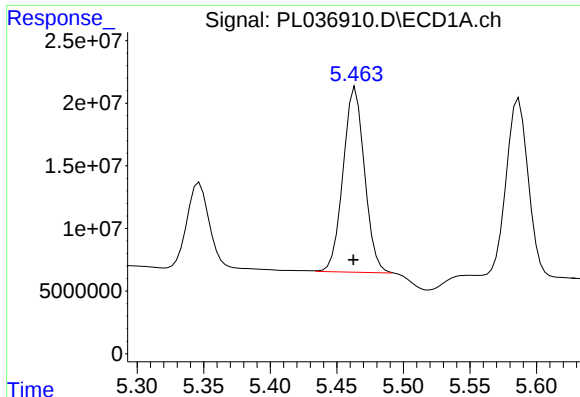


#12 4,4'-DDE

R.T.: 5.463 min
Delta R.T.: 0.000 min
Response: 165146342
Conc: 21.00 ng/ml m

Instrument :
ECD_L
ClientSampleId :
RESCHK


Manual Integrations
APPROVED

UGO
6/15/2018 11:54:15 AM

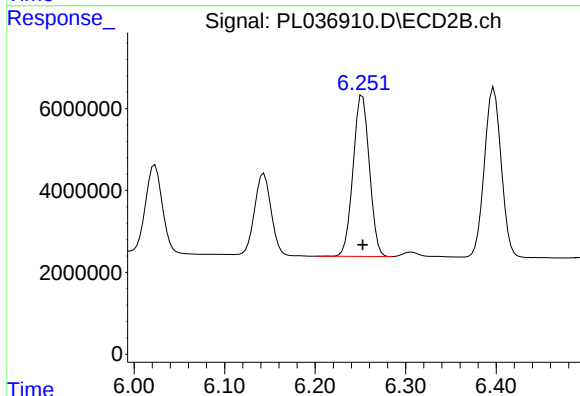


#12 4,4'-DDE

R.T.: 6.252 min
Delta R.T.: 0.000 min
Response: 49313163
Conc: 20.10 ng/ml

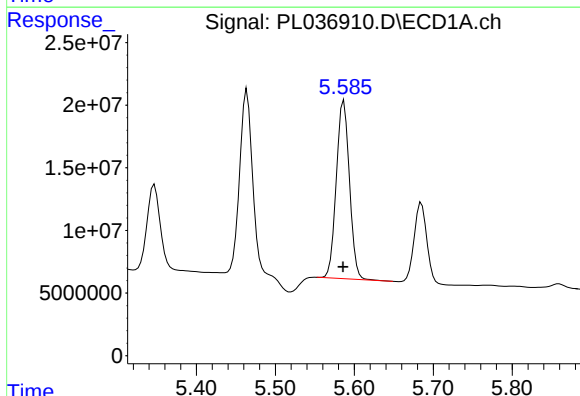


#13 Dieldrin

R.T.: 5.587 min
Delta R.T.: 0.000 min
Response: 164511653
Conc: 20.48 ng/ml

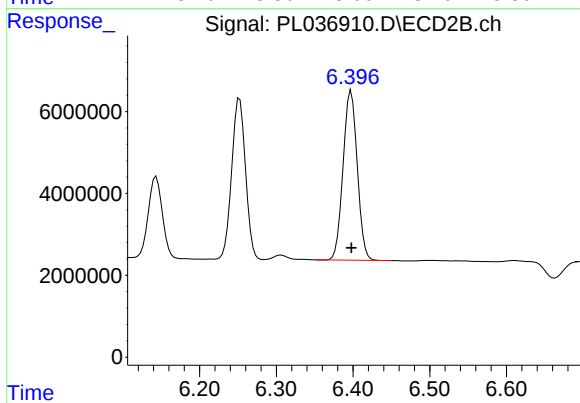

#13 Dieldrin

R.T.: 6.398 min
Delta R.T.: 0.000 min
Response: 53358753
Conc: 20.73 ng/ml

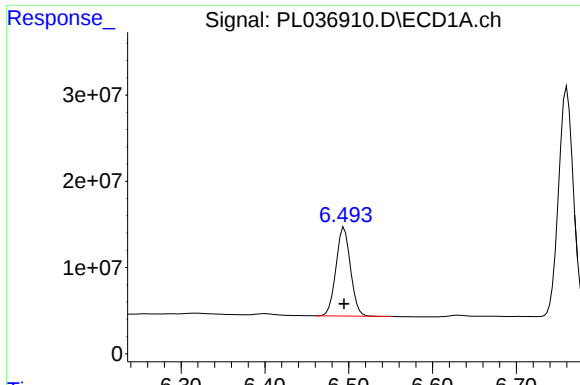


#19 Endosulfan Sulfate

R.T.: 6.495 min
Delta R.T.: 0.000 min
Response: 123630864
Conc: 20.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK


Manual Integrations
APPROVED

UGO
6/15/2018 11:54:15 AM

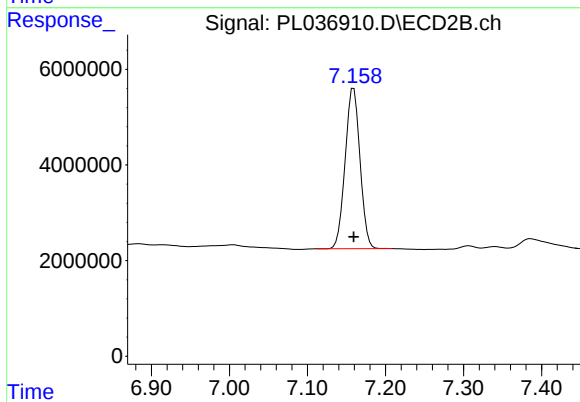


#19 Endosulfan Sulfate

R.T.: 7.159 min
Delta R.T.: 0.000 min
Response: 44383810
Conc: 20.46 ng/ml

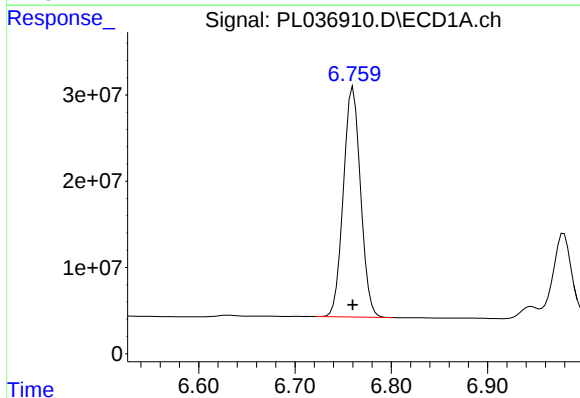


#20 Methoxychlor

R.T.: 6.760 min
Delta R.T.: 0.000 min
Response: 329897231
Conc: 103.93 ng/ml

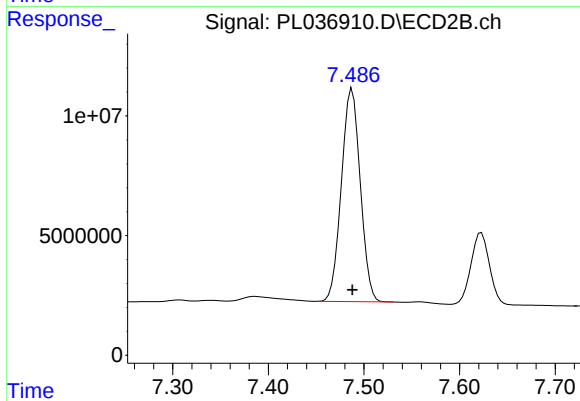

#20 Methoxychlor

R.T.: 7.488 min
Delta R.T.: 0.000 min
Response: 122494150
Conc: 101.13 ng/ml

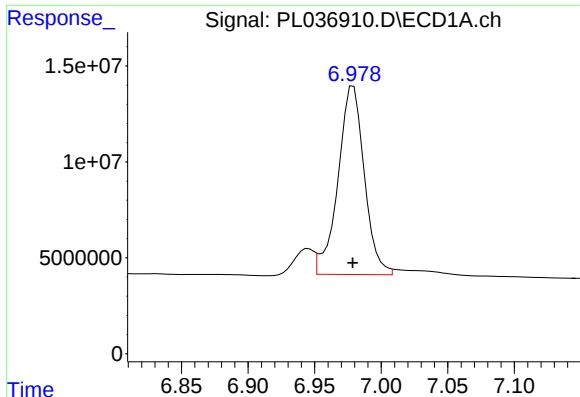


#21 Endrin ketone

R.T.: 6.978 min
Delta R.T.: 0.000 min
Response: 134496111
Conc: 20.52 ng/ml m

Instrument :
ECD_L
ClientSampleId :
RESCHK


Manual Integrations
APPROVED

UGO
6/15/2018 11:54:15 AM

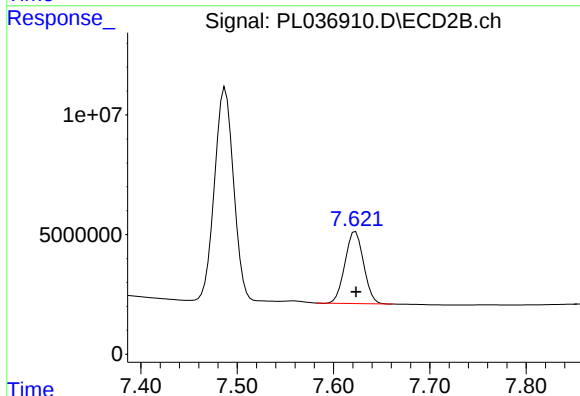


#21 Endrin ketone

R.T.: 7.623 min
Delta R.T.: 0.000 min
Response: 40267506
Conc: 17.67 ng/ml

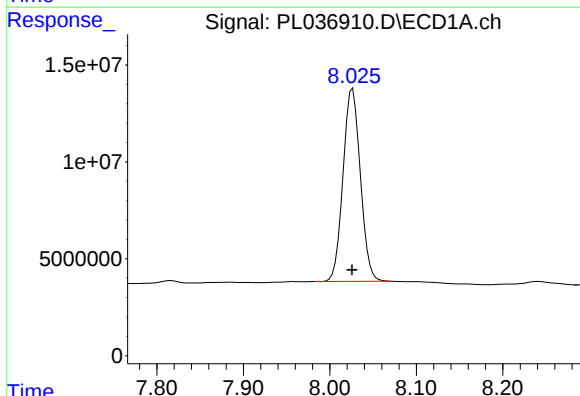

#28 Decachlorobiphenyl

R.T.: 8.026 min
Delta R.T.: 0.000 min
Response: 137826875
Conc: 21.18 ng/ml

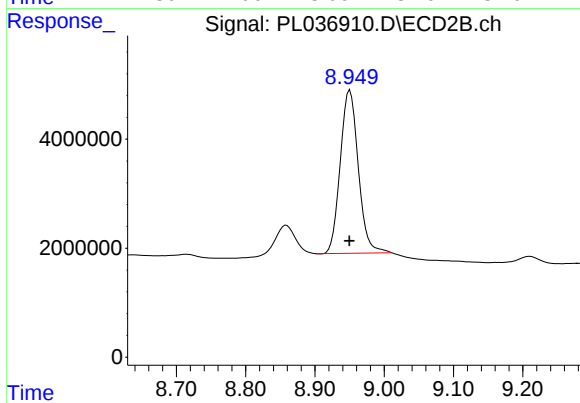

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: 0.000 min
Response: 54254847
Conc: 21.27 ng/ml