

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
 Data File : PL036916.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2018 14:37
 Operator : UA\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 15:37:51 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 14 15:36:33 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.340	3.938	711.9E6	251.0E6	95.156	96.393
28)	SA Decachlor...	8.025	8.950	589.3E6	223.4E6	92.295	90.432
Target Compounds							
23)	Chlordane-1	4.186	4.922	283.3E6	110.5E6	975.117	966.423
24)	Chlordane-2	4.680	5.384	293.7E6	113.3E6	929.956	949.083
25)	Chlordane-3	5.237	6.024	953.6E6	382.1E6	968.611	992.501
26)	Chlordane-4	5.293	6.099	868.4E6	450.6E6	986.772	981.073
27)	Chlordane-5	5.902	6.892	126.0E6	84724603	974.959	959.172



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
Data File : PL036916.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2018 14:37
Operator : UA\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 15:37:51 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
Quant Title : GC Extractables
QLast Update : Thu Jun 14 15:36:33 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

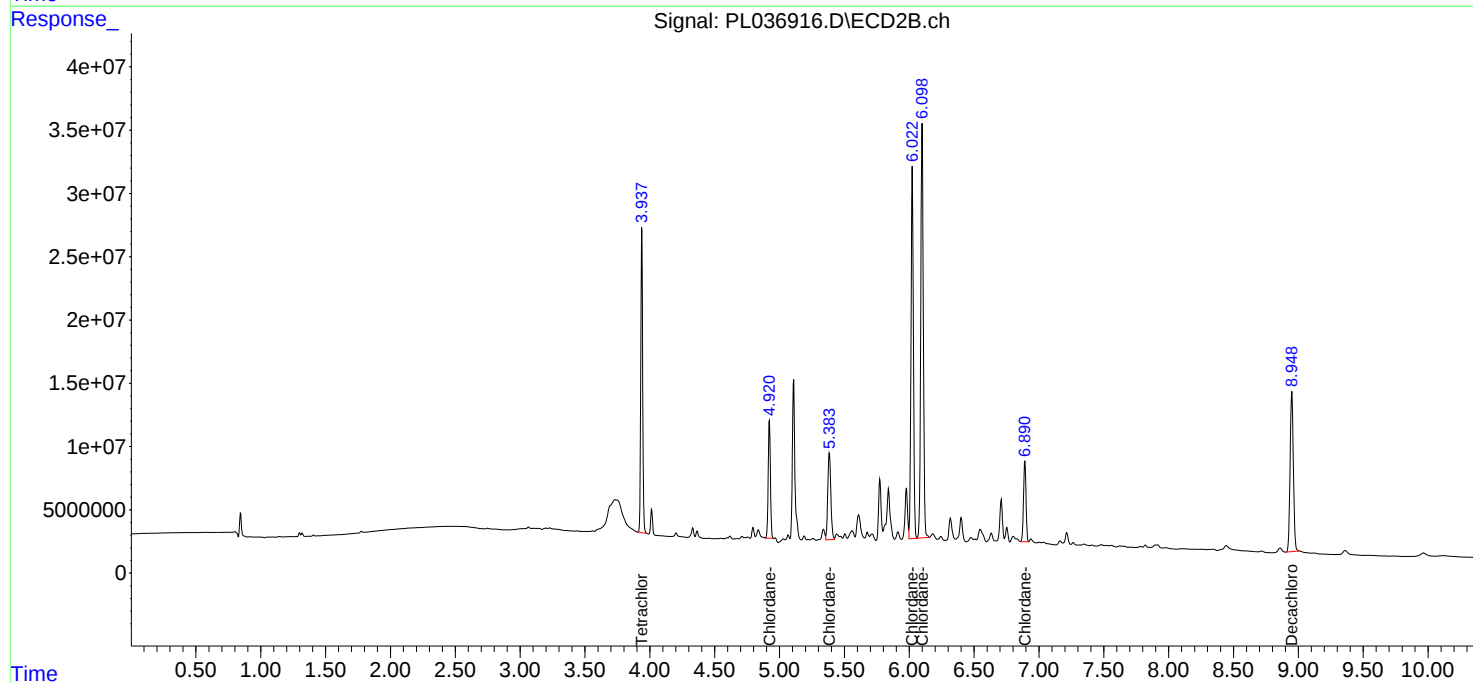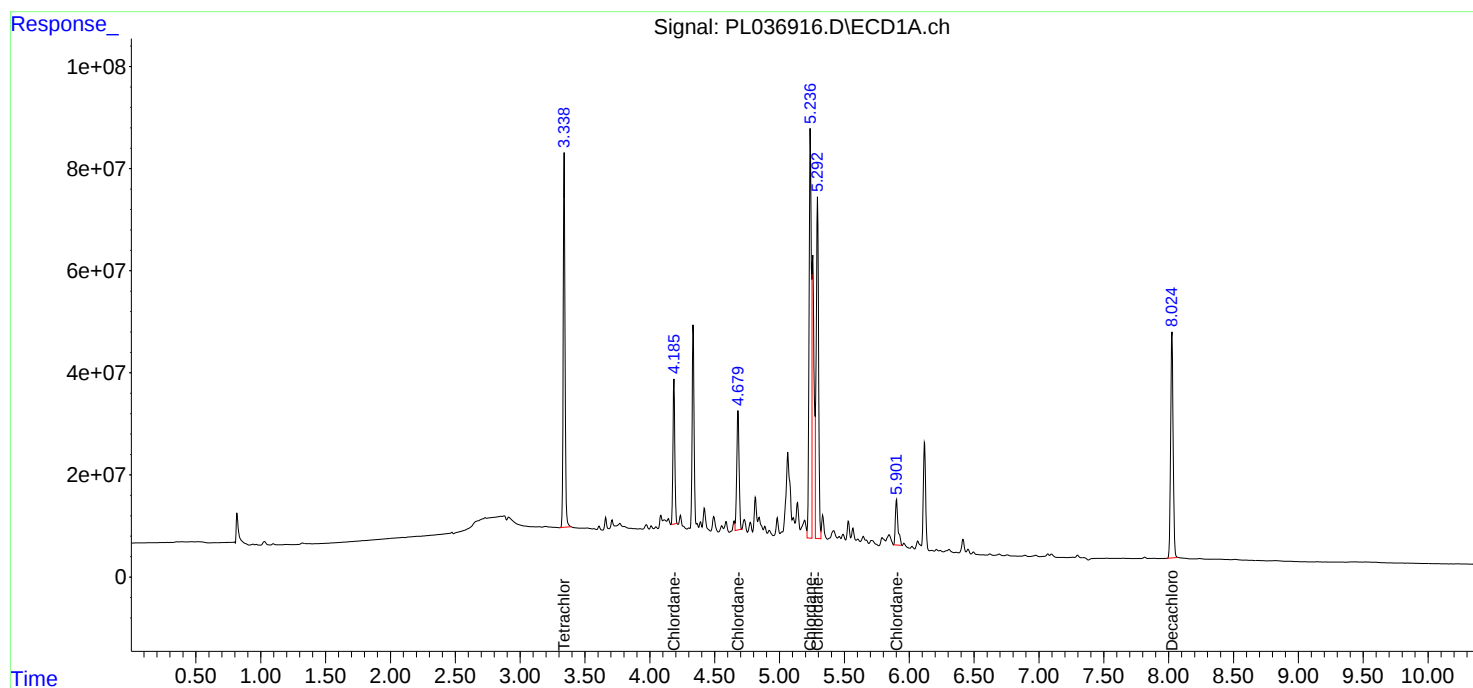


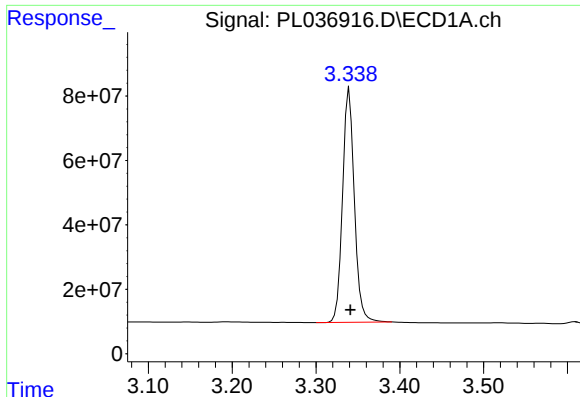

#1 Tetrachloro-m-xylene


R.T.: 3.340 min
Delta R.T.: -0.001 min
Response: 711896077
Conc: 95.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

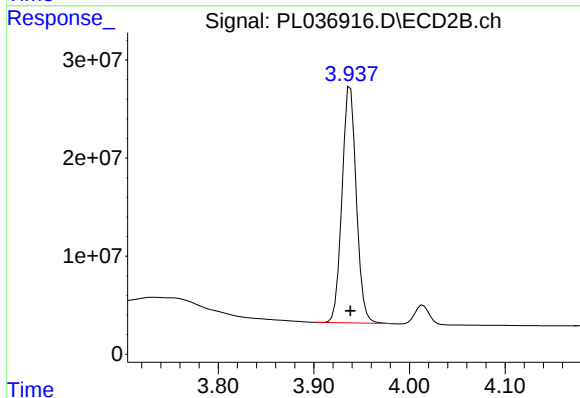


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: 0.000 min
Response: 251049619
Conc: 96.39 ng/ml

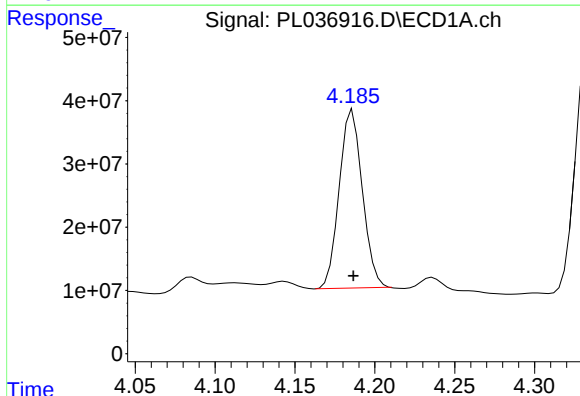


#23 Chlordane-1

R.T.: 4.186 min
Delta R.T.: 0.000 min
Response: 283328782
Conc: 975.12 ng/ml

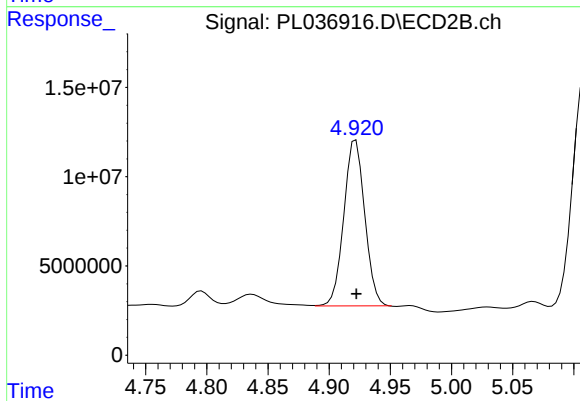

#23 Chlordane-1


R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 110514066
Conc: 966.42 ng/ml

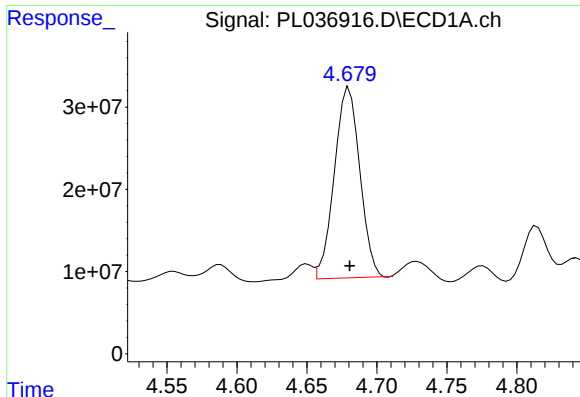

#24 Chlordane-2


R.T.: 4.680 min
Delta R.T.: 0.000 min
Response: 293672234
Conc: 929.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

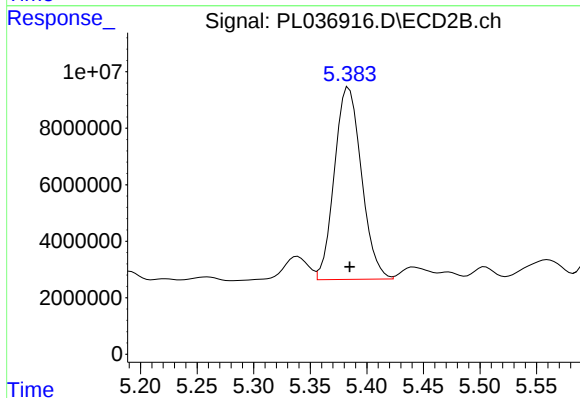


#24 Chlordane-2

R.T.: 5.384 min
Delta R.T.: 0.000 min
Response: 113261462
Conc: 949.08 ng/ml

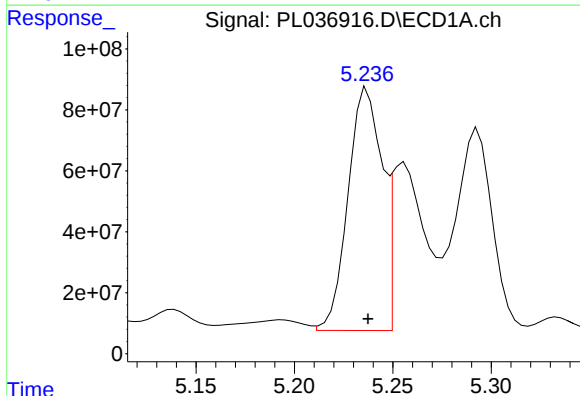


#25 Chlordane-3

R.T.: 5.237 min
Delta R.T.: 0.000 min
Response: 953583705
Conc: 968.61 ng/ml

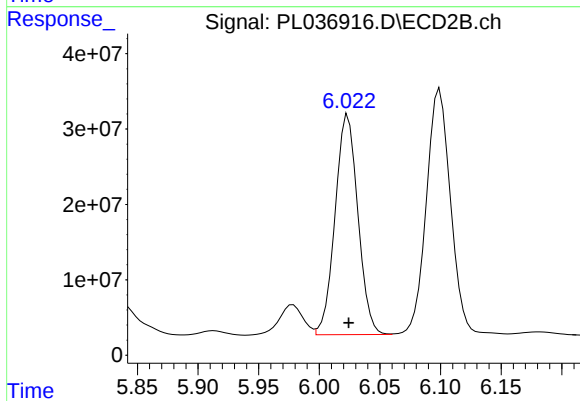

#25 Chlordane-3


R.T.: 6.024 min
Delta R.T.: 0.000 min
Response: 382140758
Conc: 992.50 ng/ml

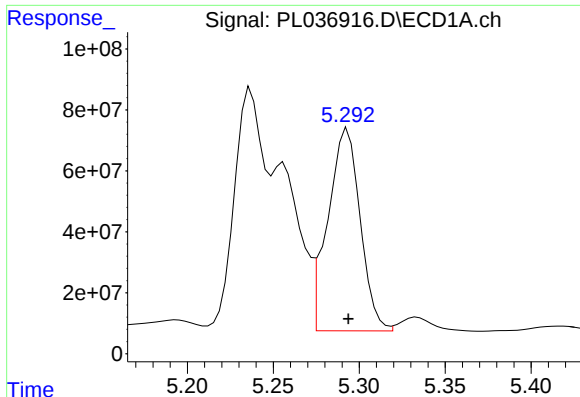

#26 Chlordane-4


R.T.: 5.293 min
Delta R.T.: 0.000 min
Response: 868362287
Conc: 986.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

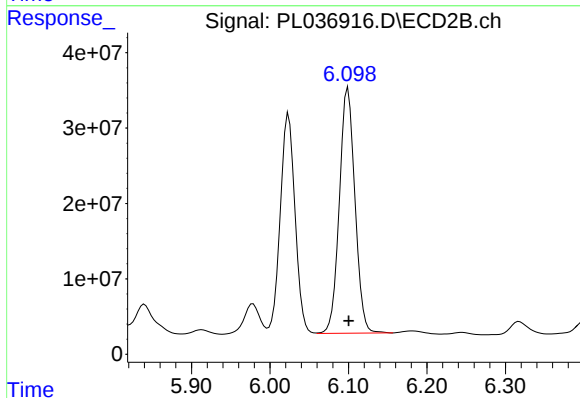


#26 Chlordane-4

R.T.: 6.099 min
Delta R.T.: 0.000 min
Response: 450577693
Conc: 981.07 ng/ml

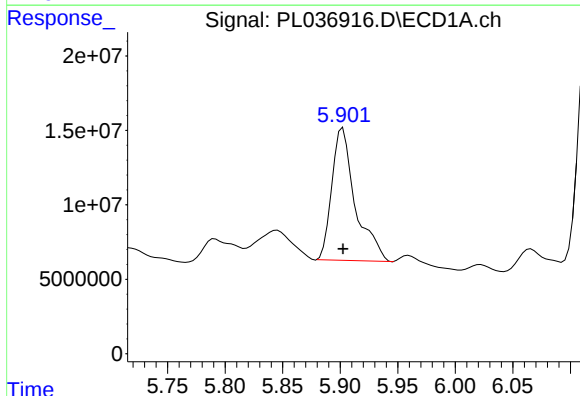


#27 Chlordane-5

R.T.: 5.902 min
Delta R.T.: 0.000 min
Response: 126040892
Conc: 974.96 ng/ml

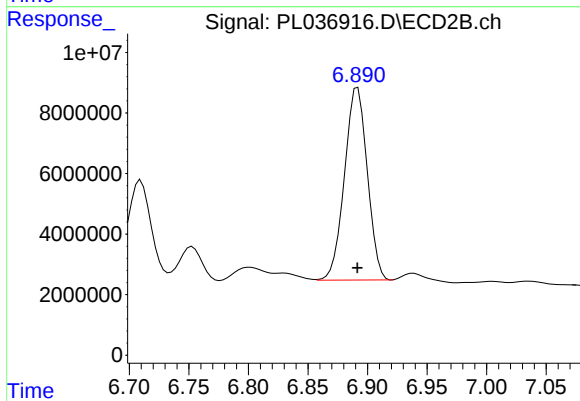

#27 Chlordane-5


R.T.: 6.892 min
Delta R.T.: 0.000 min
Response: 84724603
Conc: 959.17 ng/ml

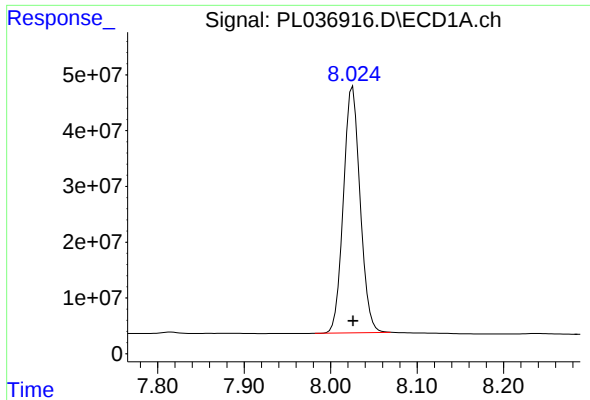

#28 Decachlorobiphenyl

R.T.: 8.025 min
Delta R.T.: 0.000 min
Response: 589308701
Conc: 92.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

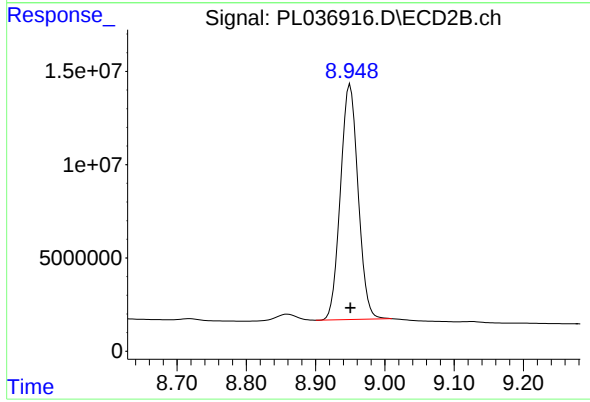

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: 0.000 min
Response: 223392600
Conc: 90.43 ng/ml