

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
 Data File : PL036917.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2018 14:52
 Operator : UA\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 15:38:00 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 14 15:36:33 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.341	3.938	540.2E6	188.9E6	72.213	72.531
28)	SA Decachlor...	8.025	8.951	453.9E6	172.0E6	71.095	69.627
Target Compounds							
23)	Chlordane-1	4.187	4.923	216.8E6	82610882	746.032	722.416
24)	Chlordane-2	4.681	5.385	225.8E6	85297657	715.137	714.758
25)	Chlordane-3	5.238	6.024	731.3E6	283.1E6	742.834	735.395
26)	Chlordane-4	5.294	6.100	642.5E6	335.1E6	730.109	729.743
27)	Chlordane-5	5.903	6.892	96320980	63839568	745.067	722.731



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
Data File : PL036917.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2018 14:52
Operator : UA\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 15:38:00 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
Quant Title : GC Extractables
QLast Update : Thu Jun 14 15:36:33 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

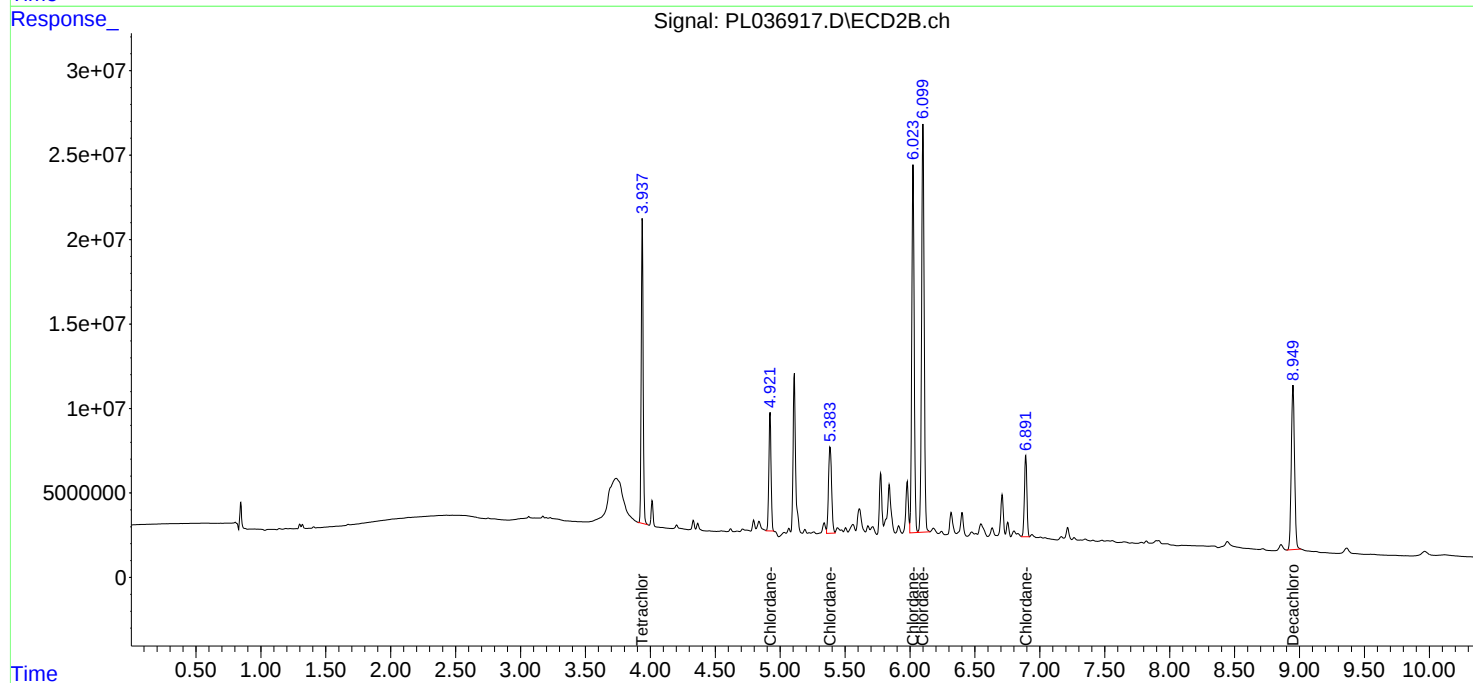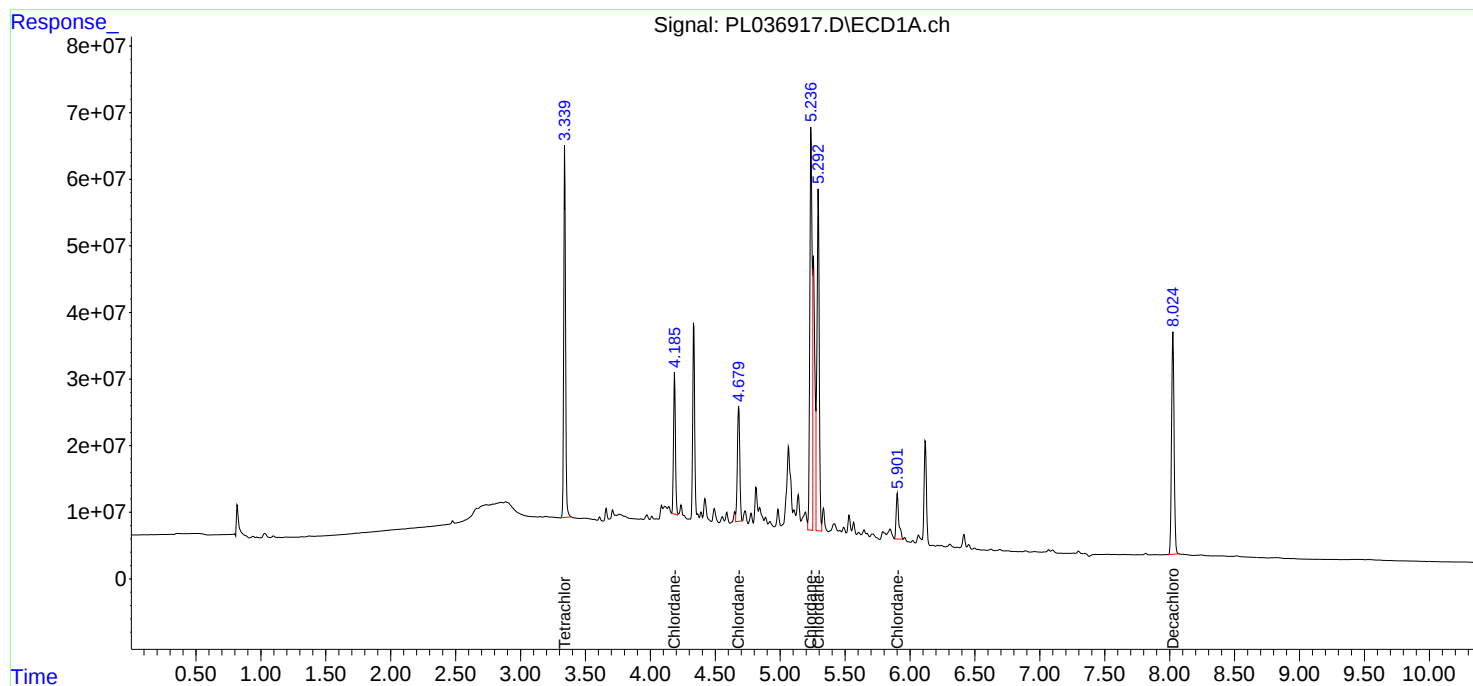


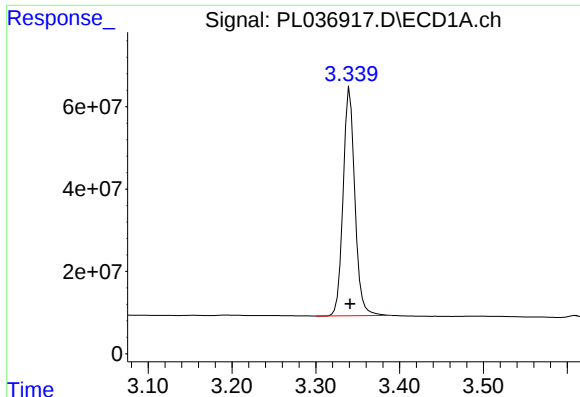

#1 Tetrachloro-m-xylene


R.T.: 3.341 min
Delta R.T.: 0.000 min
Response: 540247752
Conc: 72.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

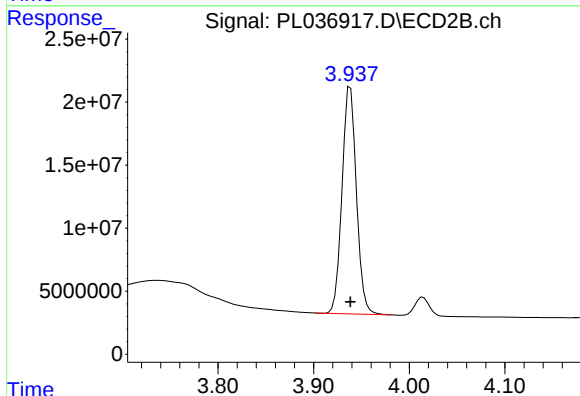


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: 0.000 min
Response: 188903388
Conc: 72.53 ng/ml

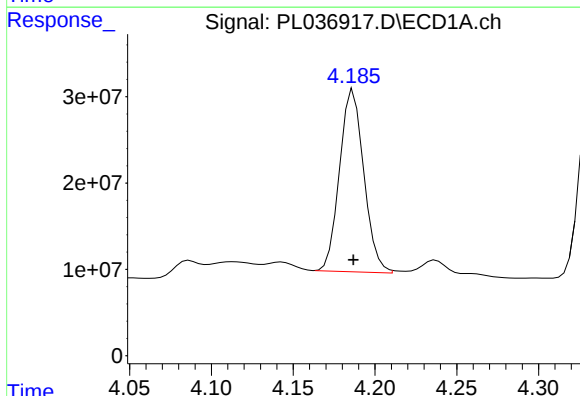


#23 Chlordane-1

R.T.: 4.187 min
Delta R.T.: 0.000 min
Response: 216766274
Conc: 746.03 ng/ml

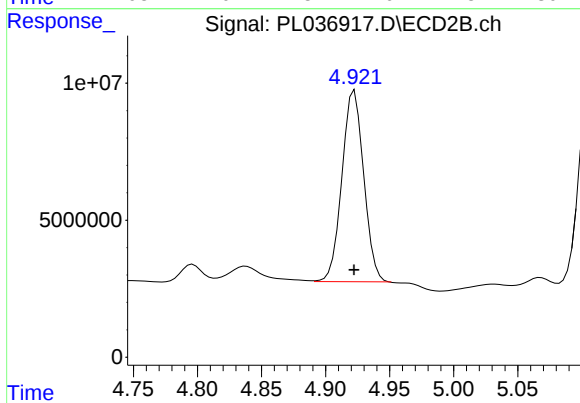

#23 Chlordane-1


R.T.: 4.923 min
Delta R.T.: 0.000 min
Response: 82610882
Conc: 722.42 ng/ml

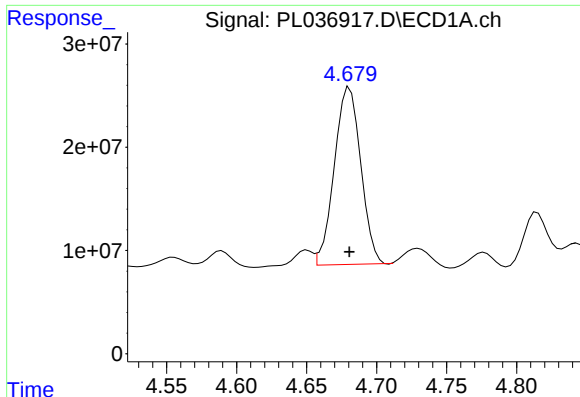

#24 Chlordane-2


R.T.: 4.681 min
Delta R.T.: 0.000 min
Response: 225834400
Conc: 715.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

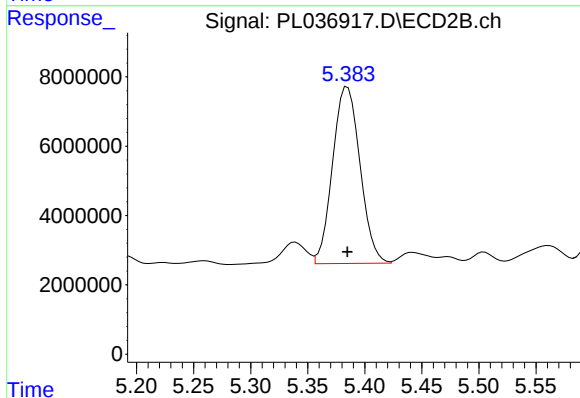


#24 Chlordane-2

R.T.: 5.385 min
Delta R.T.: 0.000 min
Response: 85297657
Conc: 714.76 ng/ml

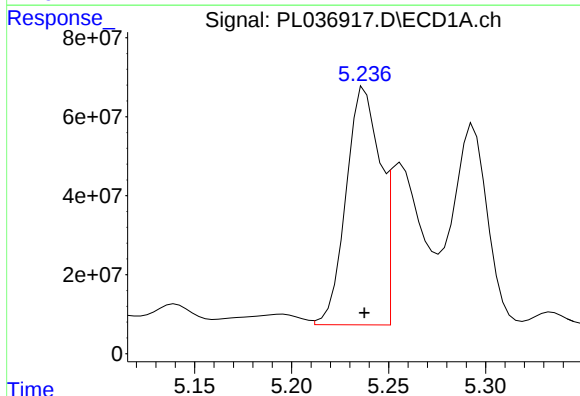


#25 Chlordane-3

R.T.: 5.238 min
Delta R.T.: 0.000 min
Response: 731309404
Conc: 742.83 ng/ml

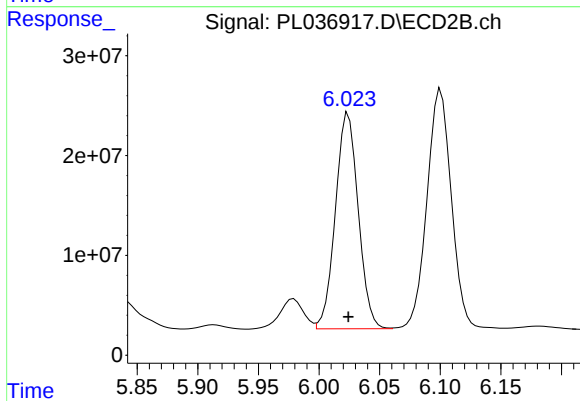

#25 Chlordane-3


R.T.: 6.024 min
Delta R.T.: 0.000 min
Response: 283147763
Conc: 735.40 ng/ml

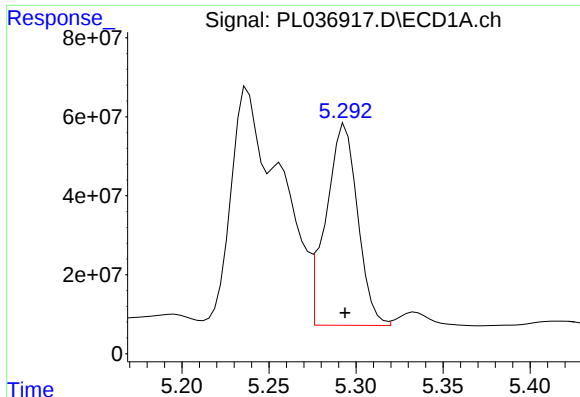

#26 Chlordane-4


R.T.: 5.294 min
Delta R.T.: 0.000 min
Response: 642497753
Conc: 730.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

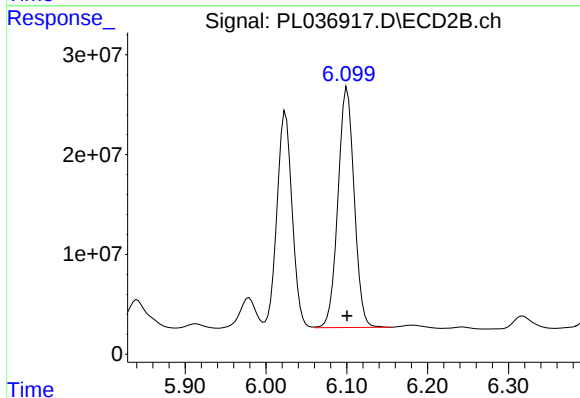


#26 Chlordane-4

R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 335149302
Conc: 729.74 ng/ml

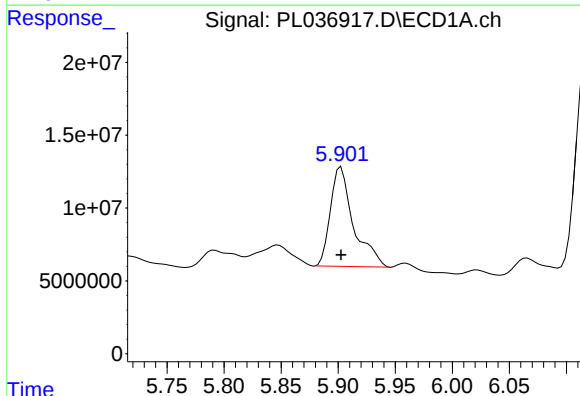


#27 Chlordane-5

R.T.: 5.903 min
Delta R.T.: 0.000 min
Response: 96320980
Conc: 745.07 ng/ml

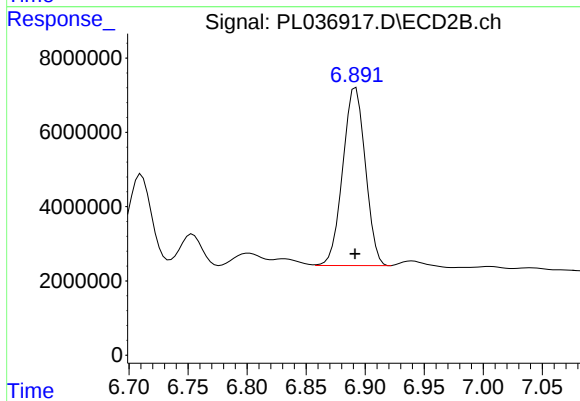

#27 Chlordane-5


R.T.: 6.892 min
Delta R.T.: 0.000 min
Response: 63839568
Conc: 722.73 ng/ml

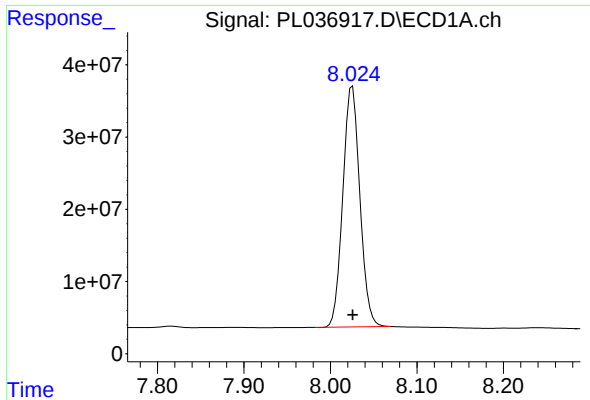

#28 Decachlorobiphenyl

R.T.: 8.025 min
Delta R.T.: 0.000 min
Response: 453942201
Conc: 71.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

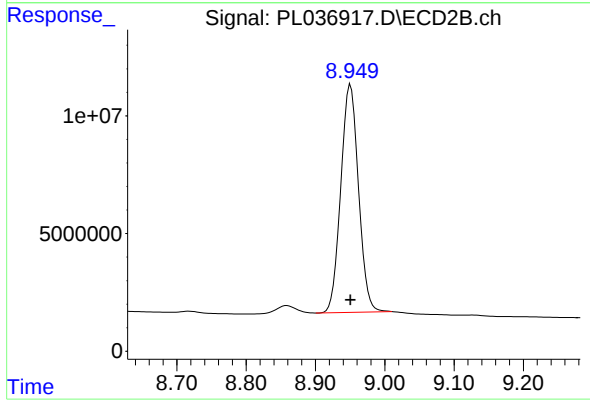

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: 0.000 min
Response: 171999049
Conc: 69.63 ng/ml