

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
 Data File : PL036919.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2018 15:20
 Operator : UA\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 15:38:07 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 14 15:36:33 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.340	3.939	176.9E6	61178552	23.647	23.490
28)	SA Decachlor...	8.026	8.950	156.9E6	61309018	24.579	24.819
Target Compounds							
23)	Chlordane-1	4.187	4.923	67633493	26630509	232.770	232.879
24)	Chlordane-2	4.680	5.385	76181788	29000098	241.241	243.008
25)	Chlordane-3	5.238	6.024	225.7E6	89734453	229.264	233.060
26)	Chlordane-4	5.293	6.100	207.8E6	108.5E6	236.144	236.351
27)	Chlordane-5	5.902	6.892	29536629	20599088	228.473	233.203



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
Data File : PL036919.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2018 15:20
Operator : UA\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 15:38:07 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
Quant Title : GC Extractables
QLast Update : Thu Jun 14 15:36:33 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

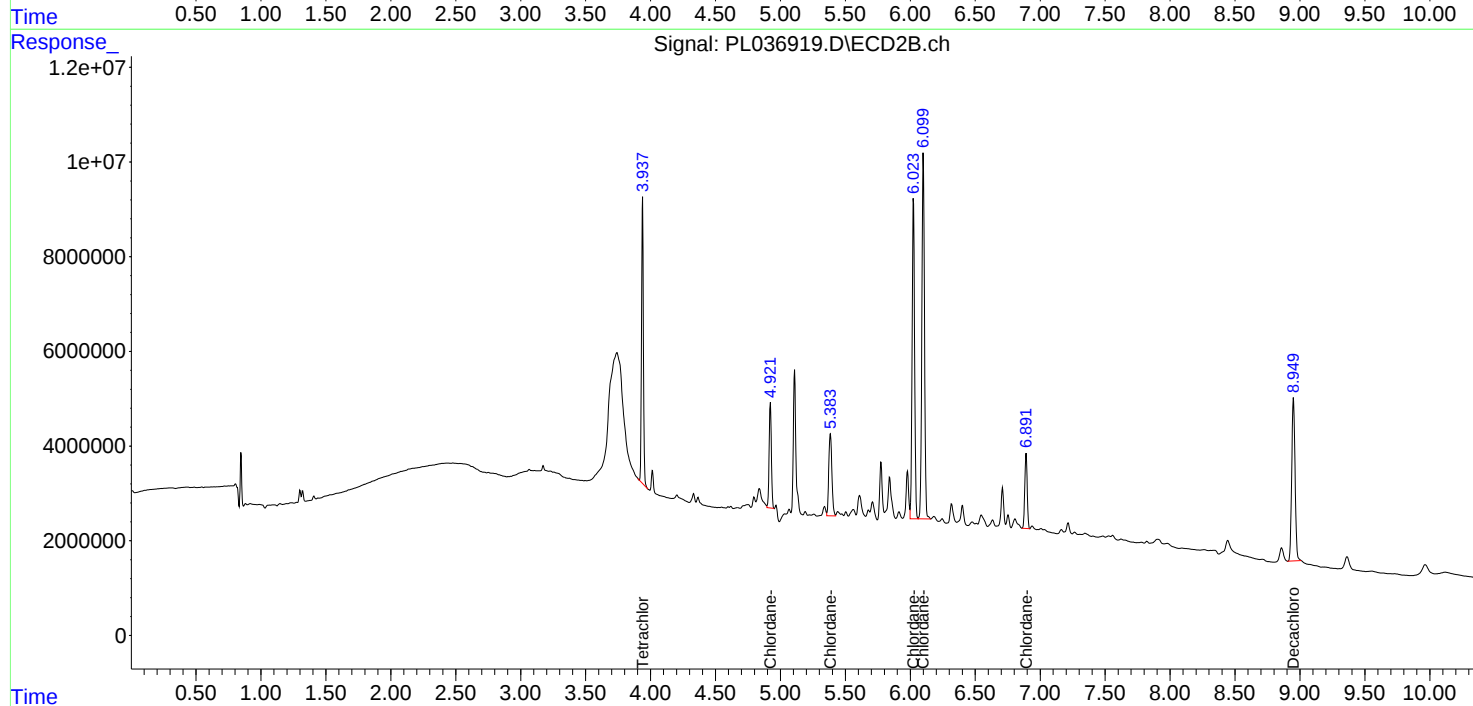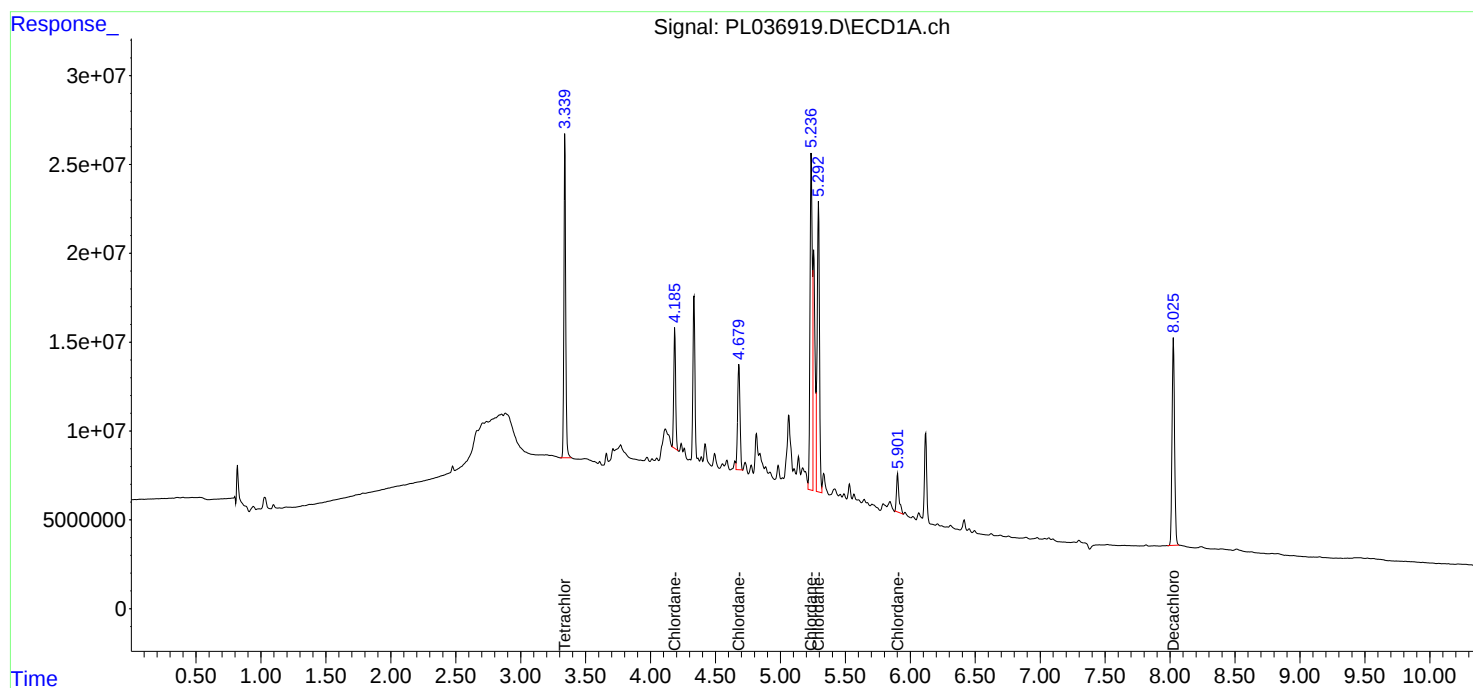


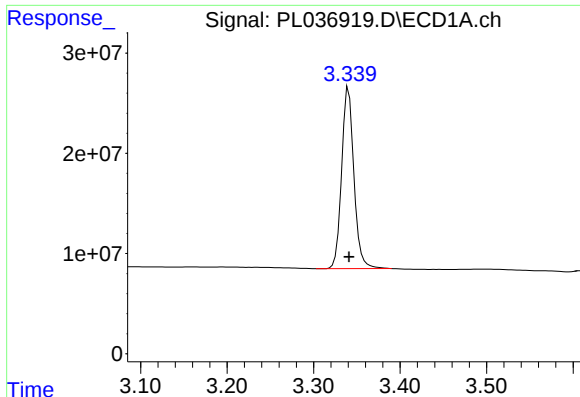

#1 Tetrachloro-m-xylene


R.T.: 3.340 min
Delta R.T.: 0.000 min
Response: 176908454
Conc: 23.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

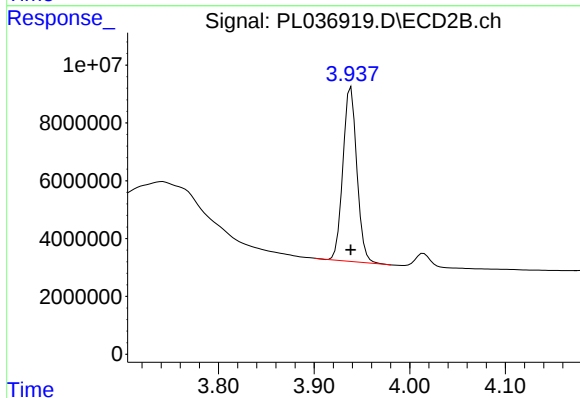


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 61178552
Conc: 23.49 ng/ml

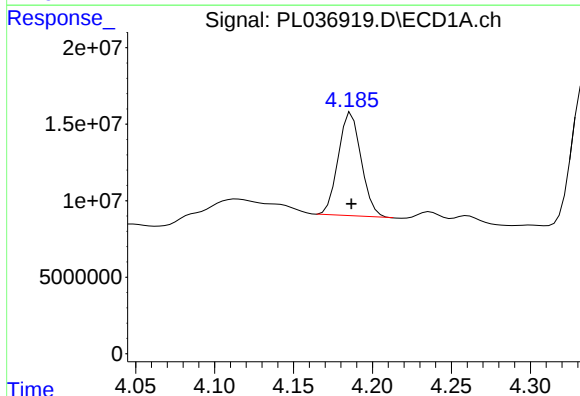


#23 Chlordane-1

R.T.: 4.187 min
Delta R.T.: 0.000 min
Response: 67633493
Conc: 232.77 ng/ml

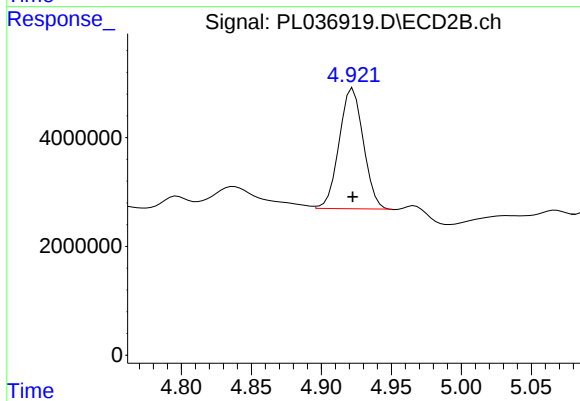

#23 Chlordane-1


R.T.: 4.923 min
Delta R.T.: 0.000 min
Response: 26630509
Conc: 232.88 ng/ml

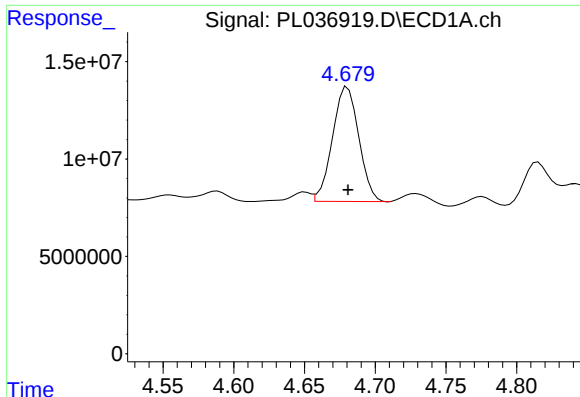

#24 Chlordane-2


R.T.: 4.680 min
Delta R.T.: 0.000 min
Response: 76181788
Conc: 241.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

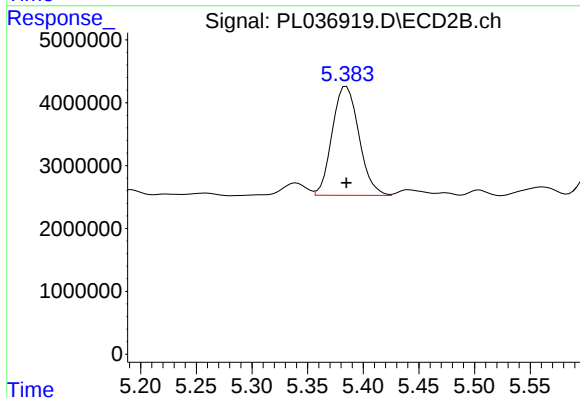


#24 Chlordane-2

R.T.: 5.385 min
Delta R.T.: 0.000 min
Response: 29000098
Conc: 243.01 ng/ml

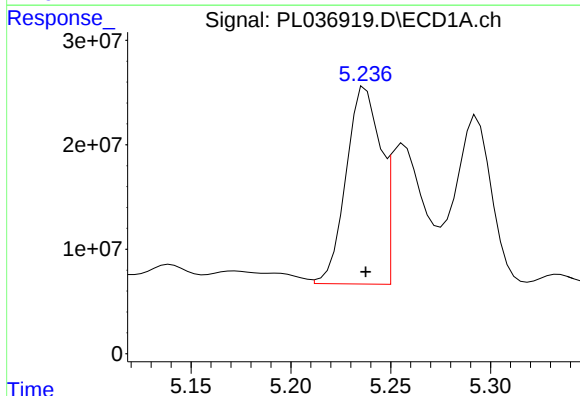


#25 Chlordane-3

R.T.: 5.238 min
Delta R.T.: 0.000 min
Response: 225706970
Conc: 229.26 ng/ml

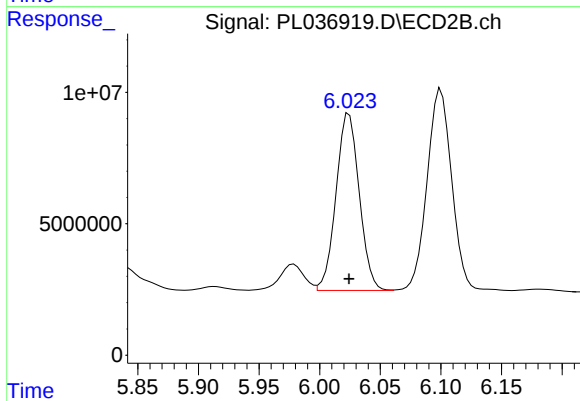

#25 Chlordane-3


R.T.: 6.024 min
Delta R.T.: 0.000 min
Response: 89734453
Conc: 233.06 ng/ml

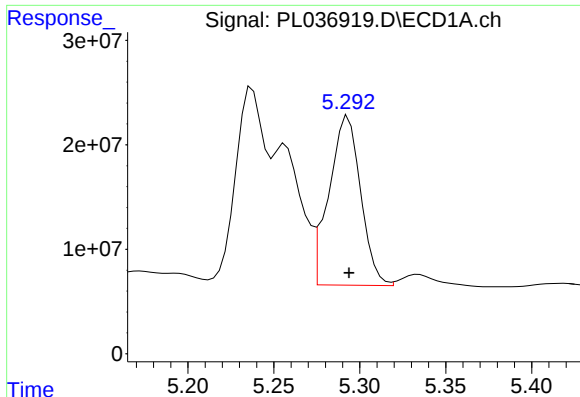

#26 Chlordane-4


R.T.: 5.293 min
Delta R.T.: 0.000 min
Response: 207807330
Conc: 236.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

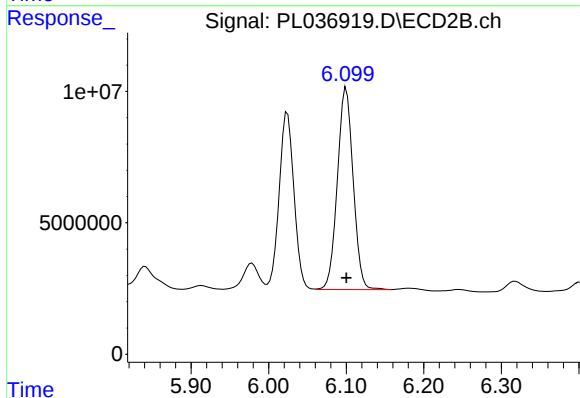


#26 Chlordane-4

R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 108549190
Conc: 236.35 ng/ml

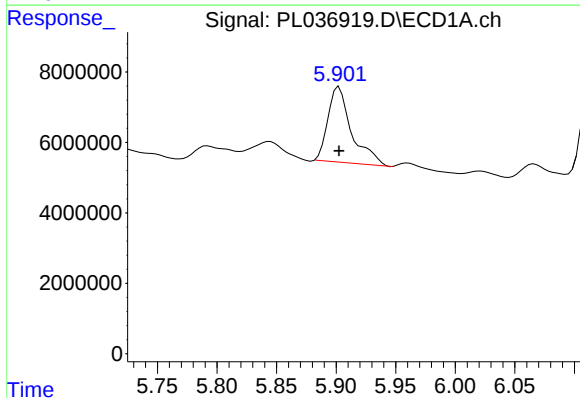


#27 Chlordane-5

R.T.: 5.902 min
Delta R.T.: 0.000 min
Response: 29536629
Conc: 228.47 ng/ml

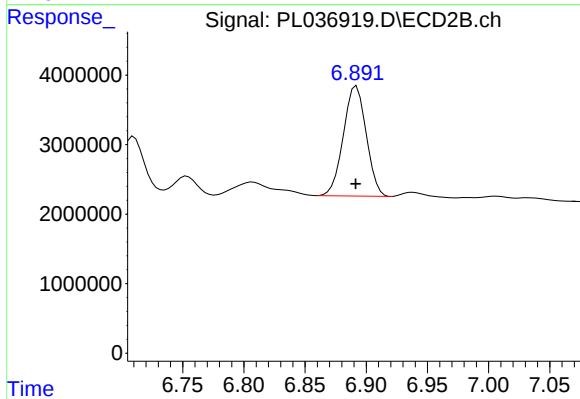

#27 Chlordane-5


R.T.: 6.892 min
Delta R.T.: 0.000 min
Response: 20599088
Conc: 233.20 ng/ml

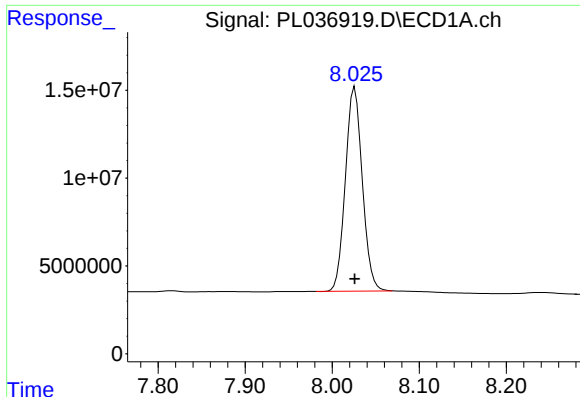

#28 Decachlorobiphenyl

R.T.: 8.026 min
Delta R.T.: 0.000 min
Response: 156939702
Conc: 24.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

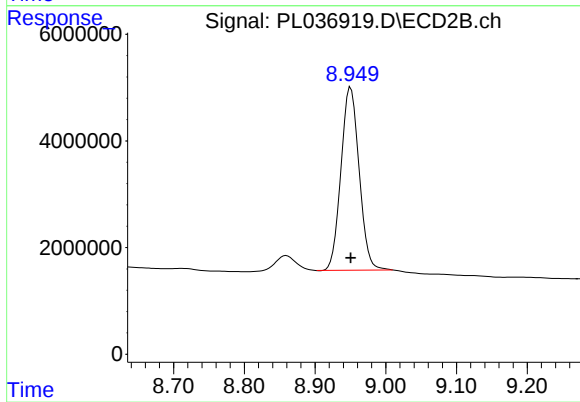

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: 0.000 min
Response: 61309018
Conc: 24.82 ng/ml