

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
 Data File : PL036927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2018 17:29
 Operator : UA\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL061418CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 00:53:49 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 14 16:13:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.340	3.938	372.7E6	130.7E6	52.411	51.142
28)	SA Decachlor...	8.025	8.950	314.7E6	121.8E6	48.366	47.729
Target Compounds							
23)	Chlordane-1	4.187	4.922	147.2E6	57751512	510.907	509.640
24)	Chlordane-2	4.680	5.384	157.3E6	60200960	512.065	518.637
25)	Chlordane-3	5.238	6.023	489.4E6	194.7E6	520.574	520.567
26)	Chlordane-4	5.294	6.099	438.2E6	232.4E6	515.727	522.062
27)	Chlordane-5	5.902	6.891	64576516	44374171	517.716	526.320



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
Data File : PL036927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2018 17:29
Operator : UA\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL061418CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 00:53:49 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
Quant Title : GC Extractables
QLast Update : Thu Jun 14 16:13:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

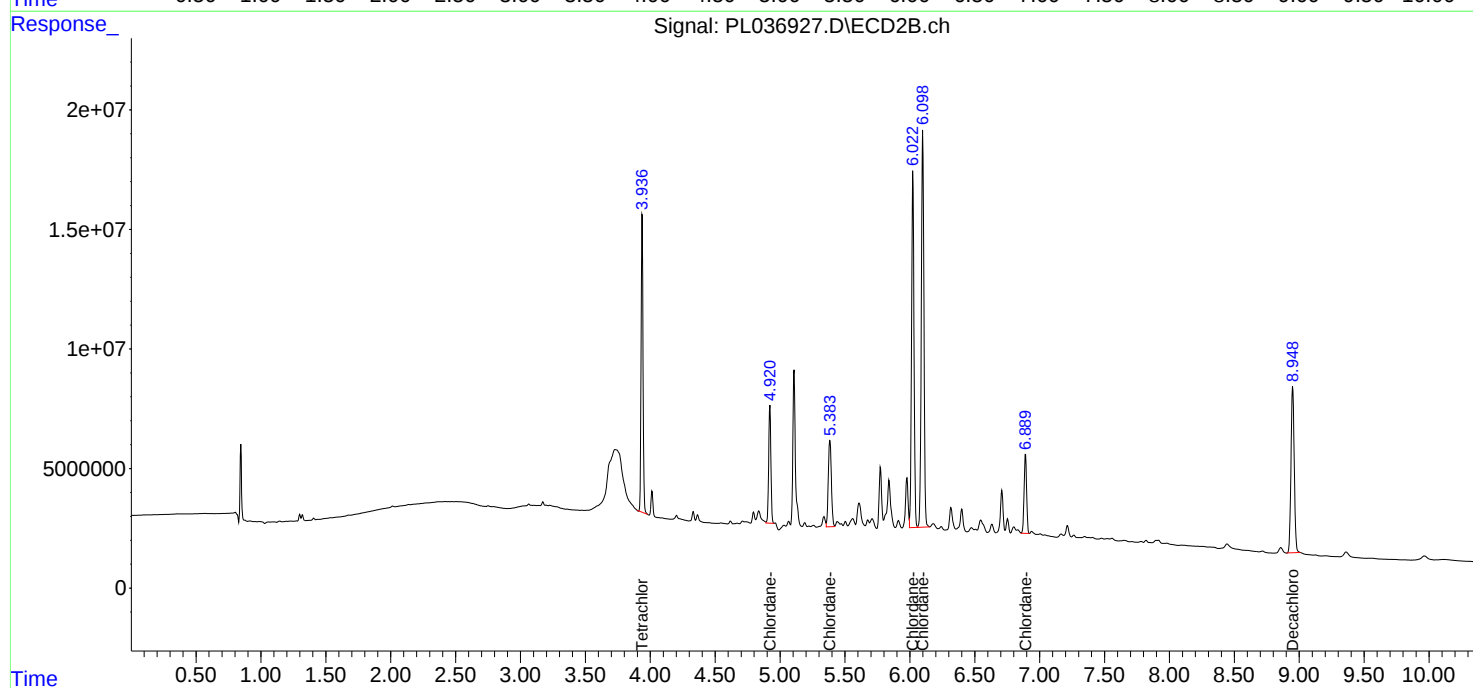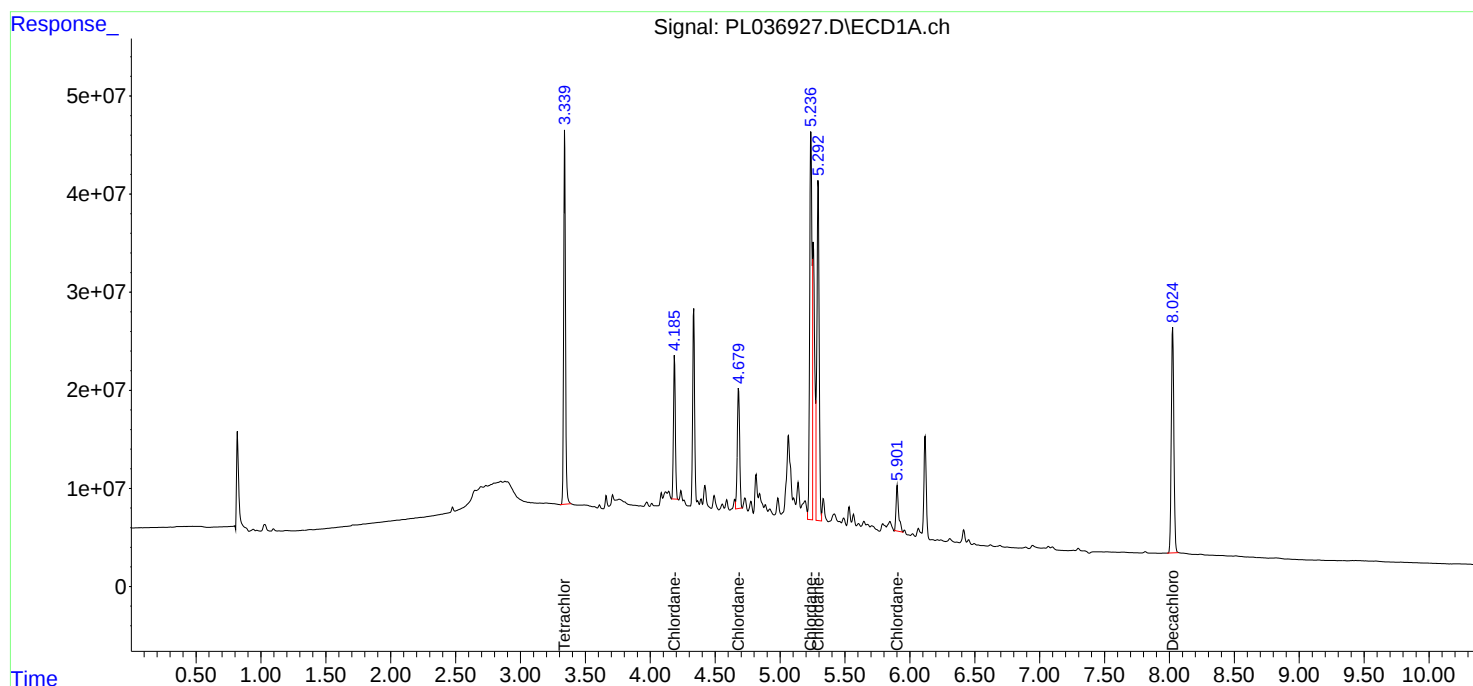


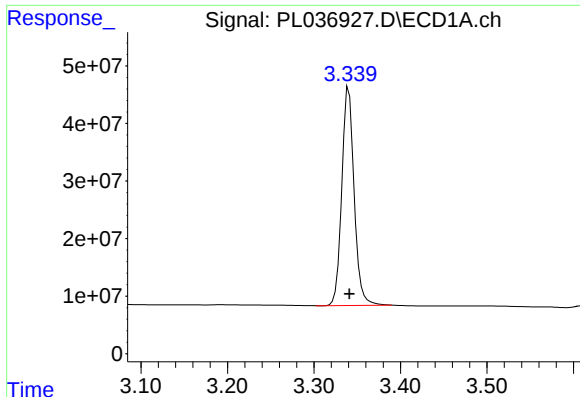

#1 Tetrachloro-m-xylene


R.T.: 3.340 min
Delta R.T.: 0.000 min
Response: 372708231
Conc: 52.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL061418CHLOR

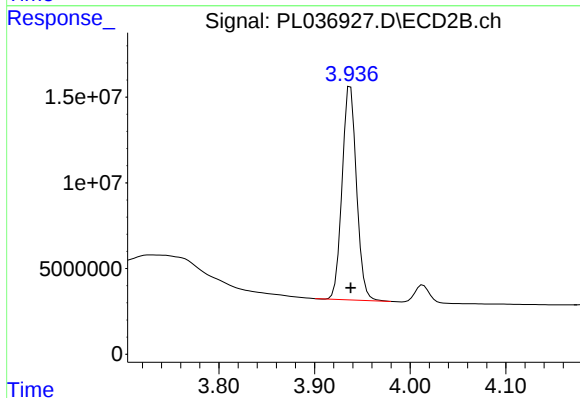


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: 0.000 min
Response: 130745993
Conc: 51.14 ng/ml

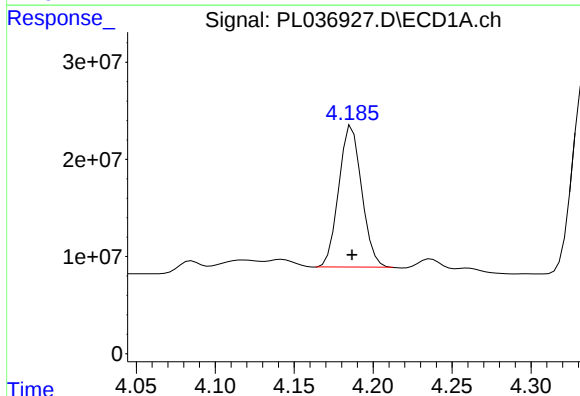


#23 Chlordane-1

R.T.: 4.187 min
Delta R.T.: 0.000 min
Response: 147211222
Conc: 510.91 ng/ml

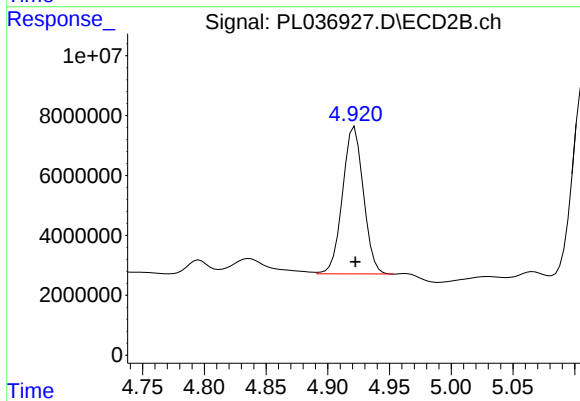

#23 Chlordane-1


R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 57751512
Conc: 509.64 ng/ml

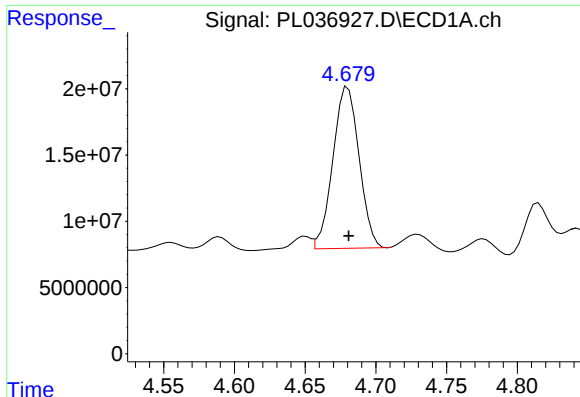

#24 Chlordane-2


R.T.: 4.680 min
Delta R.T.: 0.000 min
Response: 157295810
Conc: 512.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL061418CHLOR

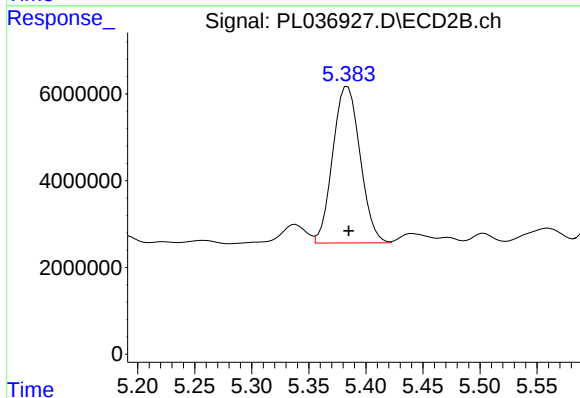


#24 Chlordane-2

R.T.: 5.384 min
Delta R.T.: 0.000 min
Response: 60200960
Conc: 518.64 ng/ml

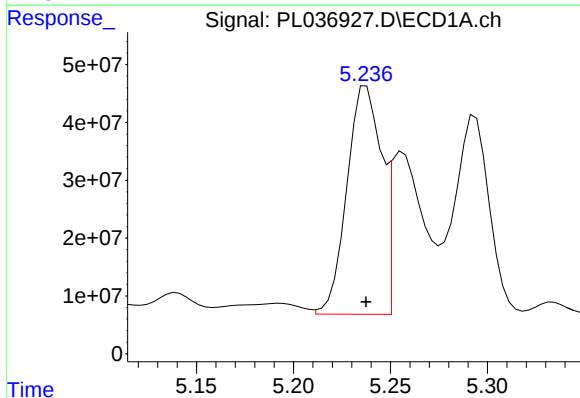


#25 Chlordane-3

R.T.: 5.238 min
Delta R.T.: 0.000 min
Response: 489353701
Conc: 520.57 ng/ml

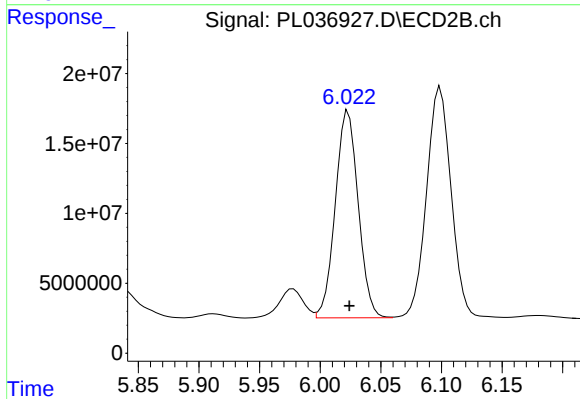

#25 Chlordane-3


R.T.: 6.023 min
Delta R.T.: -0.001 min
Response: 194747187
Conc: 520.57 ng/ml

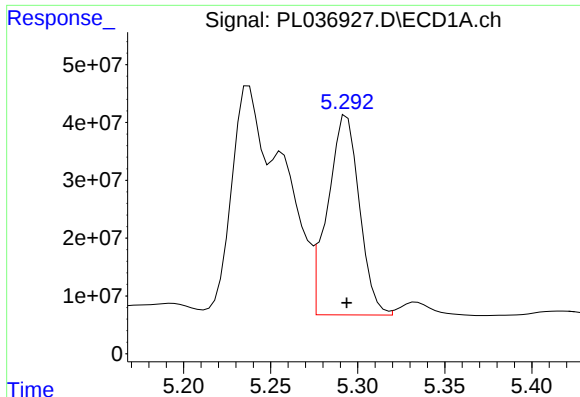

#26 Chlordane-4


R.T.: 5.294 min
Delta R.T.: 0.000 min
Response: 438224840
Conc: 515.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL061418CHLOR

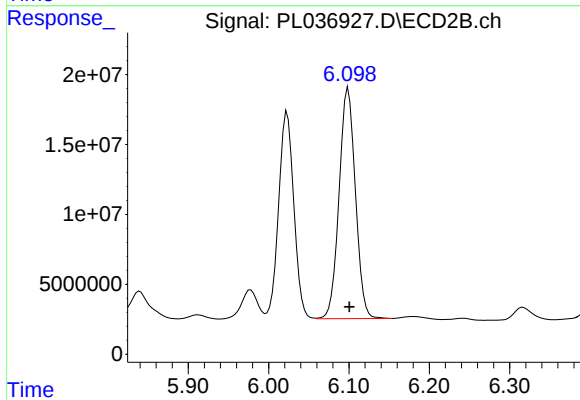


#26 Chlordane-4

R.T.: 6.099 min
Delta R.T.: -0.001 min
Response: 232445383
Conc: 522.06 ng/ml

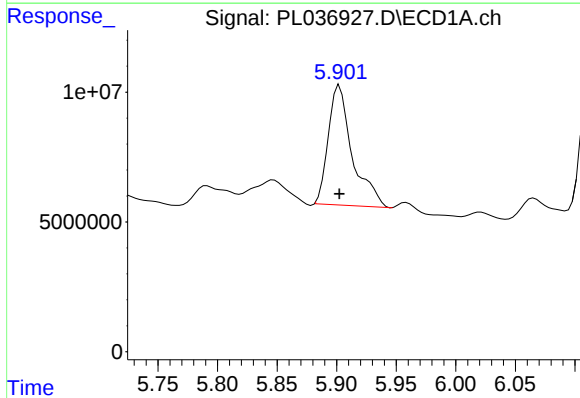


#27 Chlordane-5

R.T.: 5.902 min
Delta R.T.: 0.000 min
Response: 64576516
Conc: 517.72 ng/ml

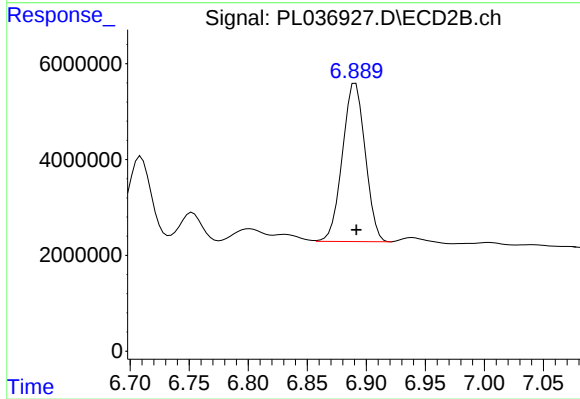

#27 Chlordane-5


R.T.: 6.891 min
Delta R.T.: 0.000 min
Response: 44374171
Conc: 526.32 ng/ml

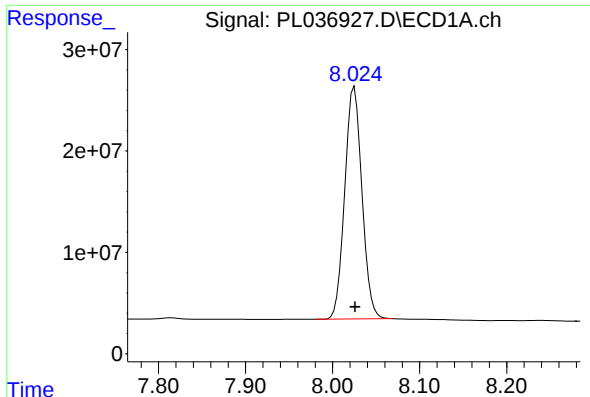

#28 Decachlorobiphenyl

R.T.: 8.025 min
Delta R.T.: 0.000 min
Response: 314665134
Conc: 48.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL061418CHLOR

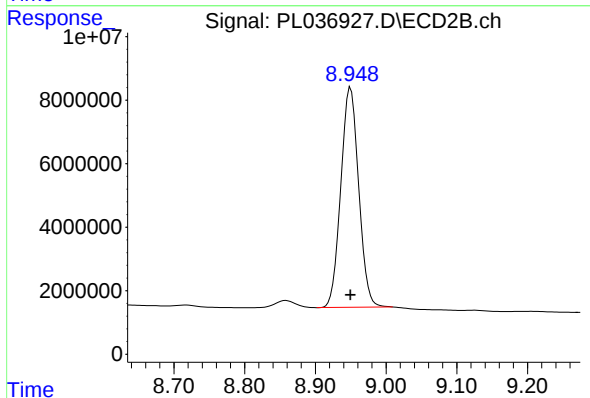

#28 Decachlorobiphenyl

R.T.: 8.950 min
Delta R.T.: 0.000 min
Response: 121755282
Conc: 47.73 ng/ml