

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
 Data File : PL036936.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2018 19:35
 Operator : UA\AJ
 Sample : J3502-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20180367-SITE-WATER

Manual Integrations
 APPROVED

UGO
 6/15/2018 11:54:45 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 02:35:32 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 14 16:13:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.341	3.937	109.8E6	42916034	15.440	16.787m
28)	SA Decachlor...	8.025	8.951	97914029	74321724	15.050	29.135m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
Data File : PL036936.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2018 19:35
Operator : UA\AJ
Sample : J3502-01
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20180367-SITE-WATER


Manual Integrations
APPROVED

UGO
6/15/2018 11:54:45 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 02:35:32 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
Quant Title : GC Extractables
QLast Update : Thu Jun 14 16:13:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

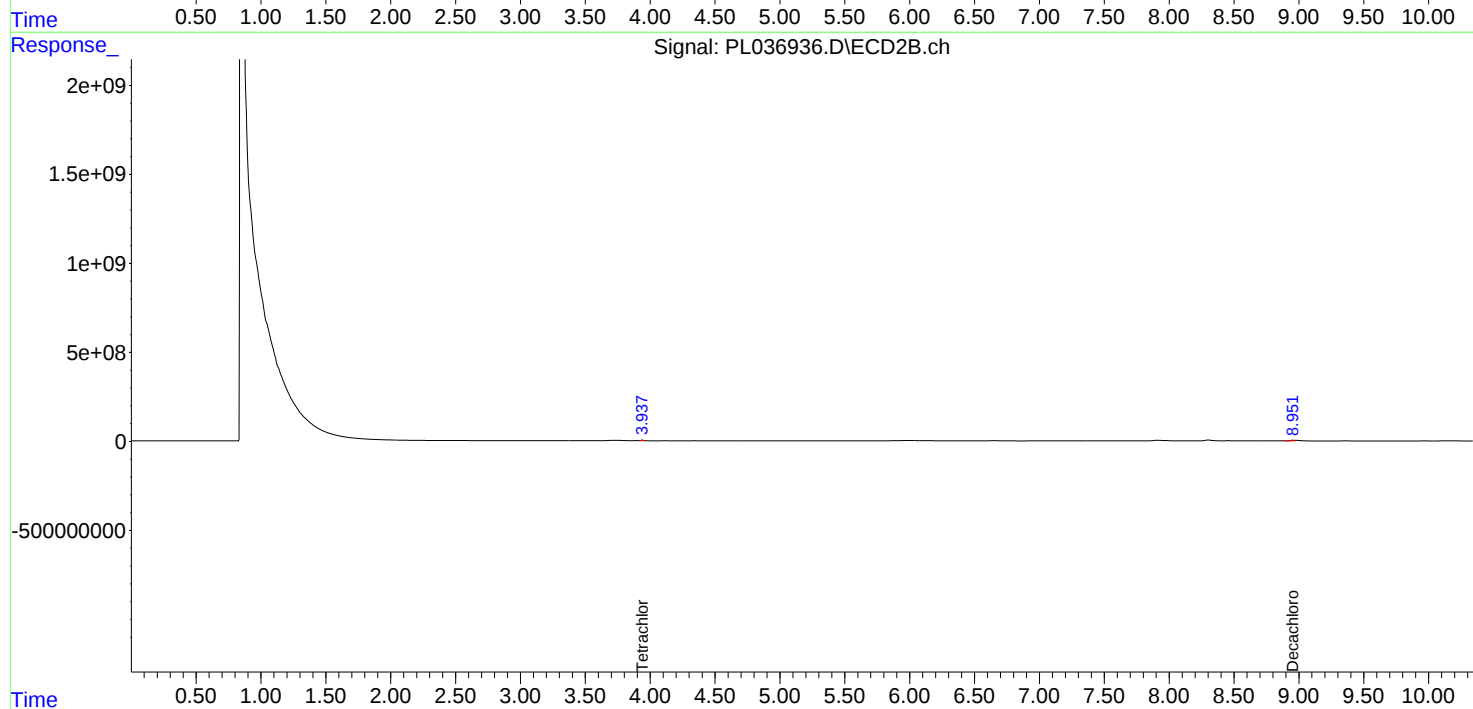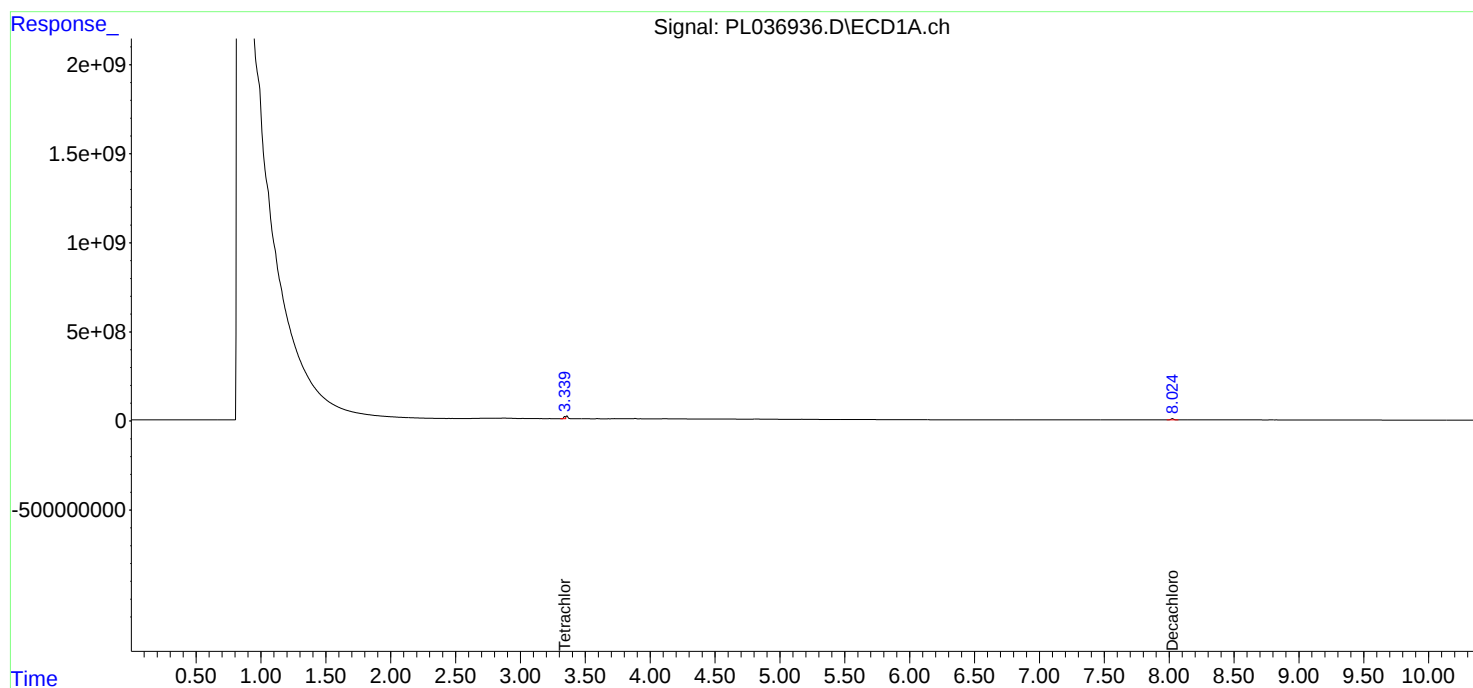

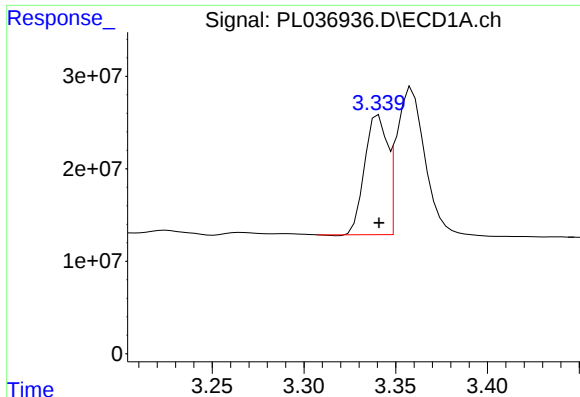


#1 Tetrachloro-m-xylene

R.T.: 3.341 min
Delta R.T.: 0.000 min
Response: 109795156
Conc: 15.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
20180367-SITE-WATER


Manual Integrations
APPROVED

UGO
6/15/2018 11:54:45 AM

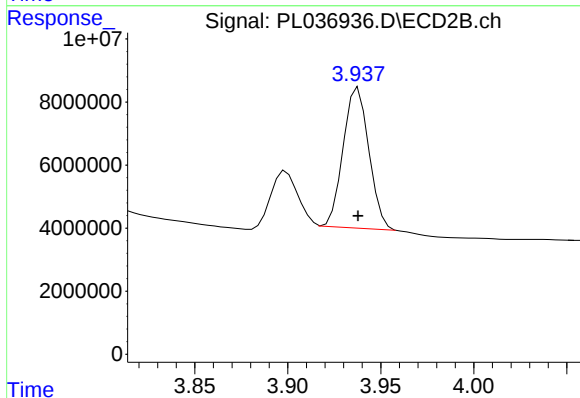


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: -0.001 min
Response: 42916034
Conc: 16.79 ng/ml m

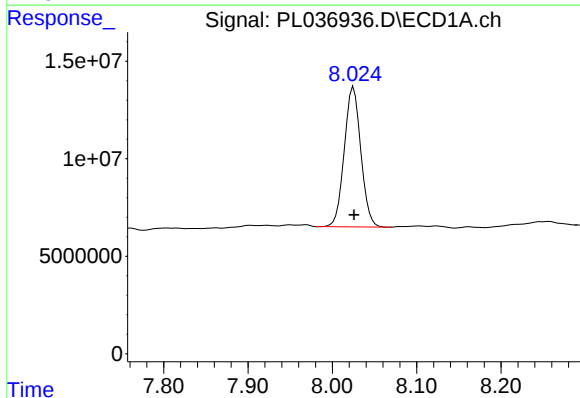

#28 Decachlorobiphenyl

R.T.: 8.025 min
Delta R.T.: 0.000 min
Response: 97914029
Conc: 15.05 ng/ml

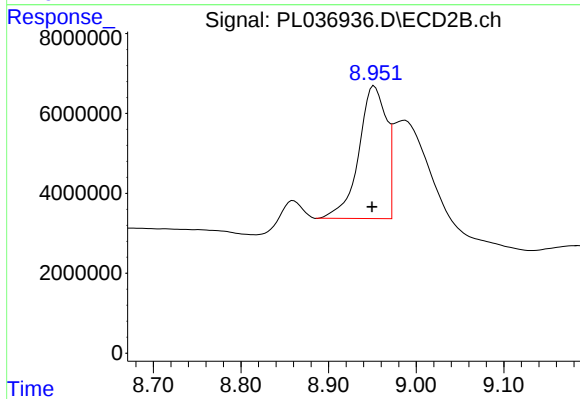

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: 0.001 min
Response: 74321724
Conc: 29.13 ng/ml m