

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
 Data File : PL036951.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2018 23:06
 Operator : UA\AJ
 Sample : J3459-02
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MH-RO-341

Manual Integrations
 APPROVED

UGO
 6/15/2018 11:55:15 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 02:36:34 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 14 16:13:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.340	3.936	139.1E6	51646524	19.560	20.202m
28)	SA Decachlor...	8.024	8.948	102.5E6	40618441	15.761	15.923

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061418\
Data File : PL036951.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2018 23:06
Operator : UA\AJ
Sample : J3459-02
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MH-RO-341


Manual Integrations
APPROVED

UGO
6/15/2018 11:55:15 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 02:36:34 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
Quant Title : GC Extractables
QLast Update : Thu Jun 14 16:13:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

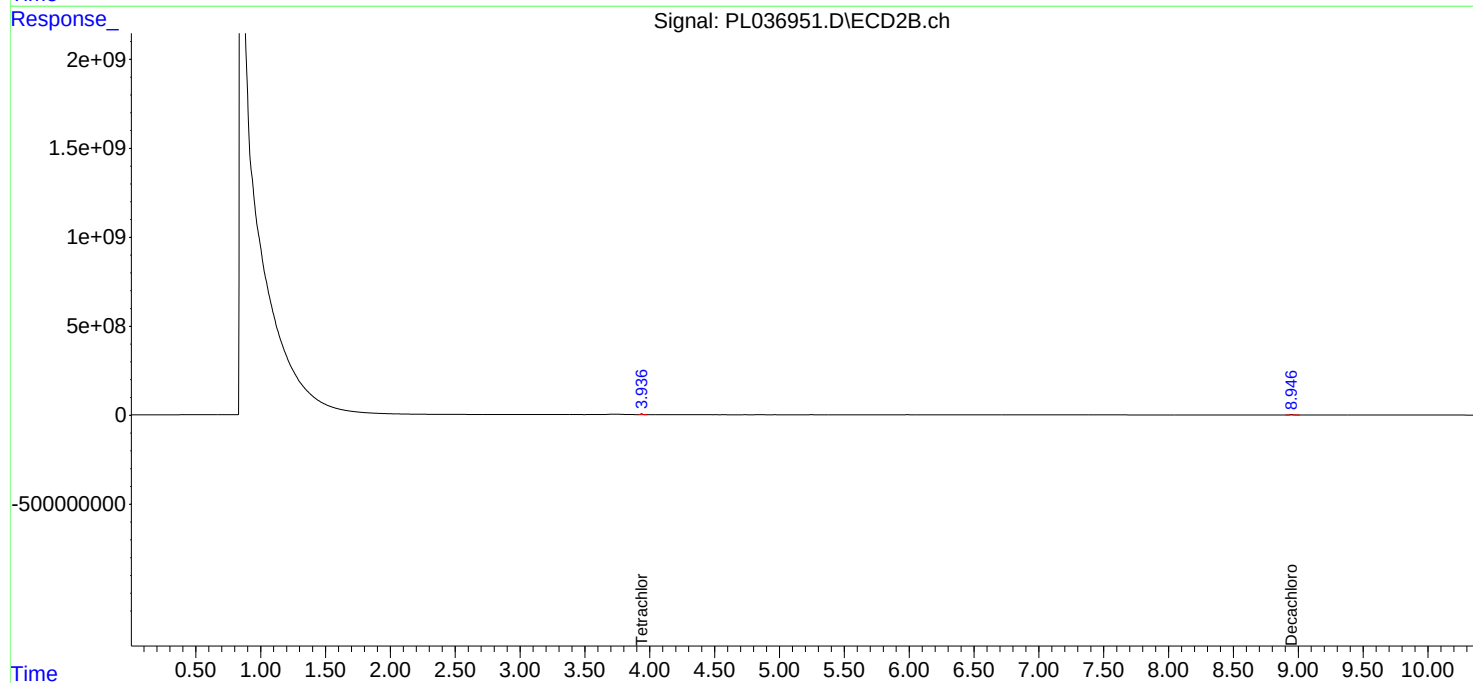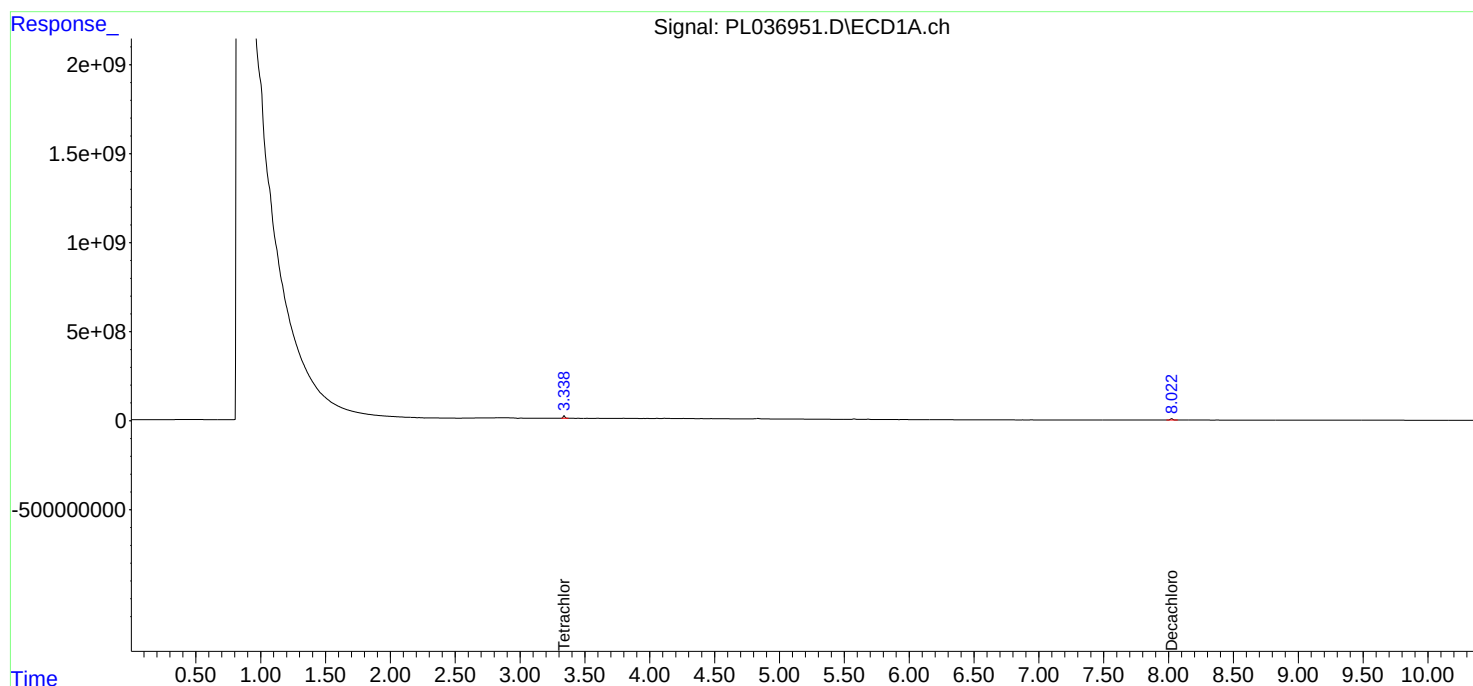

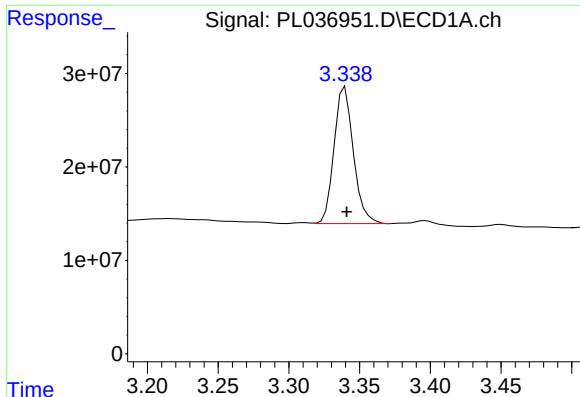


#1 Tetrachloro-m-xylene

R.T.: 3.340 min
Delta R.T.: -0.001 min
Response: 139096473
Conc: 19.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
MH-RO-341


Manual Integrations
APPROVED

UGO
6/15/2018 11:55:15 AM

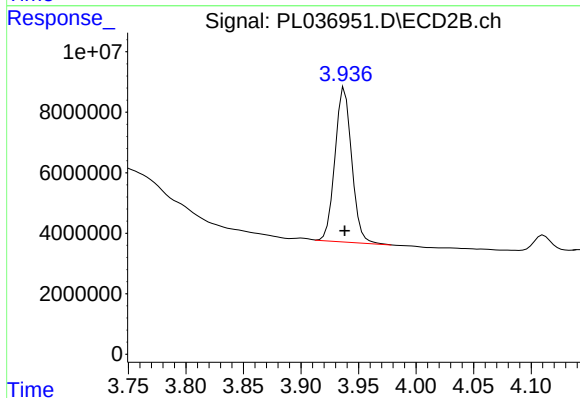


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.001 min
Response: 51646524
Conc: 20.20 ng/ml m

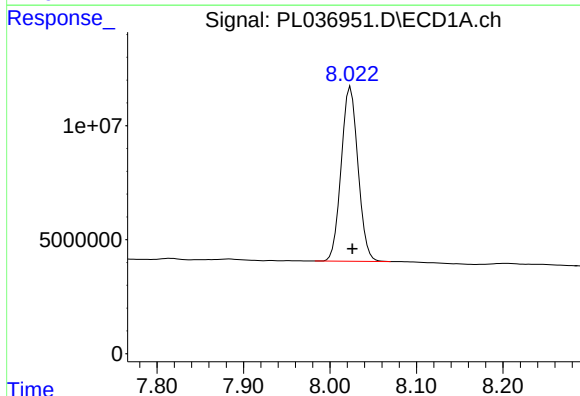

#28 Decachlorobiphenyl

R.T.: 8.024 min
Delta R.T.: -0.002 min
Response: 102542660
Conc: 15.76 ng/ml

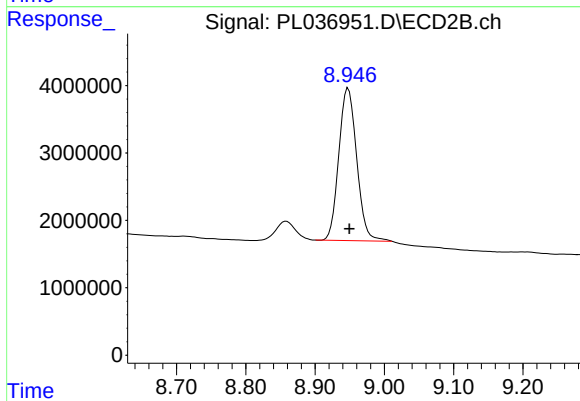

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.002 min
Response: 40618441
Conc: 15.92 ng/ml