

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061419\
 Data File : PL049522.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2019 23:09
 Operator : SM\AJ
 Sample : K3351-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RT-3425

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 03:11:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.935	91629938	22359192	8.316	7.739
28)	SA Decachlor...	7.989	8.970	86253548	25331270	6.783	7.585
Target Compounds							
2)	A alpha-BHC	0.000	4.348f	0	25121954	N.D.	6.268 #
6)	B beta-BHC	0.000	4.803f	0	5558679	N.D.	3.227 #
9)	A Endosulfan I	5.337f	0.000	5160181	0	0.353	N.D. #
10)	B gamma-Chl...	5.229f	6.033	19299937	951872	1.209	0.275 #
11)	B alpha-Chl...	0.000	6.107	0	3019477	N.D.	0.870 #
12)	B 4,4'-DDE	5.432	6.259	14196321	3120974	0.908	0.951
17)	MA 4,4'-DDT	6.175	7.051	9247068	1640945	0.751	0.585
20)	A Methoxychlor	6.701f	0.000	10522871	0	1.641	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061419\
Data File : PL049522.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2019 23:09
Operator : SM\AJ
Sample : K3351-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
RT-3425

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 03:11:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

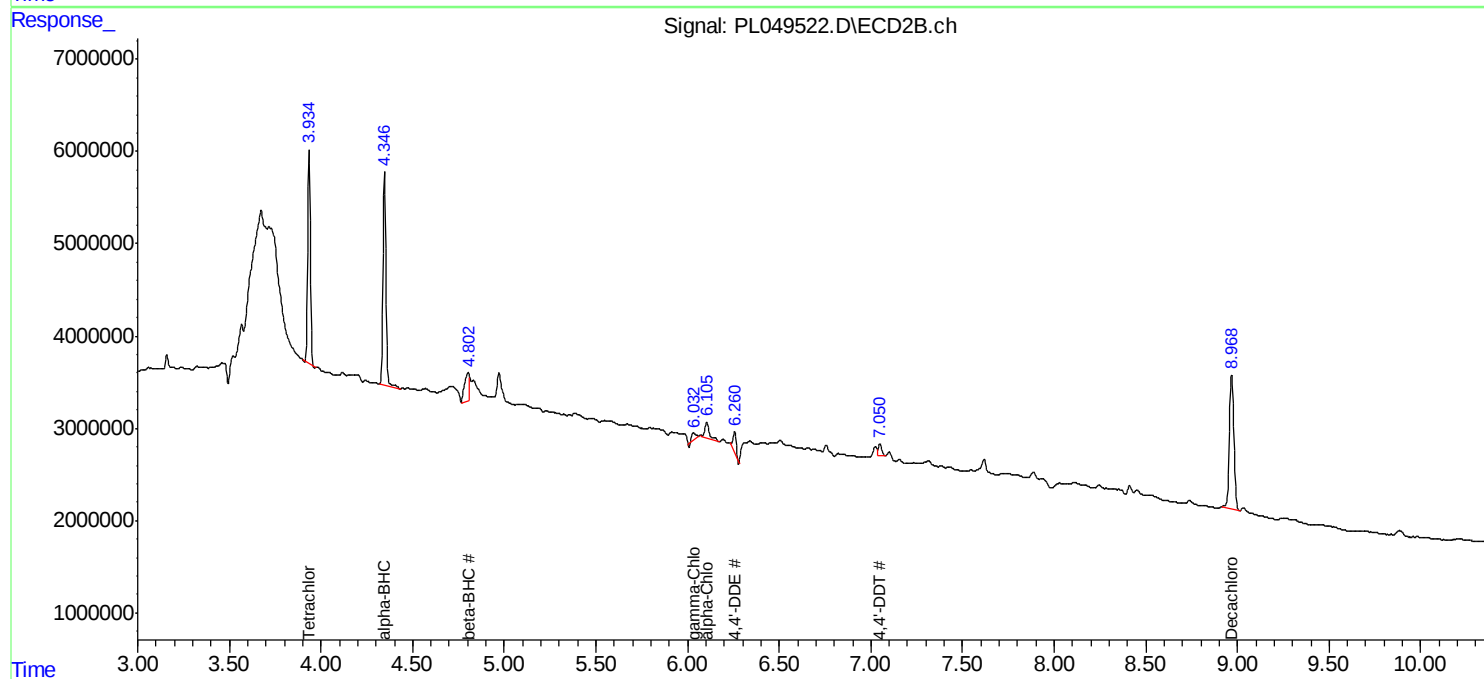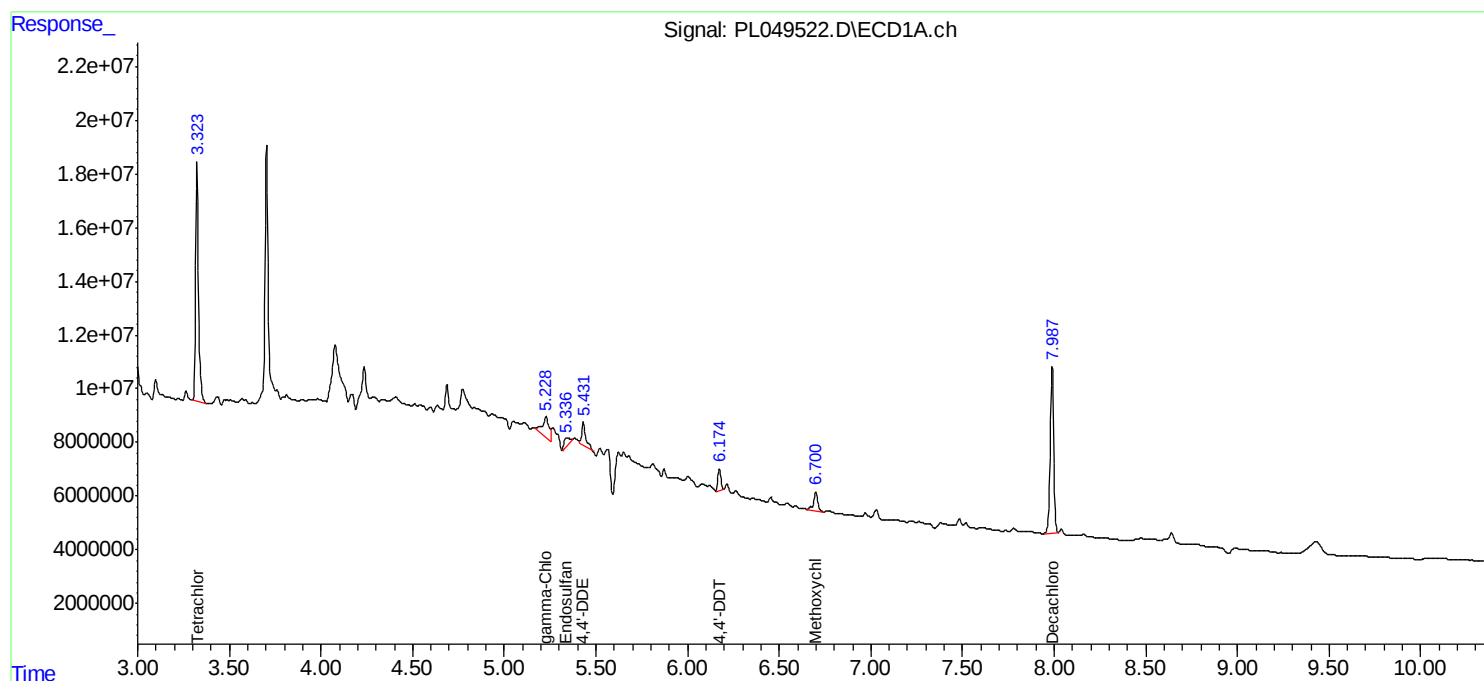


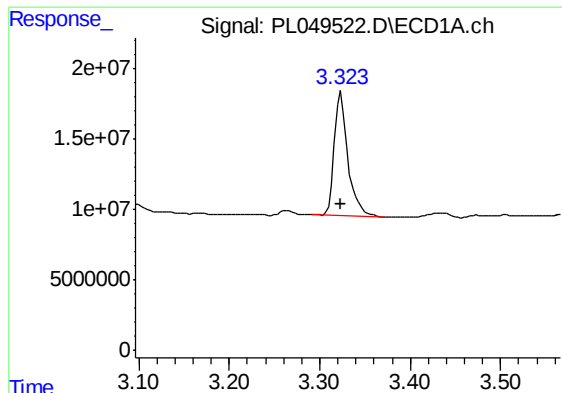

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: 0.000 min
Response: 91629938
Conc: 8.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
RT-3425

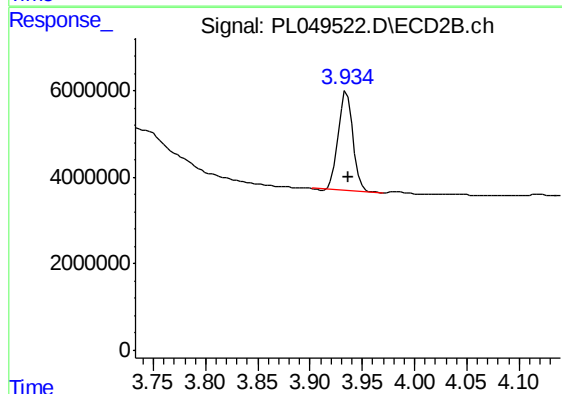


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.001 min
Response: 22359192
Conc: 7.74 ng/ml

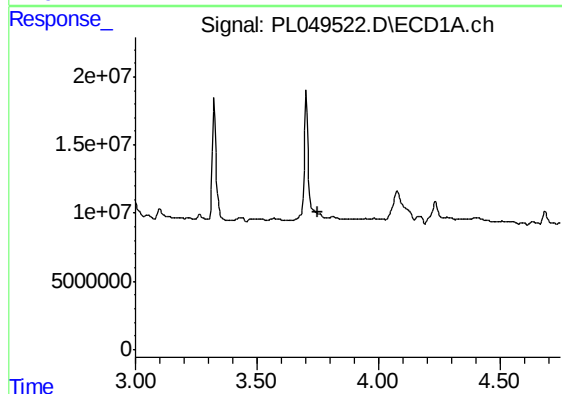


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.752 min
Response: 0
Conc: N.D.

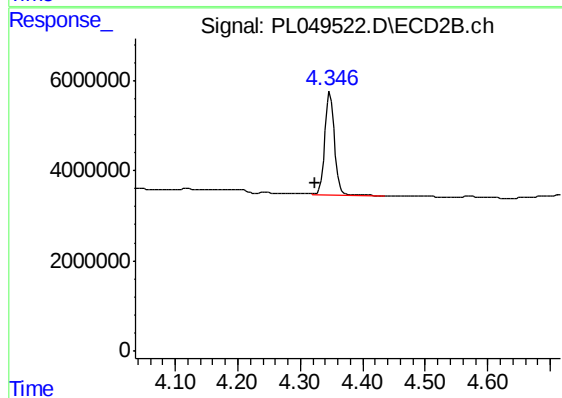

#2 alpha-BHC


R.T.: 4.348 min
Delta R.T.: 0.023 min
Response: 25121954
Conc: 6.27 ng/ml

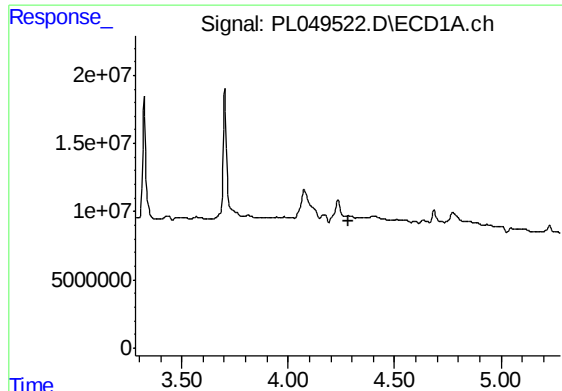

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.282 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
RT-3425

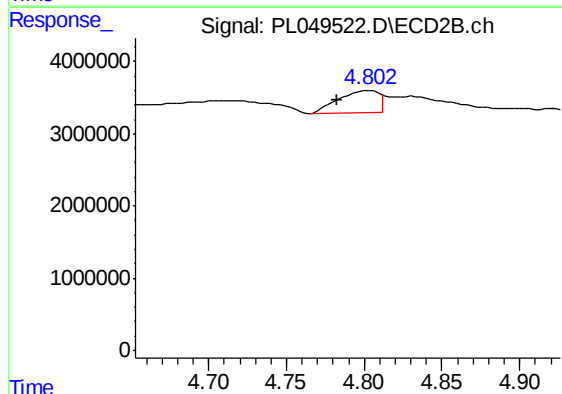


#6 beta-BHC

R.T.: 4.803 min
Delta R.T.: 0.021 min
Response: 5558679
Conc: 3.23 ng/ml

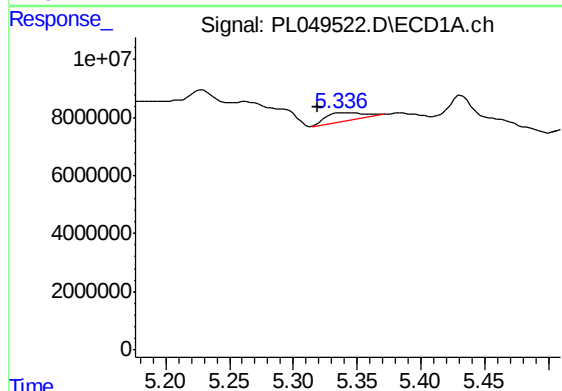


#9 Endosulfan I

R.T.: 5.337 min
Delta R.T.: 0.018 min
Response: 5160181
Conc: 0.35 ng/ml

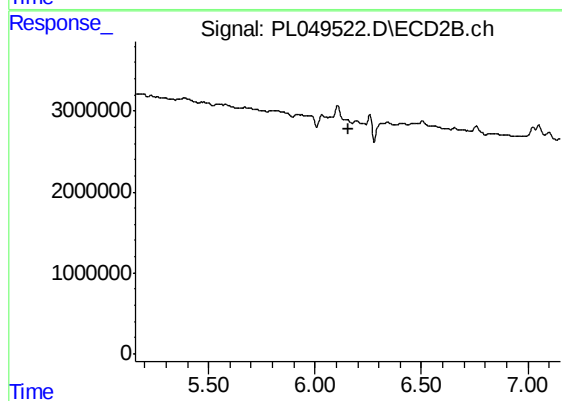

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.156 min
Response: 0
Conc: N.D.

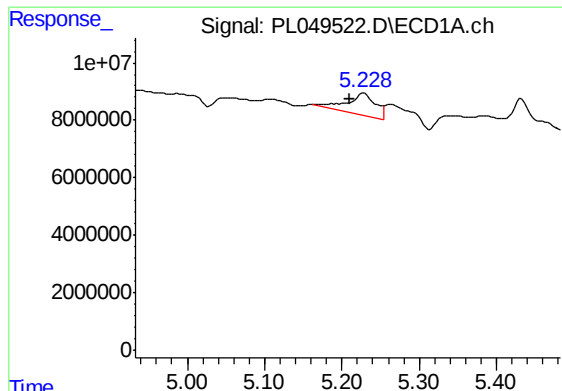

#10 gamma-Chlordane


R.T.: 5.229 min
Delta R.T.: 0.018 min
Response: 19299937
Conc: 1.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
RT-3425

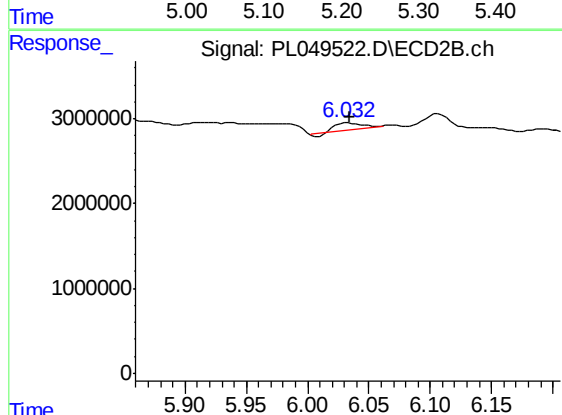


#10 gamma-Chlordane

R.T.: 6.033 min
Delta R.T.: -0.002 min
Response: 951872
Conc: 0.28 ng/ml

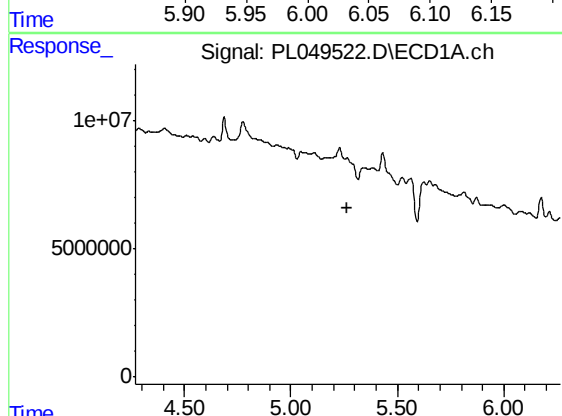


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.267 min
Response: 0
Conc: N.D.

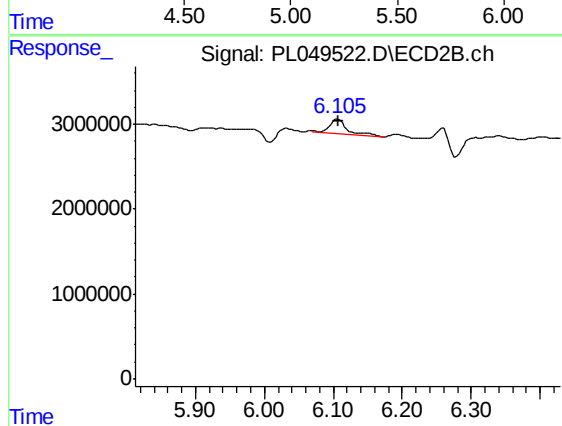

#11 alpha-Chlordane


R.T.: 6.107 min
Delta R.T.: 0.000 min
Response: 3019477
Conc: 0.87 ng/ml

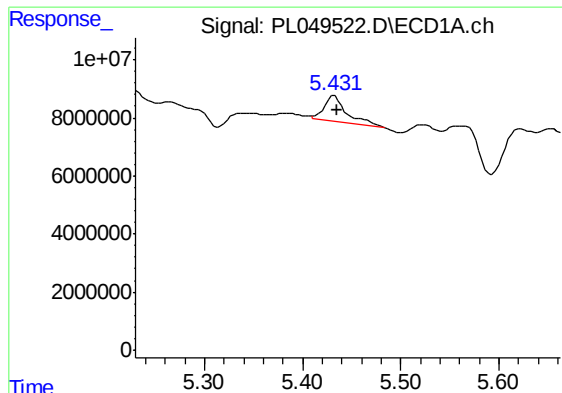

#12 4,4'-DDE


R.T.: 5.432 min
Delta R.T.: -0.002 min
Response: 14196321
Conc: 0.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
RT-3425

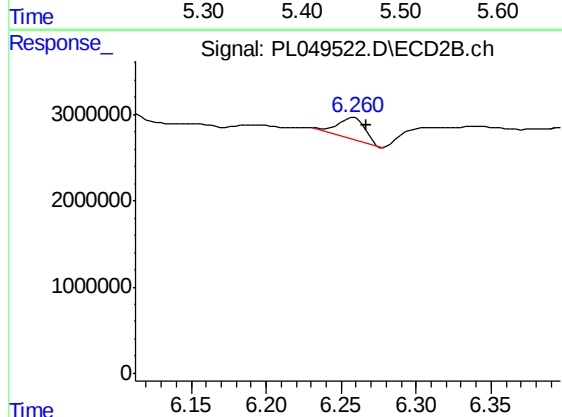


#12 4,4'-DDE

R.T.: 6.259 min
Delta R.T.: -0.008 min
Response: 3120974
Conc: 0.95 ng/ml

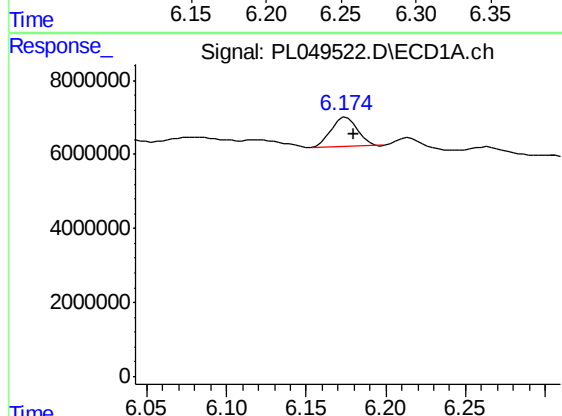


#17 4,4'-DDT

R.T.: 6.175 min
Delta R.T.: -0.005 min
Response: 9247068
Conc: 0.75 ng/ml

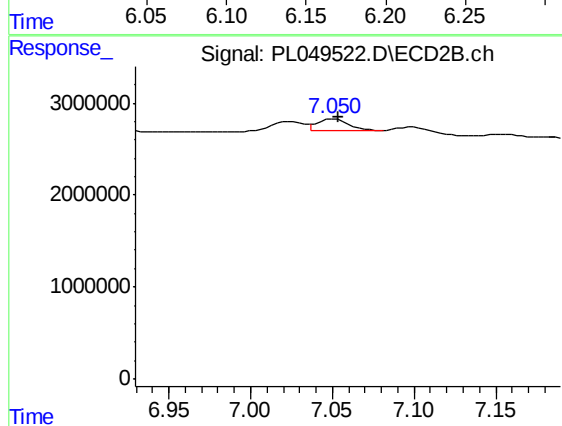

#17 4,4'-DDT


R.T.: 7.051 min
Delta R.T.: -0.002 min
Response: 1640945
Conc: 0.59 ng/ml

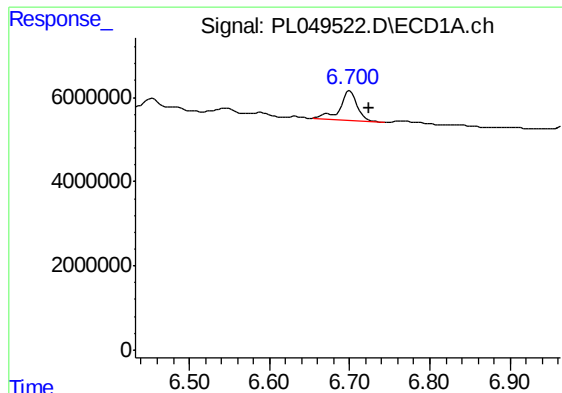

#20 Methoxychlor


R.T.: 6.701 min
Delta R.T.: -0.024 min
Response: 10522871
Conc: 1.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
RT-3425

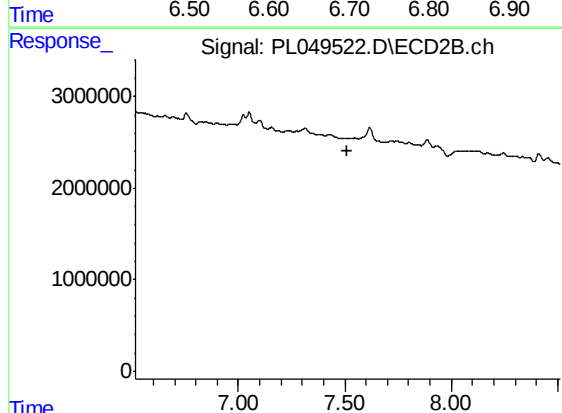


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.514 min
Response: 0
Conc: N.D.

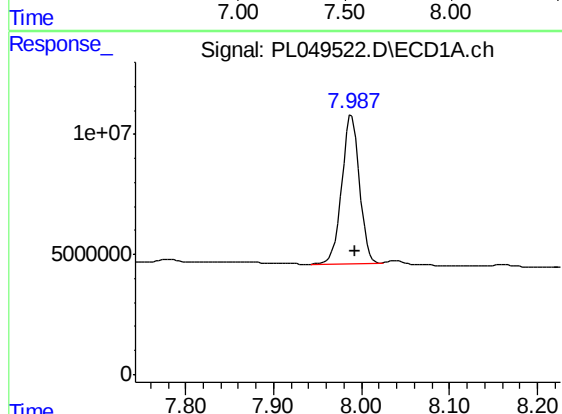

#28 Decachlorobiphenyl

R.T.: 7.989 min
Delta R.T.: -0.004 min
Response: 86253548
Conc: 6.78 ng/ml

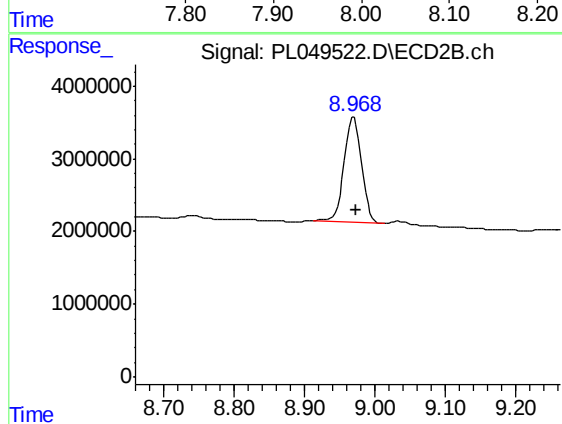

#28 Decachlorobiphenyl

R.T.: 8.970 min
Delta R.T.: -0.003 min
Response: 25331270
Conc: 7.58 ng/ml