

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061419\
 Data File : PL049526.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2019 00:08
 Operator : SM\AJ
 Sample : K3361-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BAT-B15

Manual Integrations
 APPROVED

Ankita
 6/17/2019 9:29:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 03:12:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.320	3.933	88638241	19275881	8.044m	6.672m
28)	SA Decachlor...	7.987	8.968	70889242	21541039	5.575	6.450

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061419\
Data File : PL049526.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2019 00:08
Operator : SM\AJ
Sample : K3361-04
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BAT-B15


Manual Integrations
APPROVED

Ankita
6/17/2019 9:29:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 03:12:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

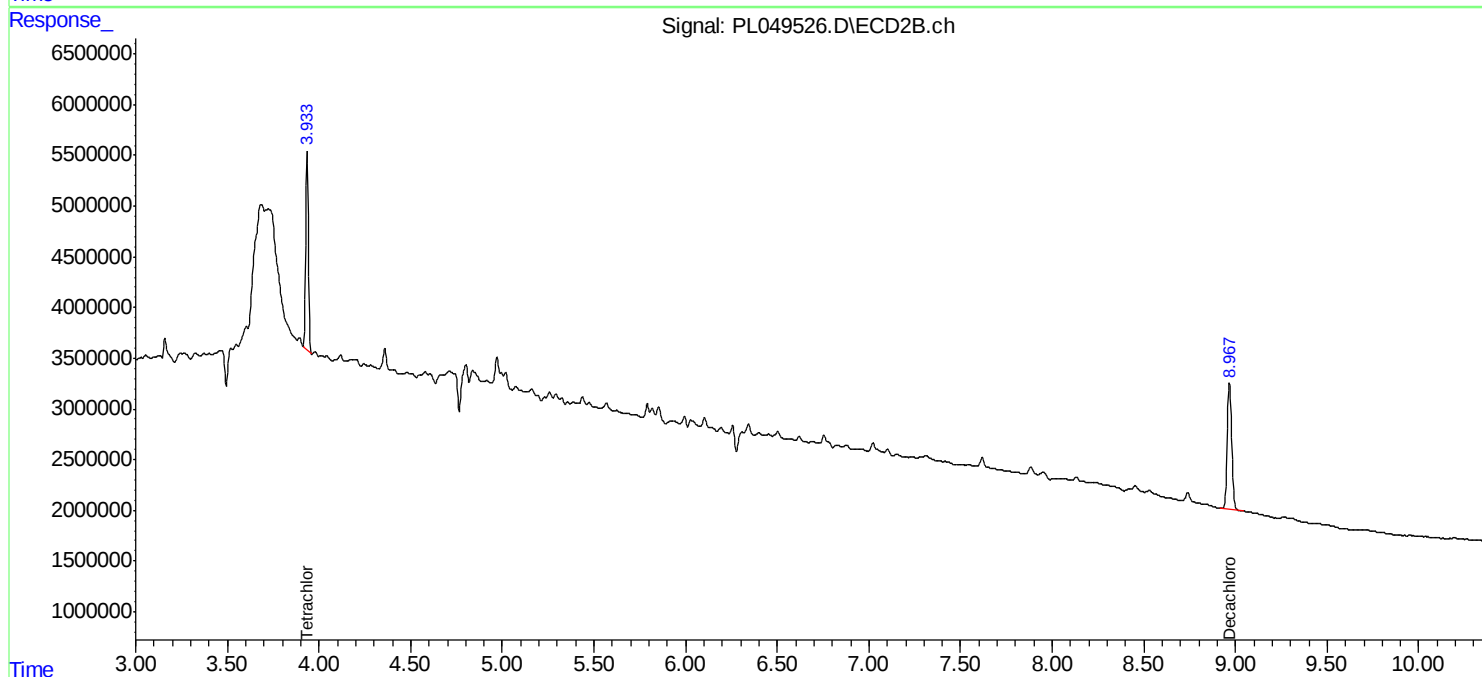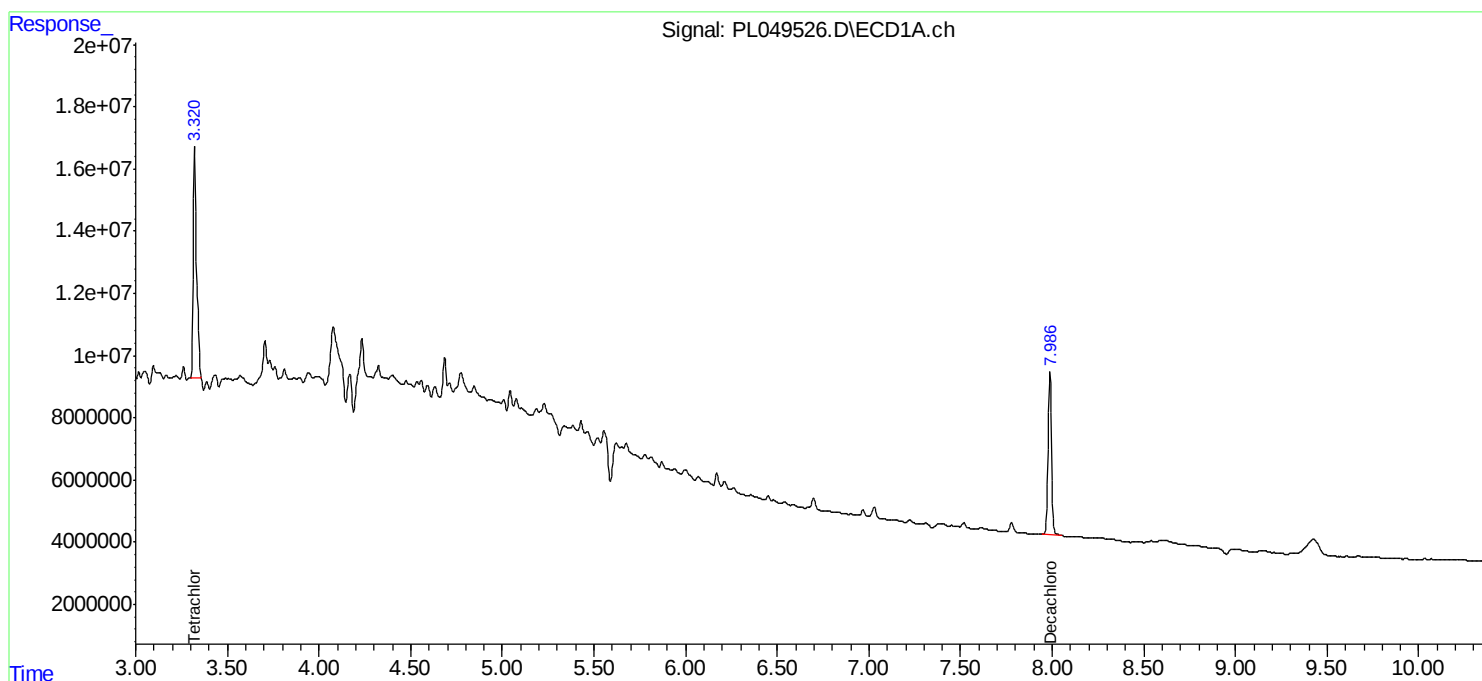

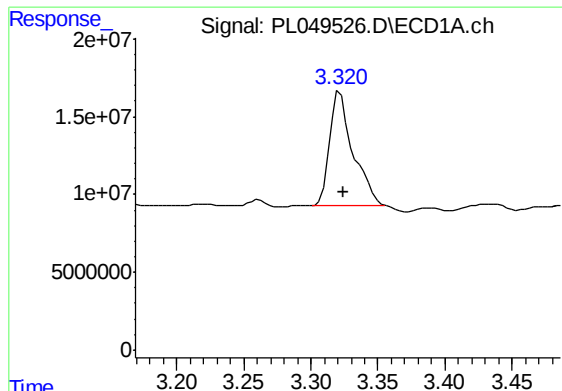


#1 Tetrachloro-m-xylene

R.T.: 3.320 min
Delta R.T.: -0.004 min
Response: 88638241
Conc: 8.04 ng/ml m

Instrument :
ECD_L
ClientSampleId :
BAT-B15


Manual Integrations
APPROVED

Ankita
6/17/2019 9:29:03 AM

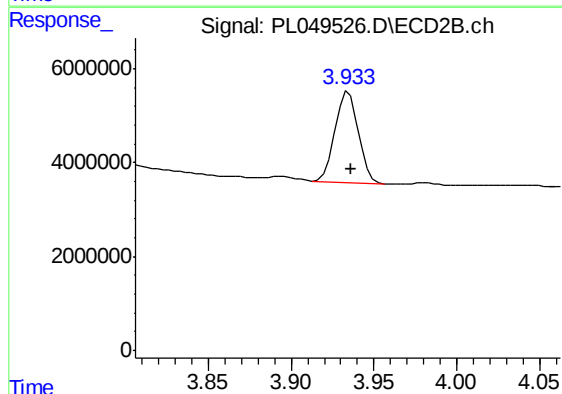


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.003 min
Response: 19275881
Conc: 6.67 ng/ml m

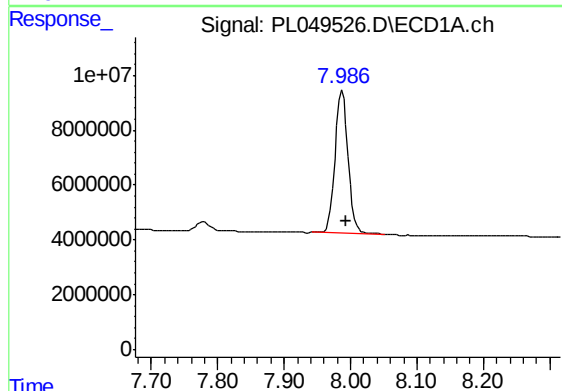

#28 Decachlorobiphenyl

R.T.: 7.987 min
Delta R.T.: -0.005 min
Response: 70889242
Conc: 5.58 ng/ml

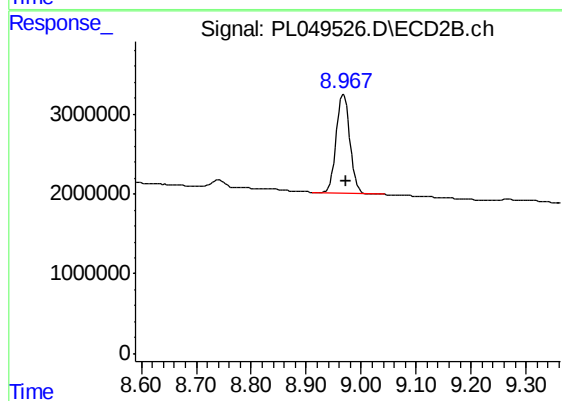

#28 Decachlorobiphenyl

R.T.: 8.968 min
Delta R.T.: -0.004 min
Response: 21541039
Conc: 6.45 ng/ml