

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061421\
 Data File : PL067392.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2021 10:42
 Operator : AR\AJ
 Sample : PB137073TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 13:12:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.483	5.527	11560956	19871816	21.028	21.079
28)	SA Decachlor...	10.227	11.432	14645869	20975020	20.666	21.058
Target Compounds							
4)	MA Heptachlor	0.000	7.163	0	450050	N.D.	0.404 #
6)	B beta-BHC	5.967f	6.758	207223	4347429	0.579	8.006 #
7)	B delta-BHC	0.000	7.006f	0	516002	N.D.	0.439 #
23)	Chlordane-1	0.000	6.898	0	354021	N.D.	12.537 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061421\
Data File : PL067392.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2021 10:42
Operator : AR\AJ
Sample : PB137073TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 13:12:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

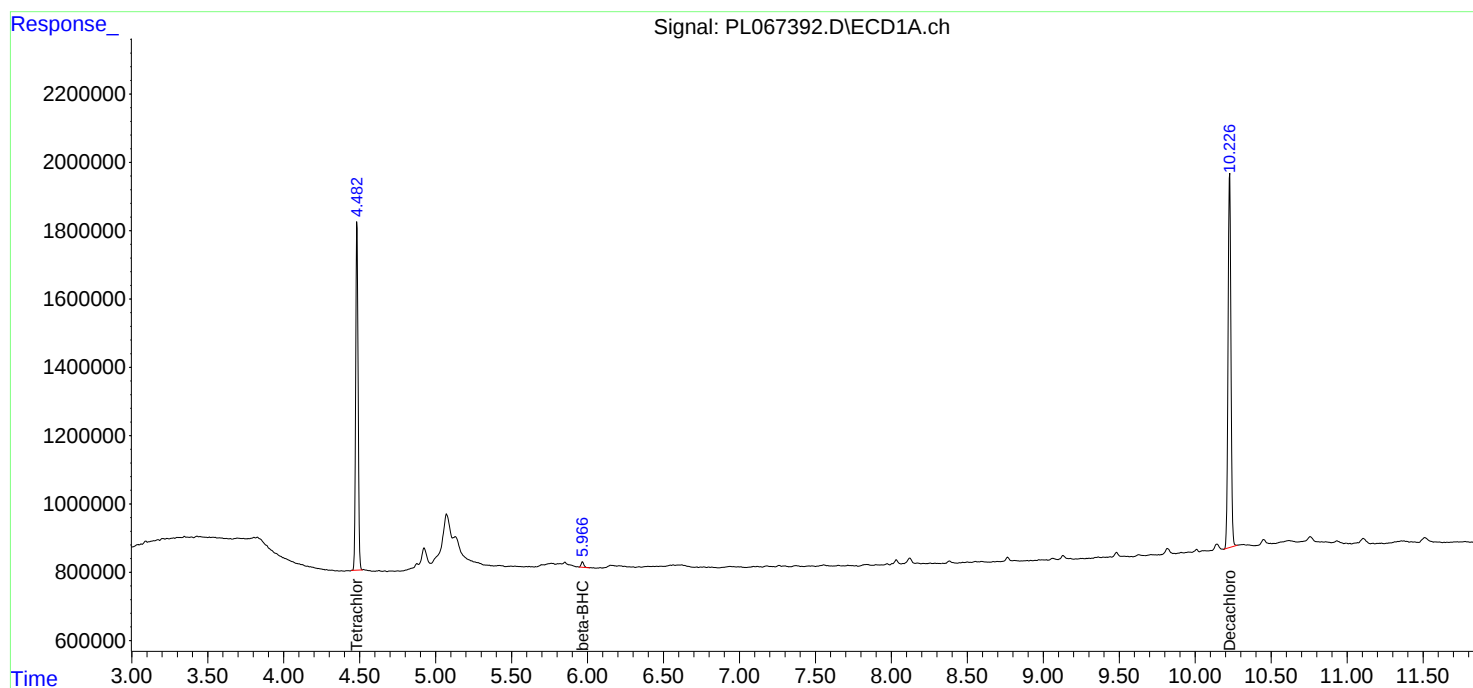


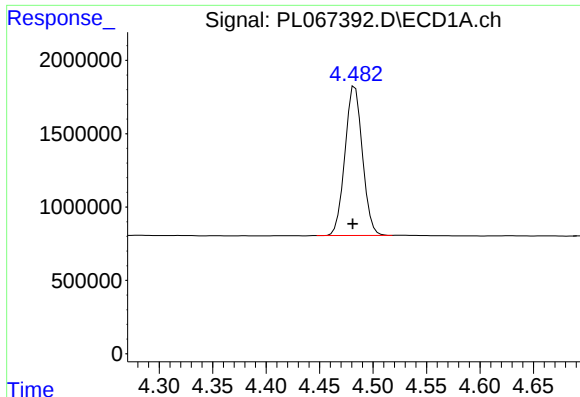

#1 Tetrachloro-m-xylene


R.T.: 4.483 min
Delta R.T.: 0.002 min
Response: 11560956
Conc: 21.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

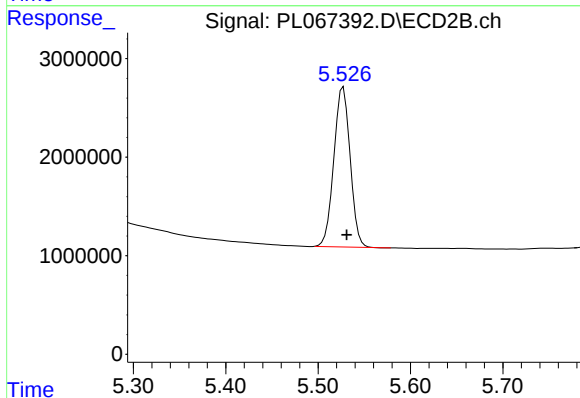


#1 Tetrachloro-m-xylene

R.T.: 5.527 min
Delta R.T.: -0.004 min
Response: 19871816
Conc: 21.08 ng/ml

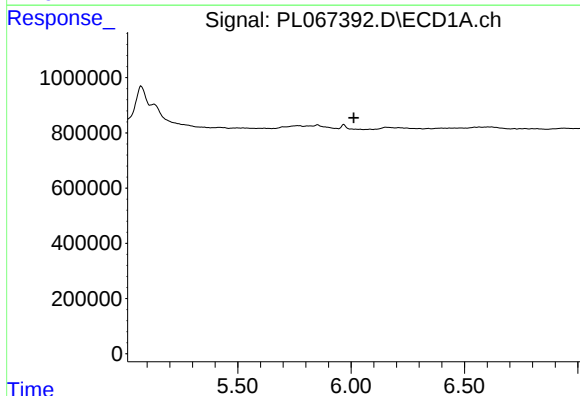


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 6.012 min
Response: 0
Conc: N.D.

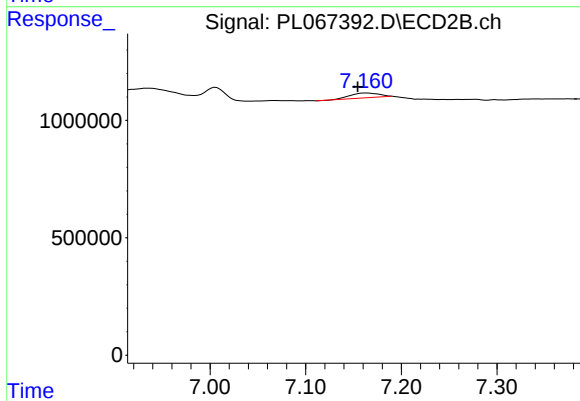

#4 Heptachlor


R.T.: 7.163 min
Delta R.T.: 0.008 min
Response: 450050
Conc: 0.40 ng/ml

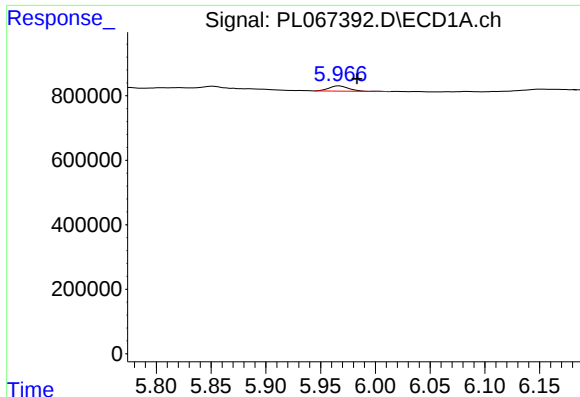

#6 beta-BHC


R.T.: 5.967 min
Delta R.T.: -0.016 min
Response: 207223
Conc: 0.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

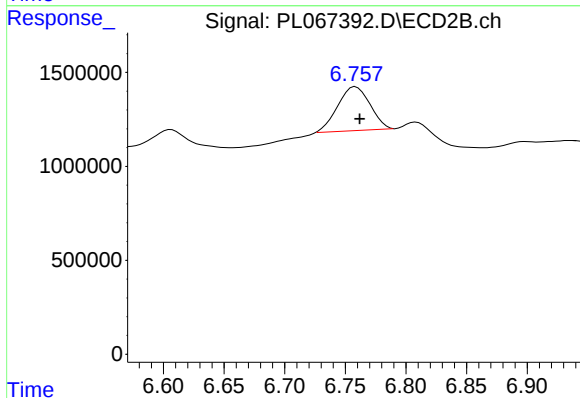


#6 beta-BHC

R.T.: 6.758 min
Delta R.T.: -0.004 min
Response: 4347429
Conc: 8.01 ng/ml

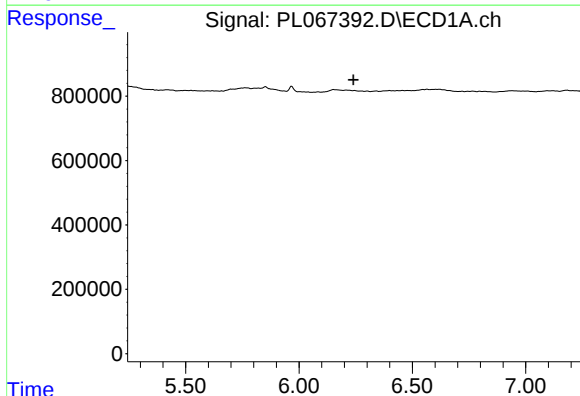


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

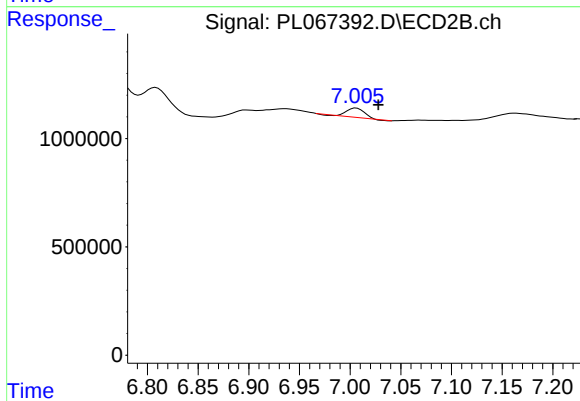

#7 delta-BHC


R.T.: 7.006 min
Delta R.T.: -0.022 min
Response: 516002
Conc: 0.44 ng/ml

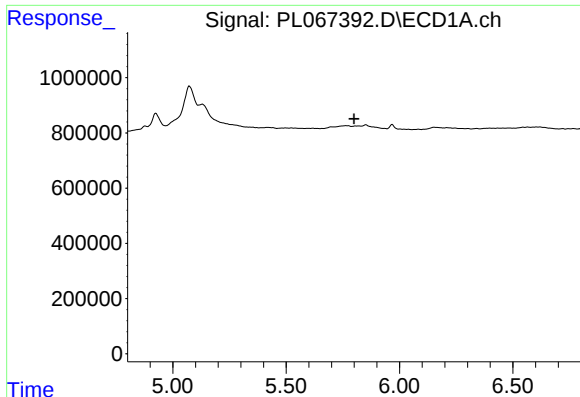

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.800 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

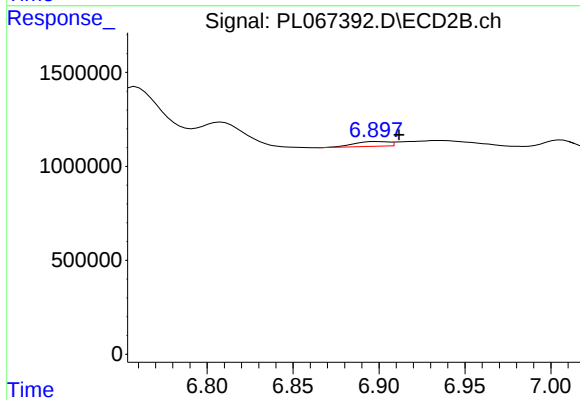


#23 Chlordane-1

R.T.: 6.898 min
Delta R.T.: -0.013 min
Response: 354021
Conc: 12.54 ng/ml

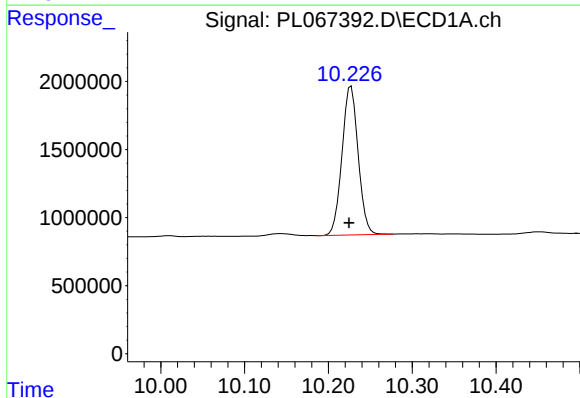

#28 Decachlorobiphenyl

R.T.: 10.227 min
Delta R.T.: 0.003 min
Response: 14645869
Conc: 20.67 ng/ml

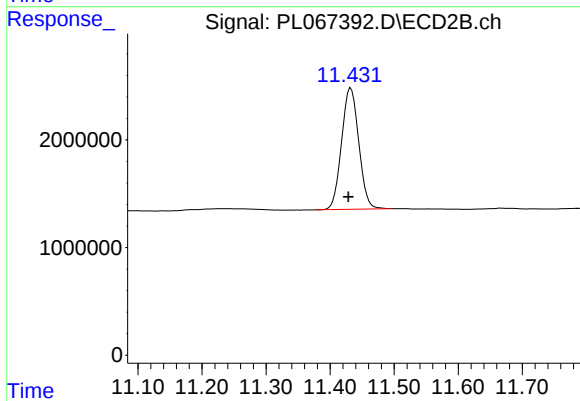

#28 Decachlorobiphenyl

R.T.: 11.432 min
Delta R.T.: 0.004 min
Response: 20975020
Conc: 21.06 ng/ml