

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061421\
 Data File : PL067397.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2021 12:05
 Operator : AR\AJ
 Sample : M2626-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 13:13:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.531	11786214	18746157	21.438	19.885
28)	SA Decachlor...	10.225	11.433	14705094	22211151	20.750	22.299
Target Compounds							
6)	B beta-BHC	5.965f	6.782f	767493	-829612	2.145	N.D. #
7)	B delta-BHC	0.000	7.009f	0	3066492	N.D.	2.609 #
8)	B Heptachlo...	0.000	7.965f	0	3197349	N.D.	3.192 #
23)	Chlordane-1	5.771f	0.000	475497	0	25.700	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061421\
Data File : PL067397.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2021 12:05
Operator : AR\AJ
Sample : M2626-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 13:13:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

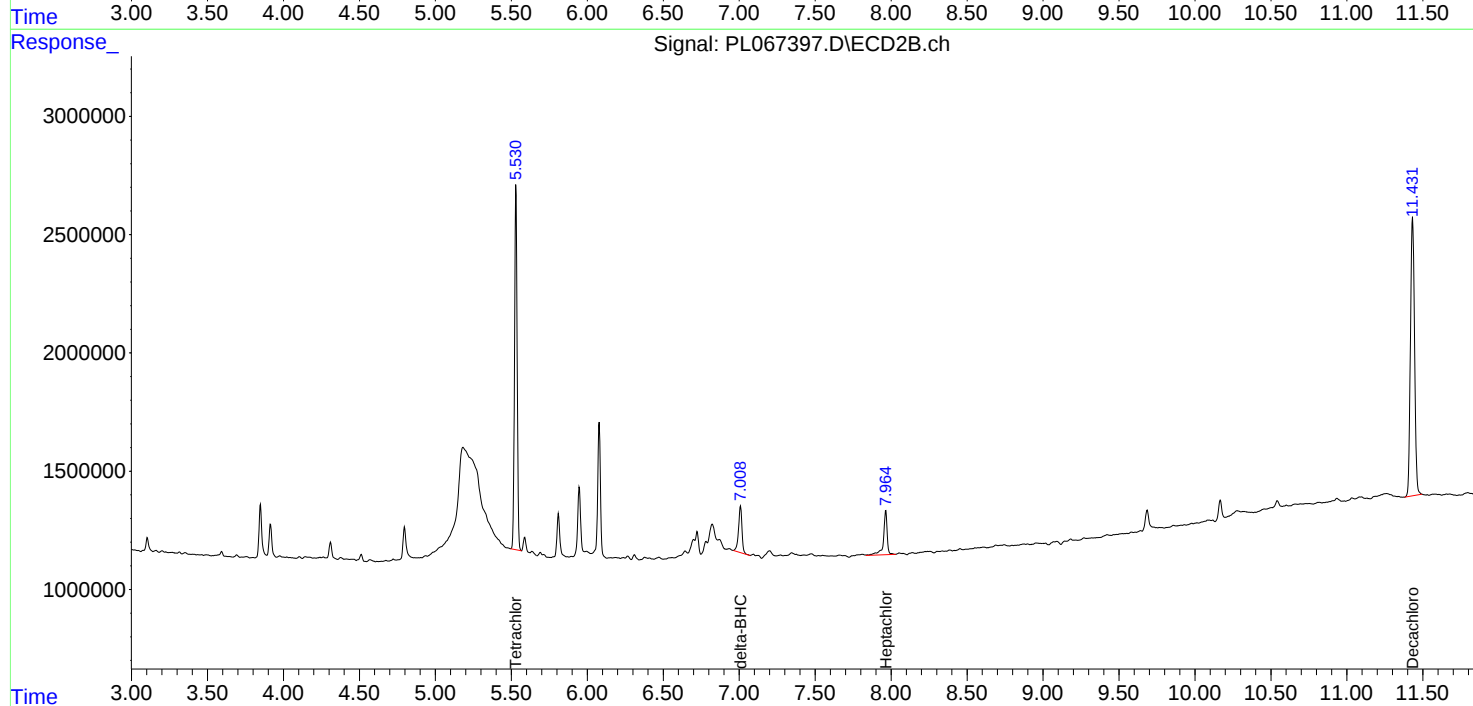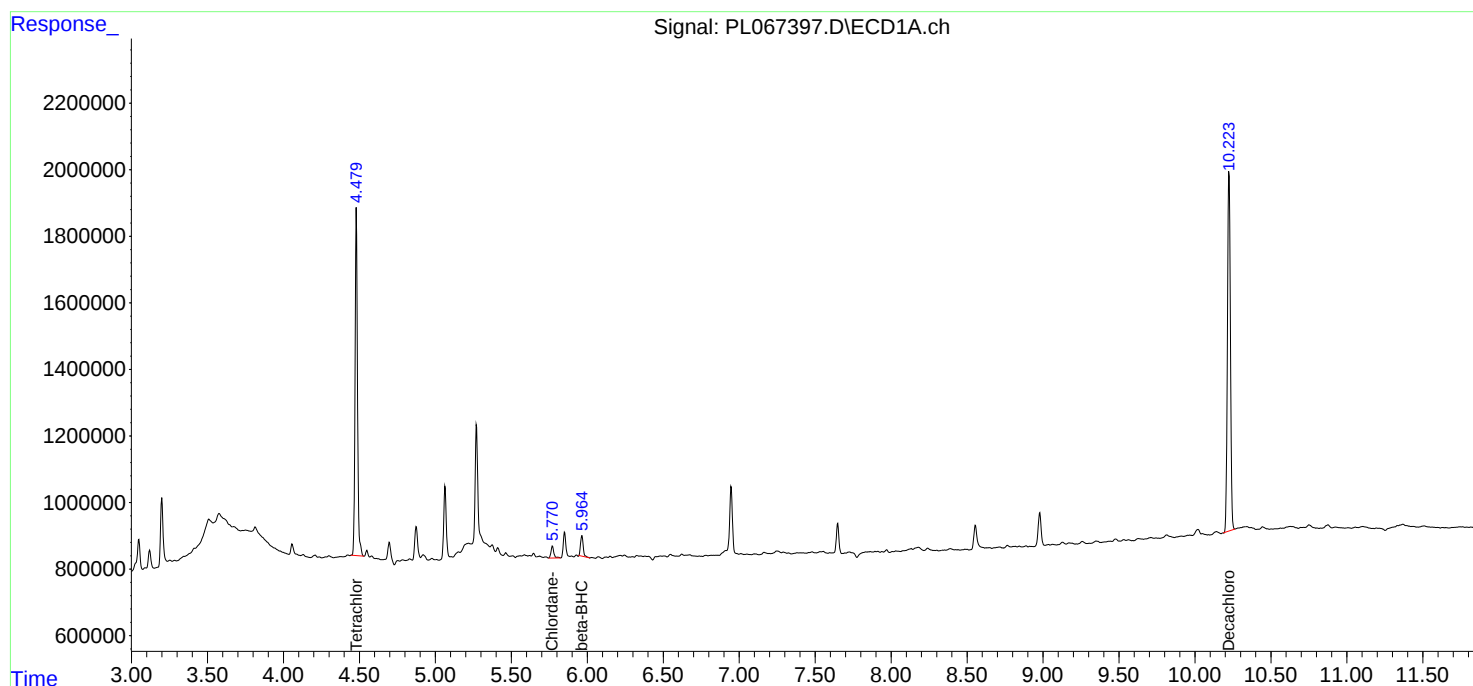


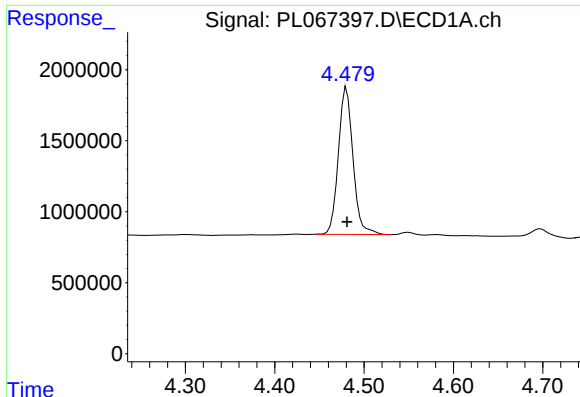

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 11786214
Conc: 21.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

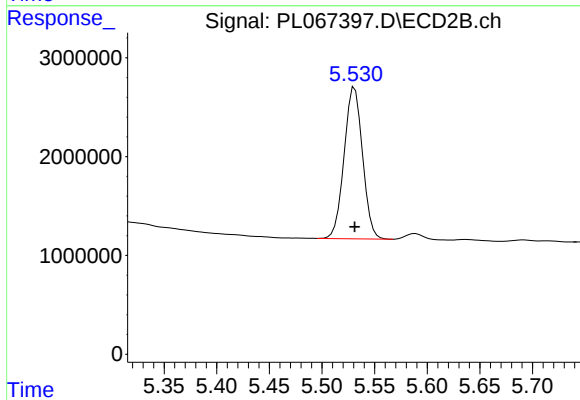


#1 Tetrachloro-m-xylene

R.T.: 5.531 min
Delta R.T.: 0.000 min
Response: 18746157
Conc: 19.88 ng/ml

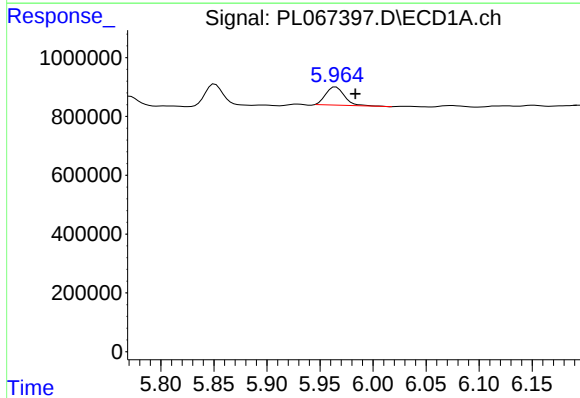


#6 beta-BHC

R.T.: 5.965 min
Delta R.T.: -0.018 min
Response: 767493
Conc: 2.14 ng/ml

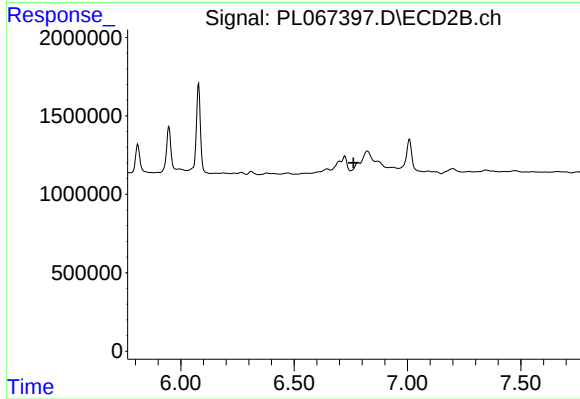

#6 beta-BHC

R.T.: 6.782 min
Delta R.T.: 0.020 min
Response: -829612
Conc: N.D.

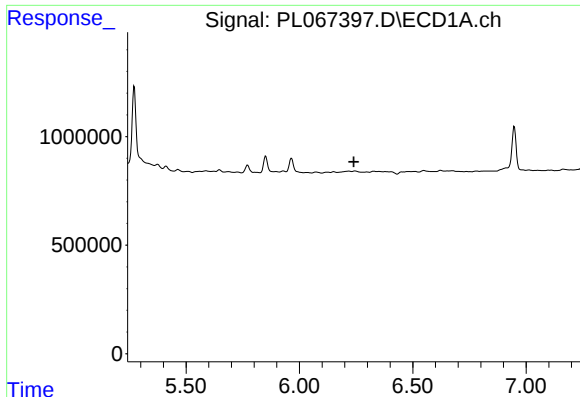

#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#7 delta-BHC


R.T.: 7.009 min
Delta R.T.: -0.019 min
Response: 3066492
Conc: 2.61 ng/ml

#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 6.907 min
Response: 0
Conc: N.D.

#8 Heptachlor epoxide


R.T.: 7.965 min
Delta R.T.: -0.026 min
Response: 3197349
Conc: 3.19 ng/ml

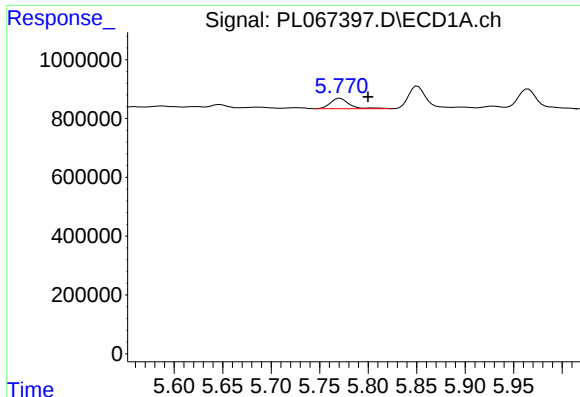

#23 Chlordane-1


R.T.: 5.771 min
Delta R.T.: -0.029 min
Response: 475497
Conc: 25.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

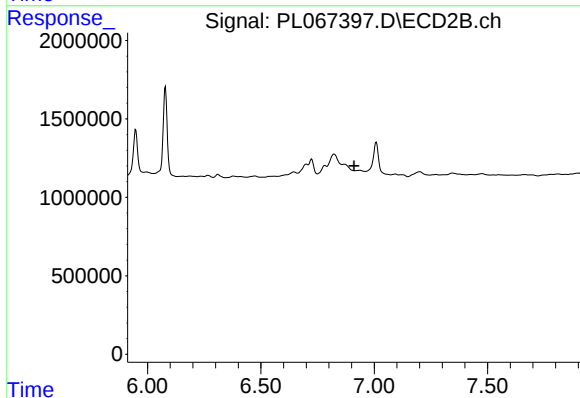


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 6.912 min
Response: 0
Conc: N.D.

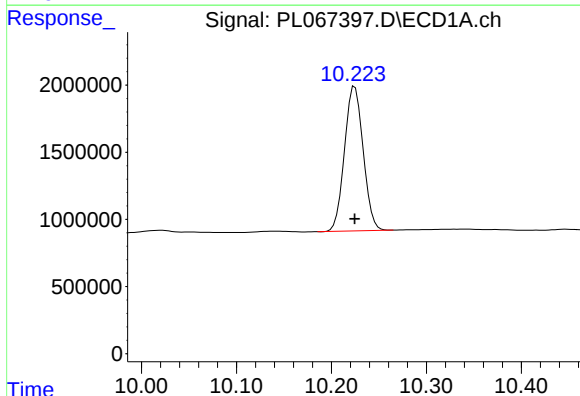

#28 Decachlorobiphenyl

R.T.: 10.225 min
Delta R.T.: 0.000 min
Response: 14705094
Conc: 20.75 ng/ml

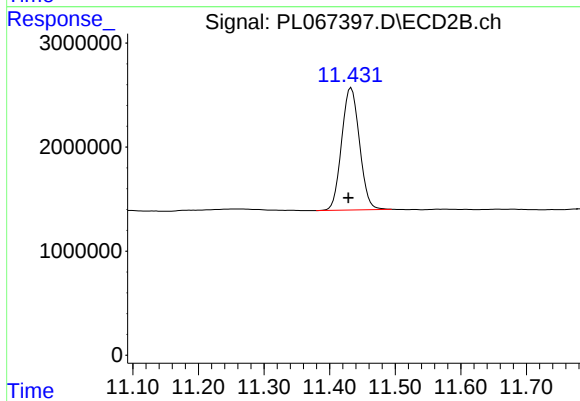

#28 Decachlorobiphenyl

R.T.: 11.433 min
Delta R.T.: 0.004 min
Response: 22211151
Conc: 22.30 ng/ml