

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061421\
 Data File : PL067401.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2021 13:11
 Operator : AR\AJ
 Sample : M2637-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 20:01:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	7607781	12759133	13.838	13.534
28)	SA Decachlor...	10.221	11.426	10237152	15609059	14.445	15.671
Target Compounds							
2)	A alpha-BHC	5.171	0.000	475122	0	0.646	N.D. #
5)	MB Aldrin	6.341	0.000	1546512	0	2.102	N.D. #
6)	B beta-BHC	5.962f	0.000	665046	0	1.859	N.D. #
7)	B delta-BHC	0.000	7.006f	0	3260201	N.D.	2.773 #
8)	B Heptachlo...	0.000	7.962f	0	2186503	N.D.	2.183 #
15)	B Endosulfa...	8.176	9.178f	311817	732547	0.506	0.919 #
18)	B Endrin al...	8.380	0.000	298529	0	0.590	N.D. #
21)	B Endrin ke...	9.127	0.000	218967	0	0.288	N.D. #
27)	Chlordane-5	8.176	0.000	311817	0	14.252	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061421\
Data File : PL067401.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2021 13:11
Operator : AR\AJ
Sample : M2637-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 20:01:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

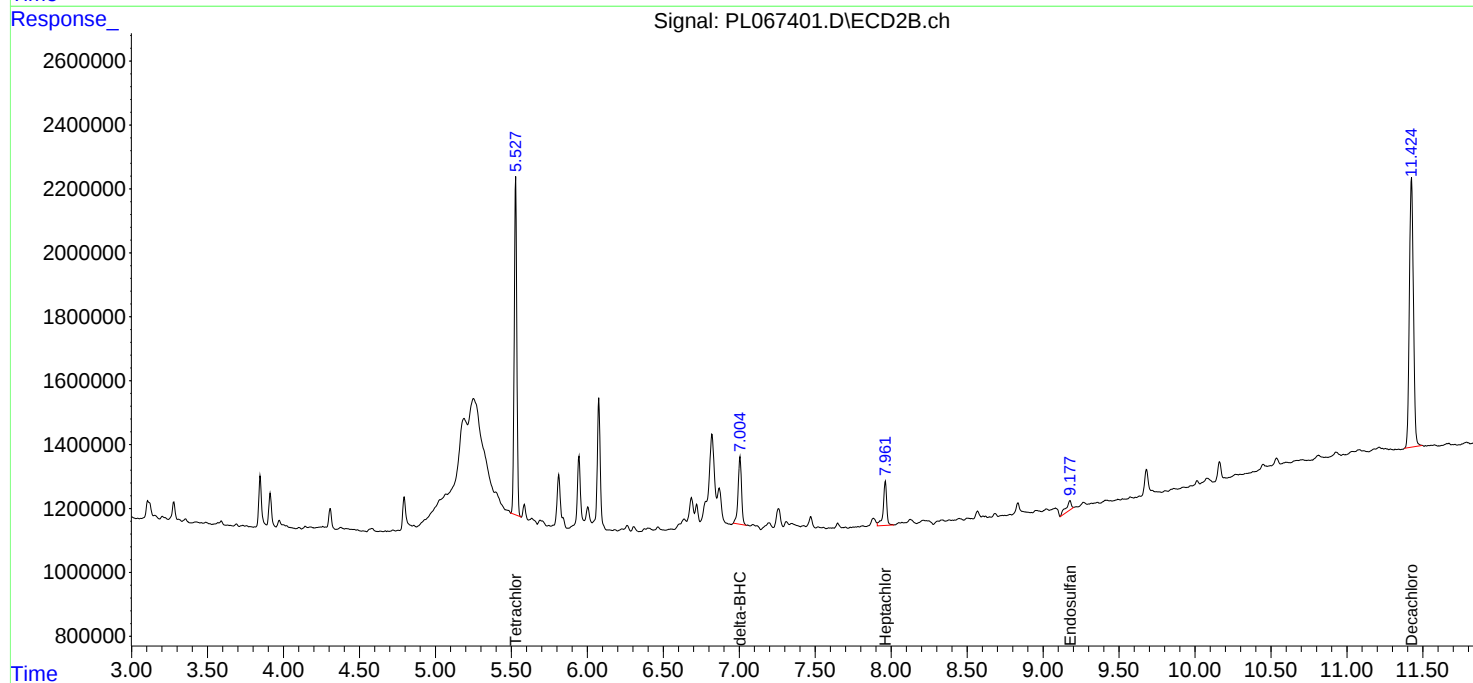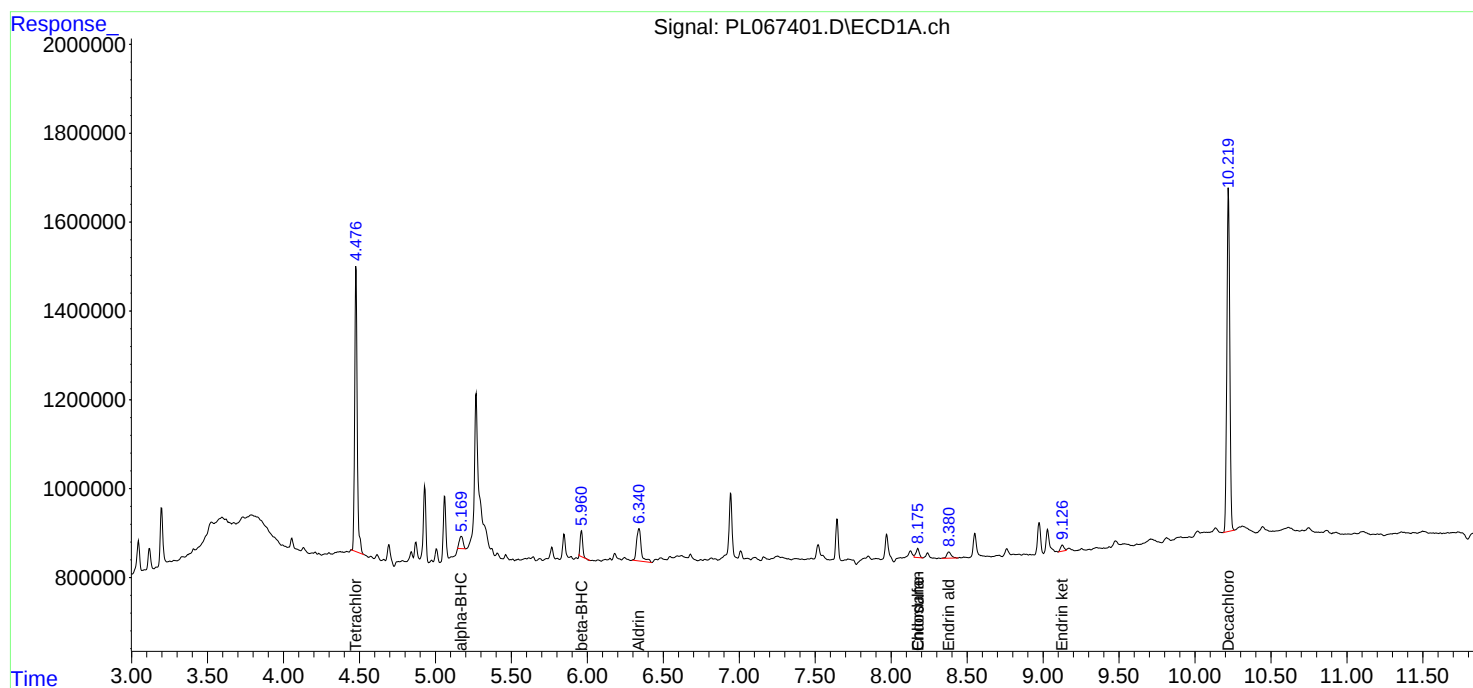


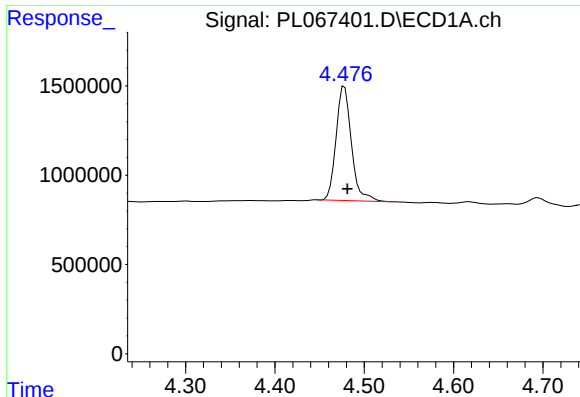

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 7607781
Conc: 13.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

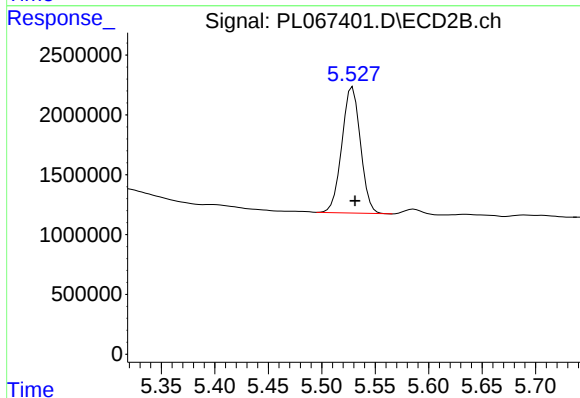


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 12759133
Conc: 13.53 ng/ml

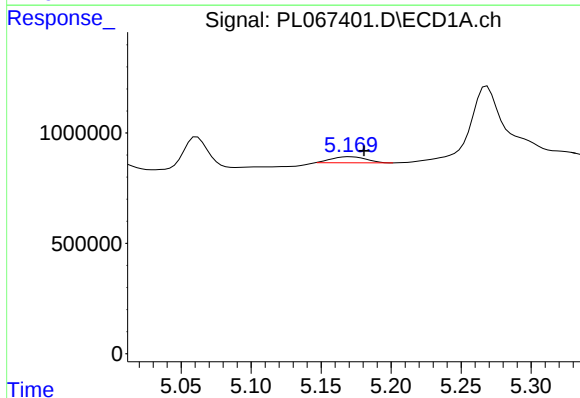


#2 alpha-BHC

R.T.: 5.171 min
Delta R.T.: -0.010 min
Response: 475122
Conc: 0.65 ng/ml

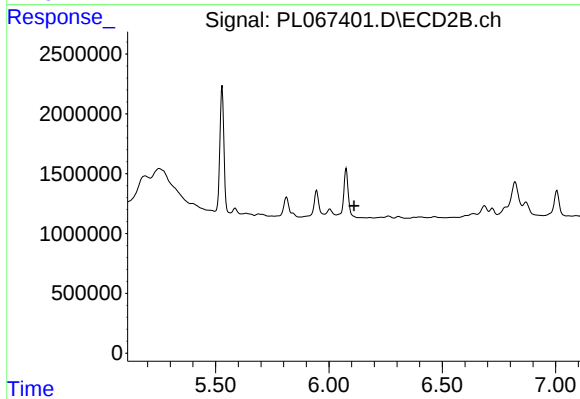

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 6.112 min
Response: 0
Conc: N.D.

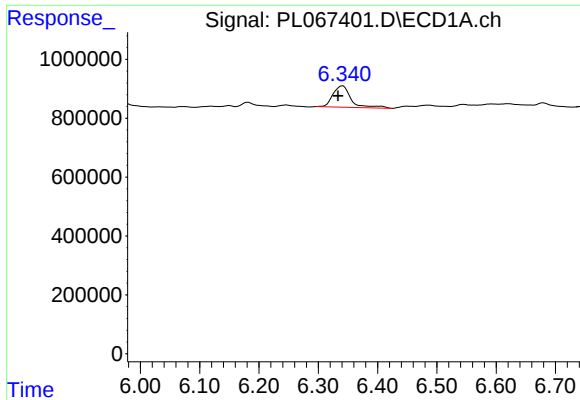

#5 Aldrin


R.T.: 6.341 min
Delta R.T.: 0.007 min
Response: 1546512
Conc: 2.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

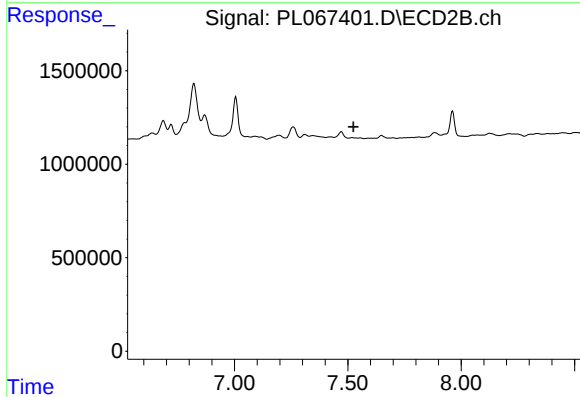


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.525 min
Response: 0
Conc: N.D.

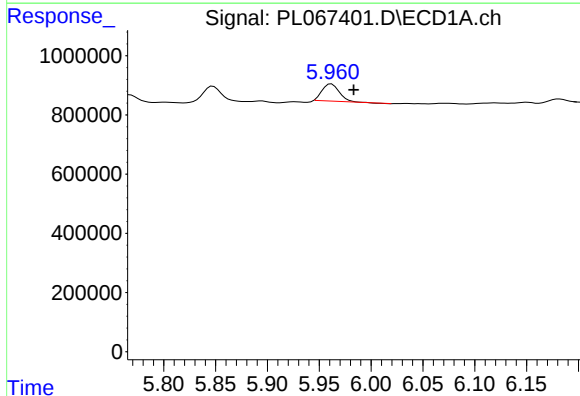


#6 beta-BHC

R.T.: 5.962 min
Delta R.T.: -0.022 min
Response: 665046
Conc: 1.86 ng/ml

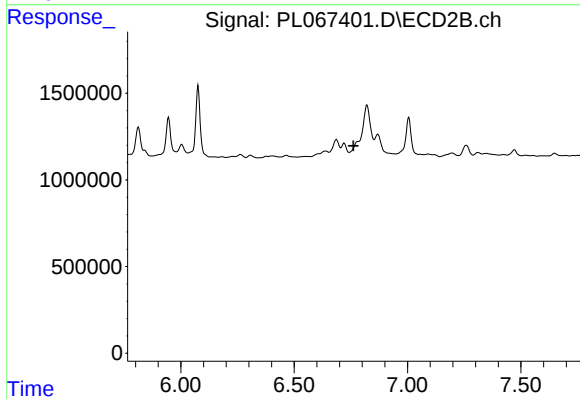

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

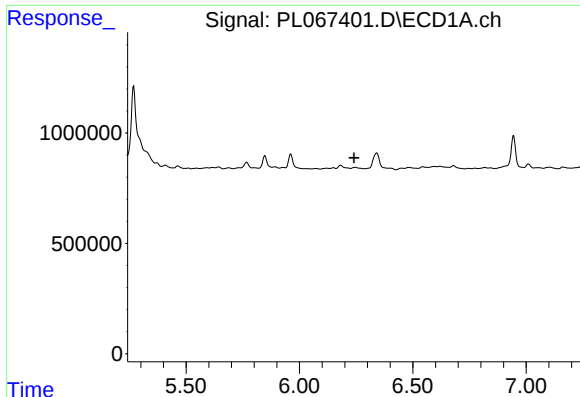

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

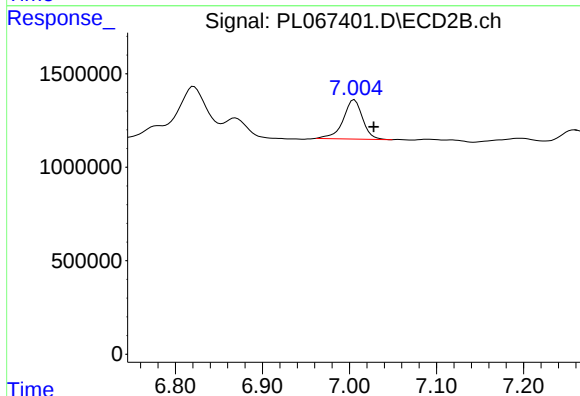


#7 delta-BHC

R.T.: 7.006 min
Delta R.T.: -0.022 min
Response: 3260201
Conc: 2.77 ng/ml

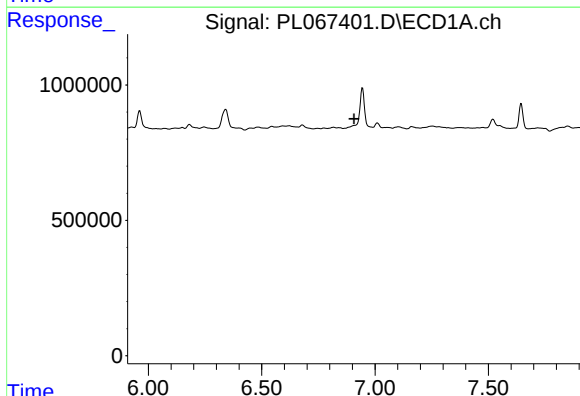


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.907 min
Response: 0
Conc: N.D.

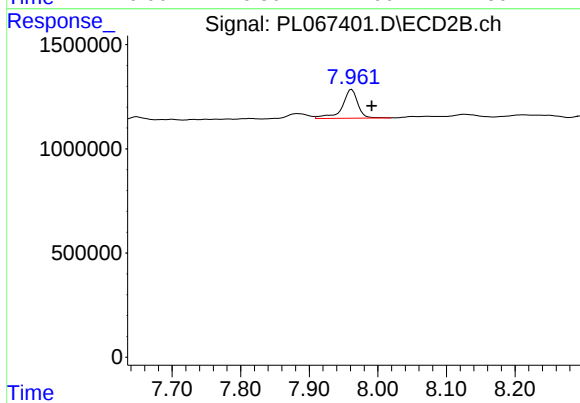

#8 Heptachlor epoxide


R.T.: 7.962 min
Delta R.T.: -0.029 min
Response: 2186503
Conc: 2.18 ng/ml

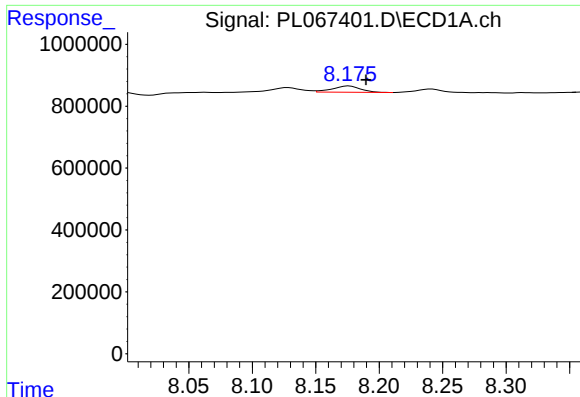

#15 Endosulfan II


R.T.: 8.176 min
Delta R.T.: -0.014 min
Response: 311817
Conc: 0.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

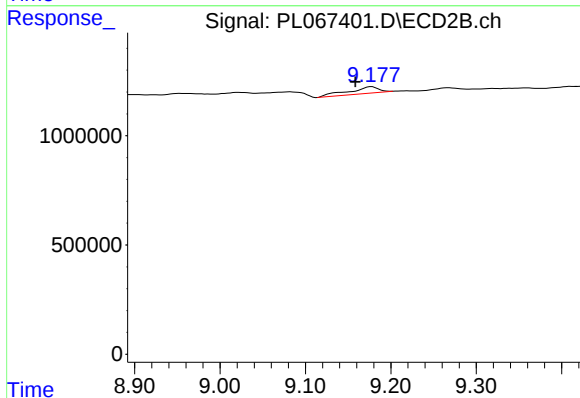


#15 Endosulfan II

R.T.: 9.178 min
Delta R.T.: 0.019 min
Response: 732547
Conc: 0.92 ng/ml

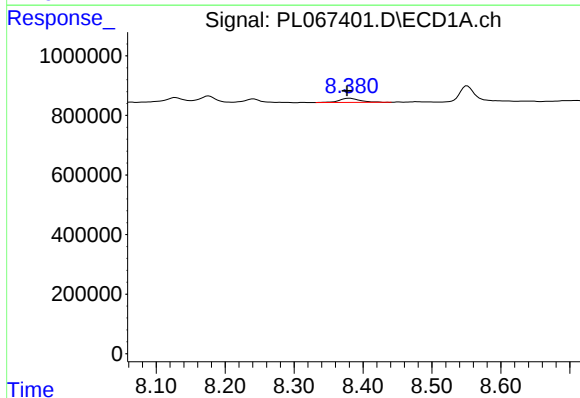


#18 Endrin aldehyde

R.T.: 8.380 min
Delta R.T.: 0.003 min
Response: 298529
Conc: 0.59 ng/ml

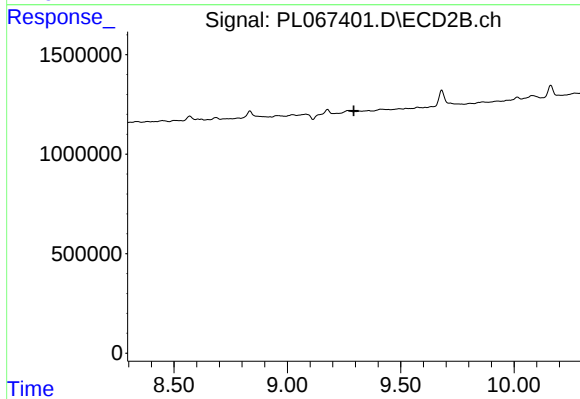

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 9.292 min
Response: 0
Conc: N.D.

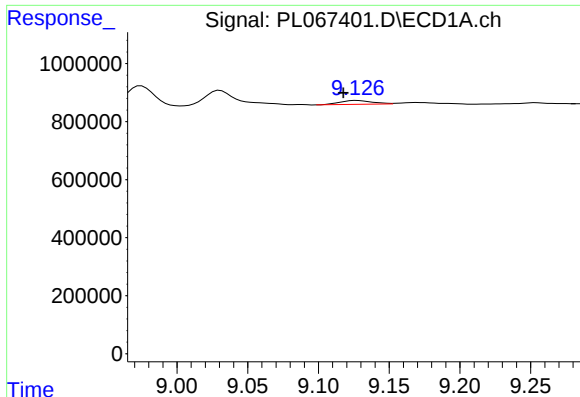

#21 Endrin ketone


R.T.: 9.127 min
Delta R.T.: 0.010 min
Response: 218967
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

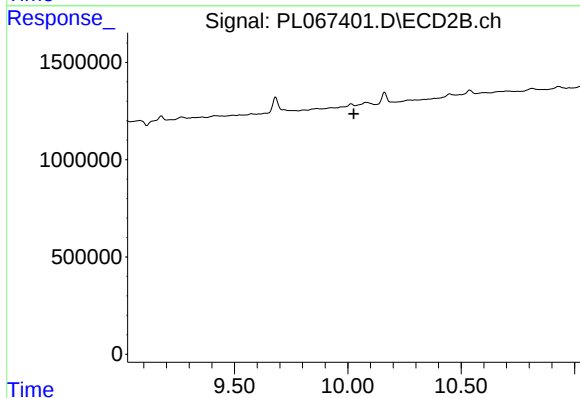


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 10.027 min
Response: 0
Conc: N.D.

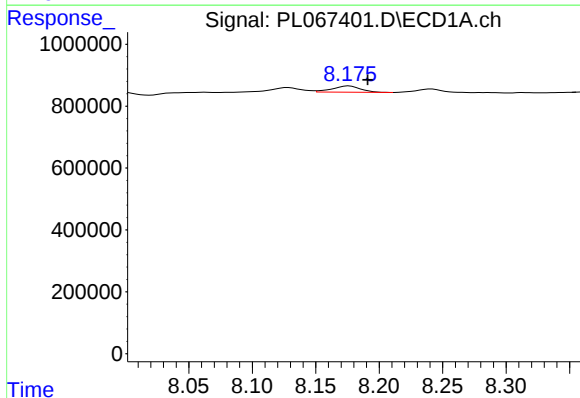


#27 Chlordane-5

R.T.: 8.176 min
Delta R.T.: -0.015 min
Response: 311817
Conc: 14.25 ng/ml

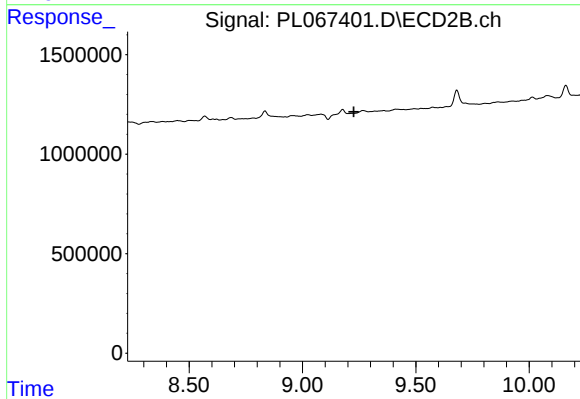

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

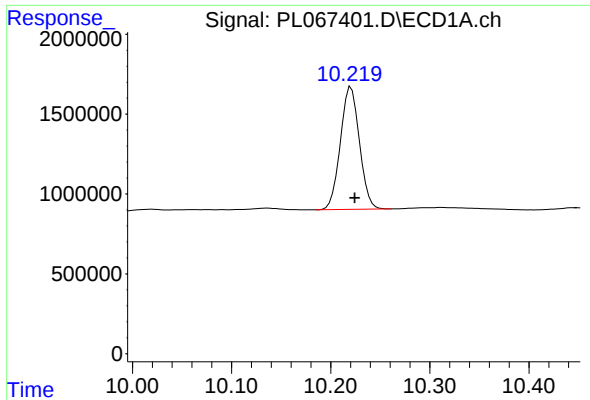

#28 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: -0.004 min
Response: 10237152
Conc: 14.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

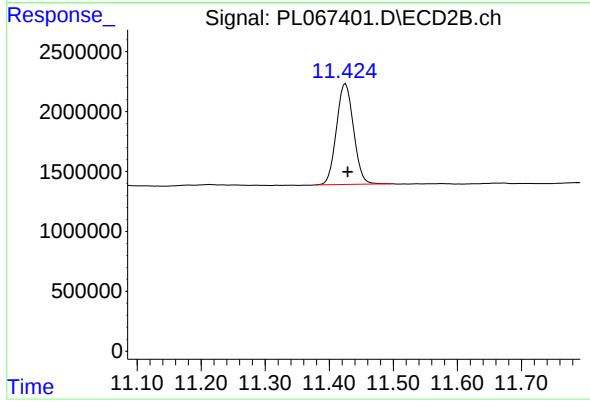

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.003 min
Response: 15609059
Conc: 15.67 ng/ml