

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061421\
 Data File : PL067414.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2021 17:00
 Operator : AR\AJ
 Sample : M2651-09
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 05:20:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	5.529	11446622	19926116	20.820	21.137
28)	SA Decachlor...	10.220	11.427	15431247	23724979	21.774	23.819
Target Compounds							
6)	B beta-BHC	5.963f	6.780f	651281	-593078	1.820	N.D. #
7)	B delta-BHC	0.000	7.006f	0	3382202	N.D.	2.877 #
8)	B Heptachlo...	0.000	7.962f	0	4920973	N.D.	4.912 #
11)	B alpha-Chl...	7.254	0.000	341640	0	0.467	N.D. #
26)	Chlordane-4	7.254	0.000	341640	0	4.675	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061421\
Data File : PL067414.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2021 17:00
Operator : AR\AJ
Sample : M2651-09
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 05:20:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

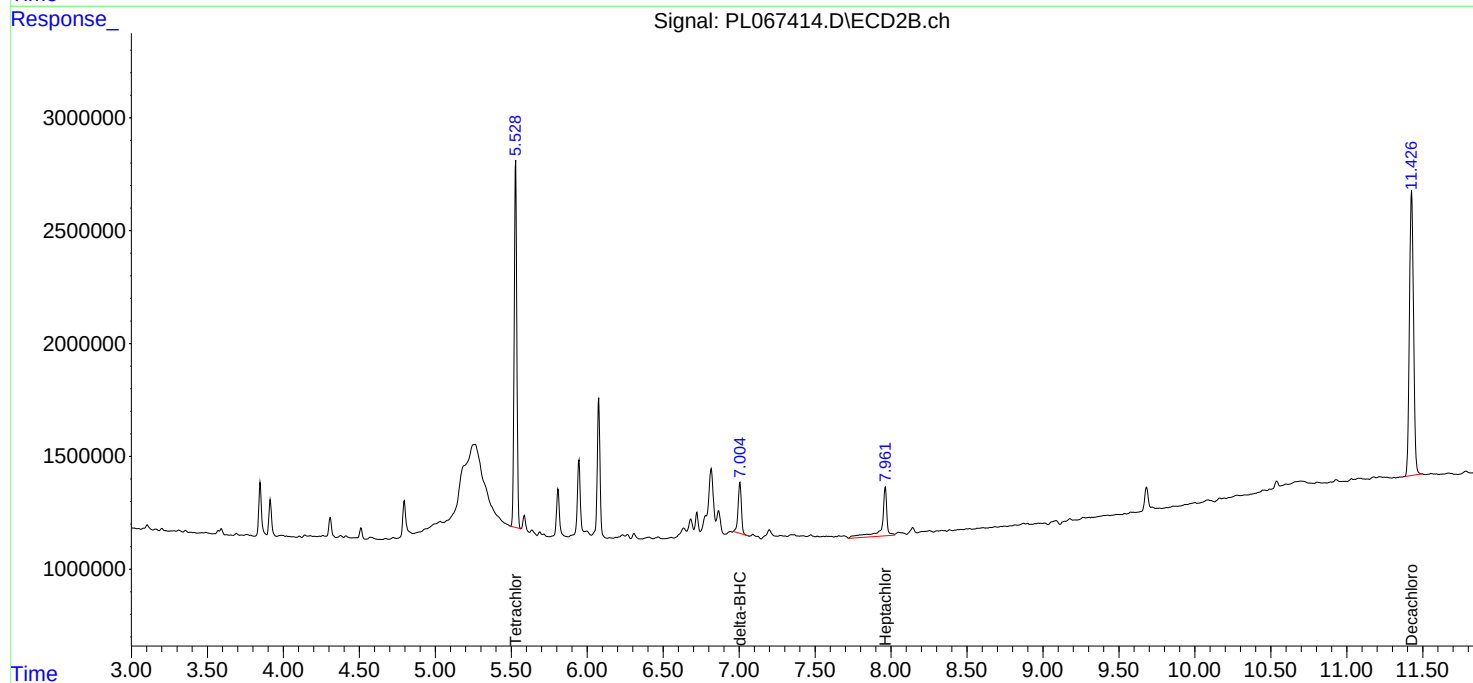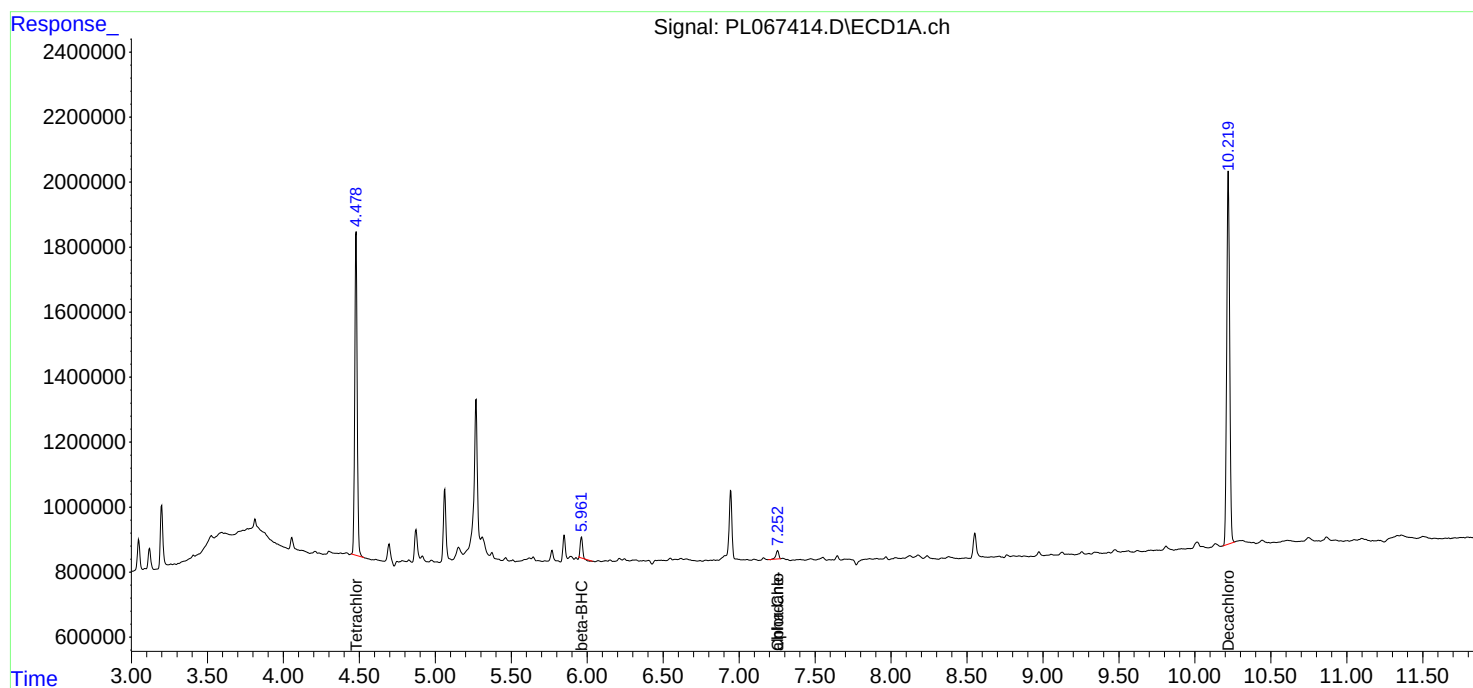


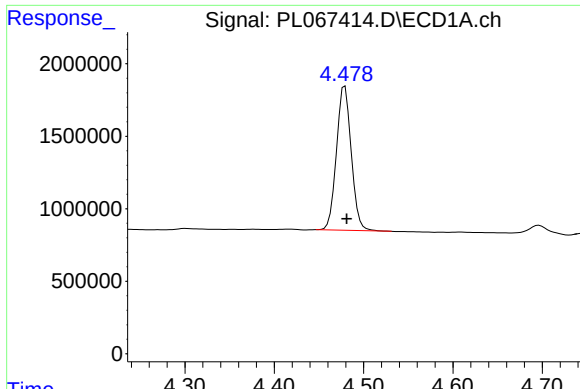

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: -0.002 min
Response: 11446622
Conc: 20.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

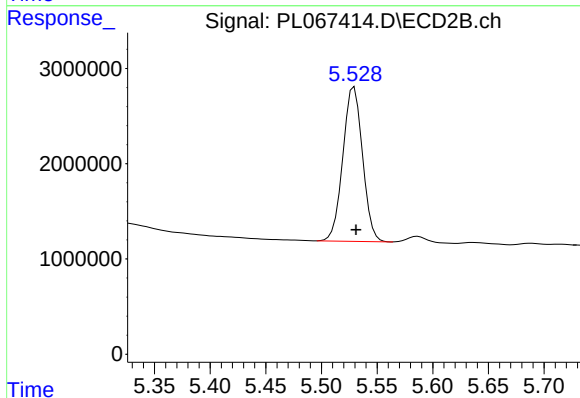


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 19926116
Conc: 21.14 ng/ml

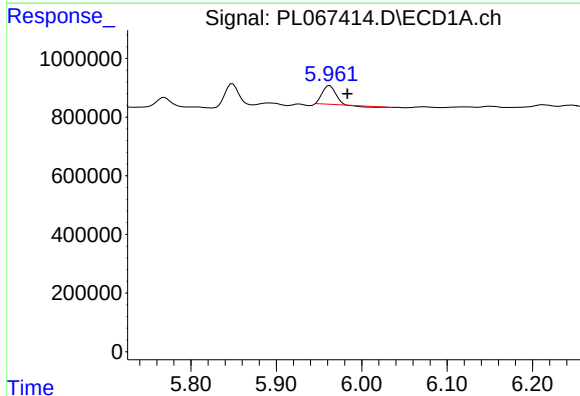


#6 beta-BHC

R.T.: 5.963 min
Delta R.T.: -0.021 min
Response: 651281
Conc: 1.82 ng/ml

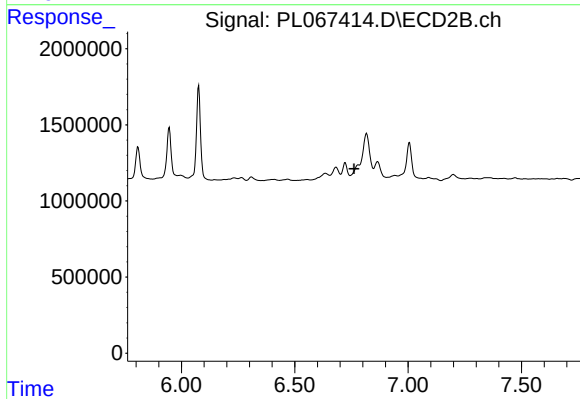

#6 beta-BHC


R.T.: 6.780 min
Delta R.T.: 0.018 min
Response: -593078
Conc: N.D.

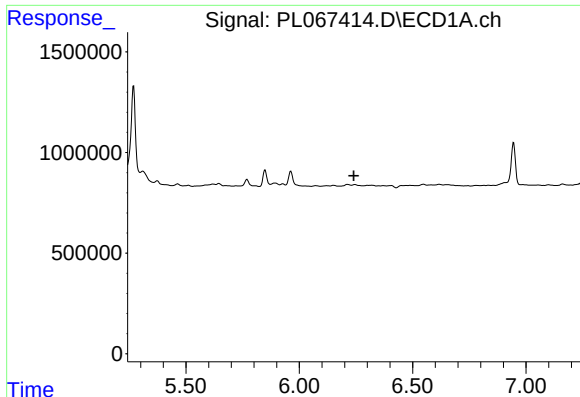

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

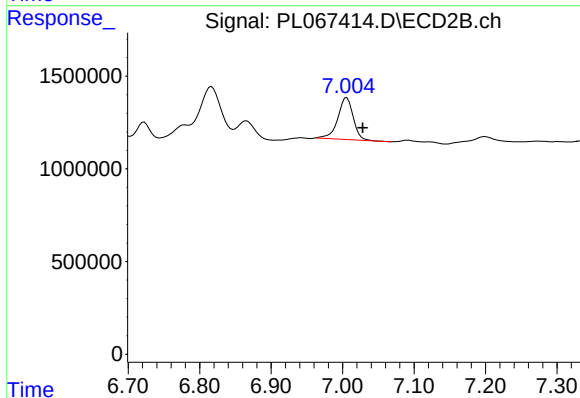


#7 delta-BHC

R.T.: 7.006 min
Delta R.T.: -0.022 min
Response: 3382202
Conc: 2.88 ng/ml

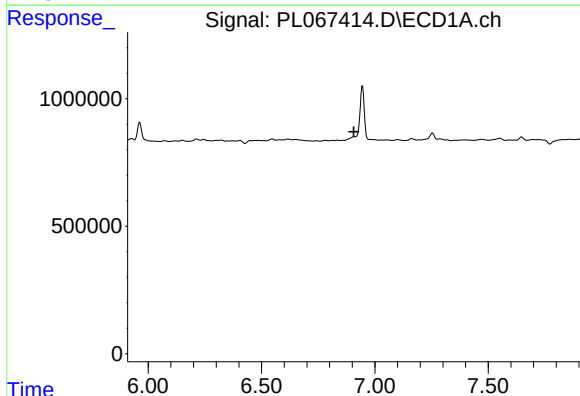


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 6.907 min
Response: 0
Conc: N.D.

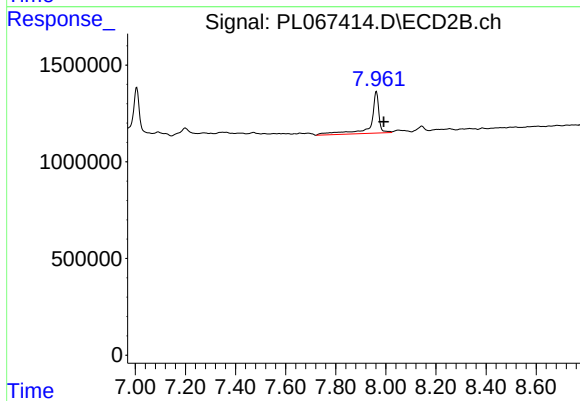

#8 Heptachlor epoxide


R.T.: 7.962 min
Delta R.T.: -0.029 min
Response: 4920973
Conc: 4.91 ng/ml

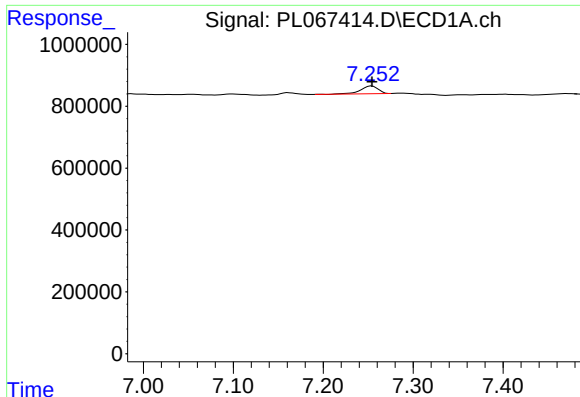

#11 alpha-Chlordane


R.T.: 7.254 min
Delta R.T.: 0.000 min
Response: 341640
Conc: 0.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

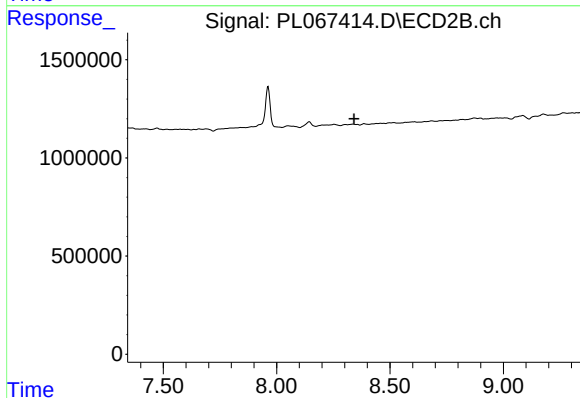


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.342 min
Response: 0
Conc: N.D.

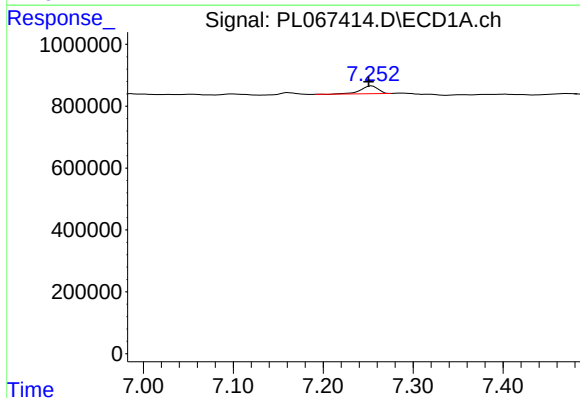


#26 Chlordane-4

R.T.: 7.254 min
Delta R.T.: 0.004 min
Response: 341640
Conc: 4.67 ng/ml

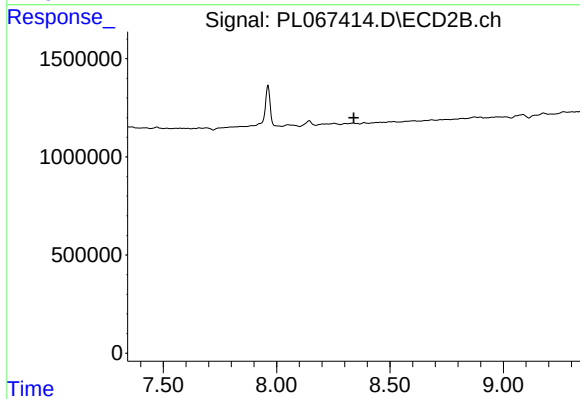

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 8.341 min
Response: 0
Conc: N.D.

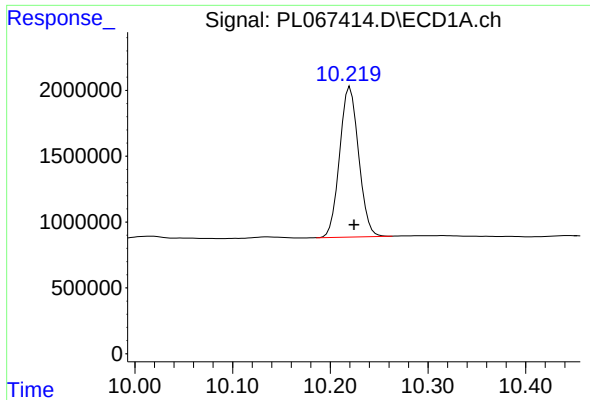

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.004 min
Response: 15431247
Conc: 21.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

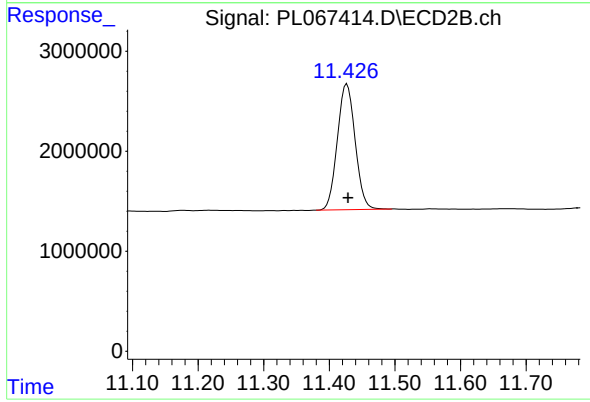

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.002 min
Response: 23724979
Conc: 23.82 ng/ml