

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061421\
 Data File : PL067415.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2021 17:17
 Operator : AR\AJ
 Sample : M2651-10
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 05:21:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	5.529	11349343	20389270	20.643	21.628
28)	SA Decachlor...	10.220	11.427	15992153	25127976	22.566	25.227
Target Compounds							
2)	A alpha-BHC	5.162f	0.000	222521	0	0.303	N.D. #
6)	B beta-BHC	5.962f	6.779f	903400	-1180516	2.525	N.D. #
7)	B delta-BHC	0.000	7.005f	0	4223157	N.D.	3.593 #
8)	B Heptachlo...	0.000	7.962f	0	3879698	N.D.	3.873 #
15)	B Endosulfa...	0.000	9.178f	0	791639	N.D.	0.993 #
24)	Chlordane-2	6.465f	0.000	350382	0	13.085	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061421\
Data File : PL067415.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2021 17:17
Operator : AR\AJ
Sample : M2651-10
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 05:21:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

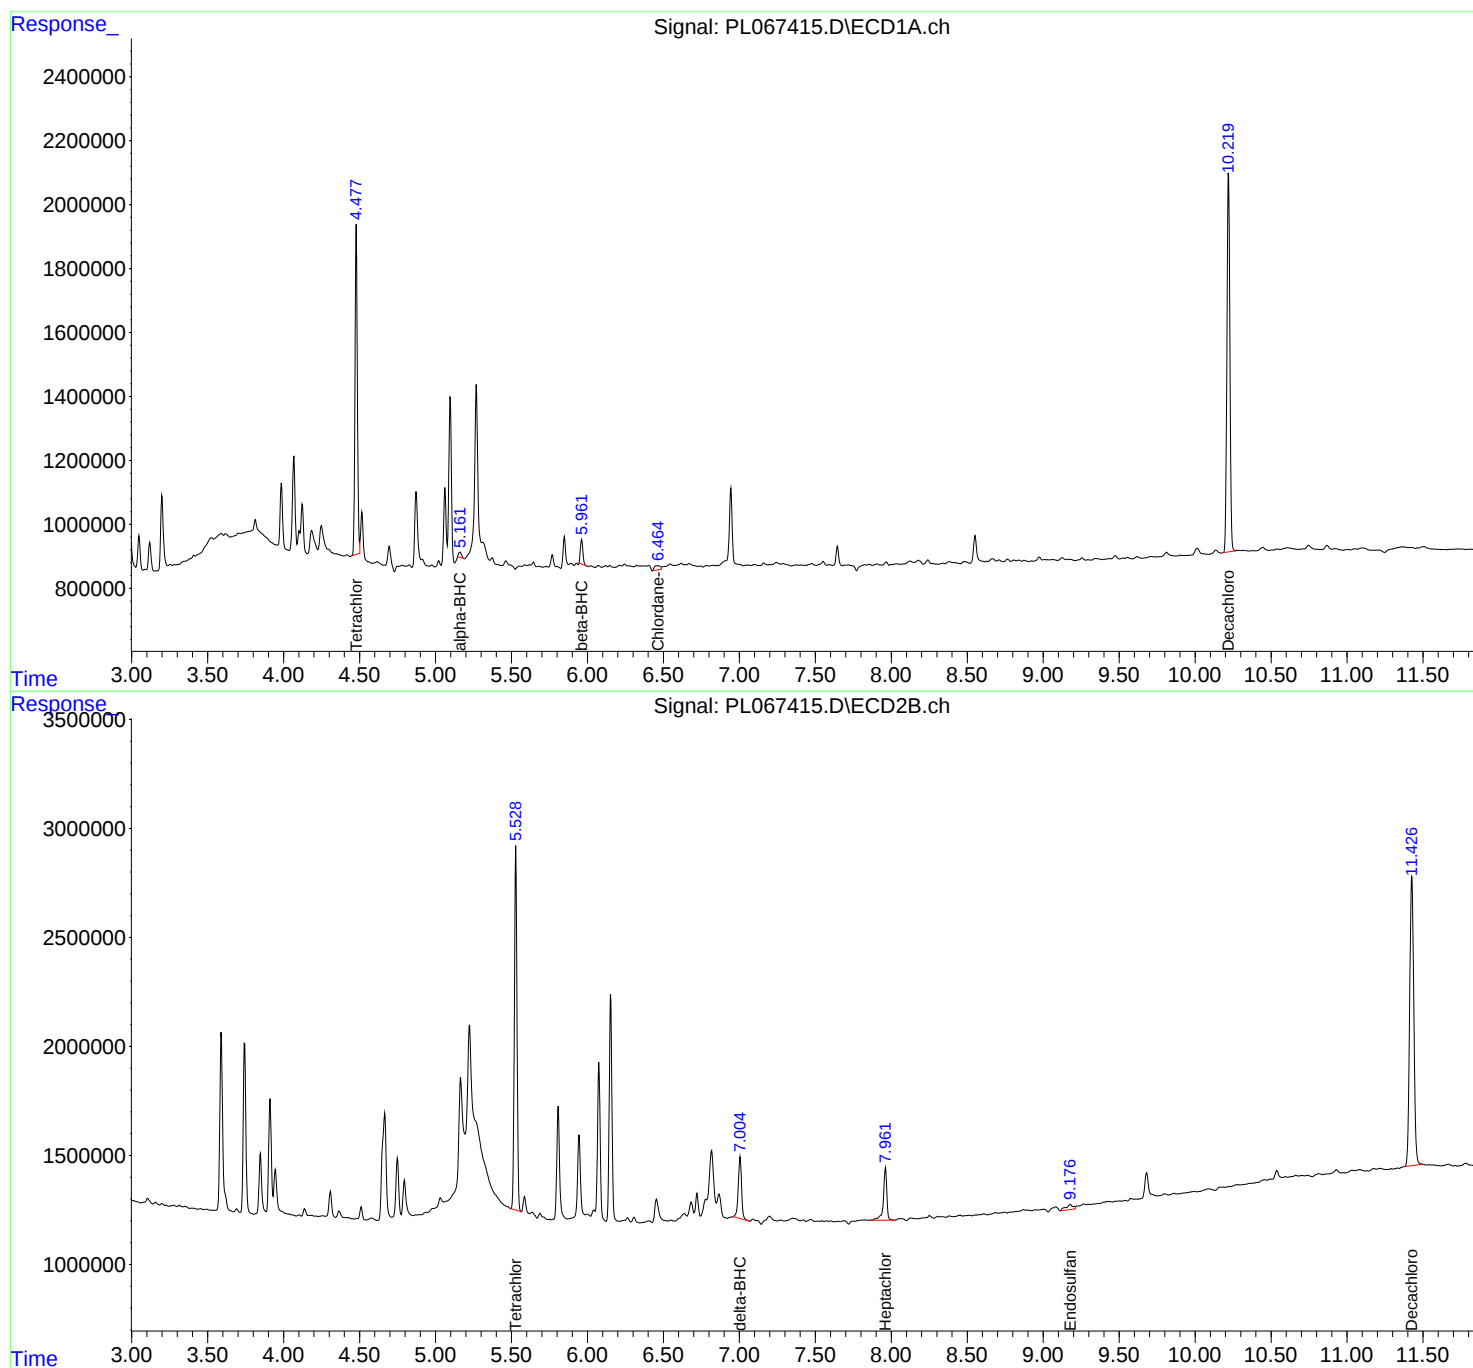


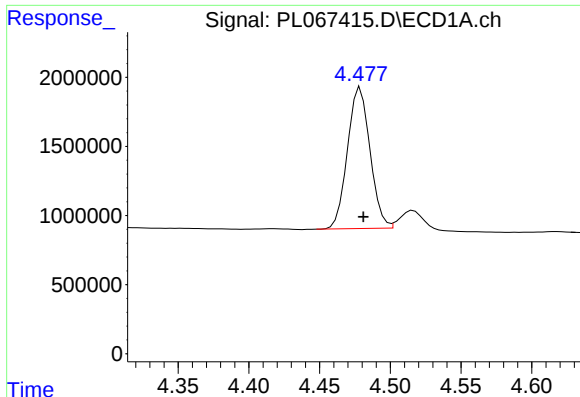

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: -0.002 min
Response: 11349343
Conc: 20.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

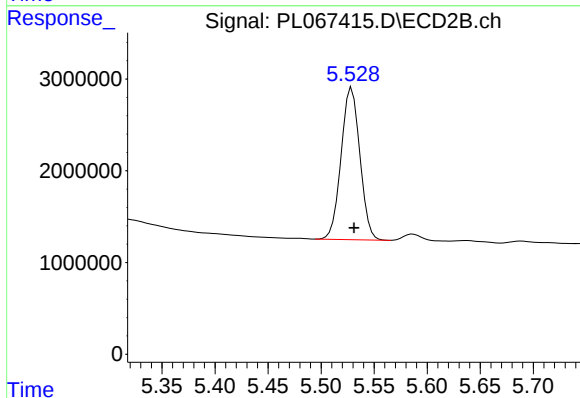


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 20389270
Conc: 21.63 ng/ml

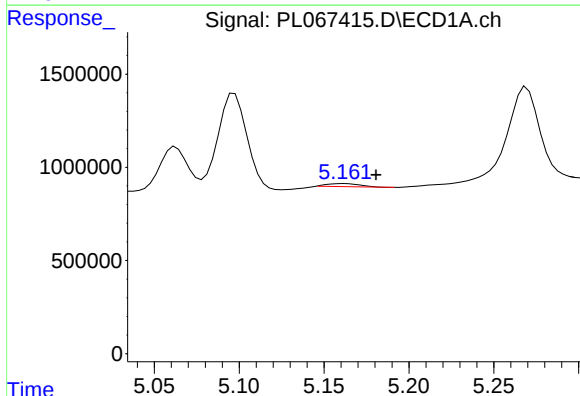


#2 alpha-BHC

R.T.: 5.162 min
Delta R.T.: -0.019 min
Response: 222521
Conc: 0.30 ng/ml

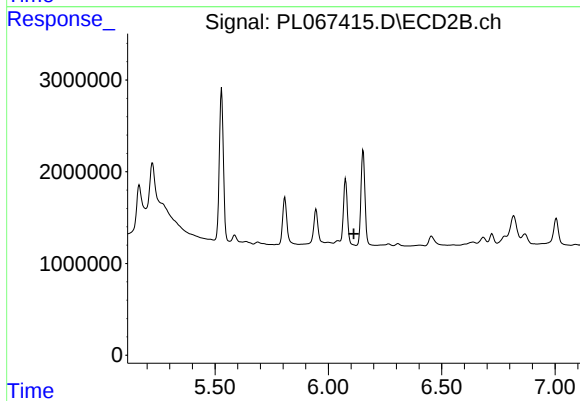

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 6.112 min
Response: 0
Conc: N.D.

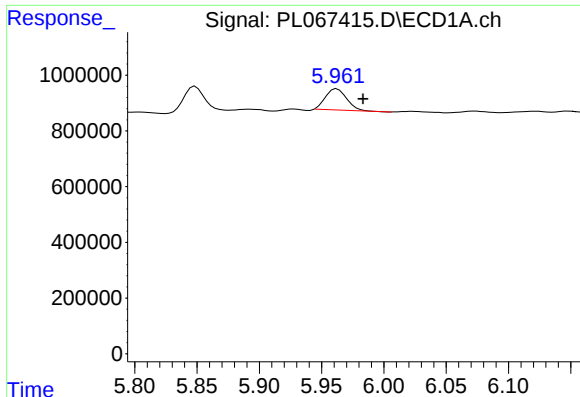

#6 beta-BHC


R.T.: 5.962 min
Delta R.T.: -0.021 min
Response: 903400
Conc: 2.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

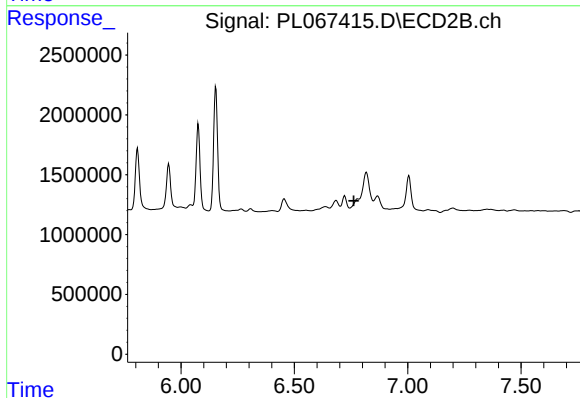


#6 beta-BHC

R.T.: 6.779 min
Delta R.T.: 0.017 min
Response: -1180516
Conc: N.D.

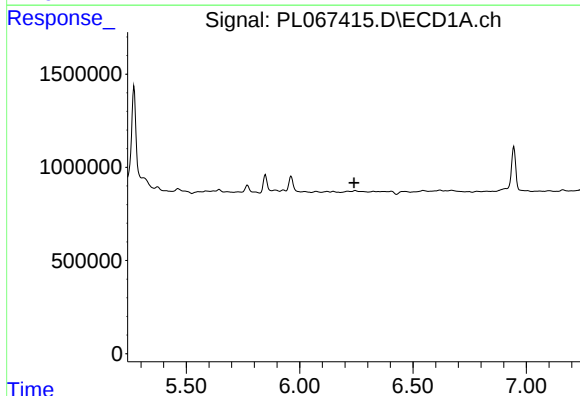


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

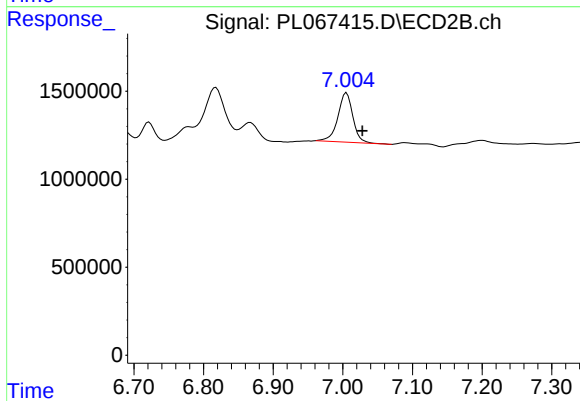

#7 delta-BHC


R.T.: 7.005 min
Delta R.T.: -0.023 min
Response: 4223157
Conc: 3.59 ng/ml

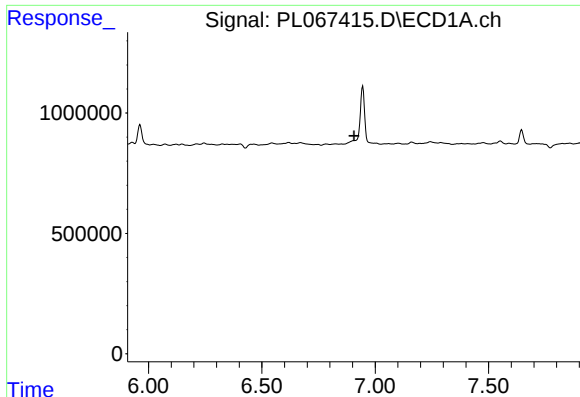

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 6.907 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

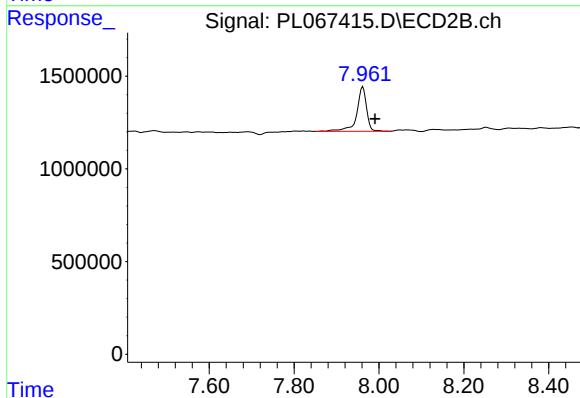


#8 Heptachlor epoxide

R.T.: 7.962 min
Delta R.T.: -0.029 min
Response: 3879698
Conc: 3.87 ng/ml

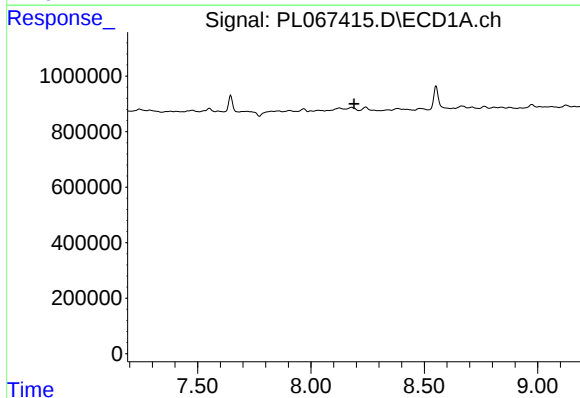


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.190 min
Response: 0
Conc: N.D.

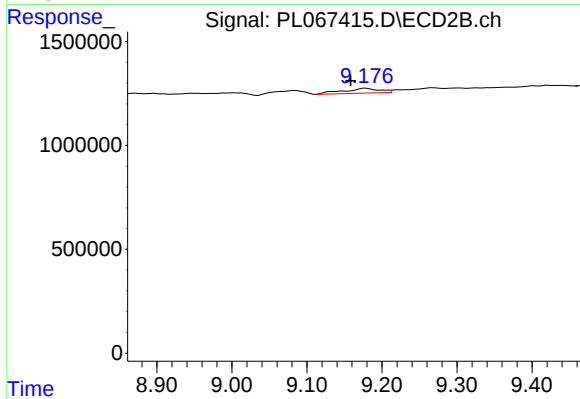

#15 Endosulfan II


R.T.: 9.178 min
Delta R.T.: 0.019 min
Response: 791639
Conc: 0.99 ng/ml

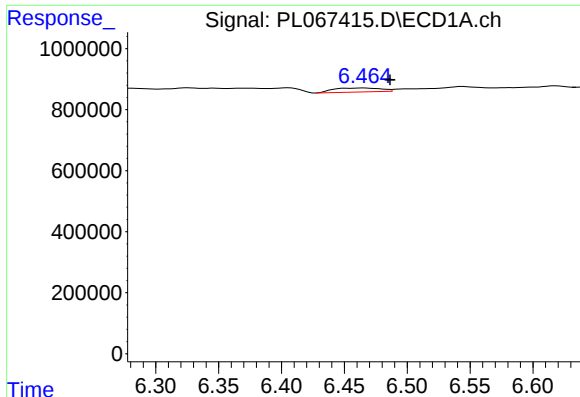

#24 Chlordane-2


R.T.: 6.465 min
Delta R.T.: -0.021 min
Response: 350382
Conc: 13.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

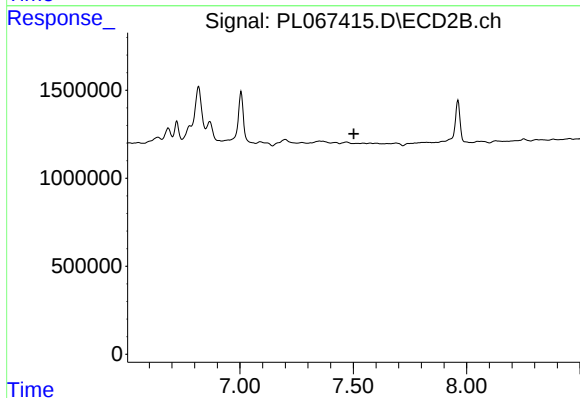


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

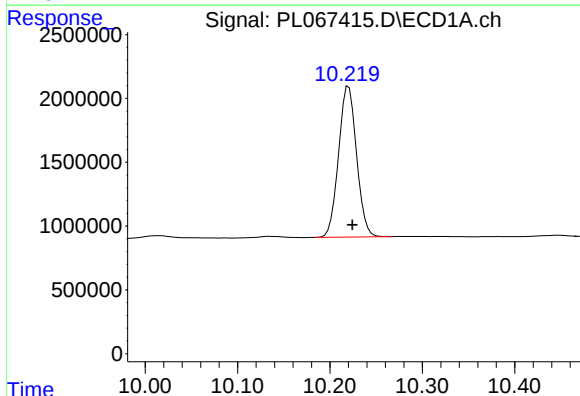

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.004 min
Response: 15992153
Conc: 22.57 ng/ml

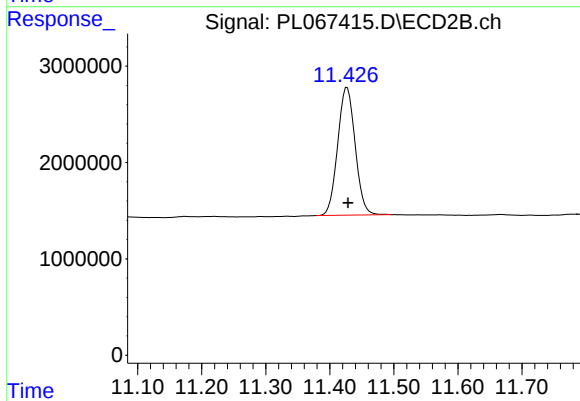

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.002 min
Response: 25127976
Conc: 25.23 ng/ml