

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061421\
 Data File : PL067441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2021 01:18
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 05:27:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.528	10635392	18837991	19.345	19.982
28)	SA Decachlor...	10.220	11.426	12680449	19670842	17.893	19.749
Target Compounds							
2)	A alpha-BHC	5.168	0.000	262971	0	0.358	N.D. #
4)	MA Heptachlor	5.988f	0.000	466569	0	0.619	N.D. #
6)	B beta-BHC	5.988	0.000	466569	0	1.304	N.D. #
8)	B Heptachlo...	0.000	7.994	0	724964	N.D.	0.724 #
13)	MA Dieldrin	0.000	8.695	0	345847	N.D.	0.381 #
20)	A Methoxychlor	0.000	9.892f	0	54436	N.D.	0.140 #
21)	B Endrin ke...	0.000	10.031	0	185385	N.D.	0.205 #
24)	Chlordane-2	6.486	0.000	189694	0	7.084	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061421\
Data File : PL067441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2021 01:18
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 05:27:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

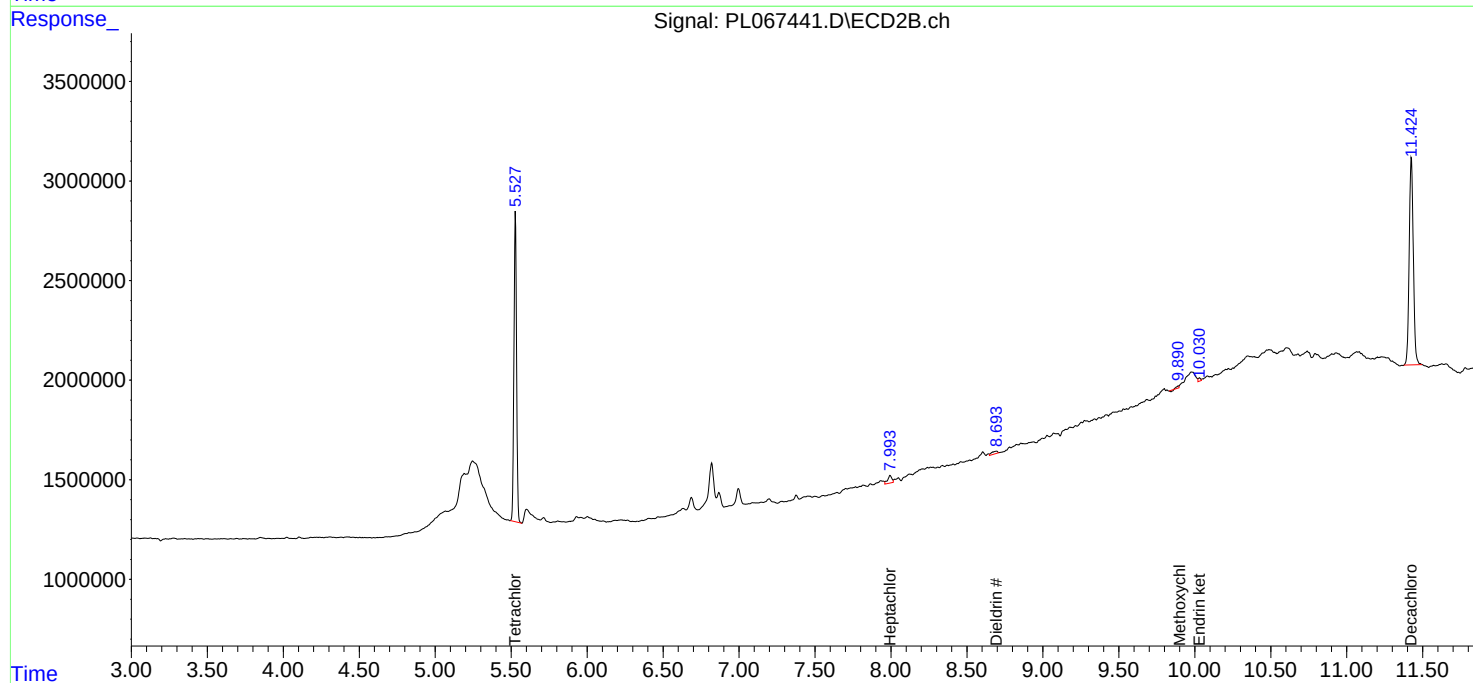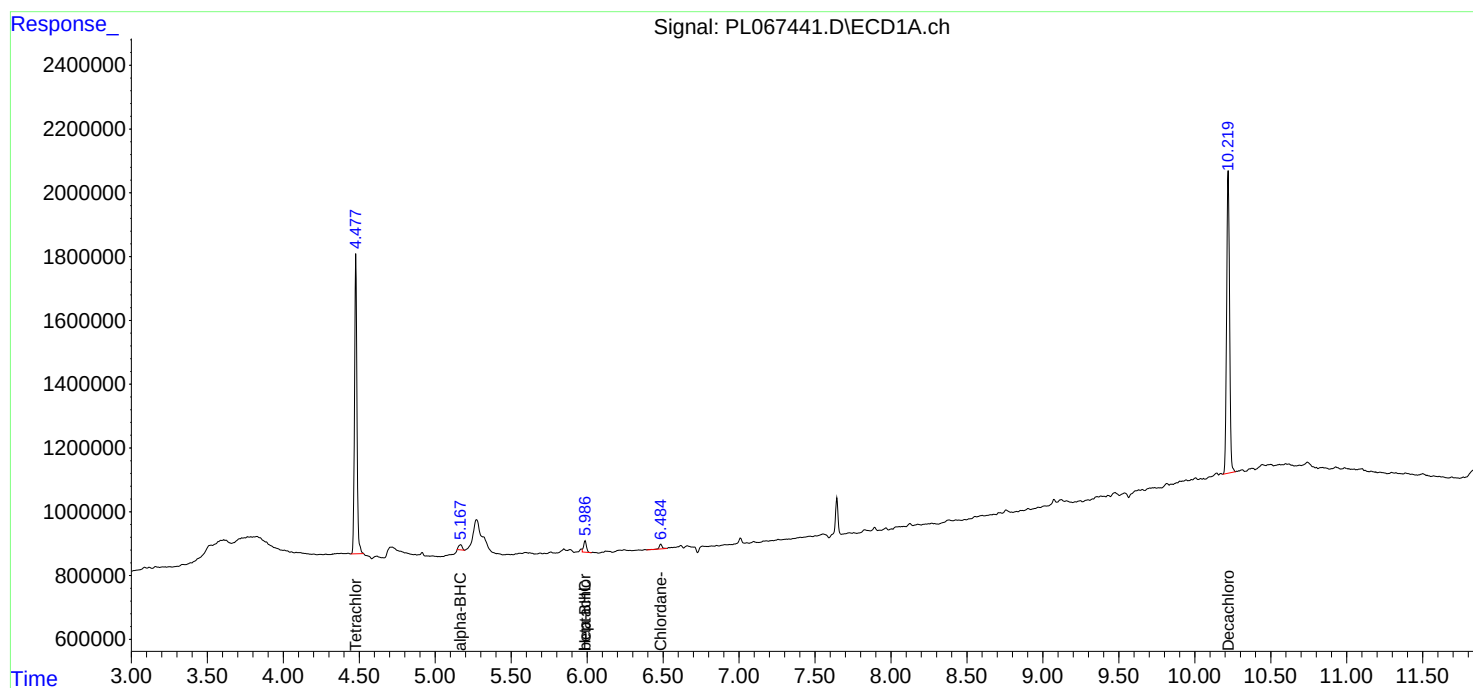


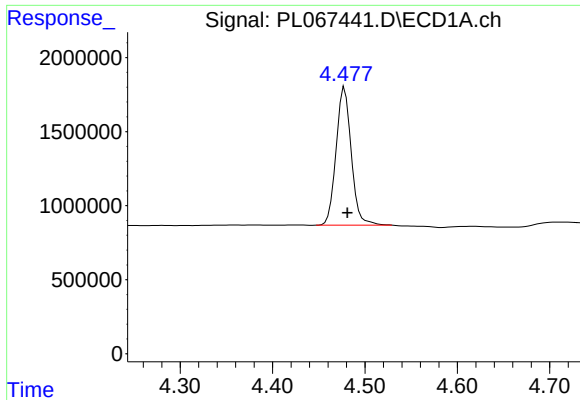

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 10635392
Conc: 19.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

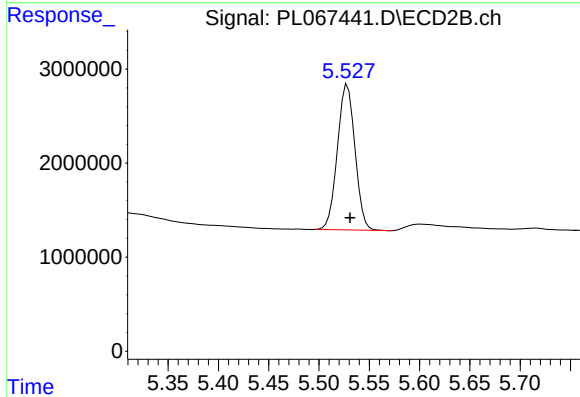


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 18837991
Conc: 19.98 ng/ml

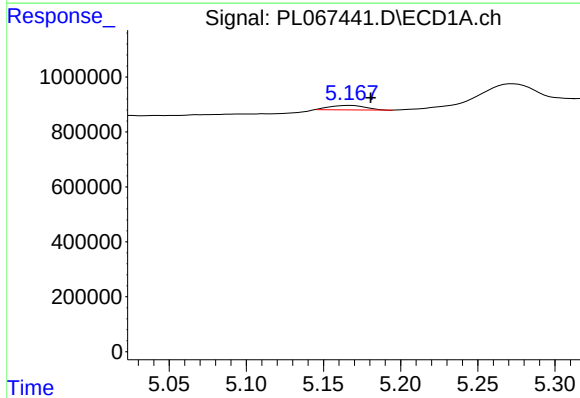


#2 alpha-BHC

R.T.: 5.168 min
Delta R.T.: -0.013 min
Response: 262971
Conc: 0.36 ng/ml

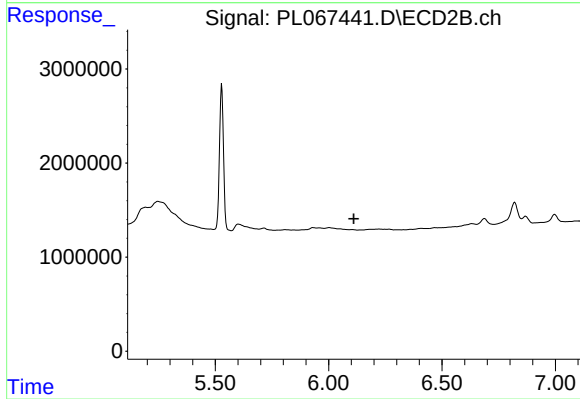

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 6.112 min
Response: 0
Conc: N.D.

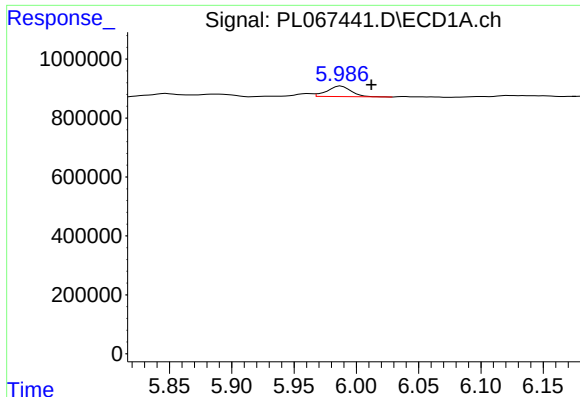

#4 Heptachlor


R.T.: 5.988 min
Delta R.T.: -0.024 min
Response: 466569
Conc: 0.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

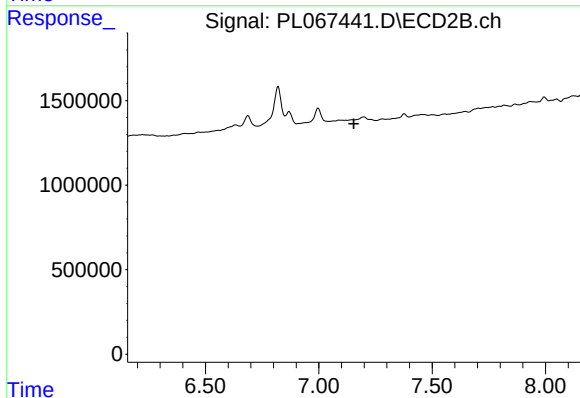


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.155 min
Response: 0
Conc: N.D.

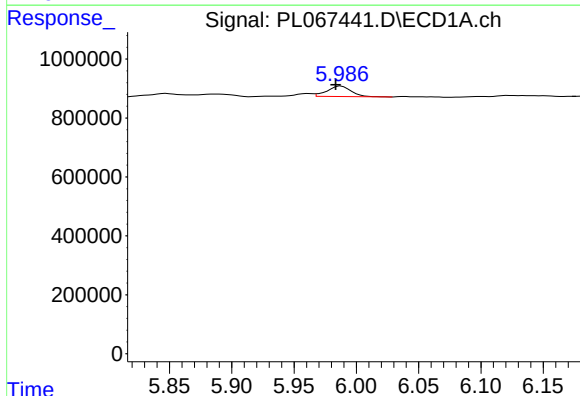


#6 beta-BHC

R.T.: 5.988 min
Delta R.T.: 0.004 min
Response: 466569
Conc: 1.30 ng/ml

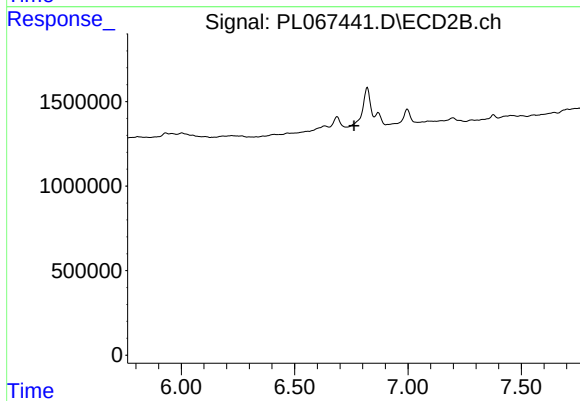

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

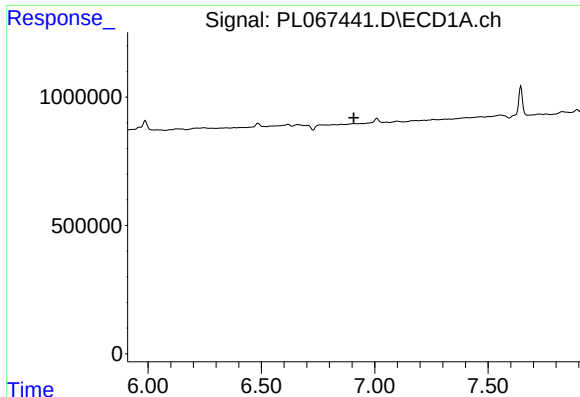

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 6.907 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

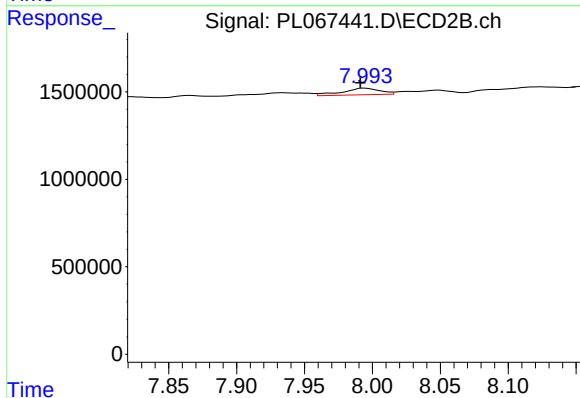


#8 Heptachlor epoxide

R.T.: 7.994 min
Delta R.T.: 0.003 min
Response: 724964
Conc: 0.72 ng/ml

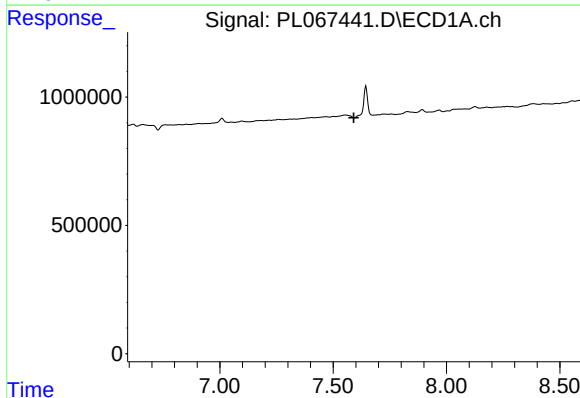


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 7.592 min
Response: 0
Conc: N.D.

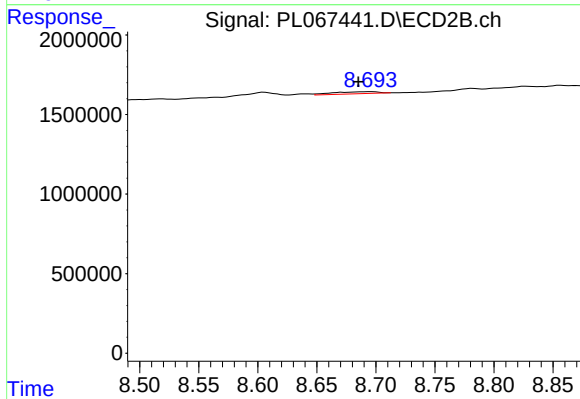

#13 Dieldrin


R.T.: 8.695 min
Delta R.T.: 0.010 min
Response: 345847
Conc: 0.38 ng/ml

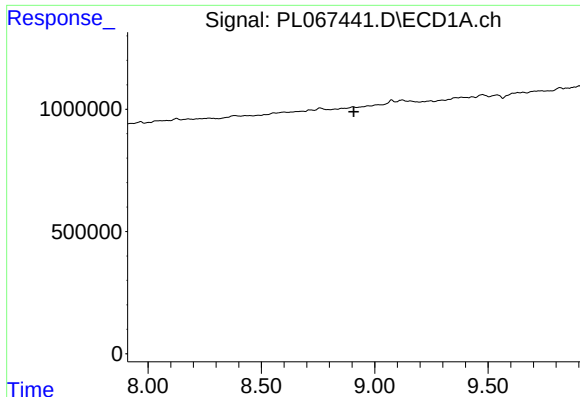

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 8.908 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

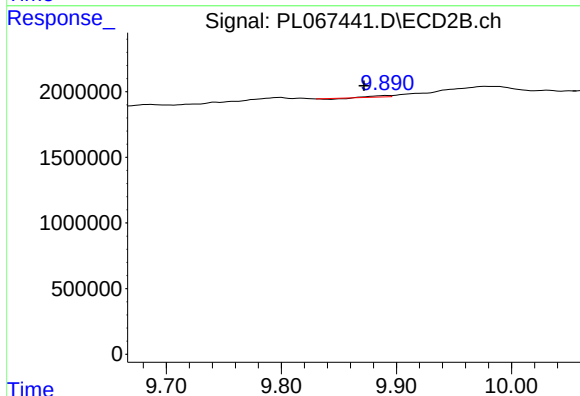


#20 Methoxychlor

R.T.: 9.892 min
Delta R.T.: 0.020 min
Response: 54436
Conc: 0.14 ng/ml

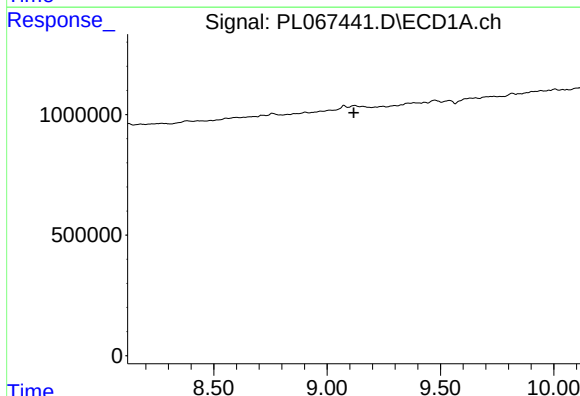


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.118 min
Response: 0
Conc: N.D.

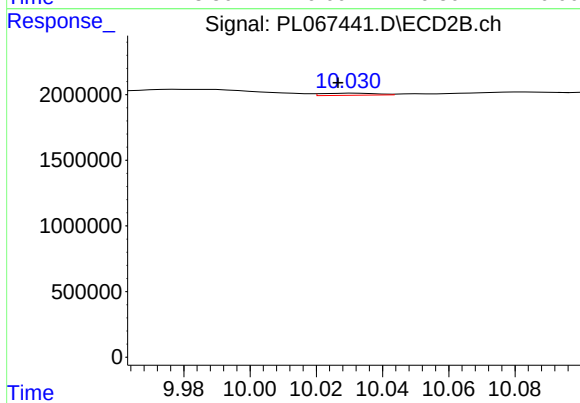

#21 Endrin ketone


R.T.: 10.031 min
Delta R.T.: 0.005 min
Response: 185385
Conc: 0.20 ng/ml

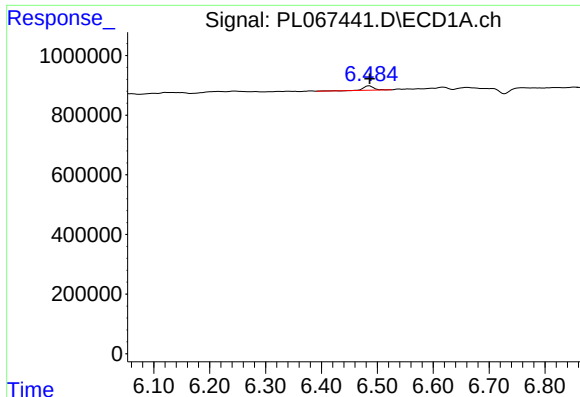

#24 Chlordane-2


R.T.: 6.486 min
Delta R.T.: 0.000 min
Response: 189694
Conc: 7.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

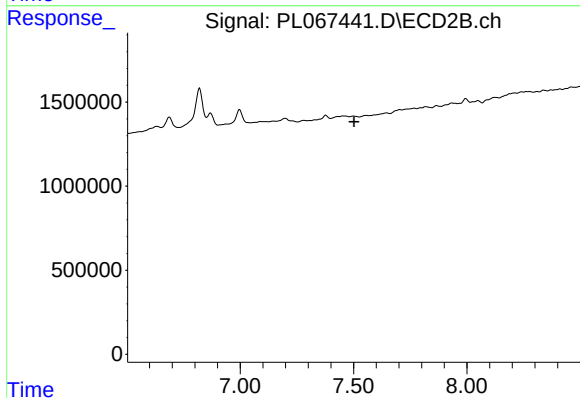


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

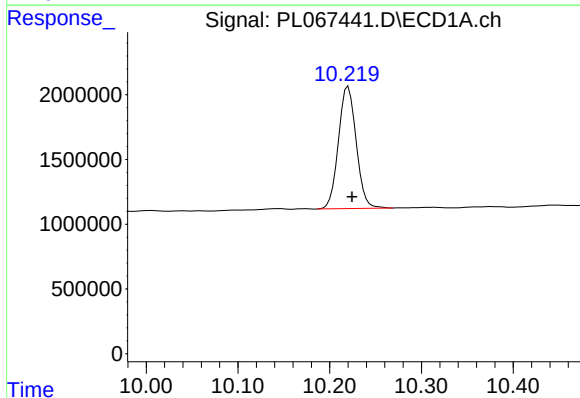

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.004 min
Response: 12680449
Conc: 17.89 ng/ml

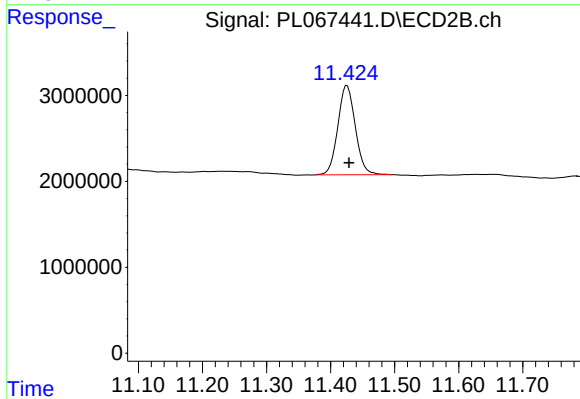

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.003 min
Response: 19670842
Conc: 19.75 ng/ml