

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061421\
 Data File : PL067435.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2021 23:39
 Operator : AR\AJ
 Sample : M2674-07
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TMR-DS-01-060921

Manual Integrations
 APPROVED

Ankita
 6/15/2021 2:40:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 05:25:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	5.529	9753496	15128846	17.741	16.048
28)	SA Decachlor...	10.220	11.427	14203765	21874937	20.042	21.962
Target Compounds							
9)	A Endosulfan I	7.313	8.410	3049387	53460515	4.536	58.546m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061421\
Data File : PL067435.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2021 23:39
Operator : AR\AJ
Sample : M2674-07
Misc :
ALS Vial : 44 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampled :
TMR-DS-01-060921


Manual Integrations
APPROVED

Ankita
6/15/2021 2:40:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 05:25:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

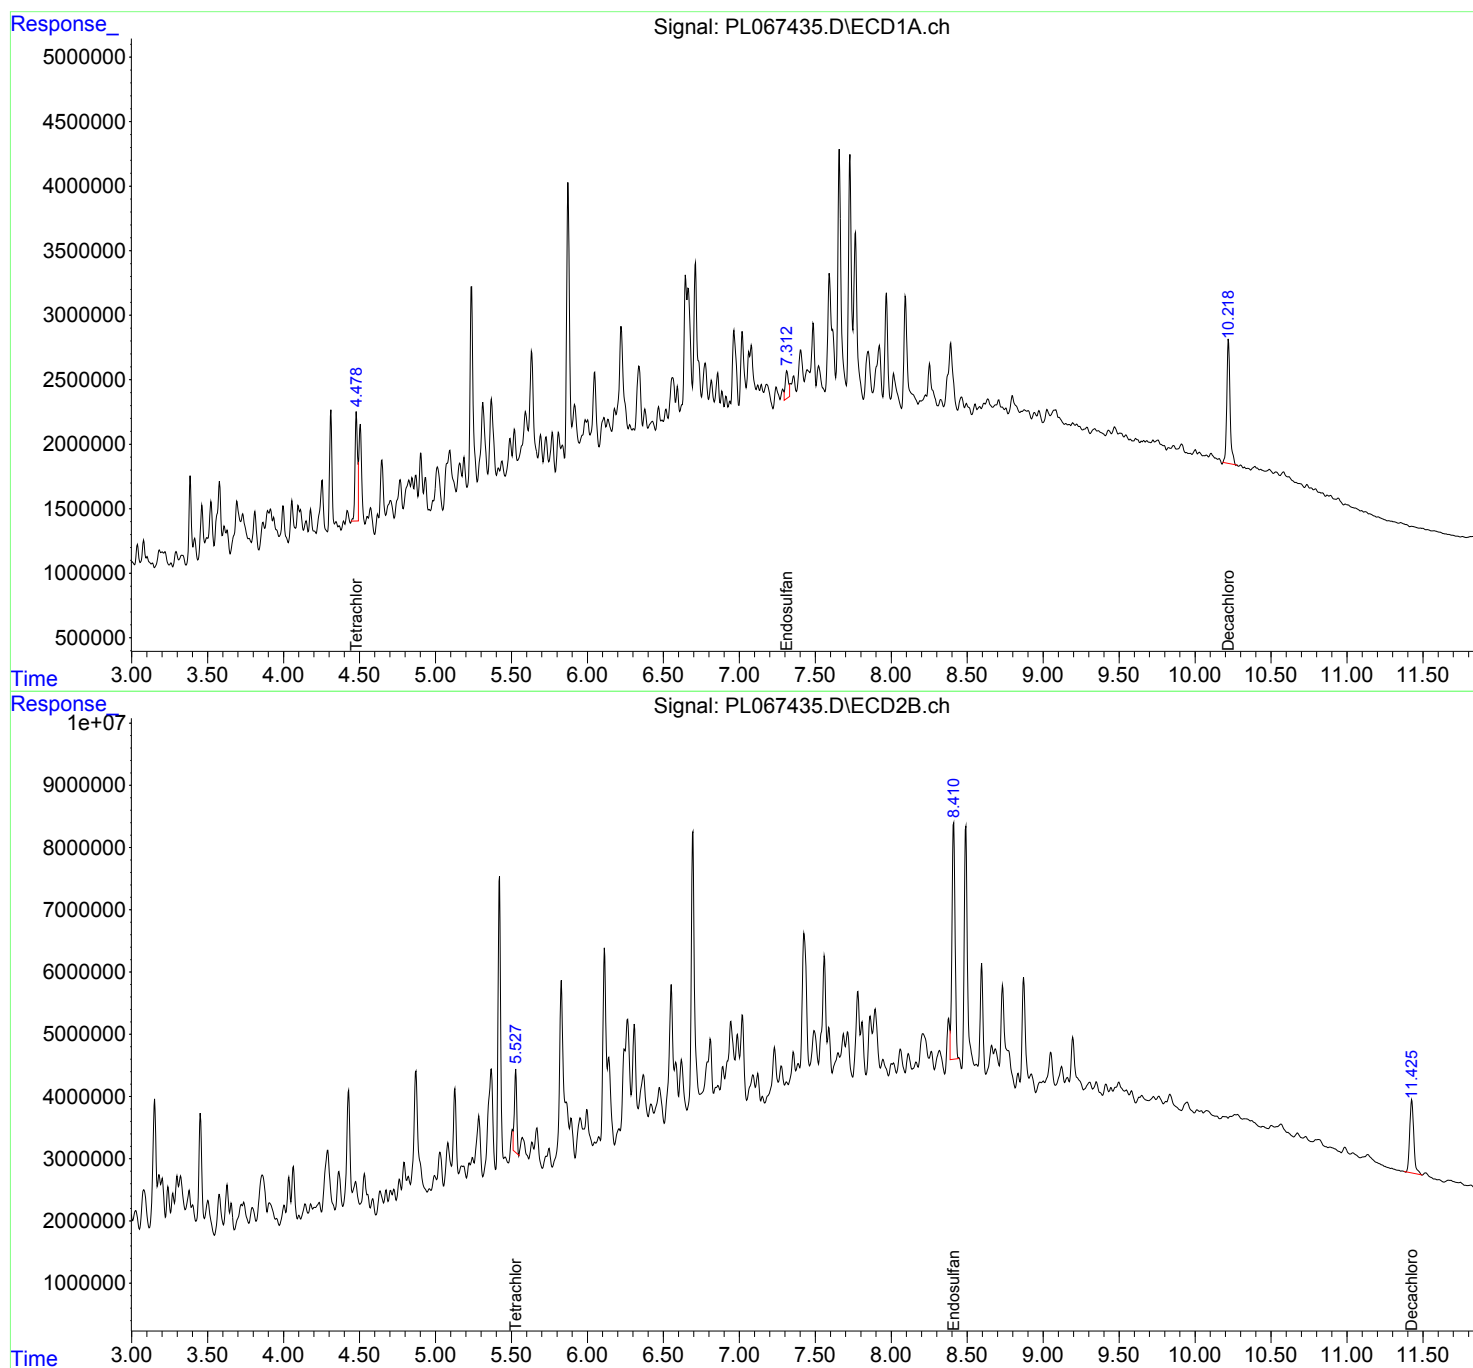

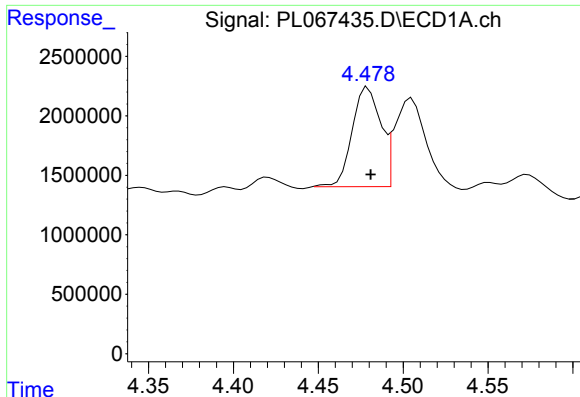


#1 Tetrachloro-m-xylene

R.T.: 4.479 min
Delta R.T.: -0.002 min
Response: 9753496
Conc: 17.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
TMR-DS-01-060921


Manual Integrations
APPROVED

Ankita
6/15/2021 2:40:35 PM

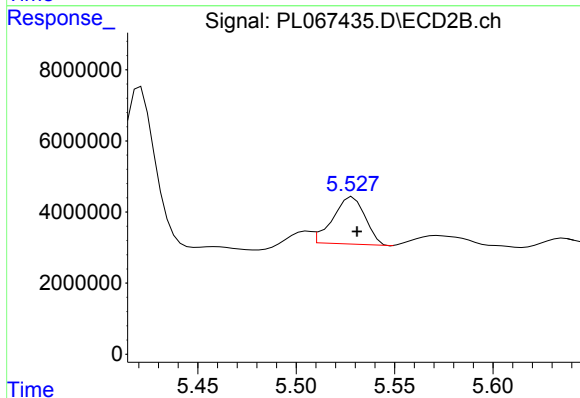


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 15128846
Conc: 16.05 ng/ml

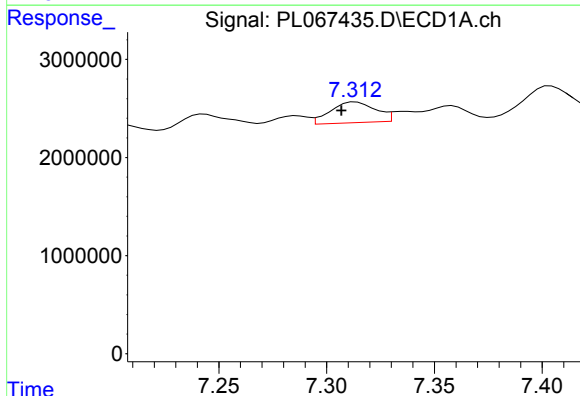


#9 Endosulfan I

R.T.: 7.313 min
Delta R.T.: 0.006 min
Response: 3049387
Conc: 4.54 ng/ml

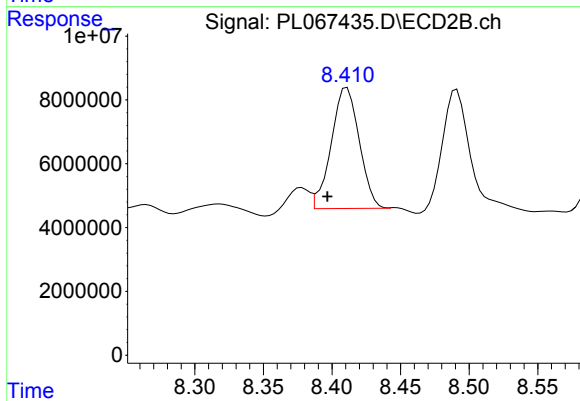

#9 Endosulfan I

R.T.: 8.410 min
Delta R.T.: 0.013 min
Response: 53460515
Conc: 58.55 ng/ml m

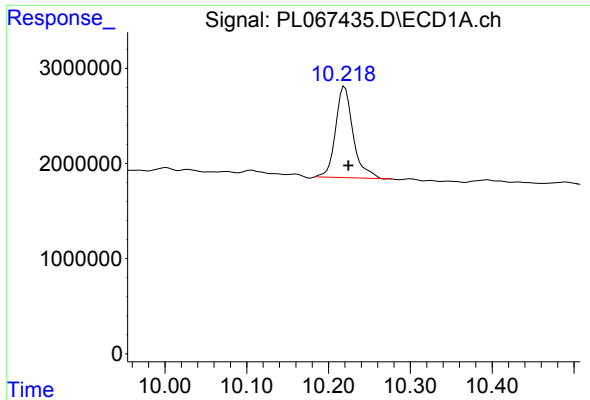


#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.004 min
Response: 14203765
Conc: 20.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
TMR-DS-01-060921

Manual Integrations
APPROVED

Ankita
6/15/2021 2:40:35 PM

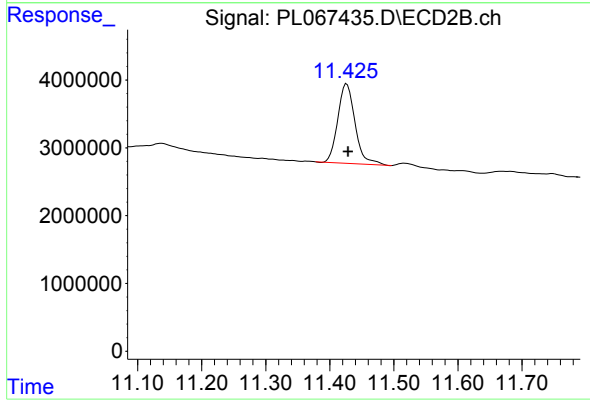

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.002 min
Response: 21874937
Conc: 21.96 ng/ml