

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061421\
 Data File : PL067437.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2021 00:12
 Operator : AR\AJ
 Sample : M2674-09
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TMR-DS-03-060921

Manual Integrations
 APPROVED

Ankita
 6/15/2021 2:40:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 05:26:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.529	9479838	14381999	17.243	15.256
28)	SA Decachlor...	10.219	11.427	14150687	21812616	19.968	21.899
Target Compounds							
2)	A alpha-BHC	5.188	6.112	2253188	72639850	3.063	58.748m#
13)	MA Dieldrin	7.592	8.685	28705755	6193717	40.950m	6.820m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061421\
Data File : PL067437.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2021 00:12
Operator : AR\AJ
Sample : M2674-09
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TMR-DS-03-060921


Manual Integrations
APPROVED

Ankita
6/15/2021 2:40:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 05:26:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

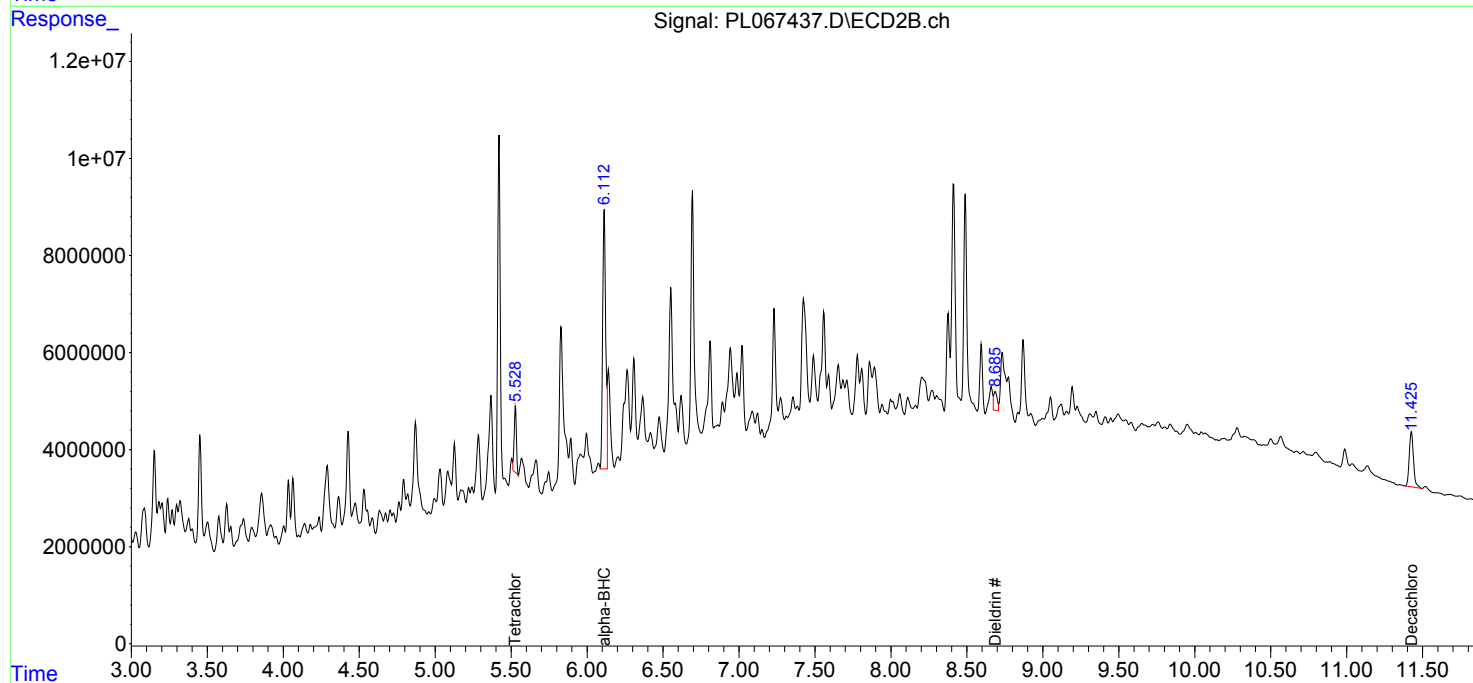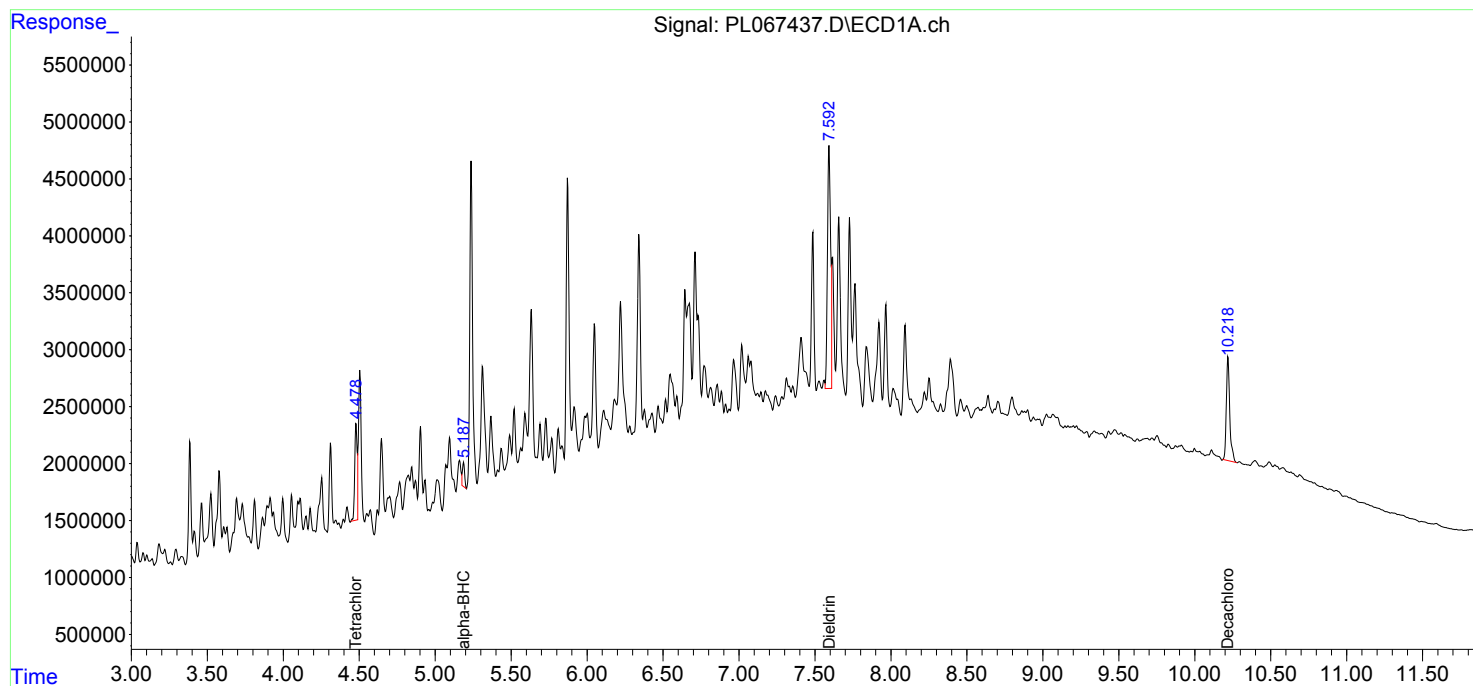

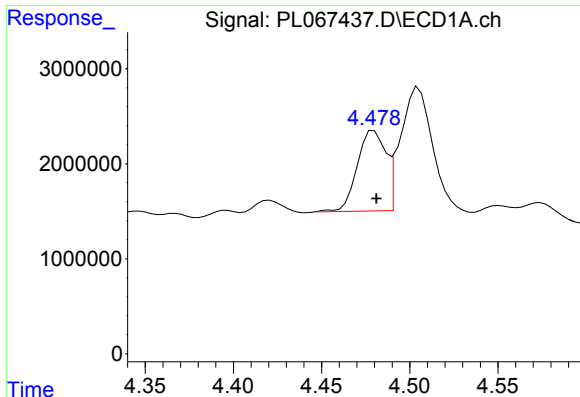


#1 Tetrachloro-m-xylene

R.T.: 4.480 min
Delta R.T.: -0.001 min
Response: 9479838
Conc: 17.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
TMR-DS-03-060921


Manual Integrations
APPROVED

Ankita
6/15/2021 2:40:39 PM

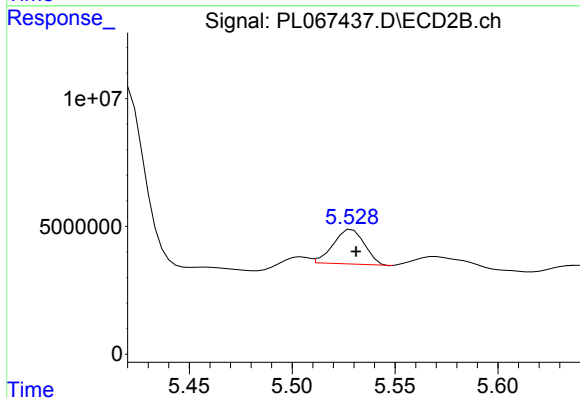


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 14381999
Conc: 15.26 ng/ml

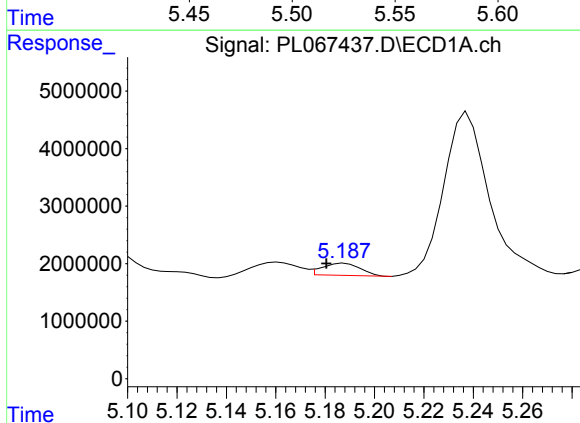


#2 alpha-BHC

R.T.: 5.188 min
Delta R.T.: 0.007 min
Response: 2253188
Conc: 3.06 ng/ml

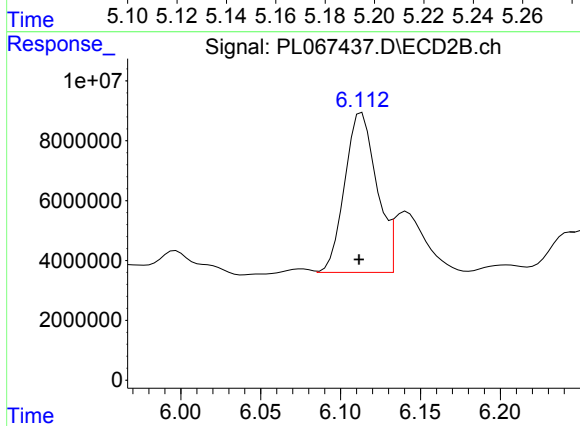

#2 alpha-BHC

R.T.: 6.112 min
Delta R.T.: 0.000 min
Response: 72639850
Conc: 58.75 ng/ml m

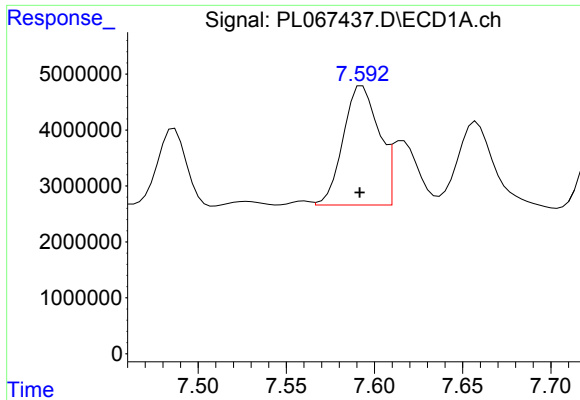


#13 Dieldrin

R.T.: 7.592 min
Delta R.T.: 0.000 min
Response: 28705755
Conc: 40.95 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TMR-DS-03-060921


Manual Integrations
APPROVED

Ankita
6/15/2021 2:40:39 PM

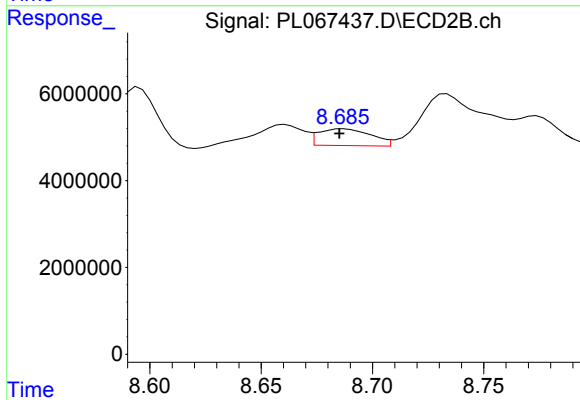


#13 Dieldrin

R.T.: 8.685 min
Delta R.T.: 0.000 min
Response: 6193717
Conc: 6.82 ng/ml m

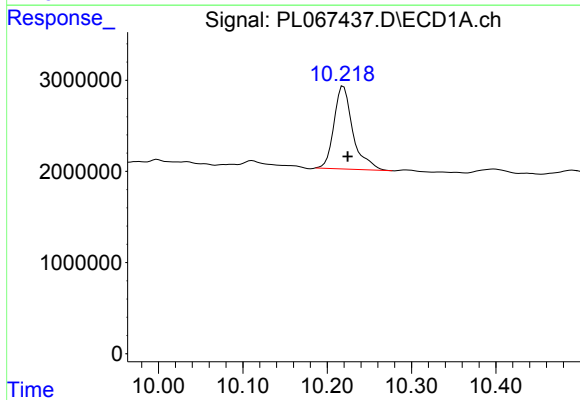

#28 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.005 min
Response: 14150687
Conc: 19.97 ng/ml

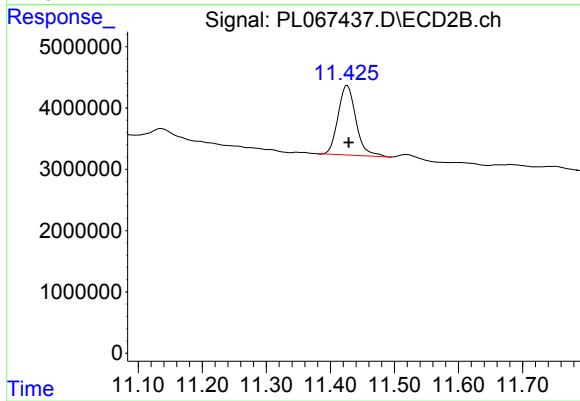

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.002 min
Response: 21812616
Conc: 21.90 ng/ml